




2021-5-12

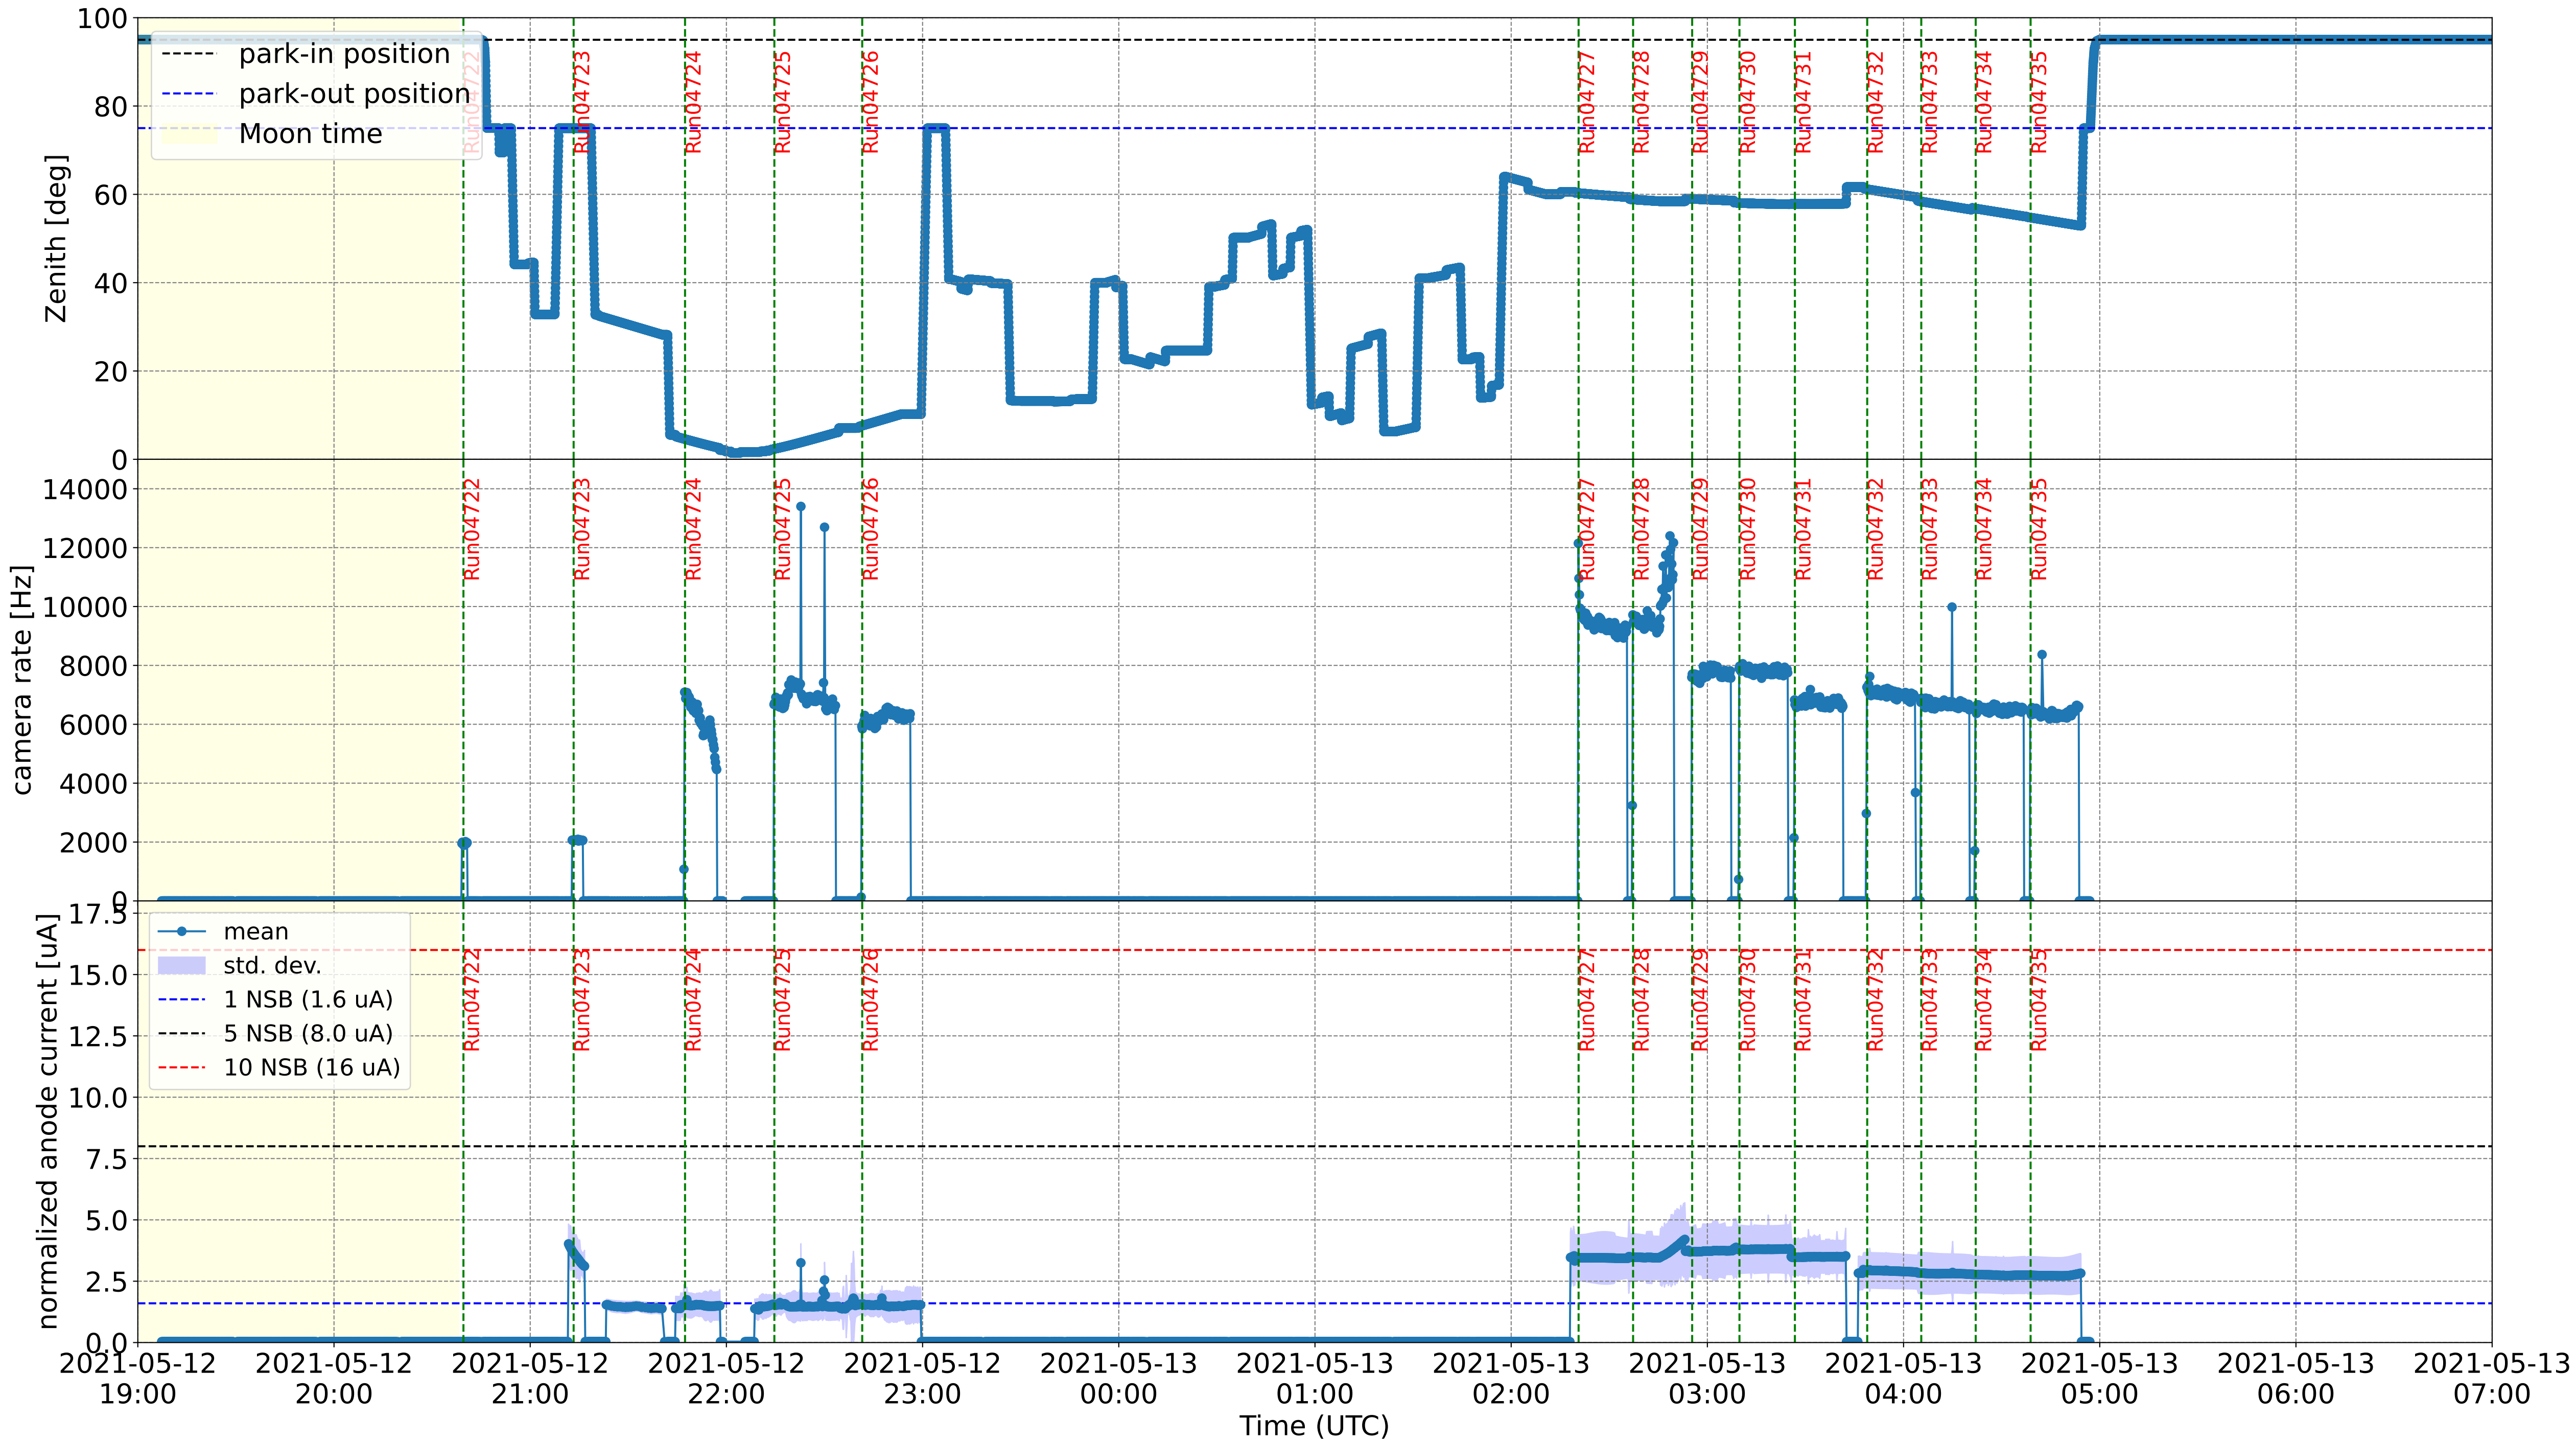


2021-5-12






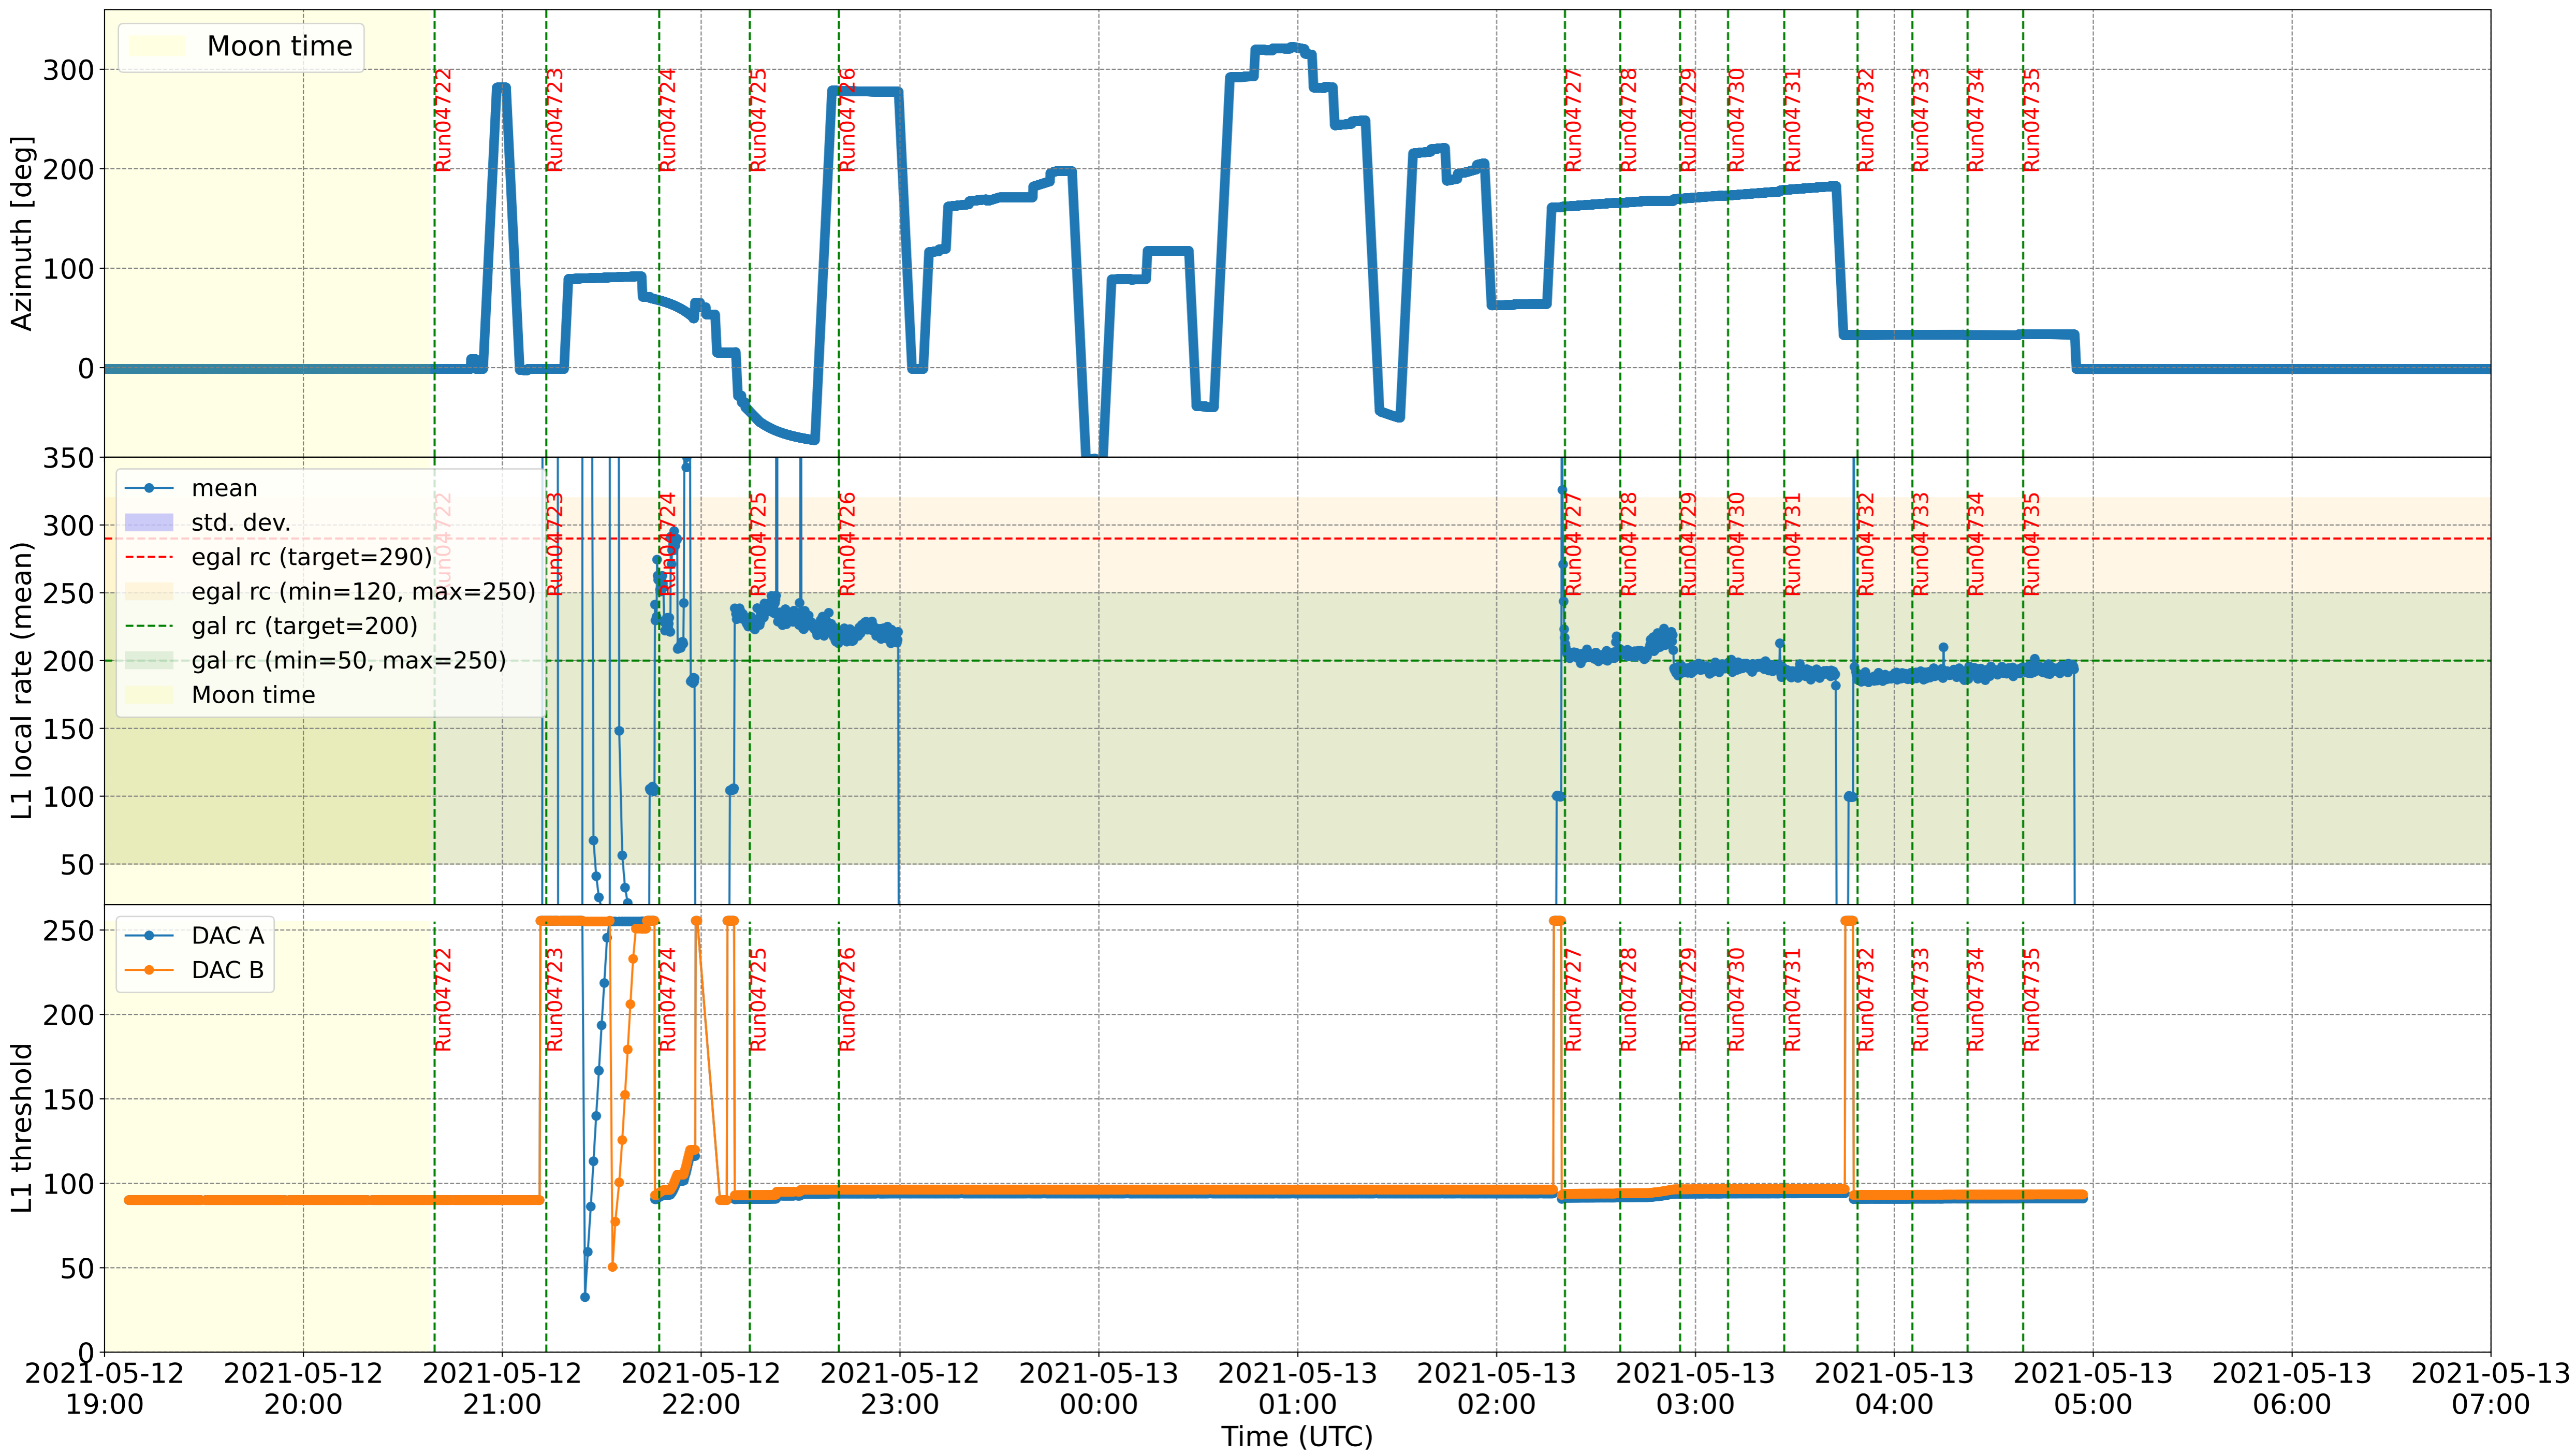








2021-5-12






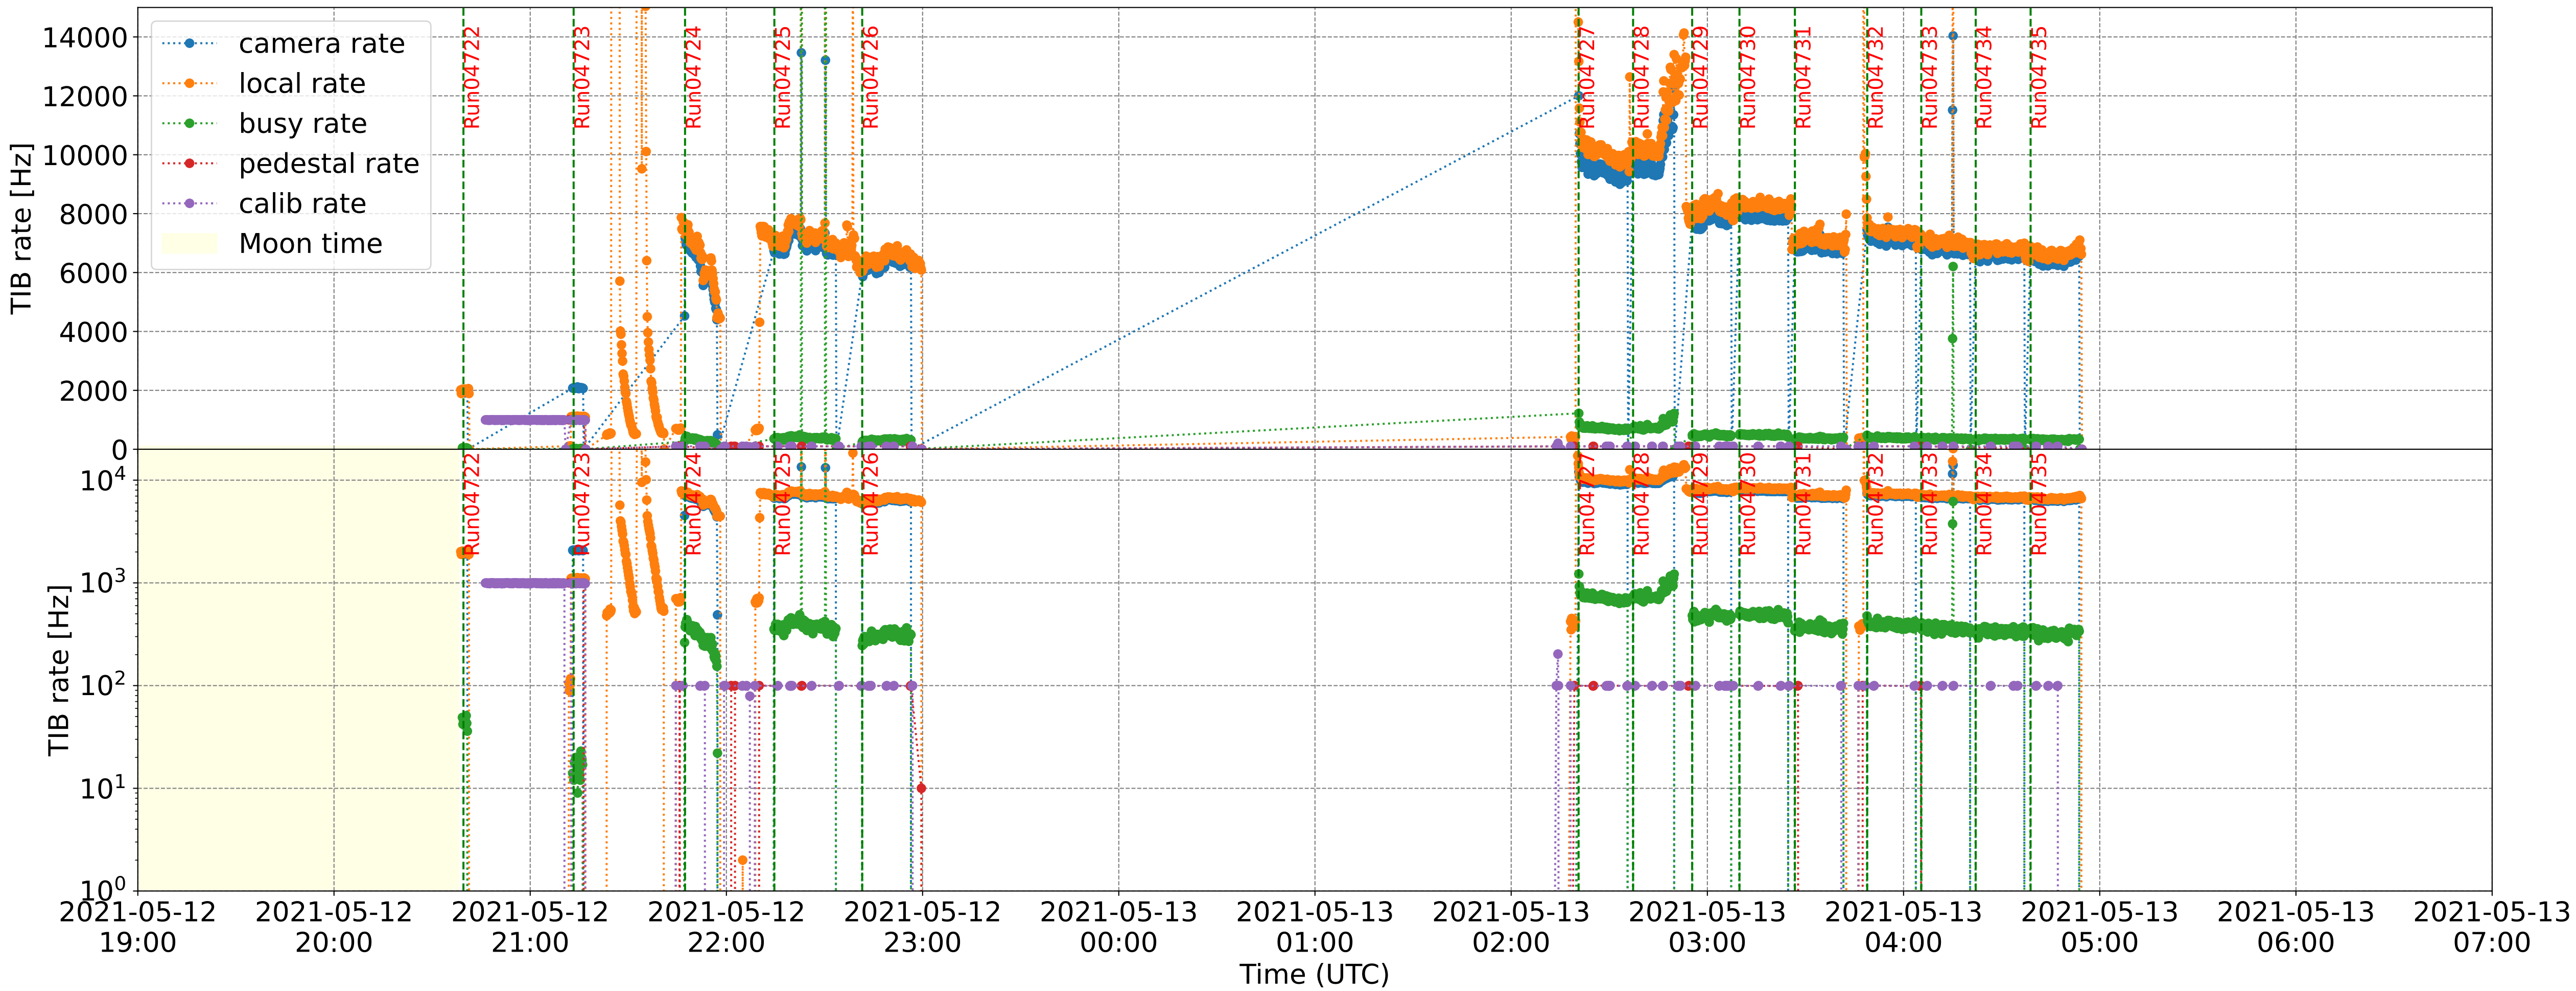








# Calibration Box (2021-5-12)

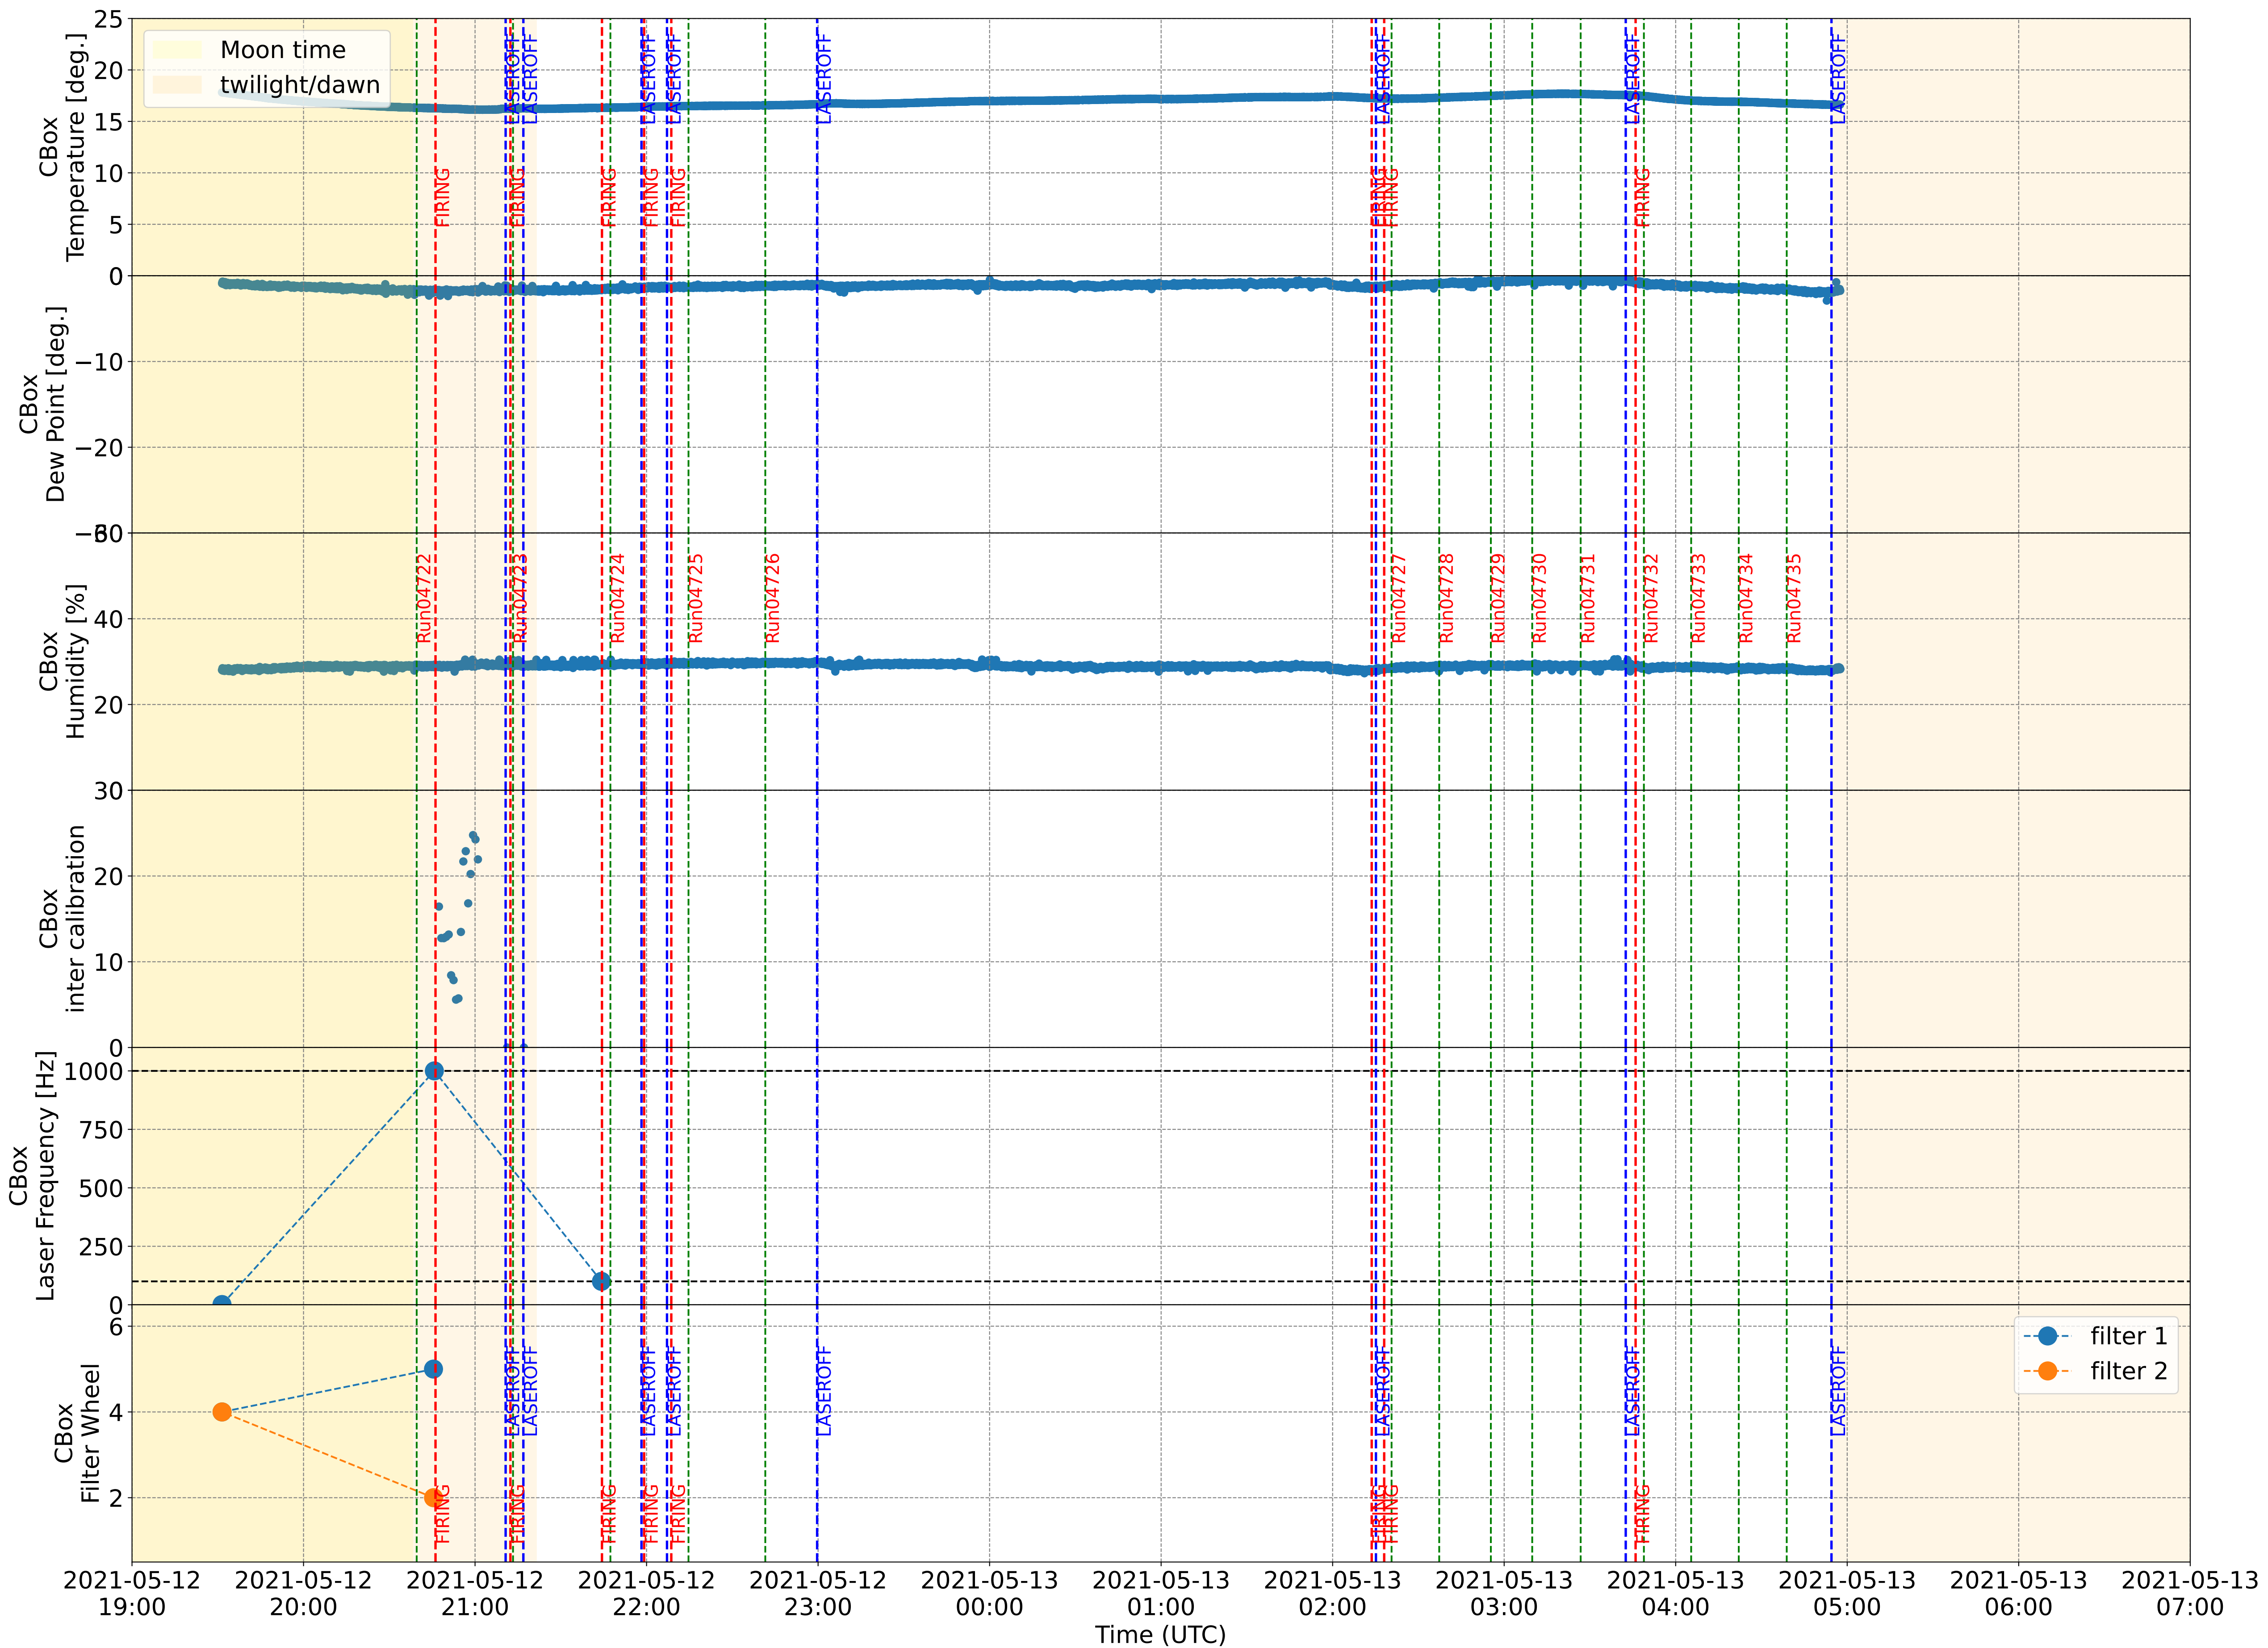

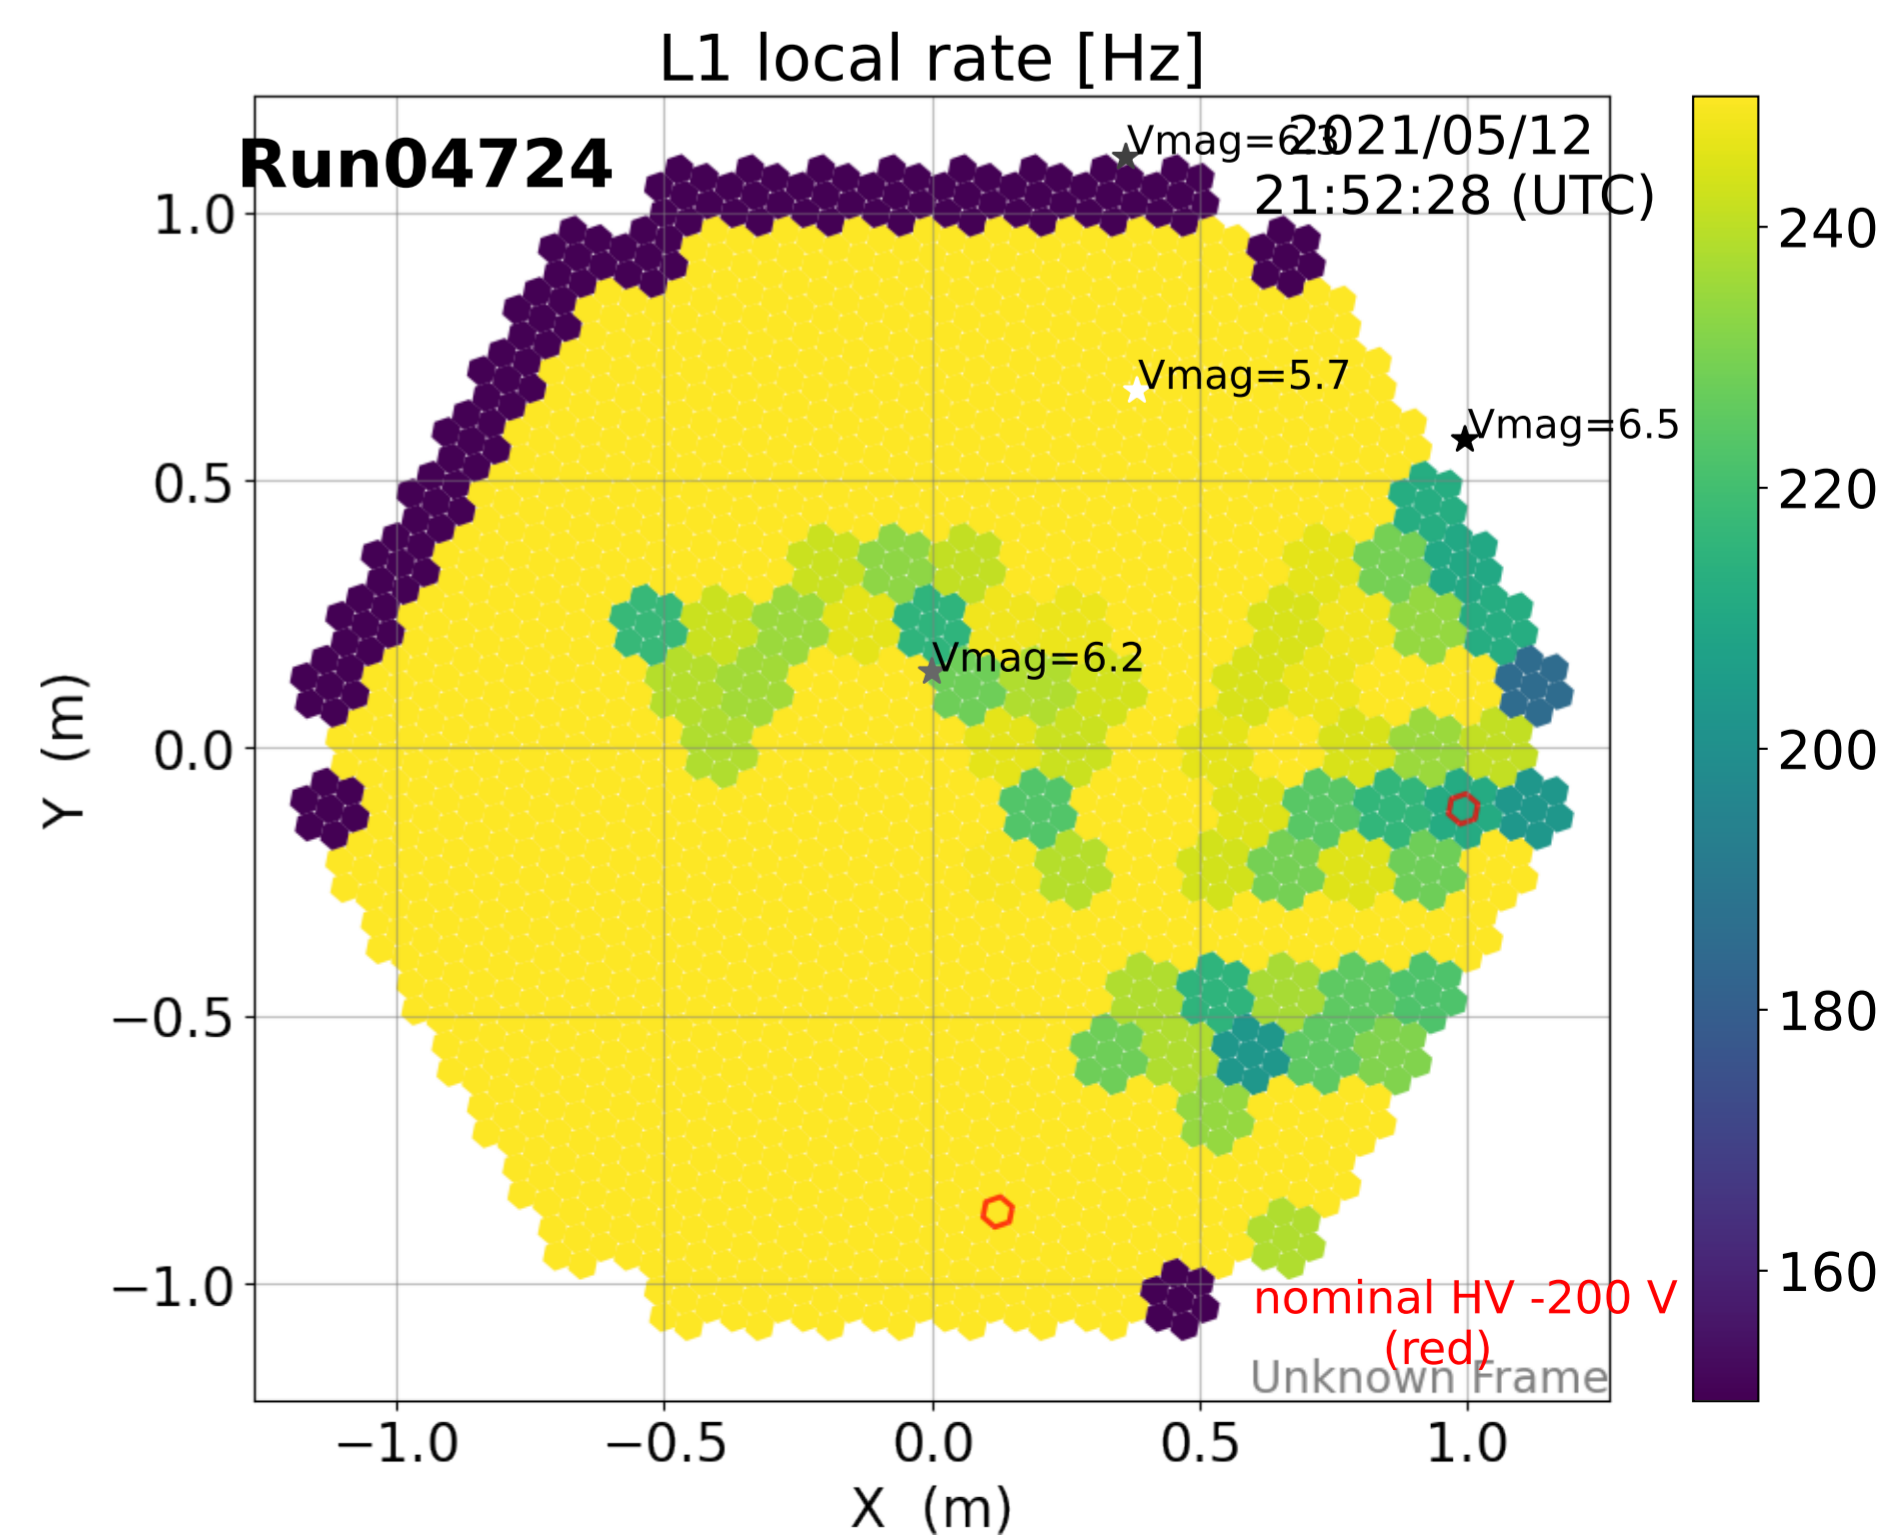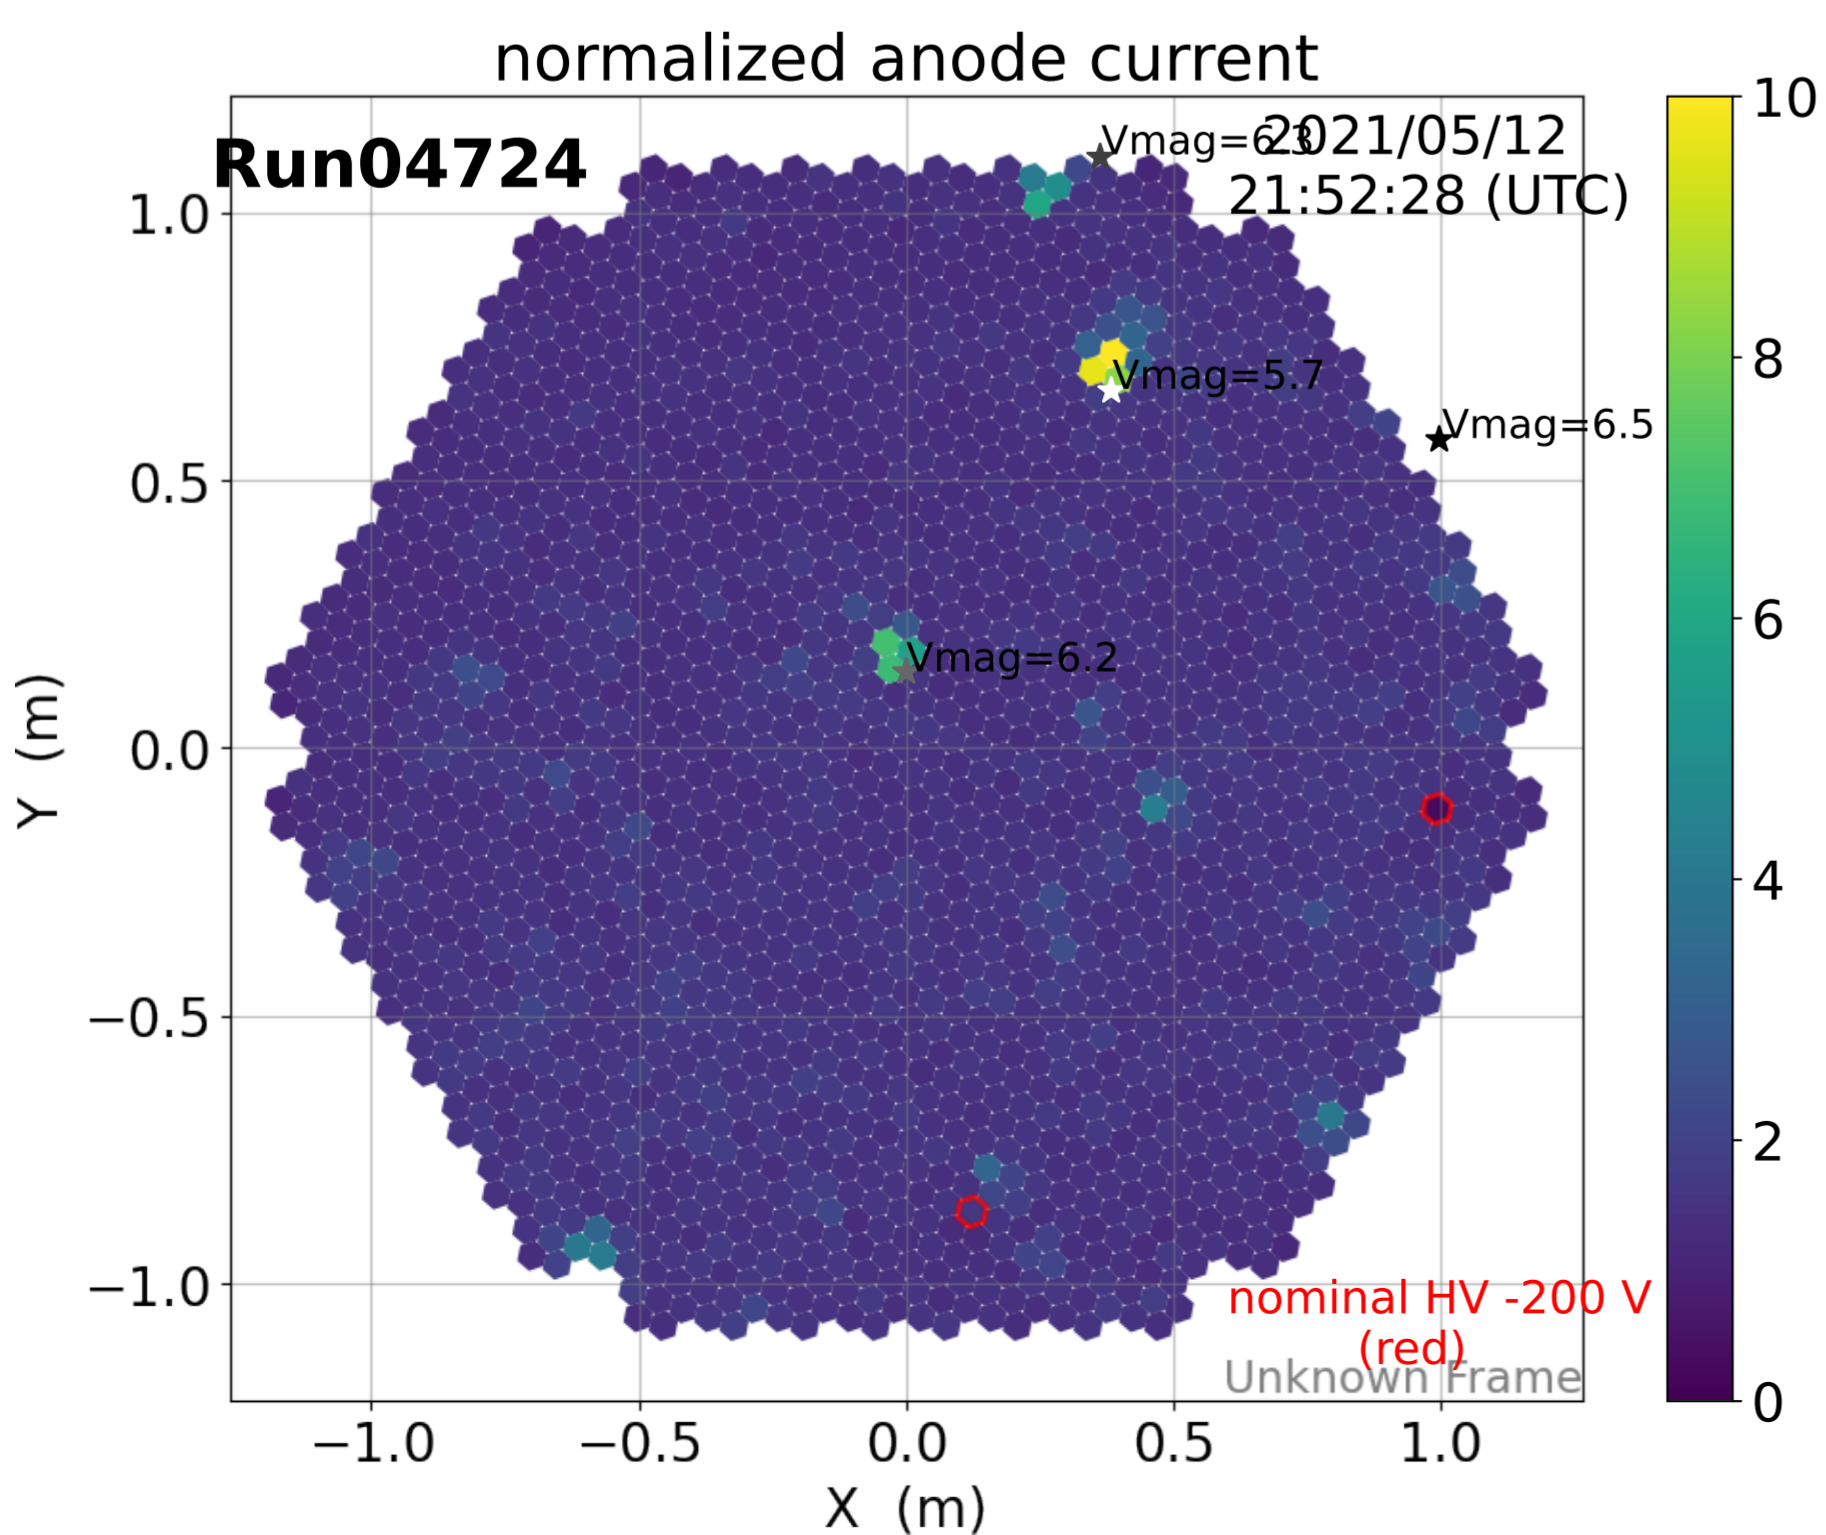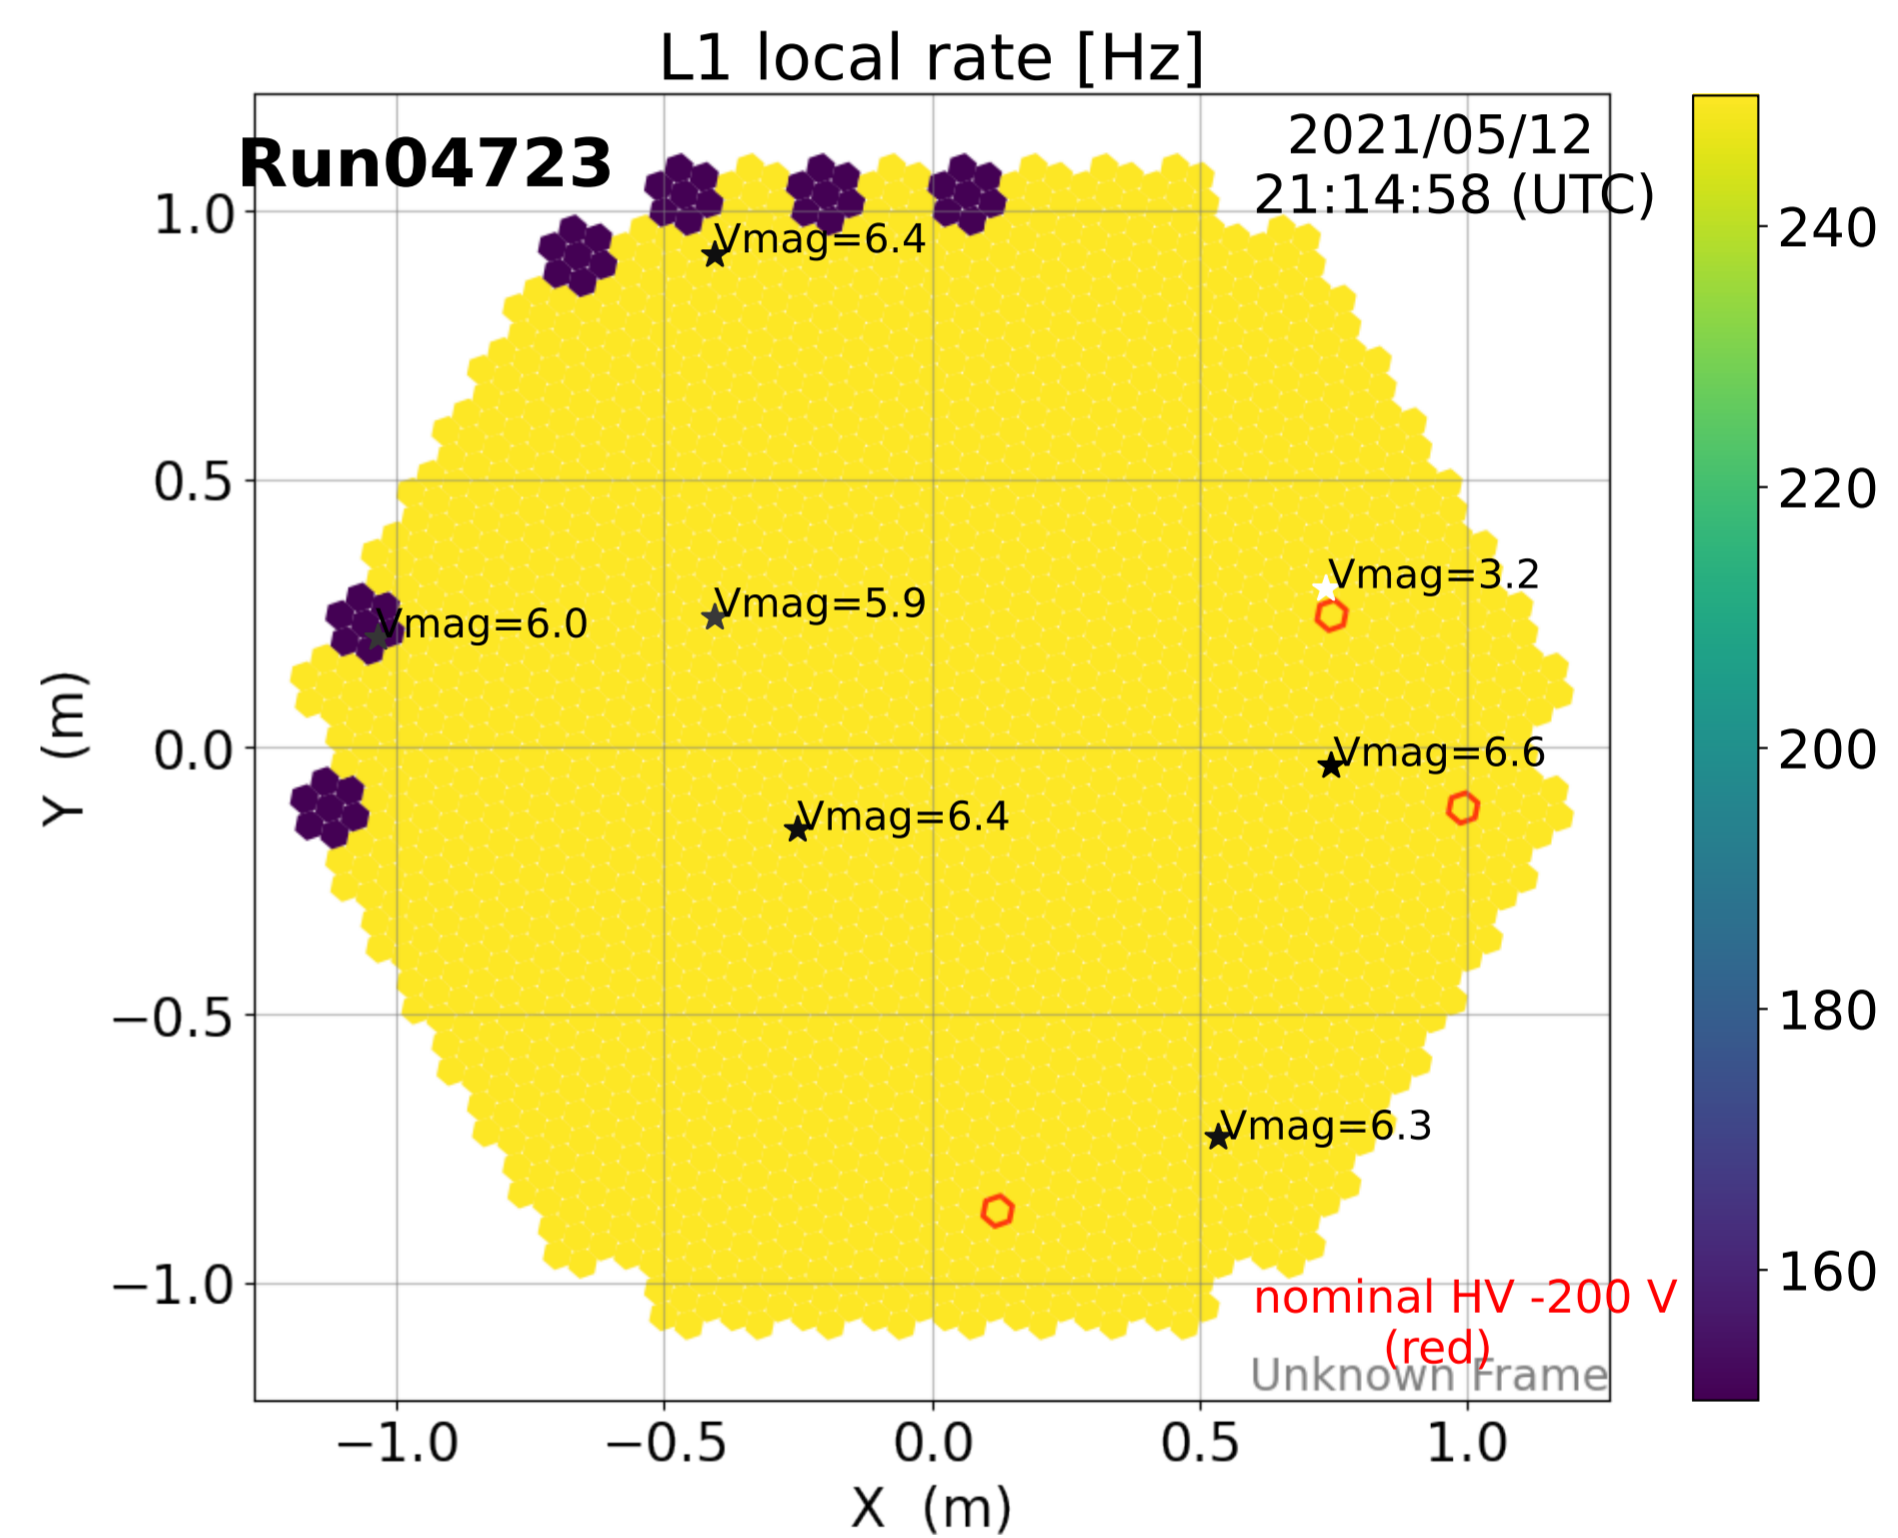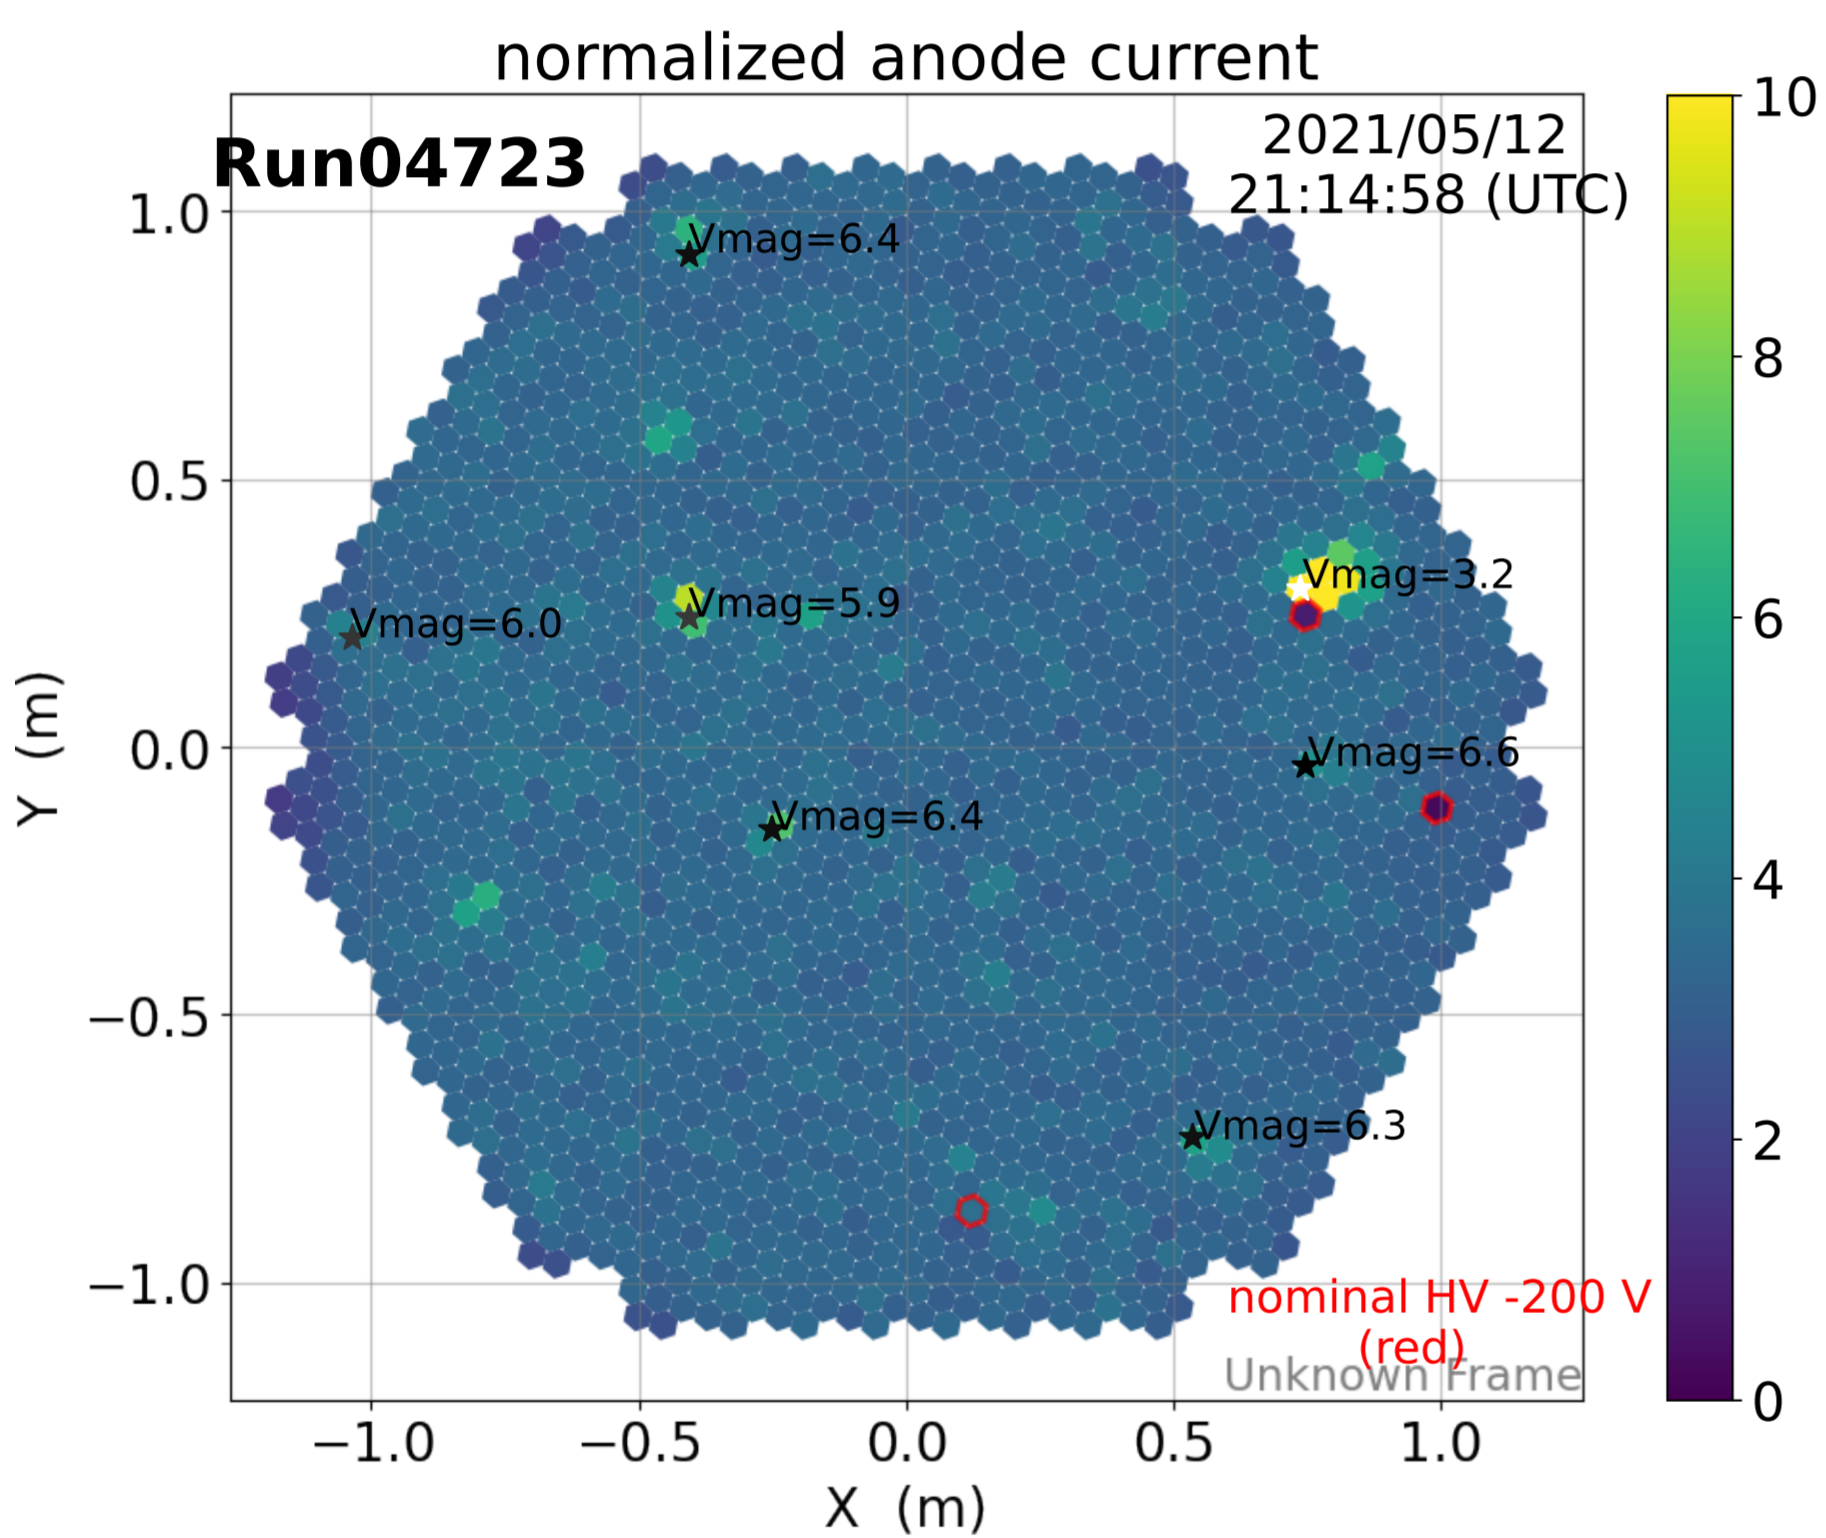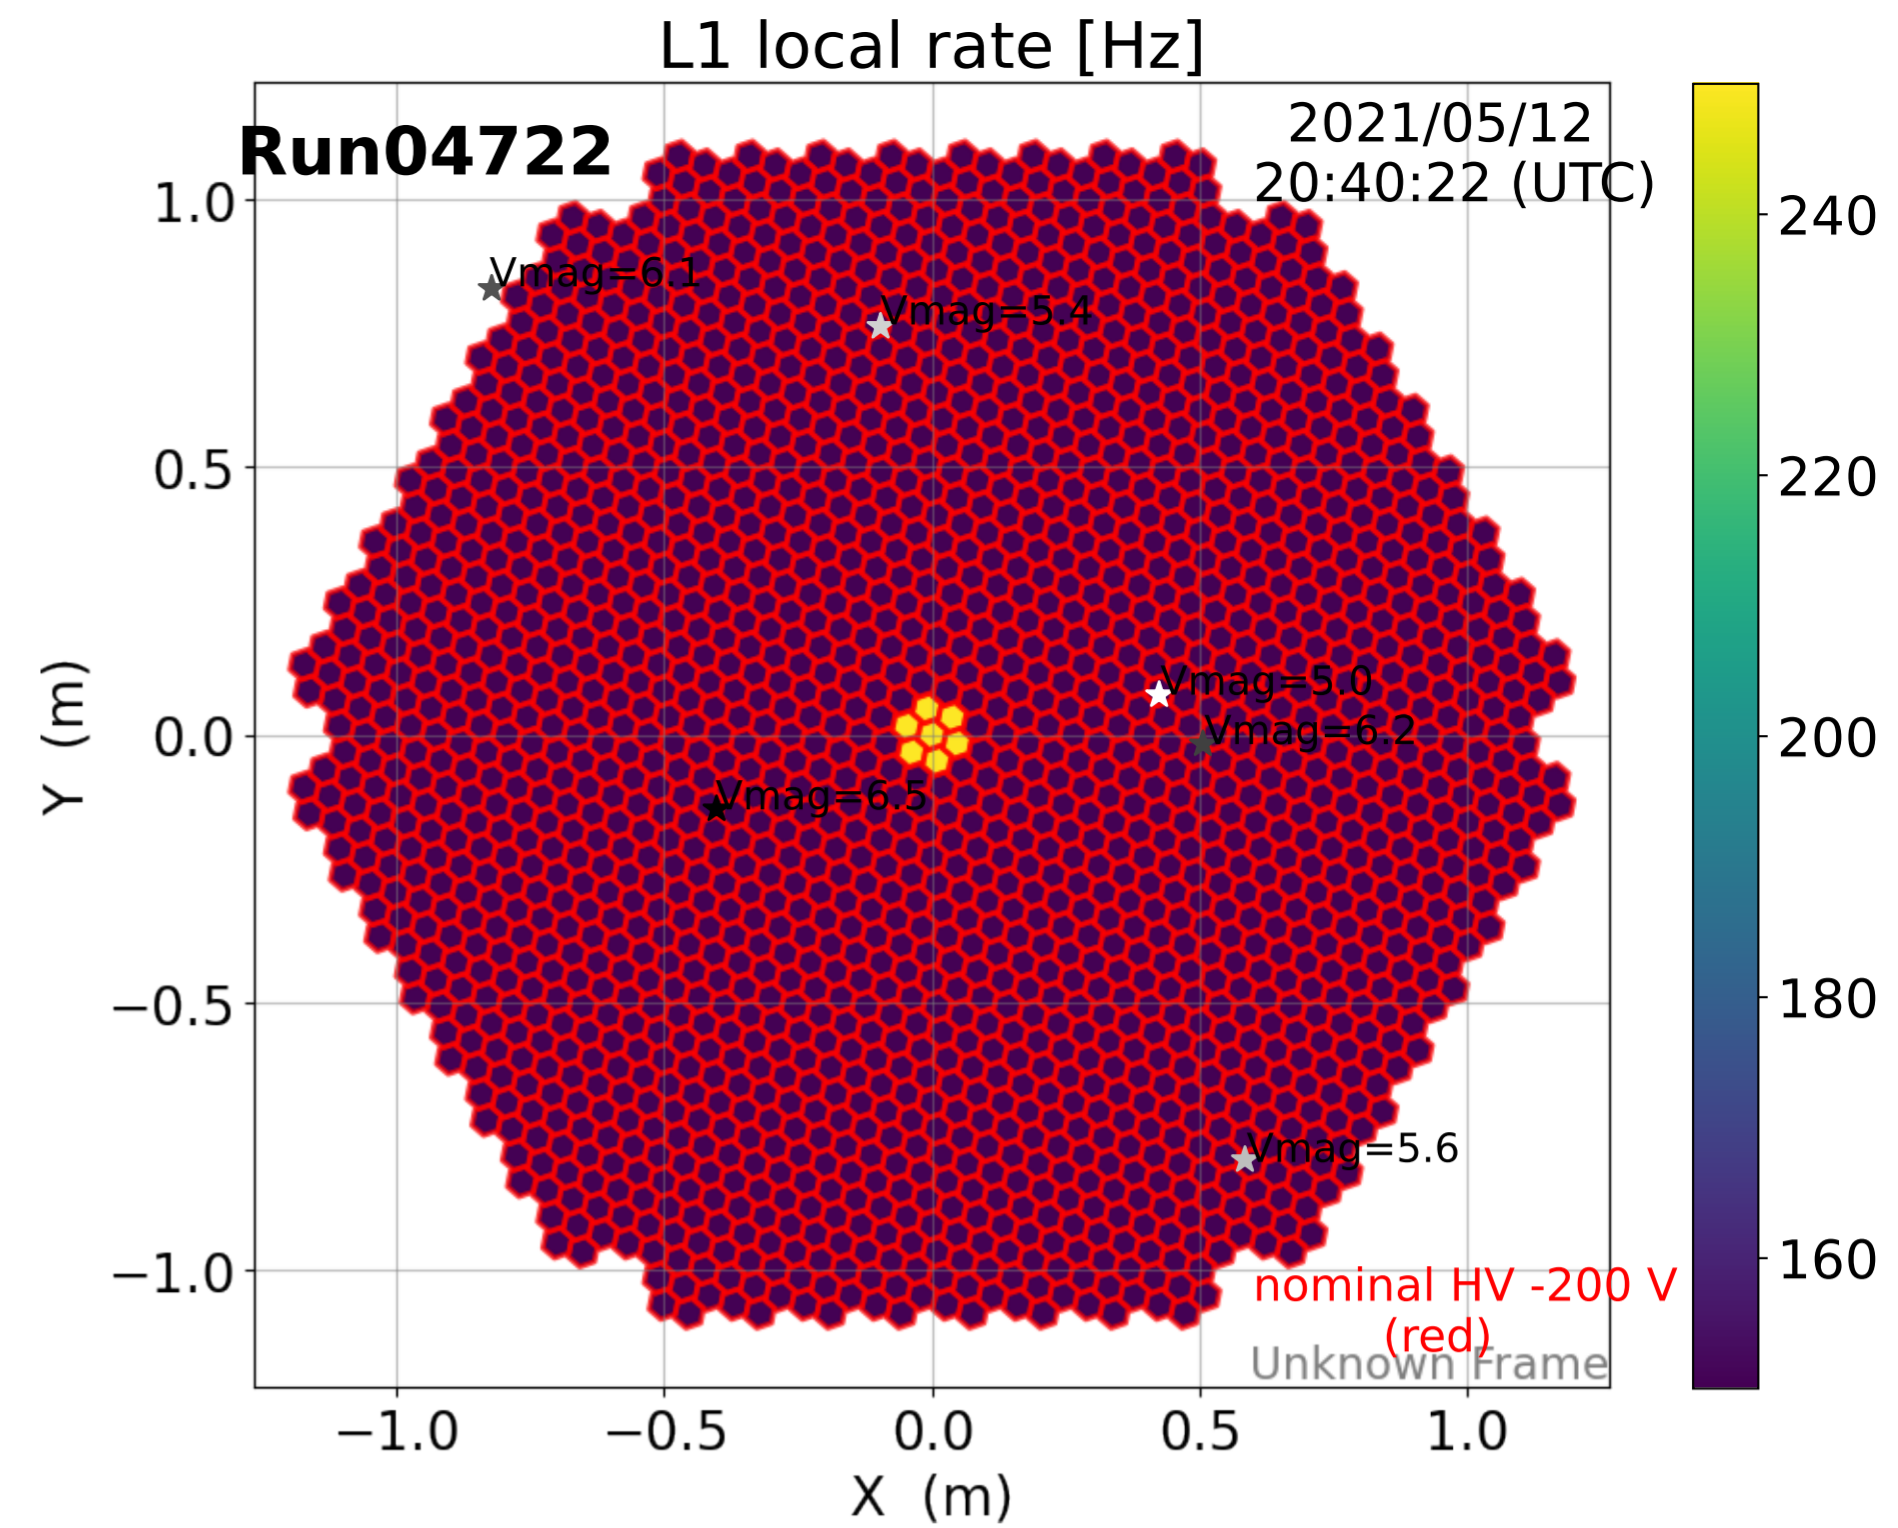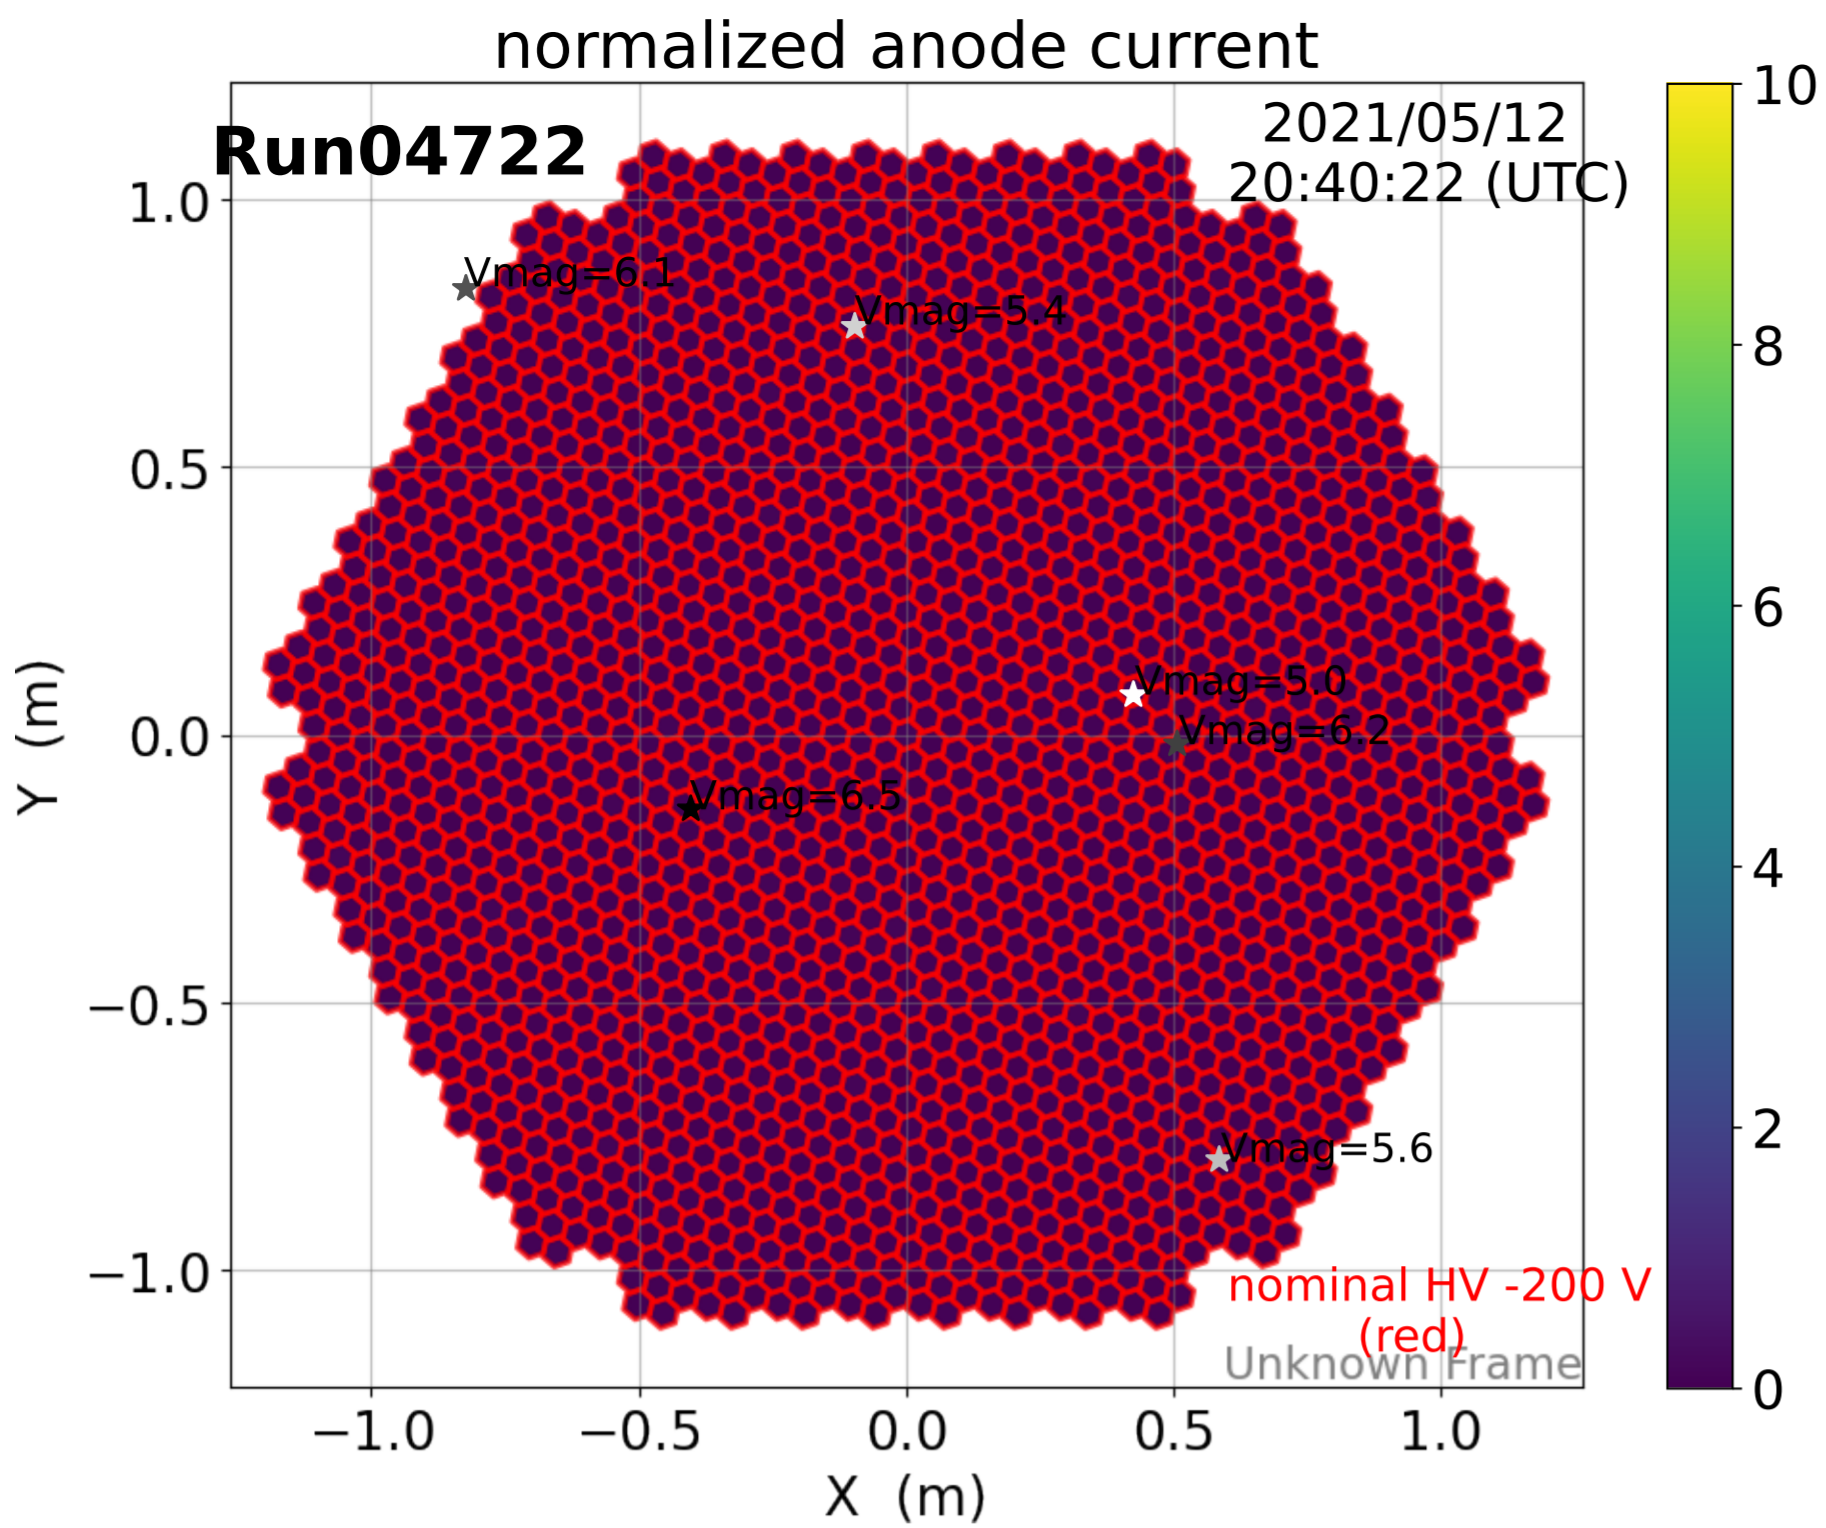

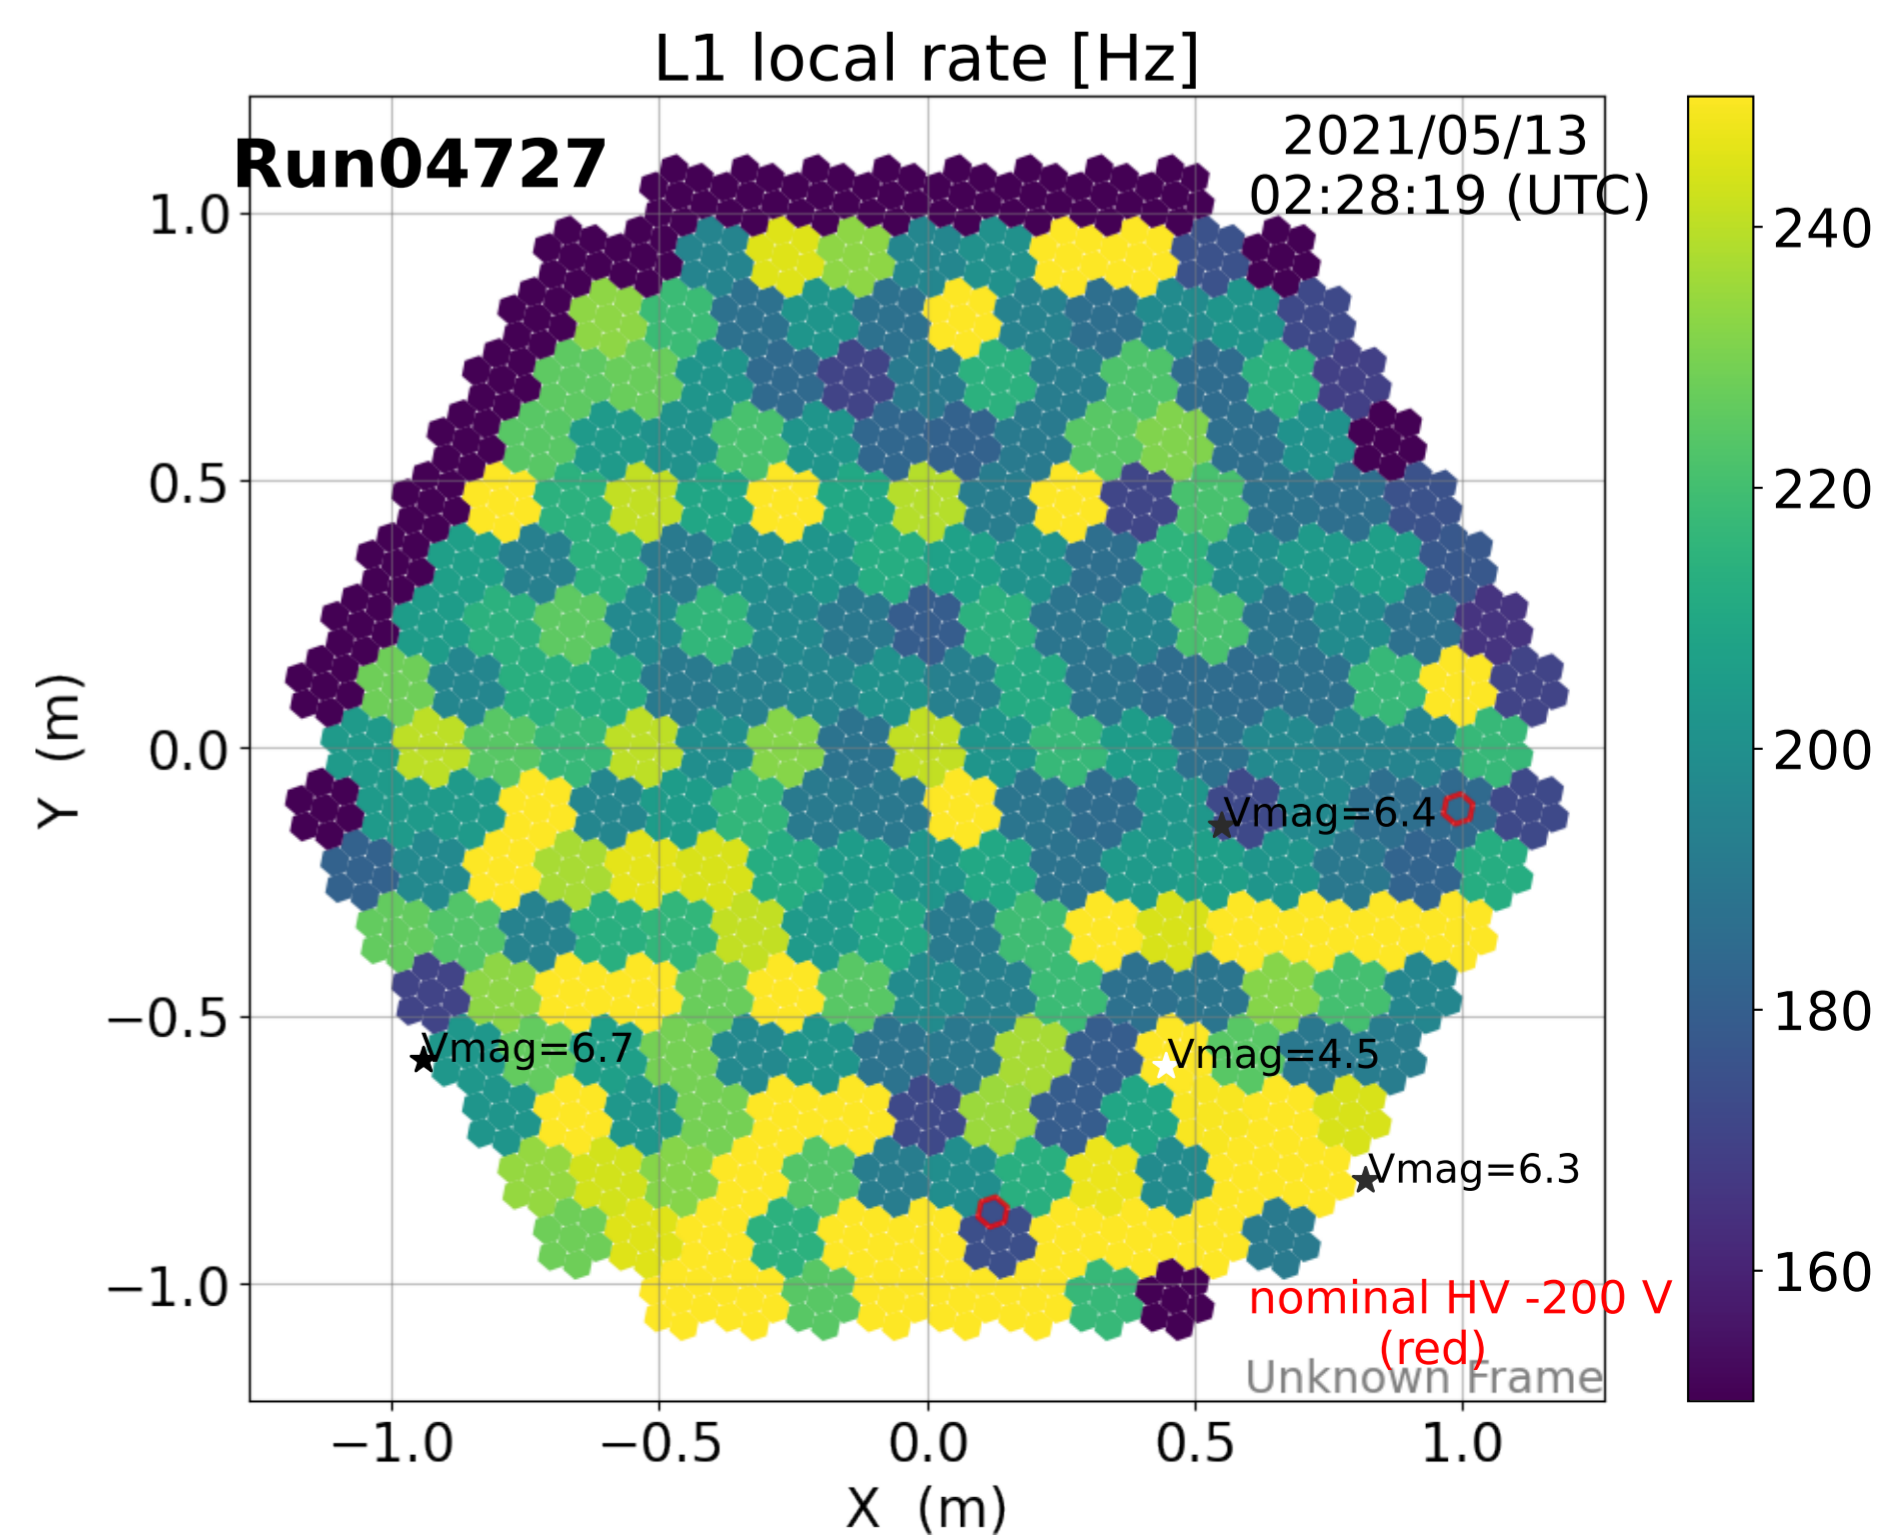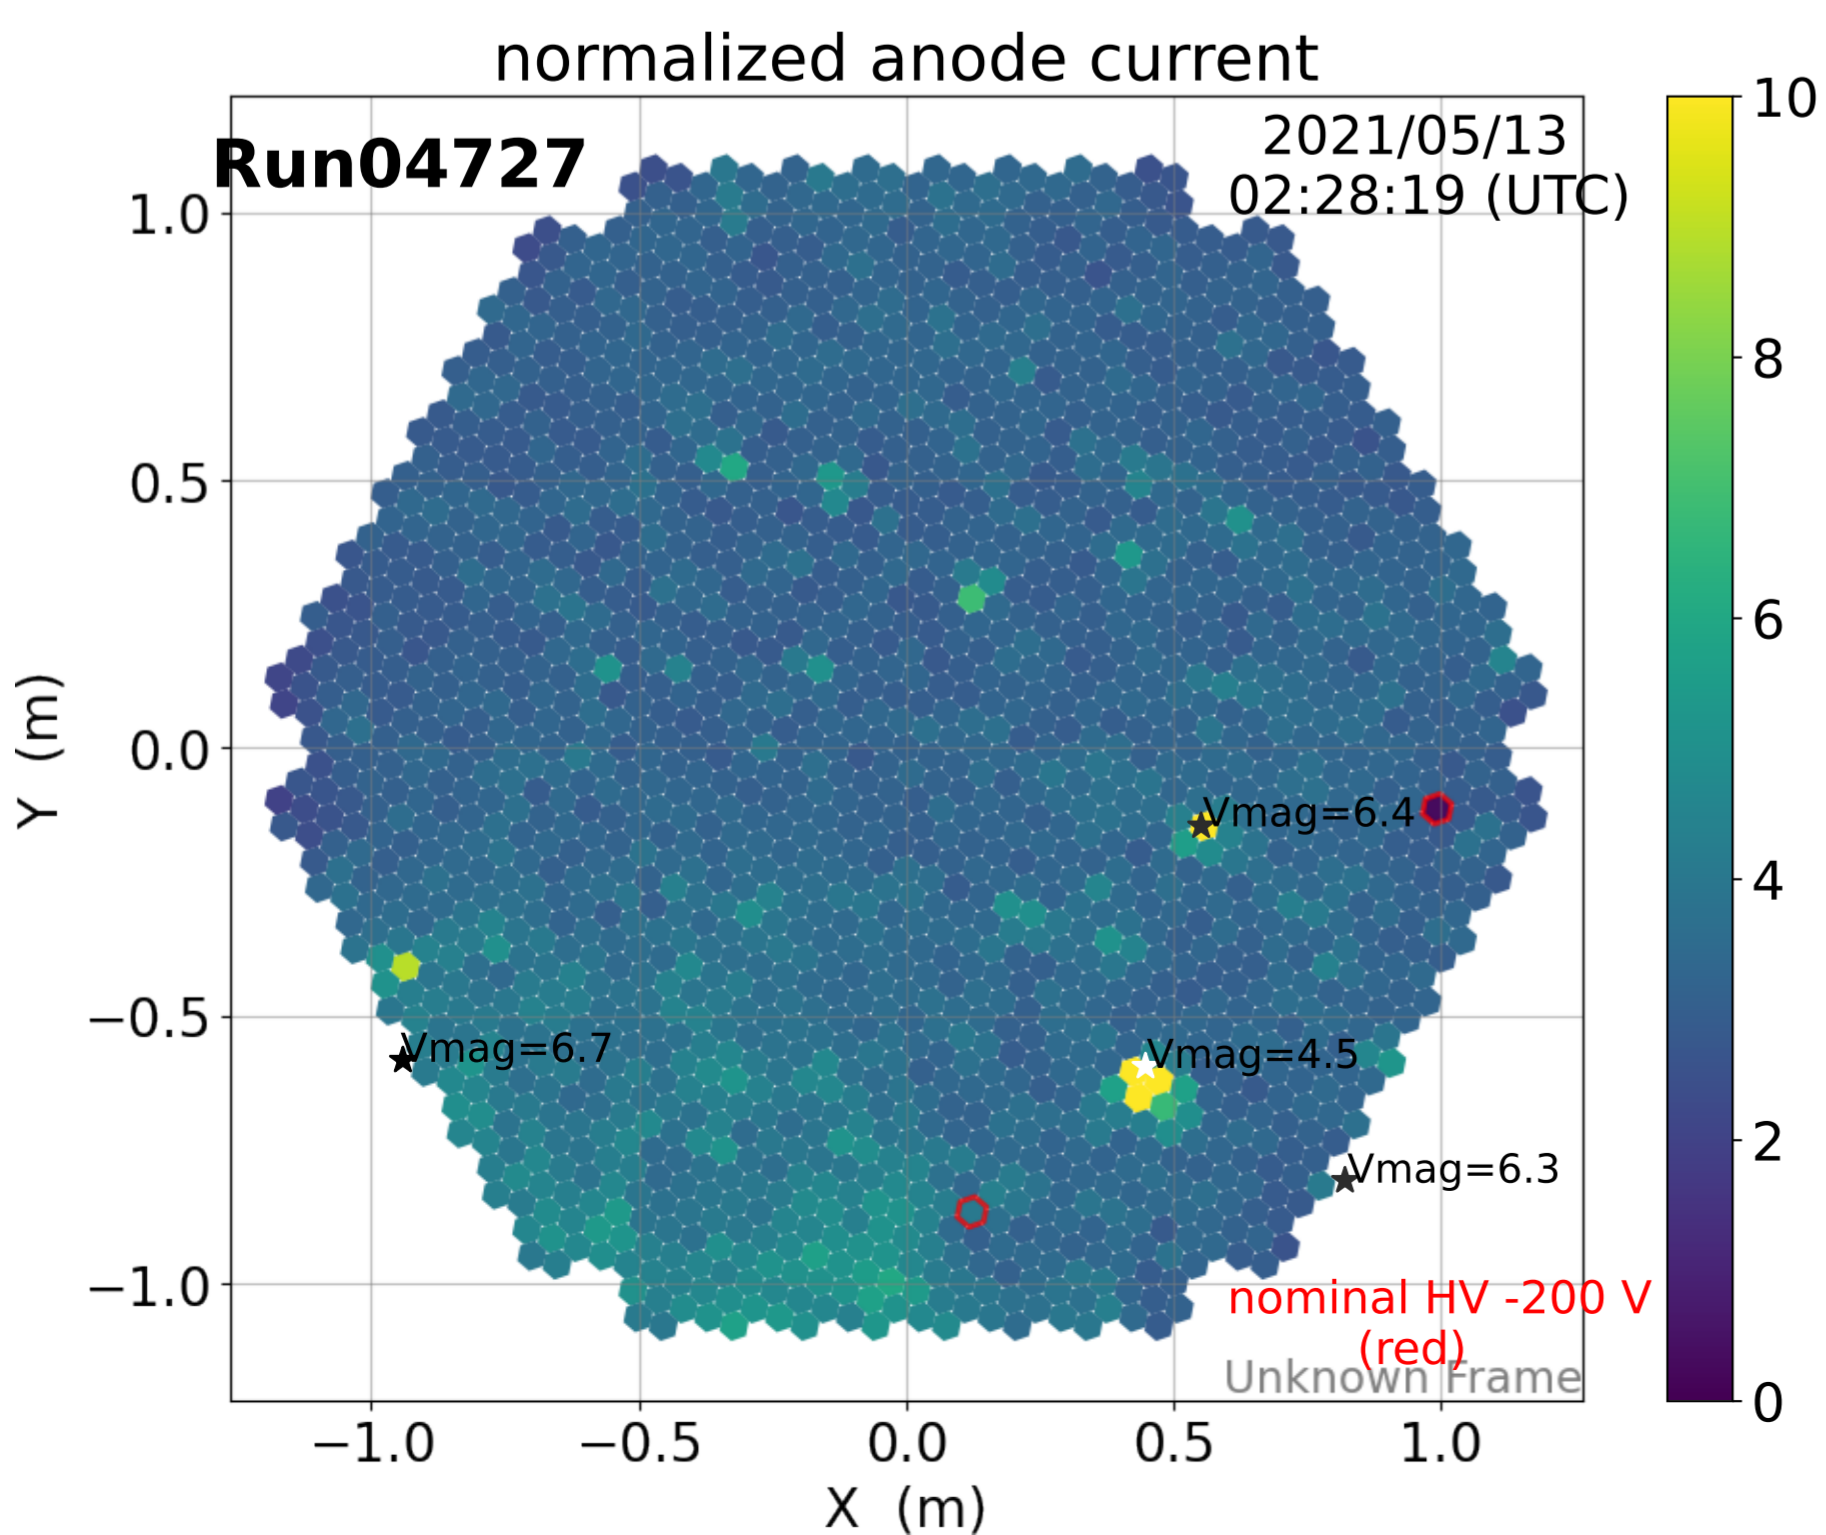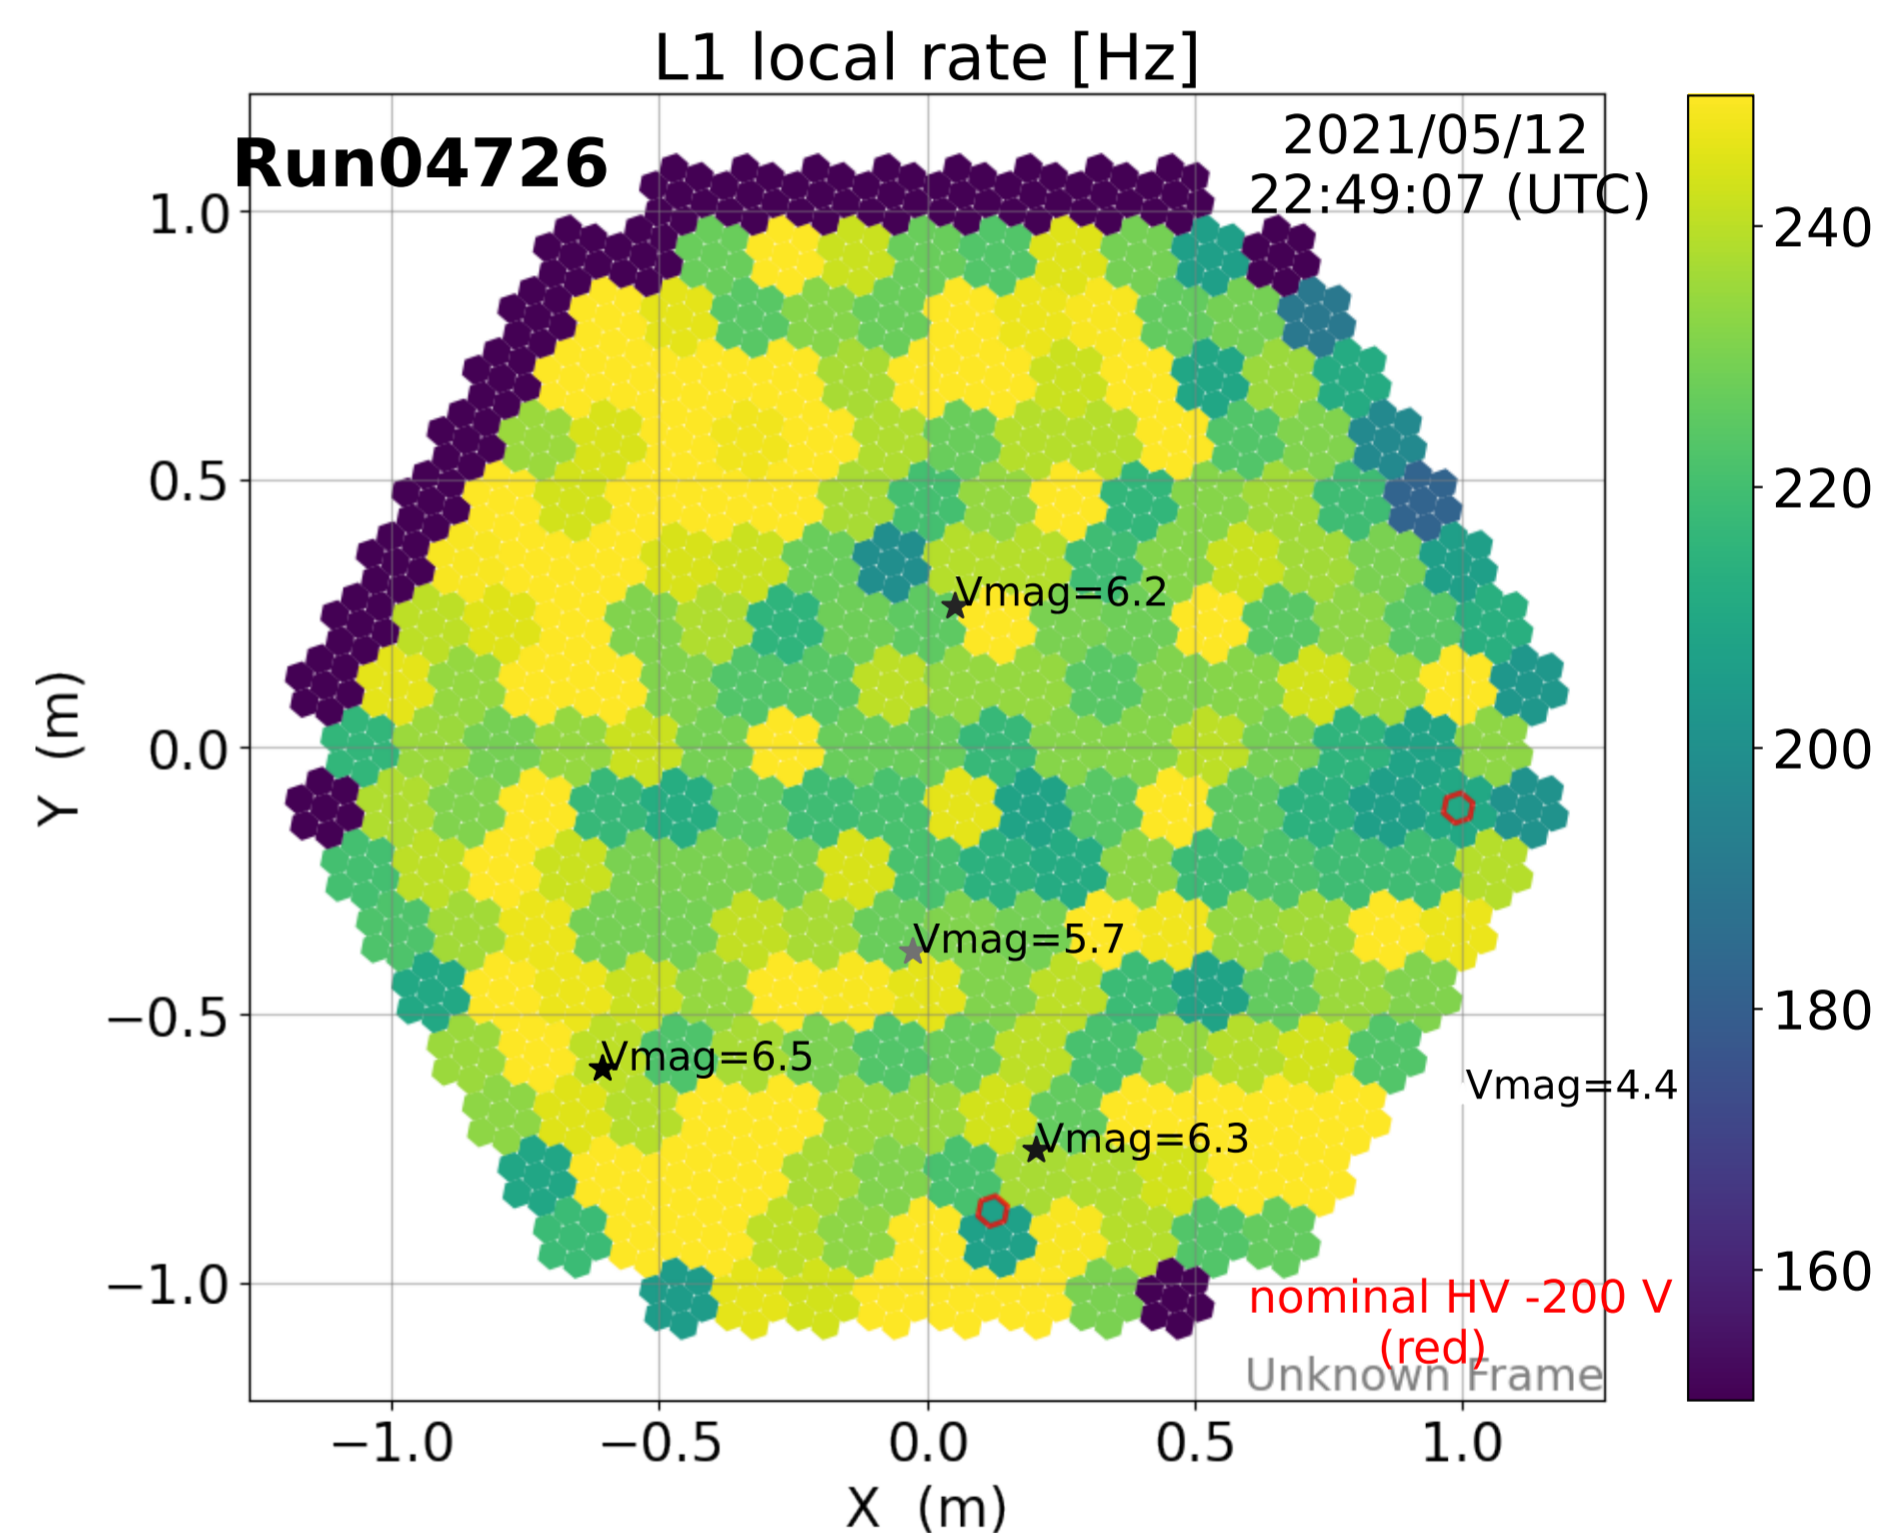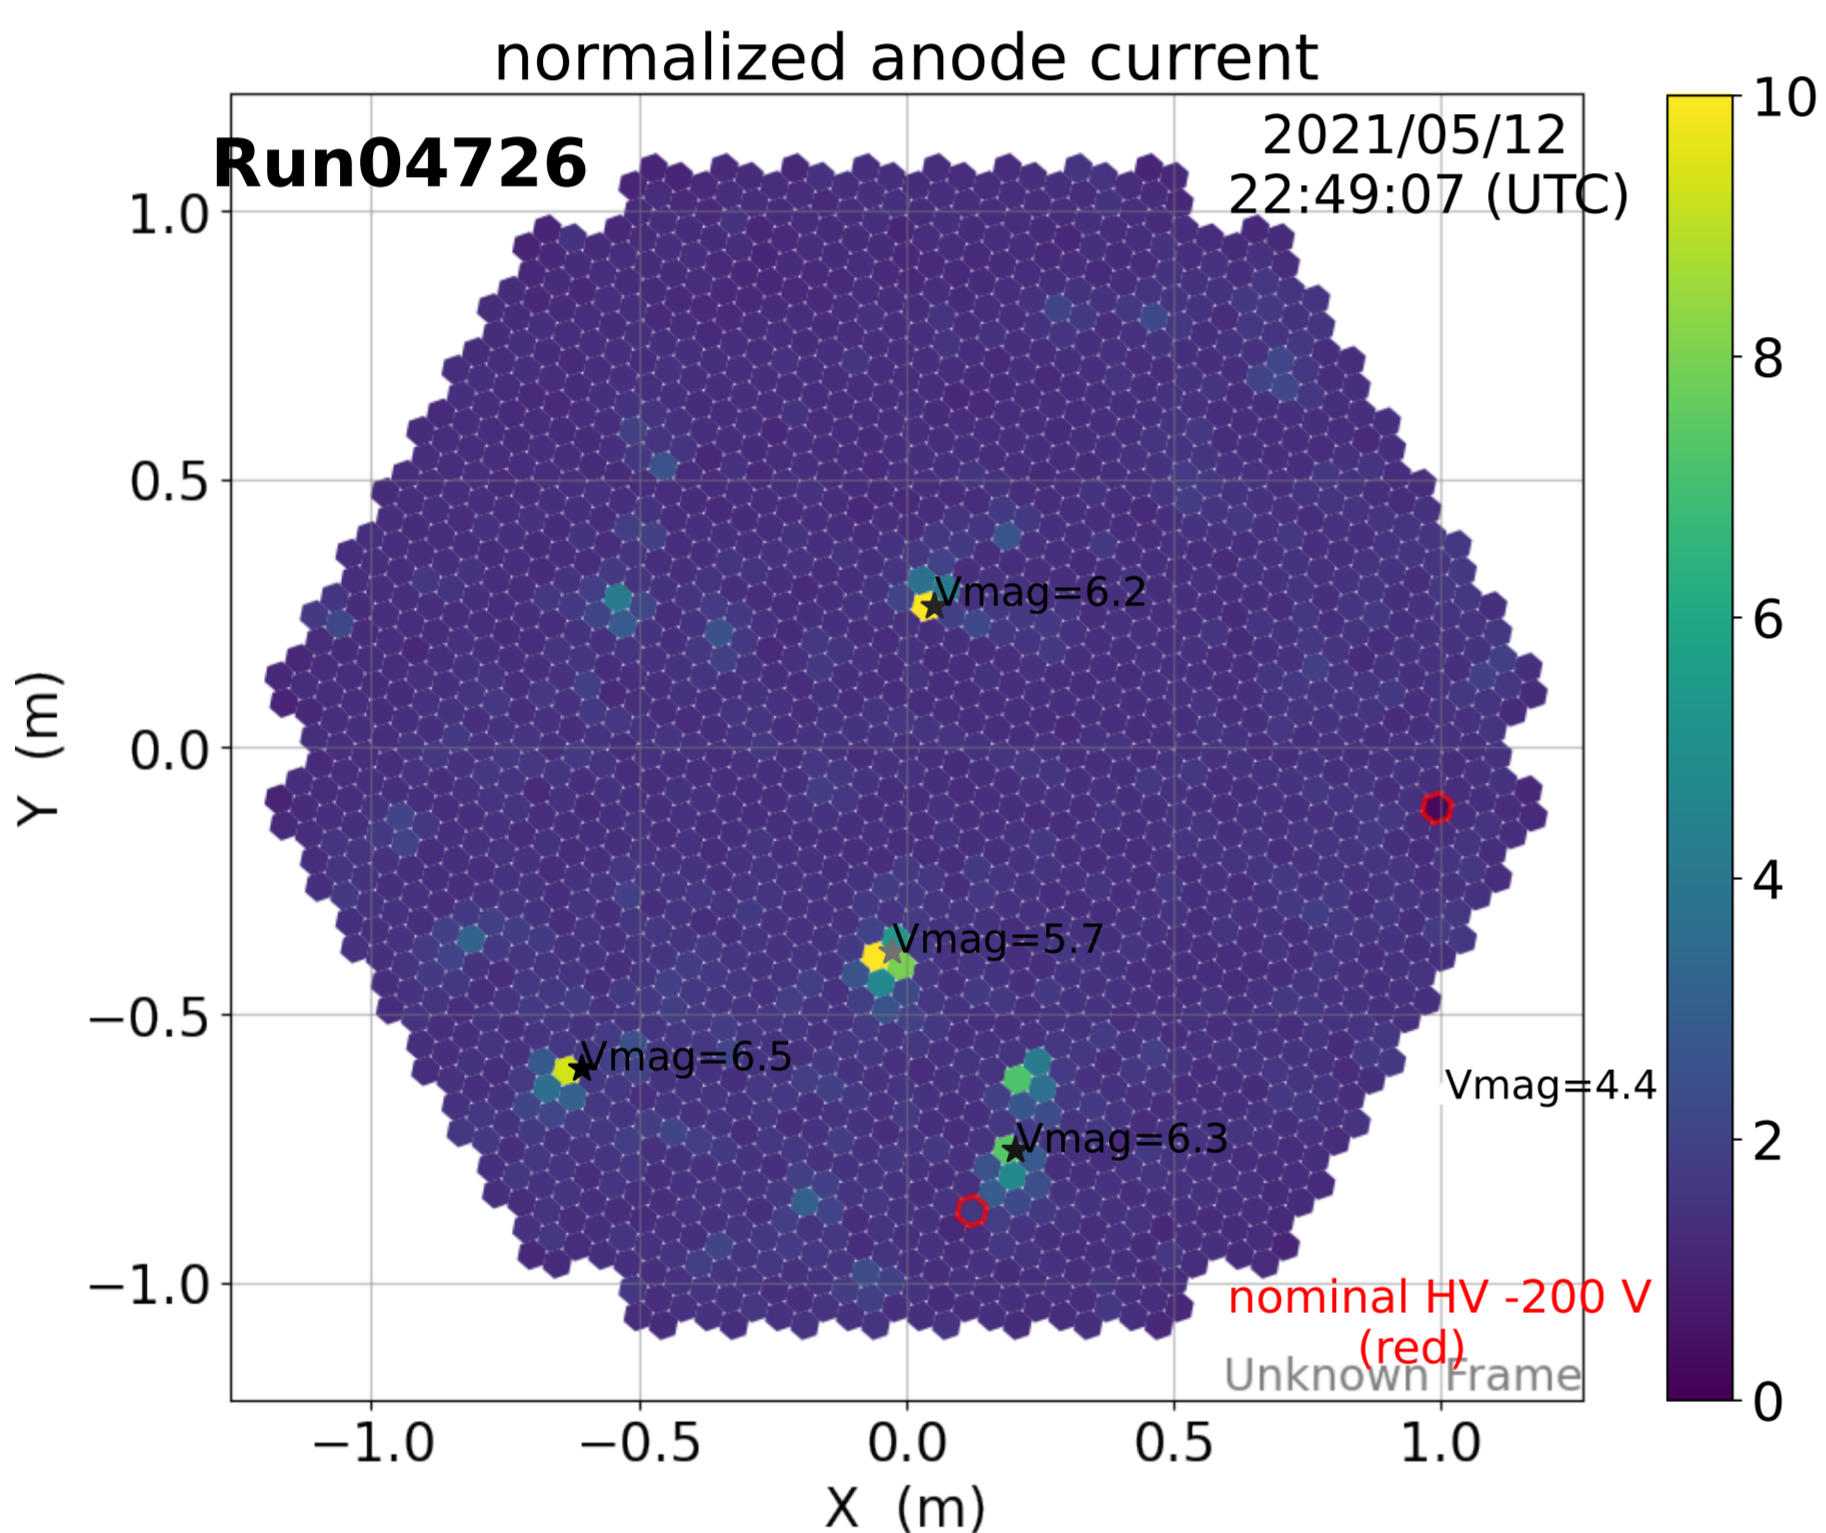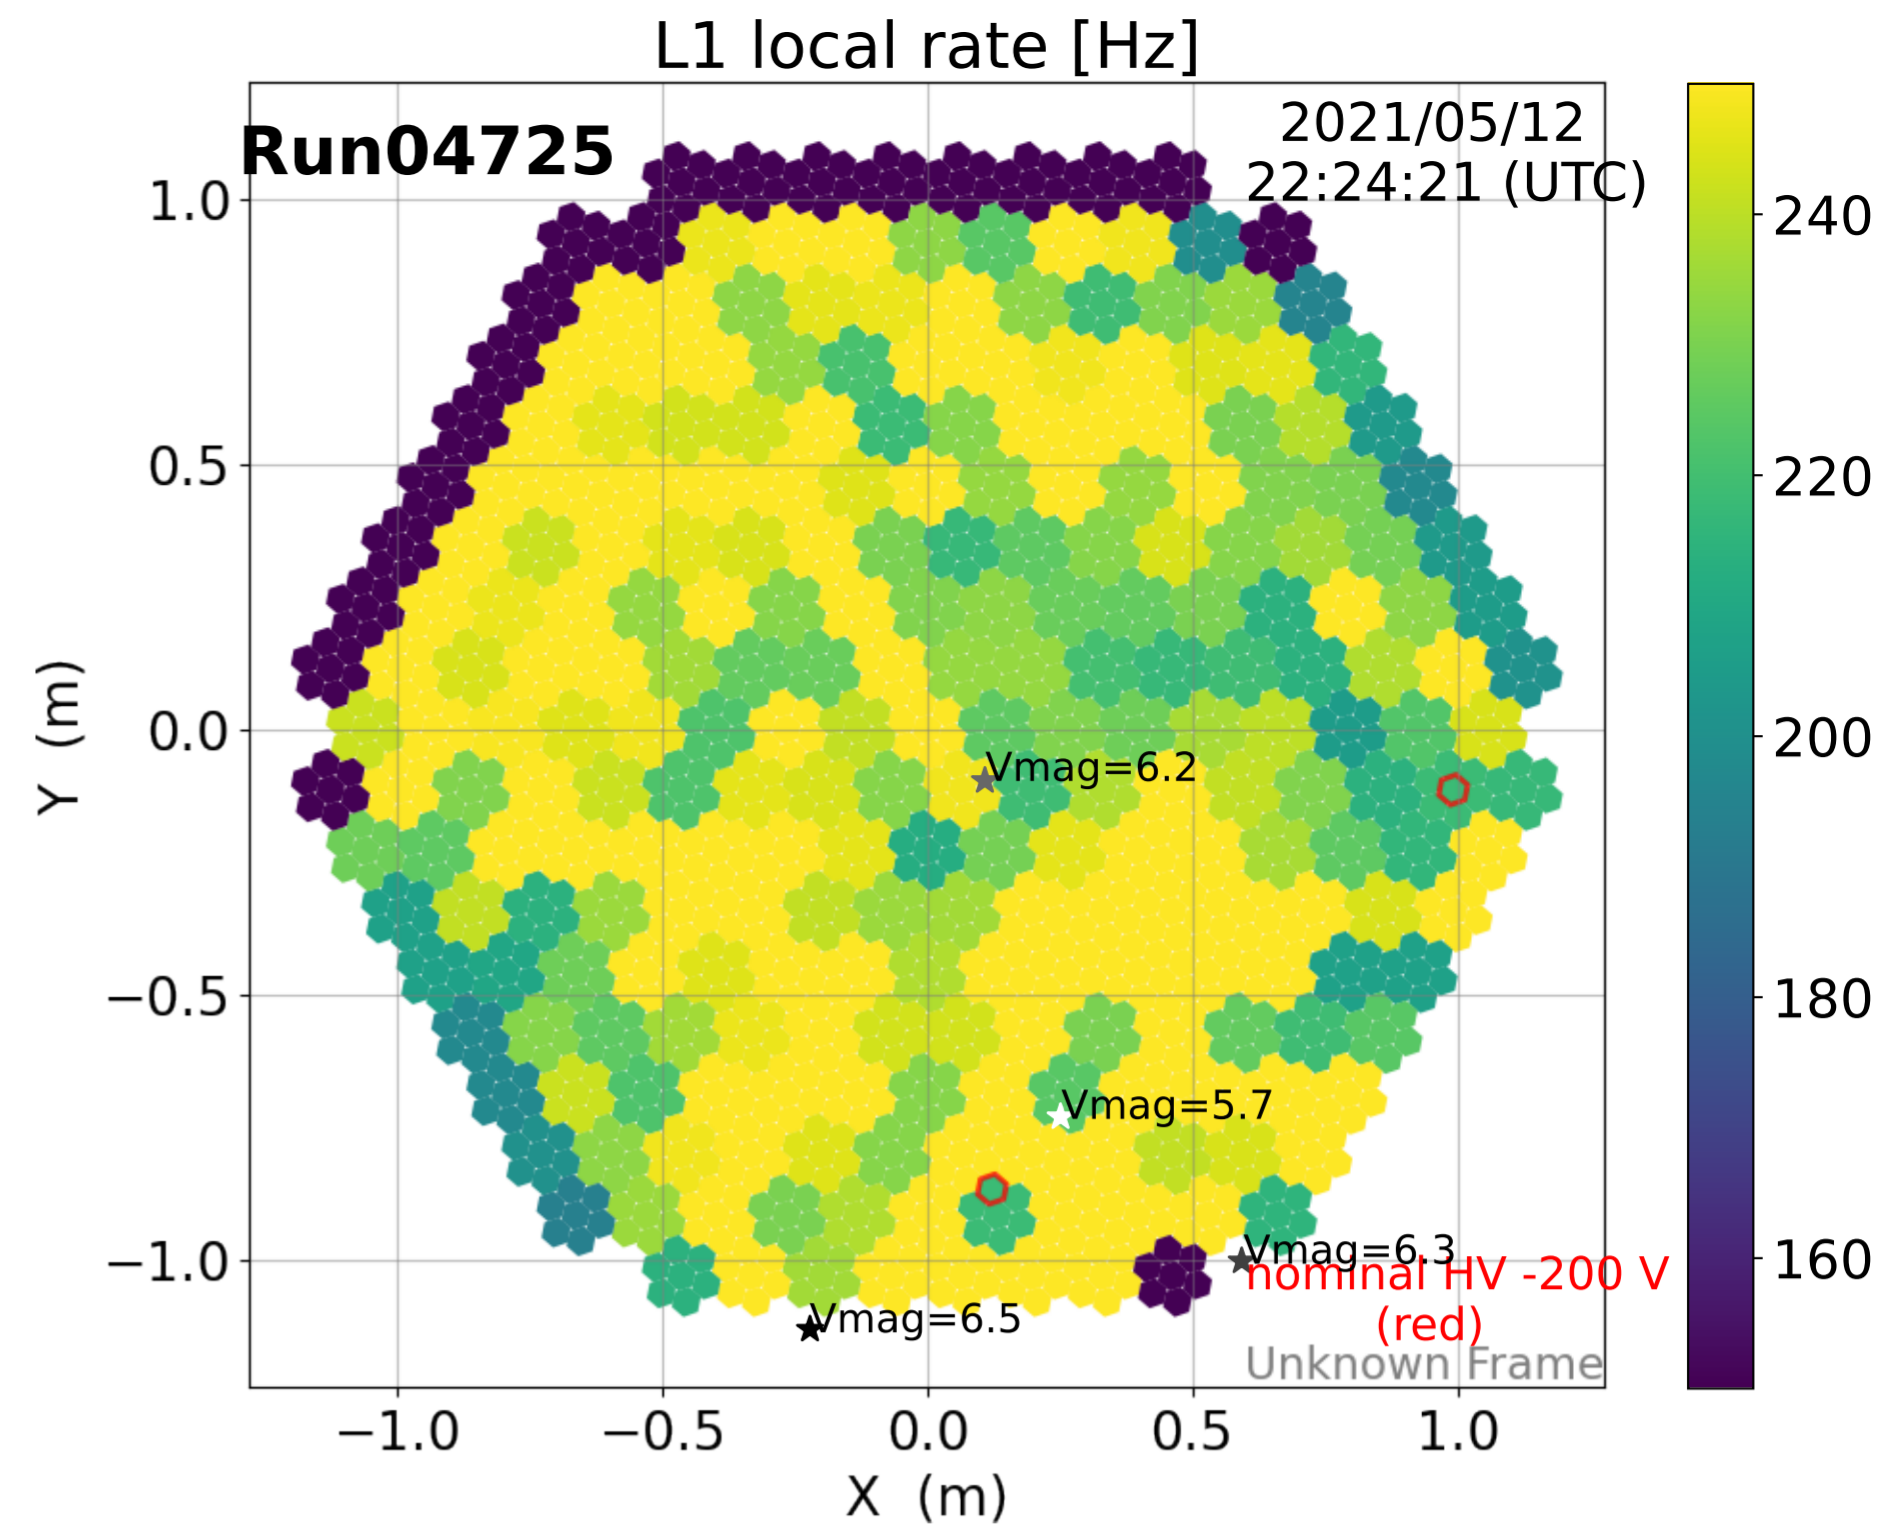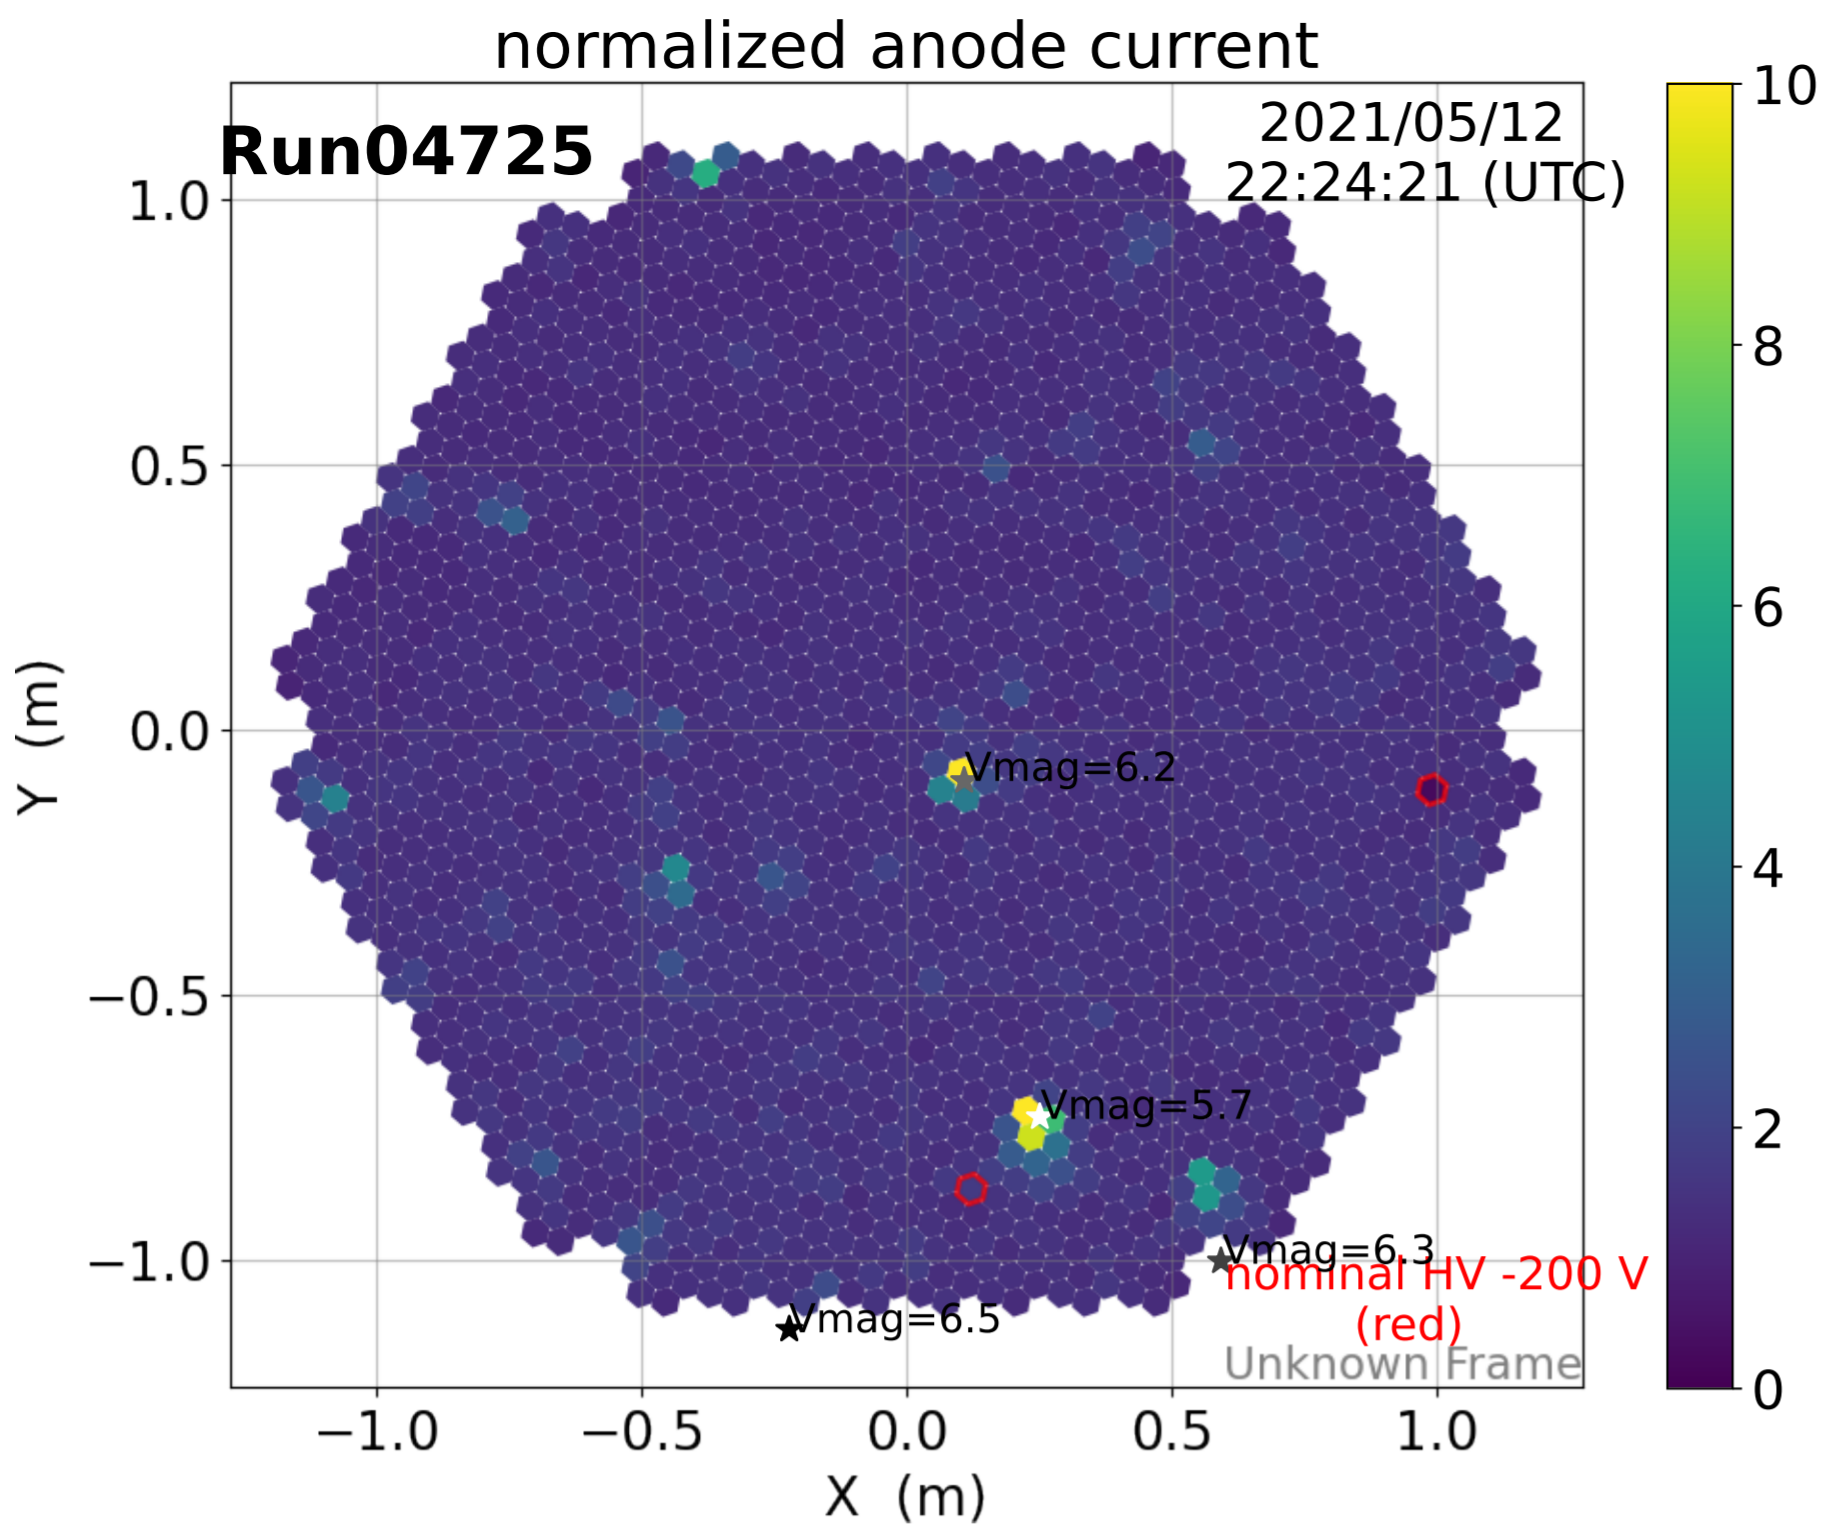


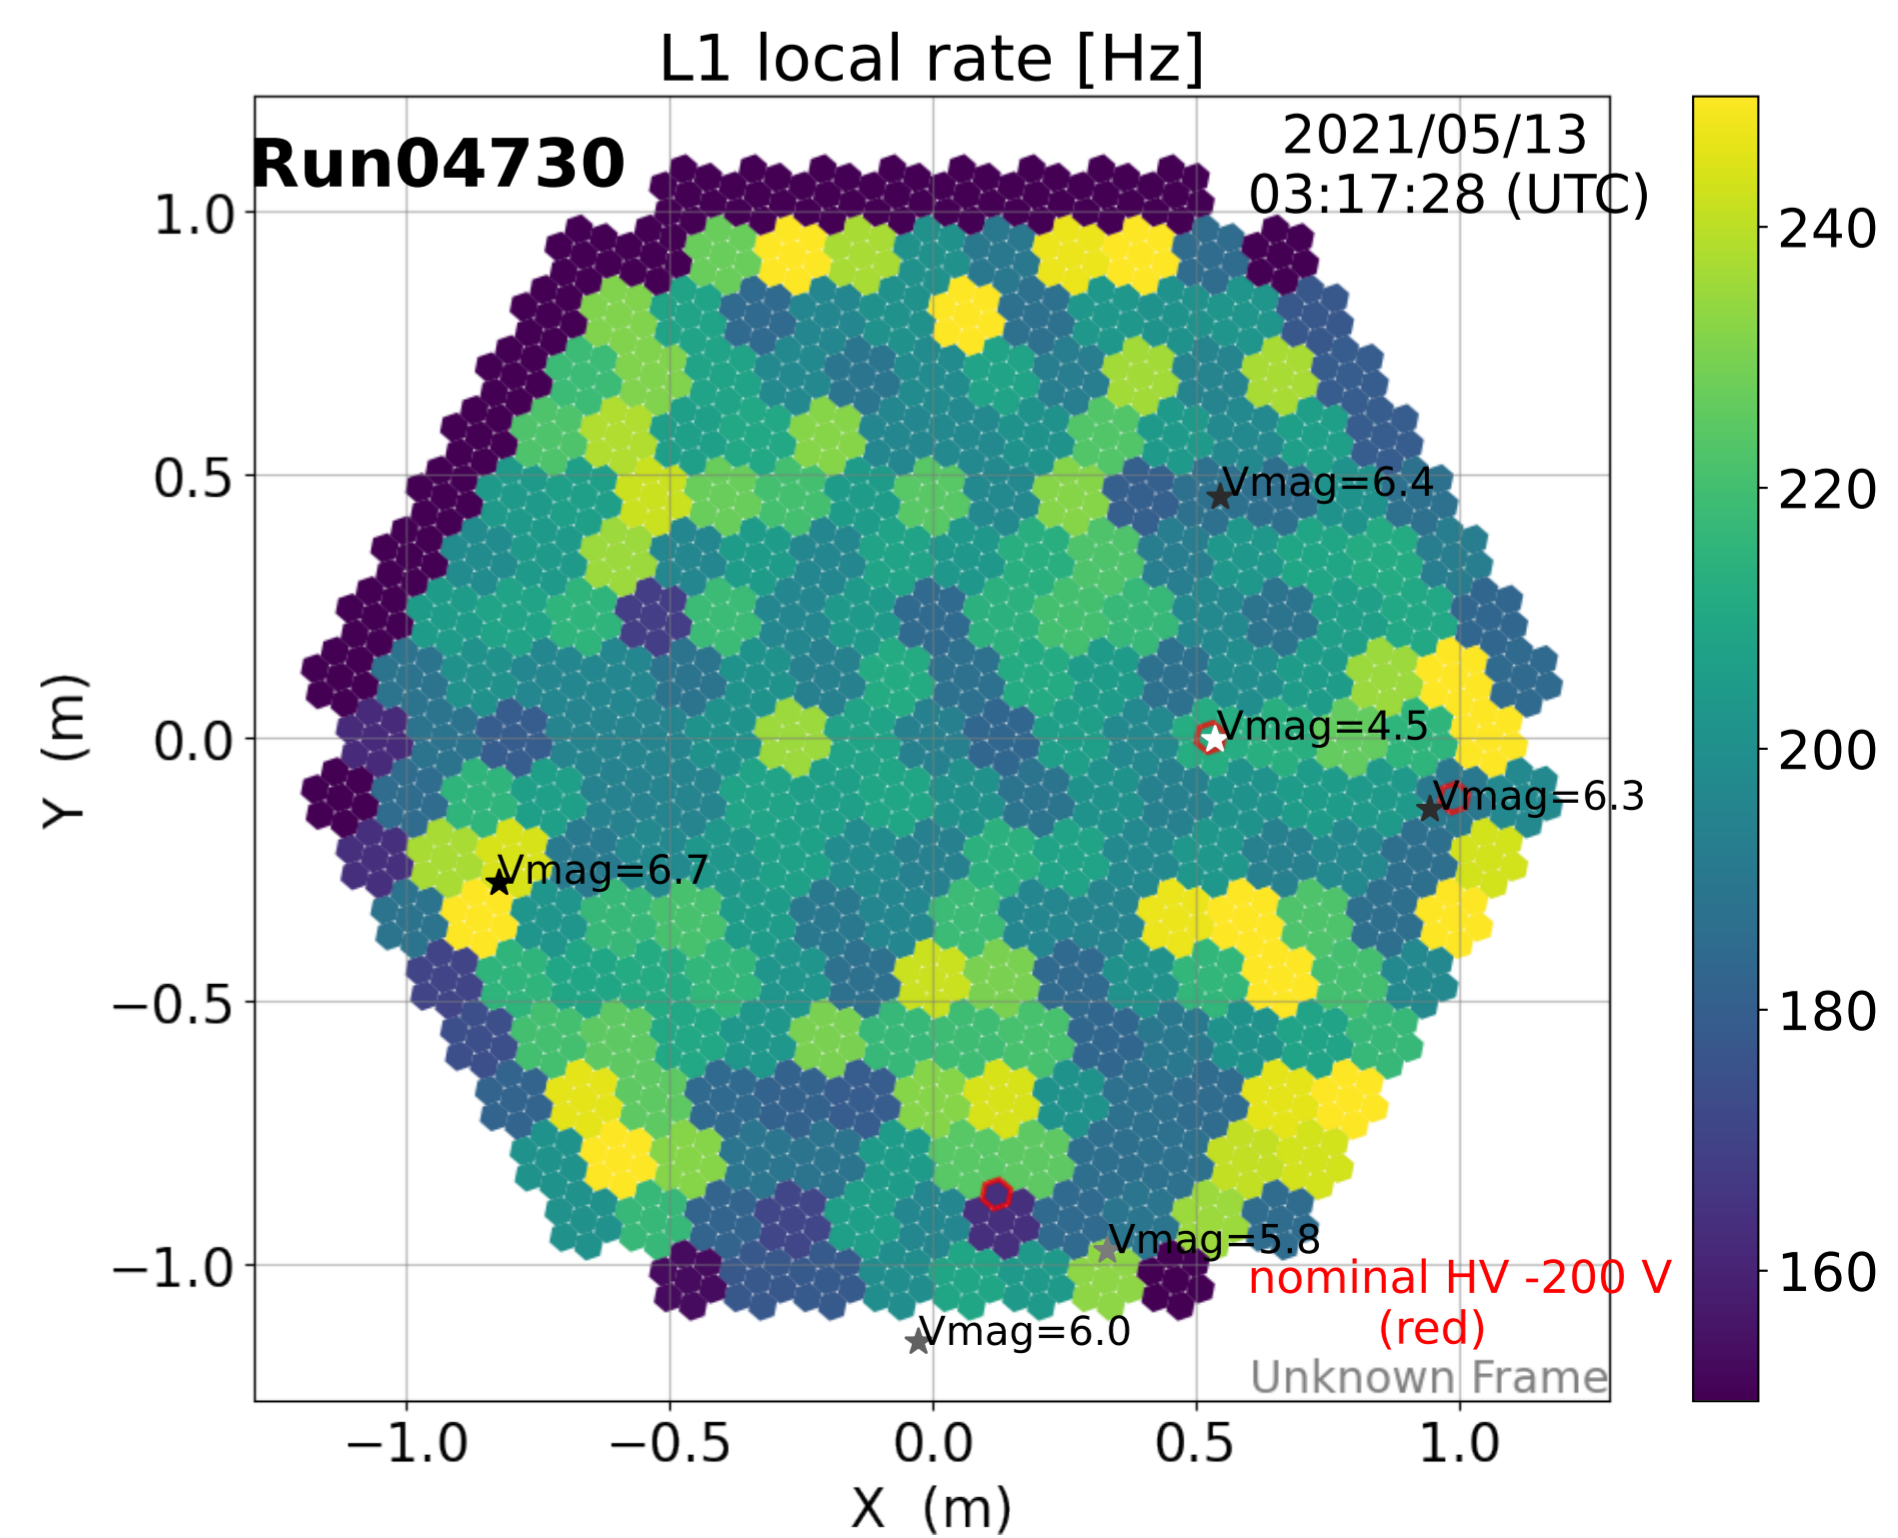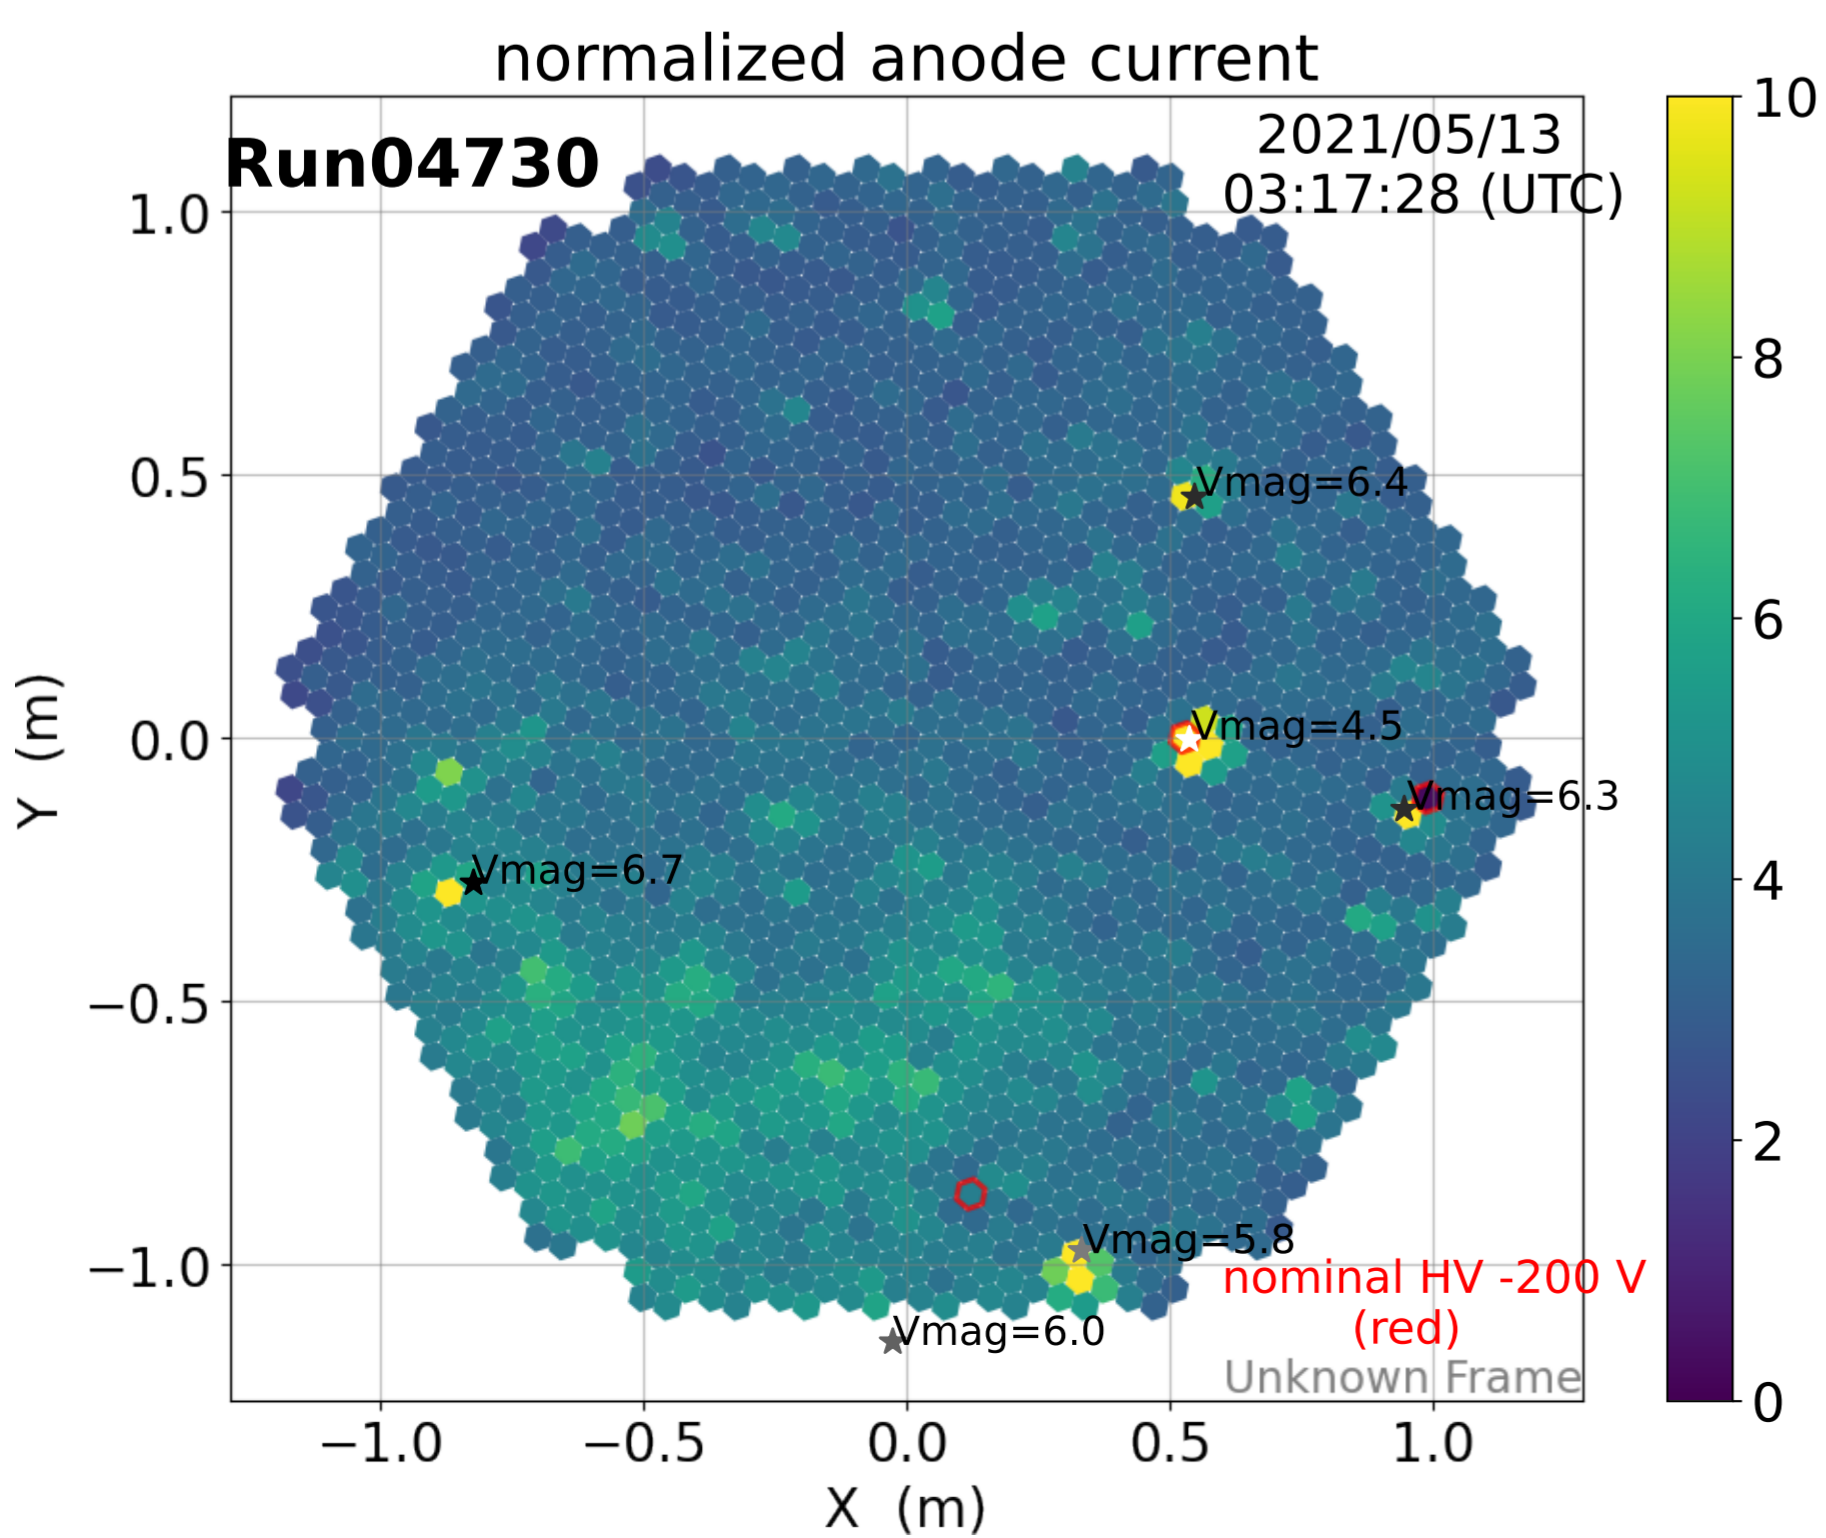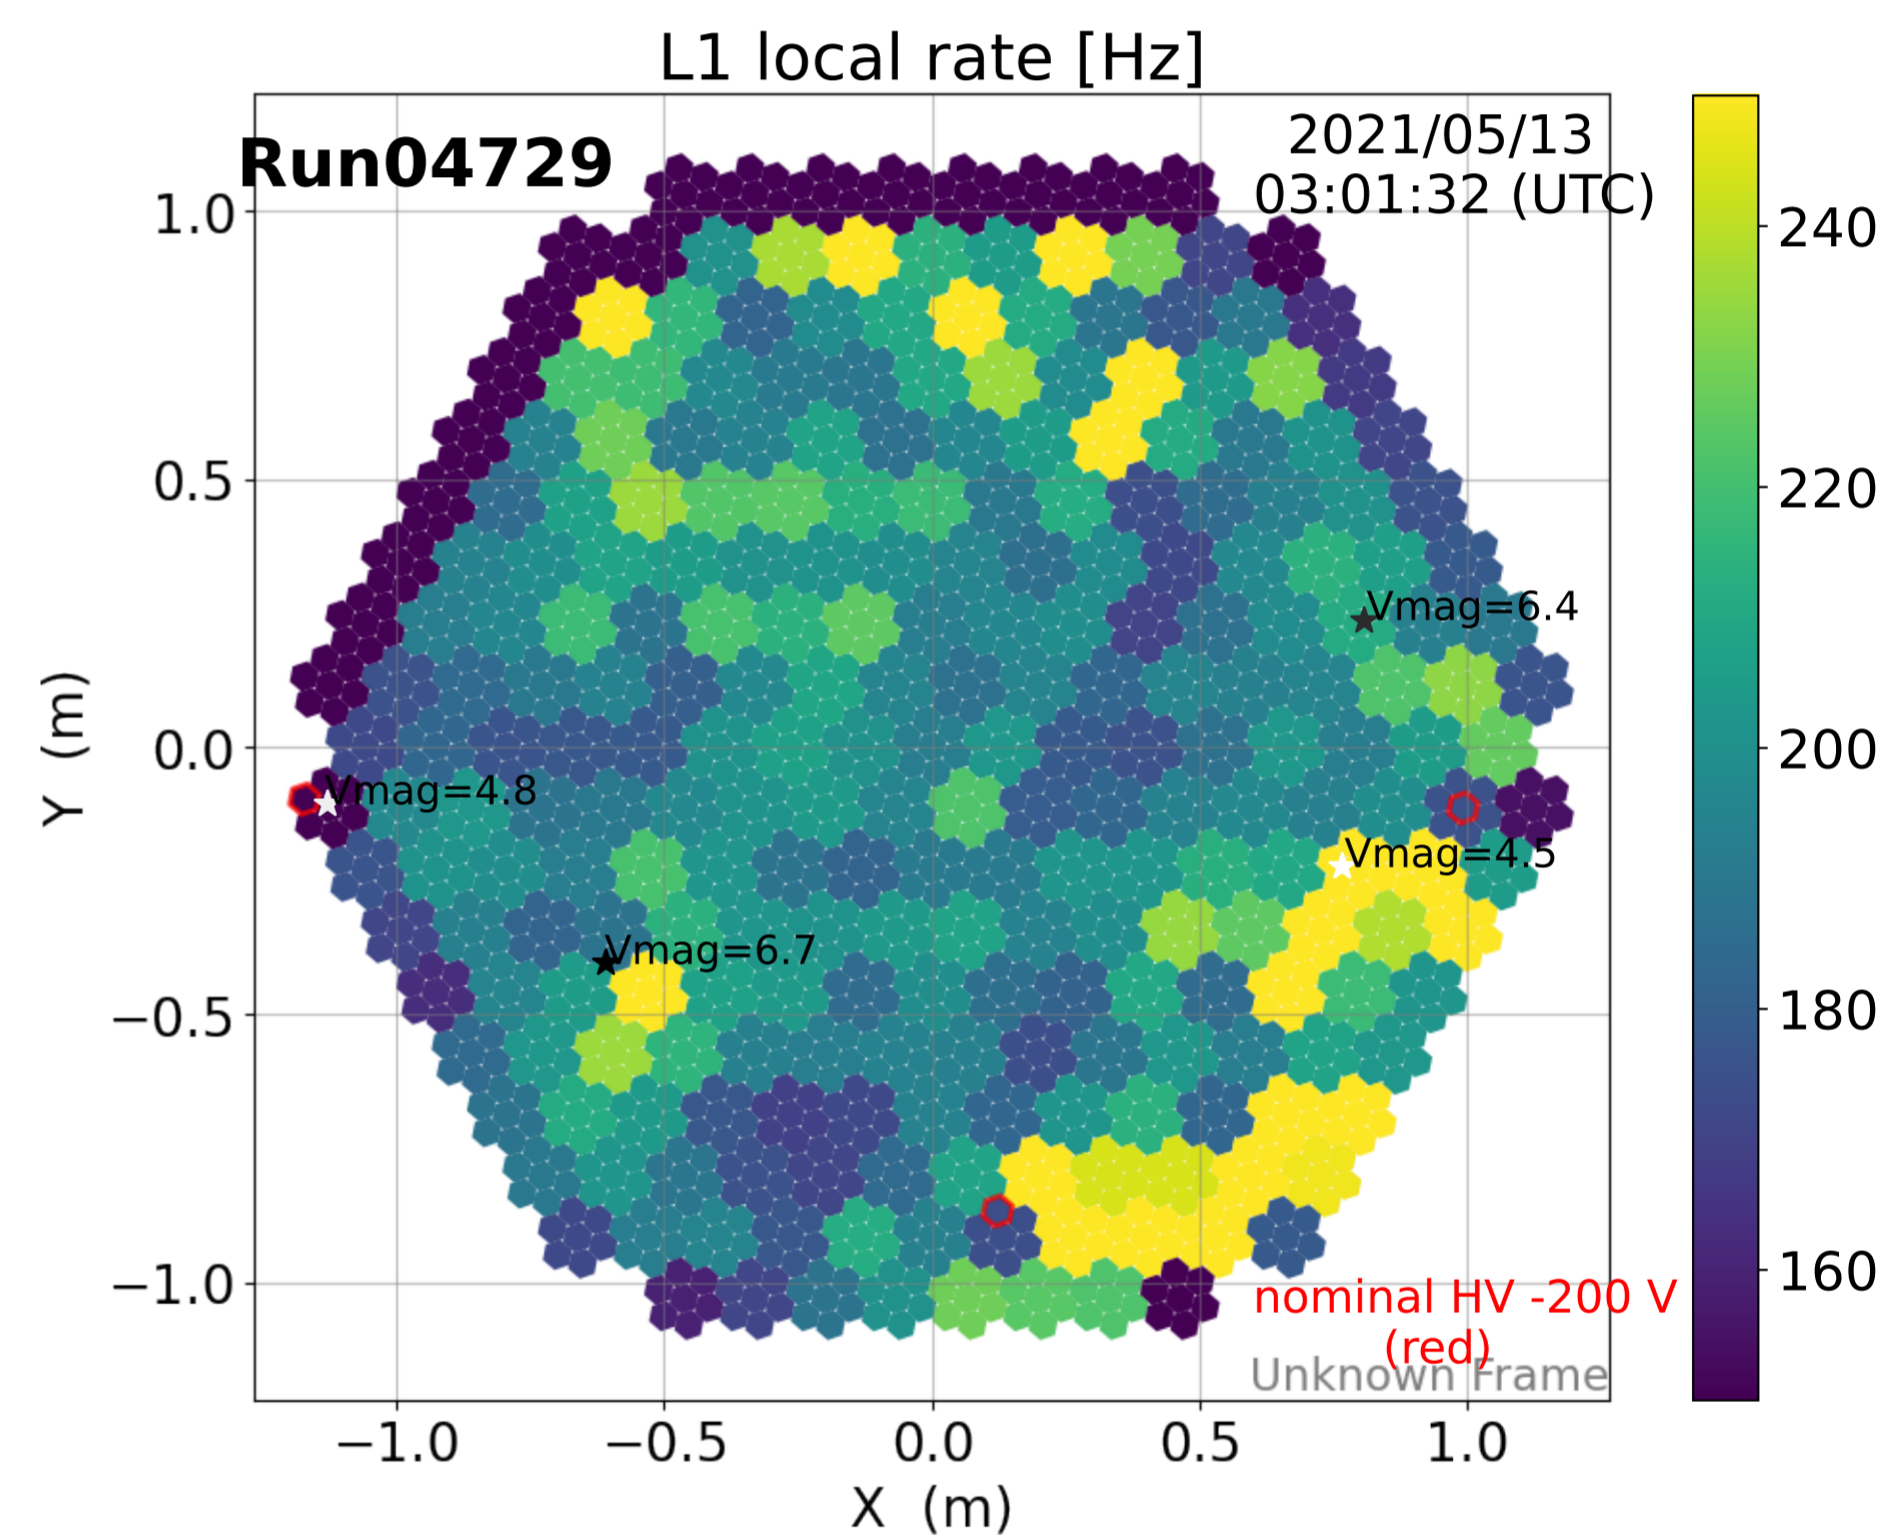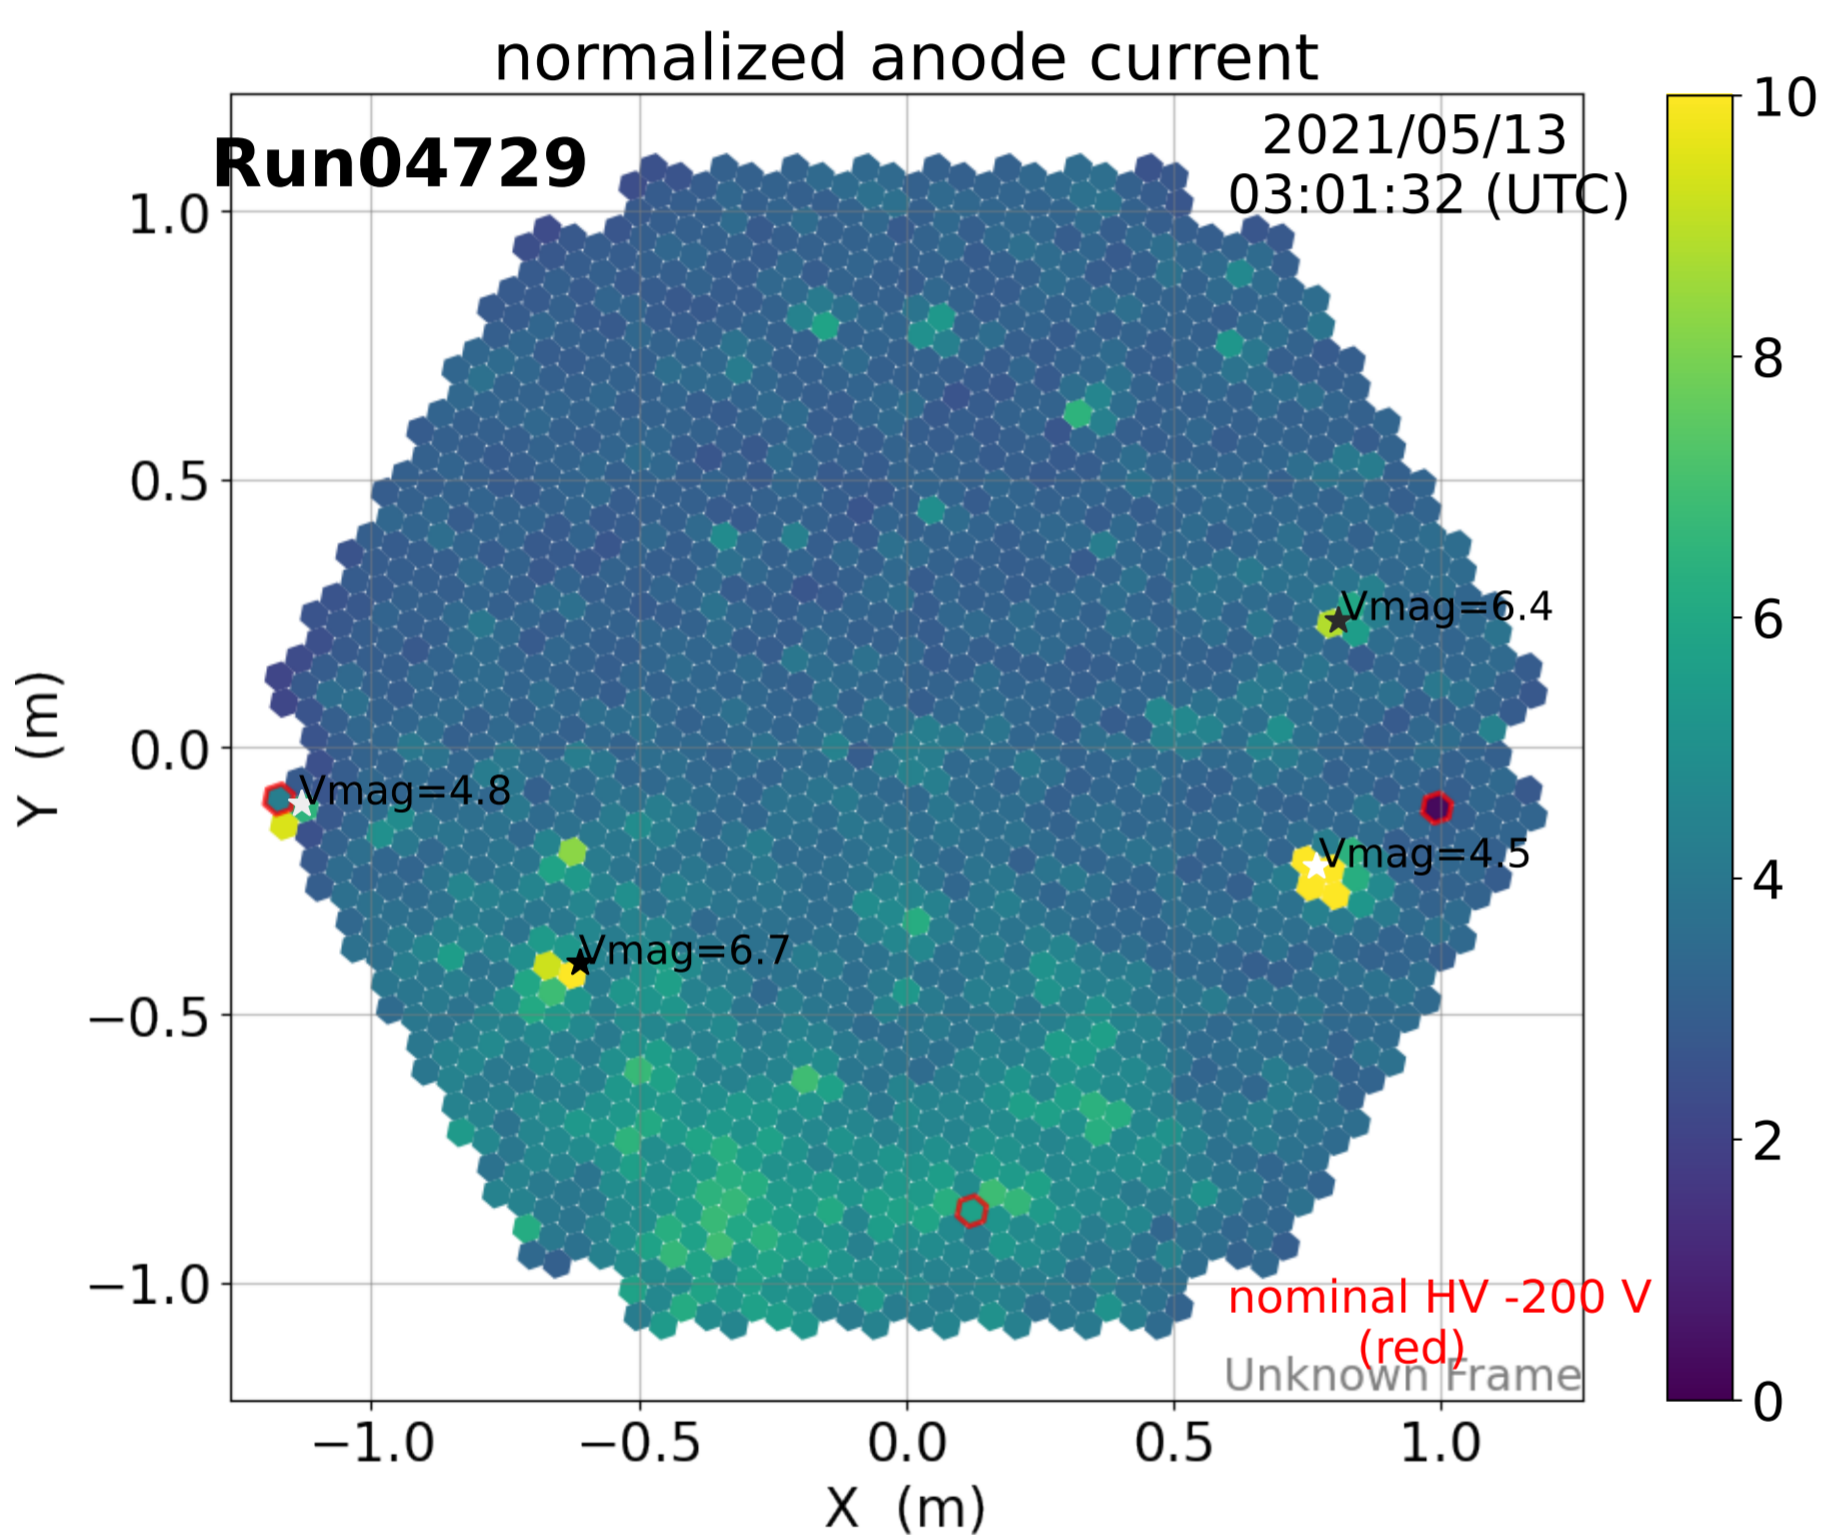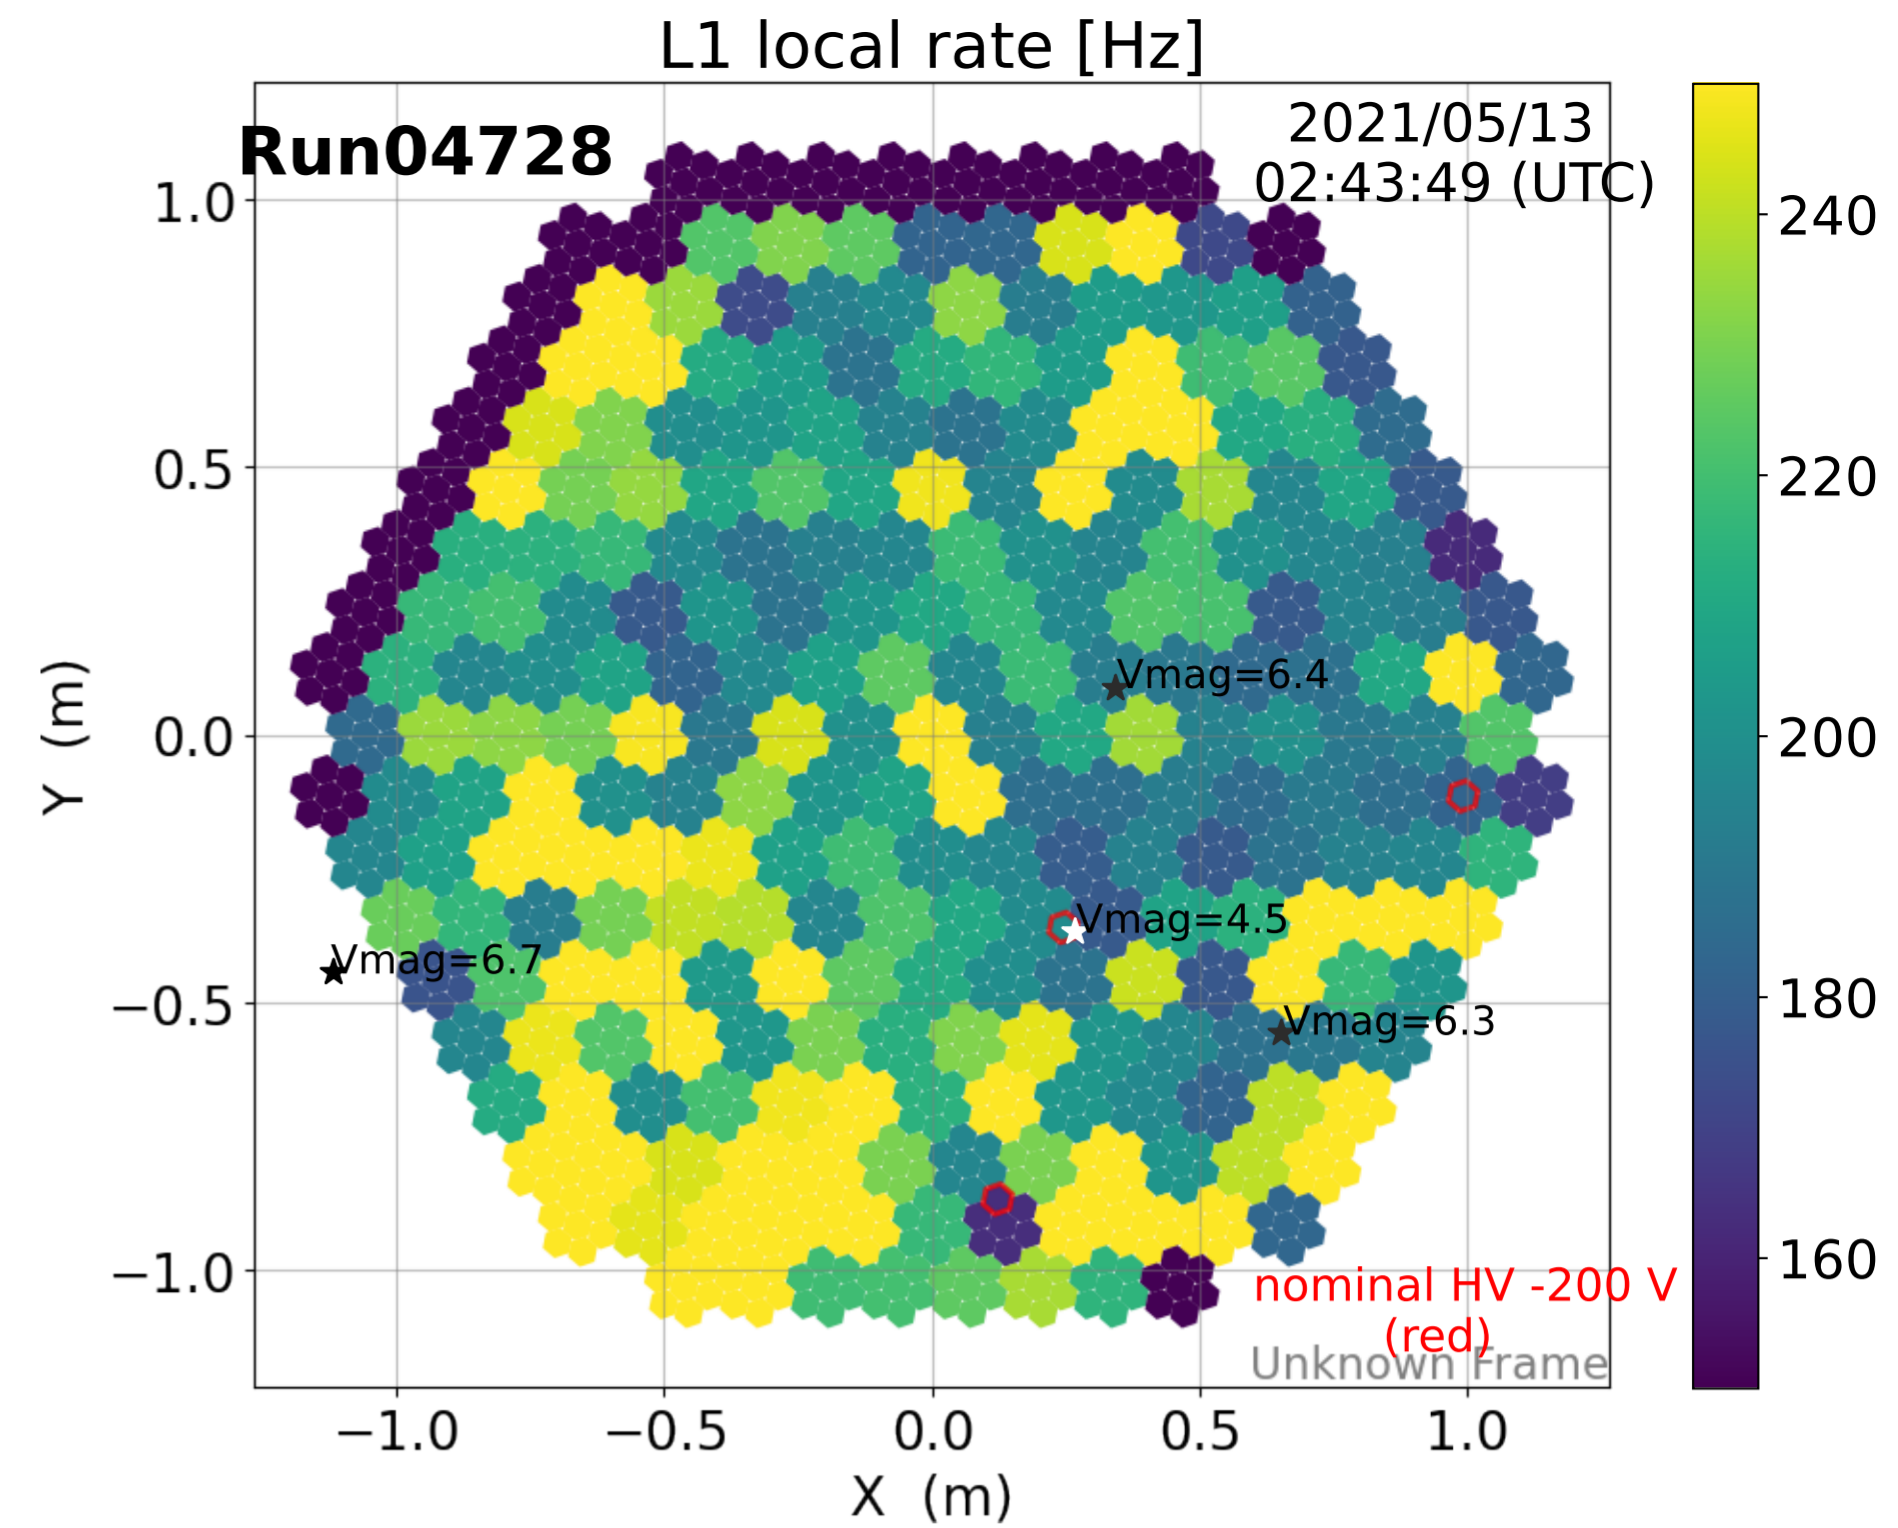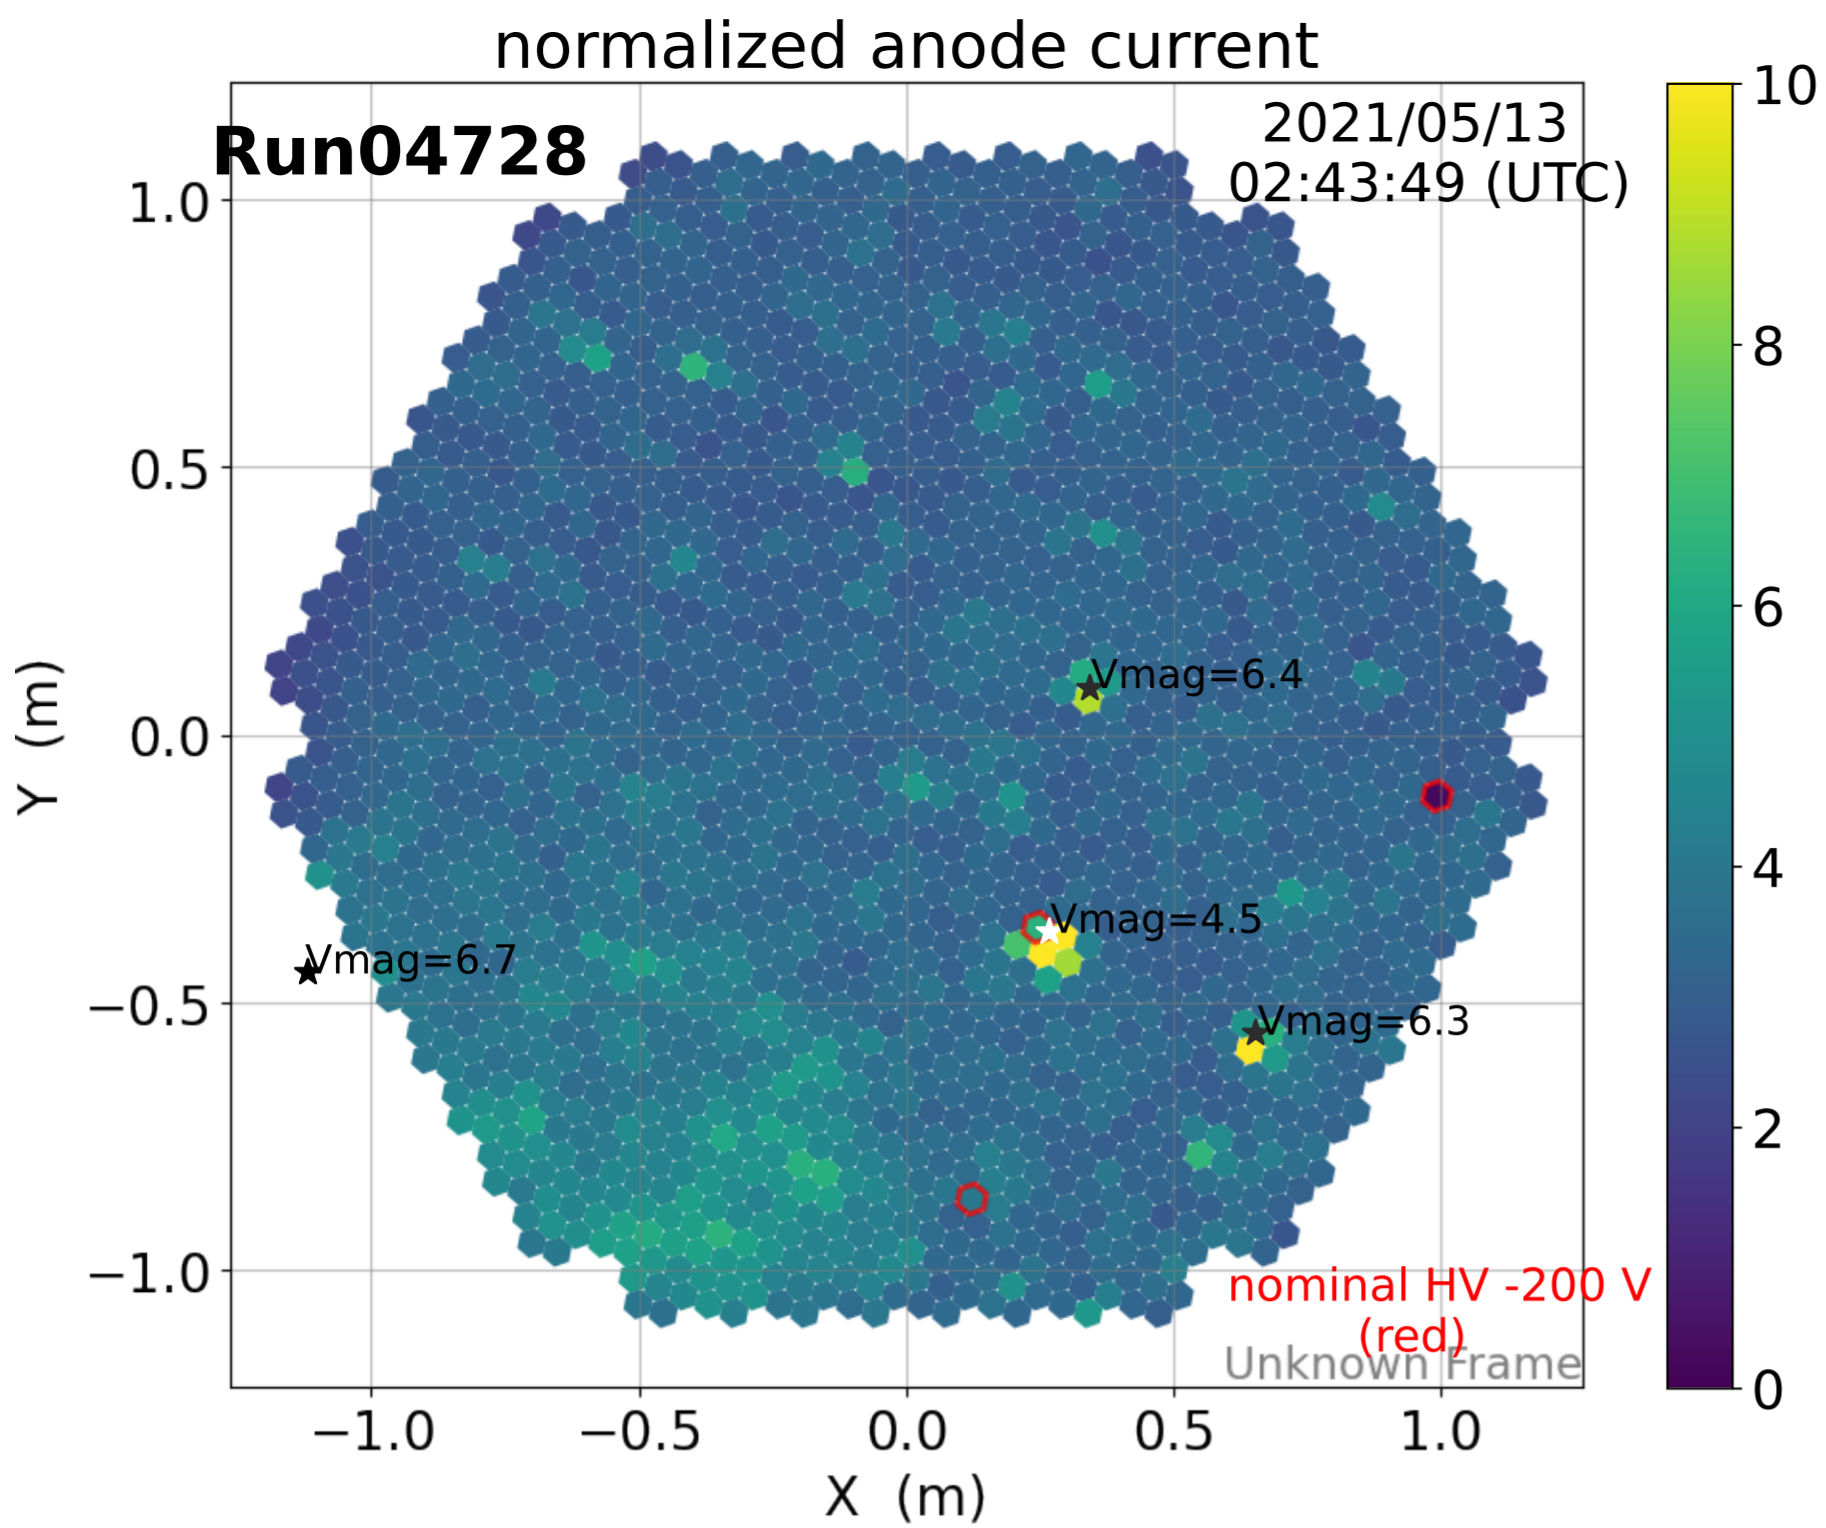

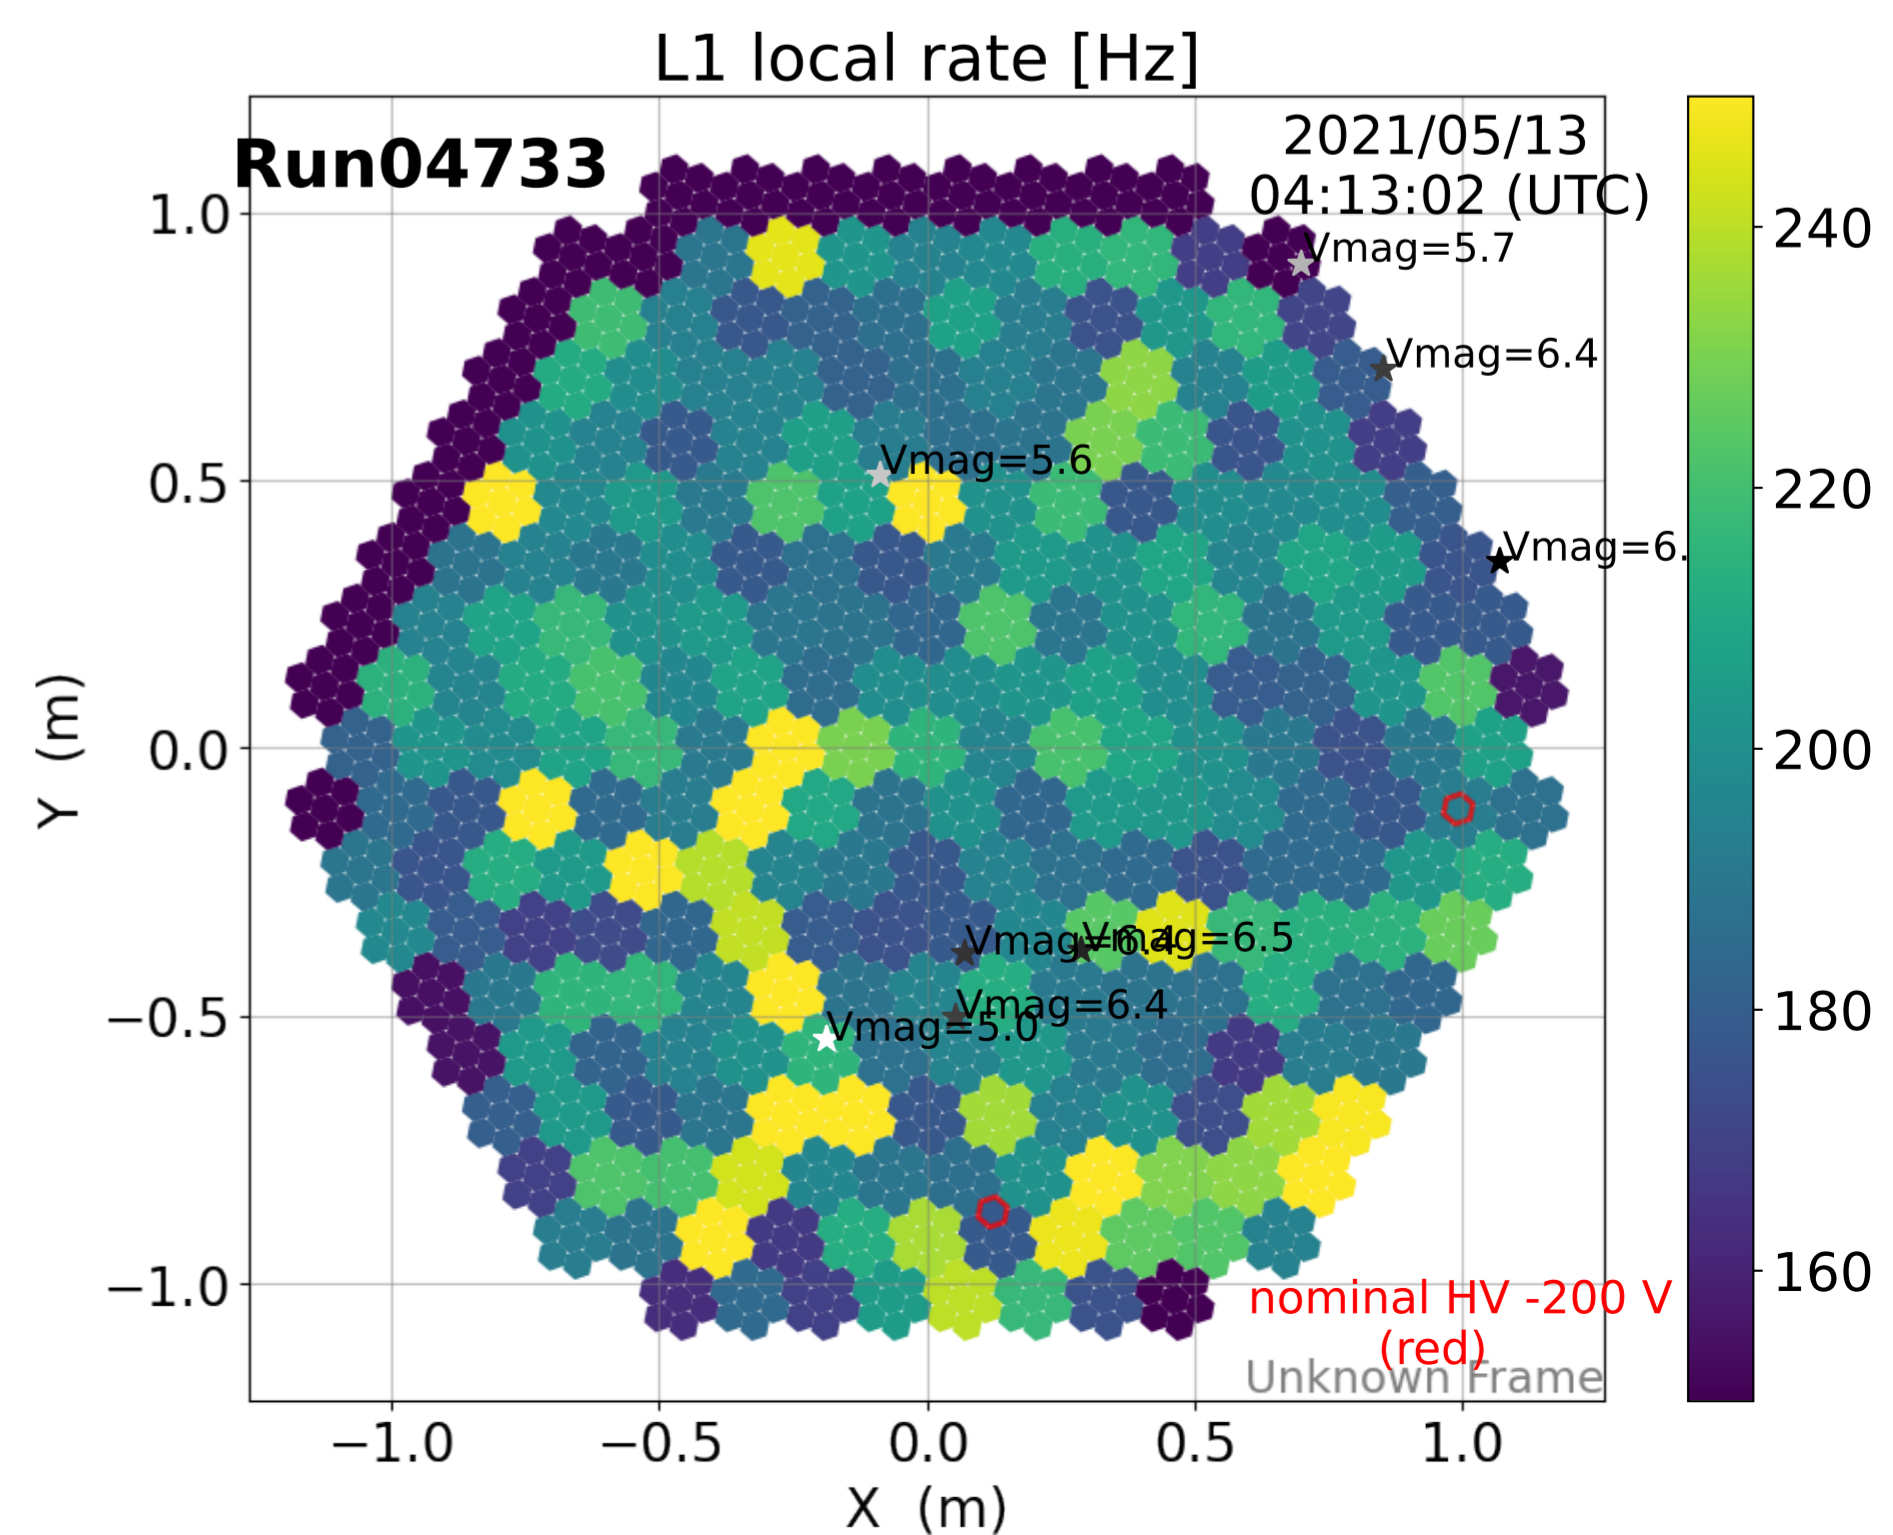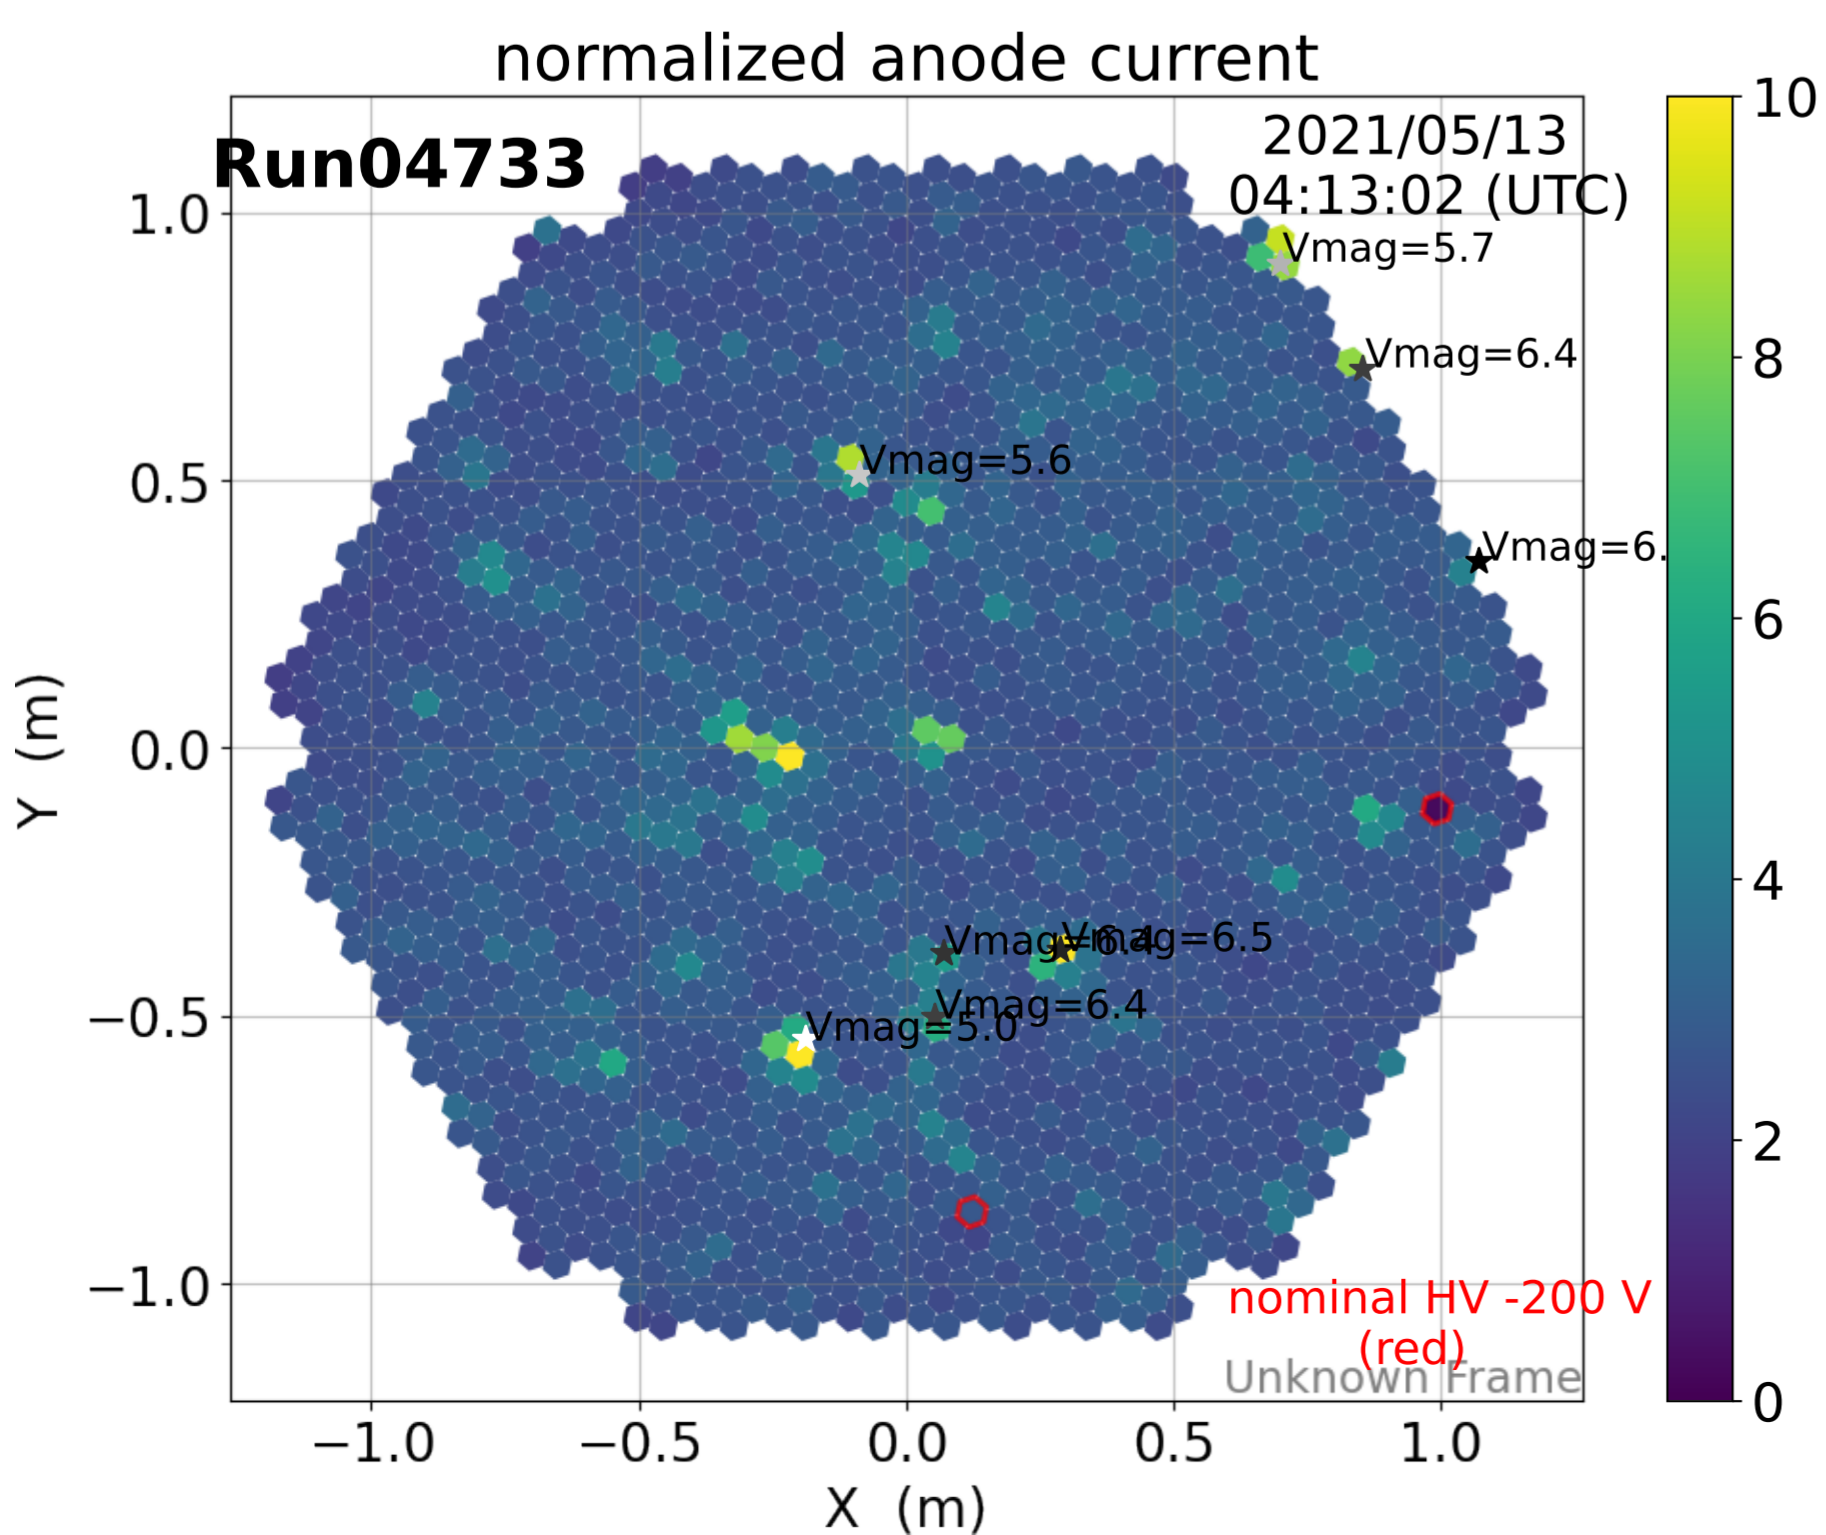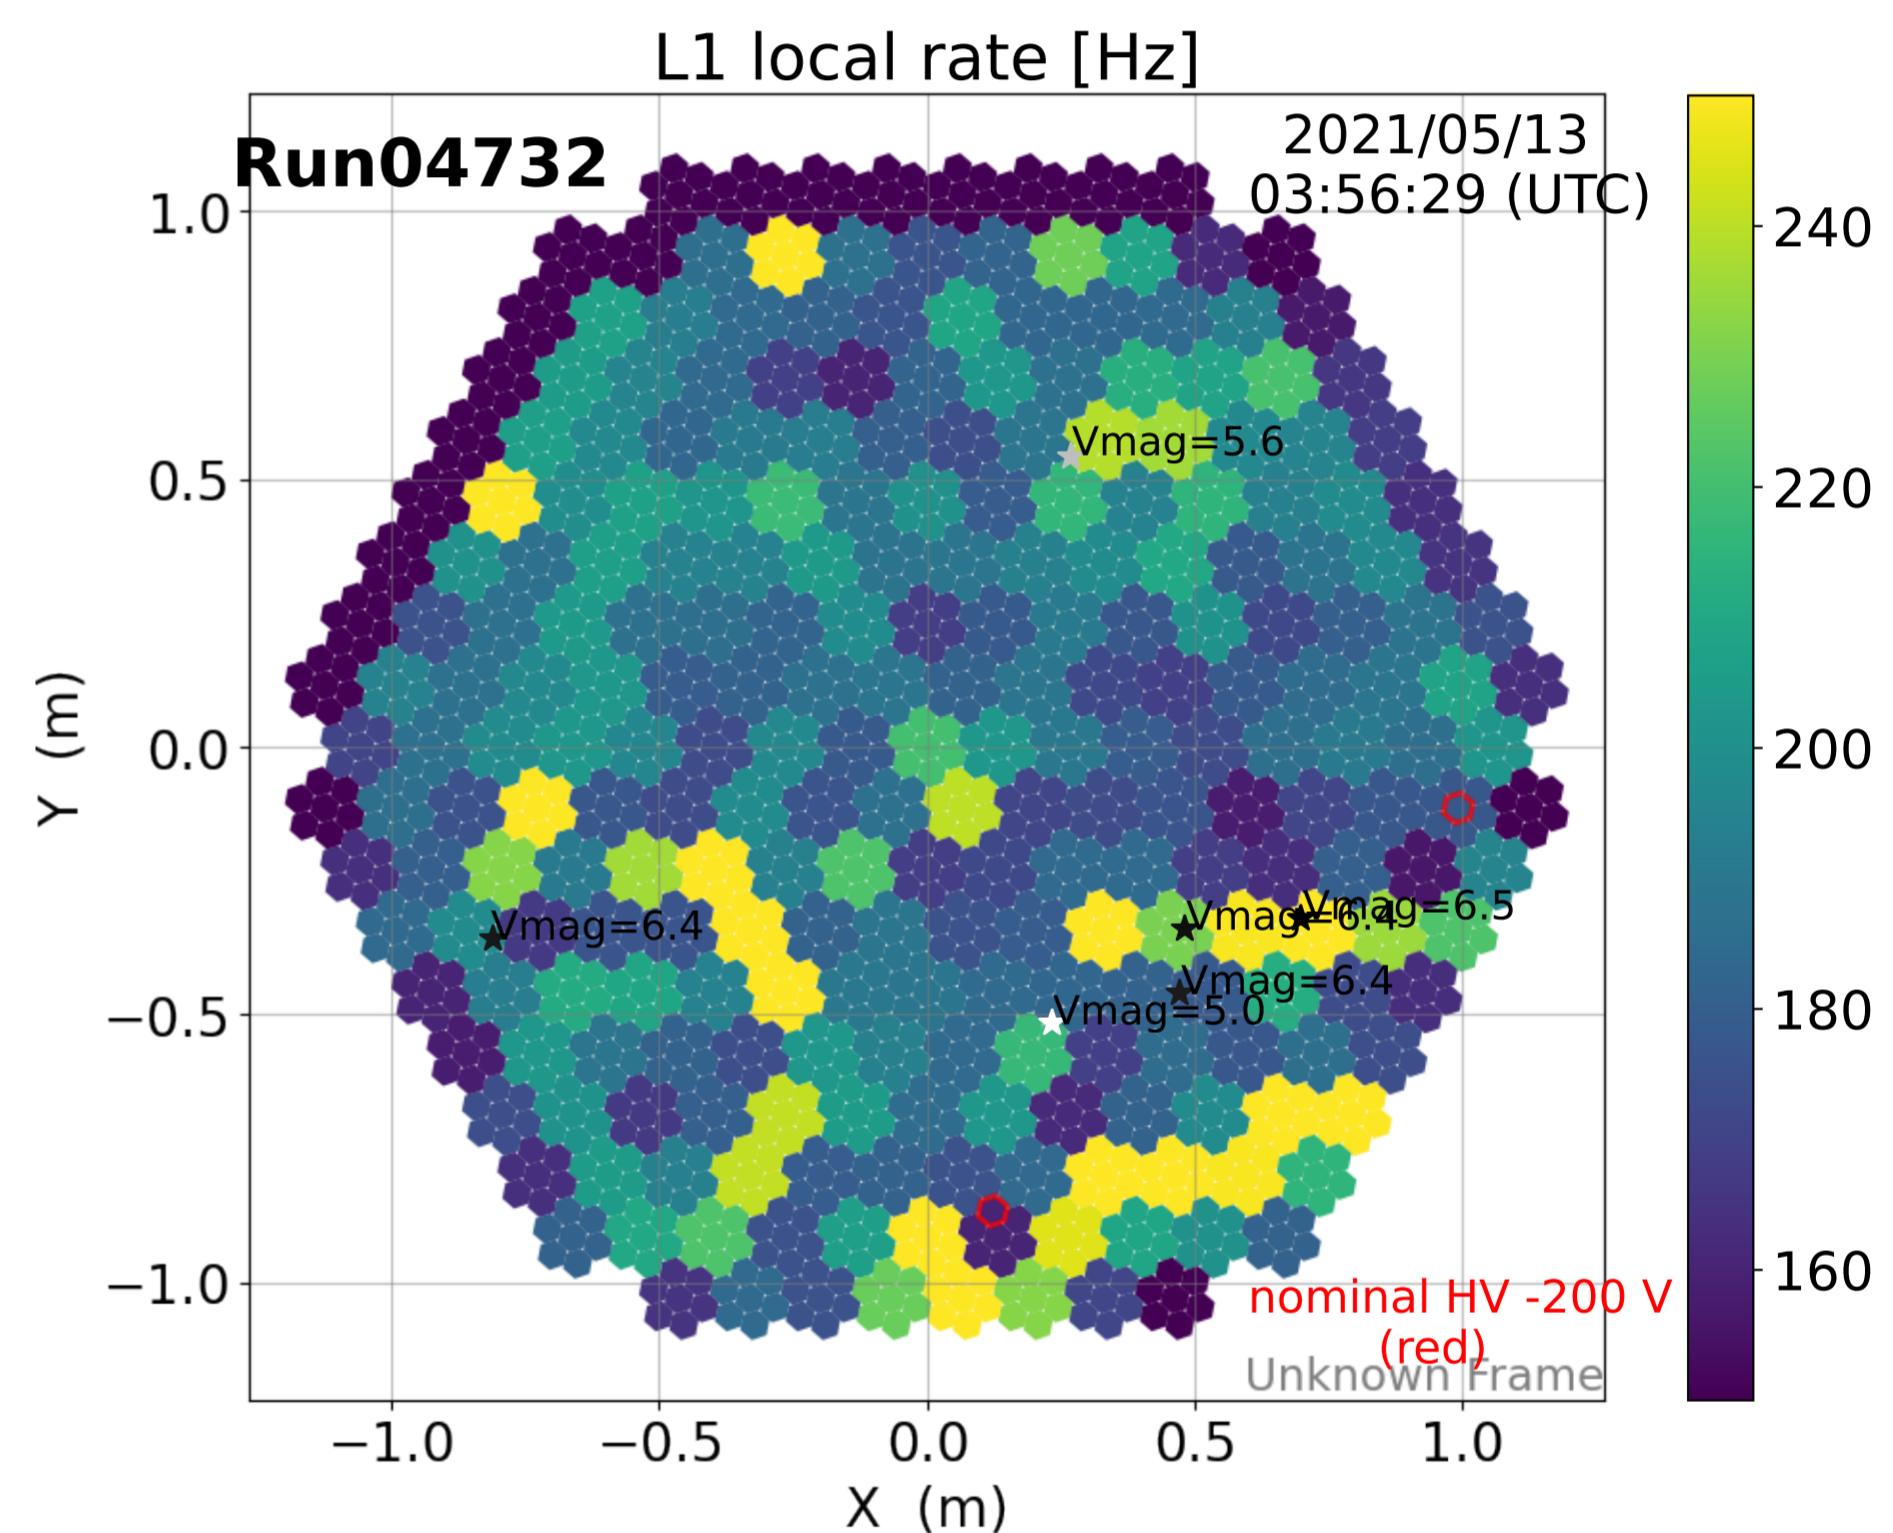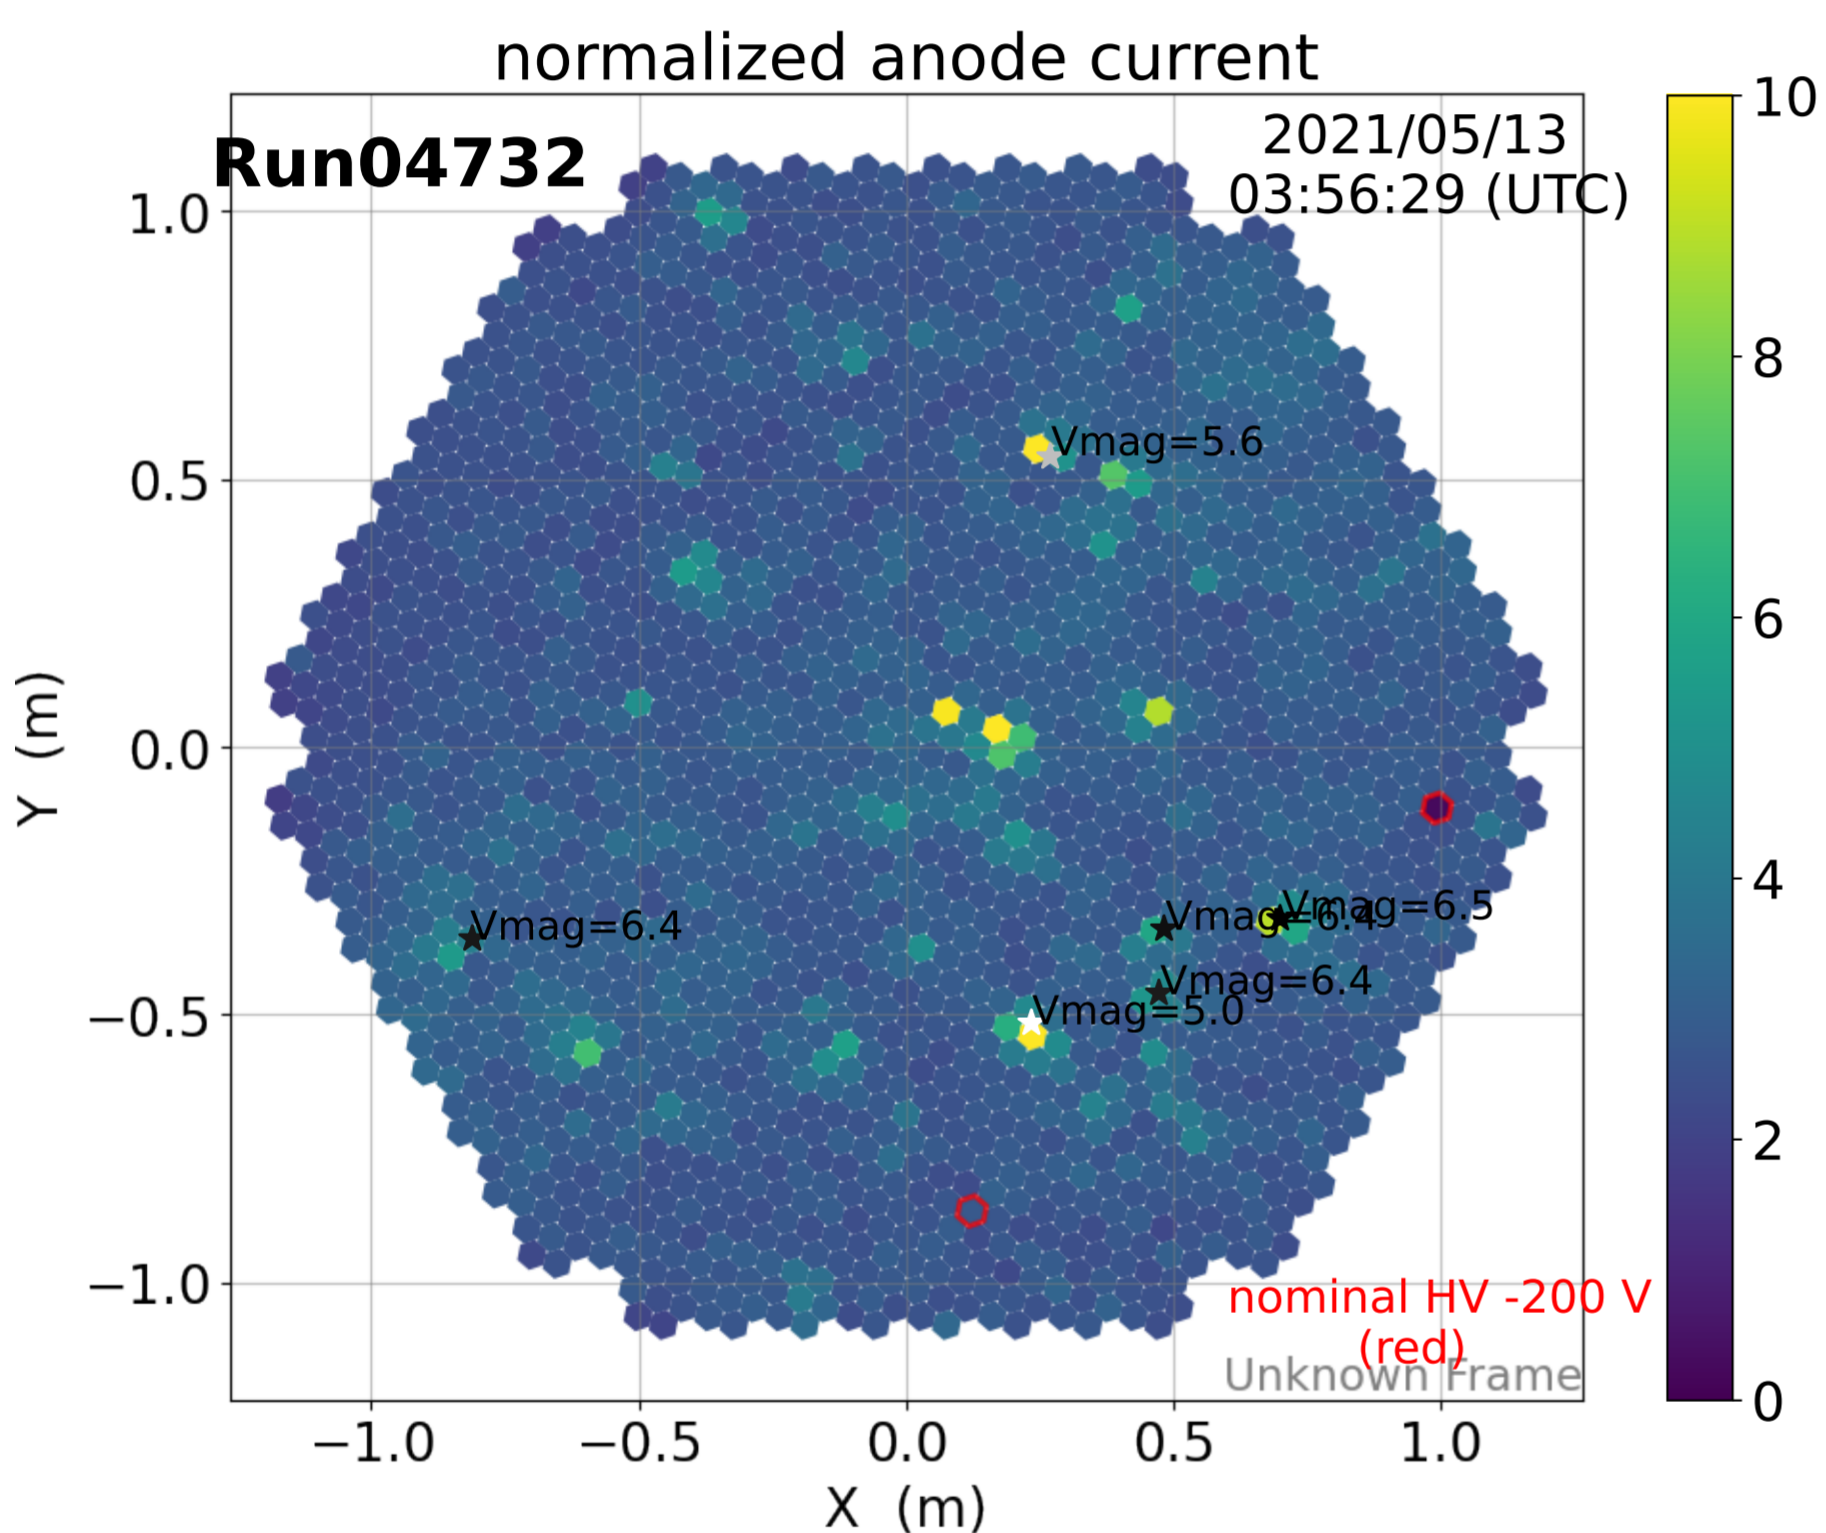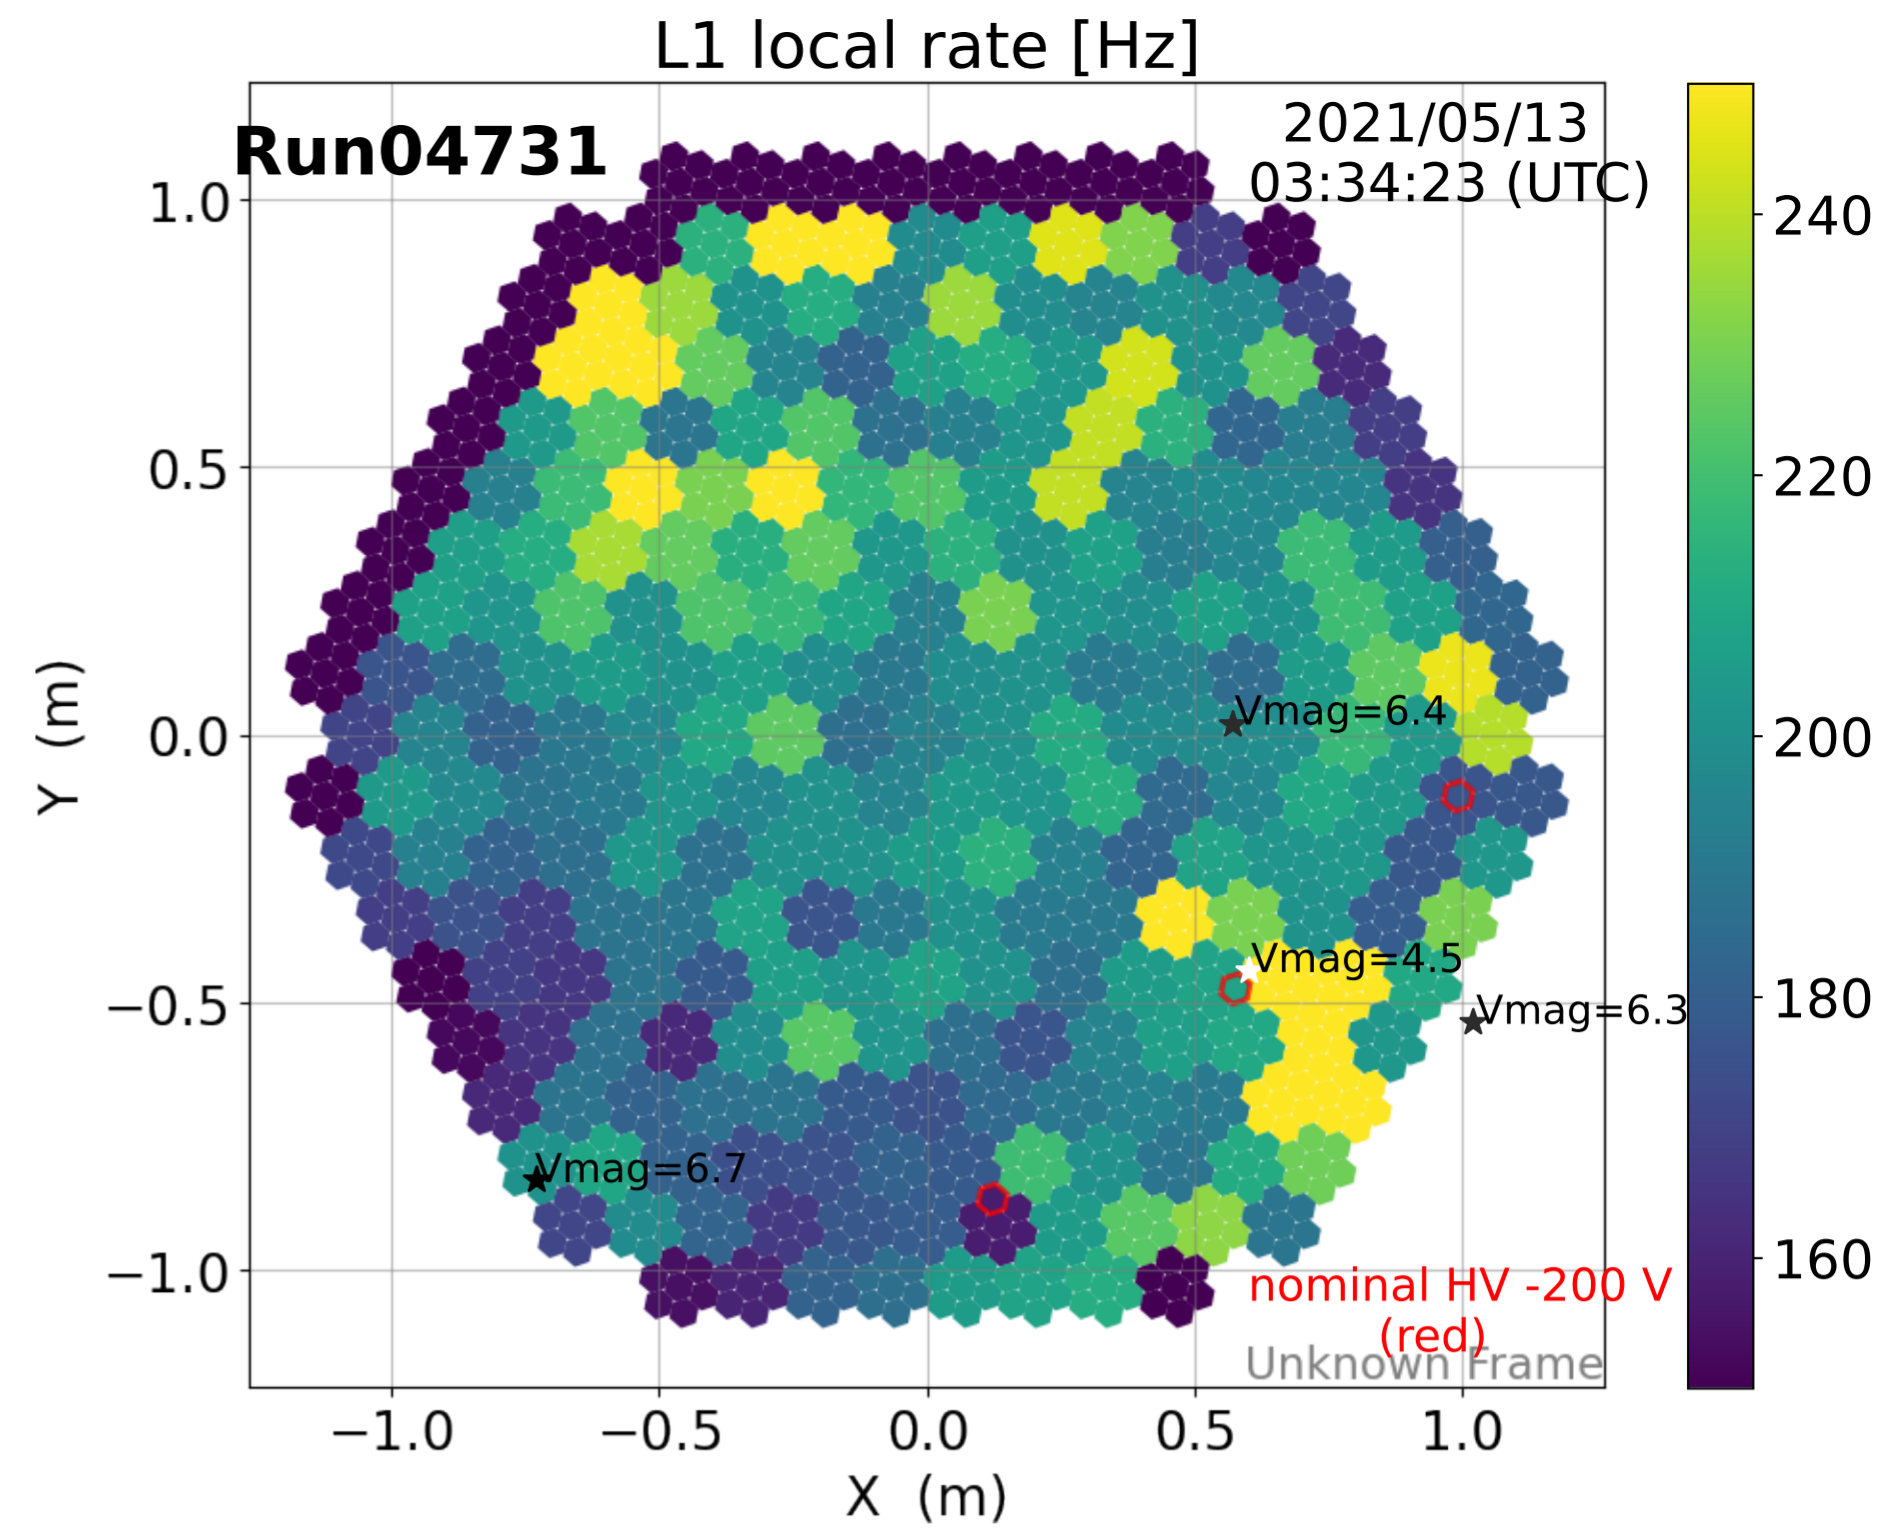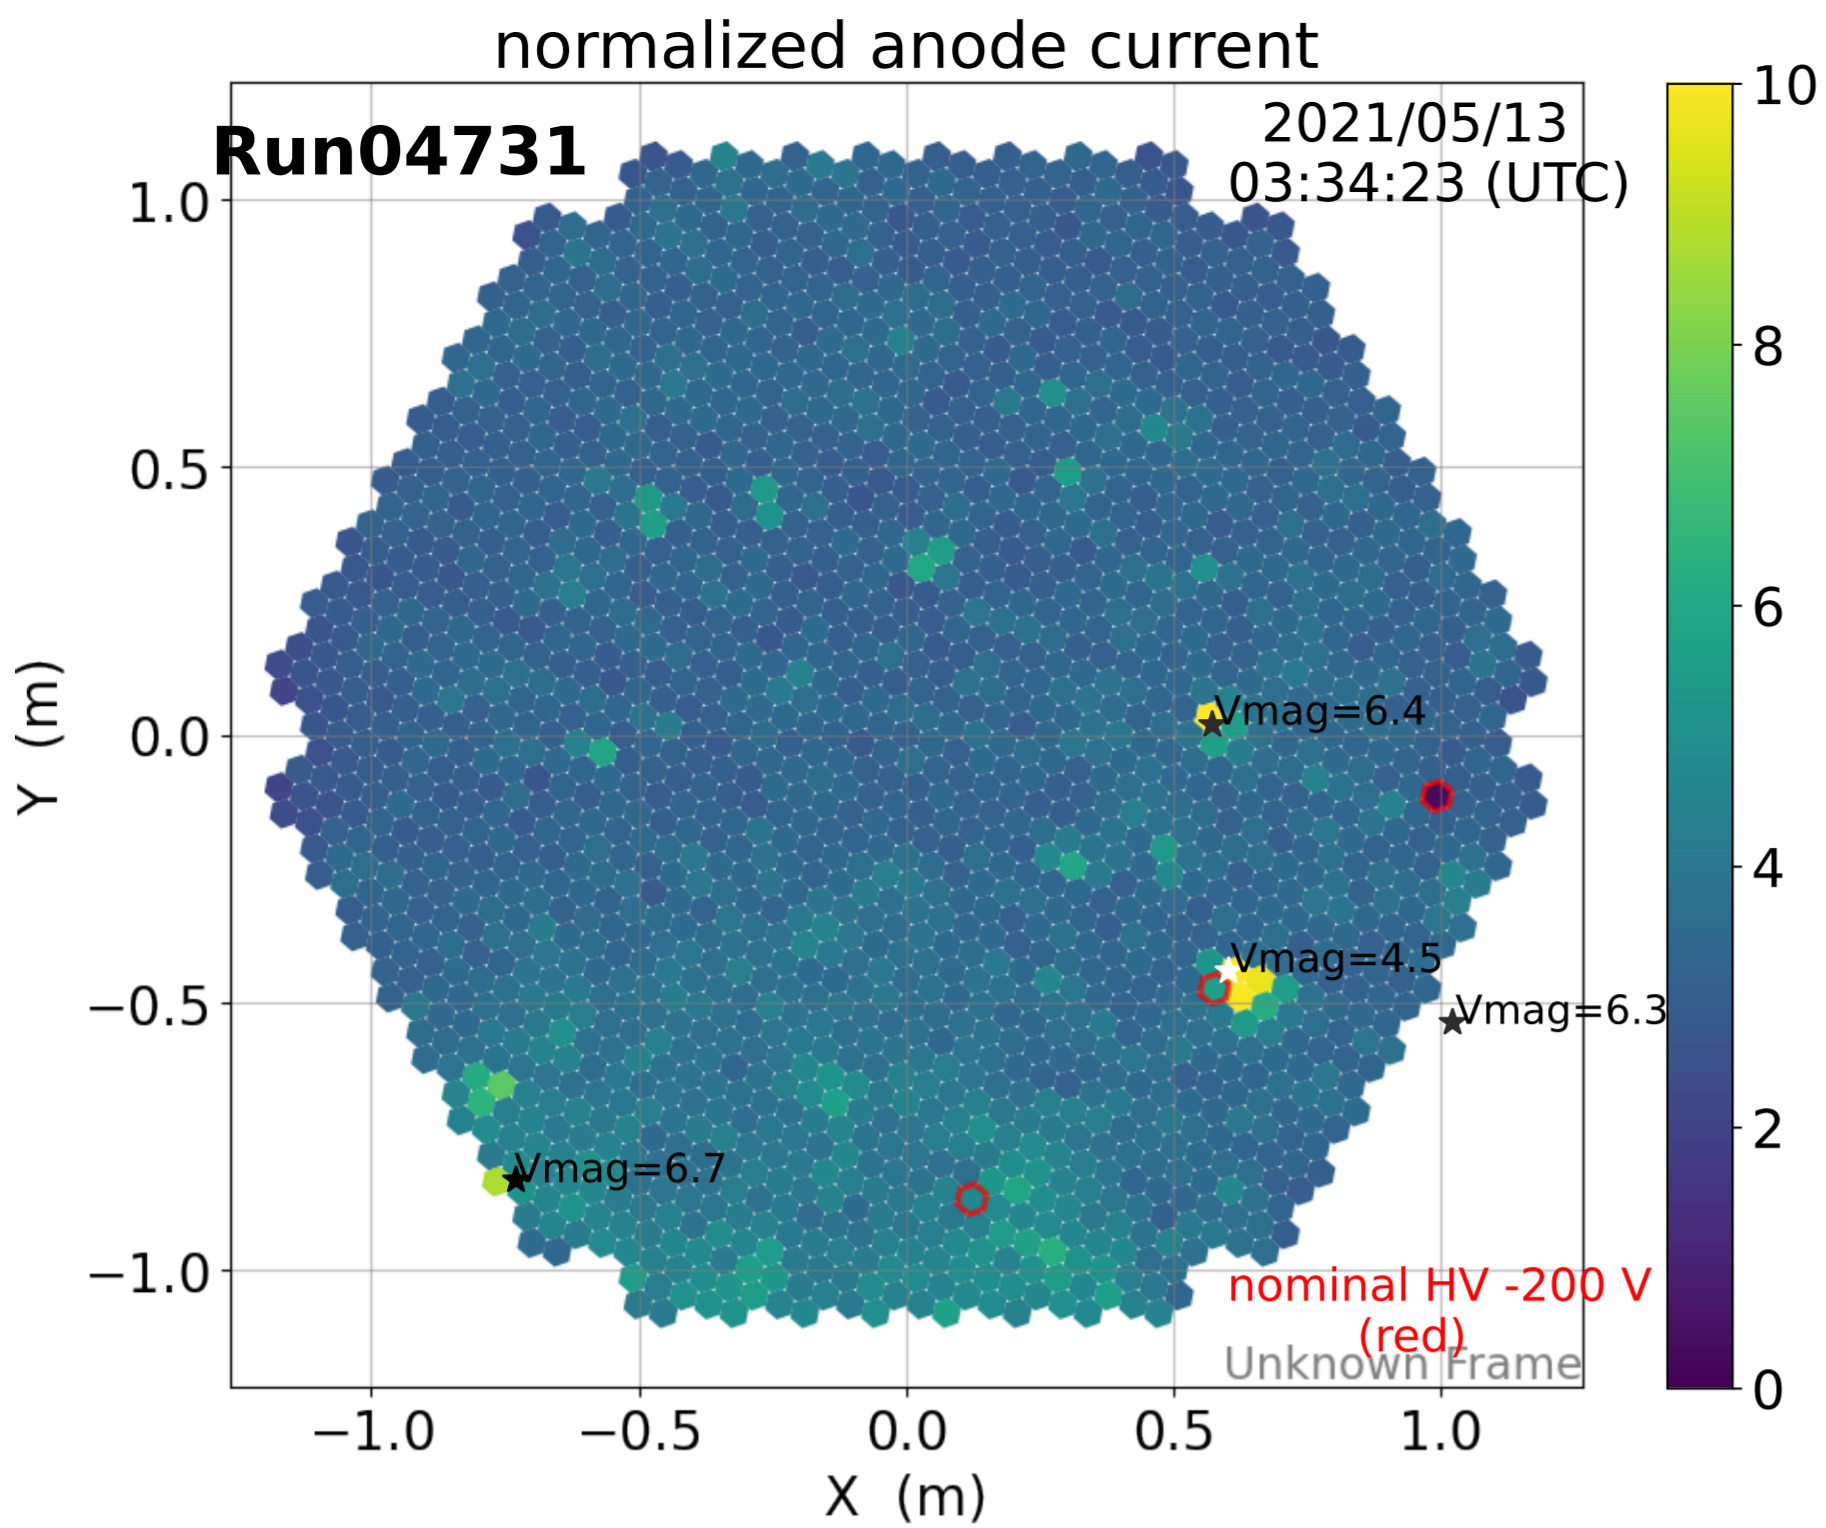





normalized anode current

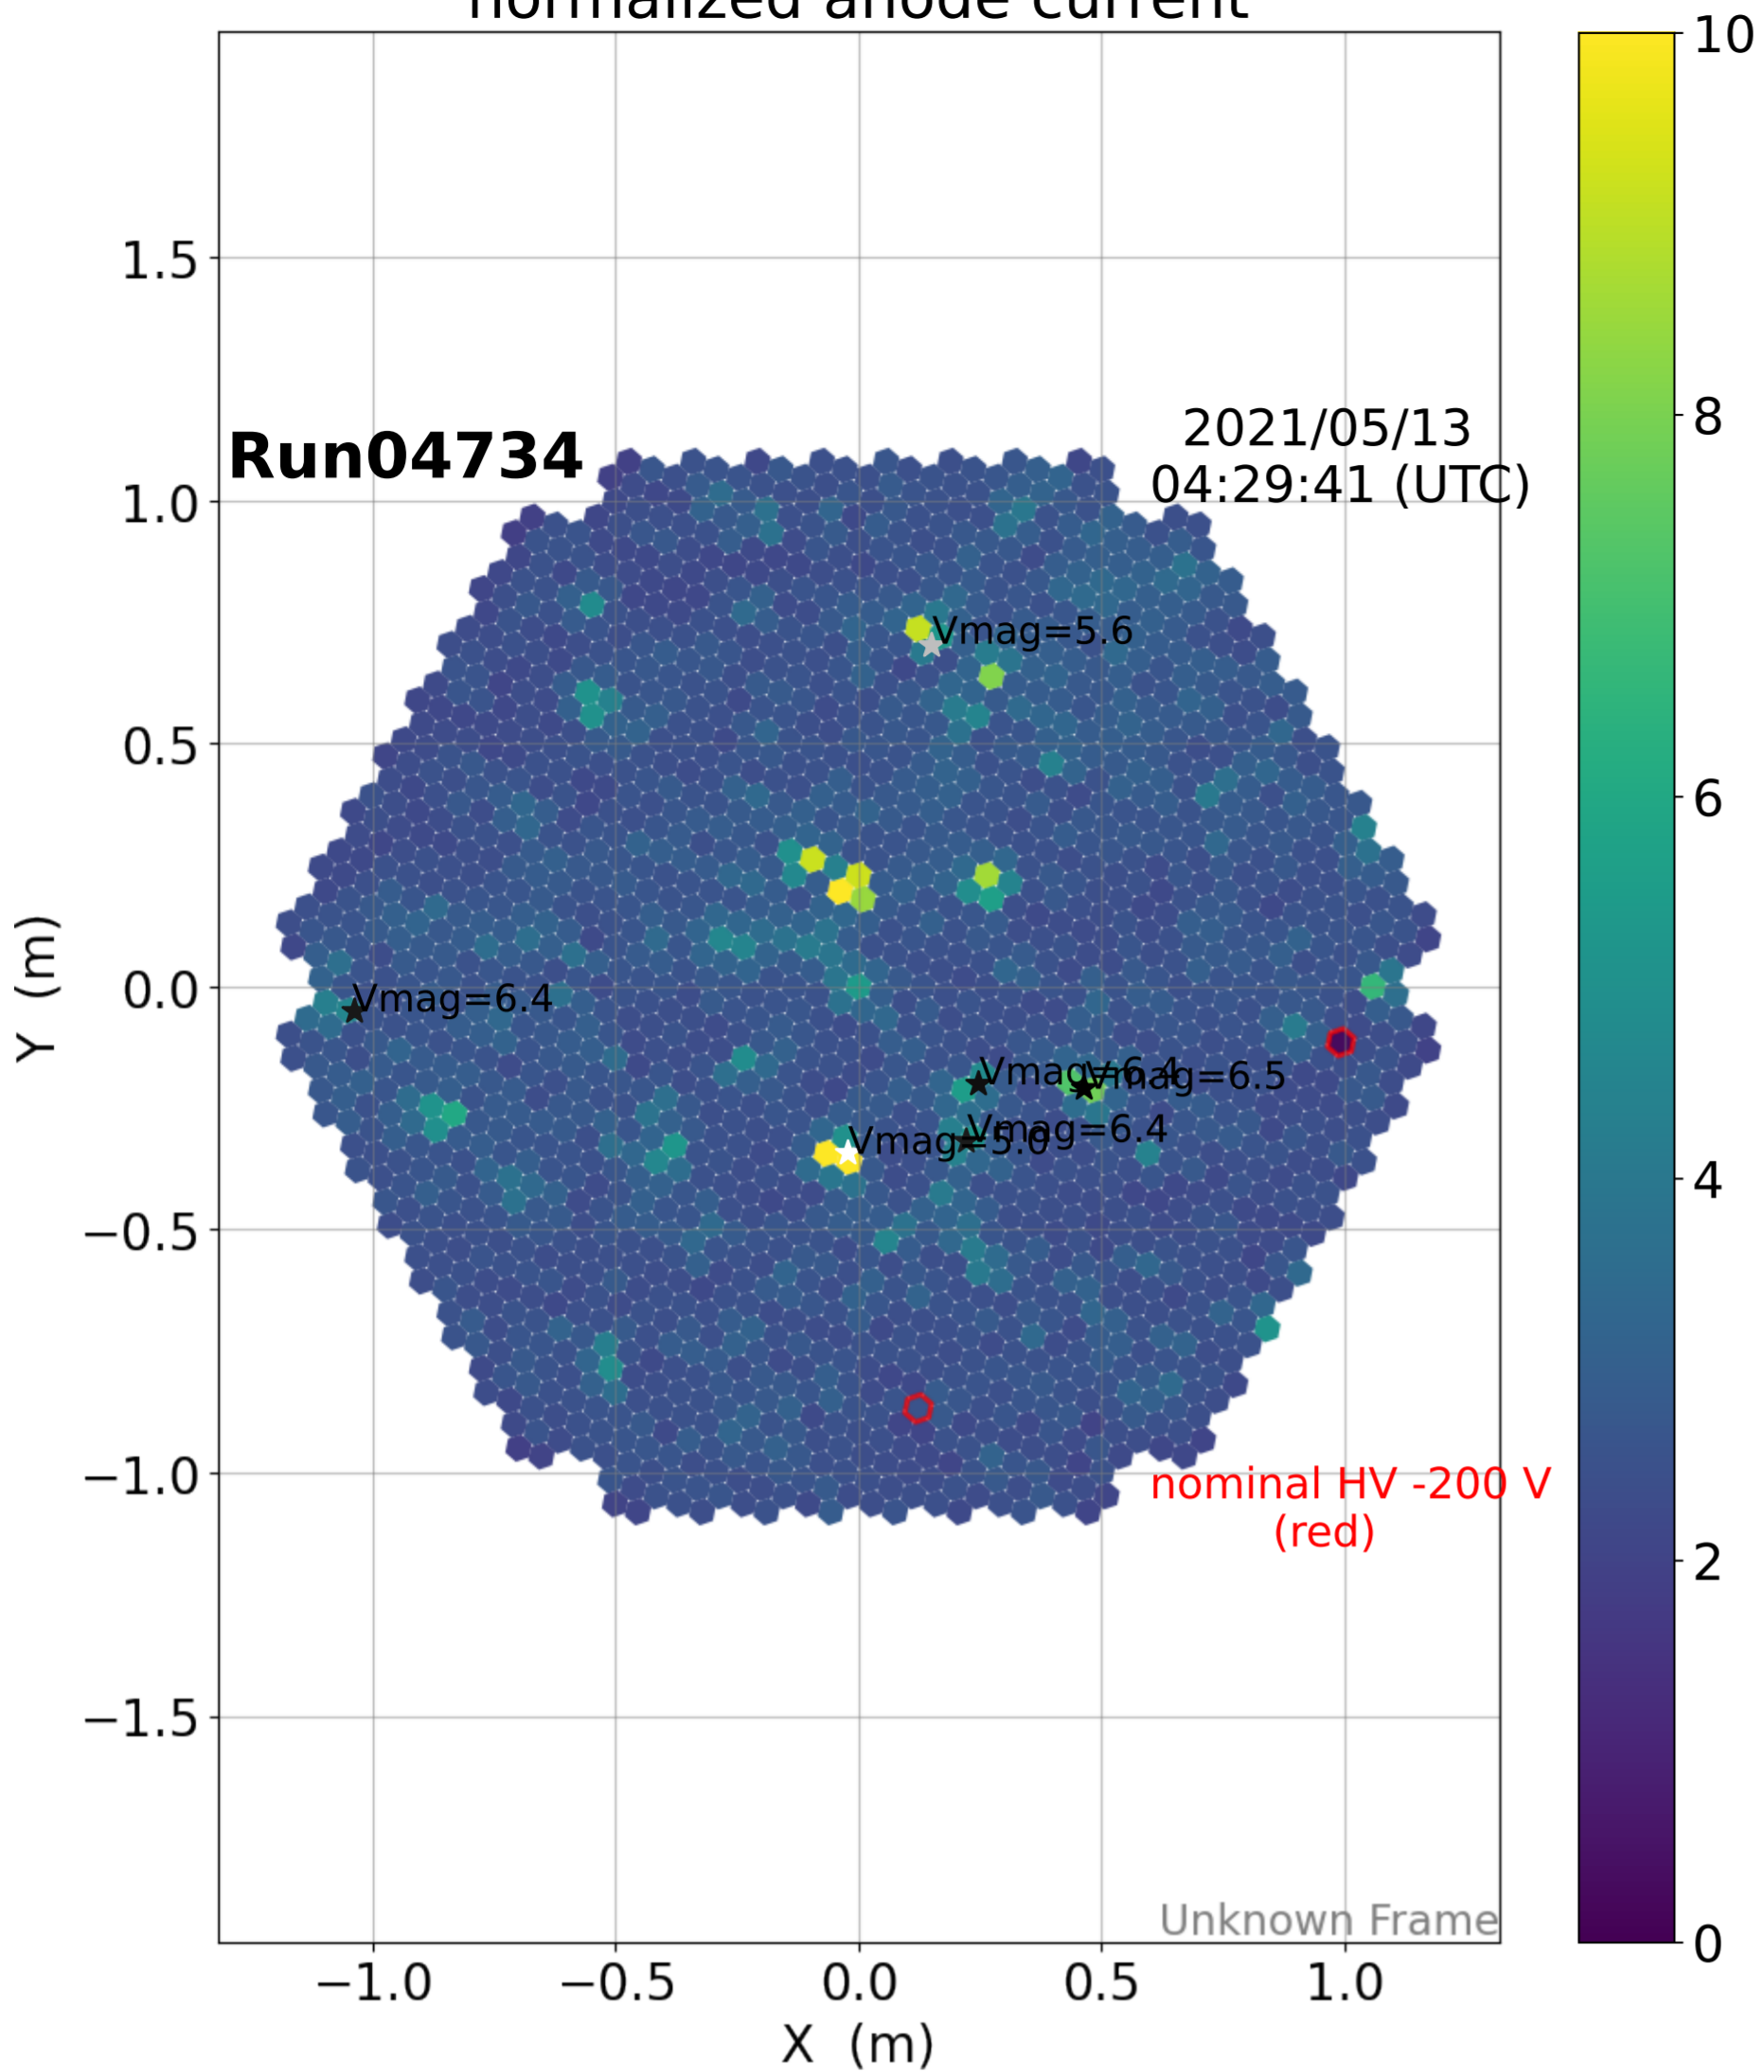

L1 local rate [Hz]

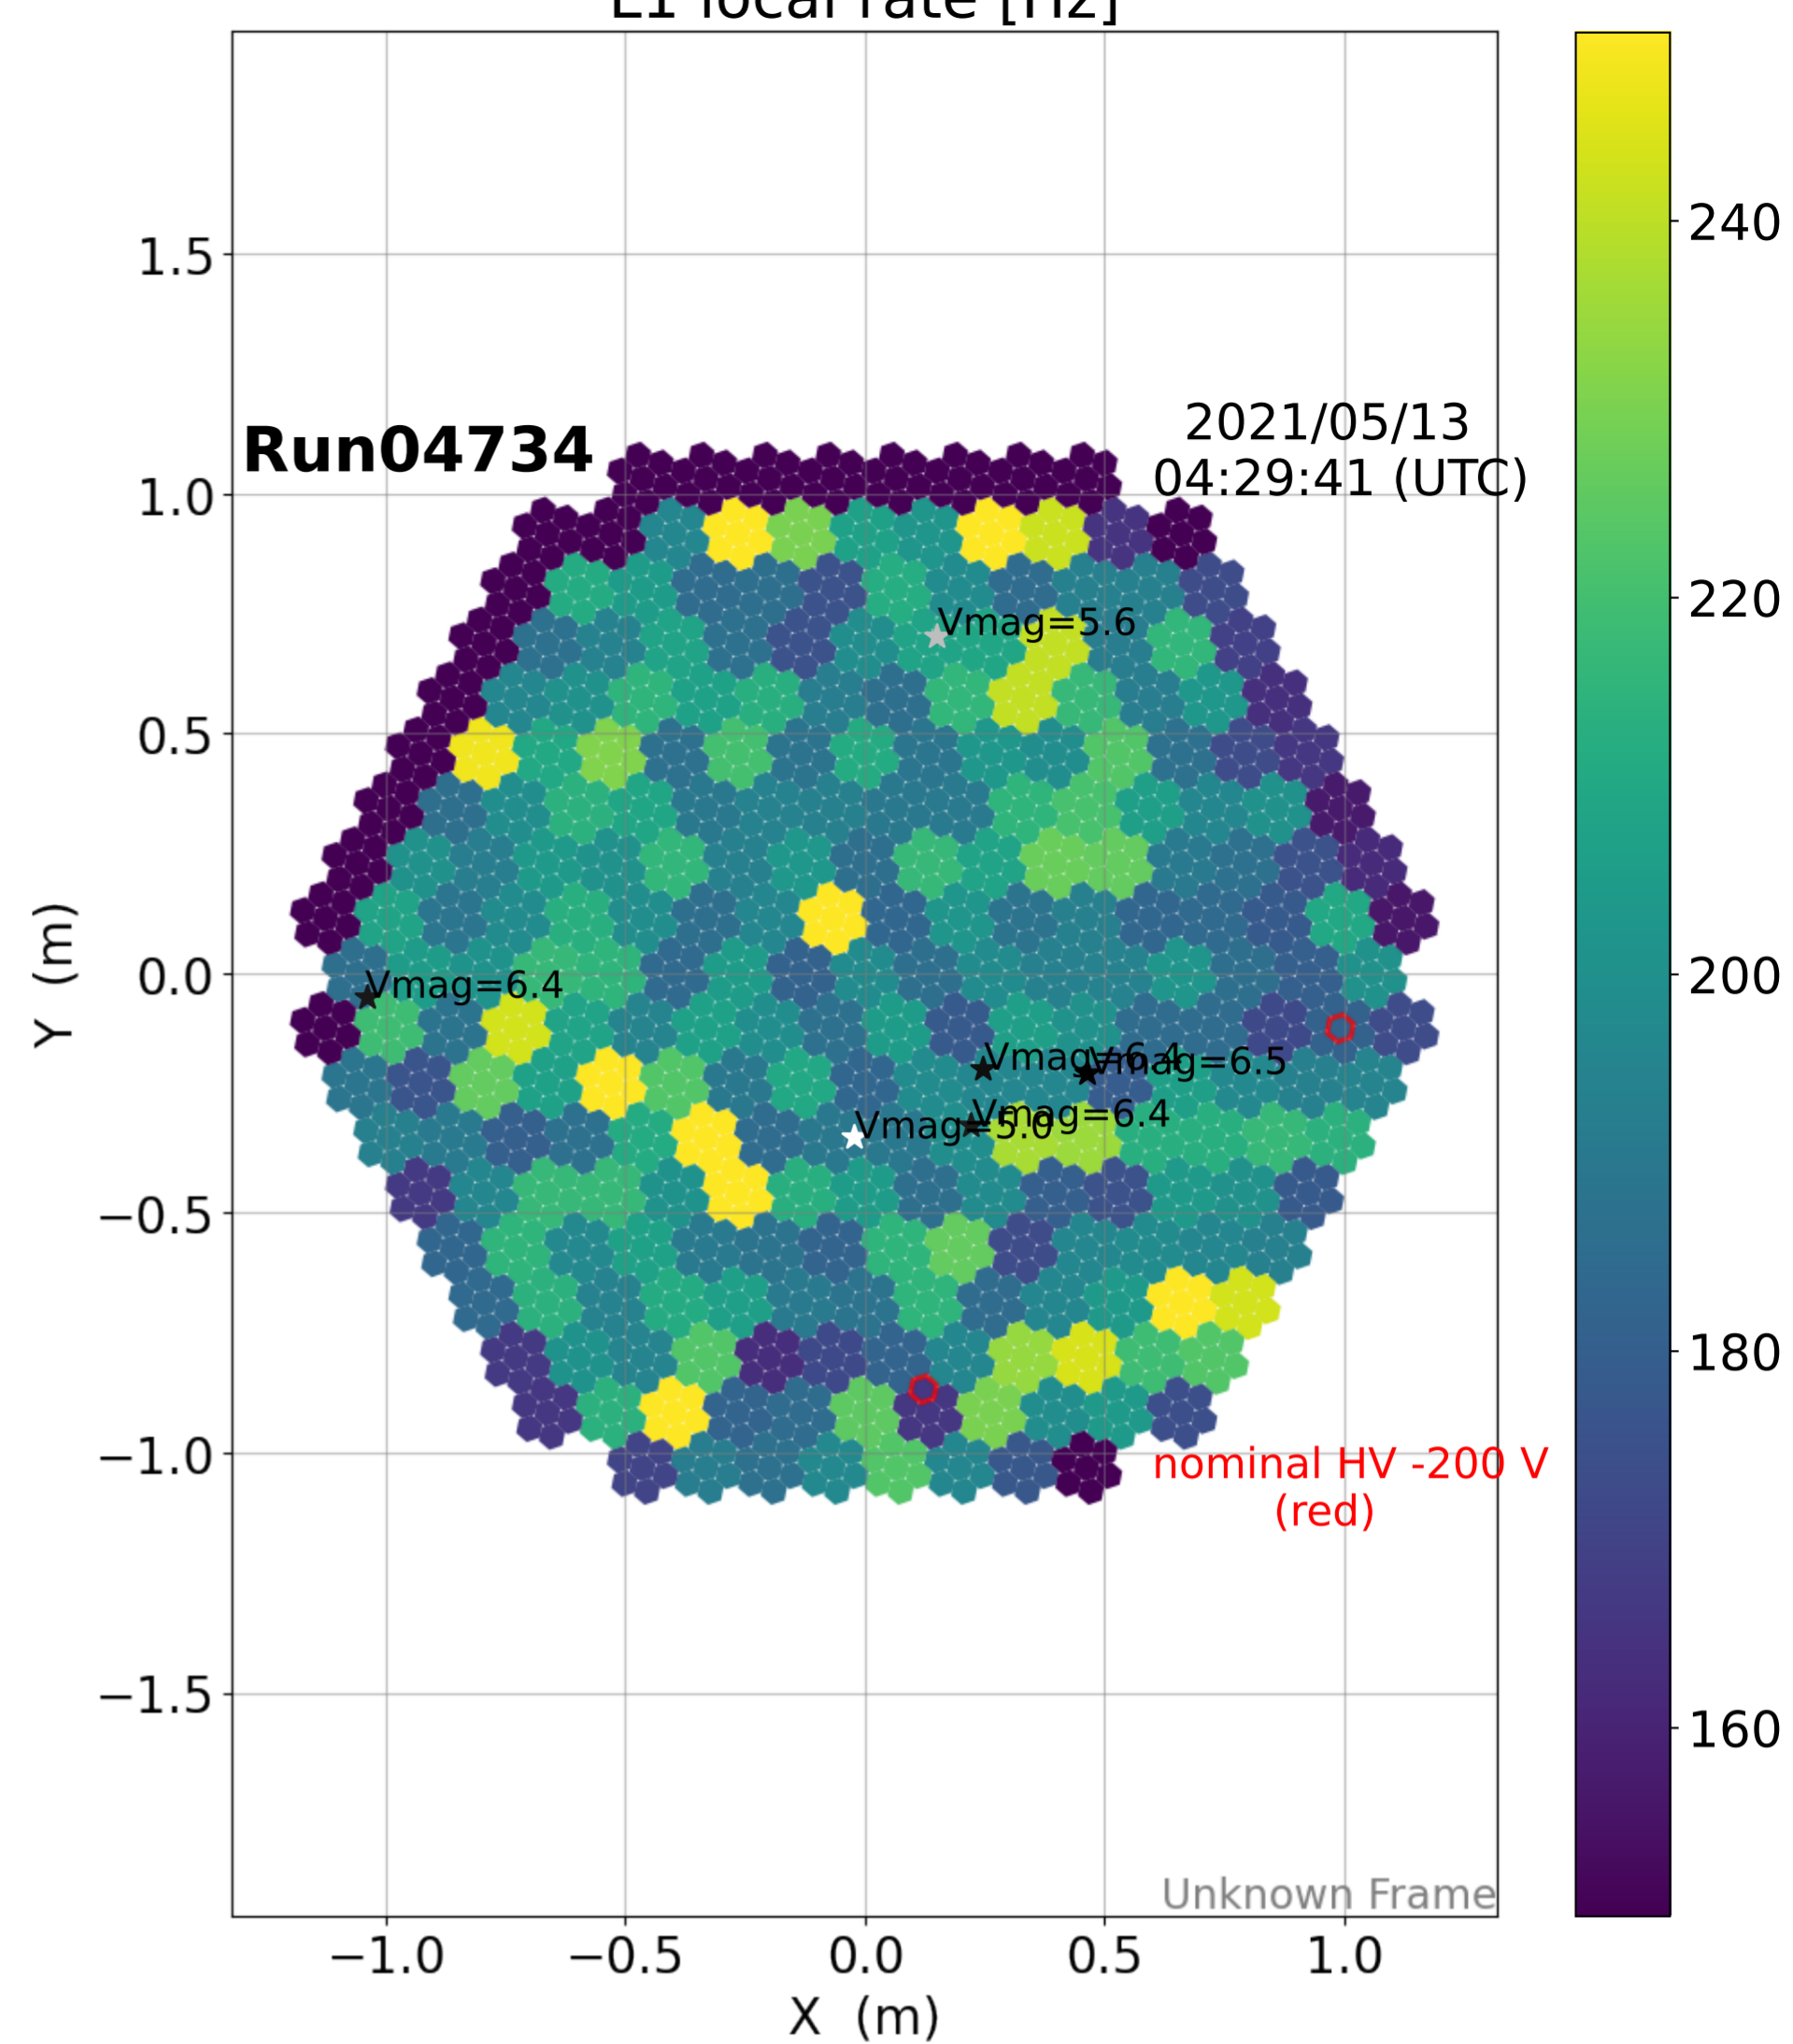

normalized anode current

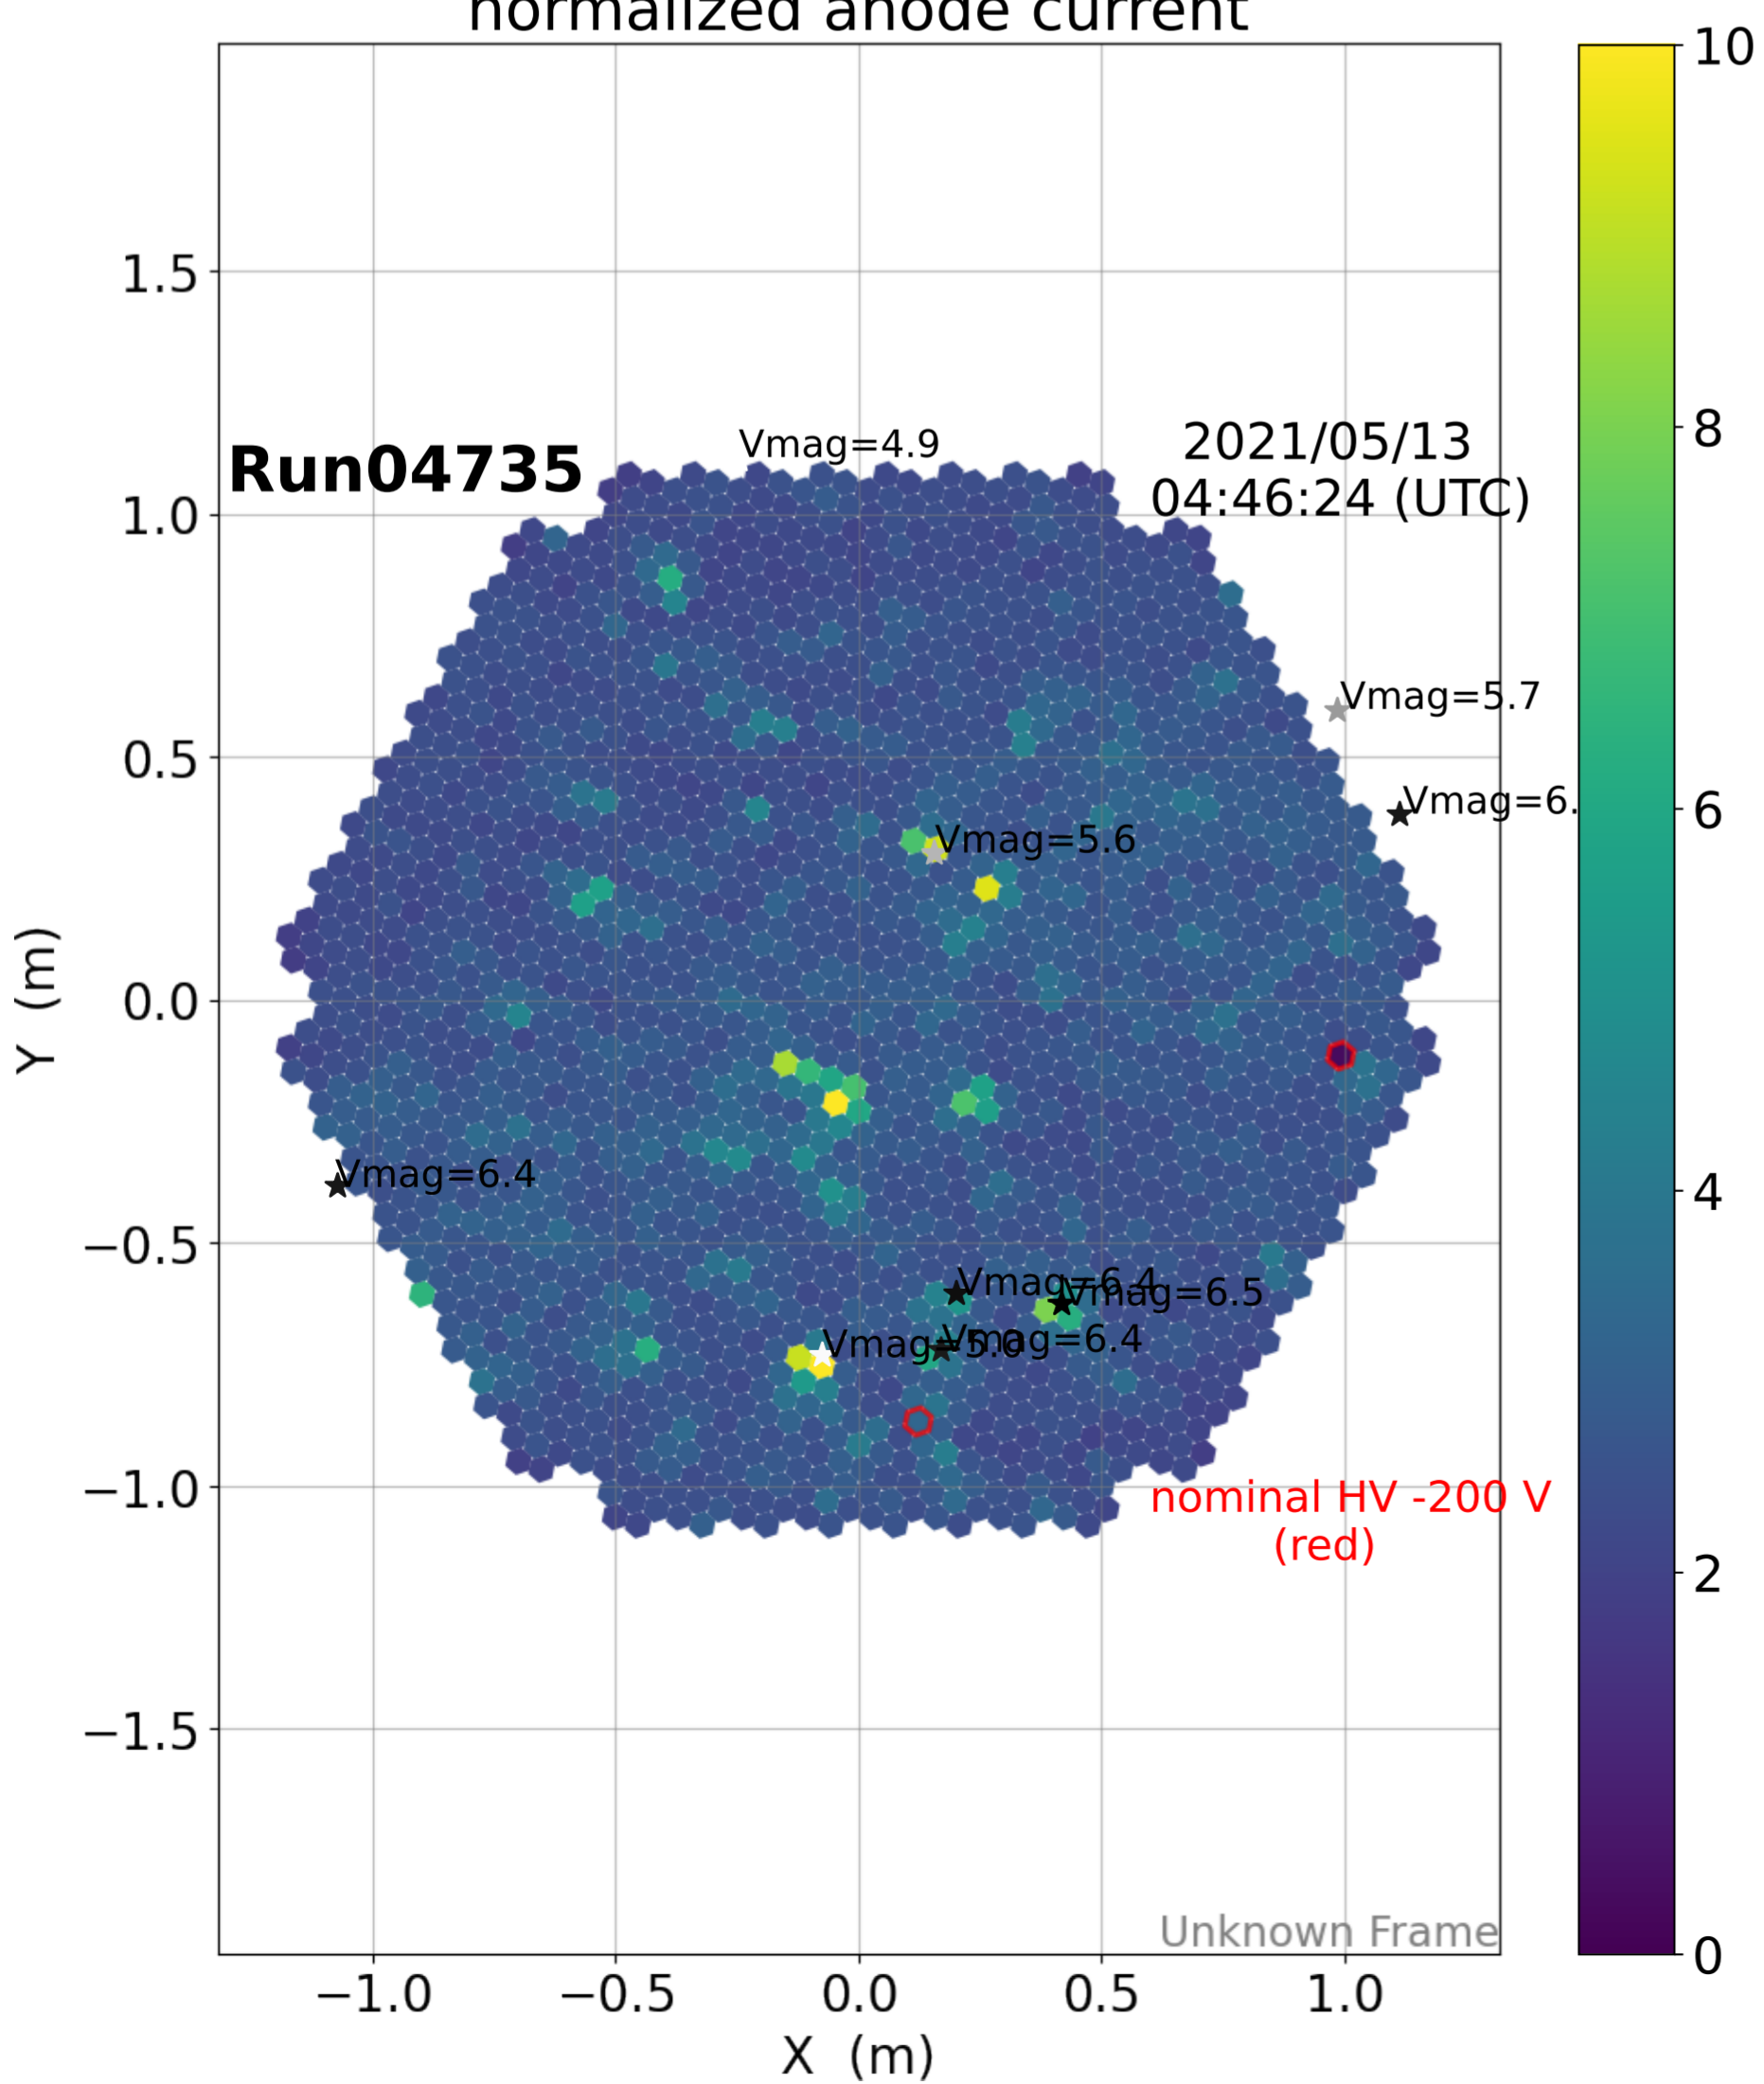

L1 local rate [Hz]

