




2021-5-29

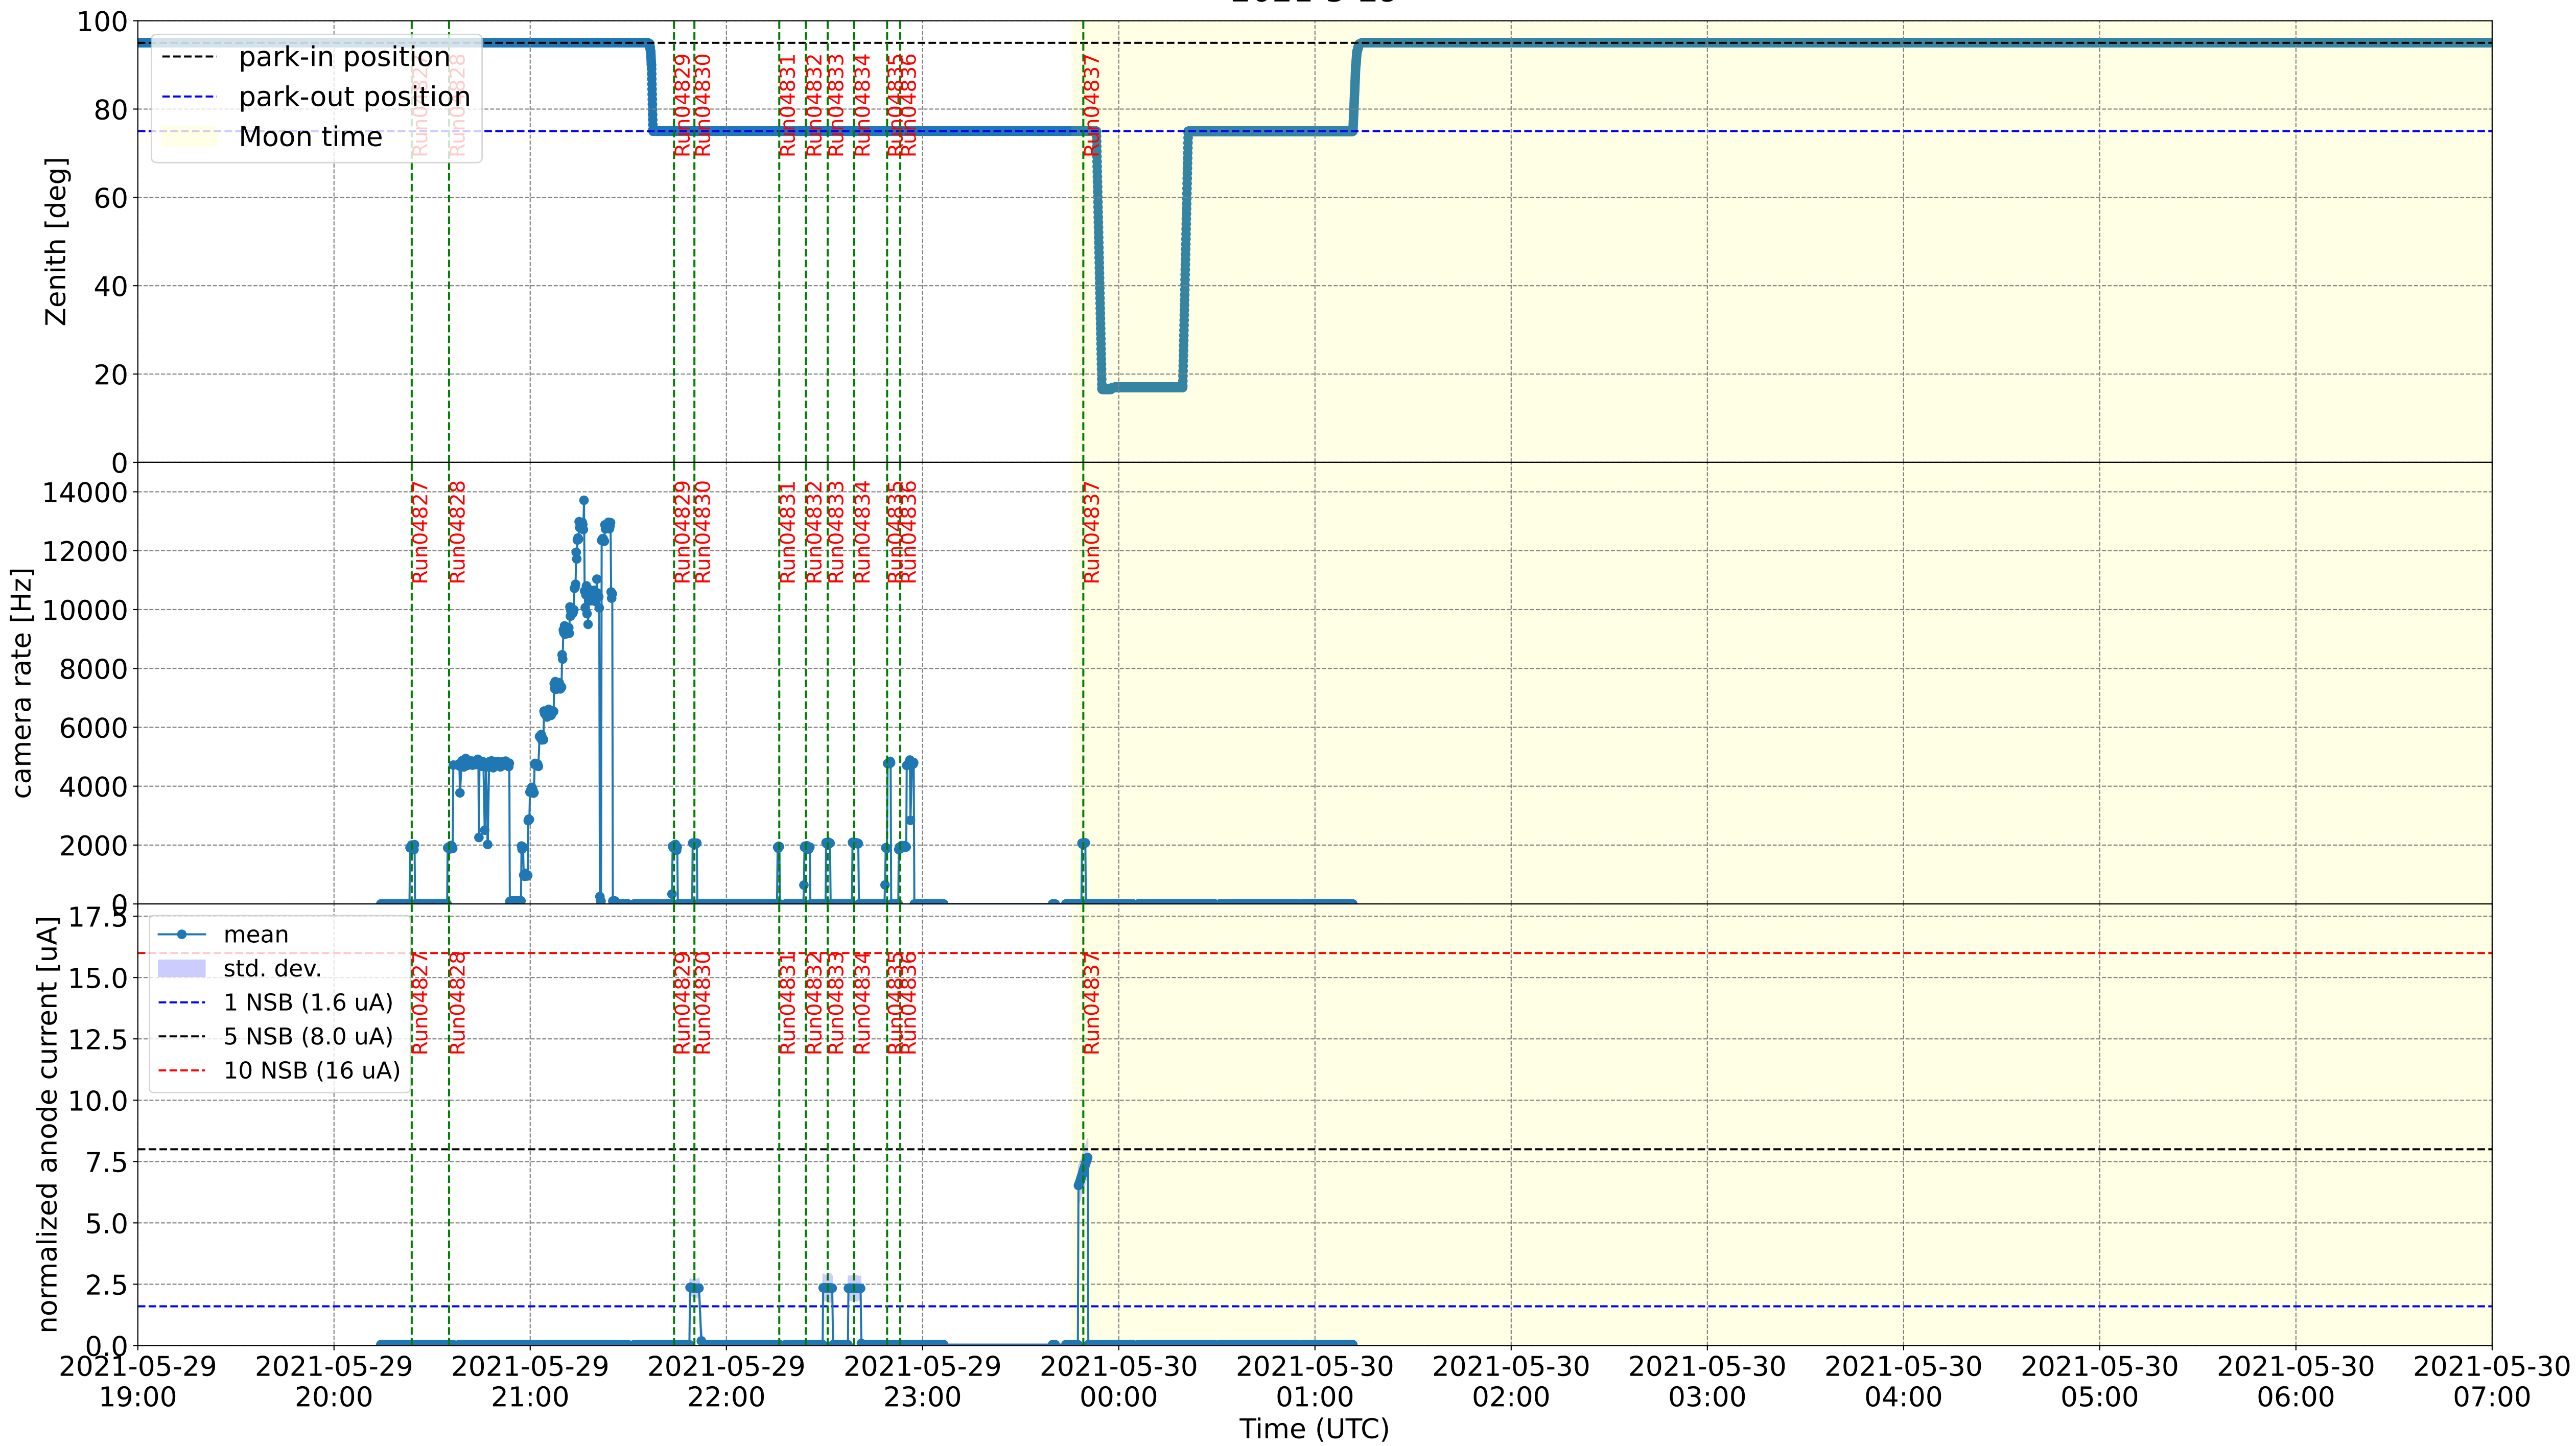


2021-5-29






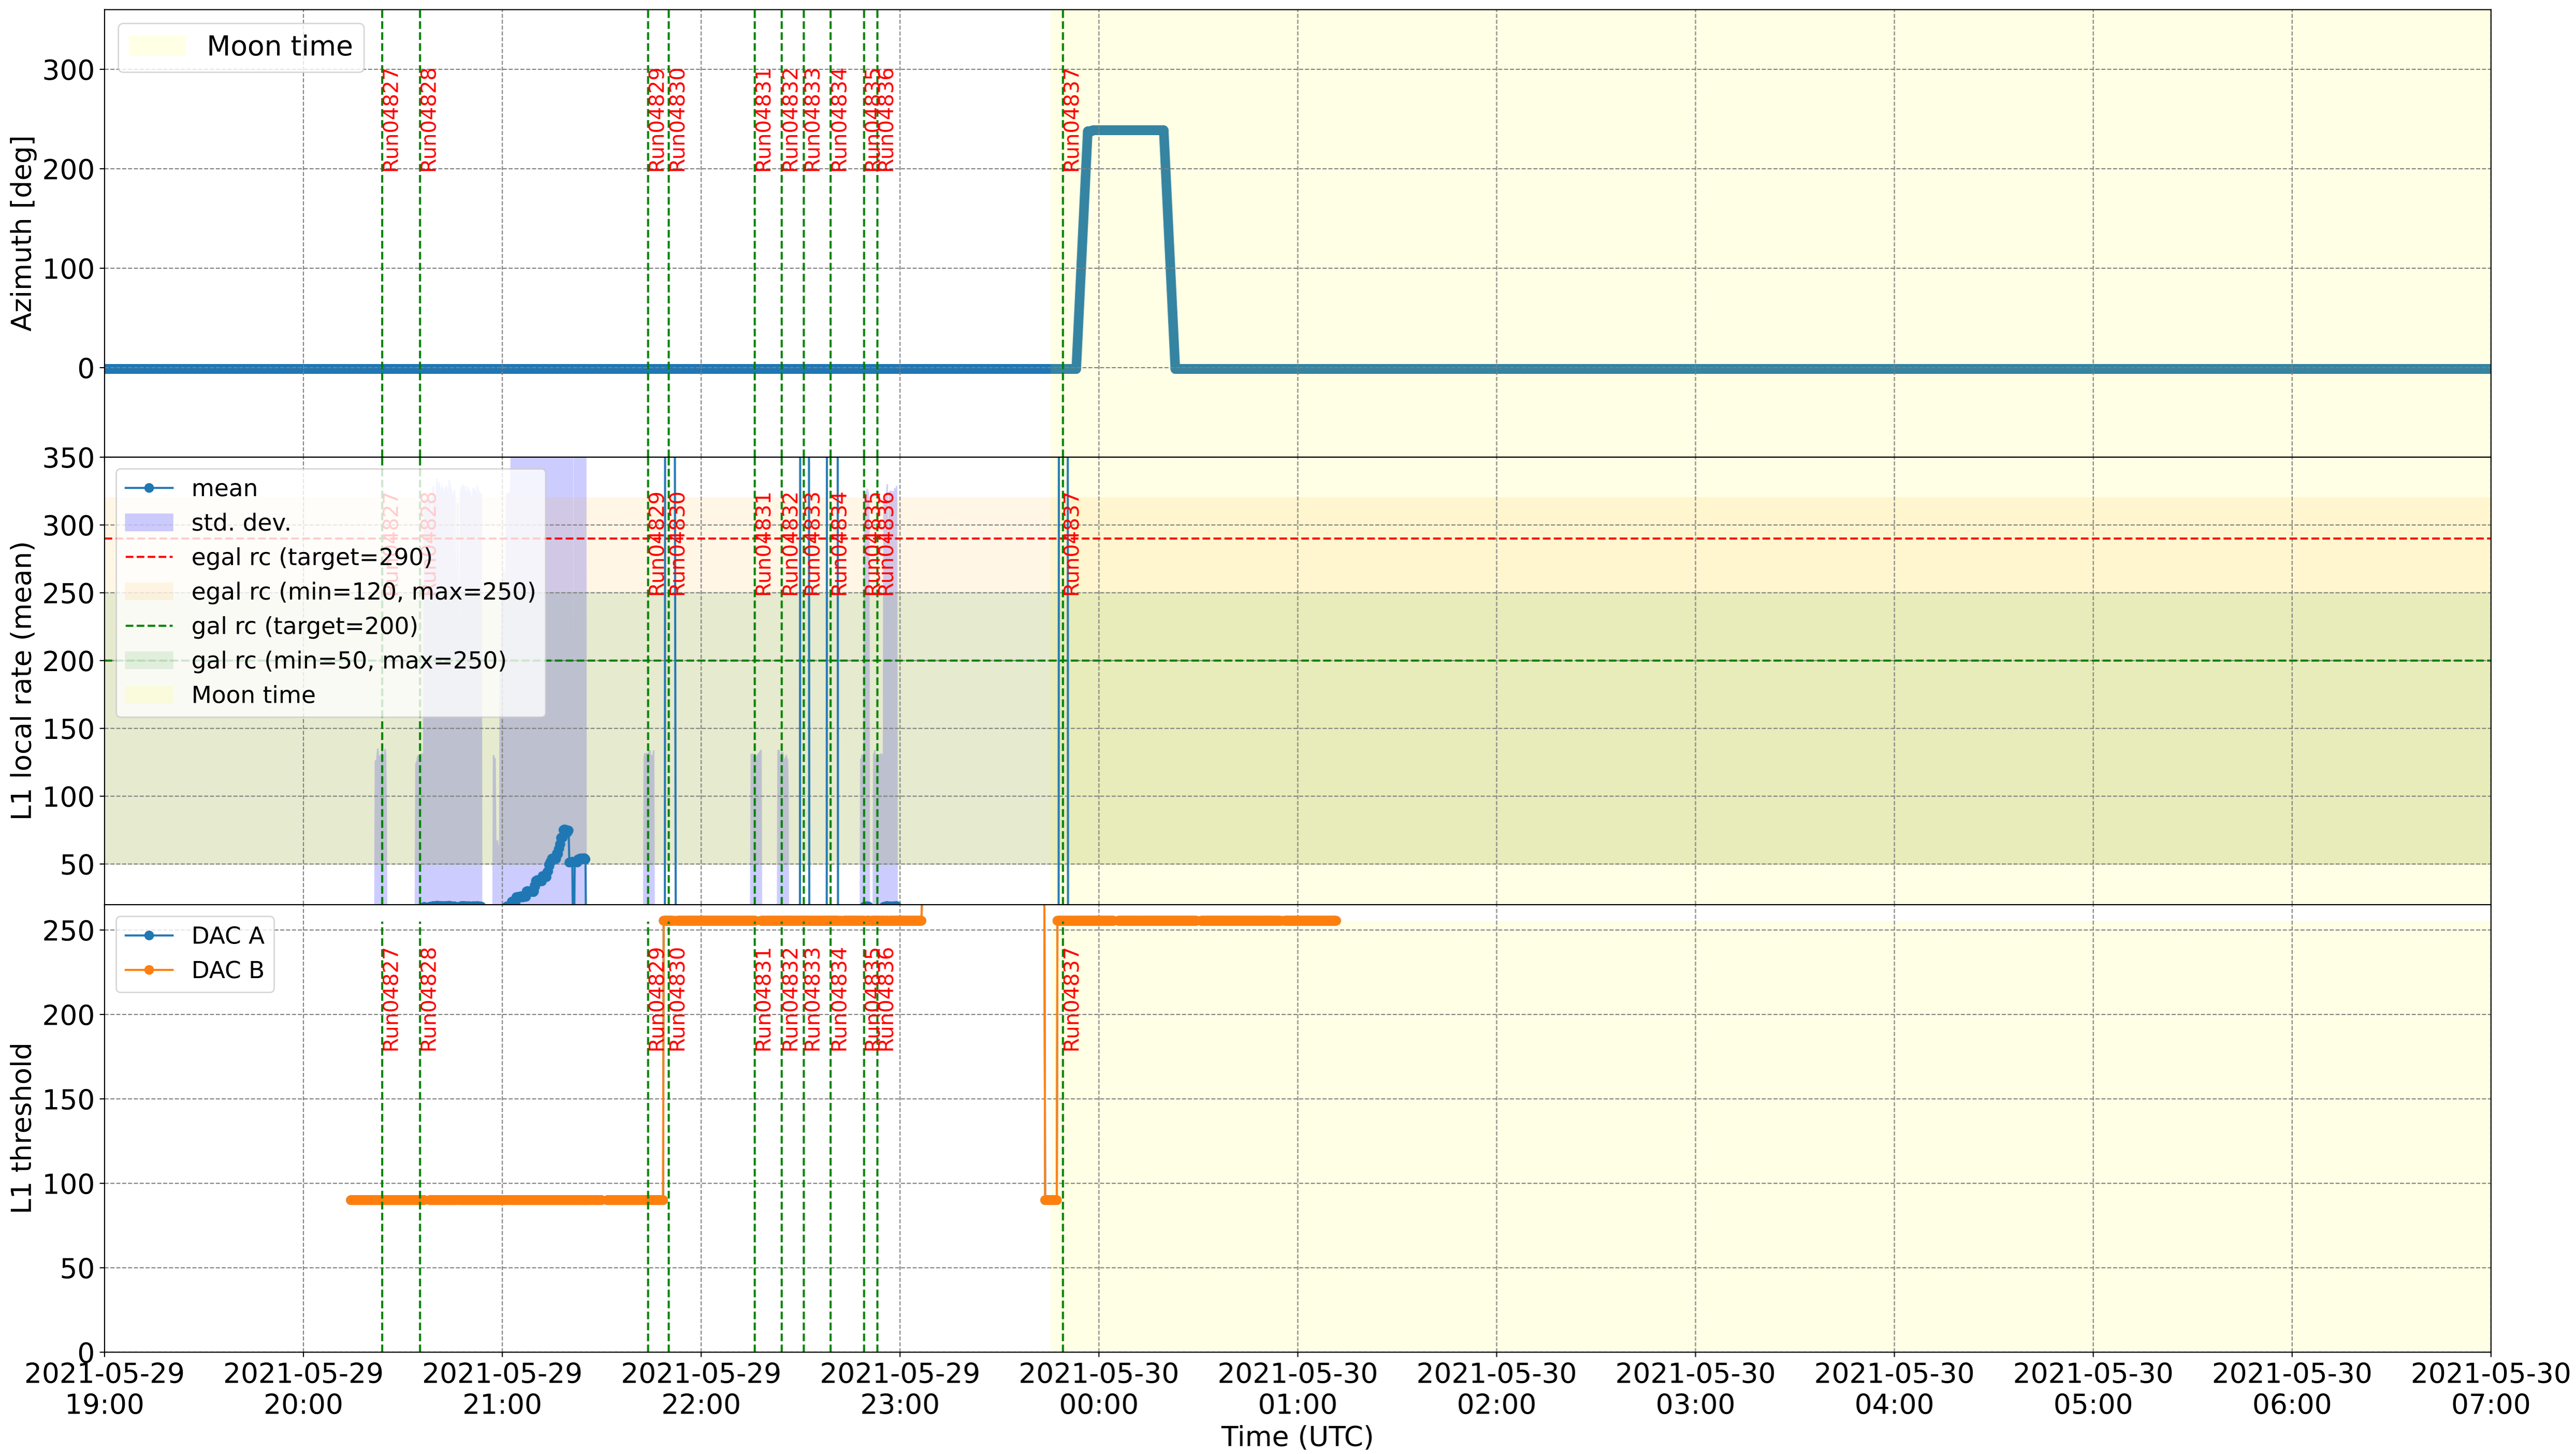








2021-5-29






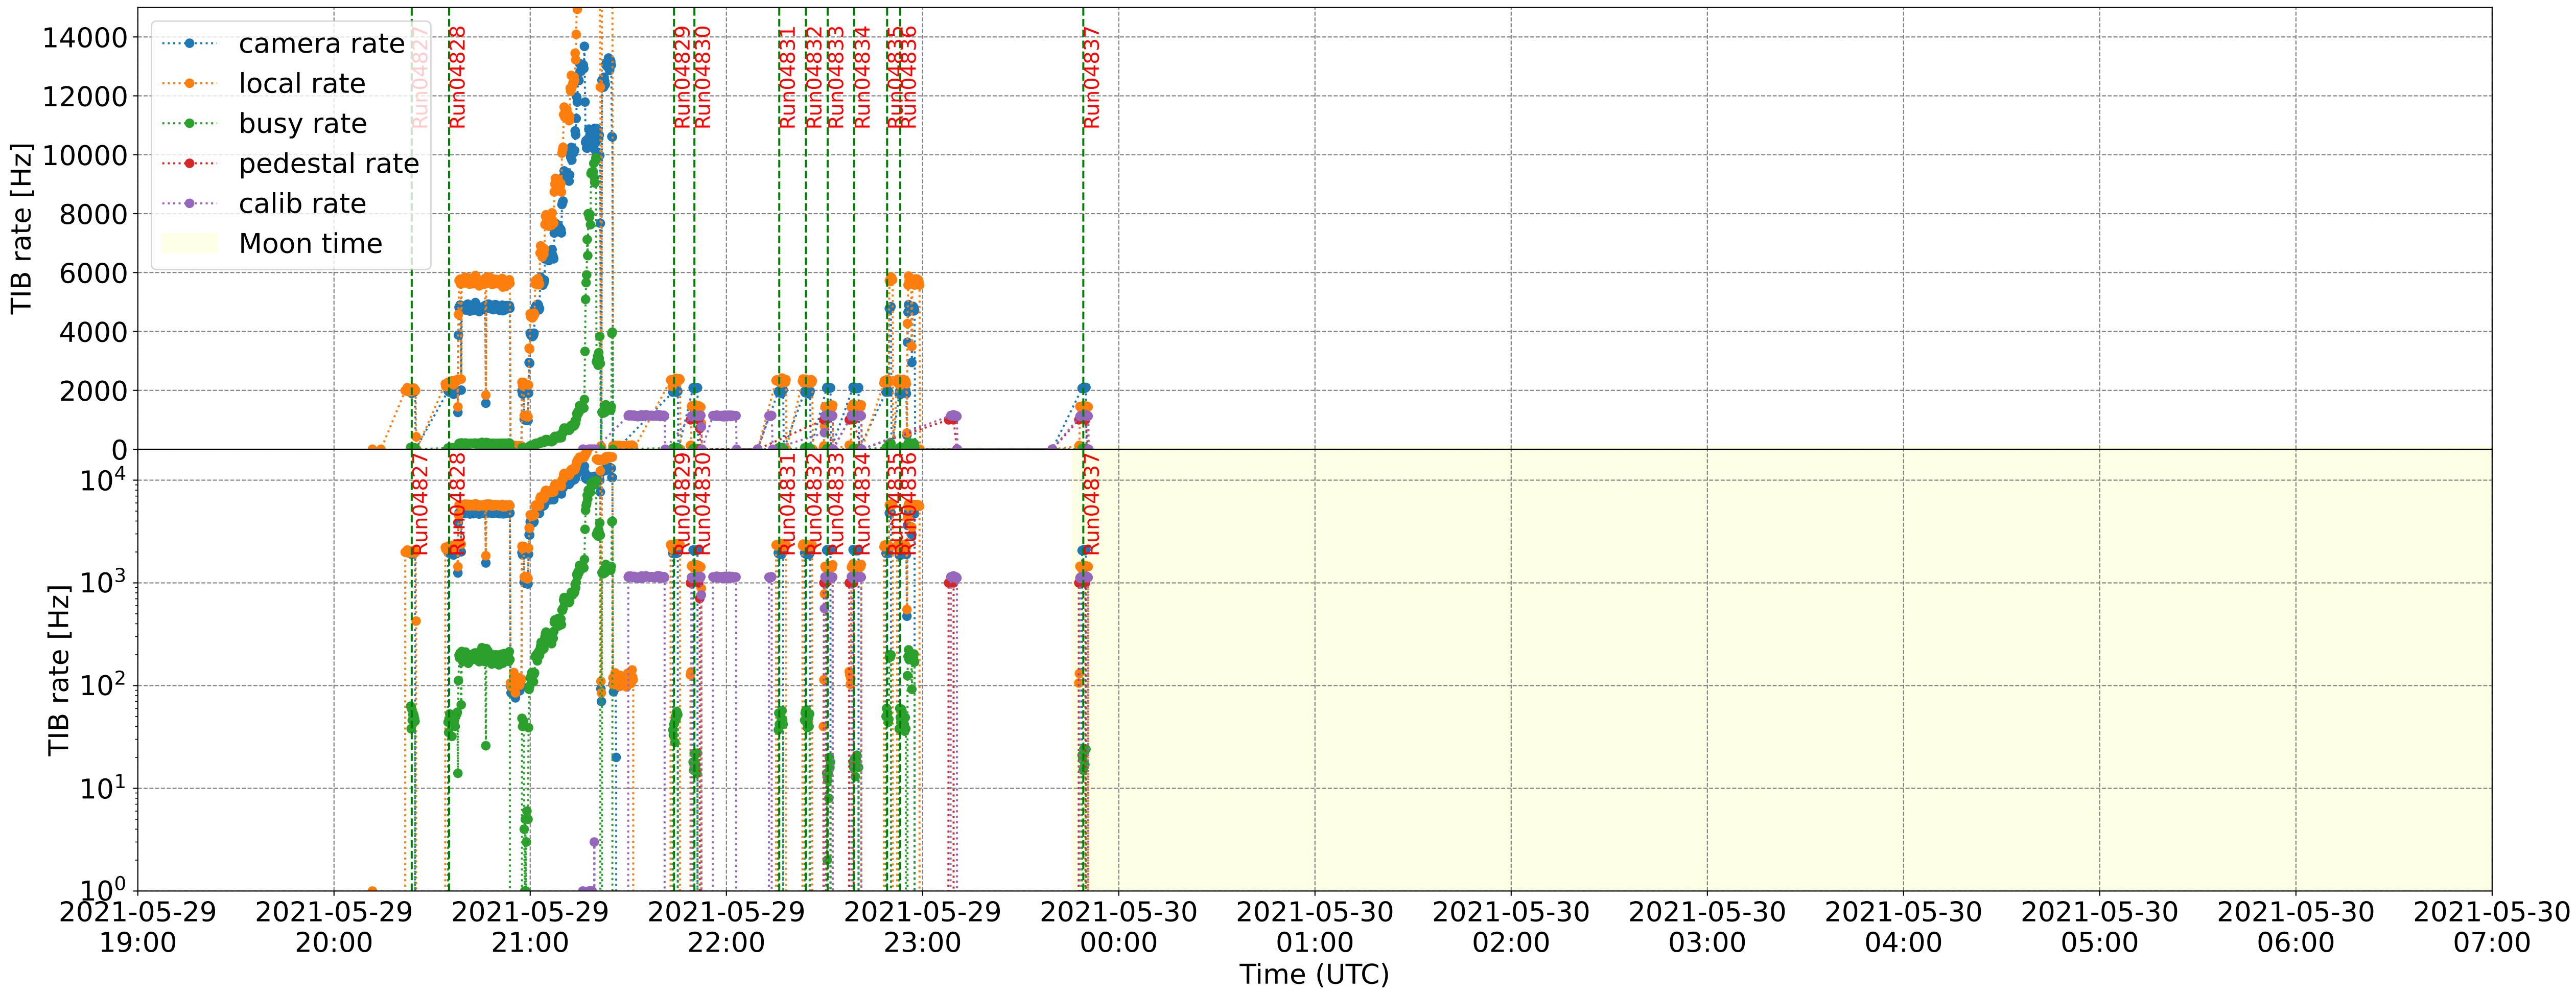


Calibration Box (2021-5-29)

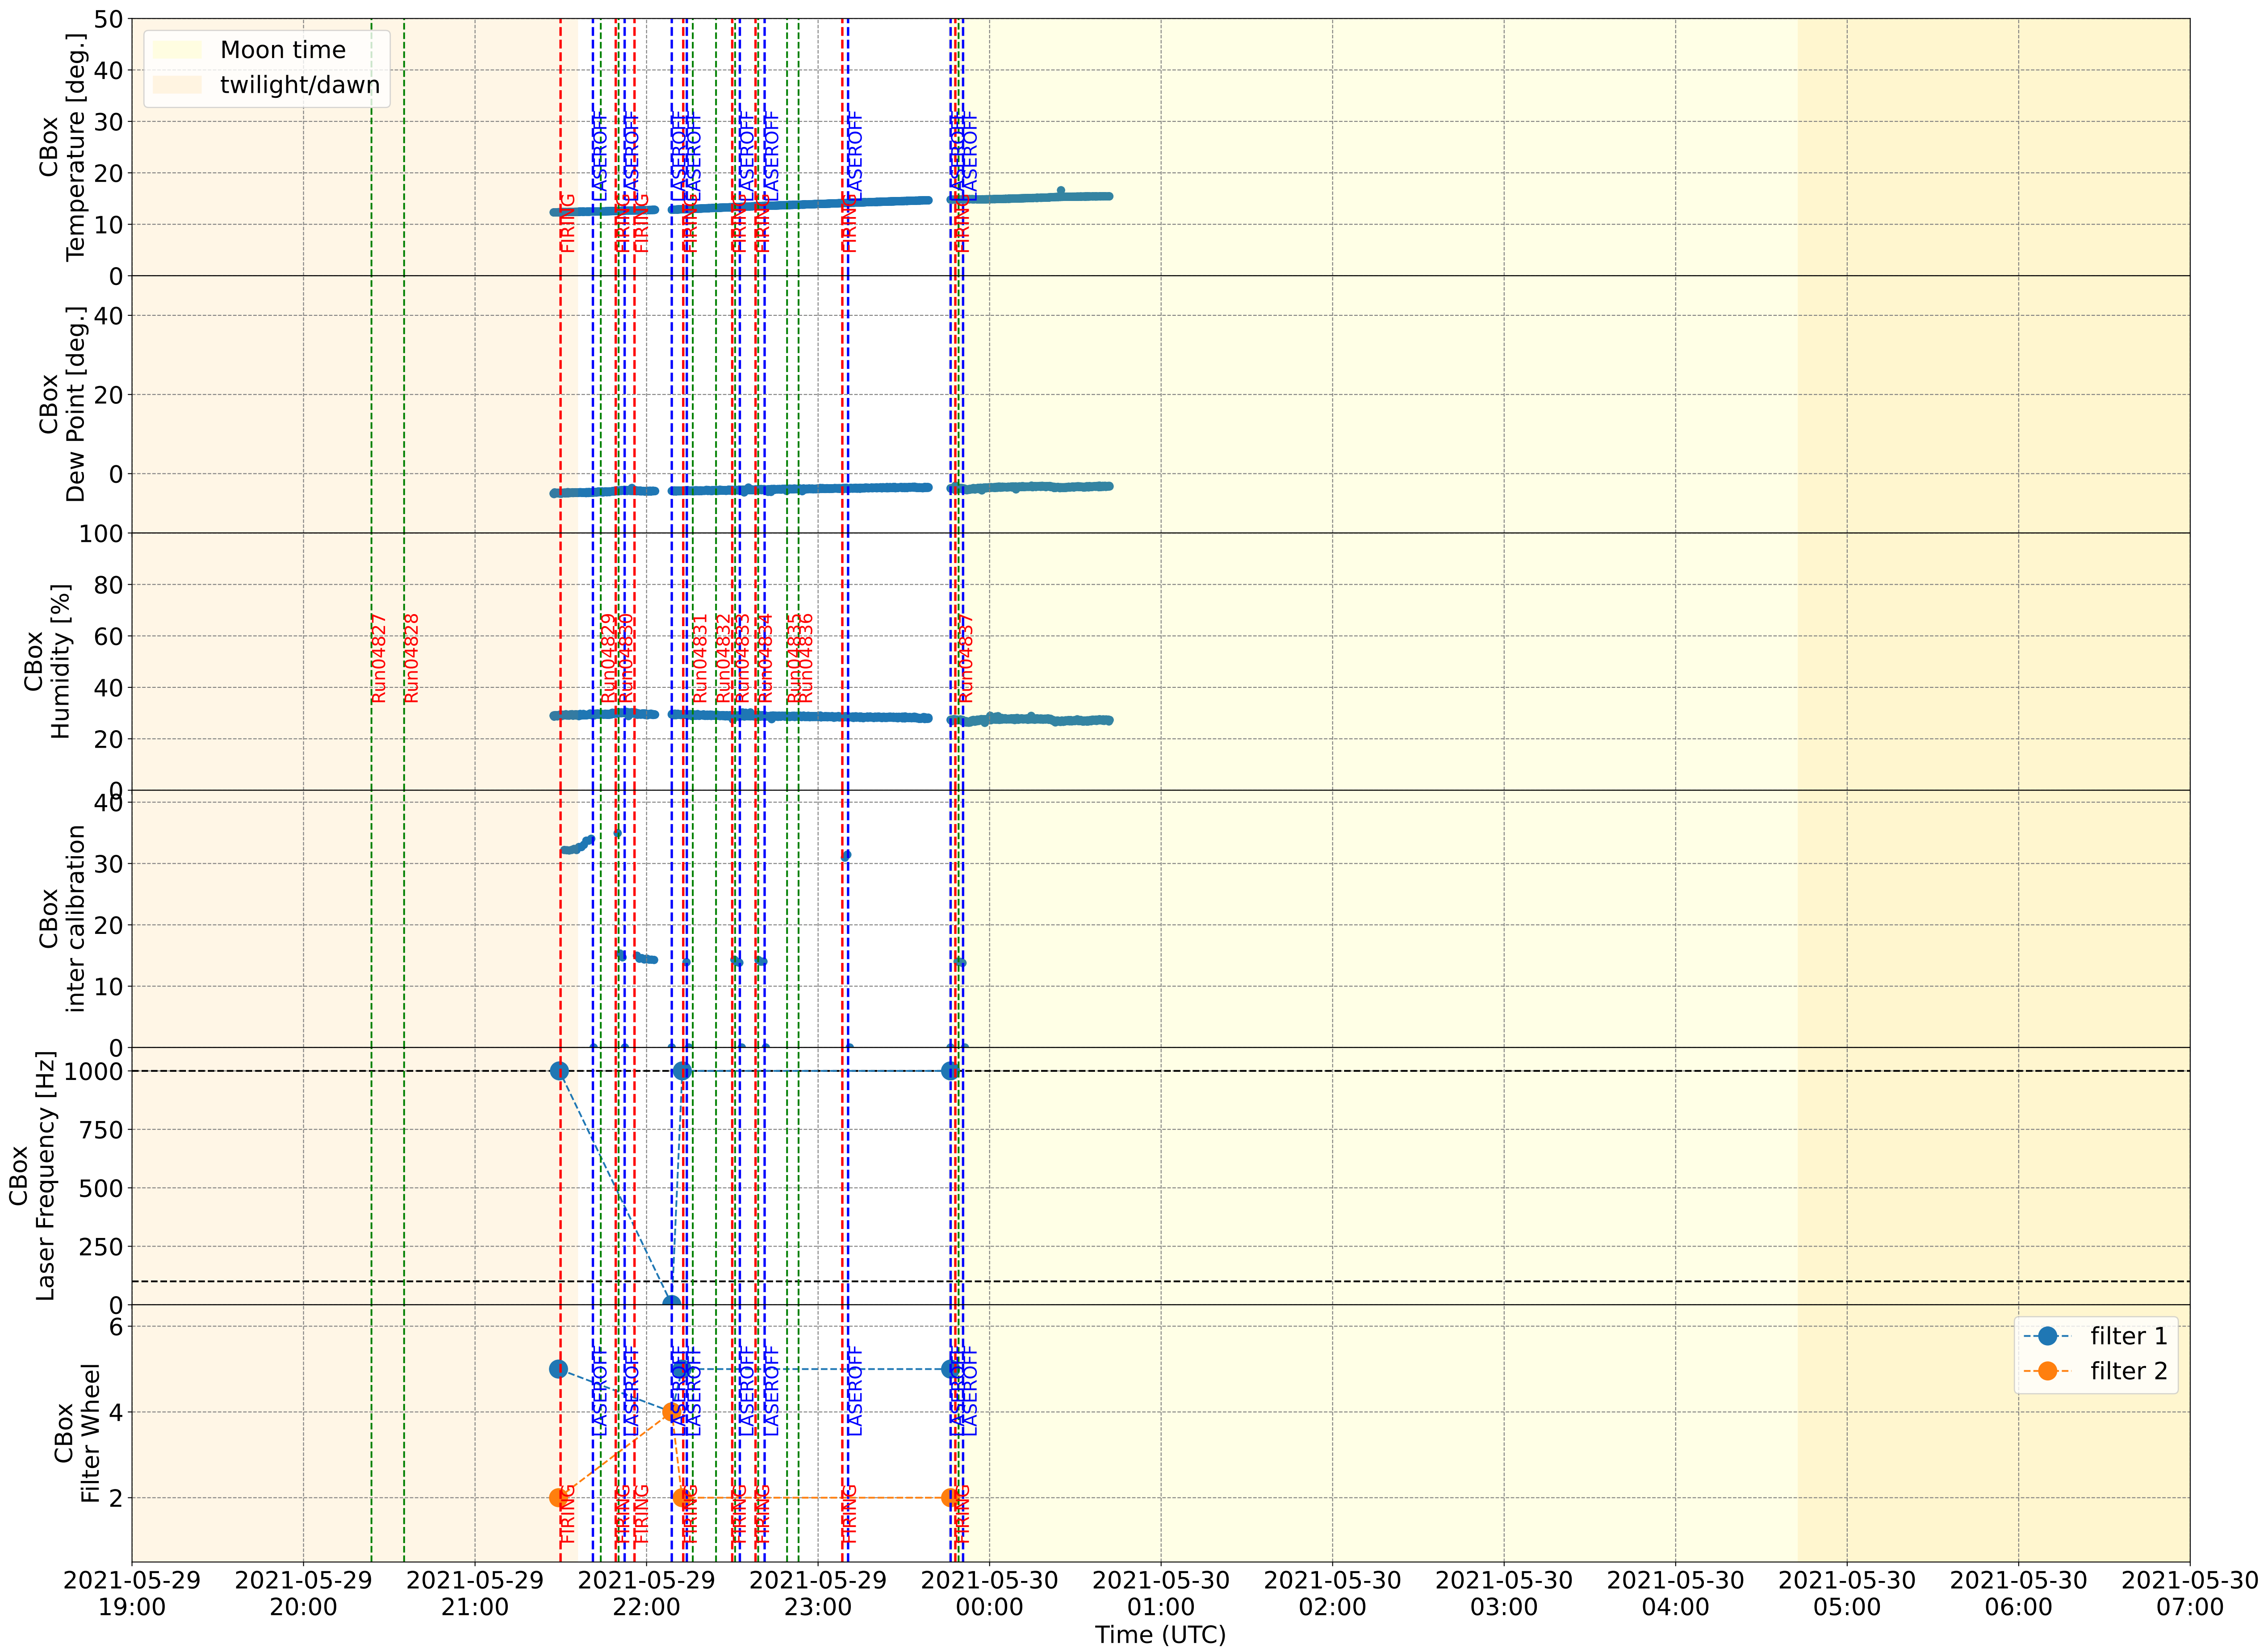


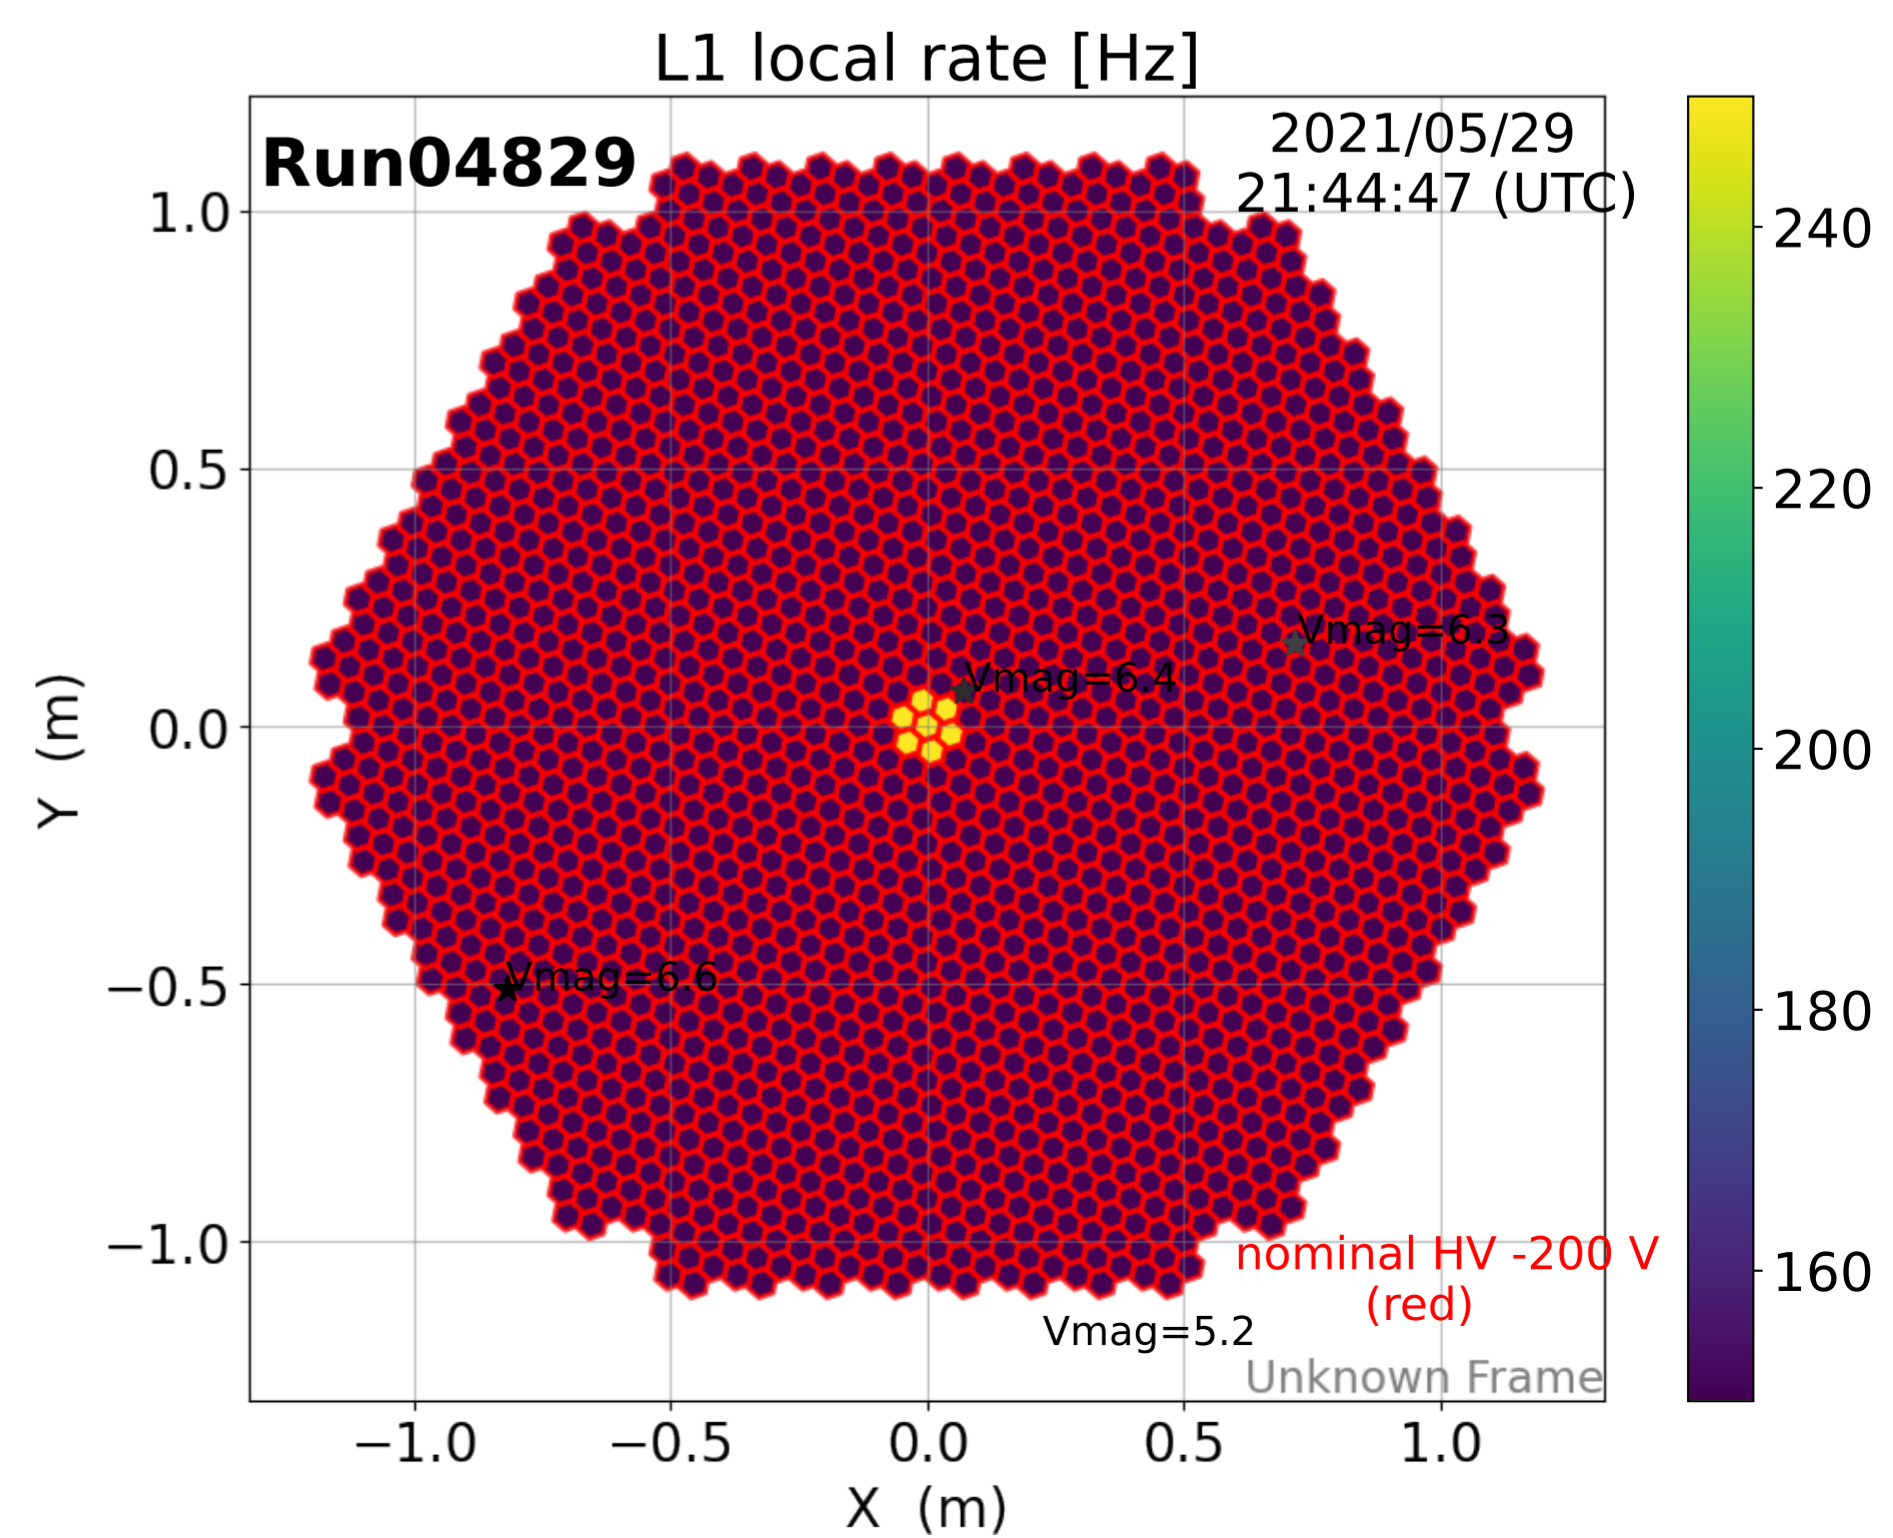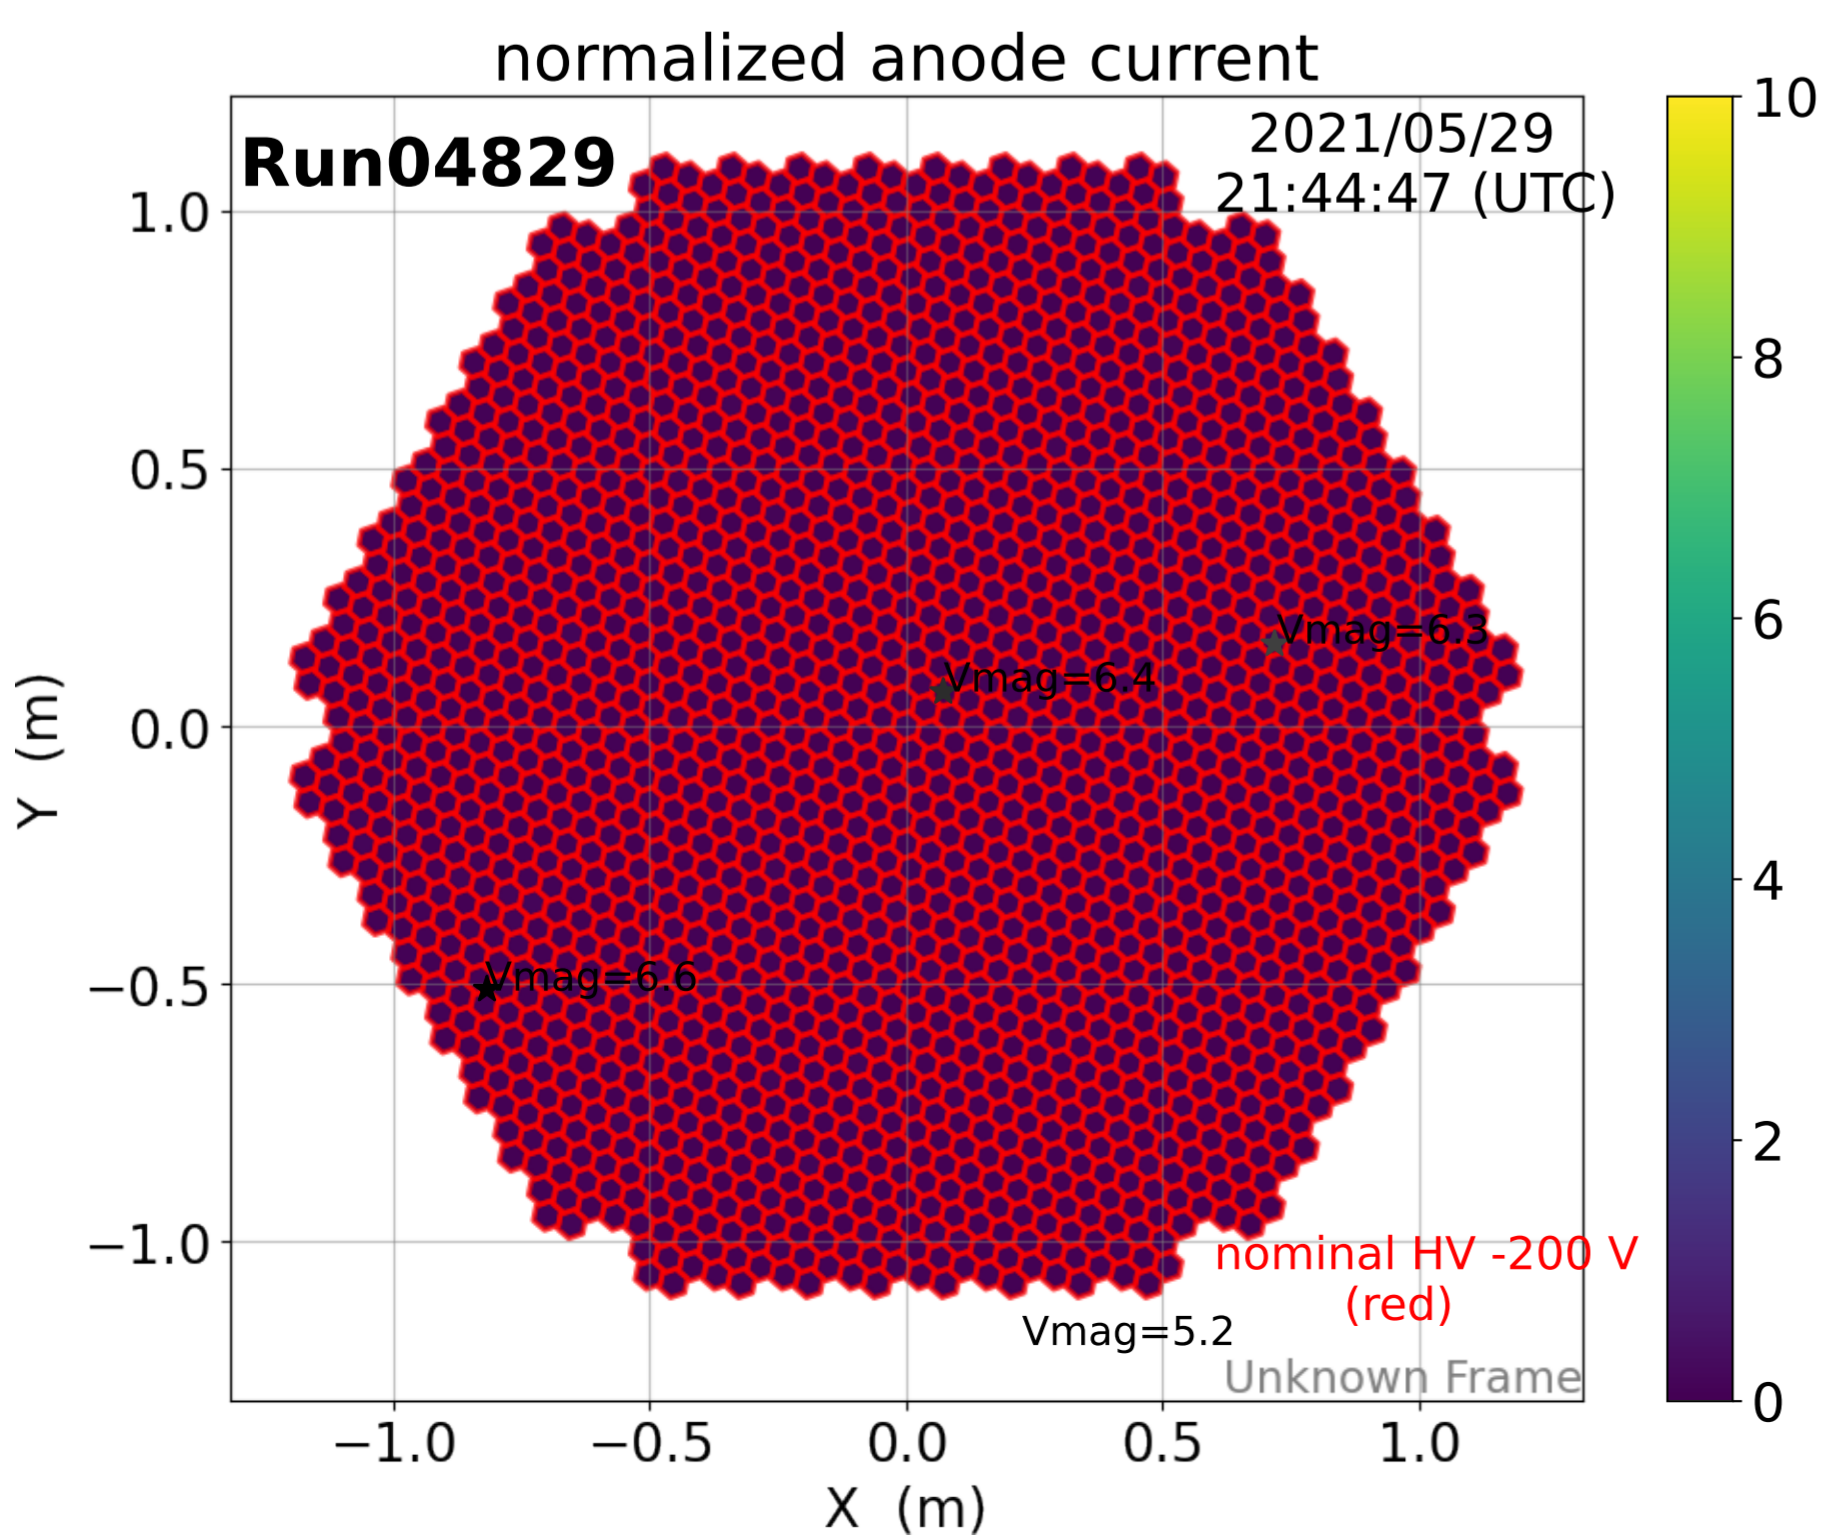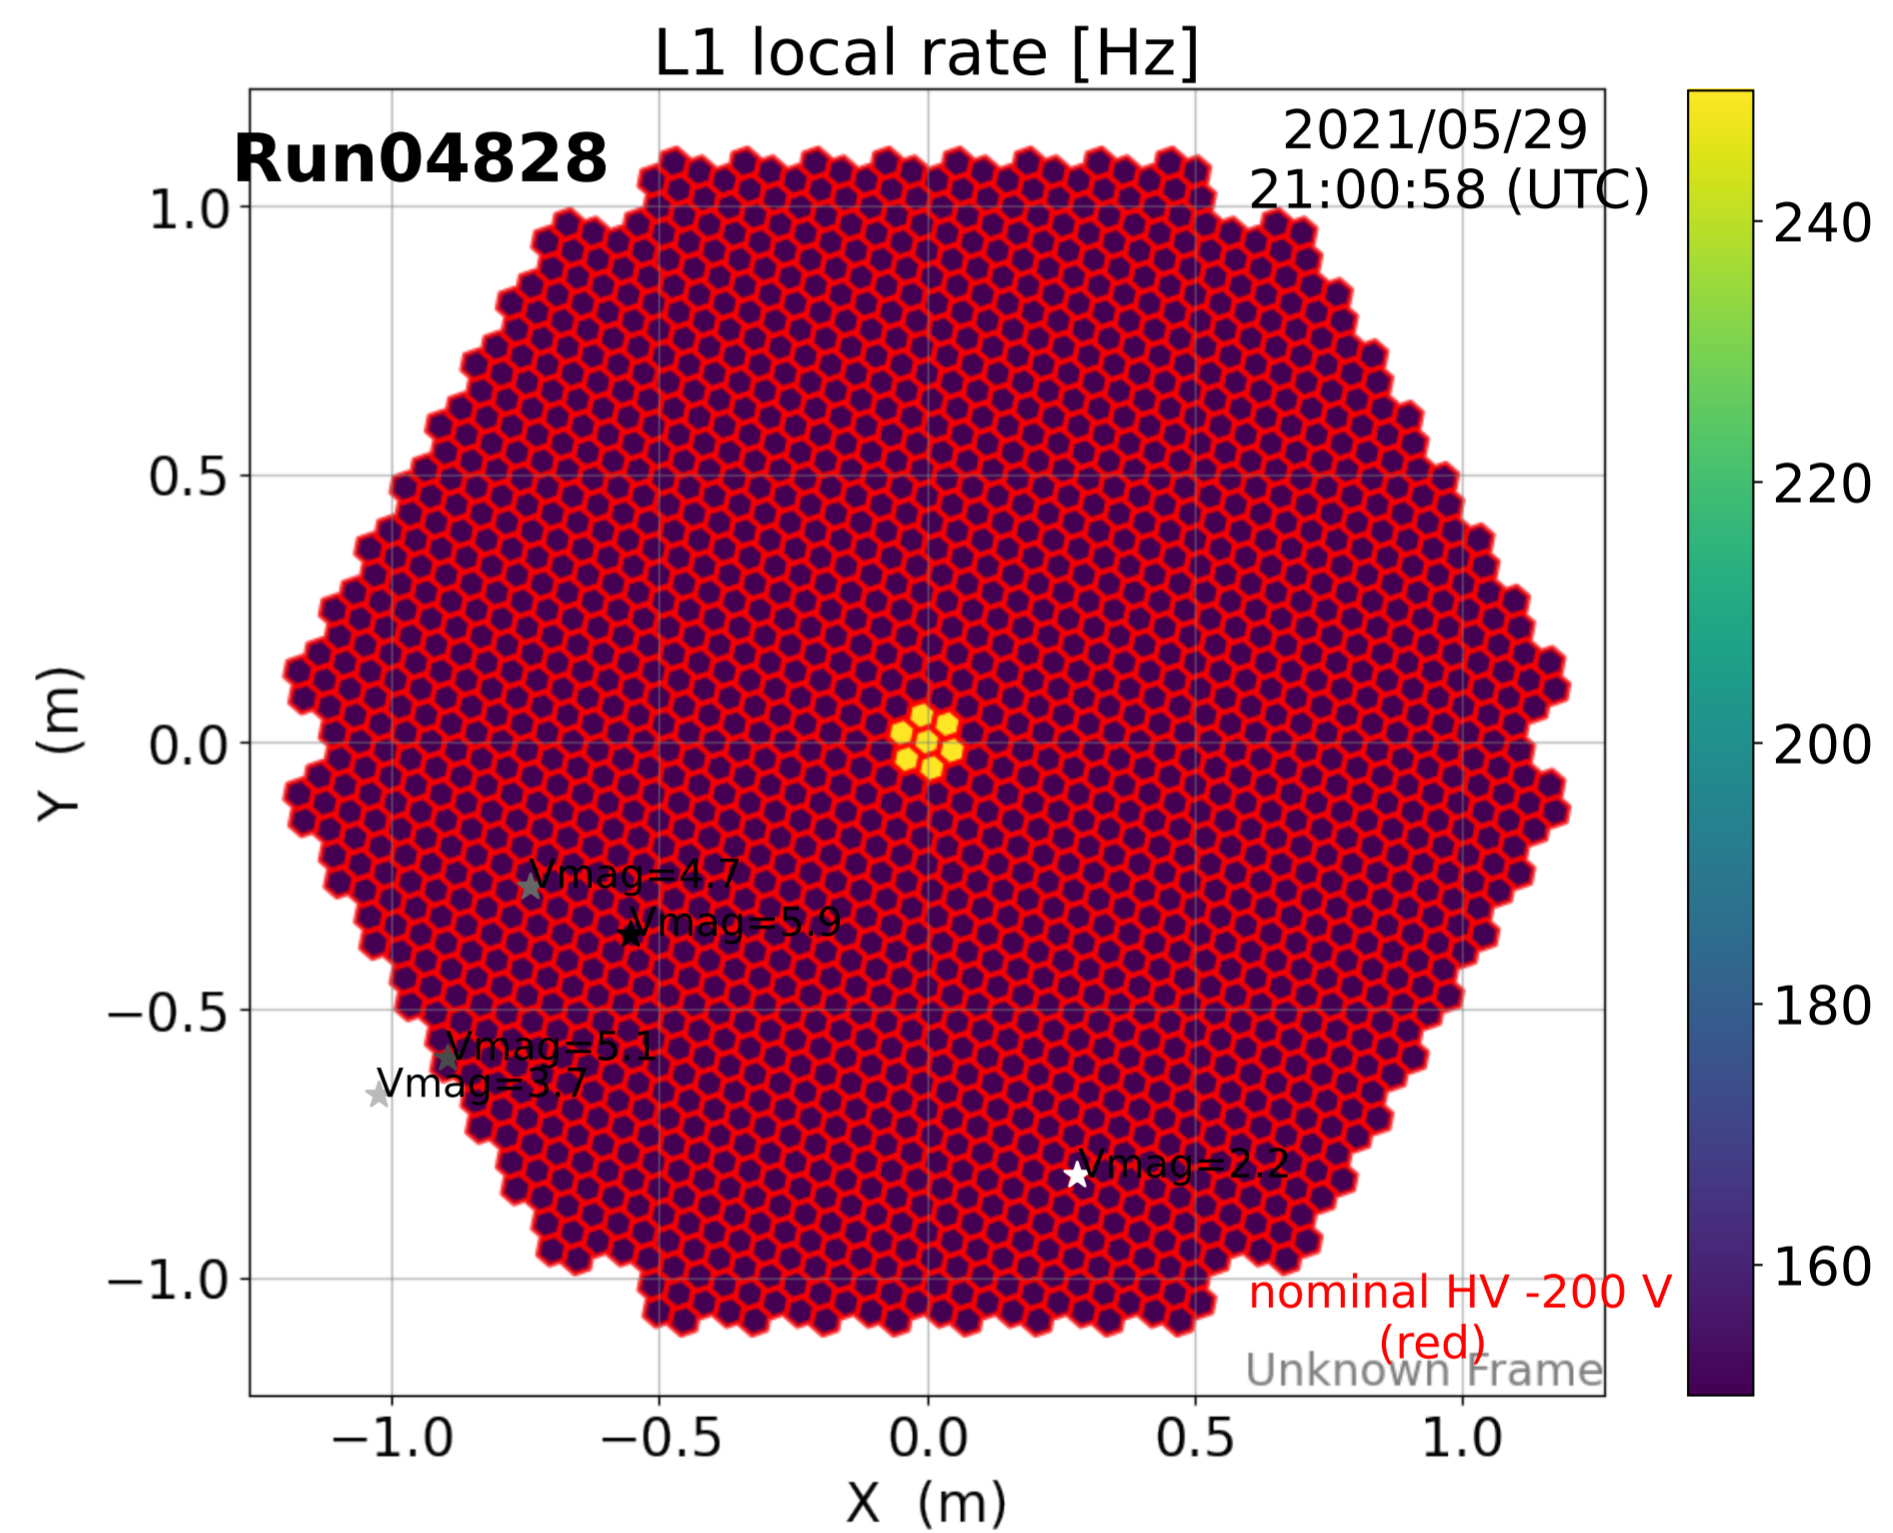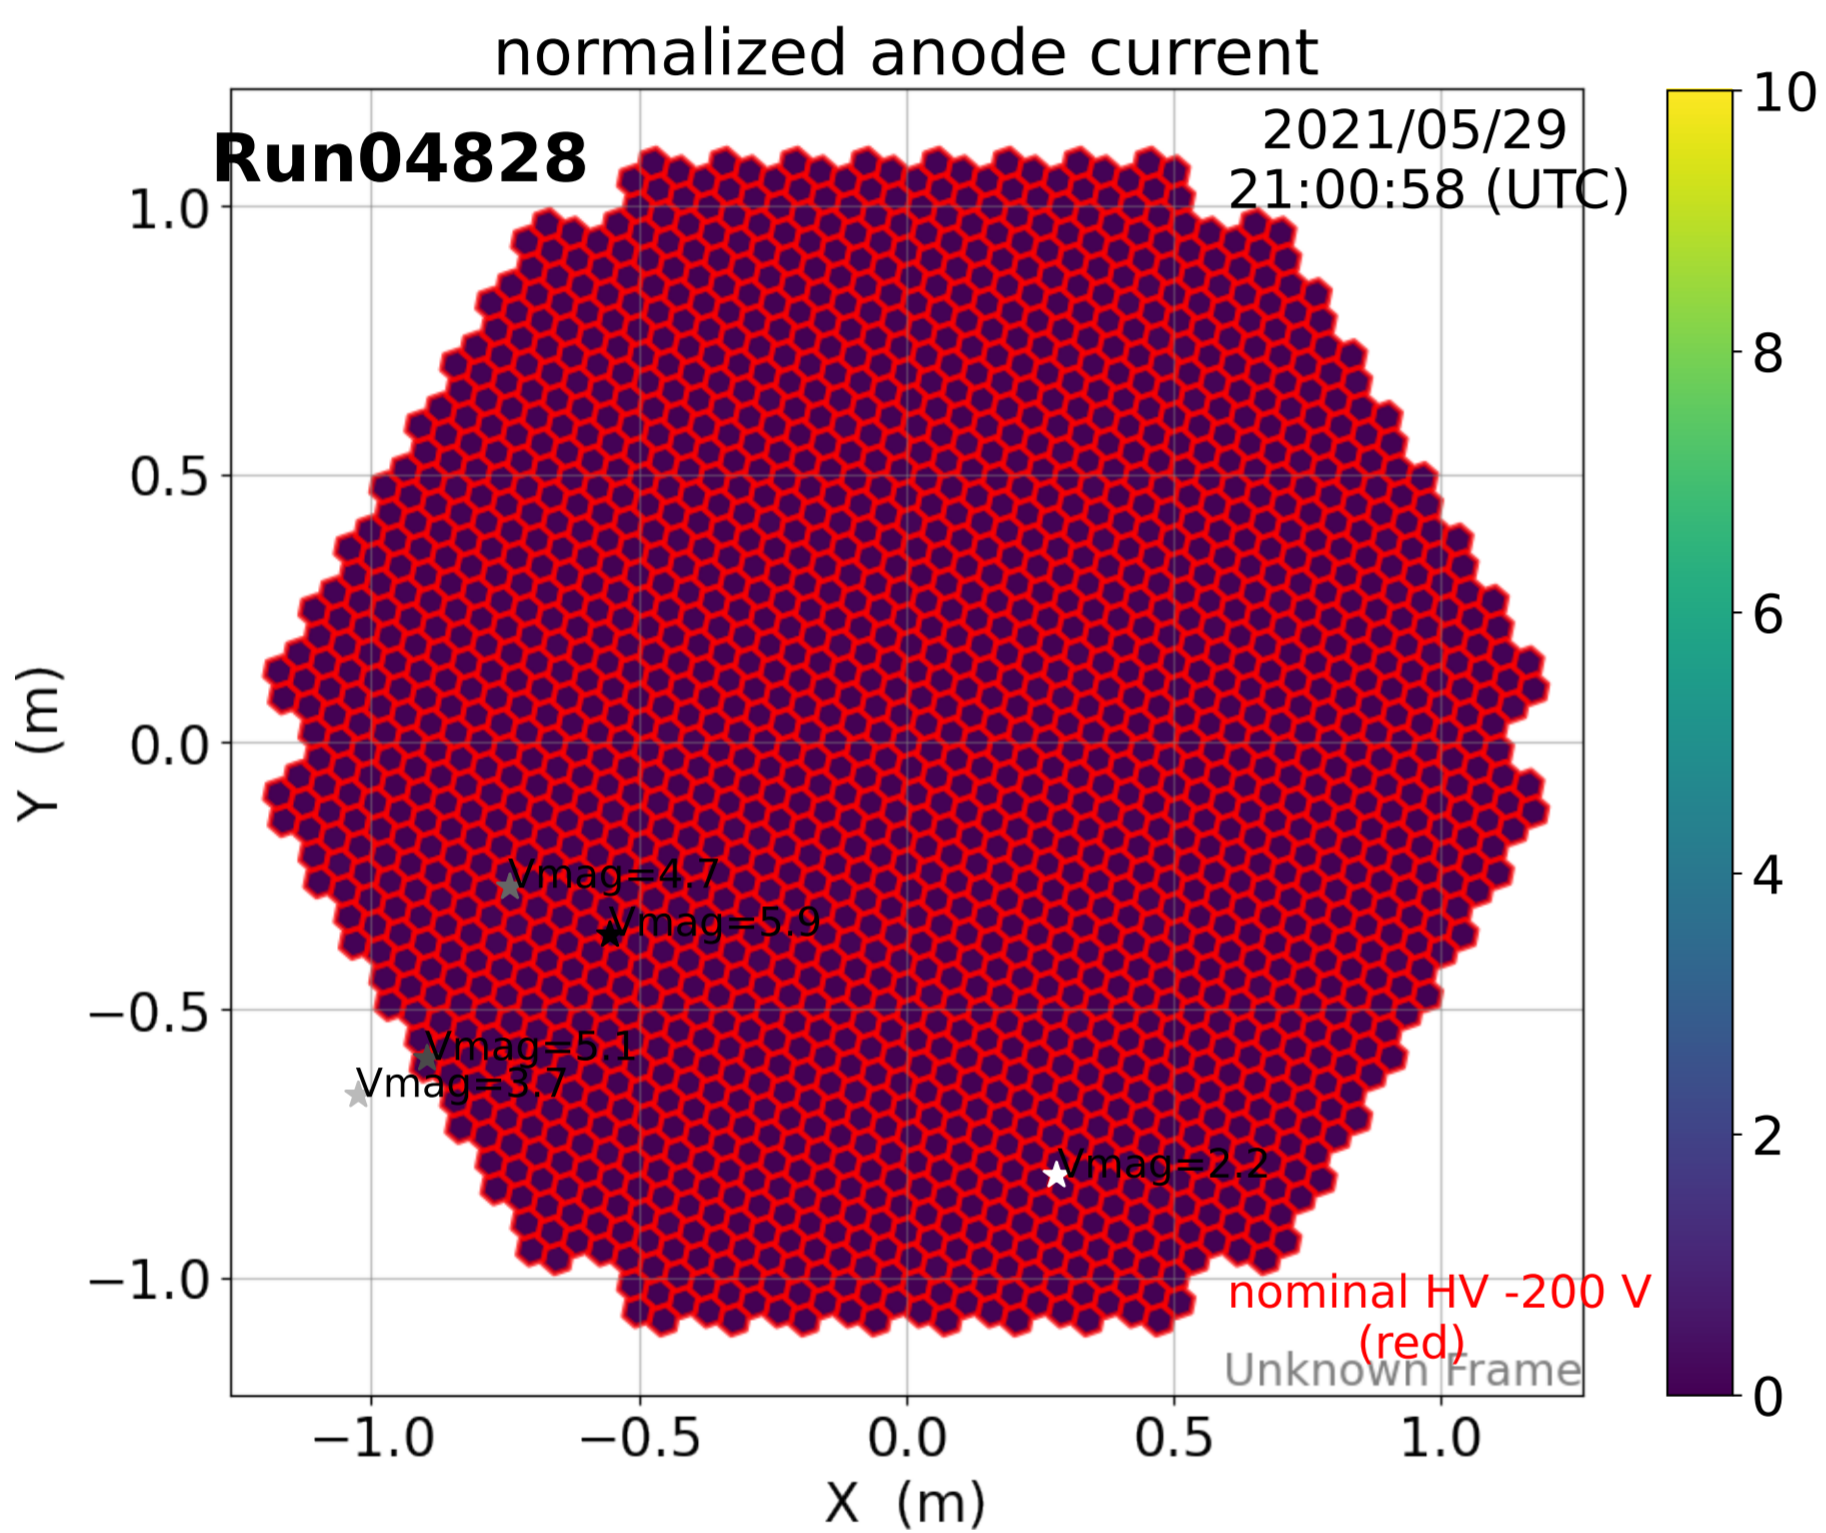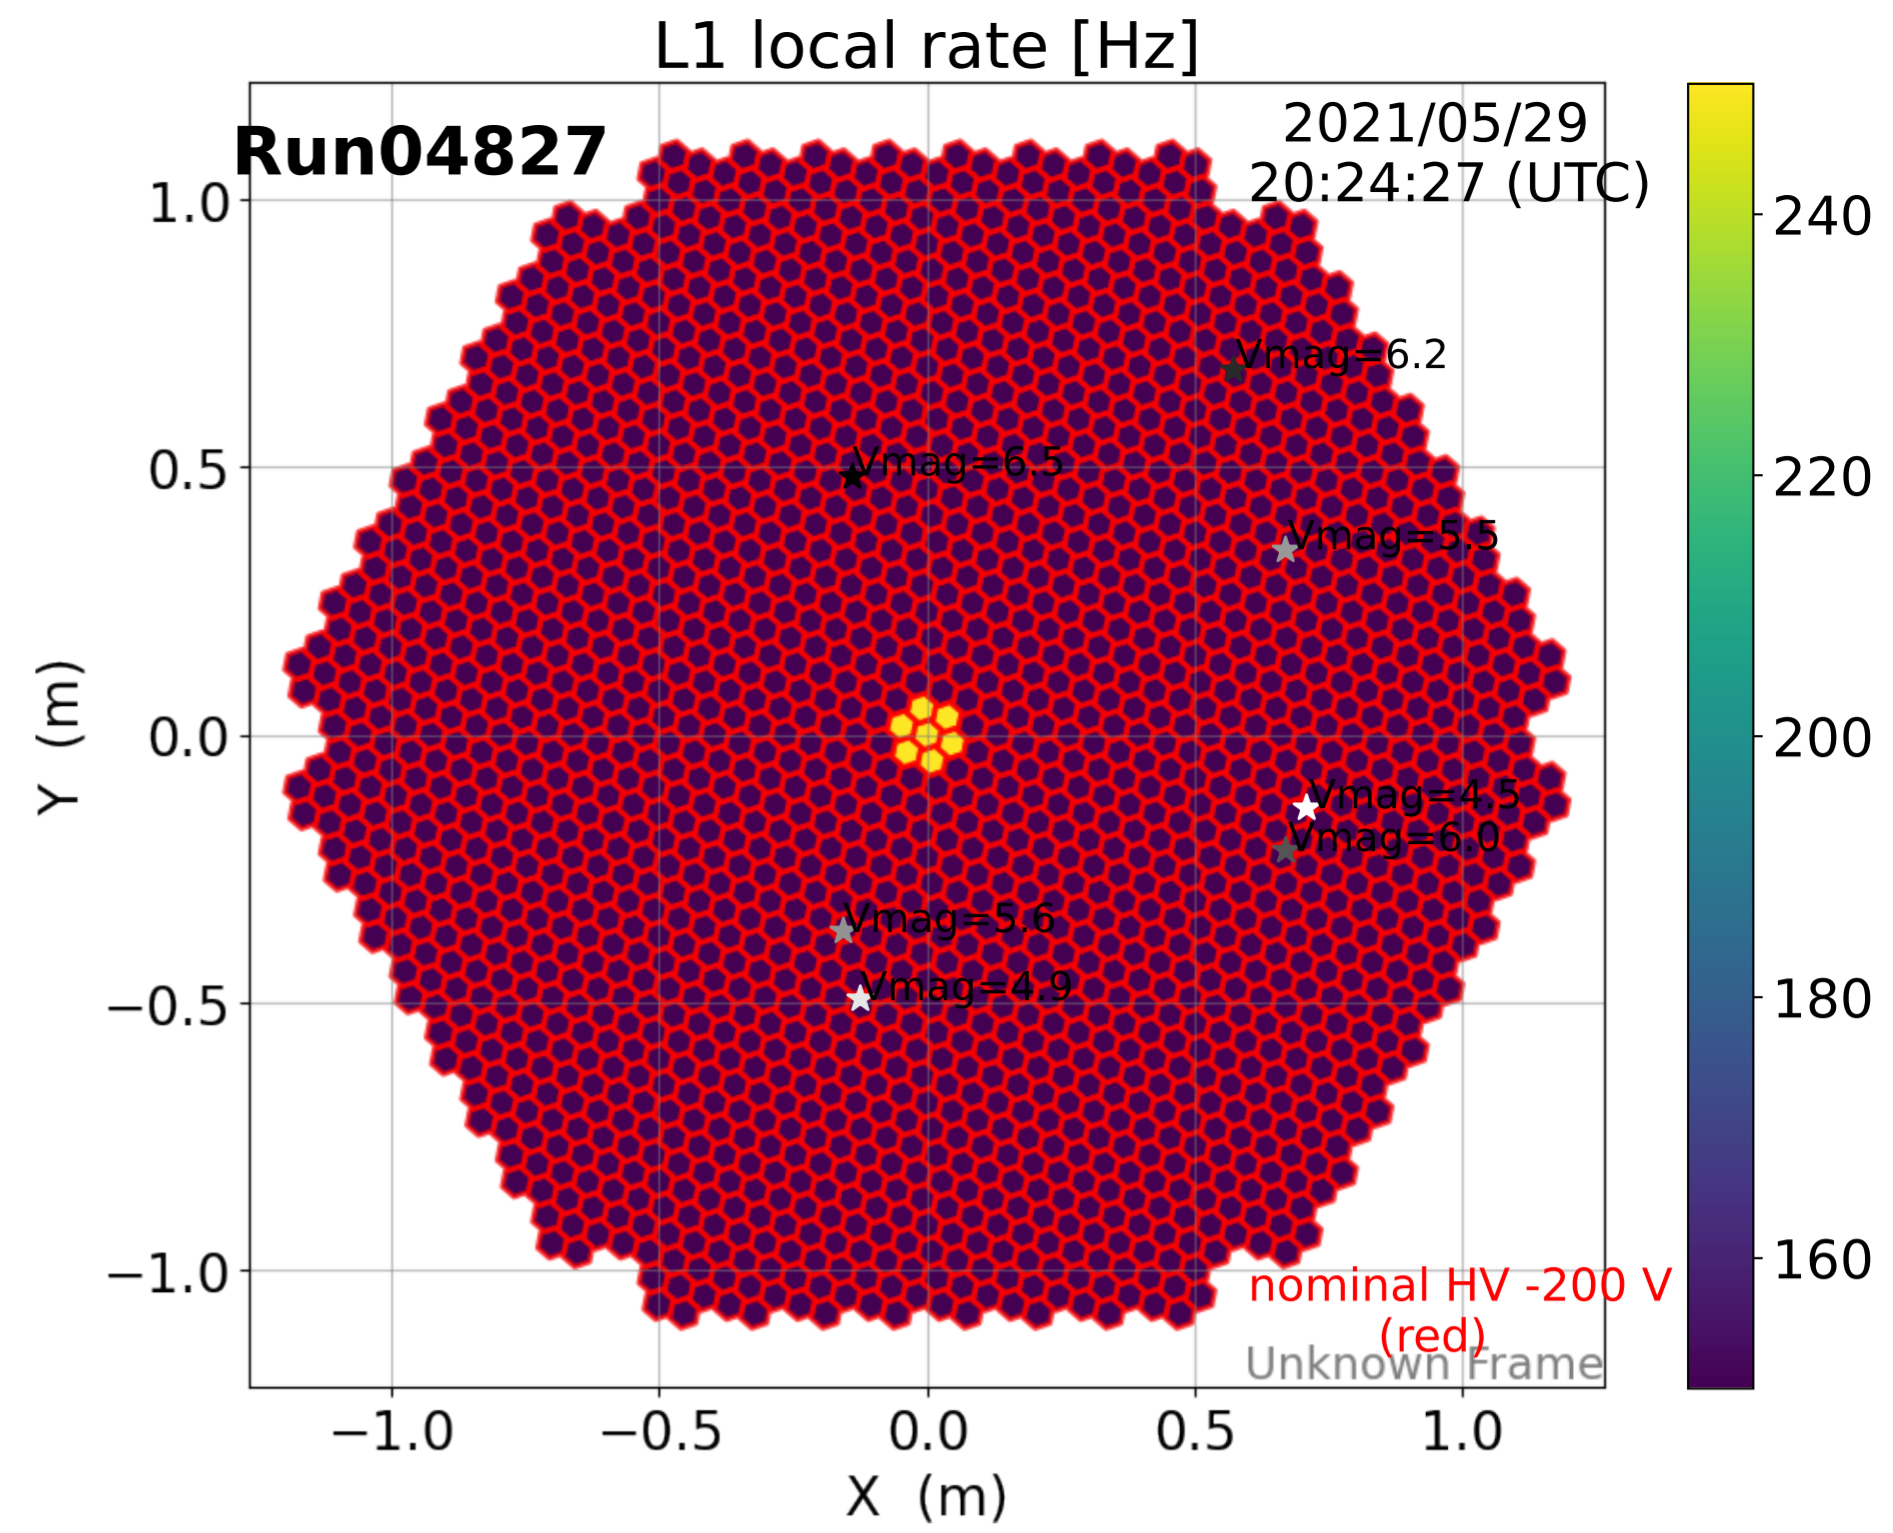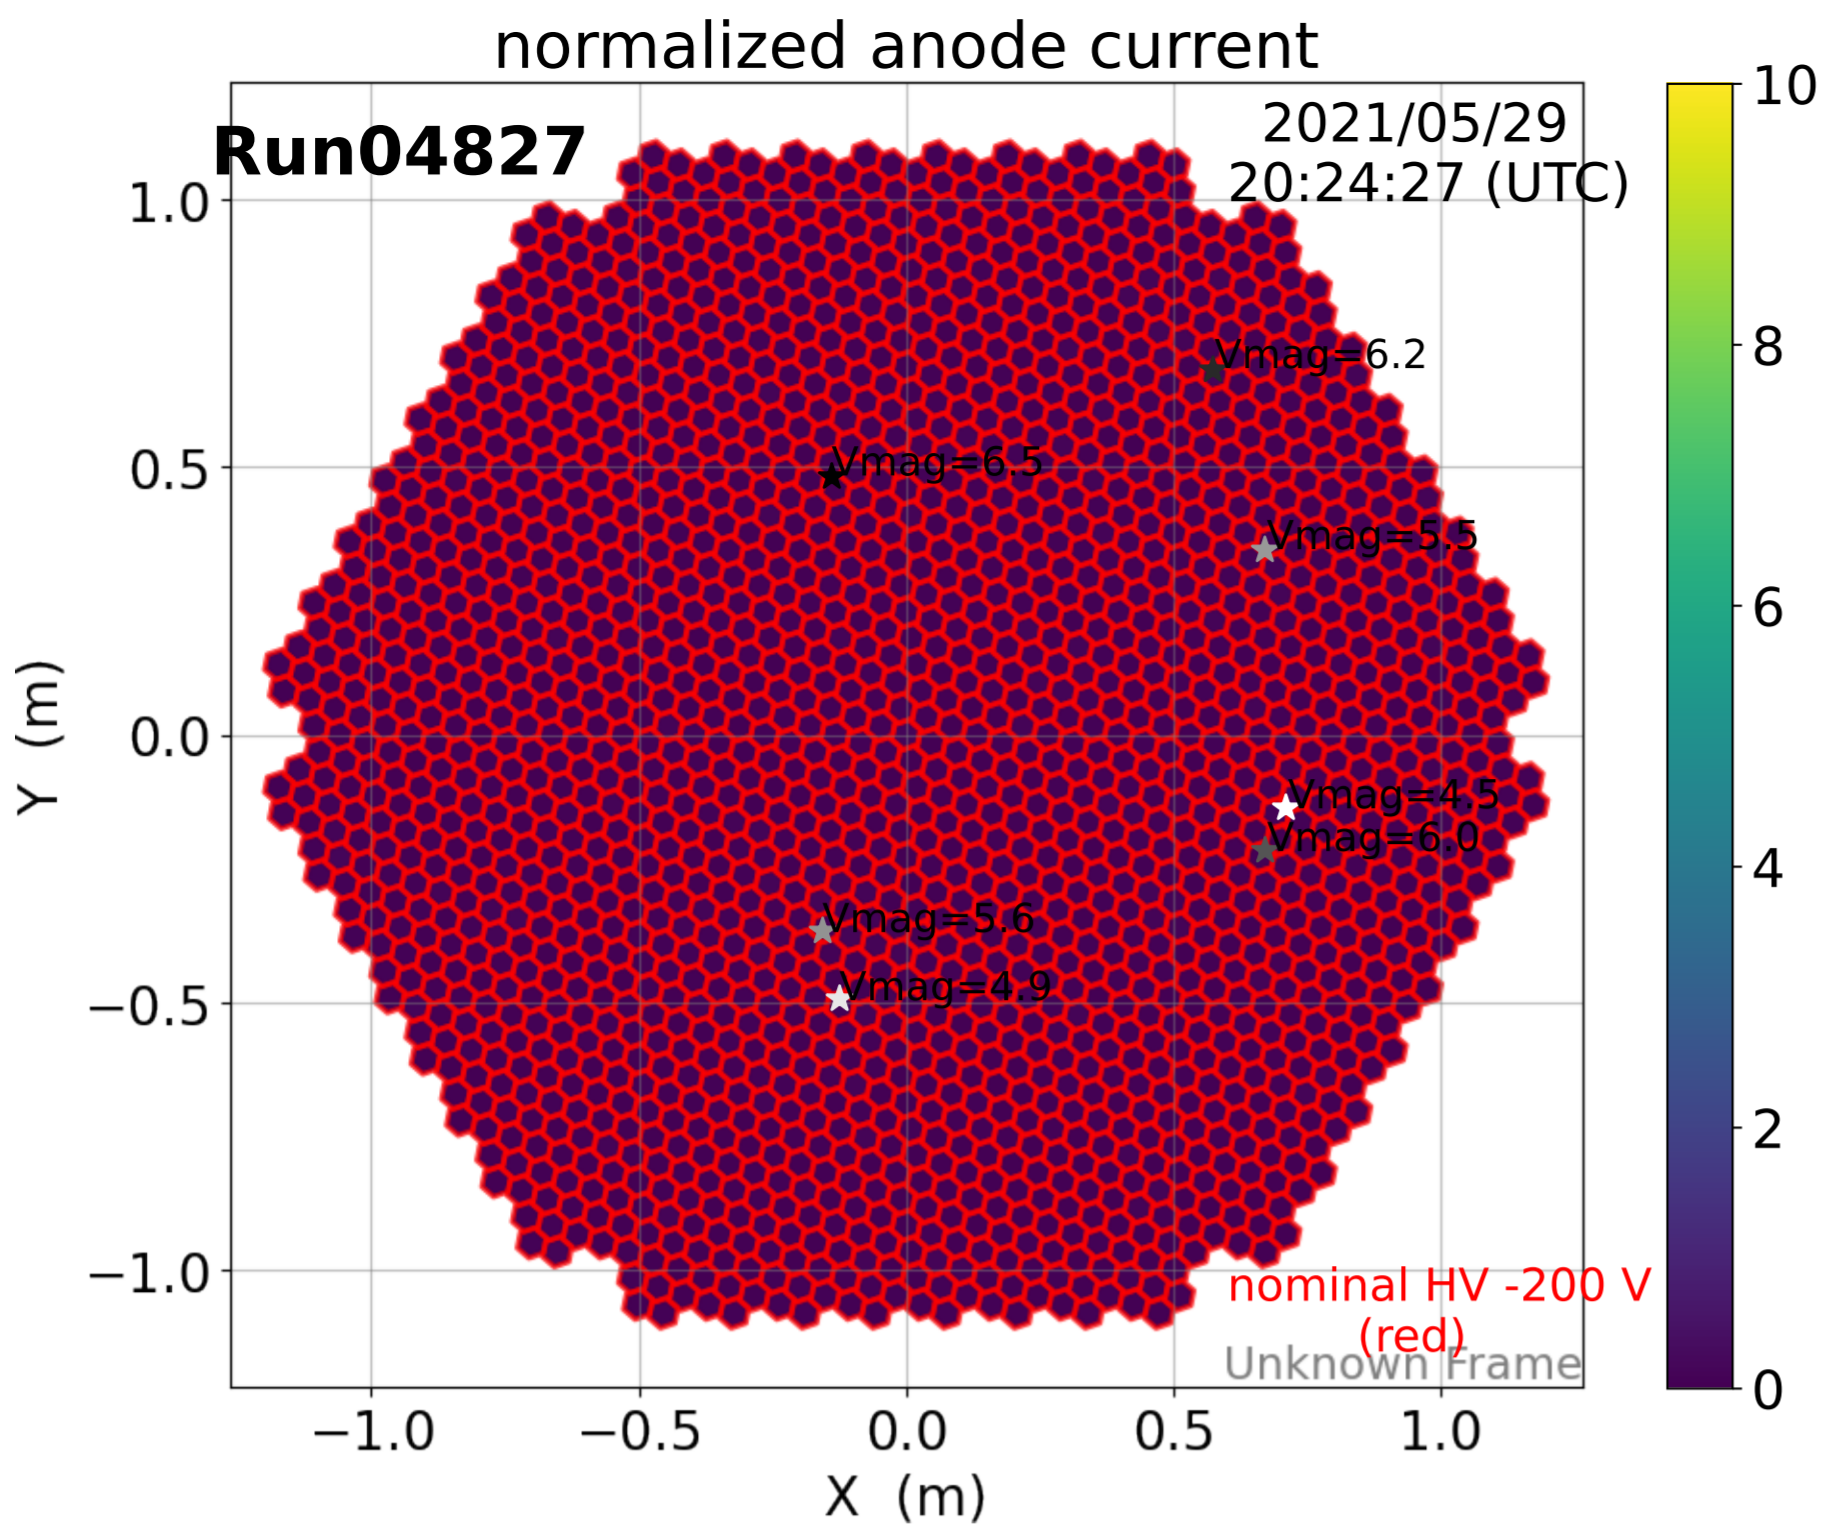

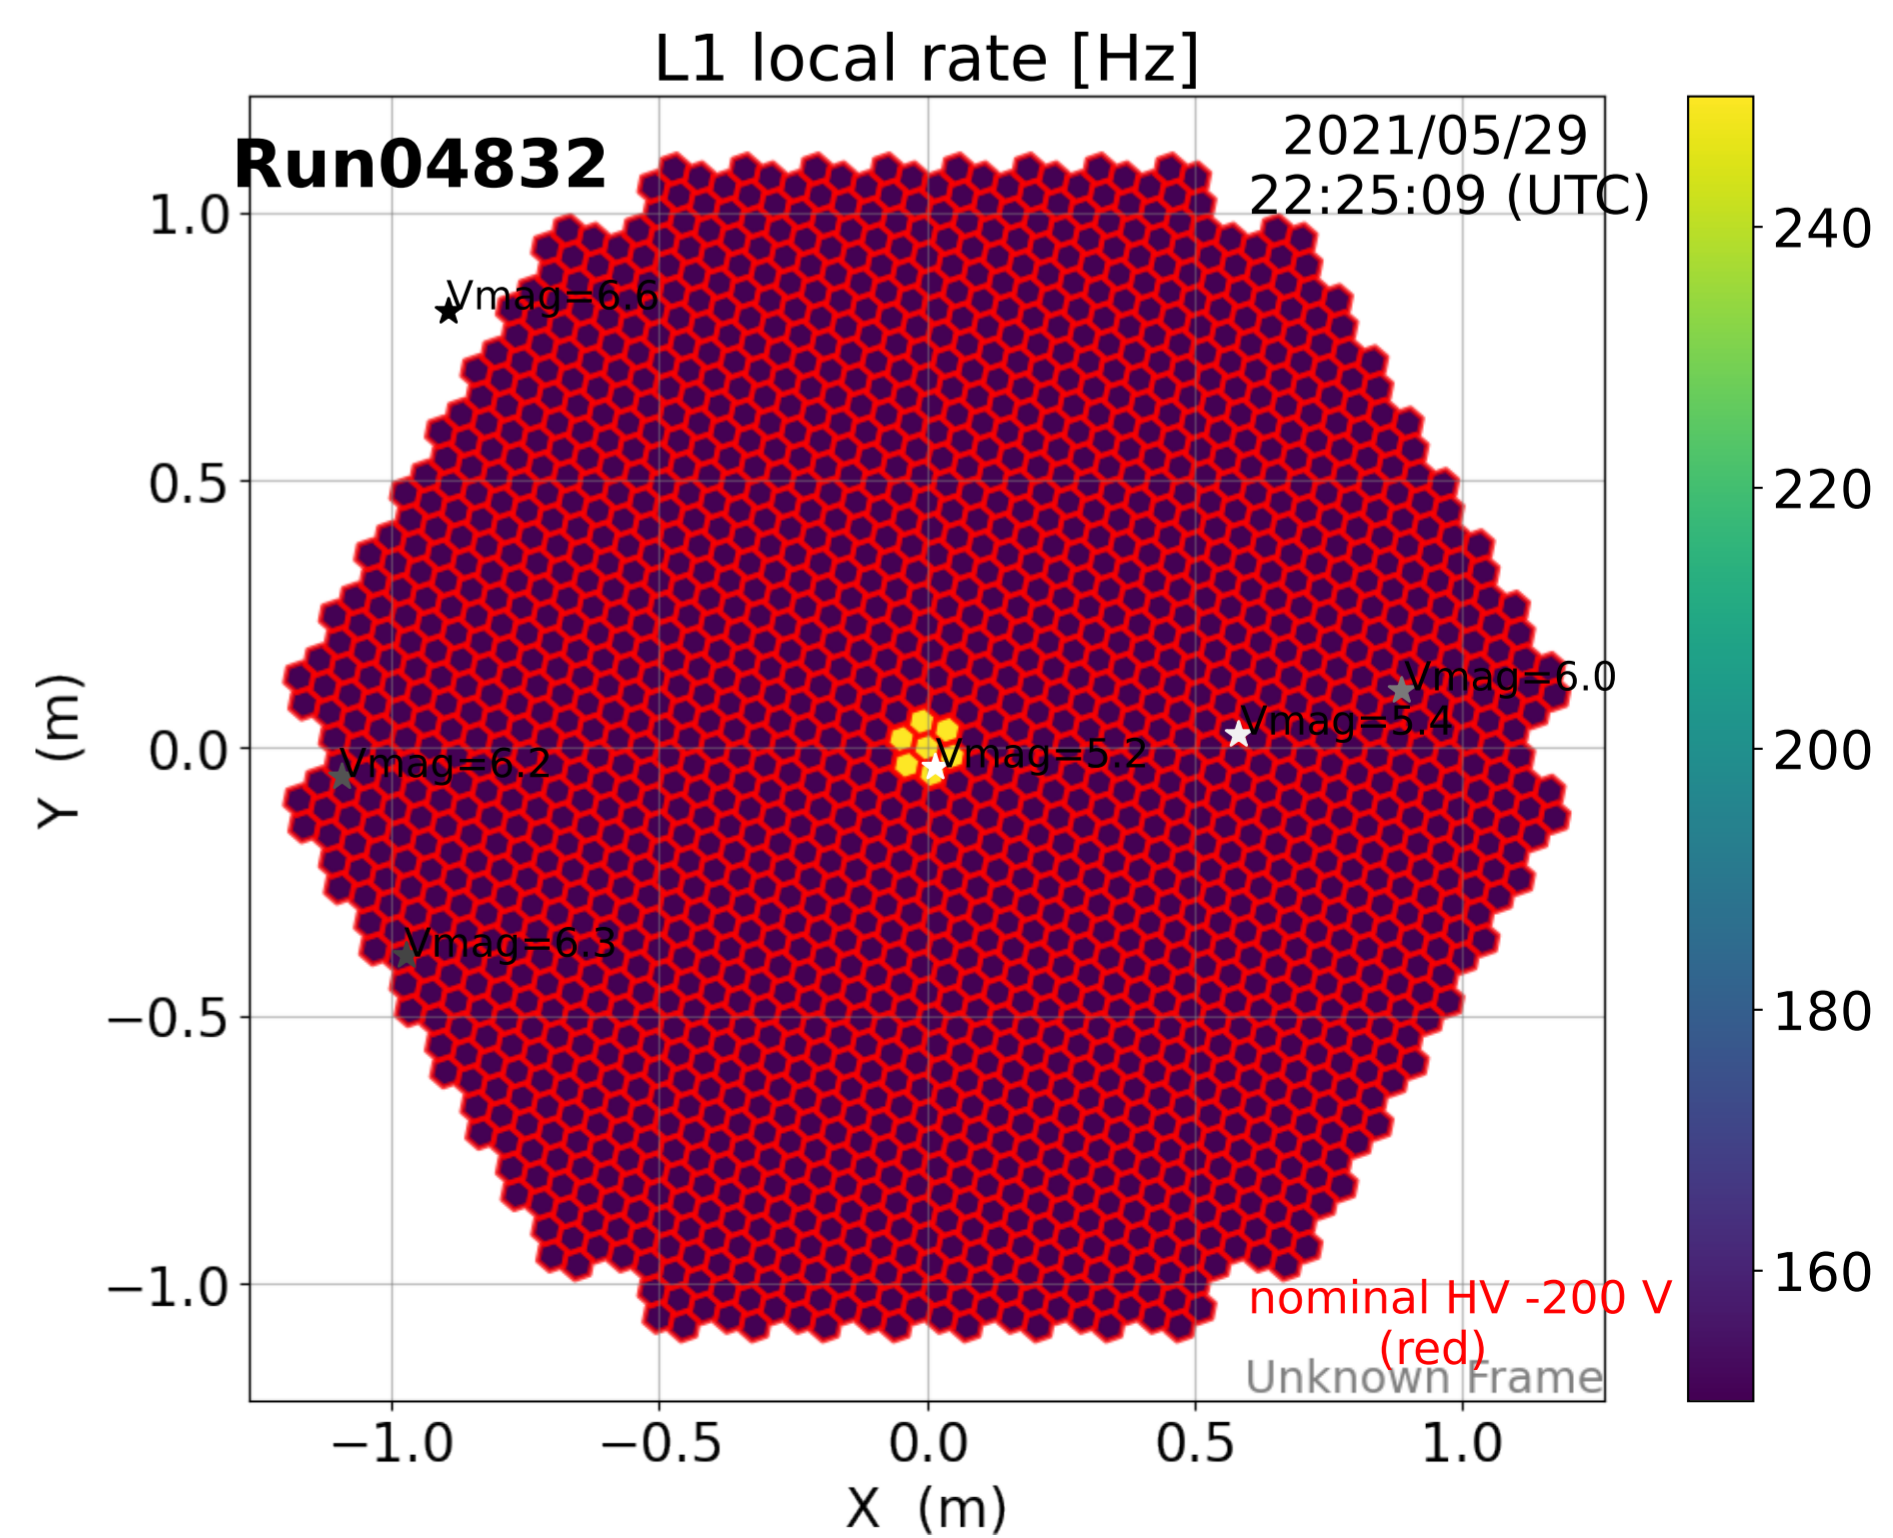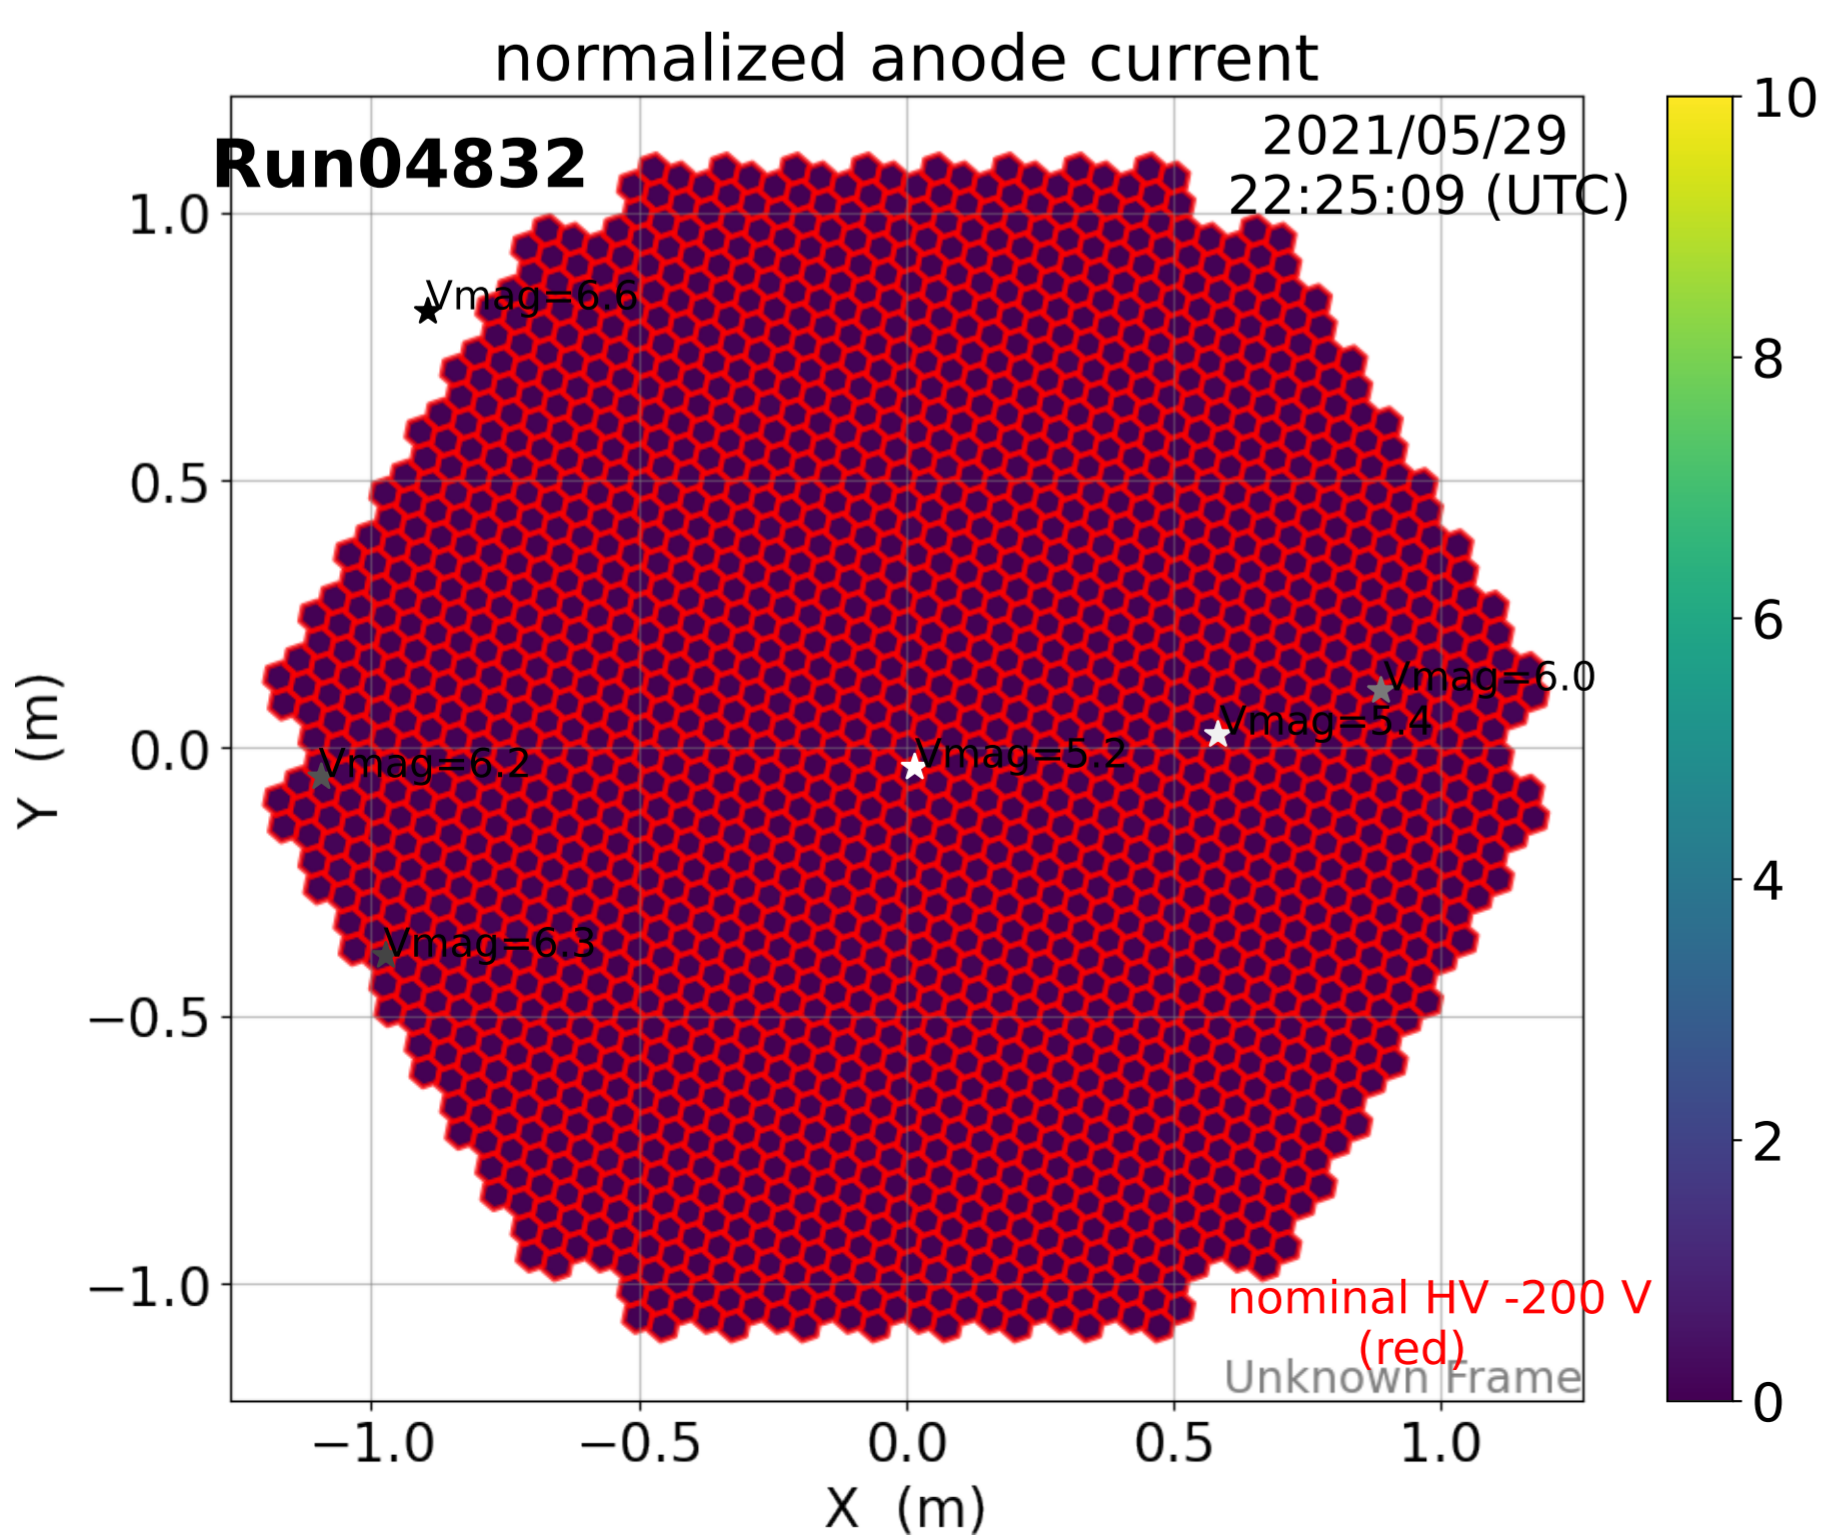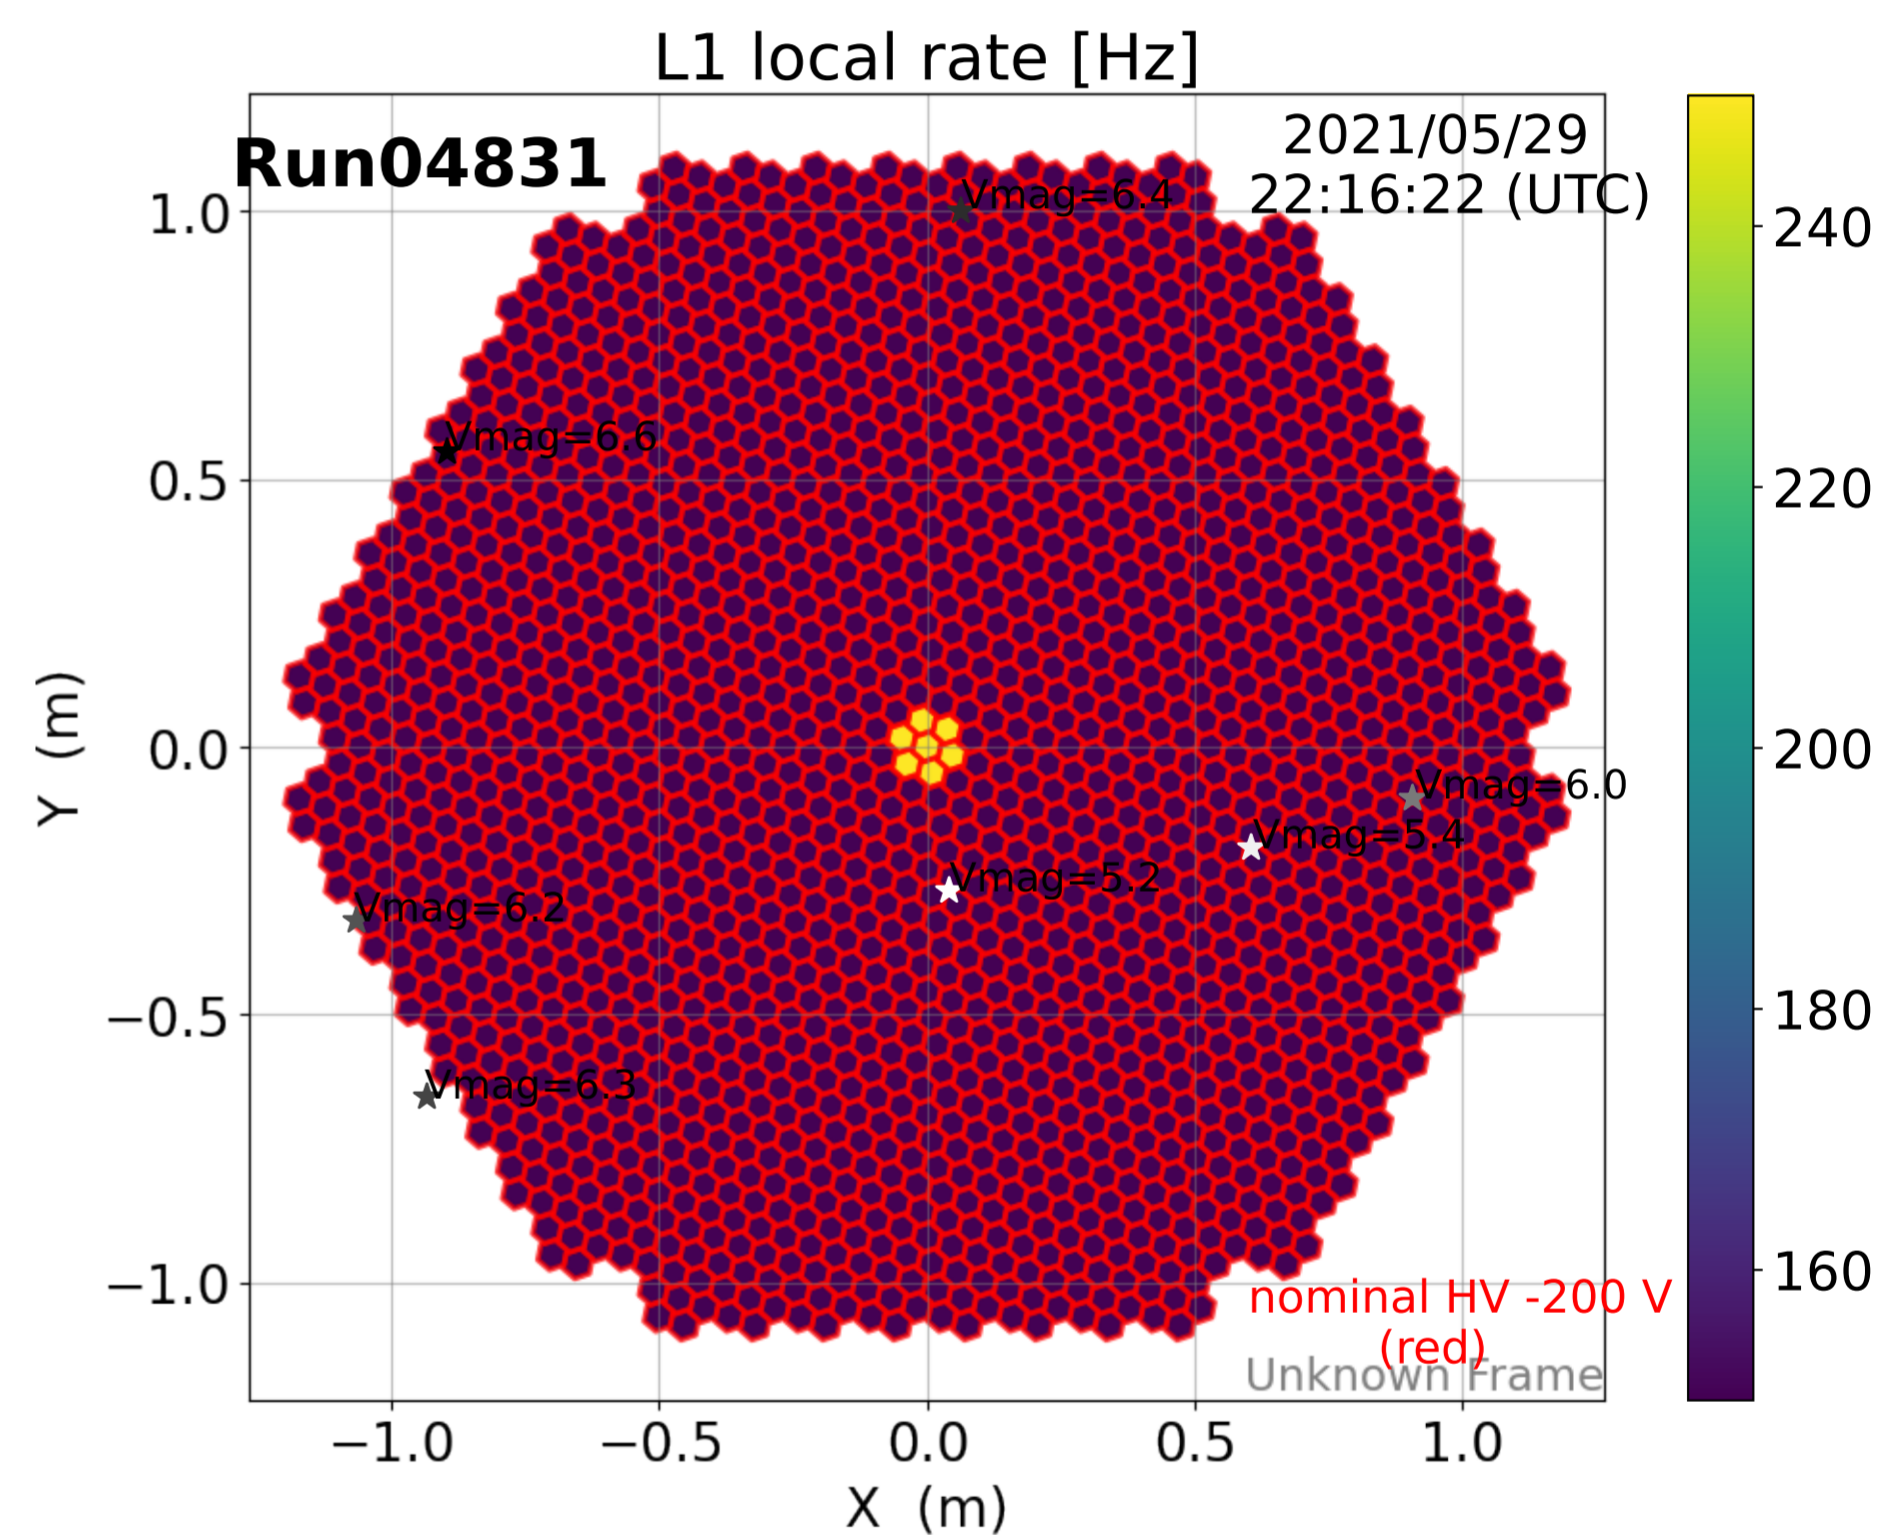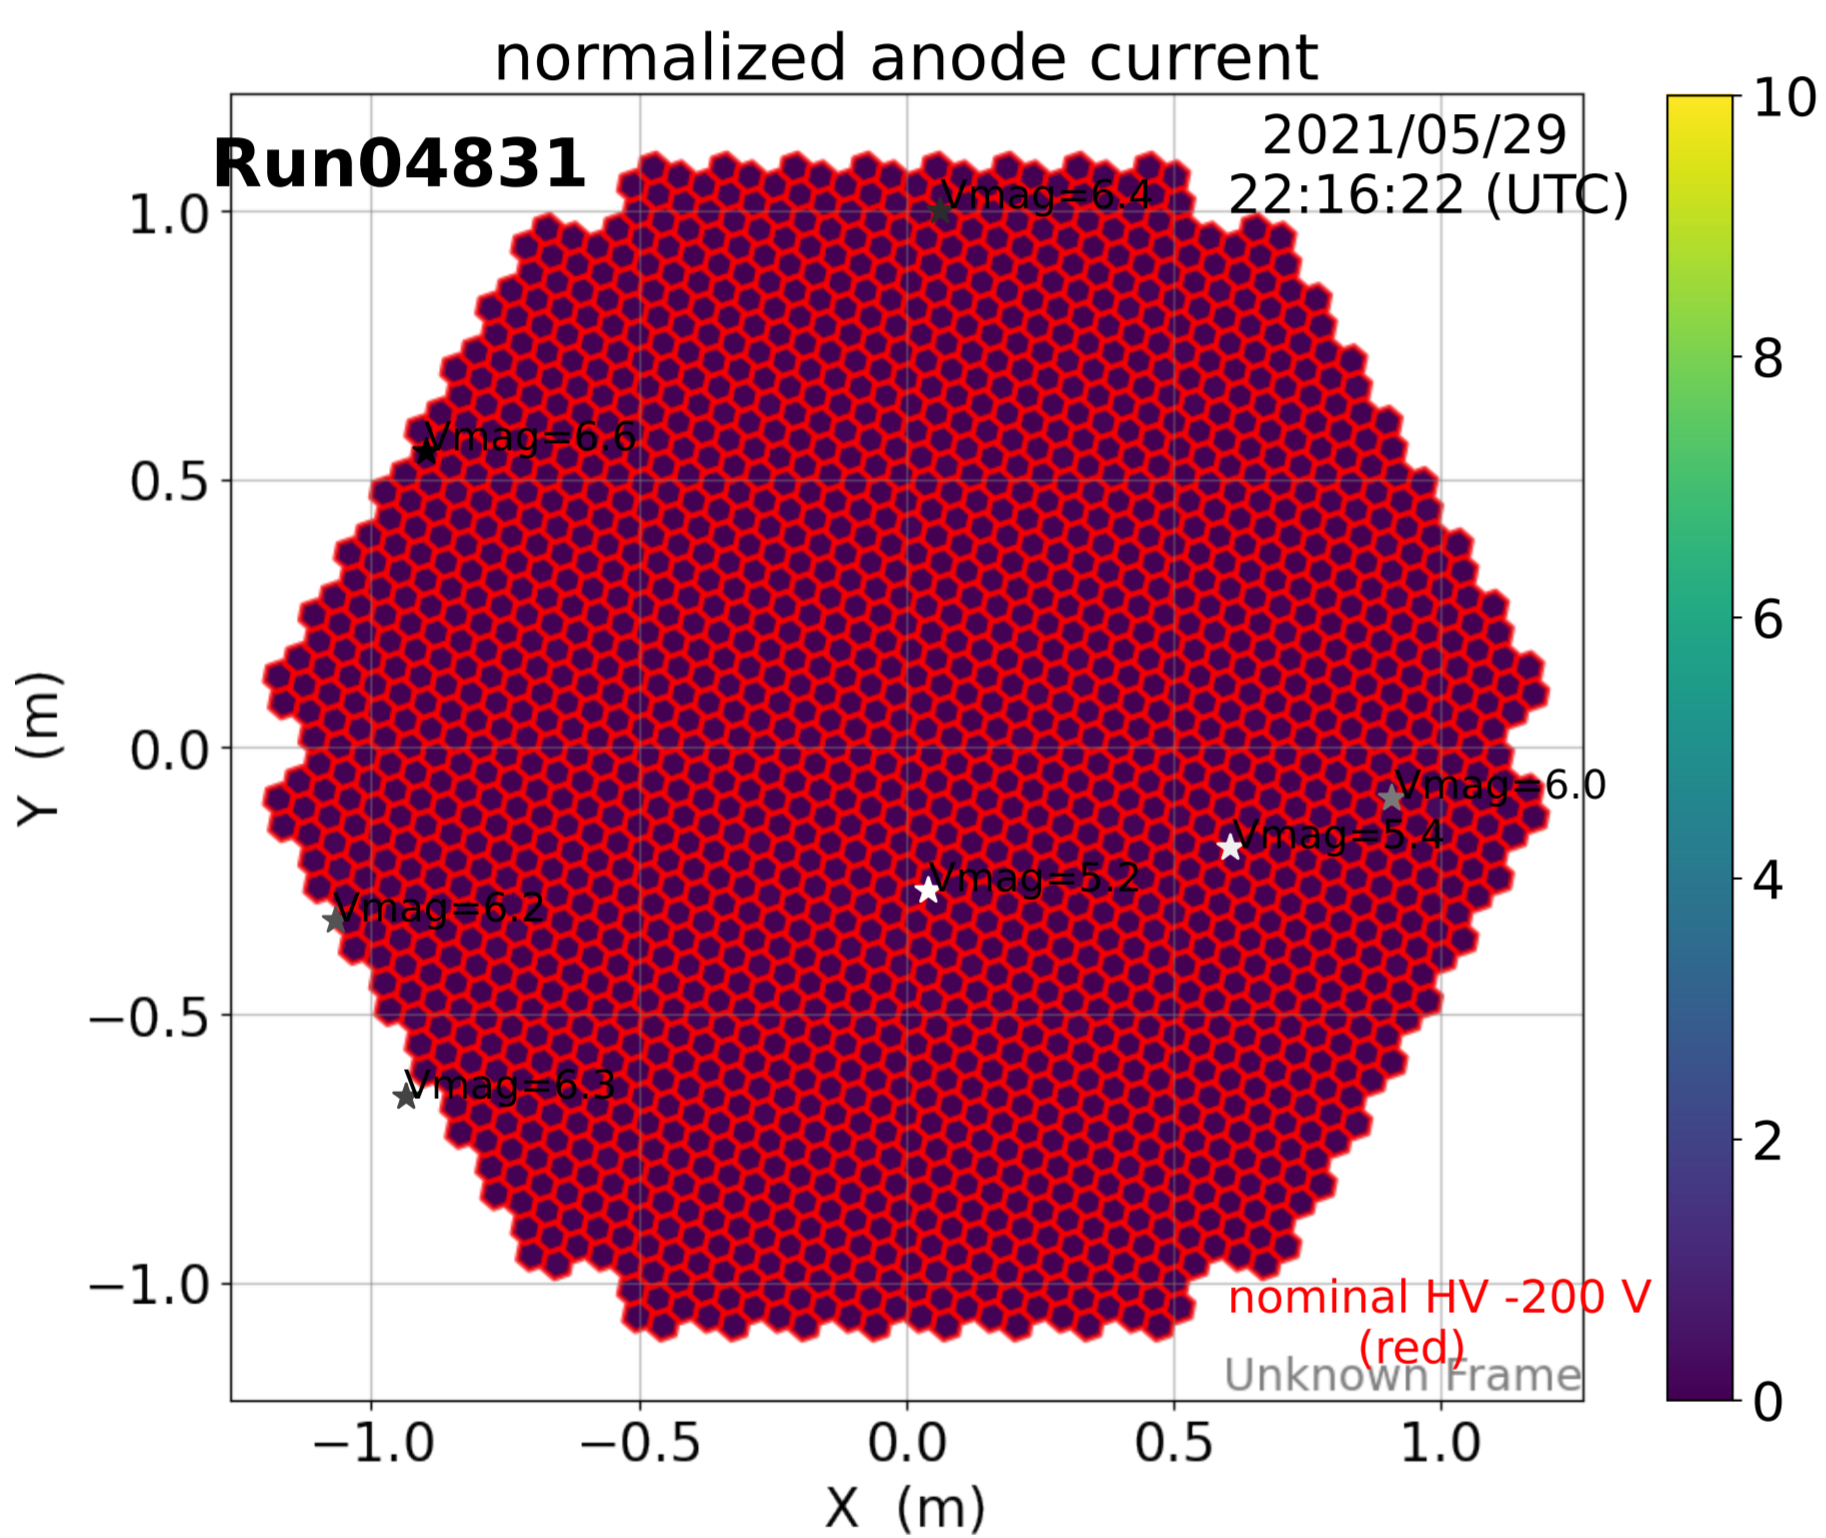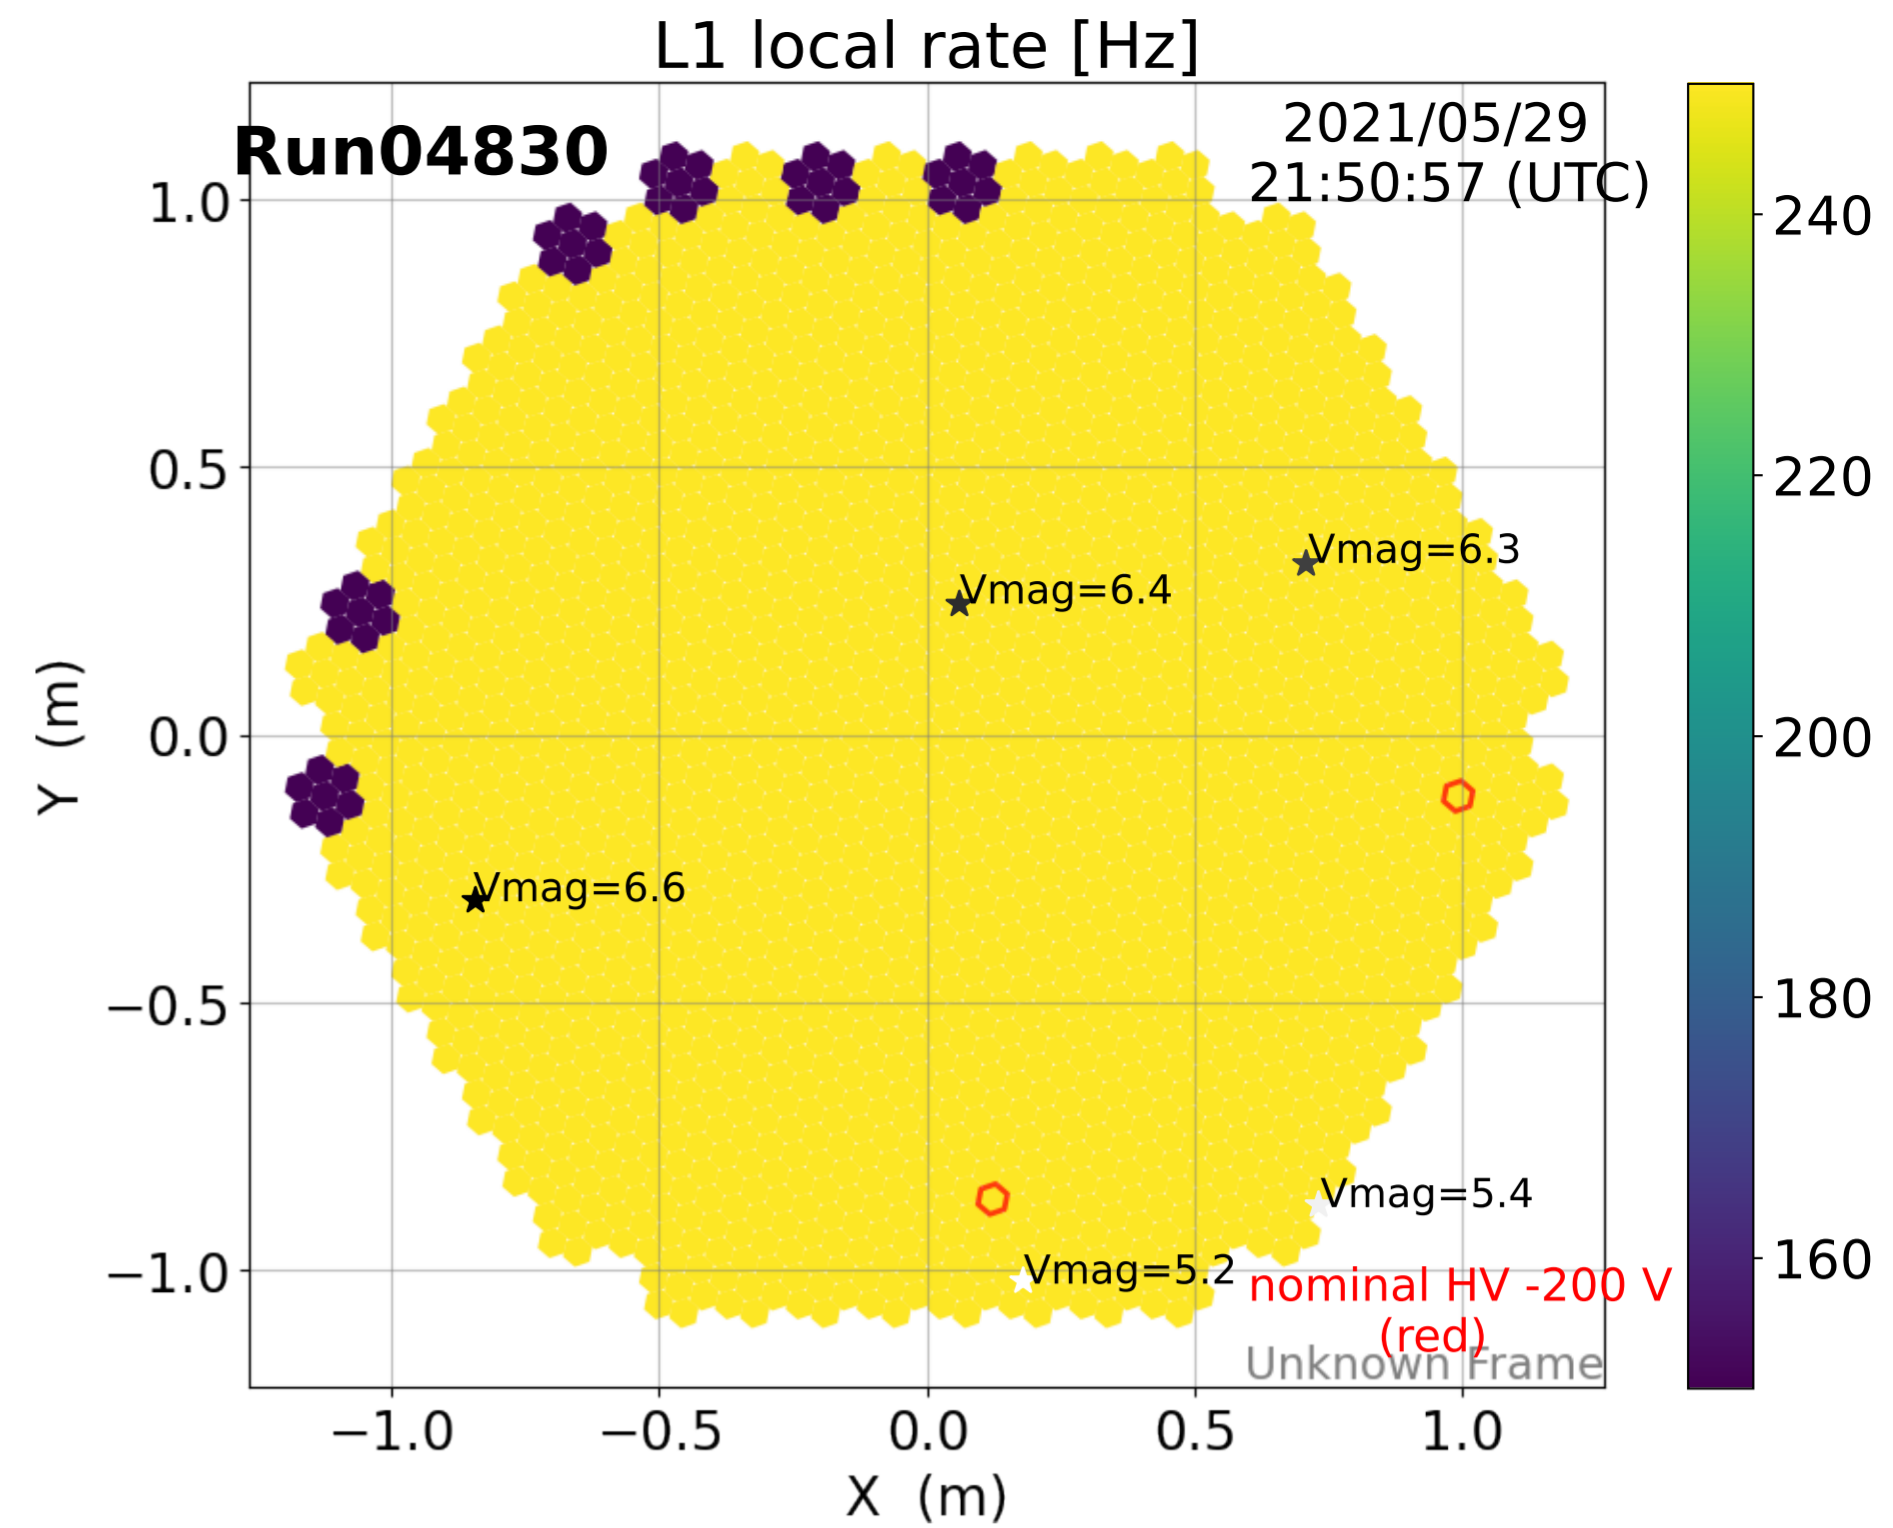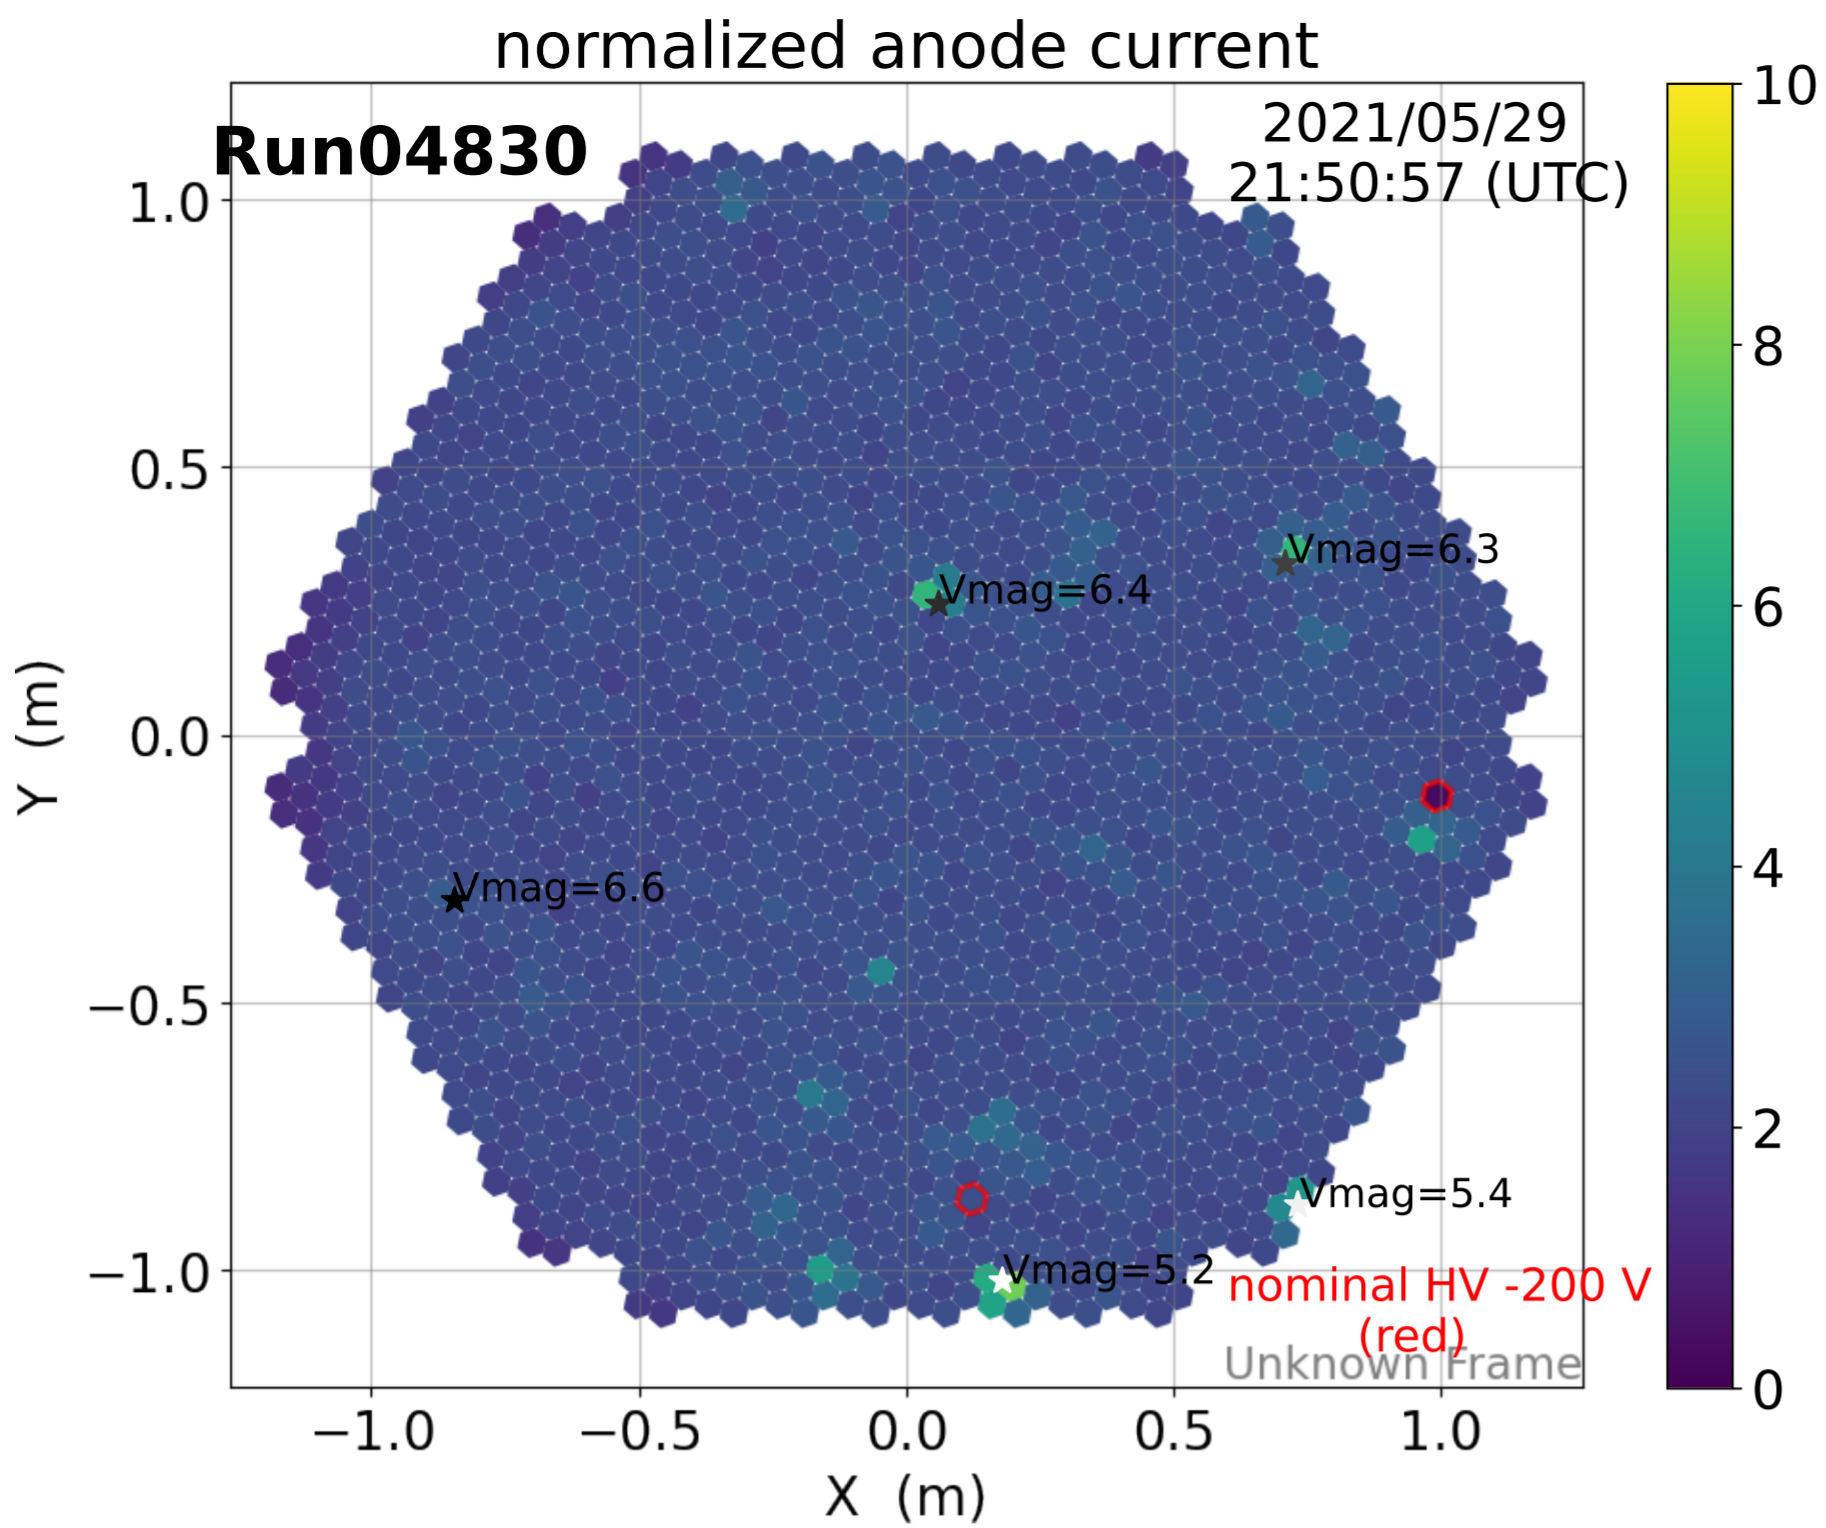


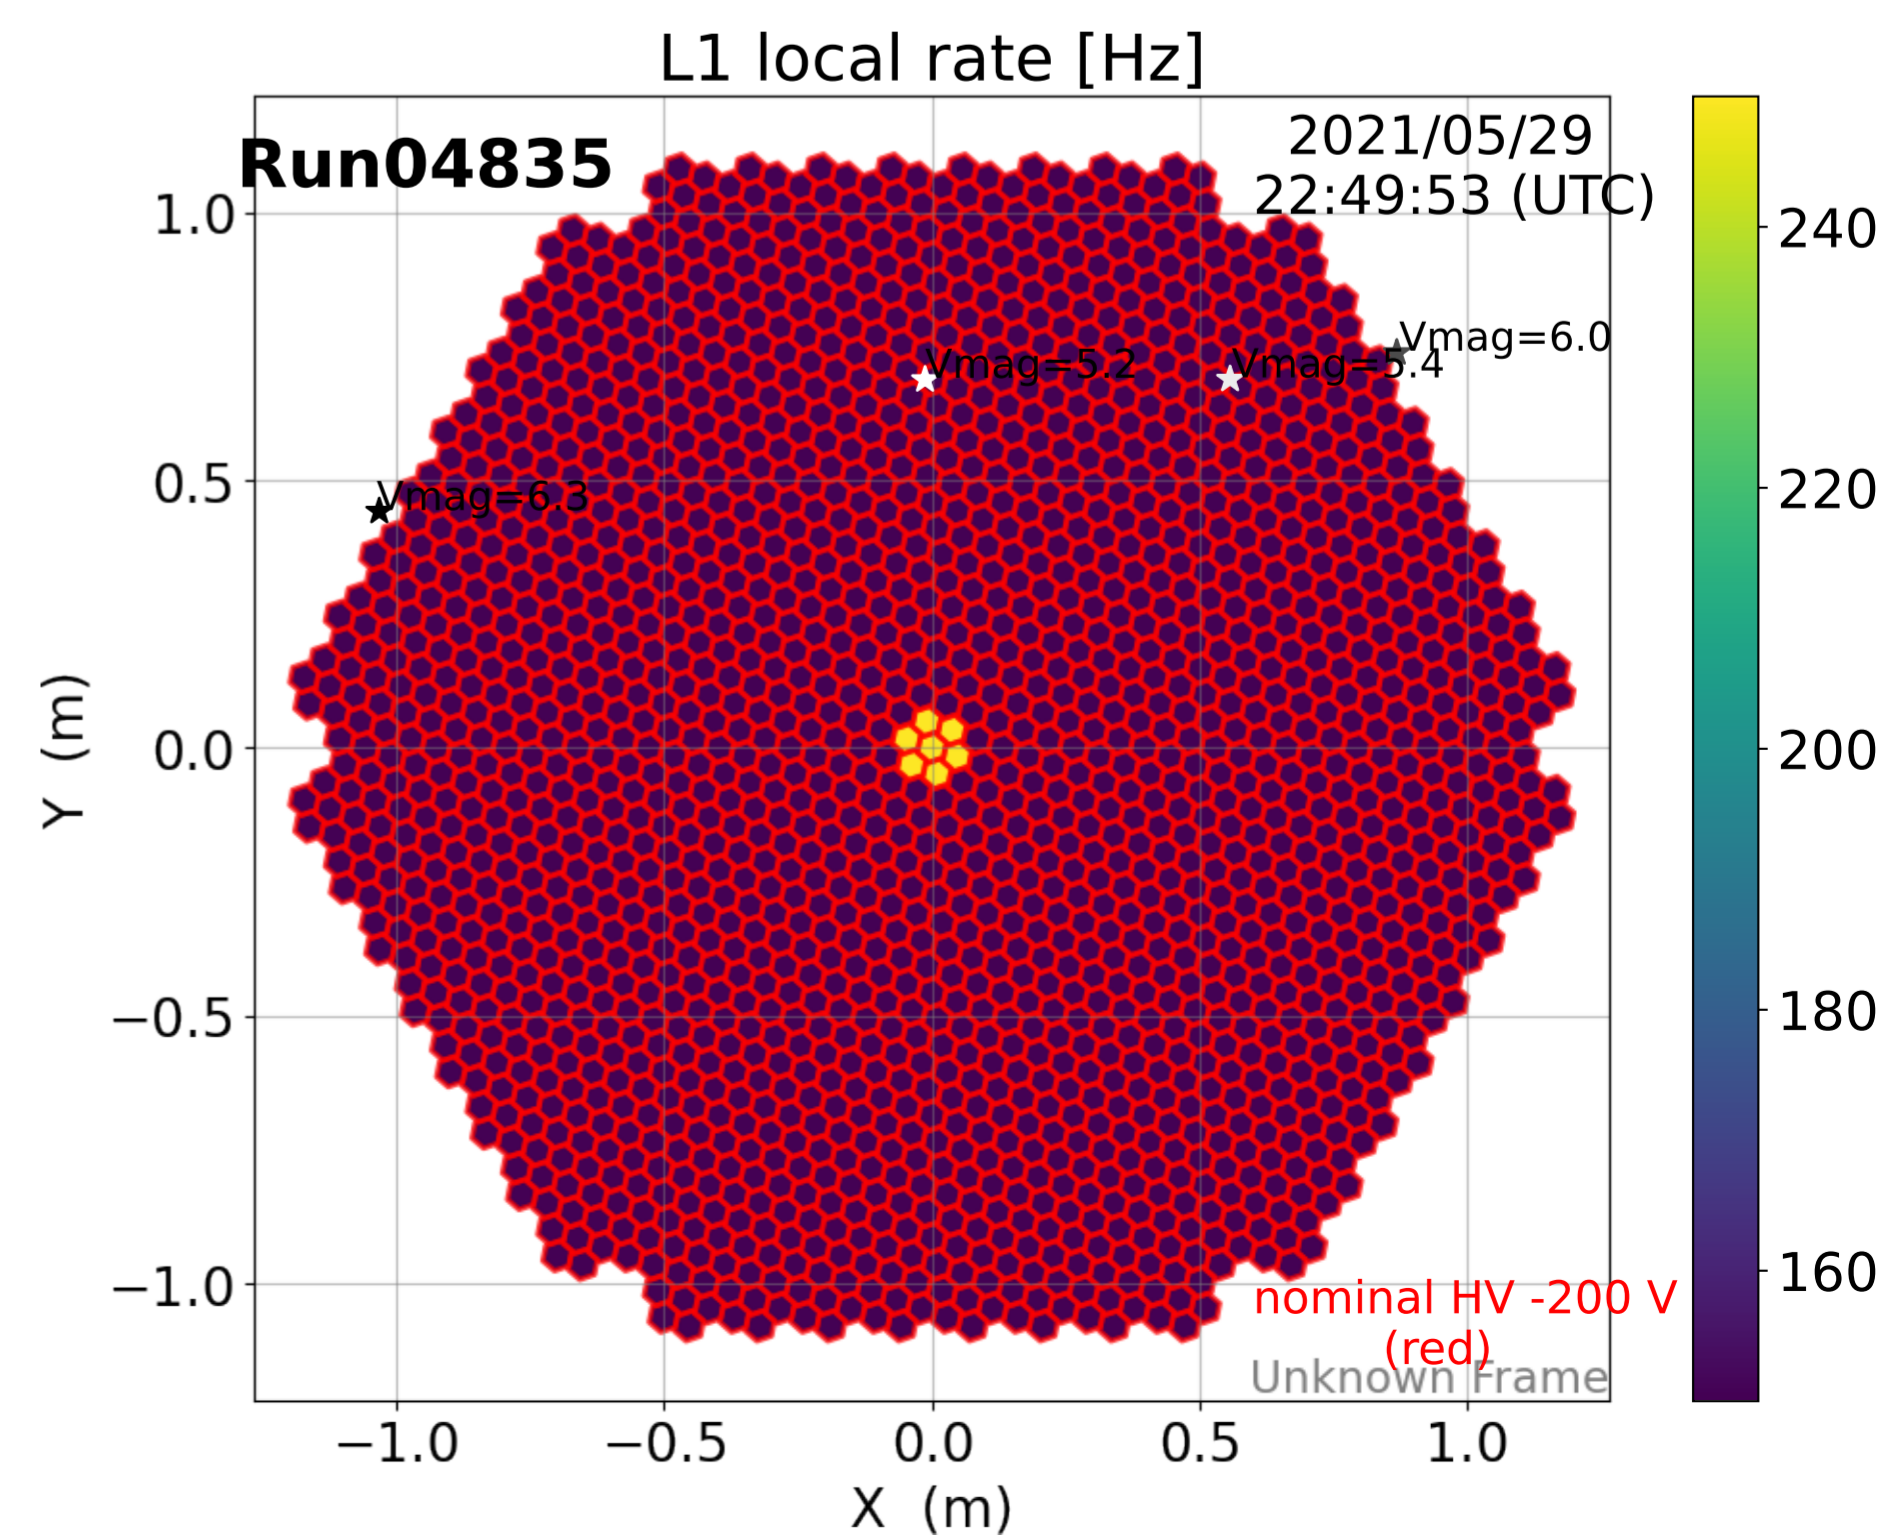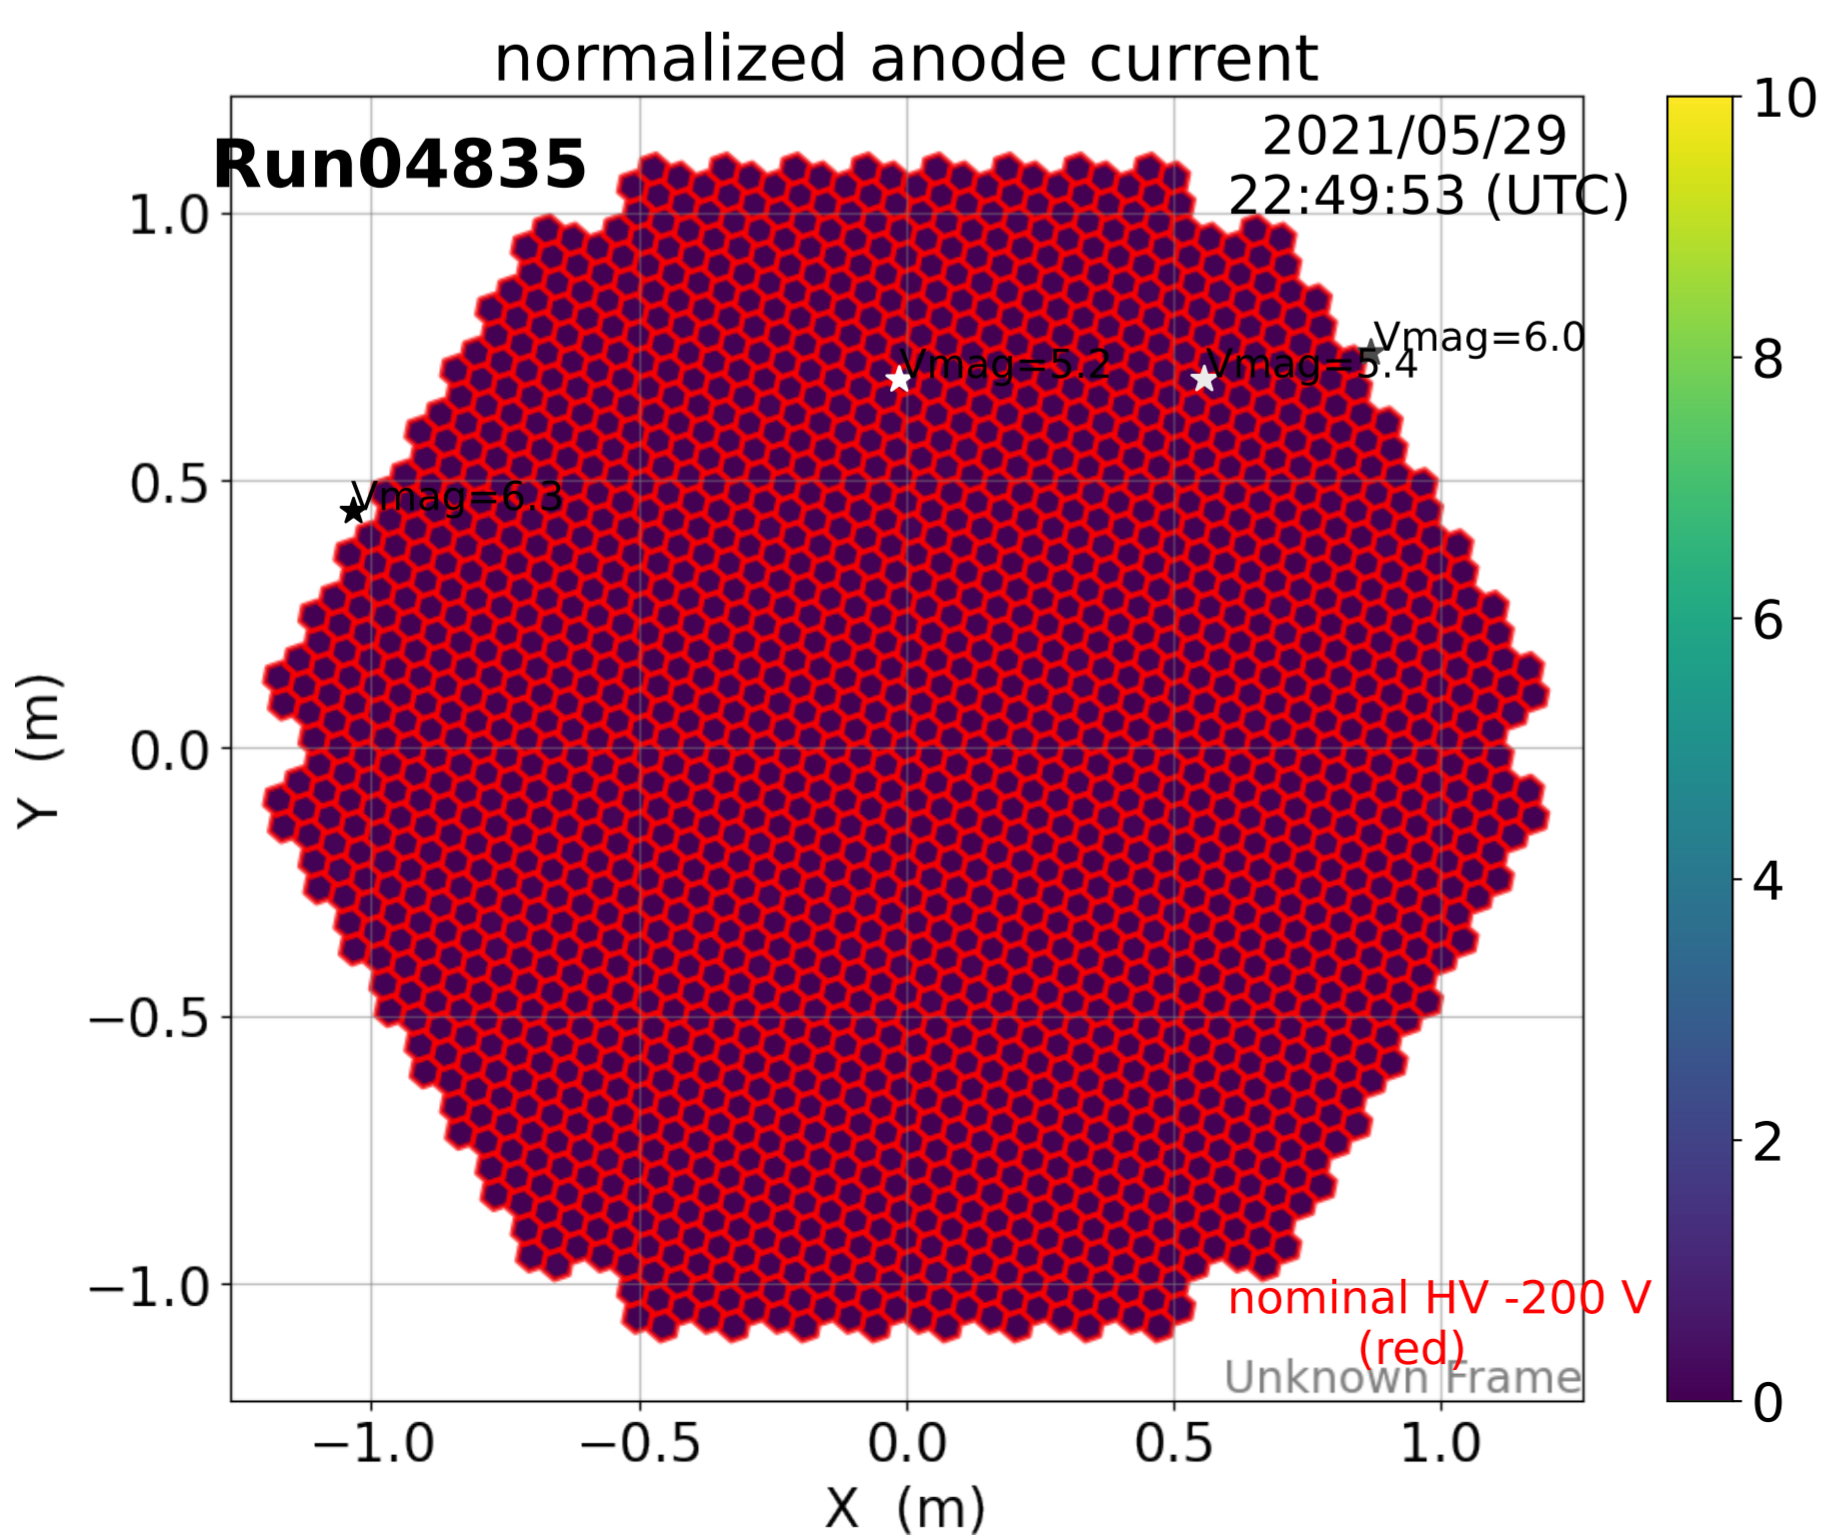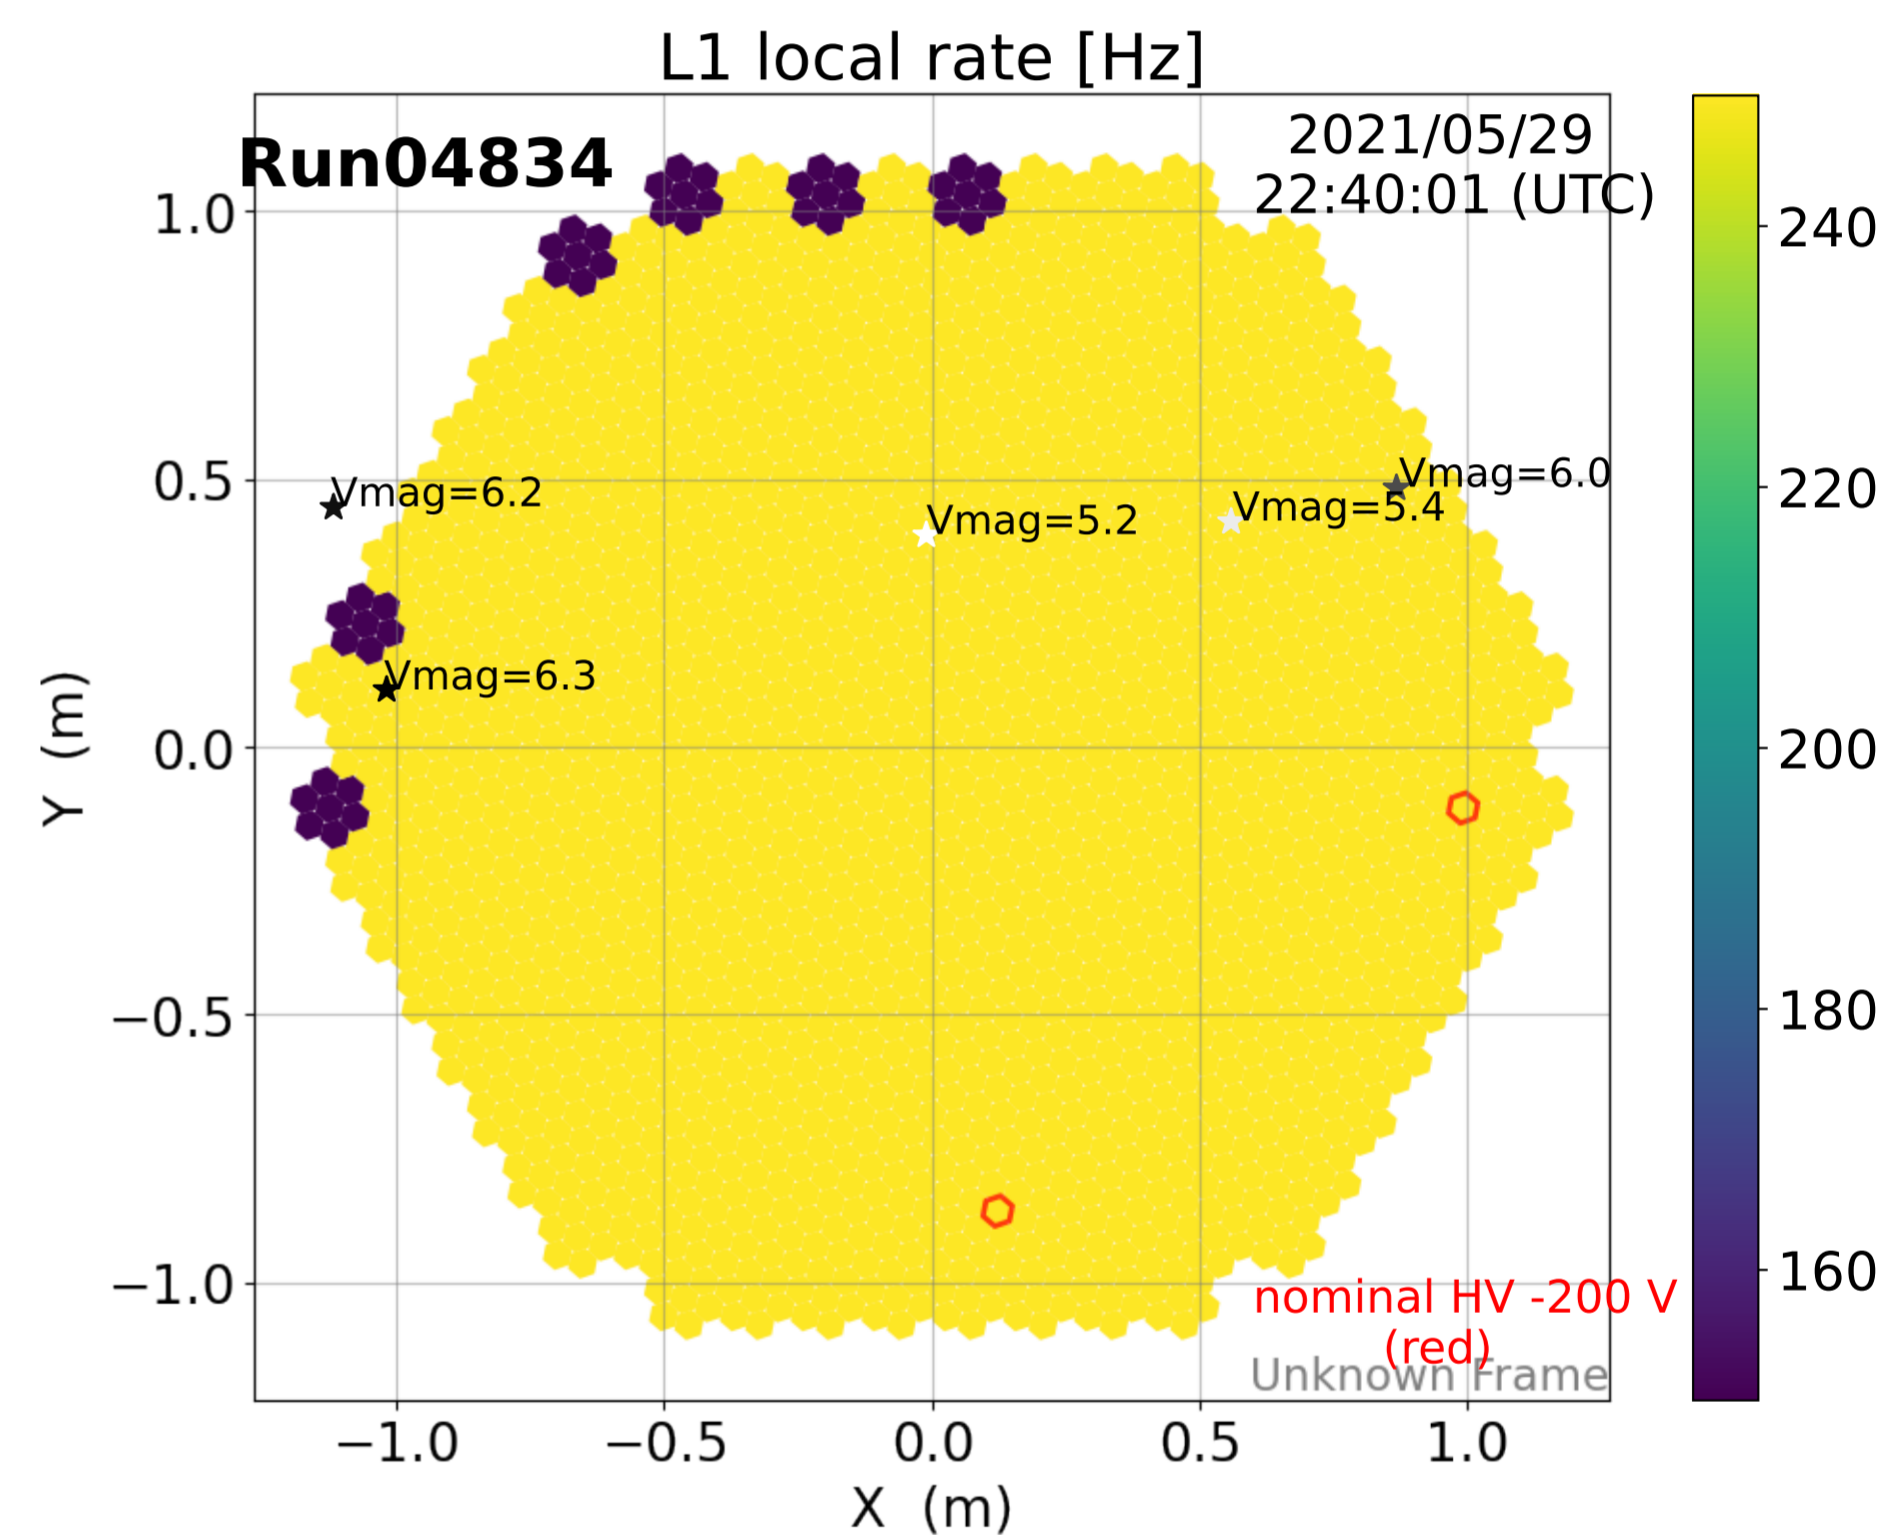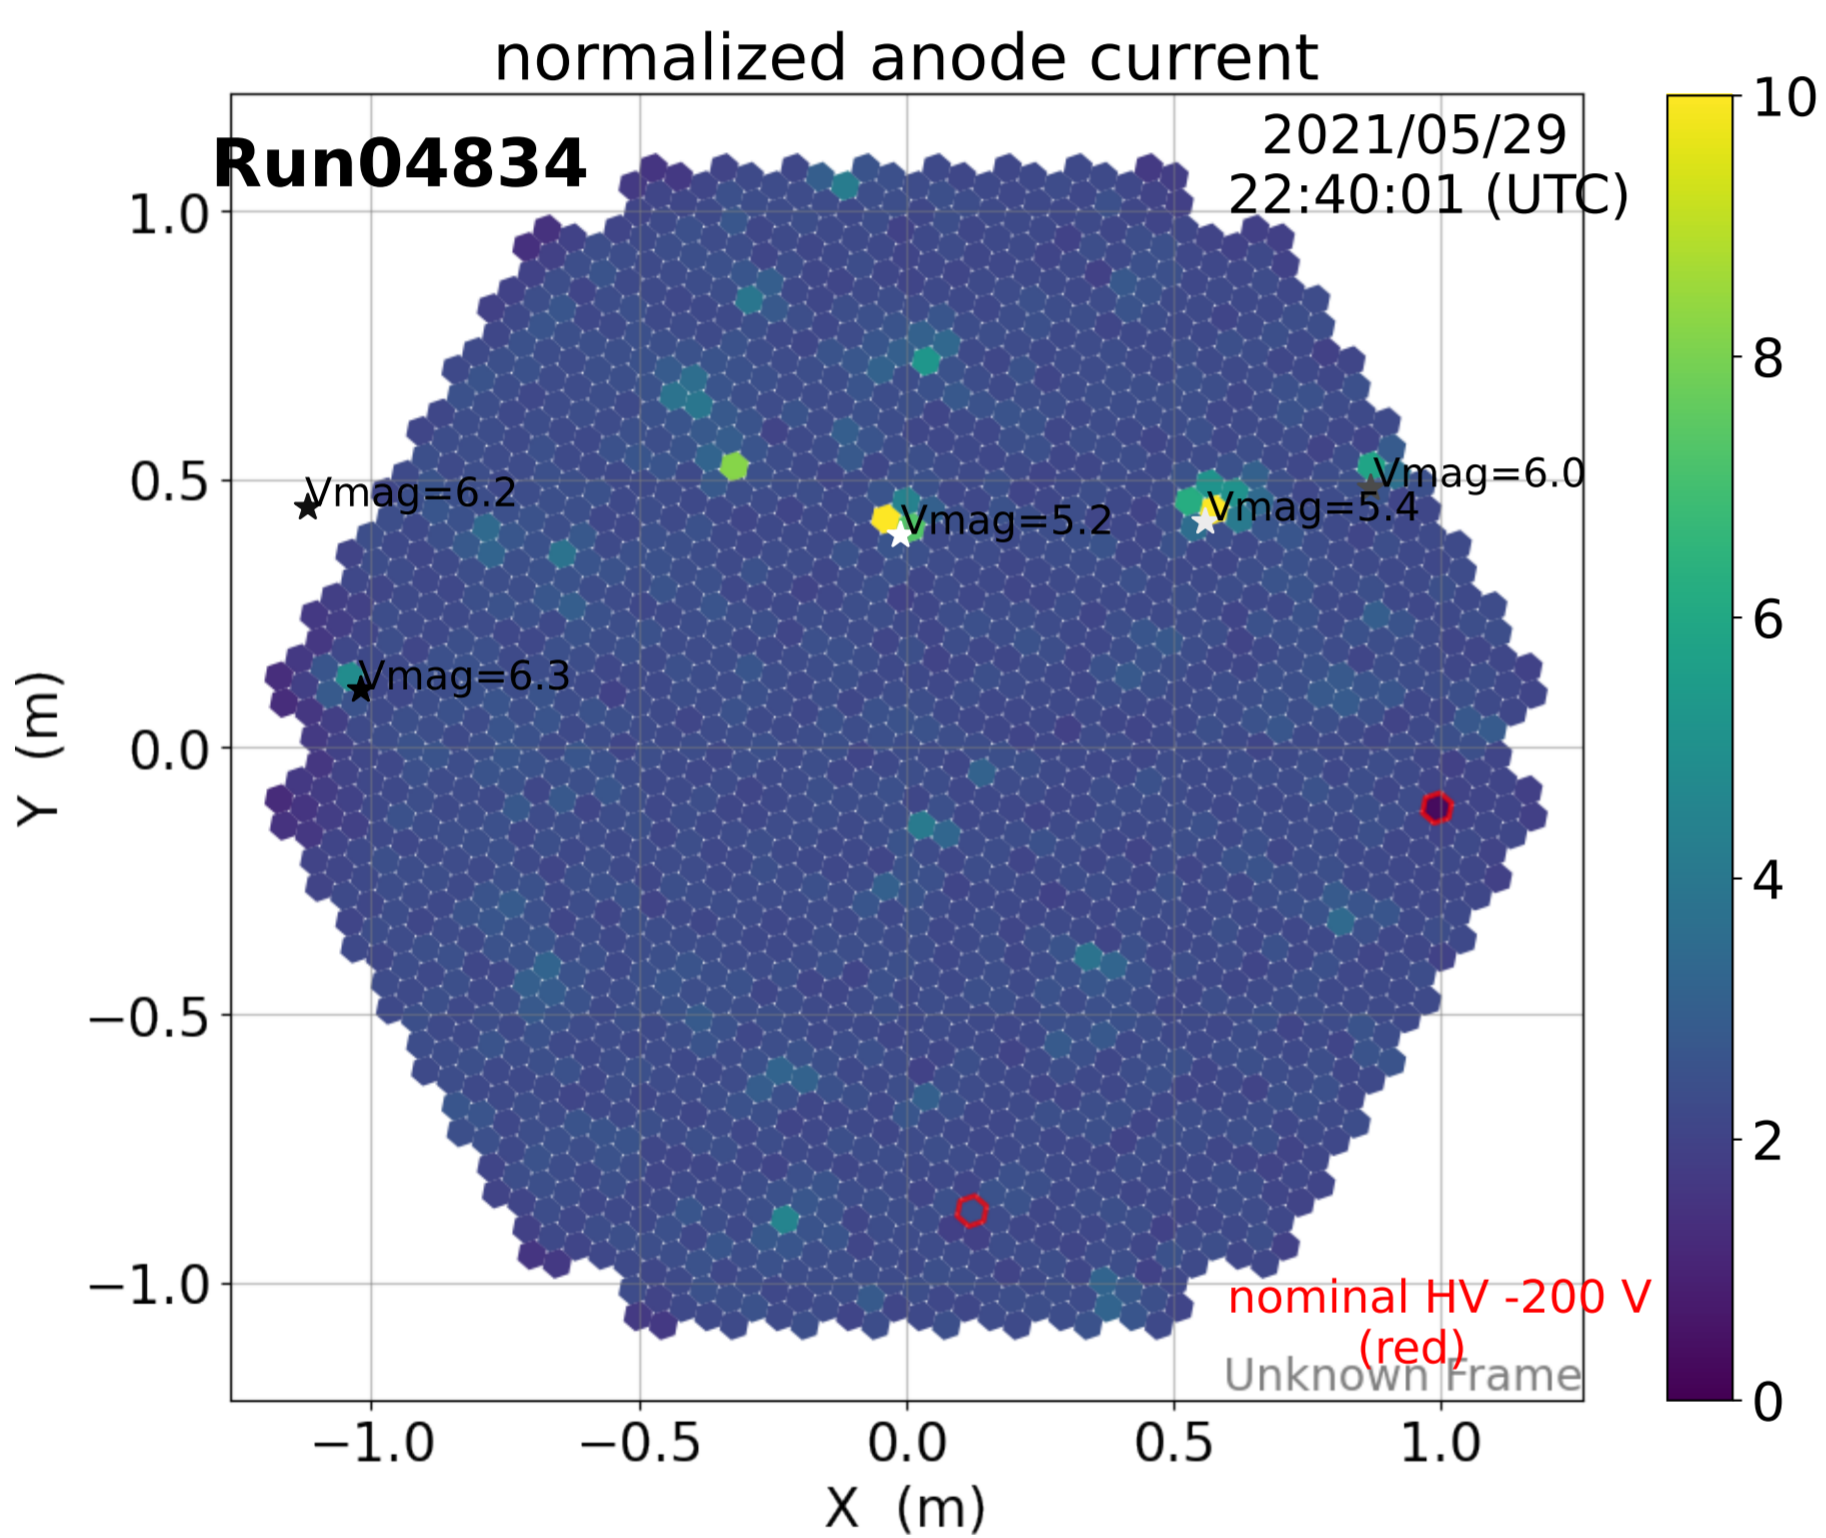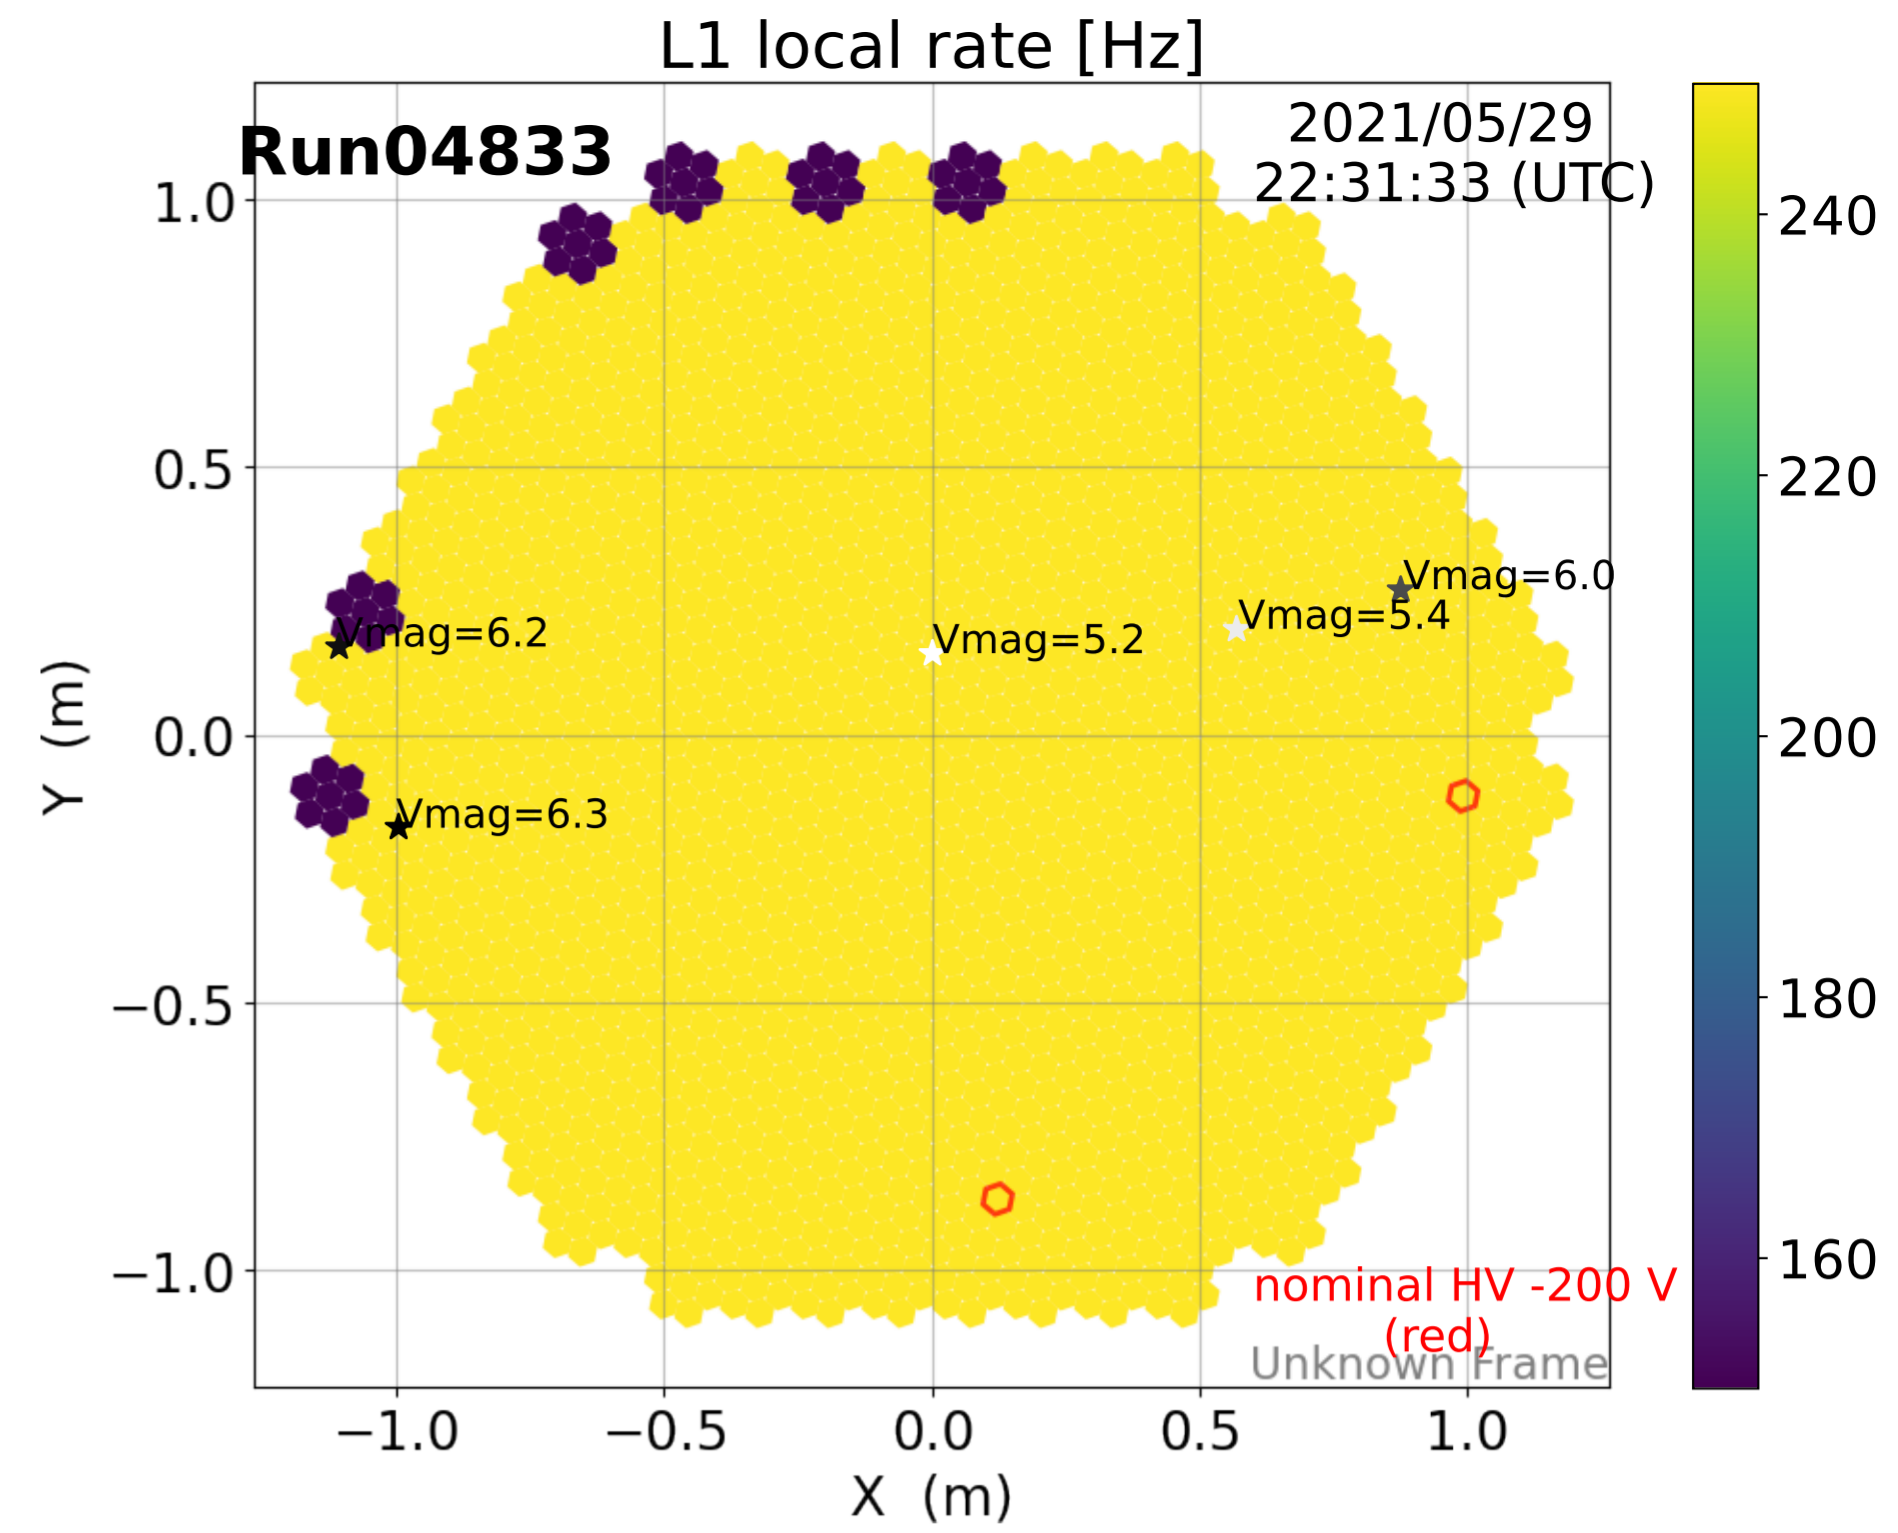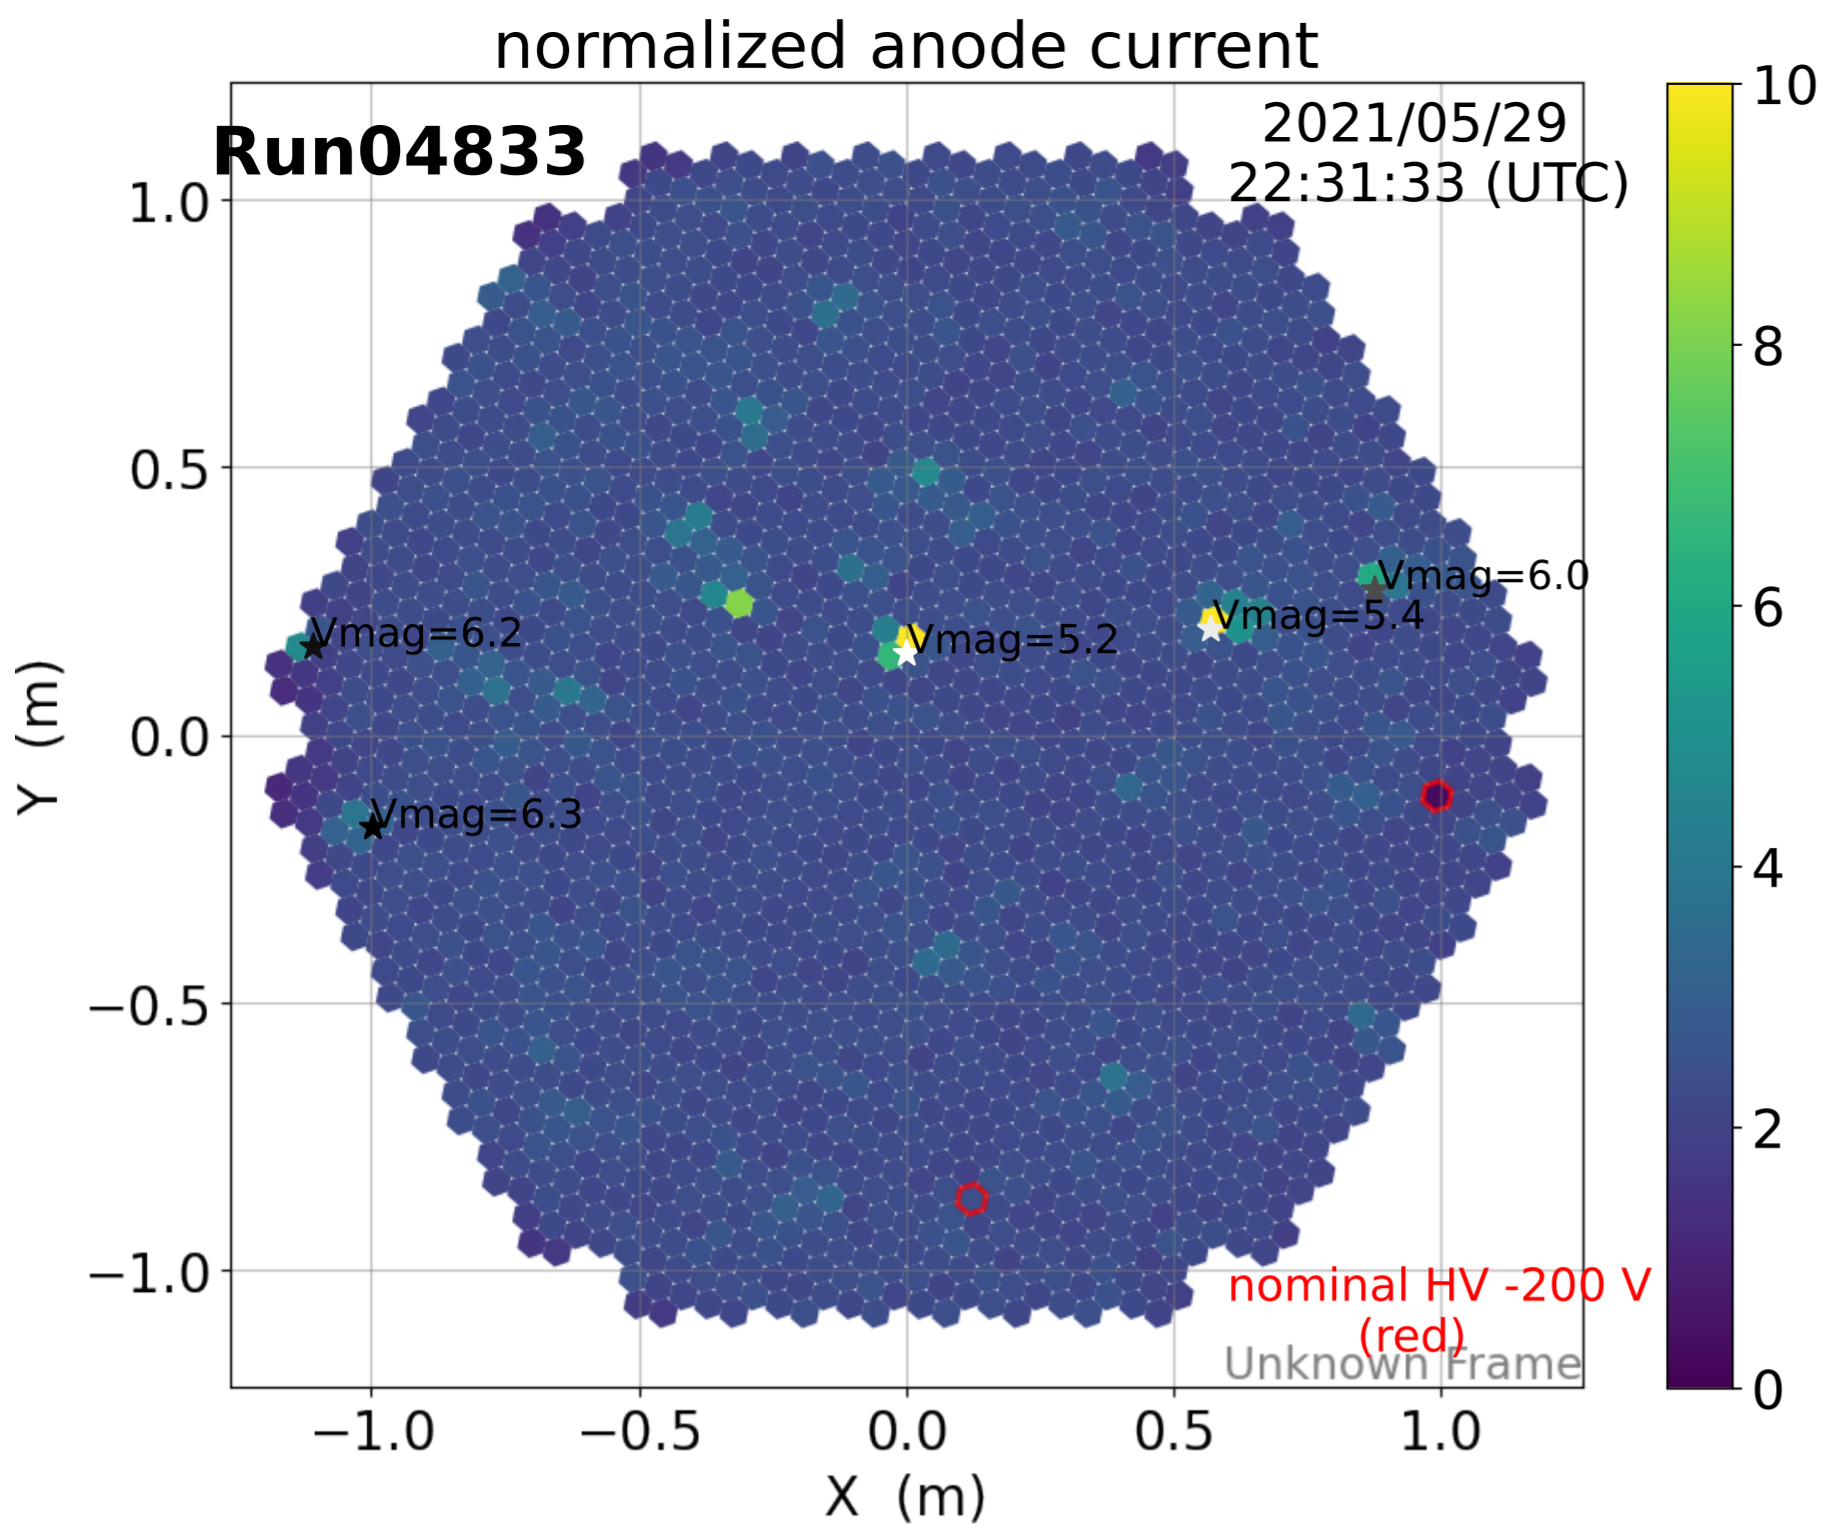


normalized anode current

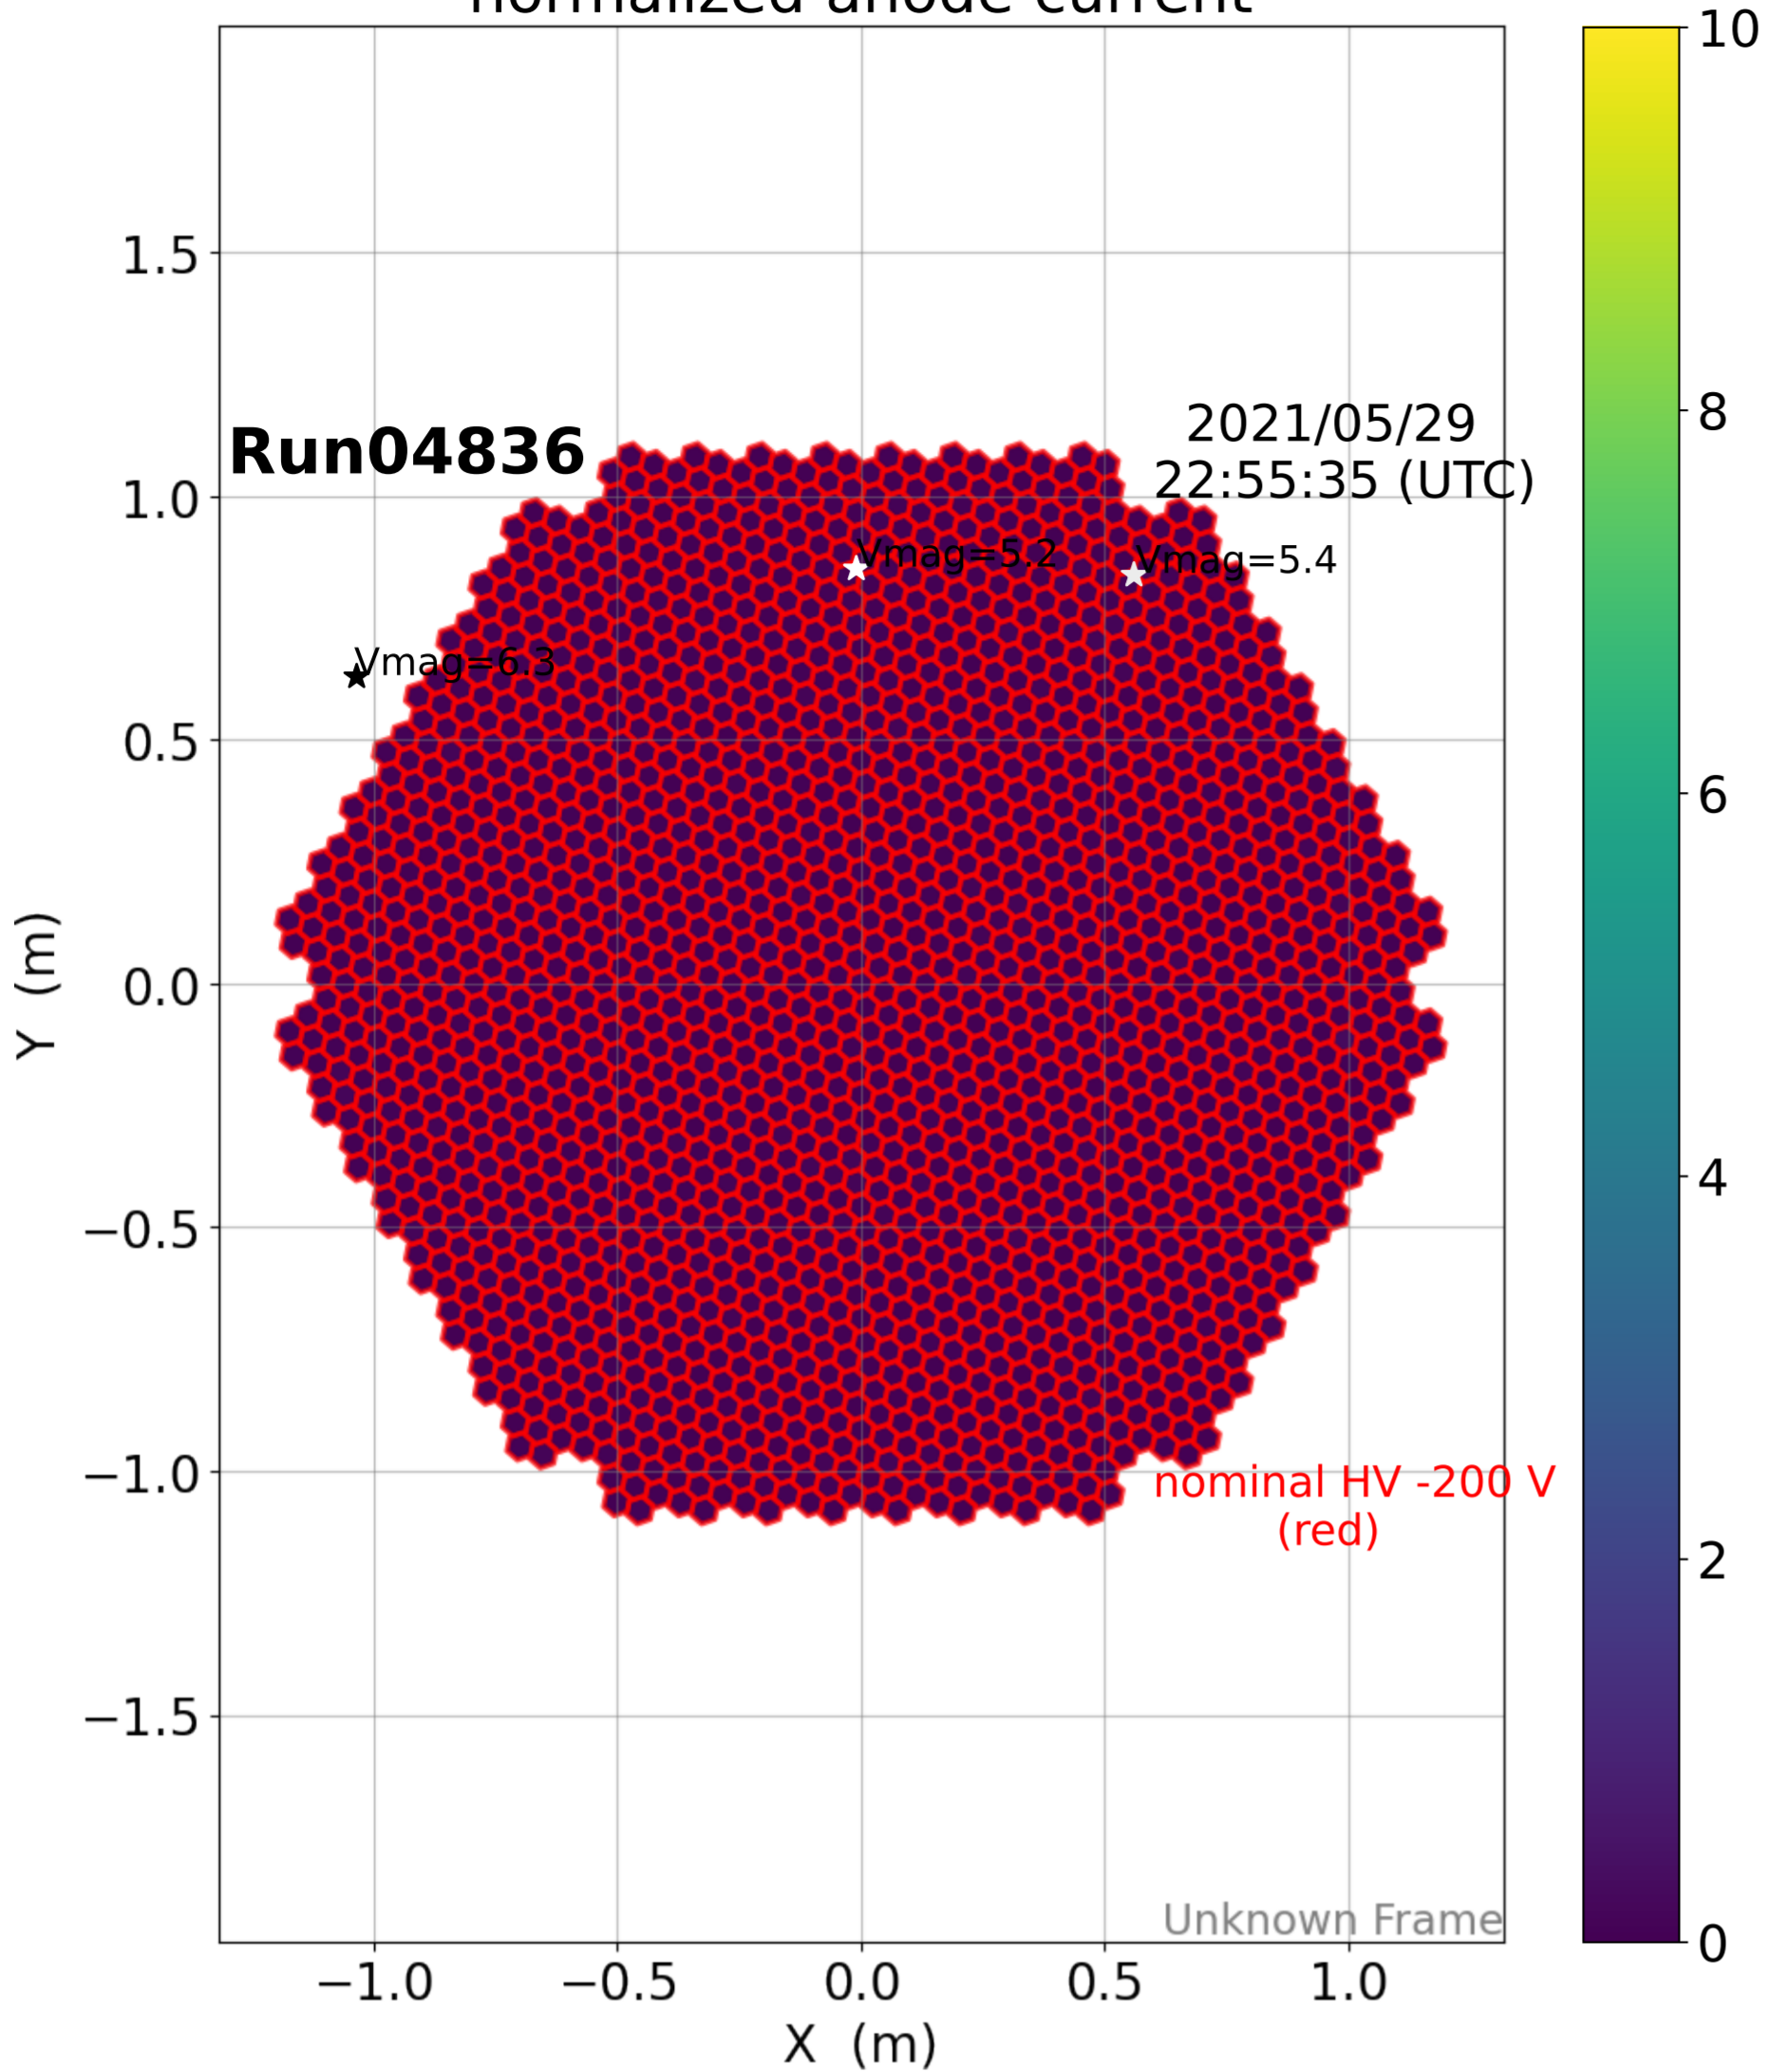

L1 local rate [Hz]

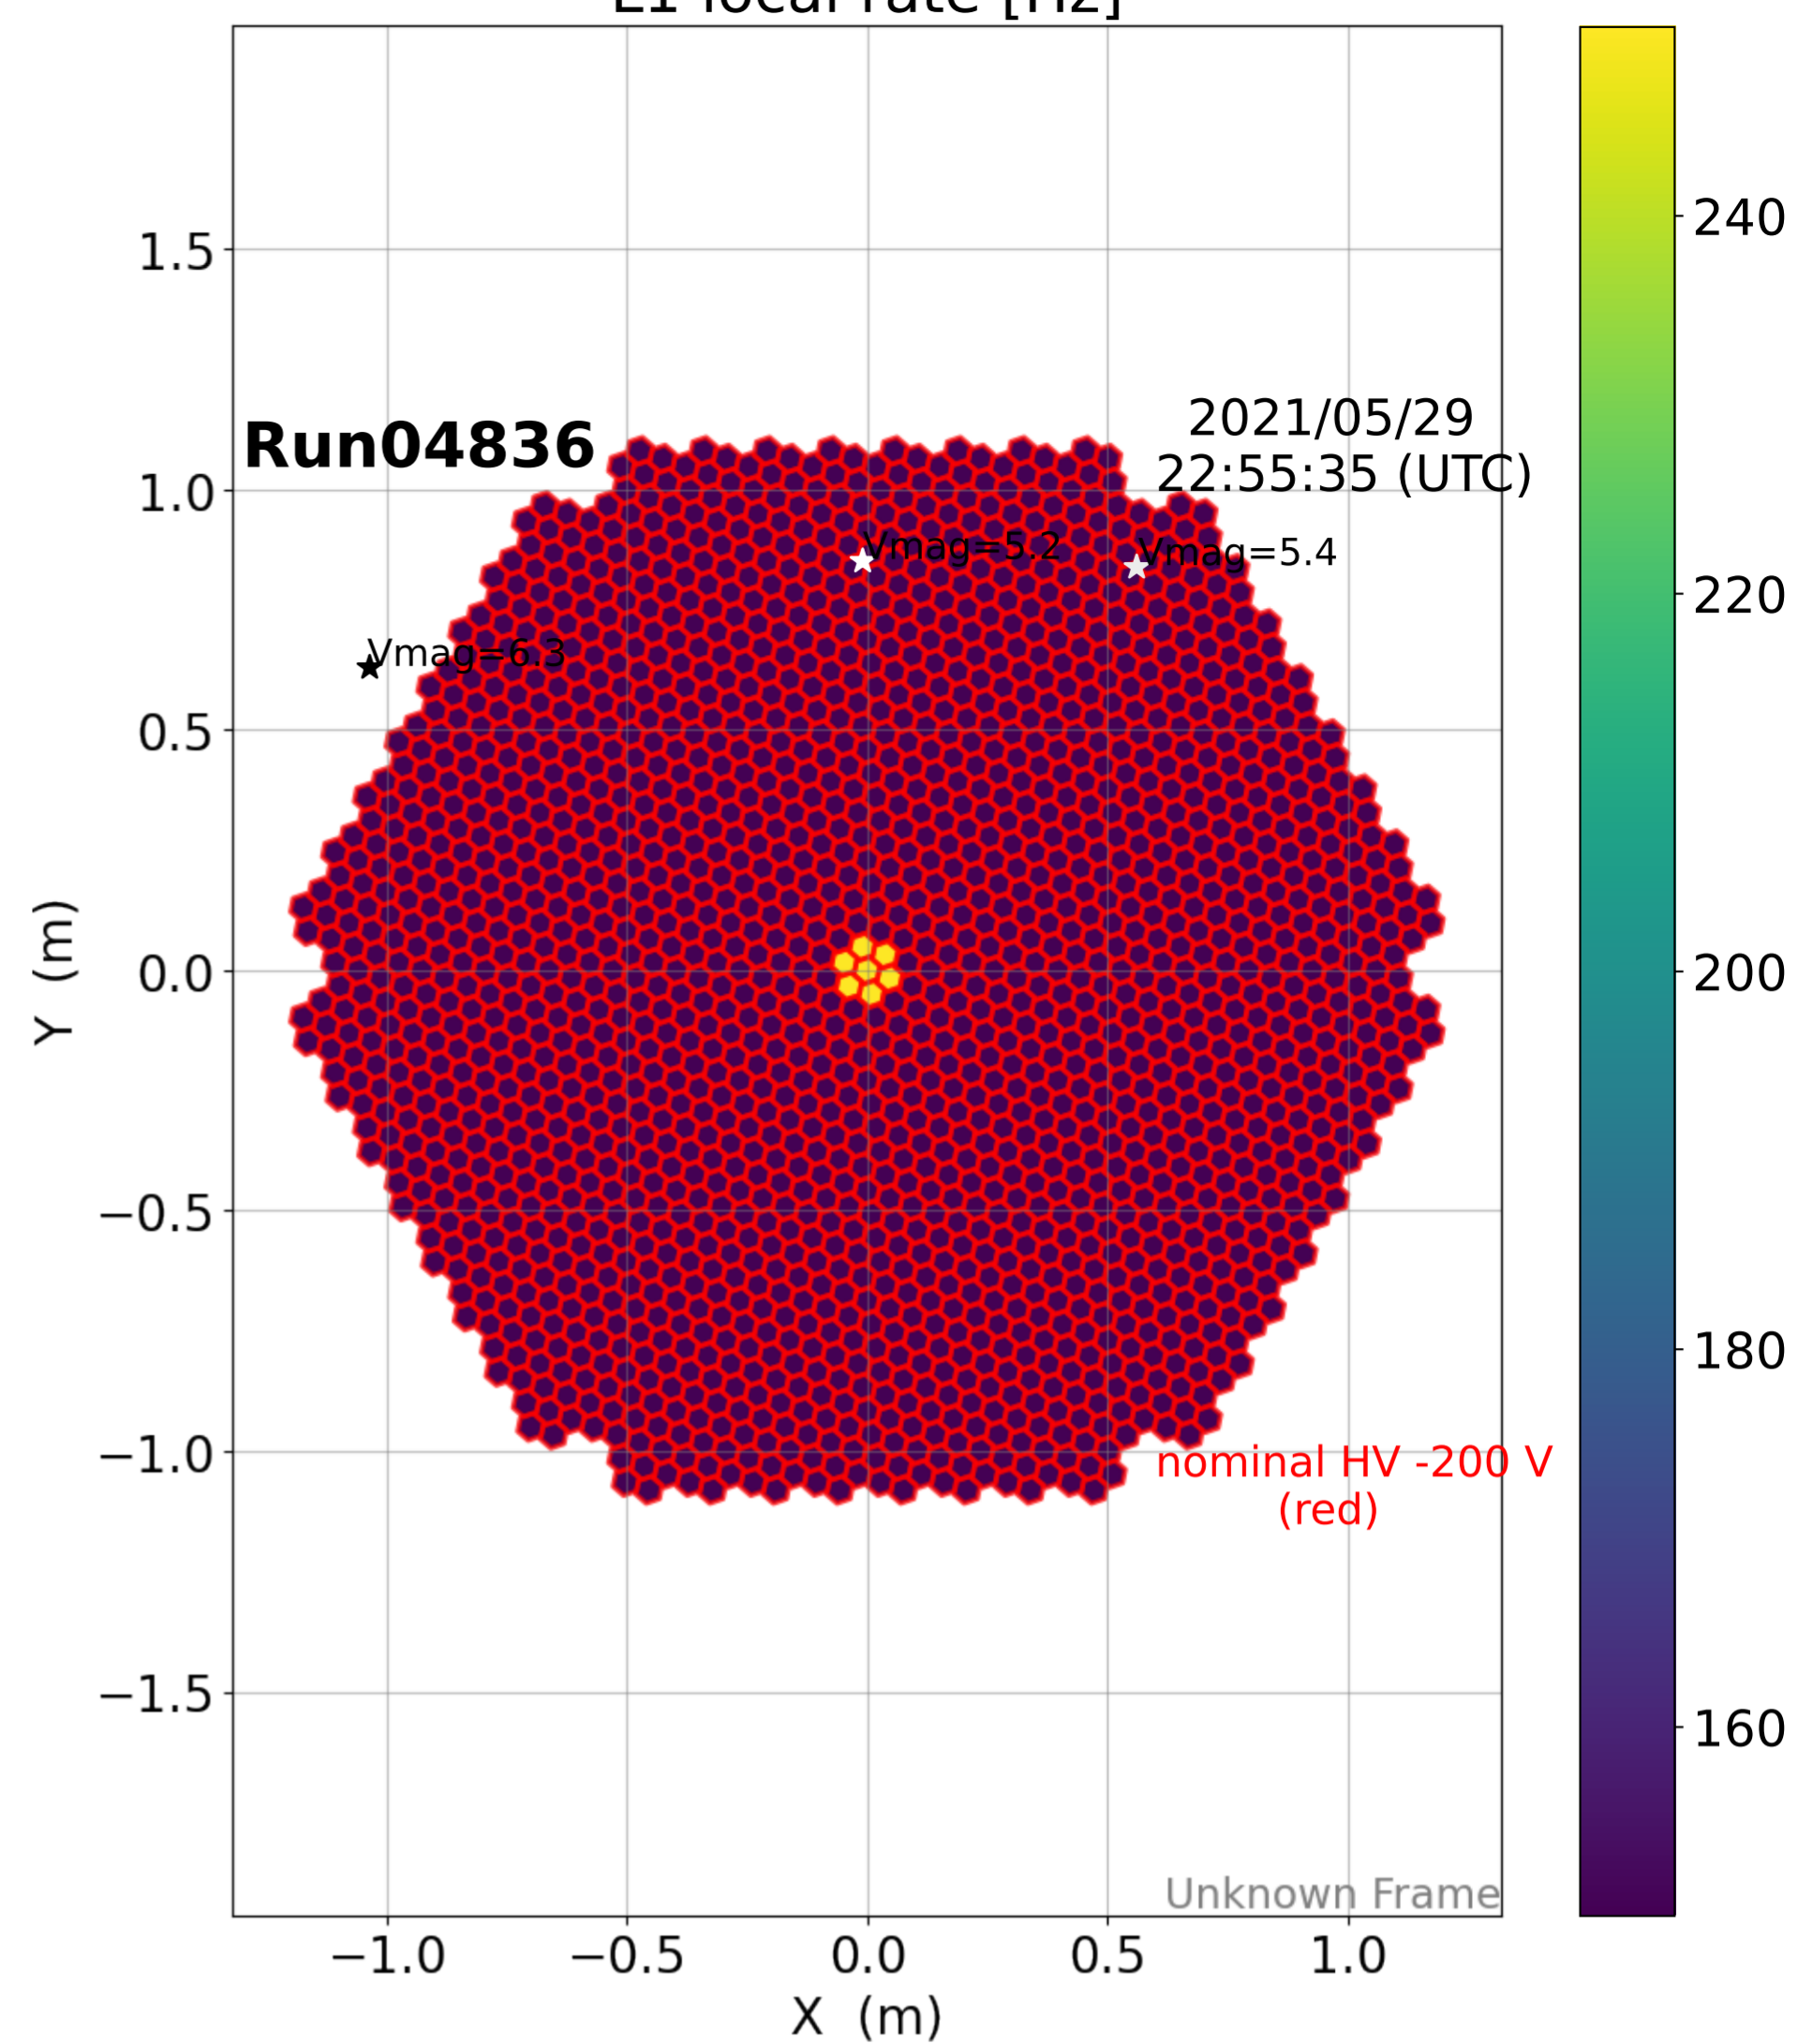

normalized anode current

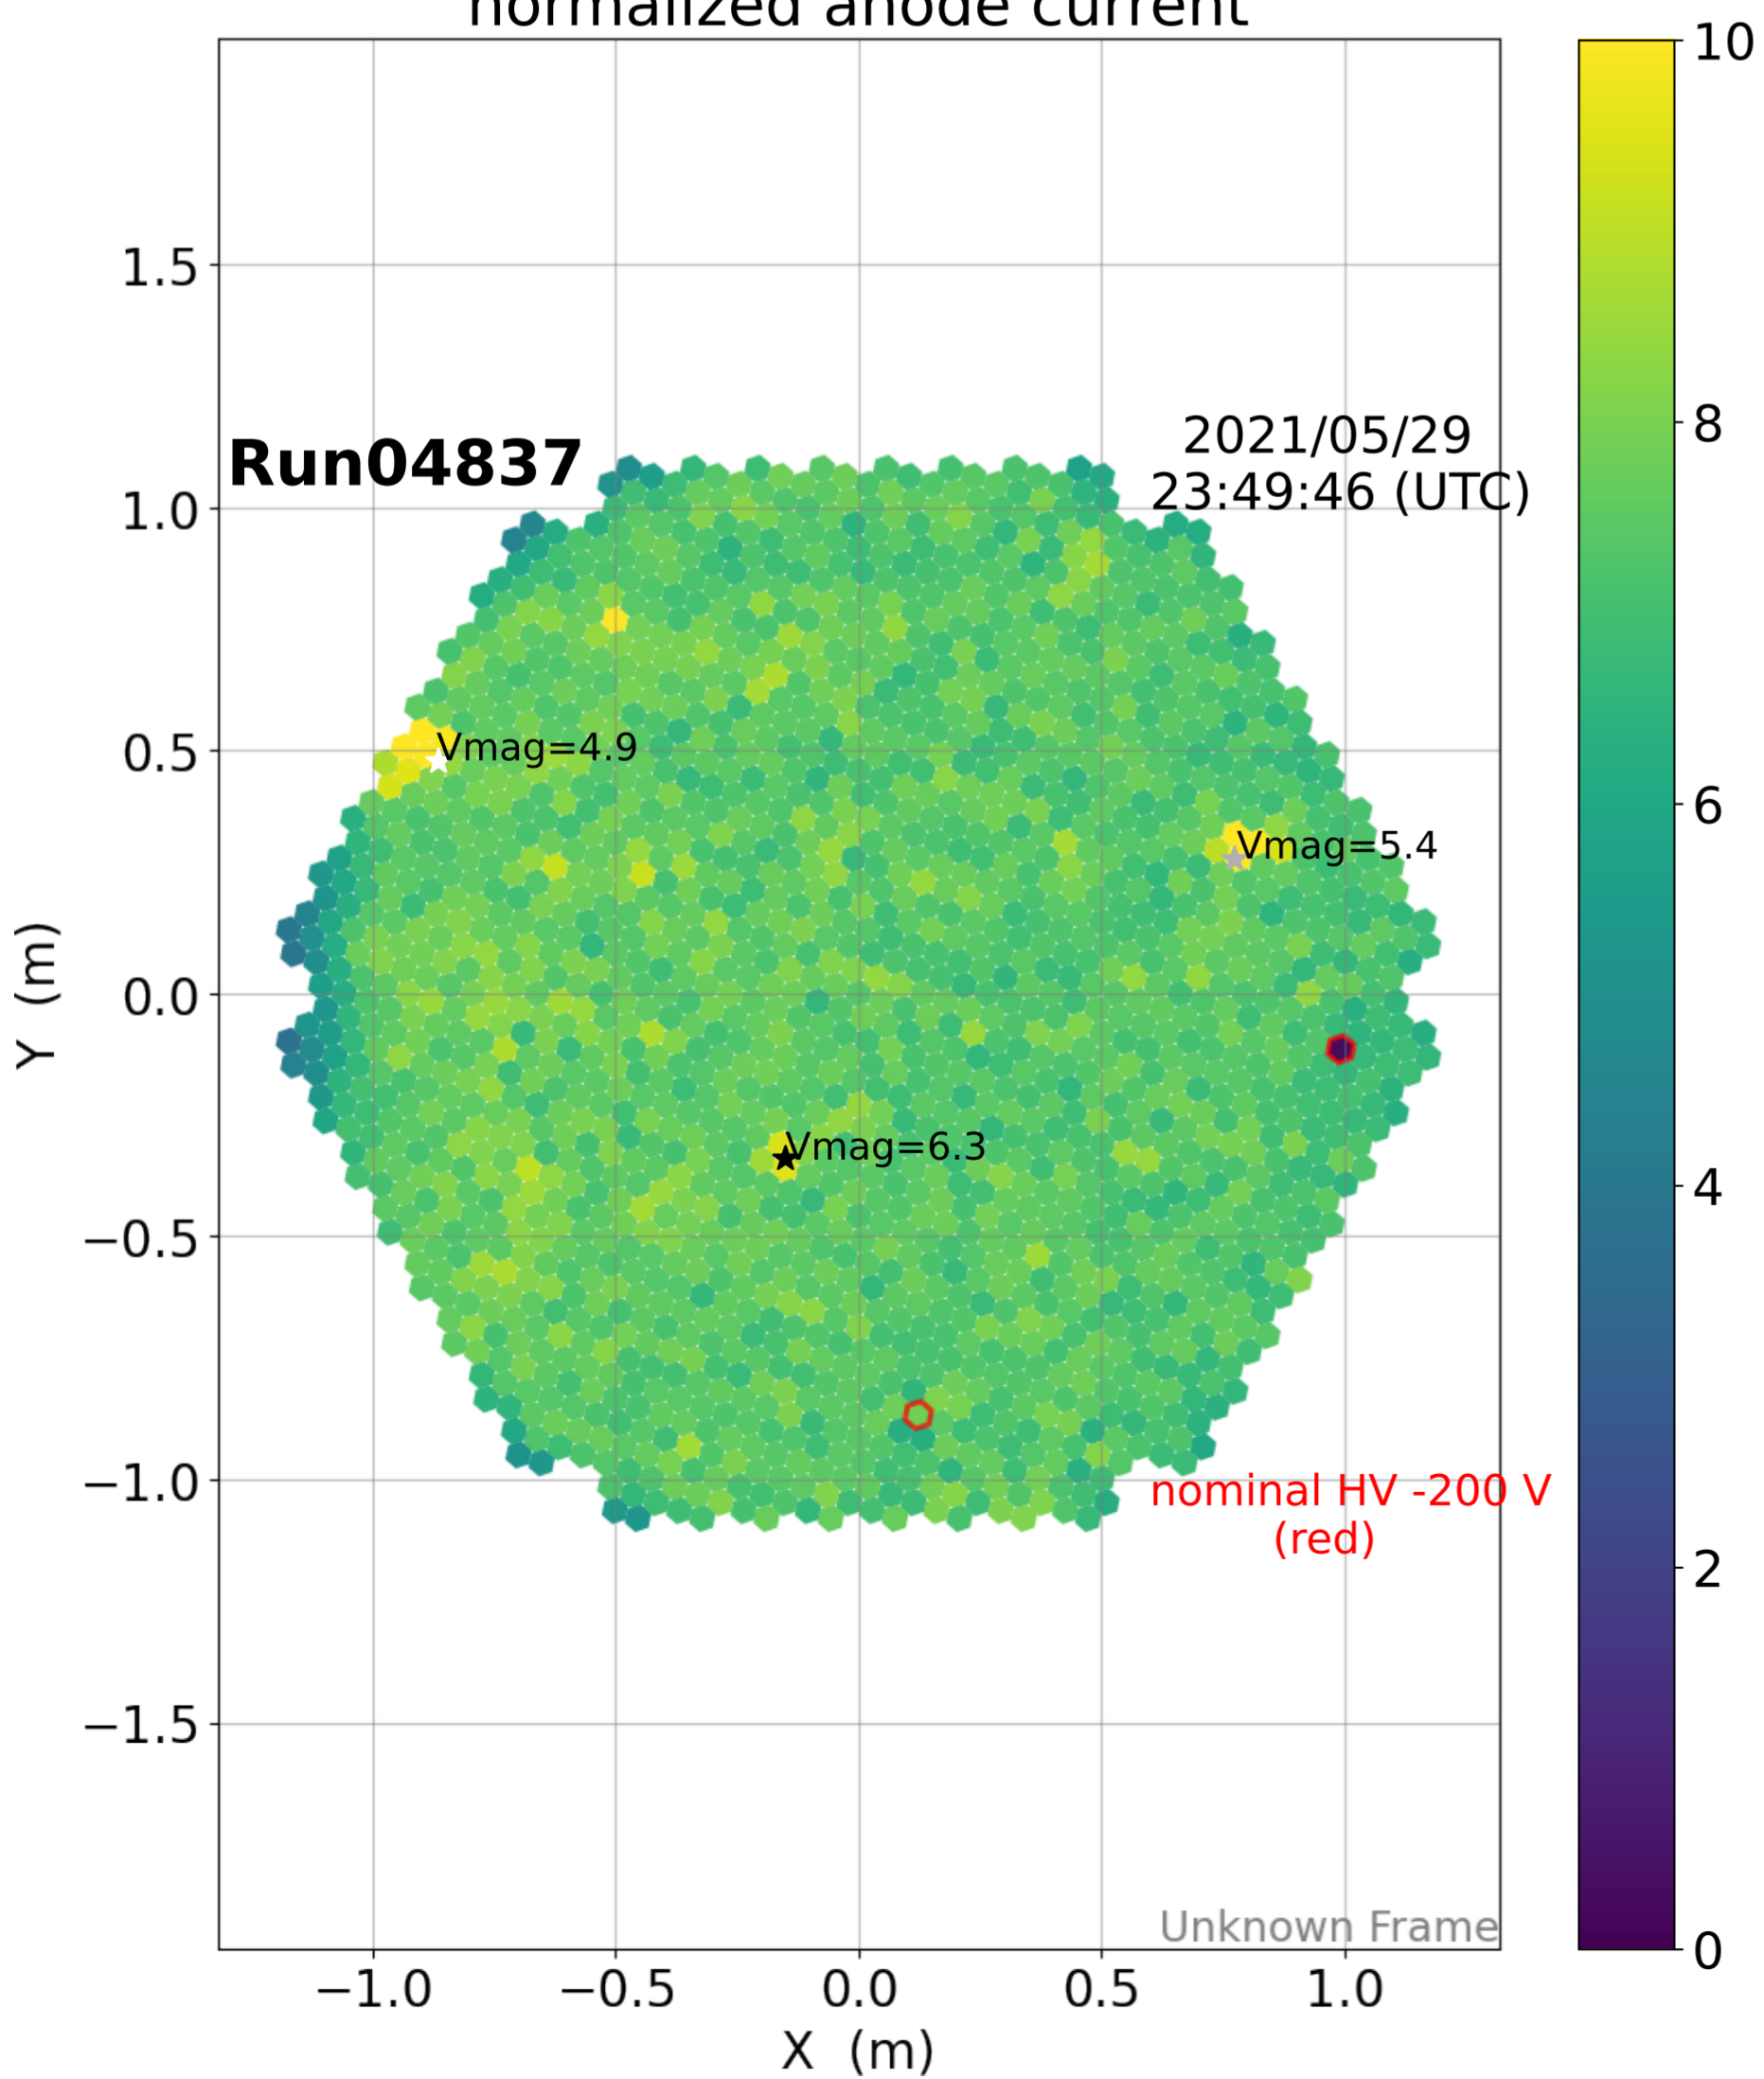

L1 local rate [Hz]

