




2021-7-17

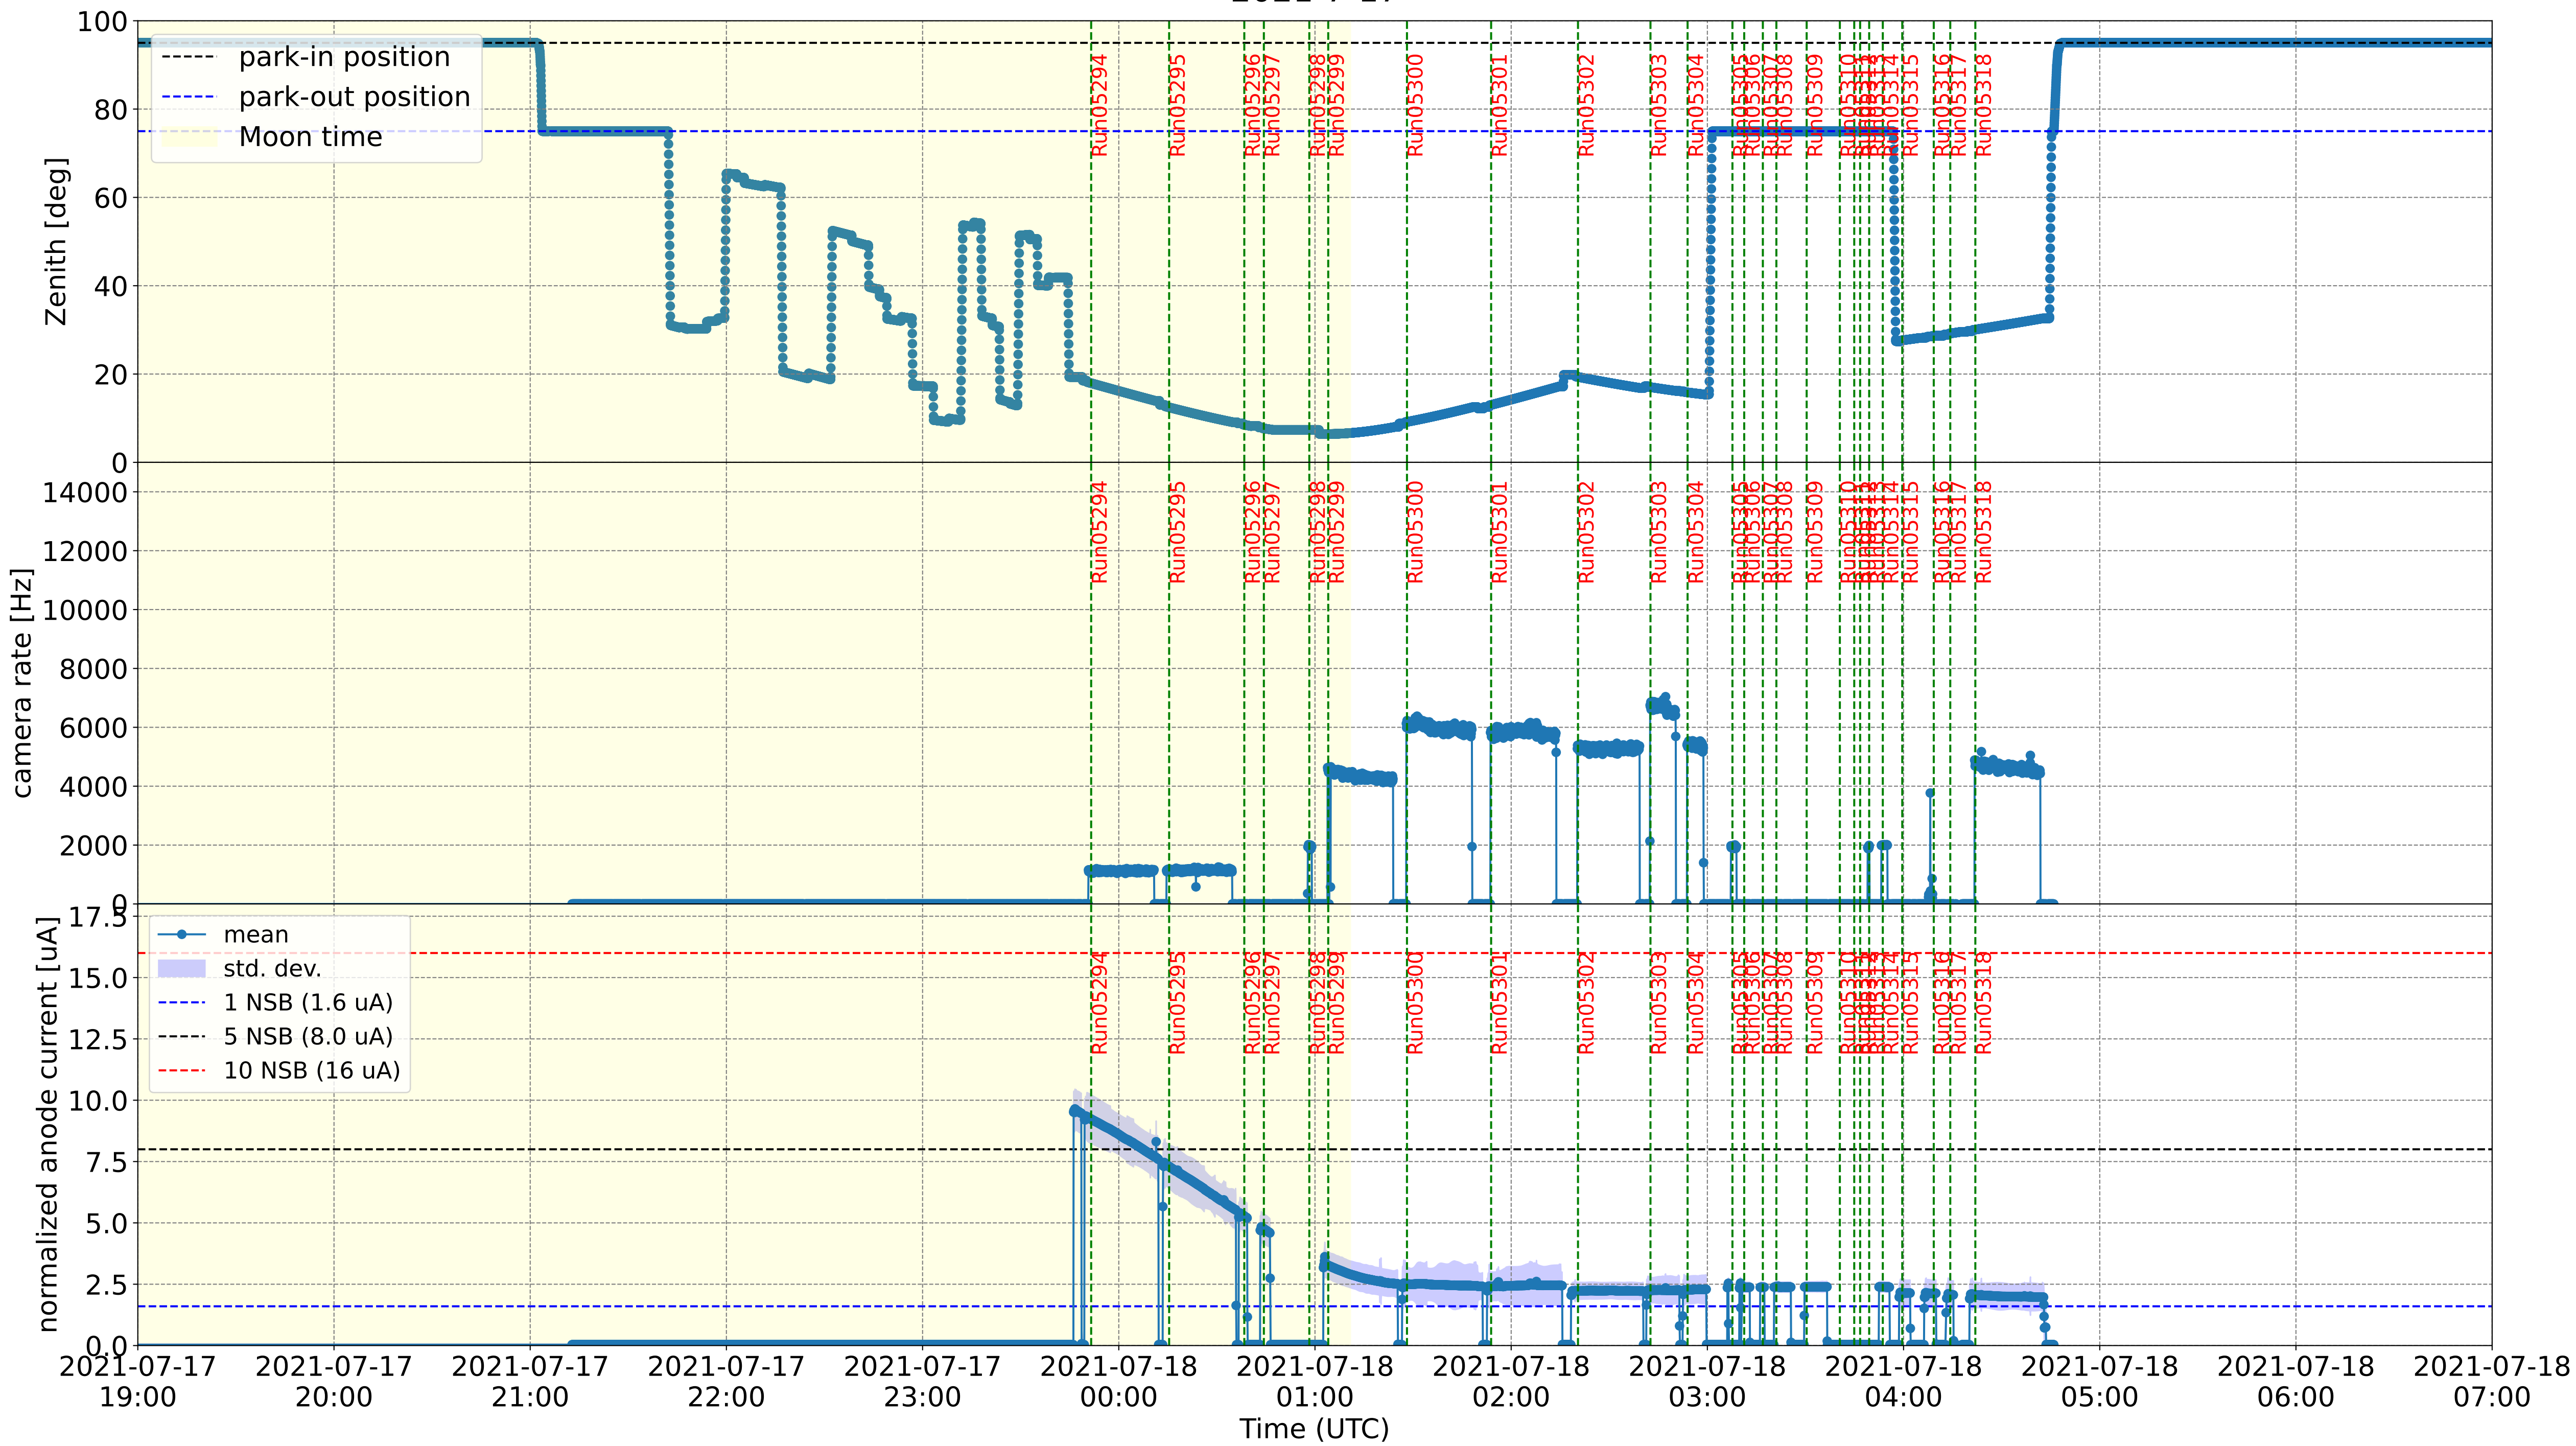

2021-7-17

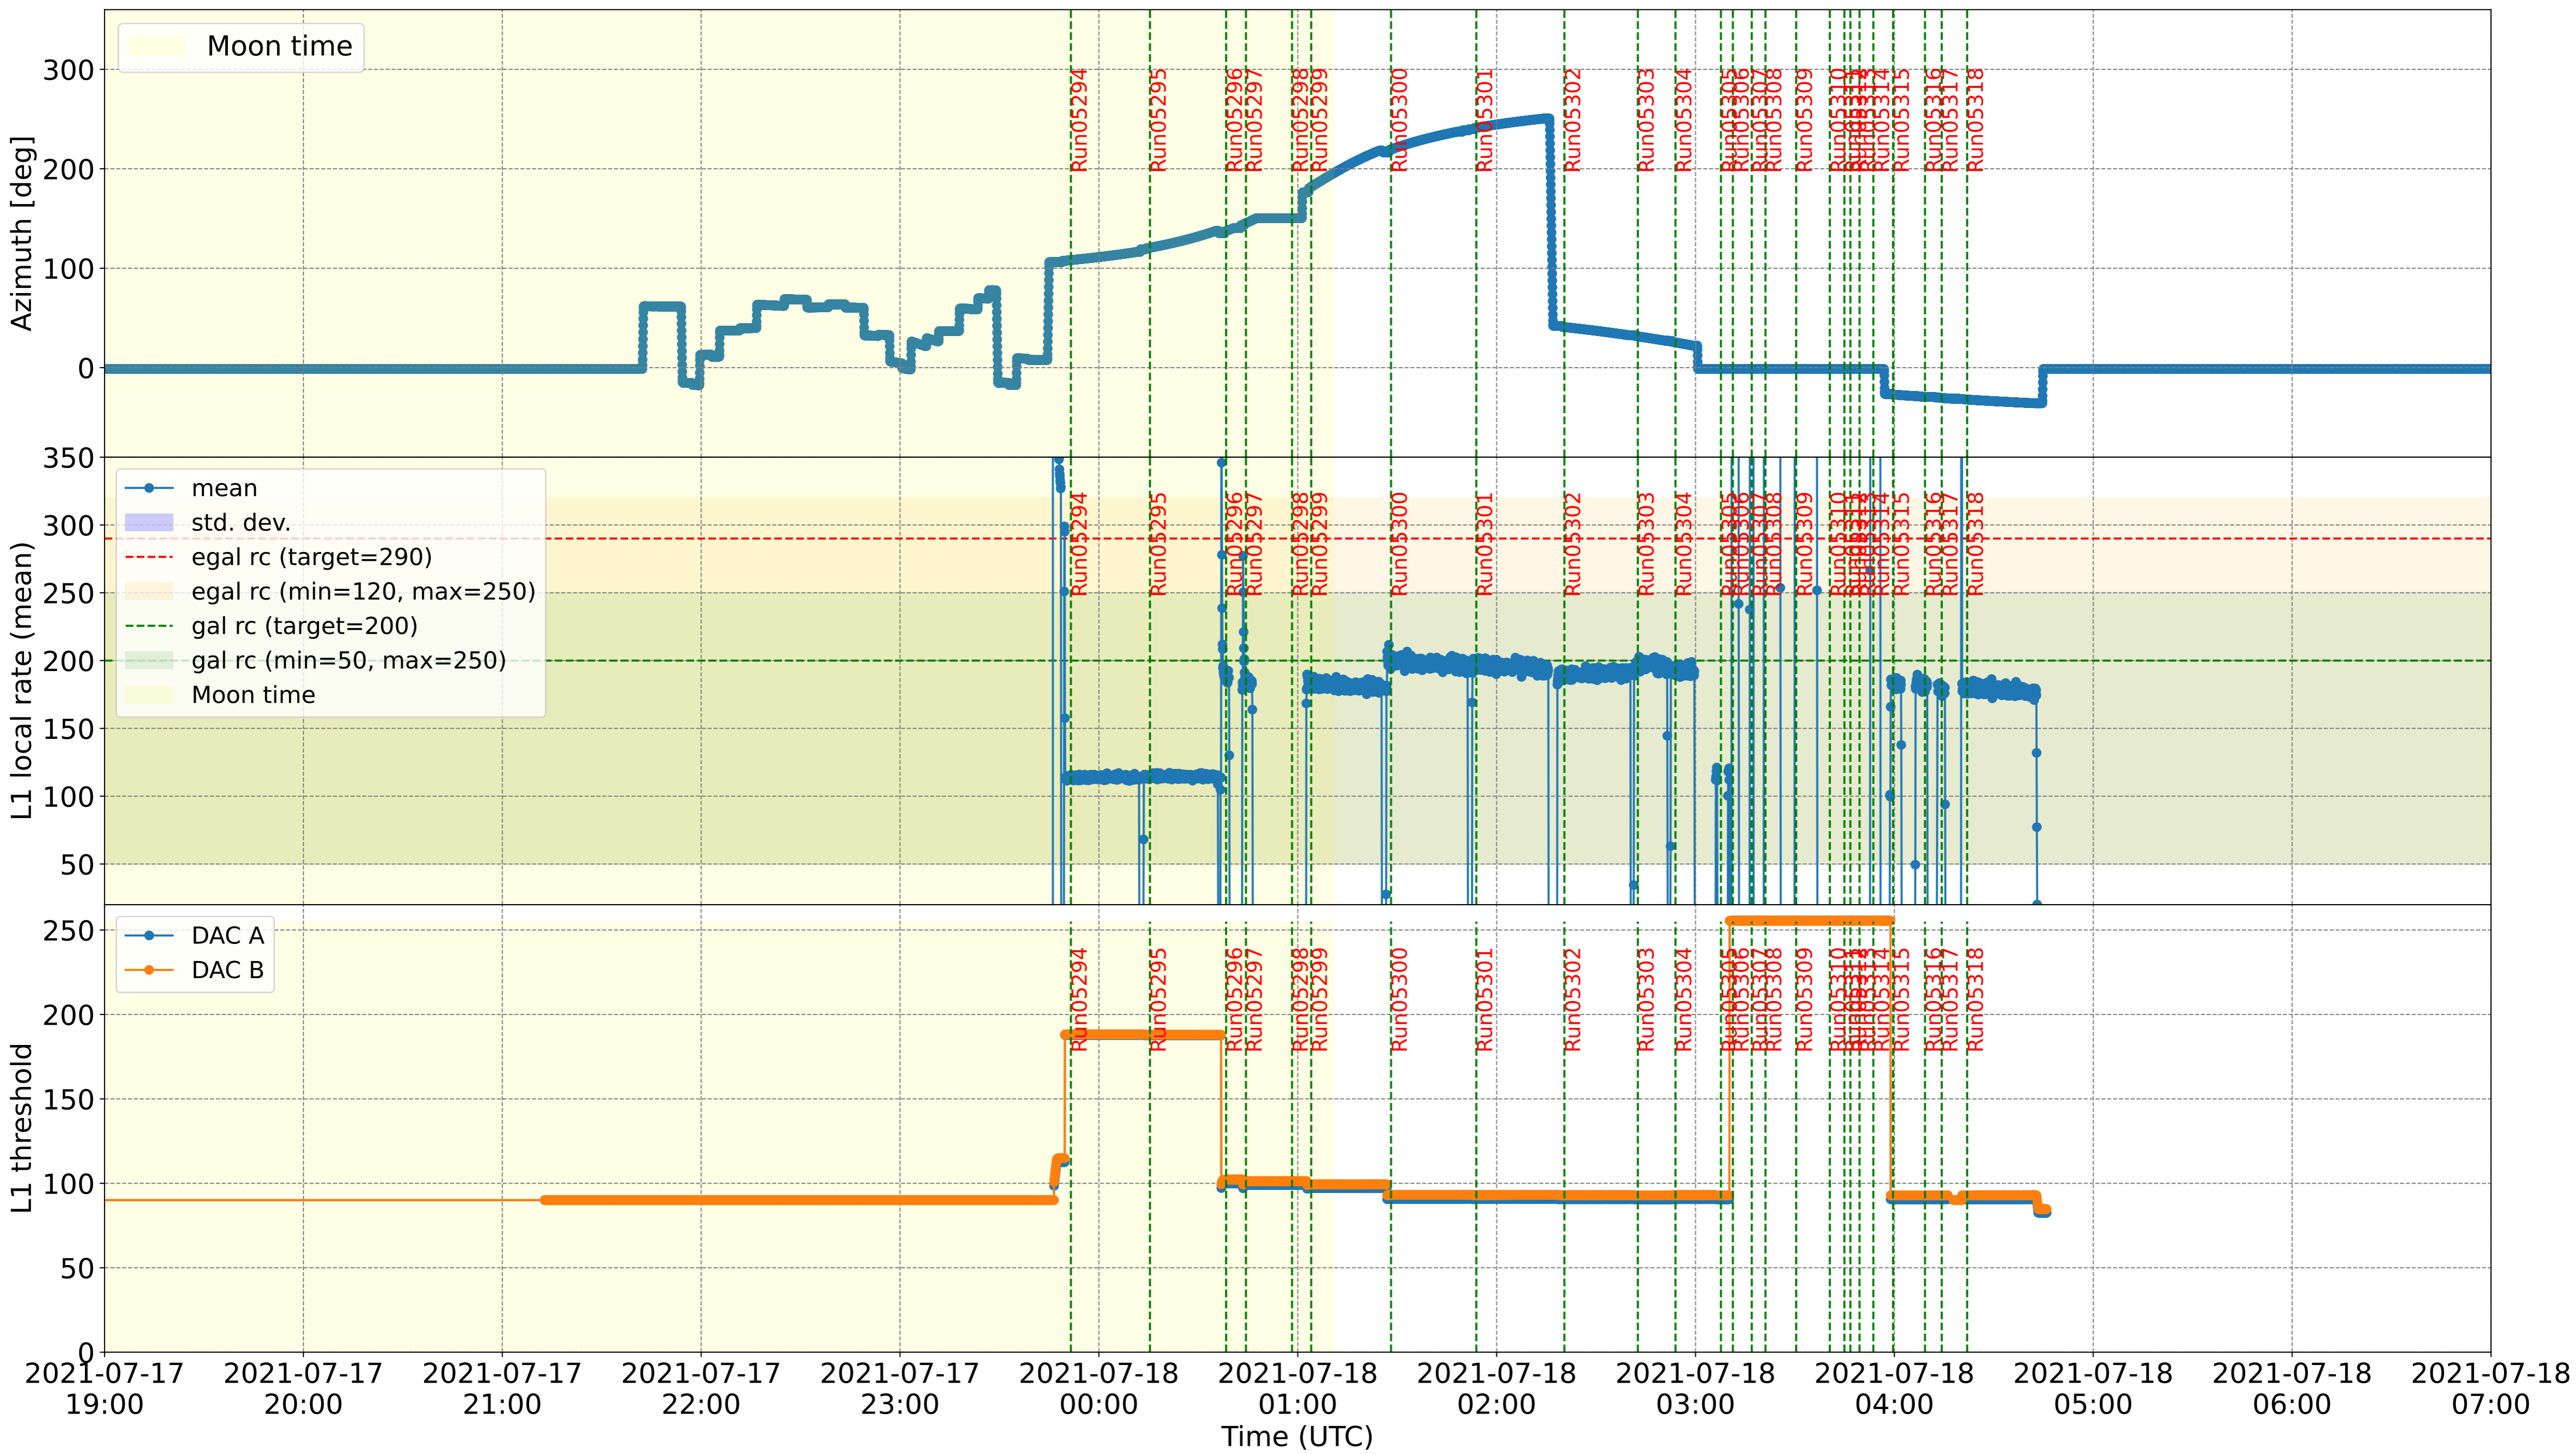


2021-7-17






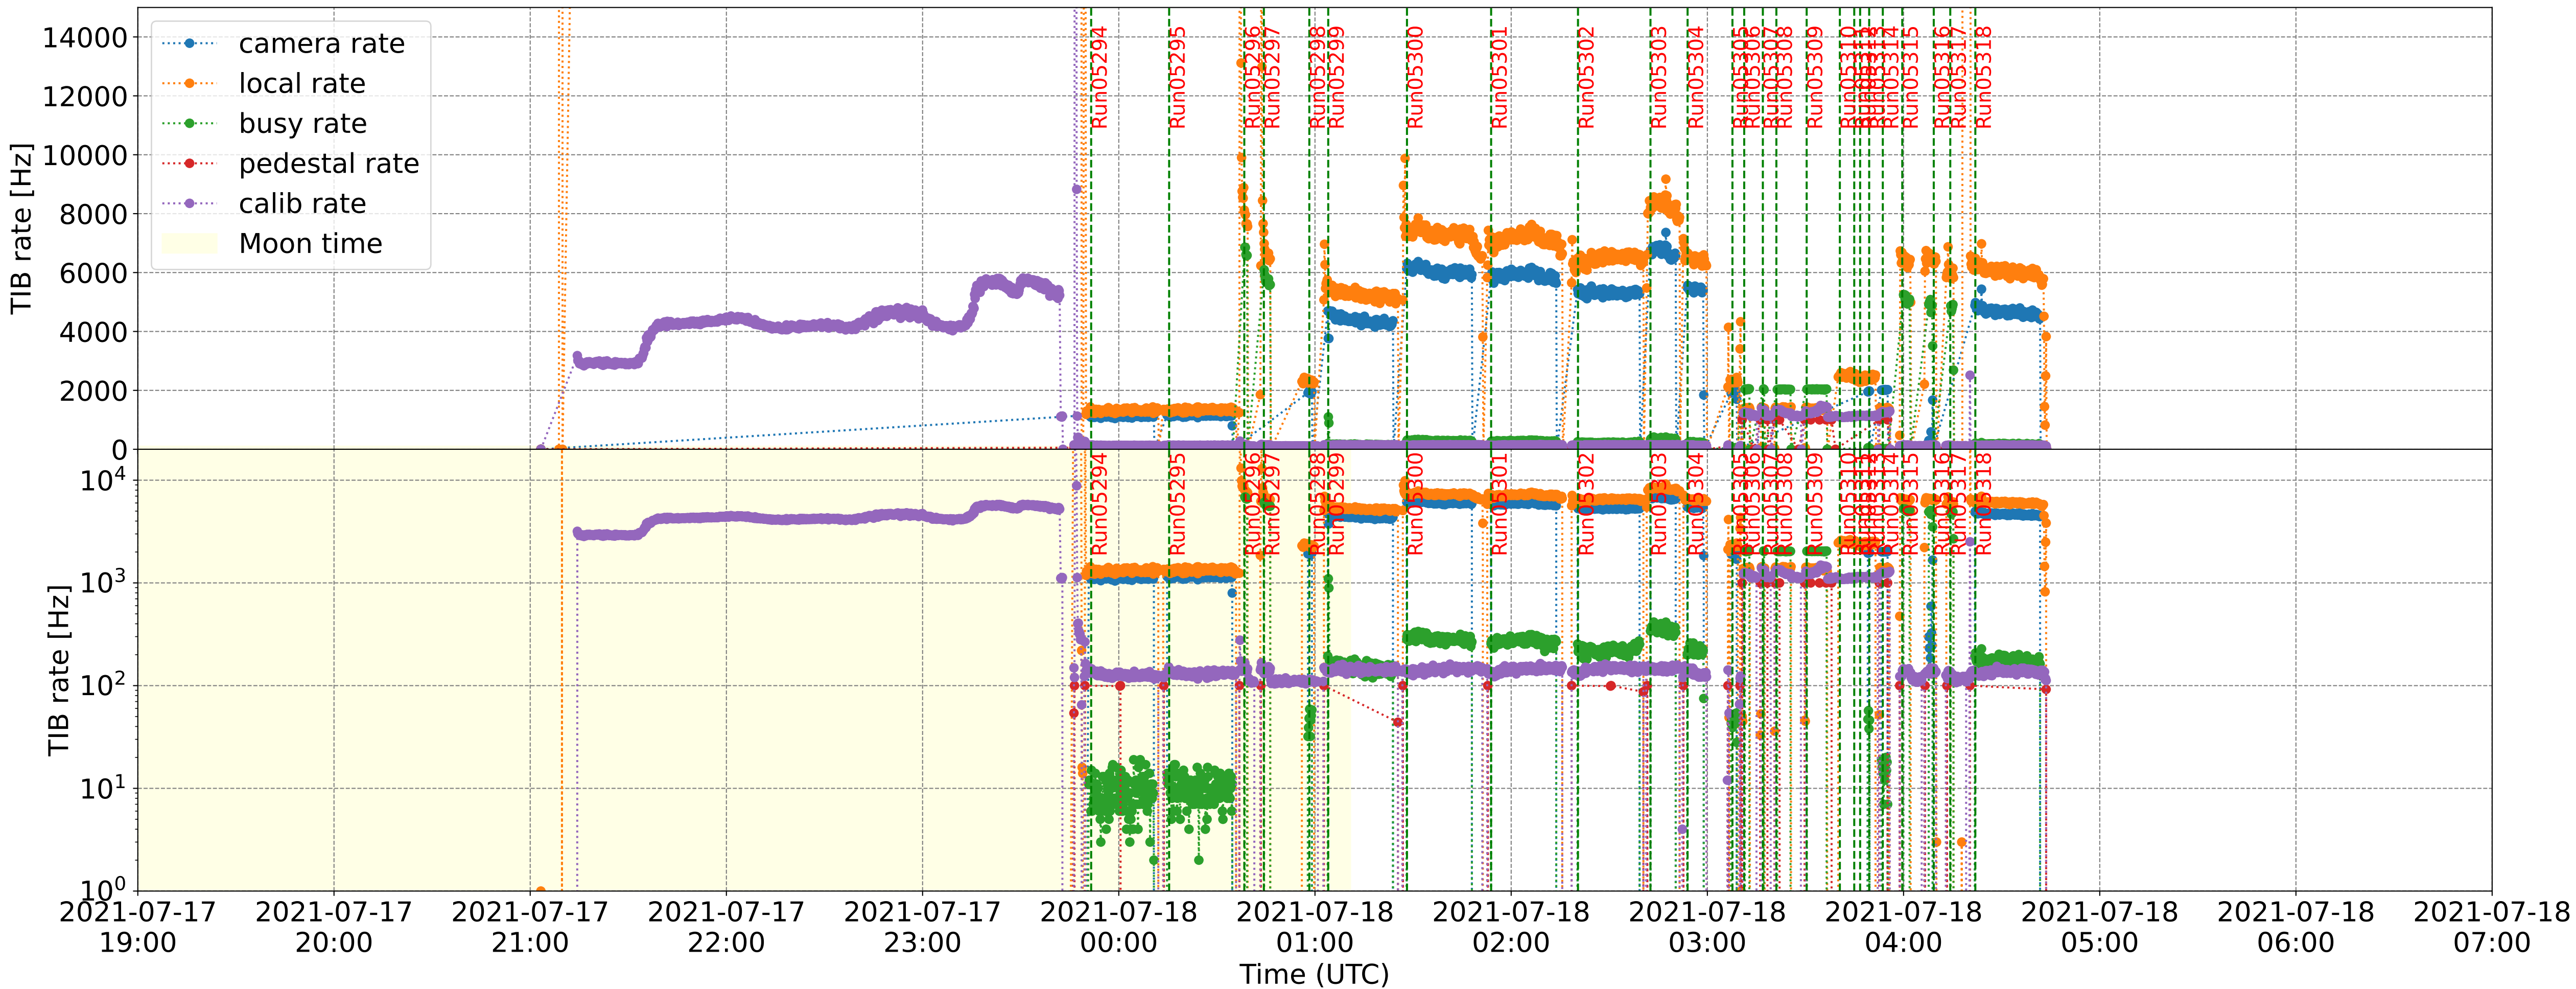










# Calibration Box (2021-7-17)

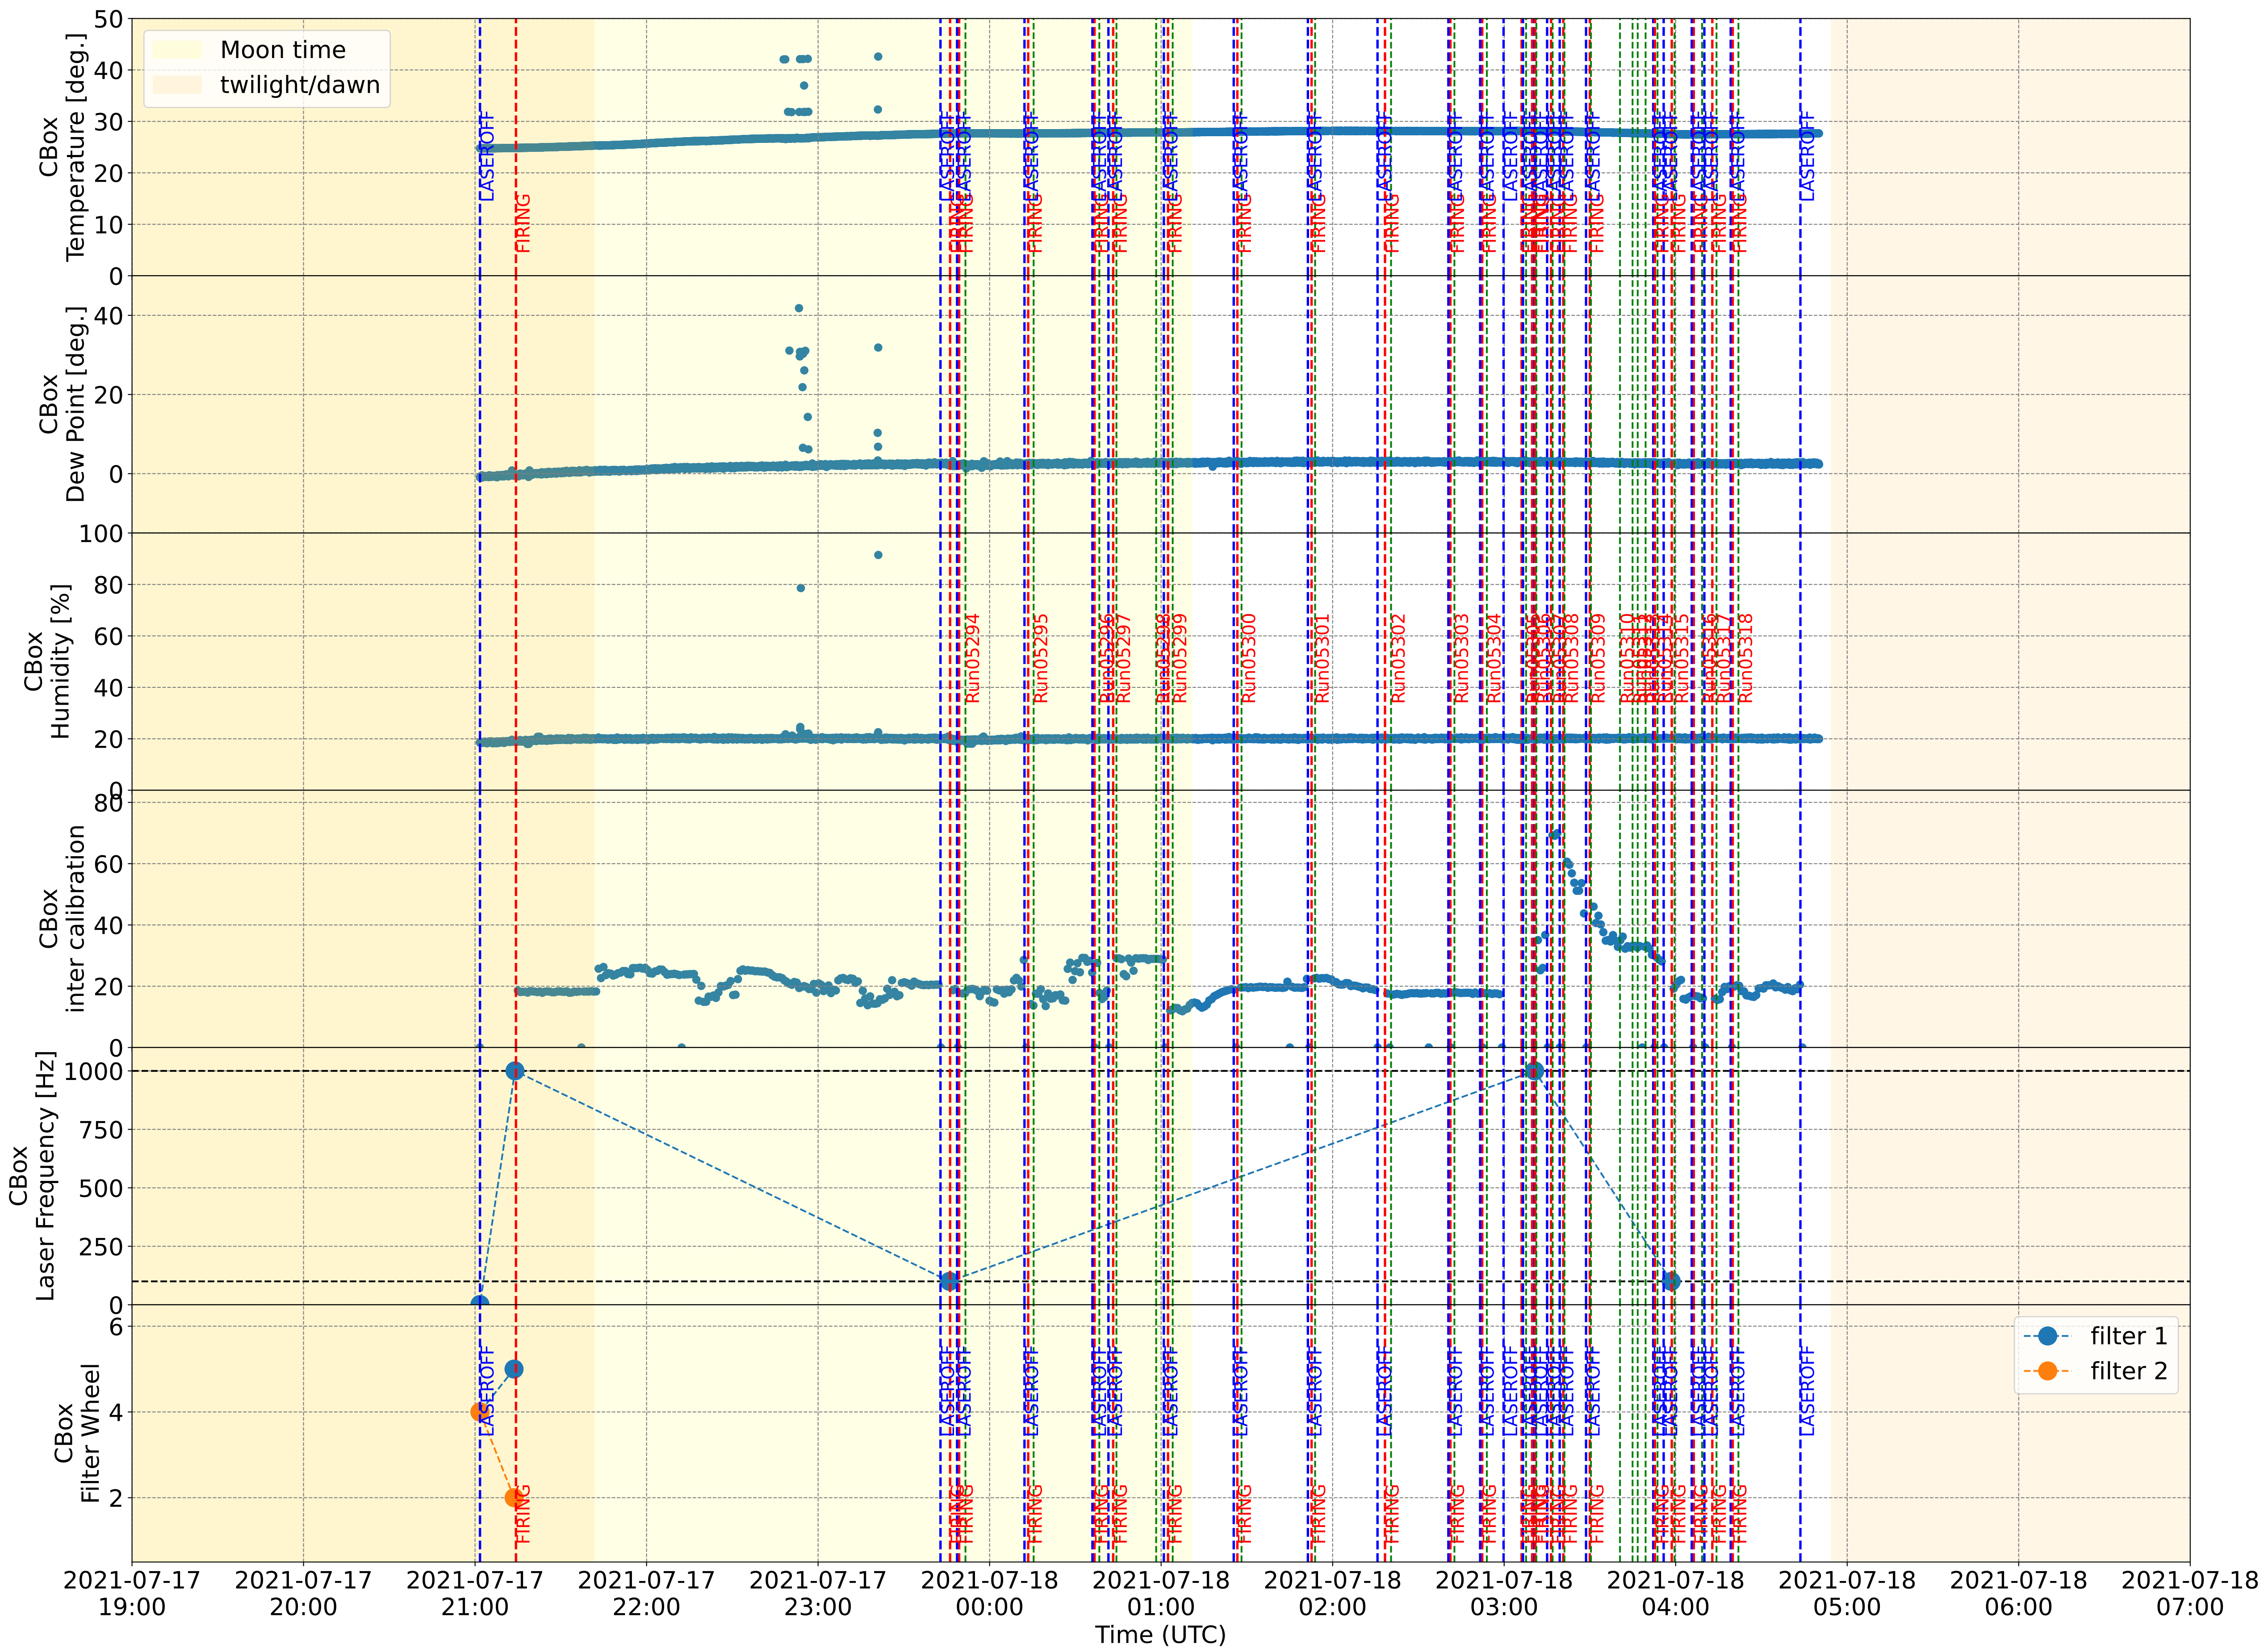









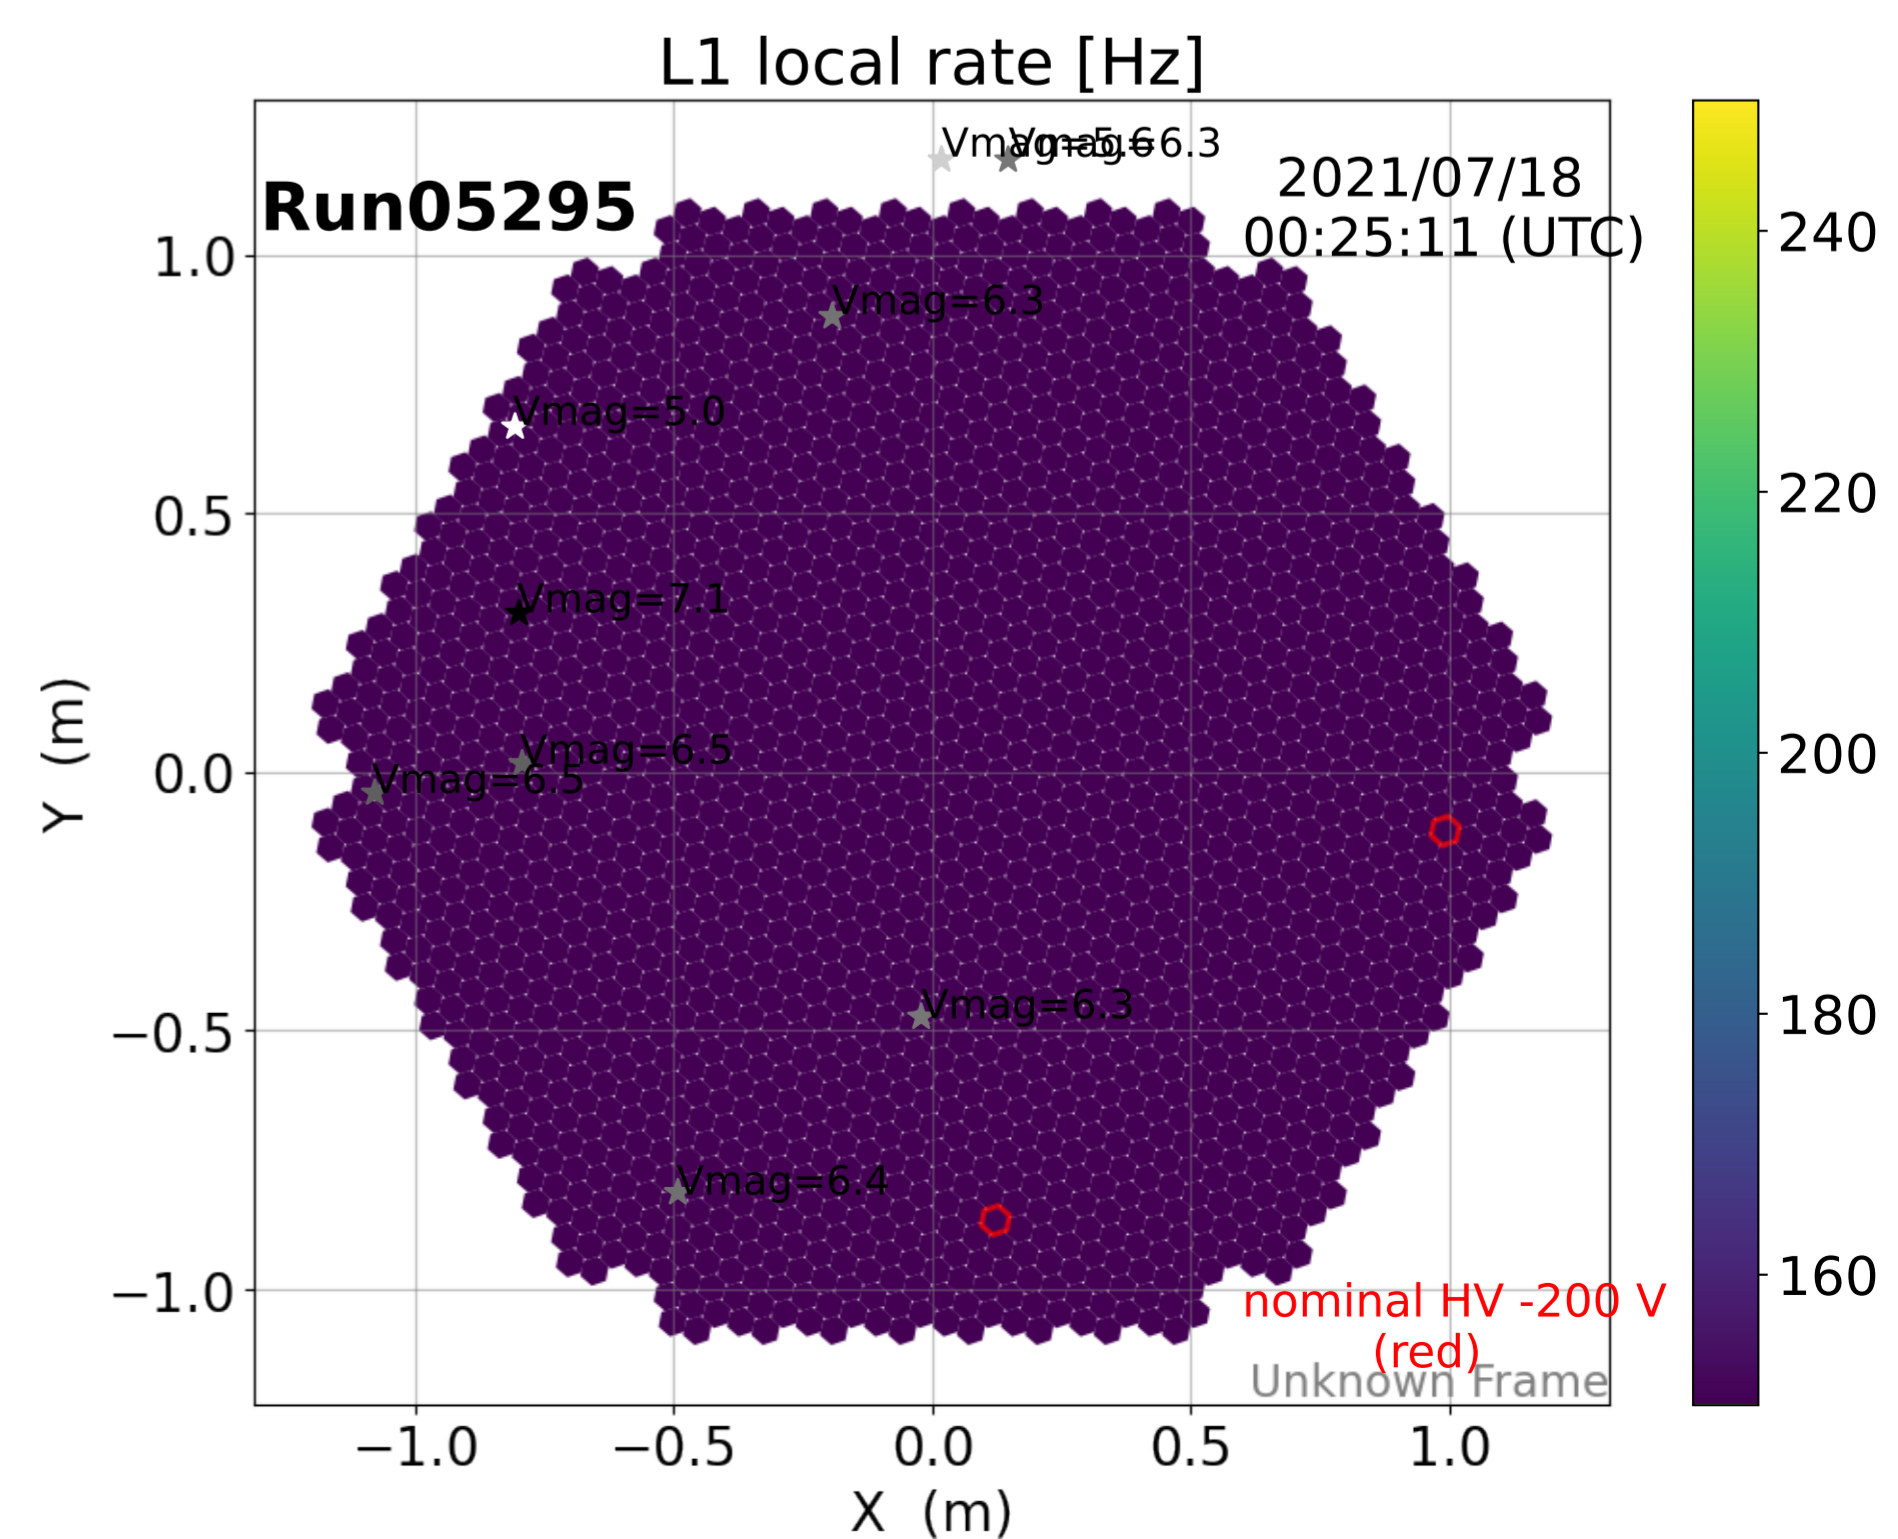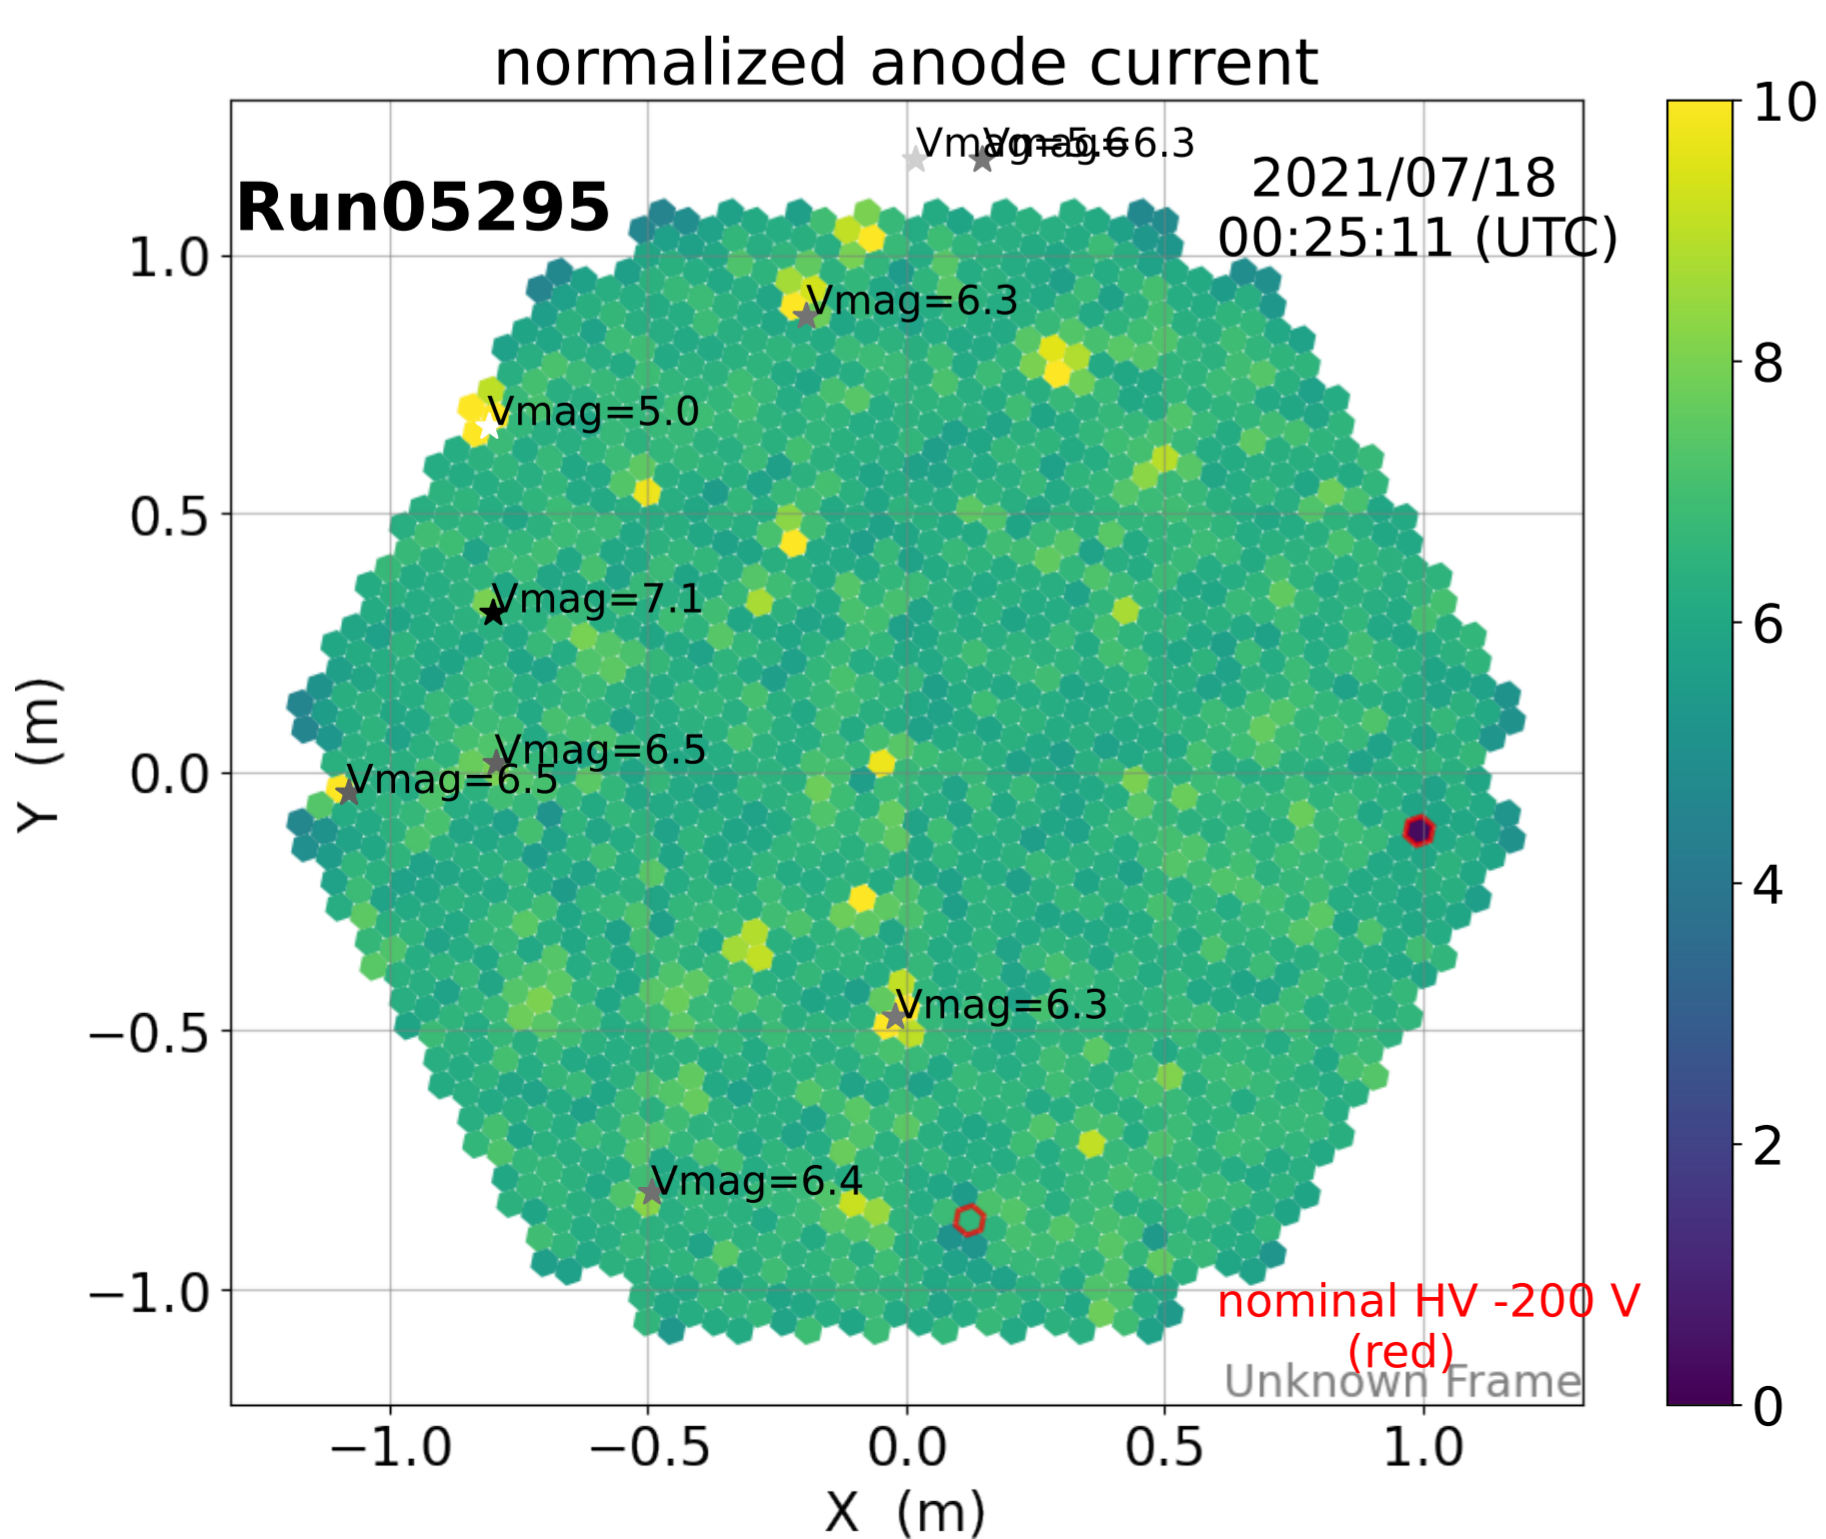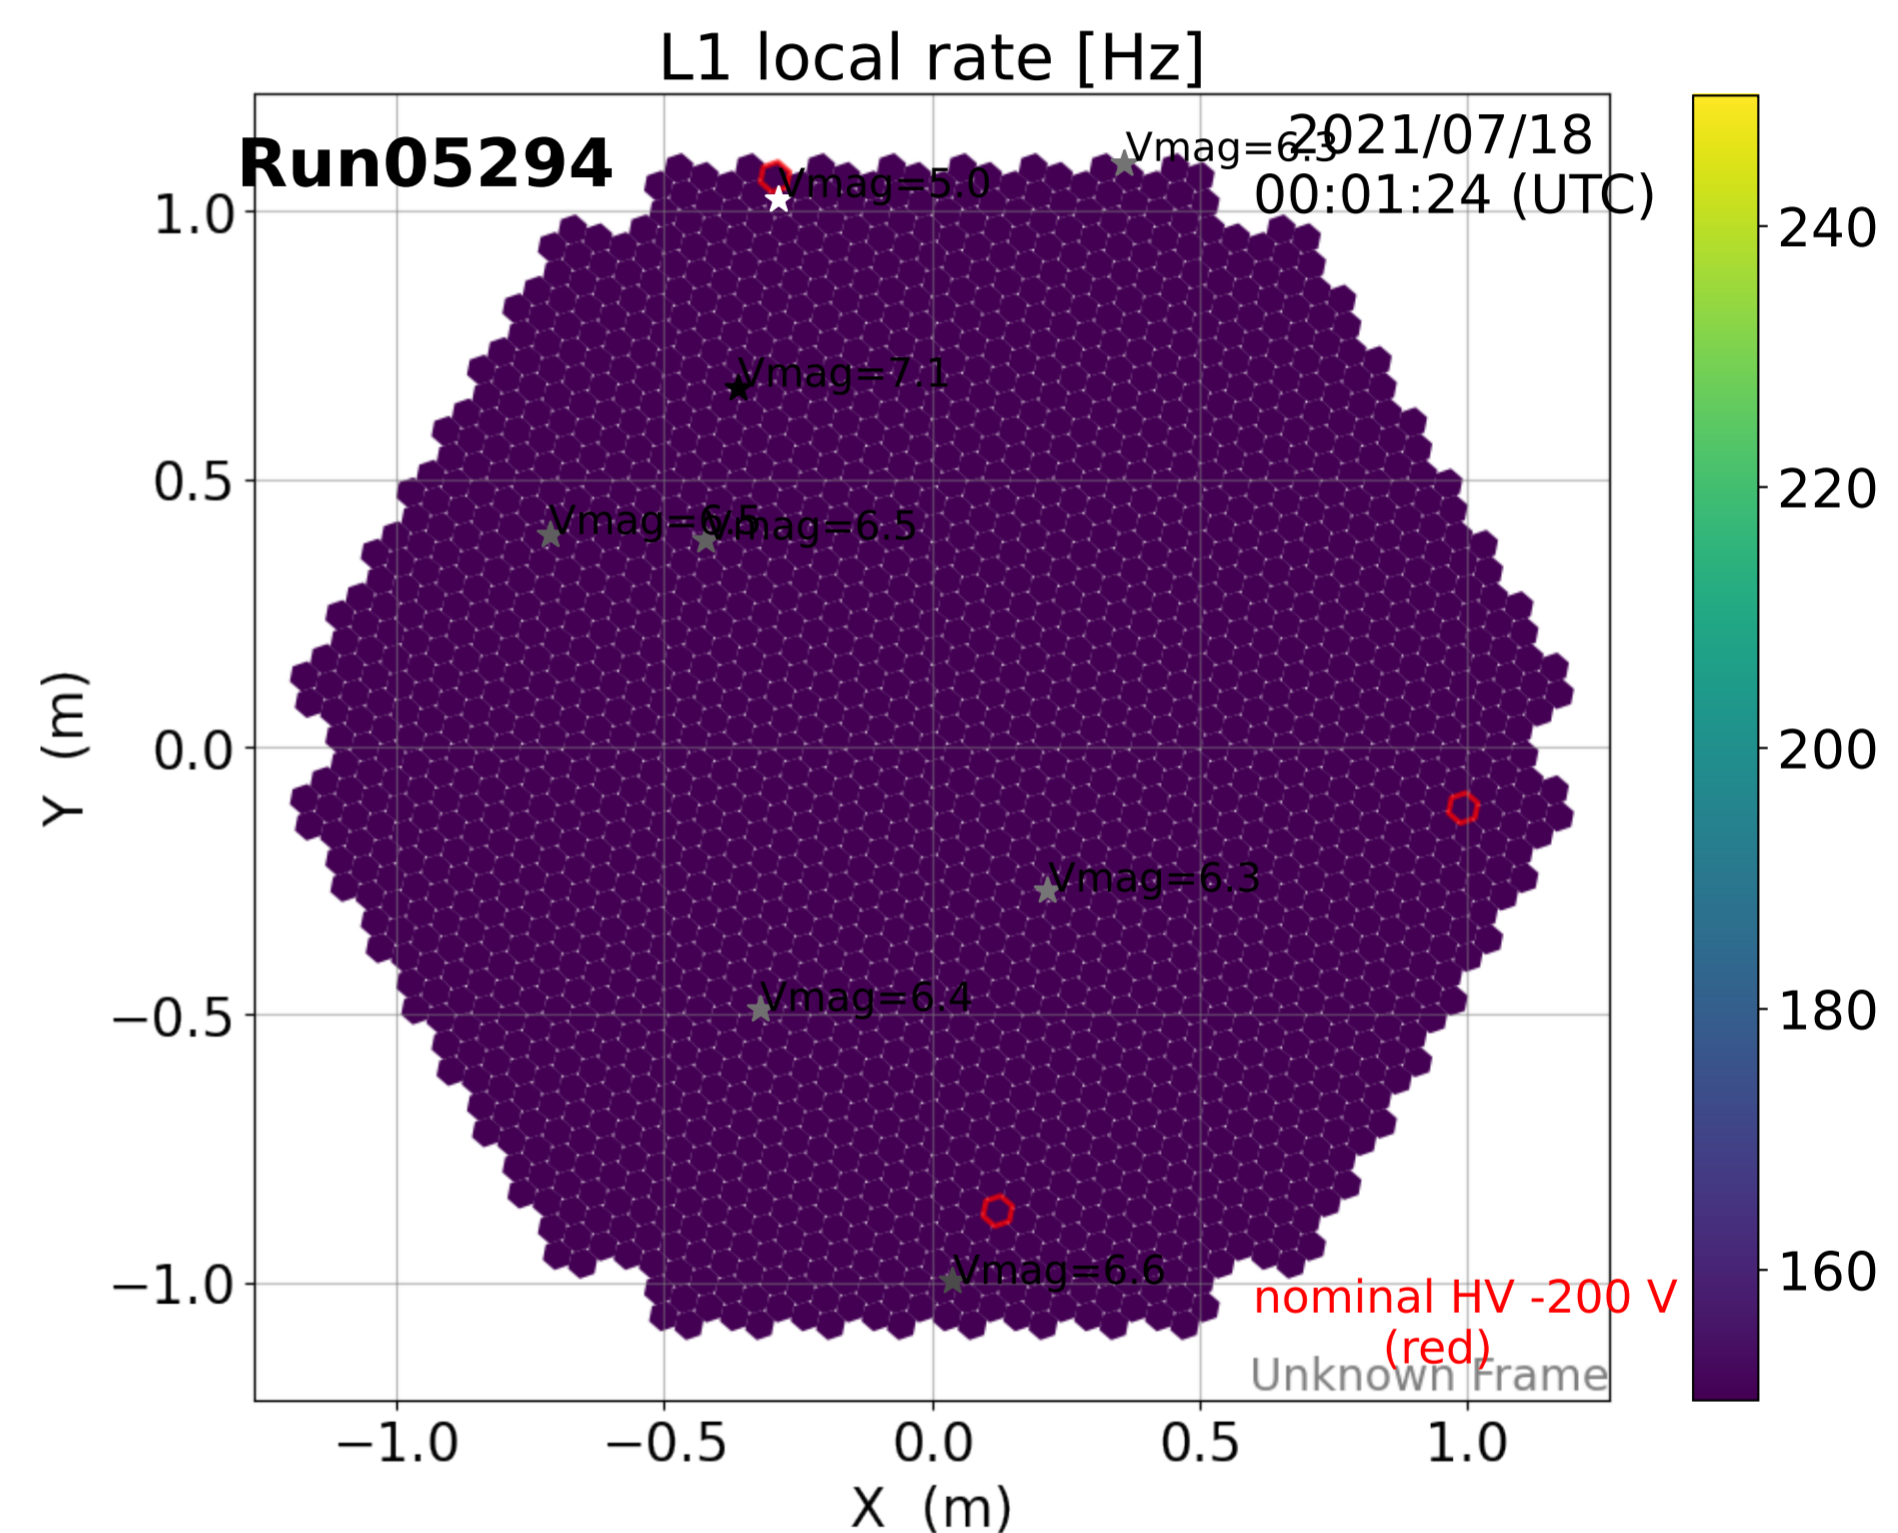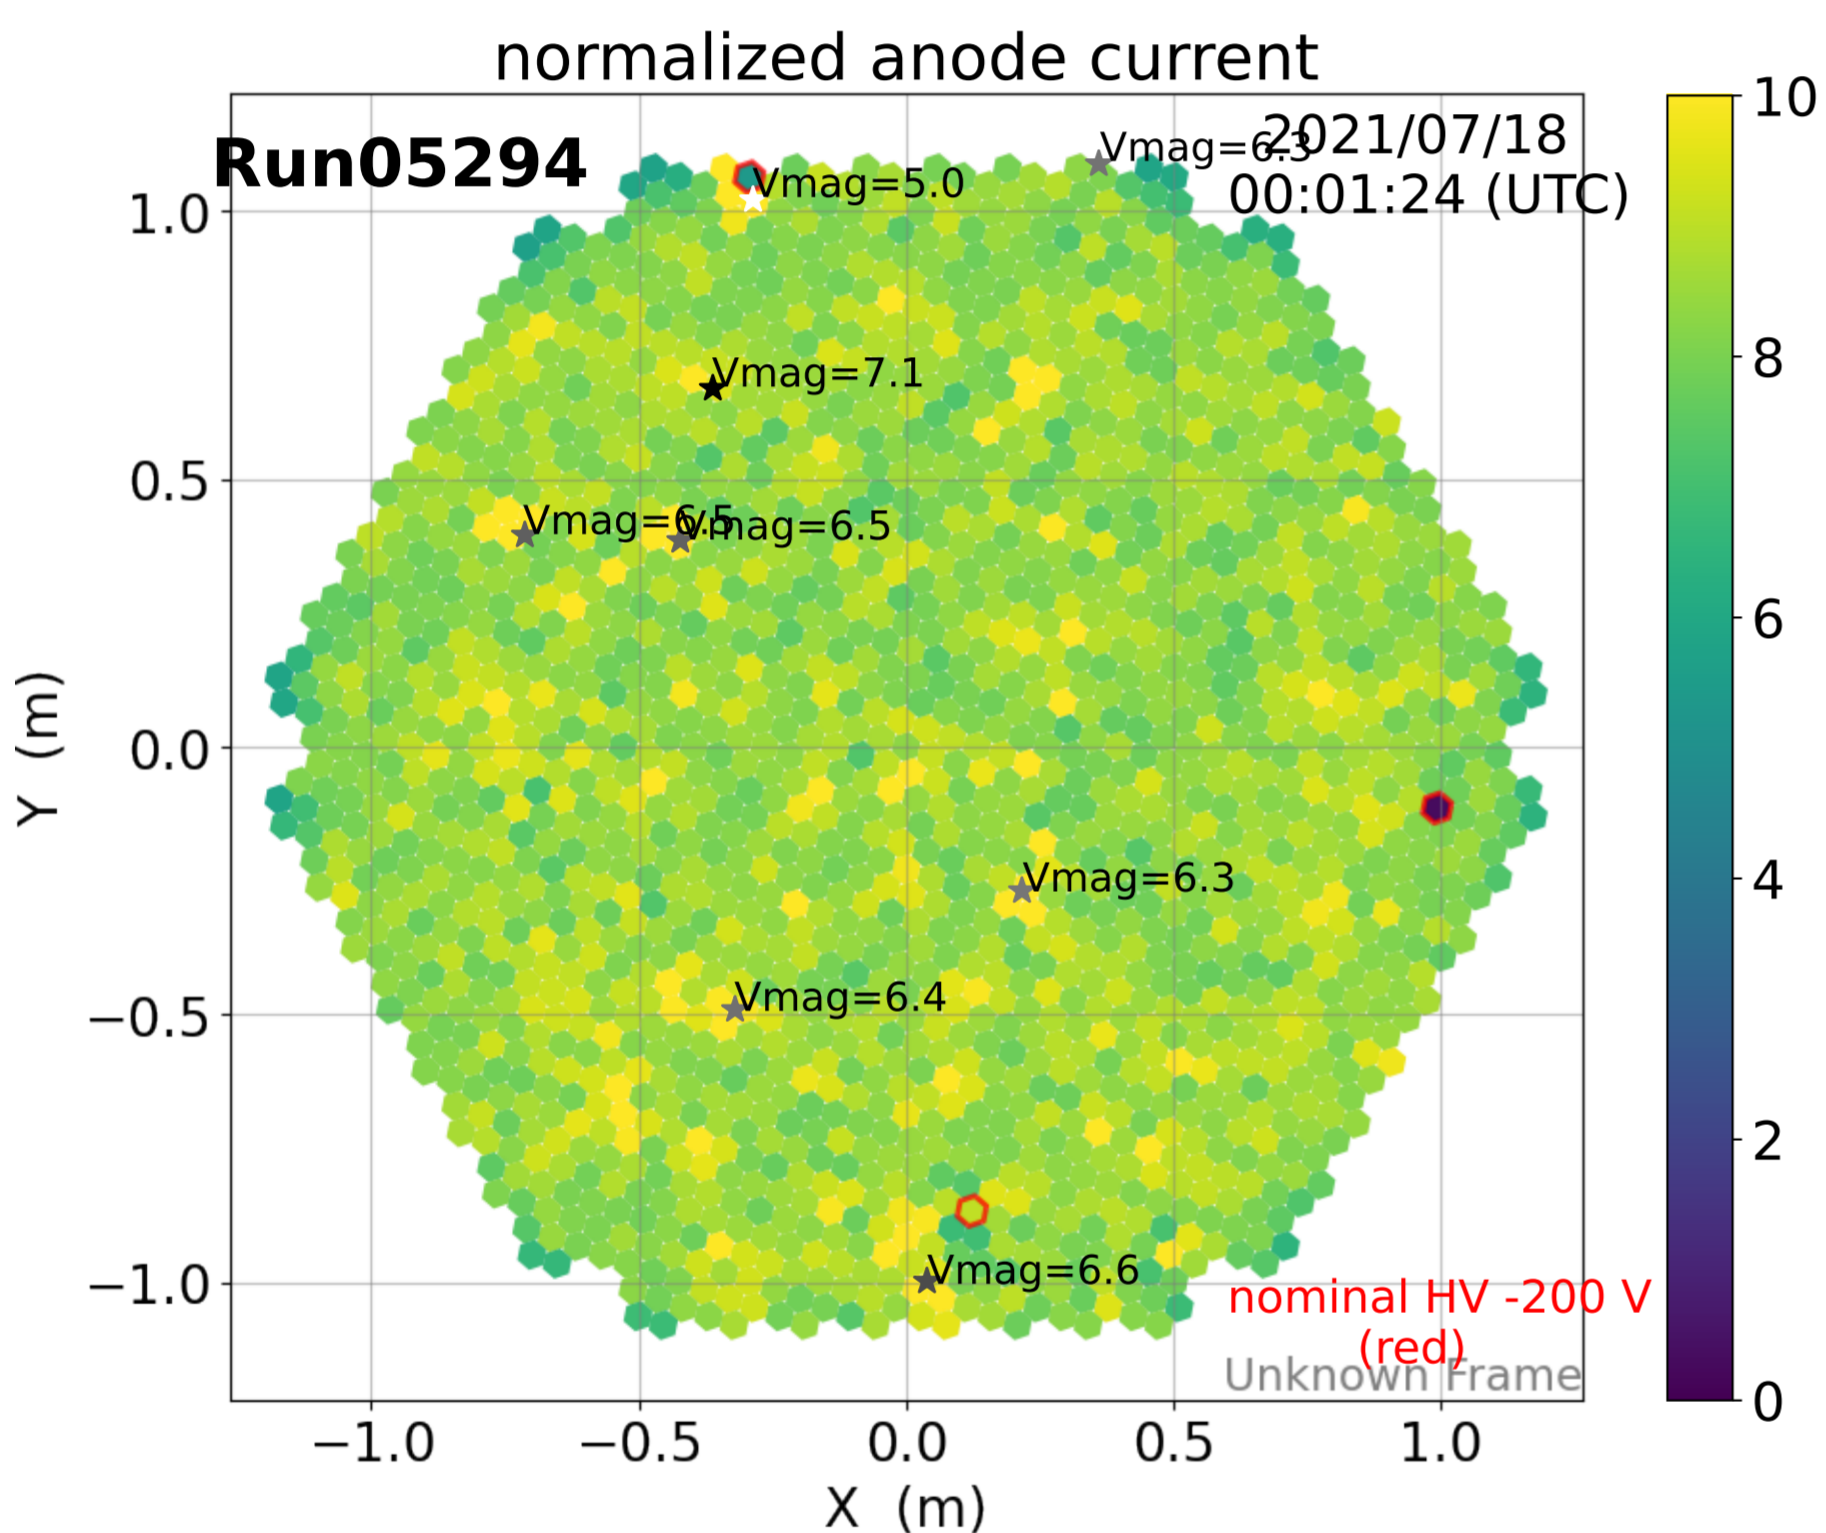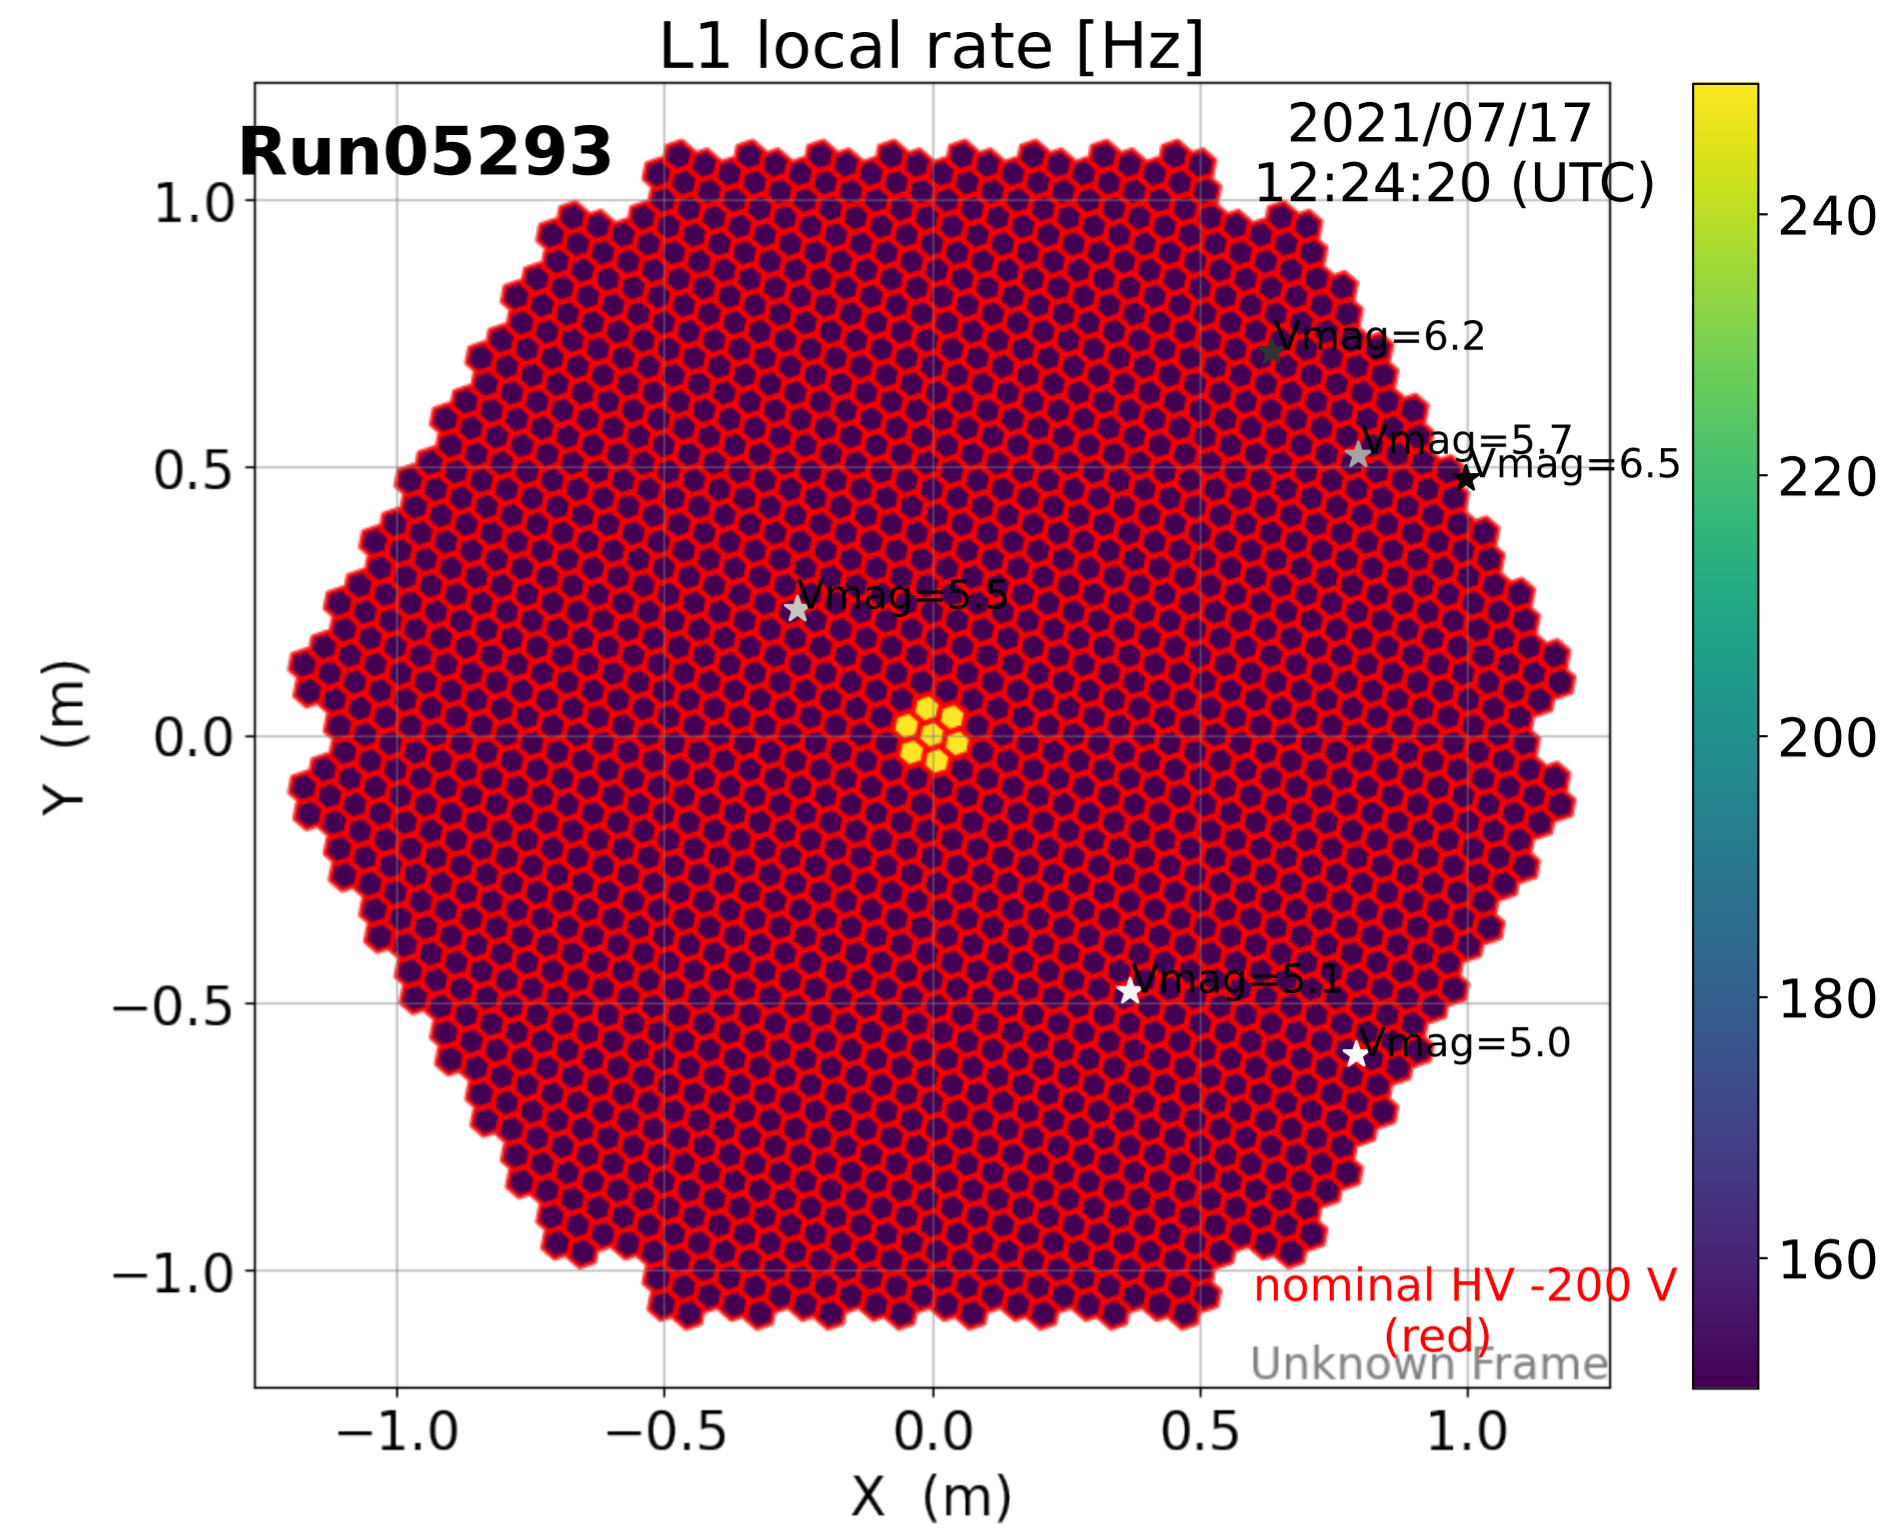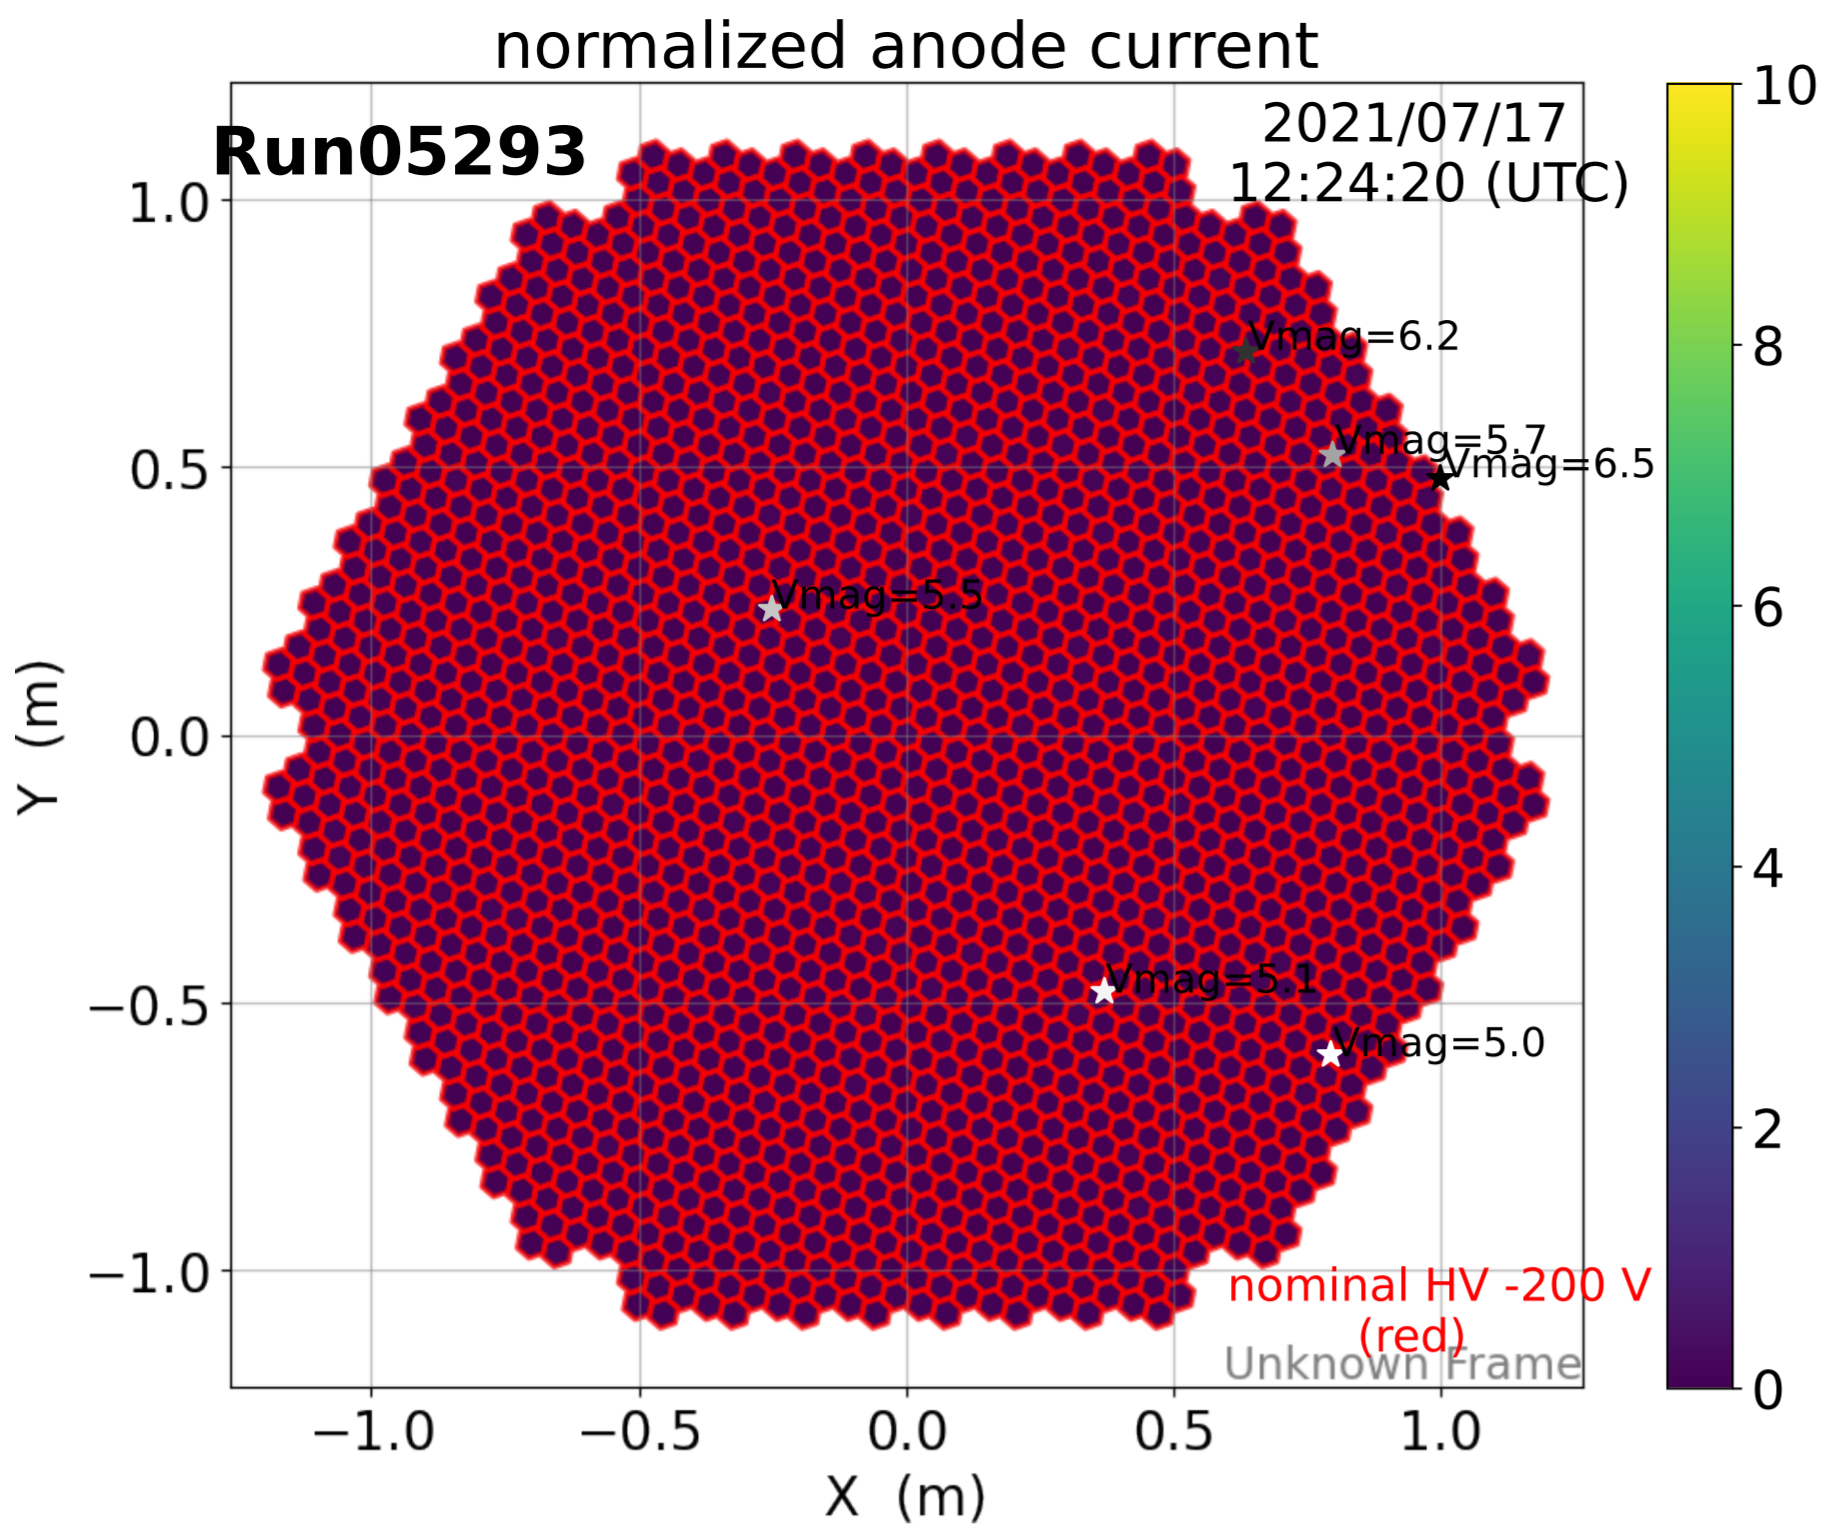









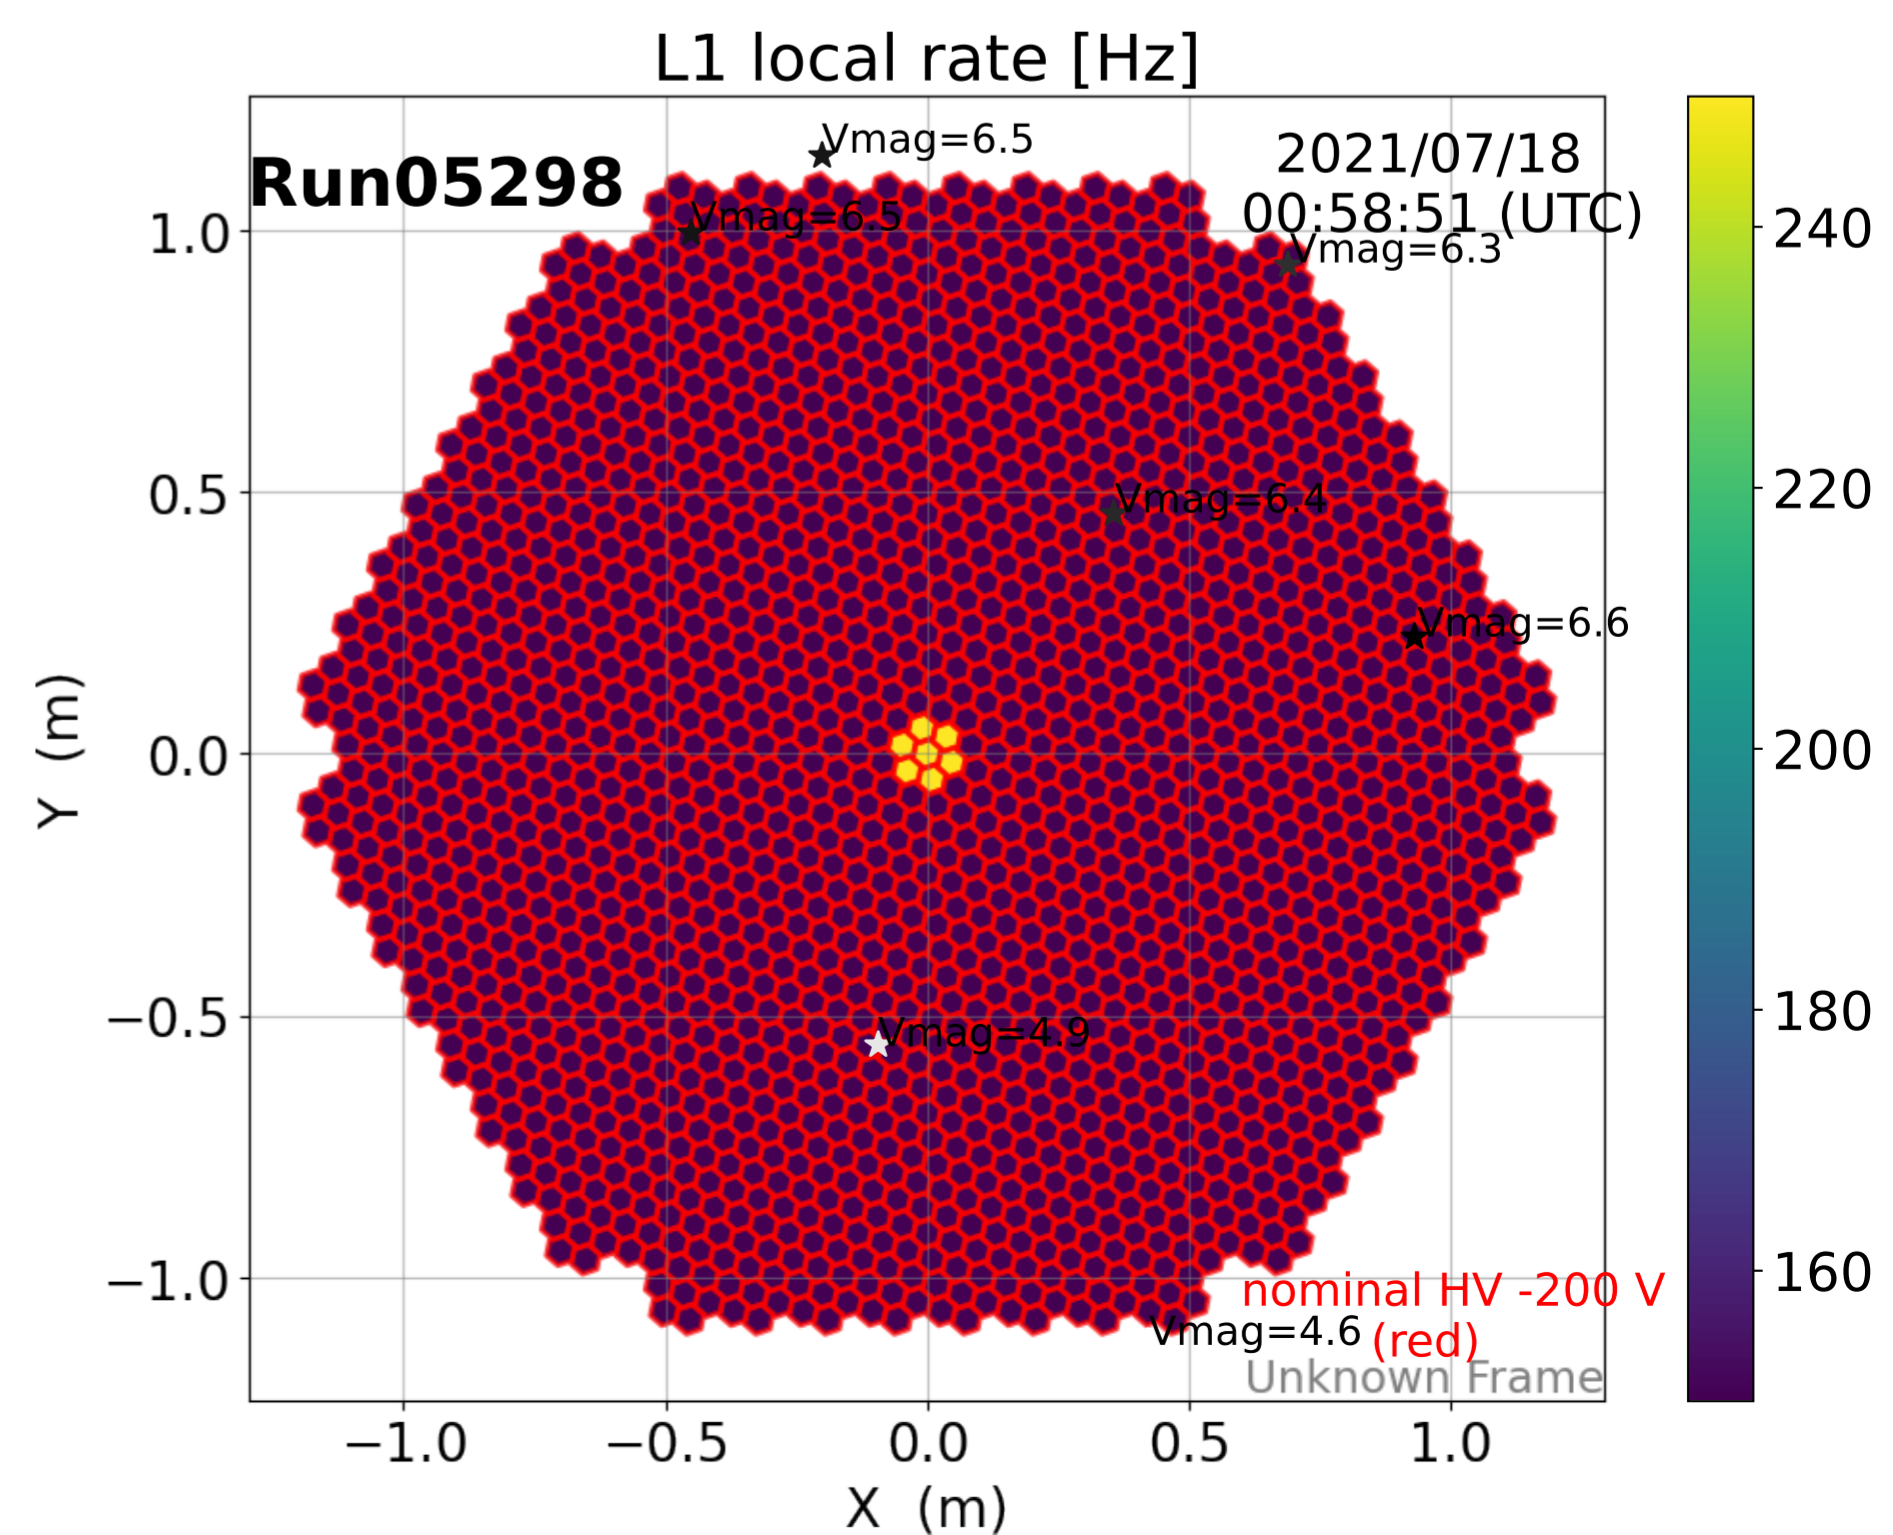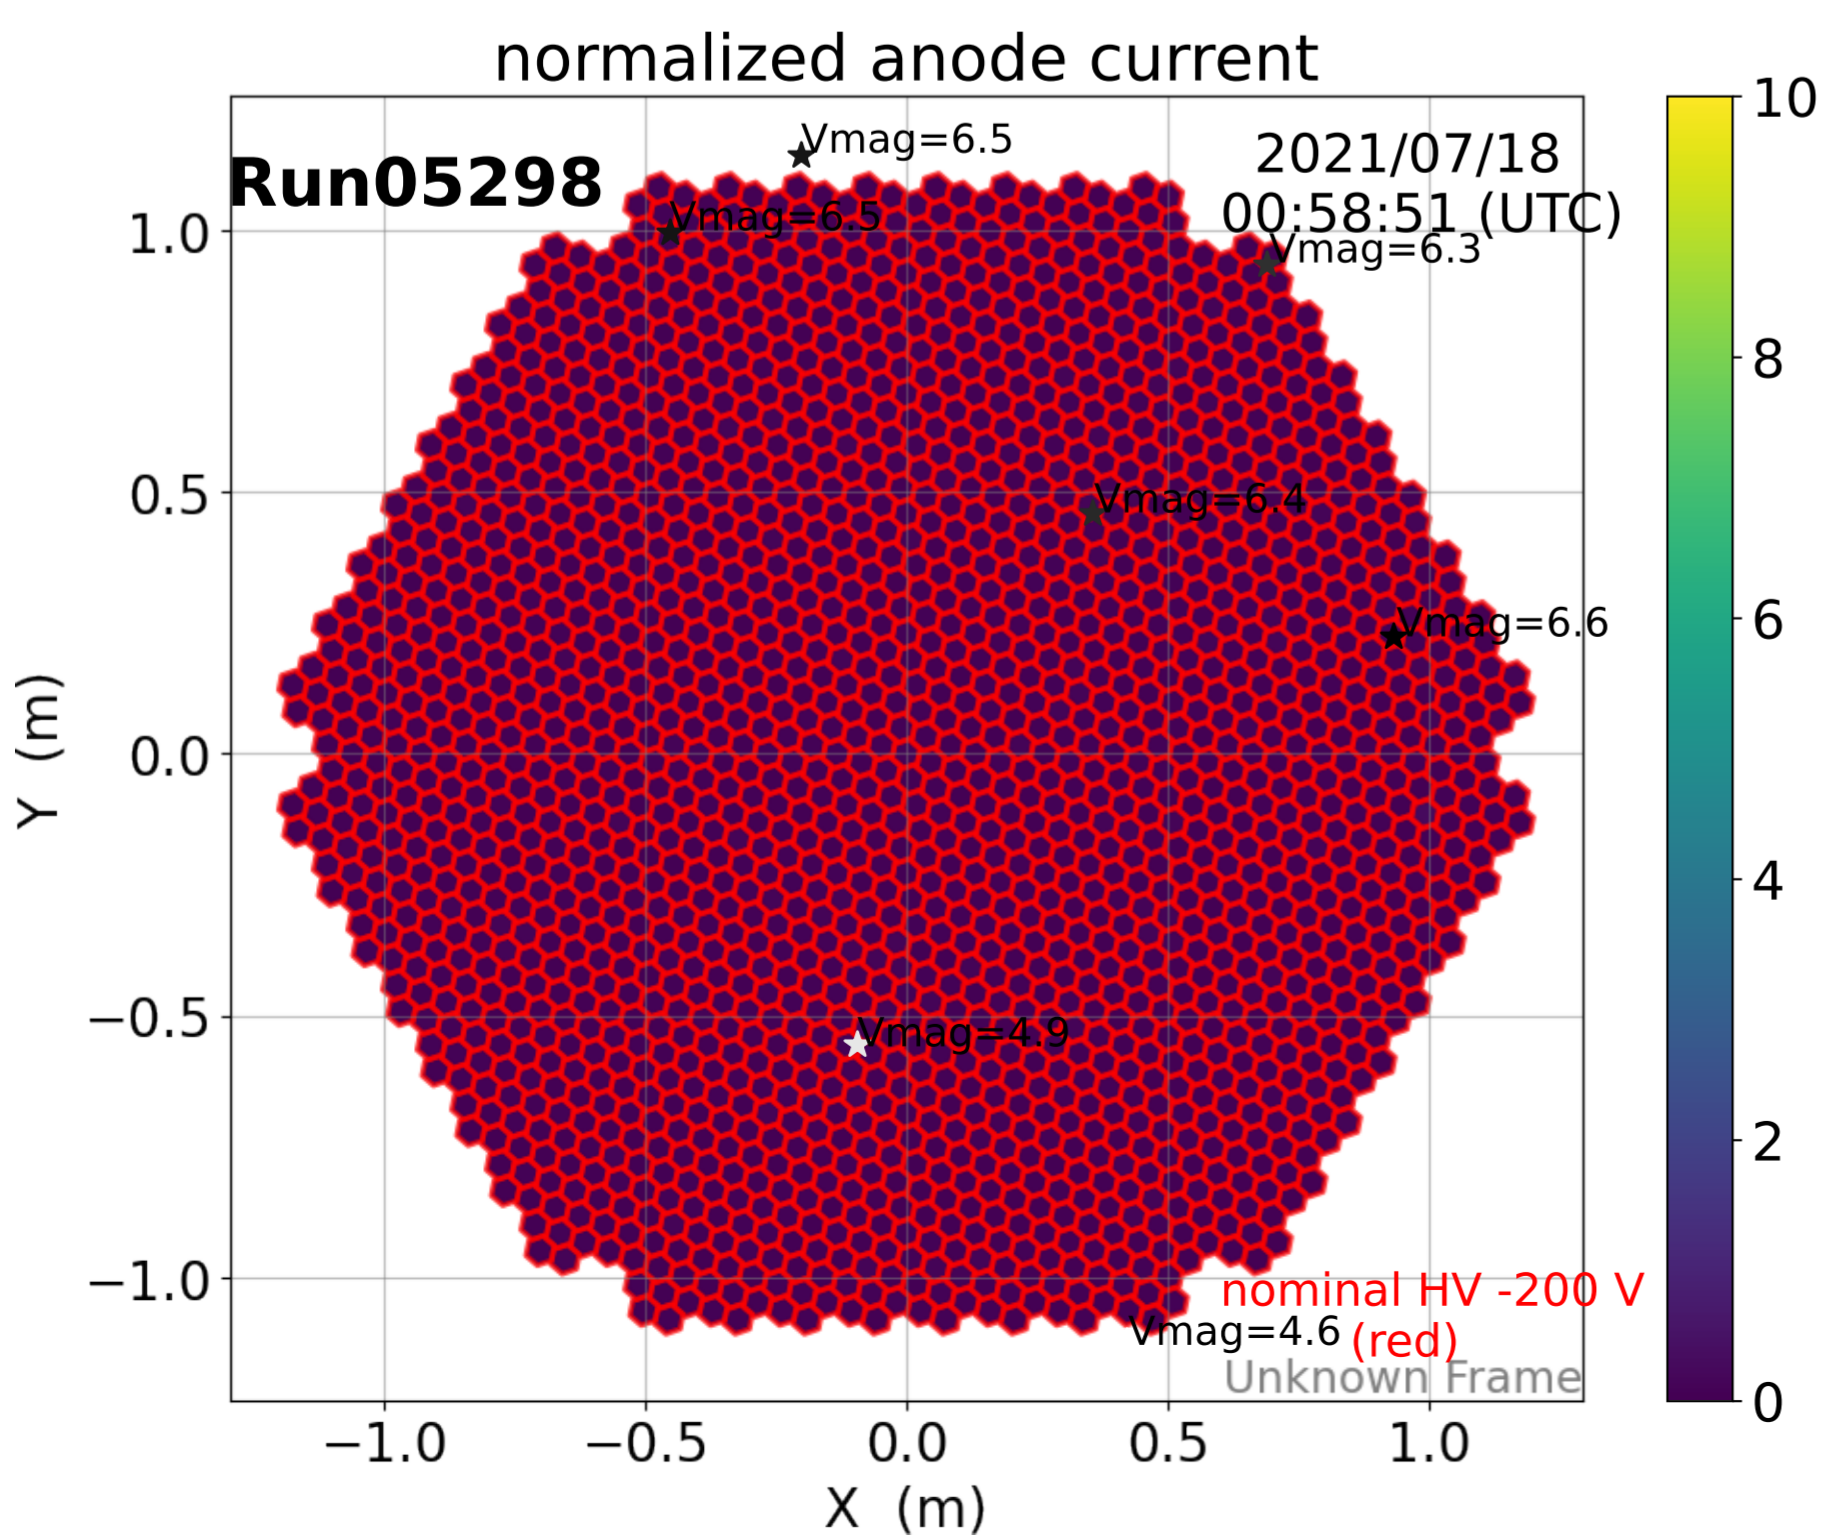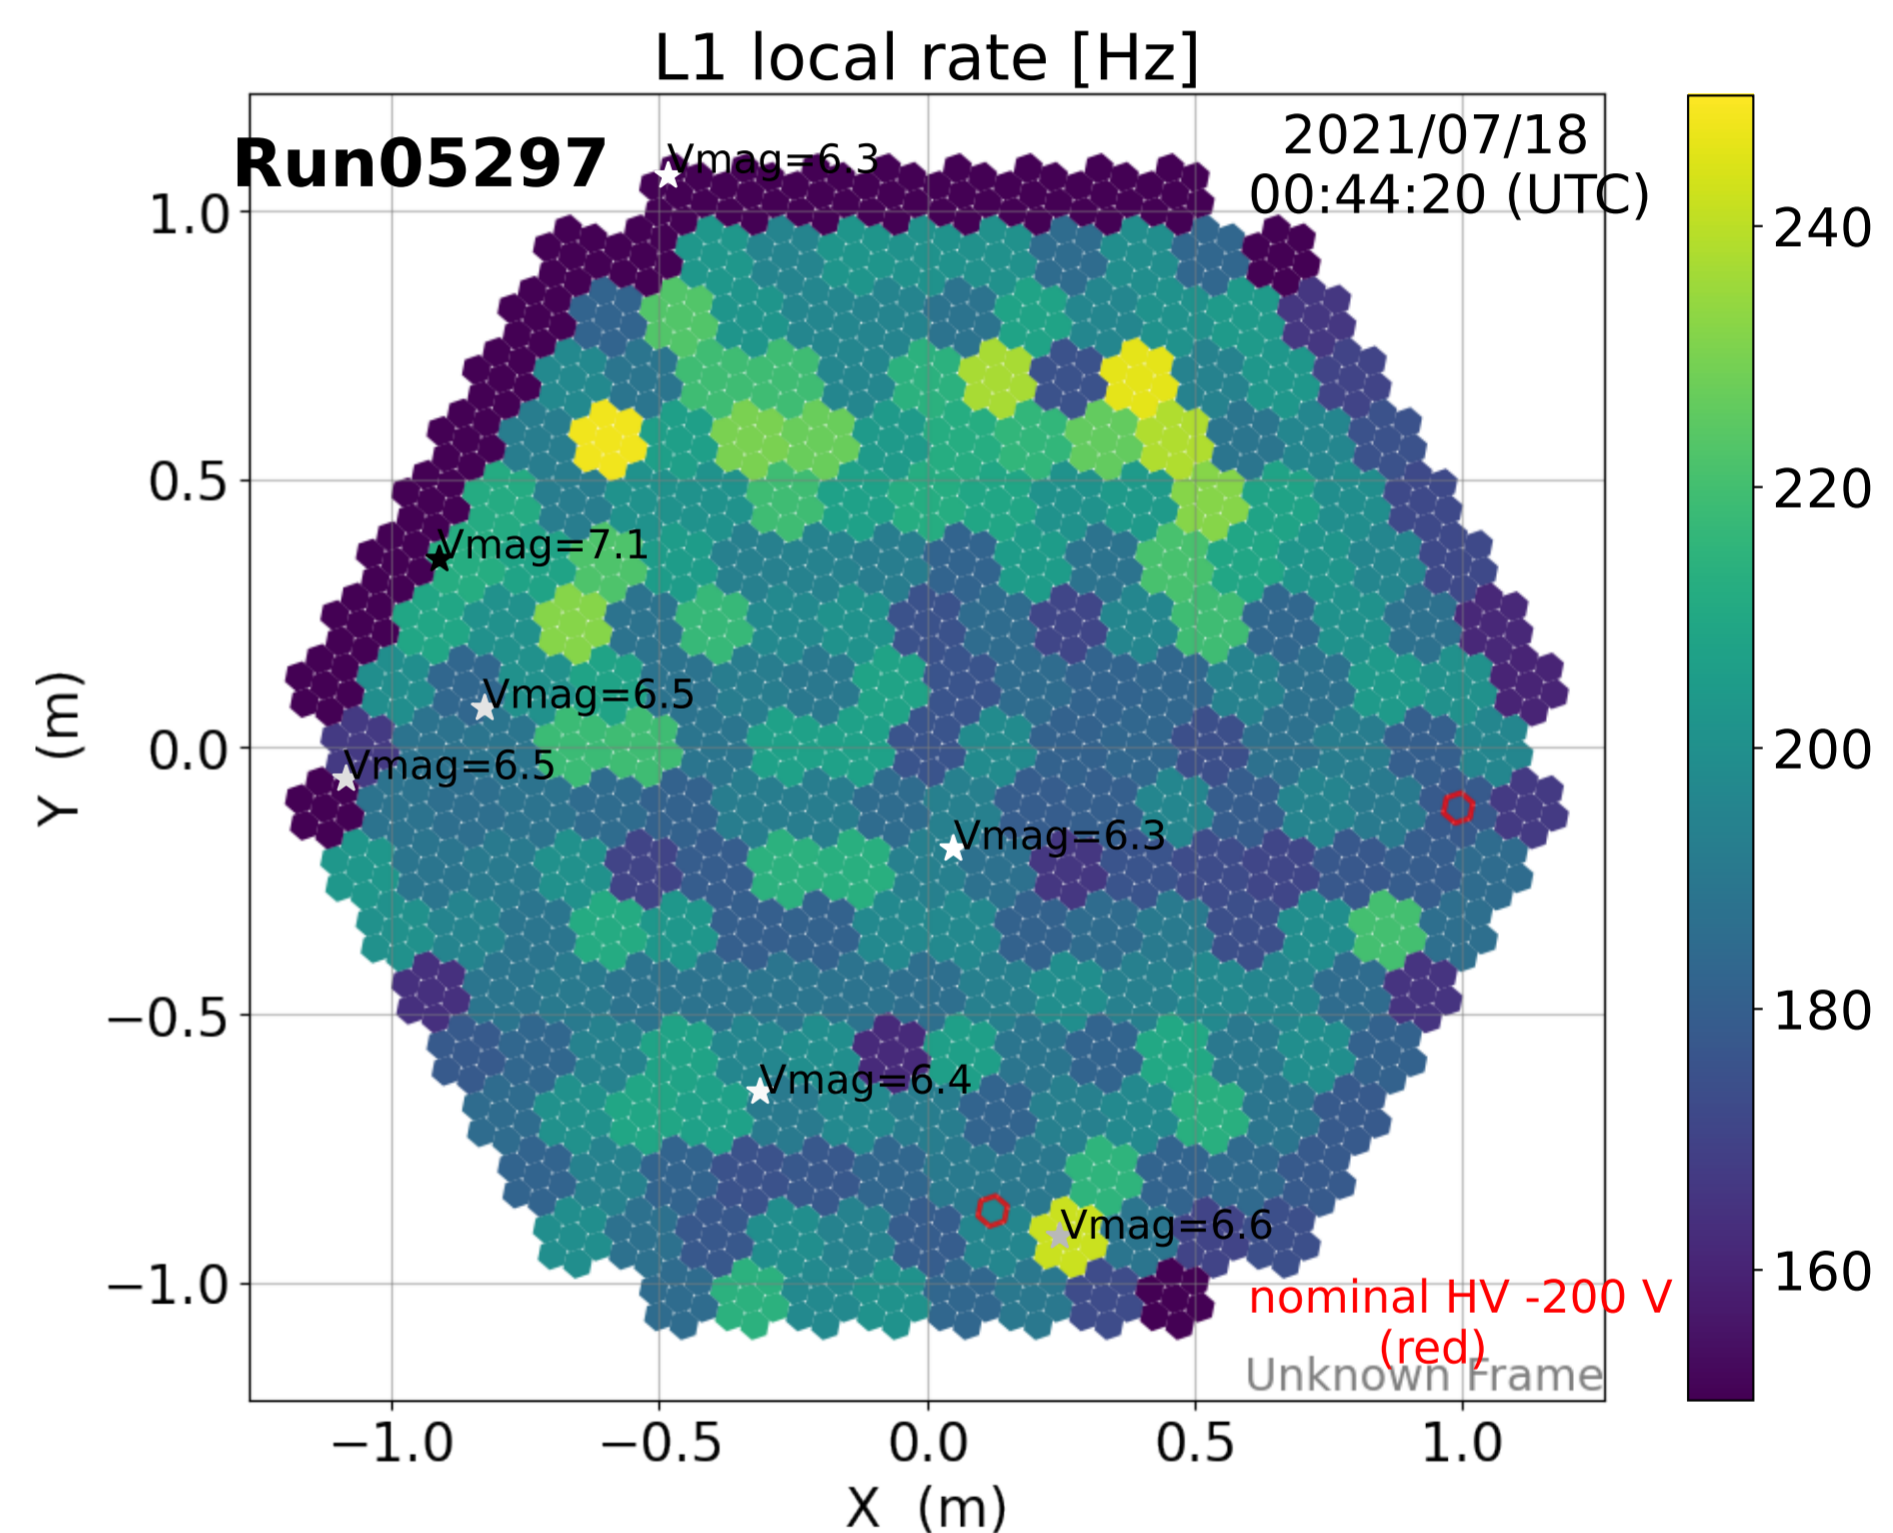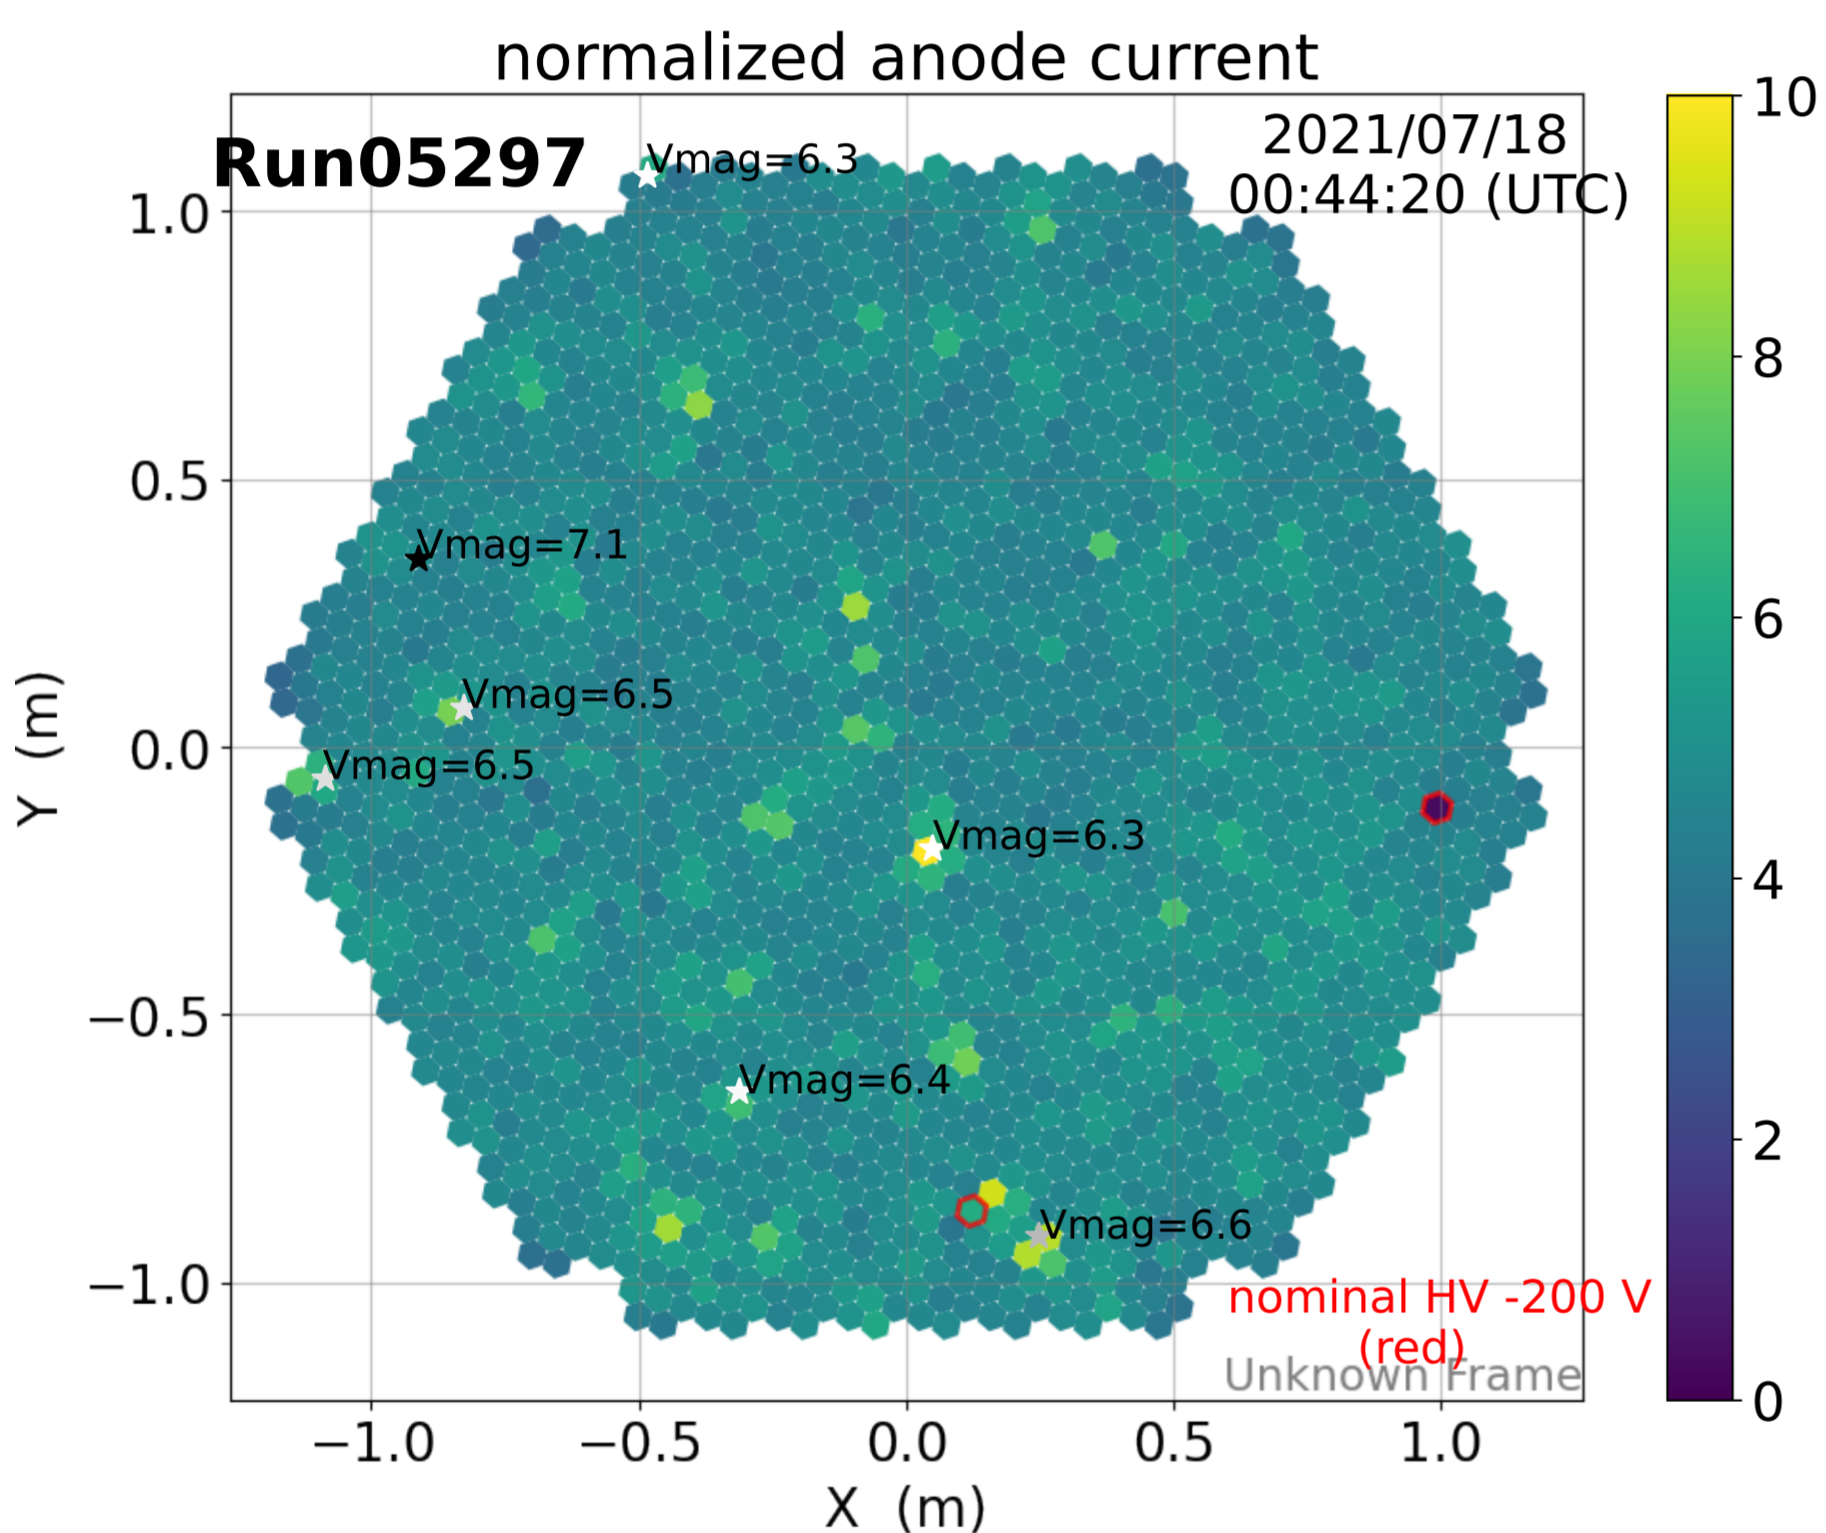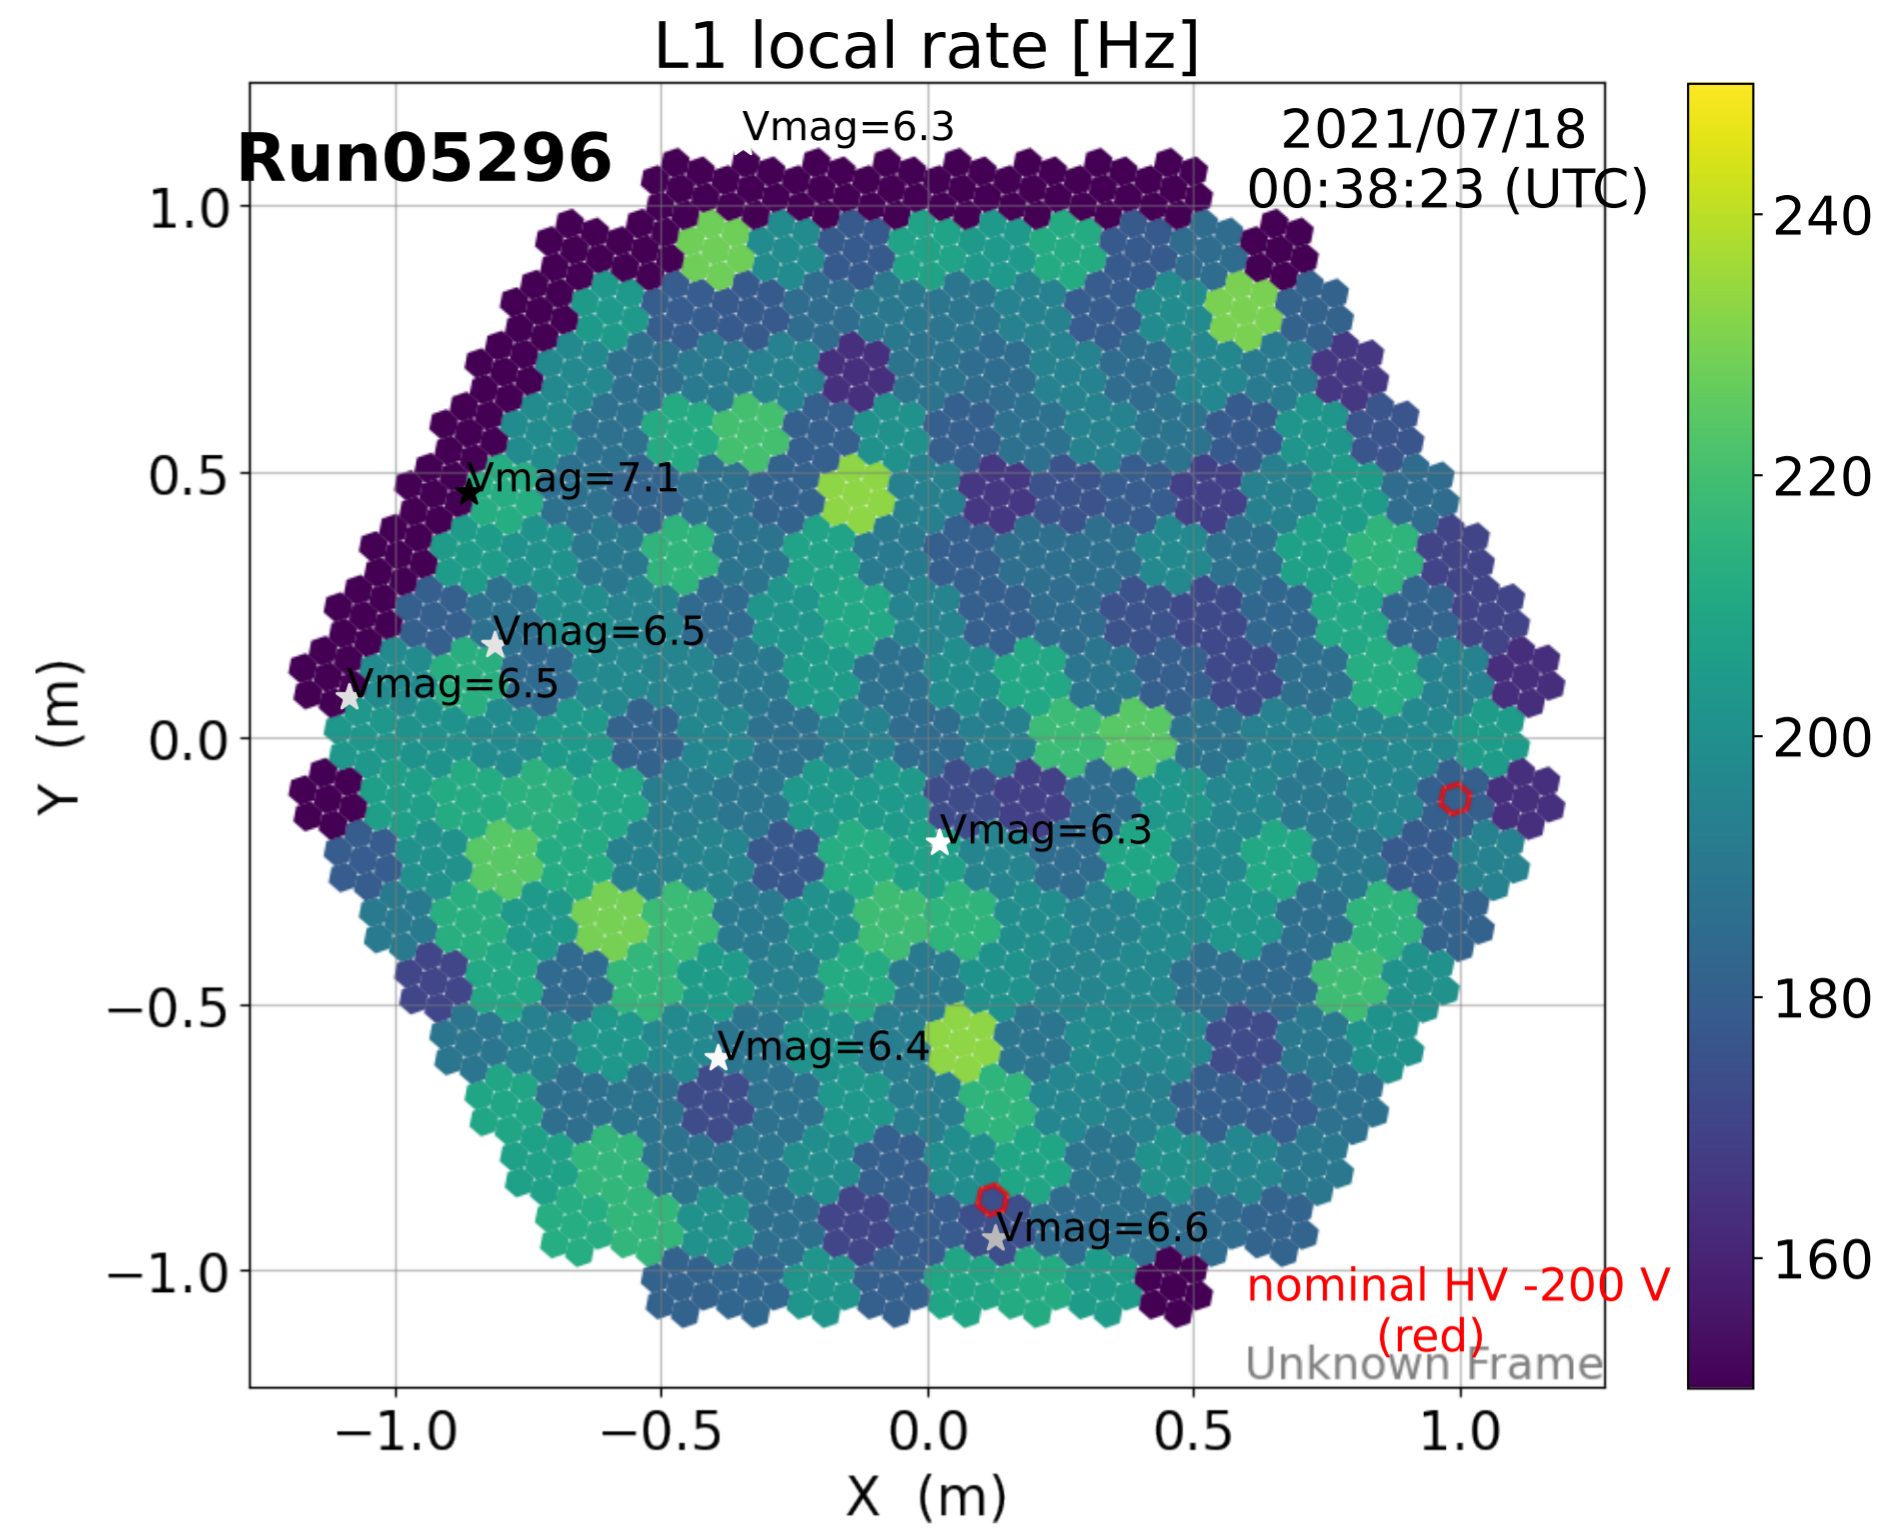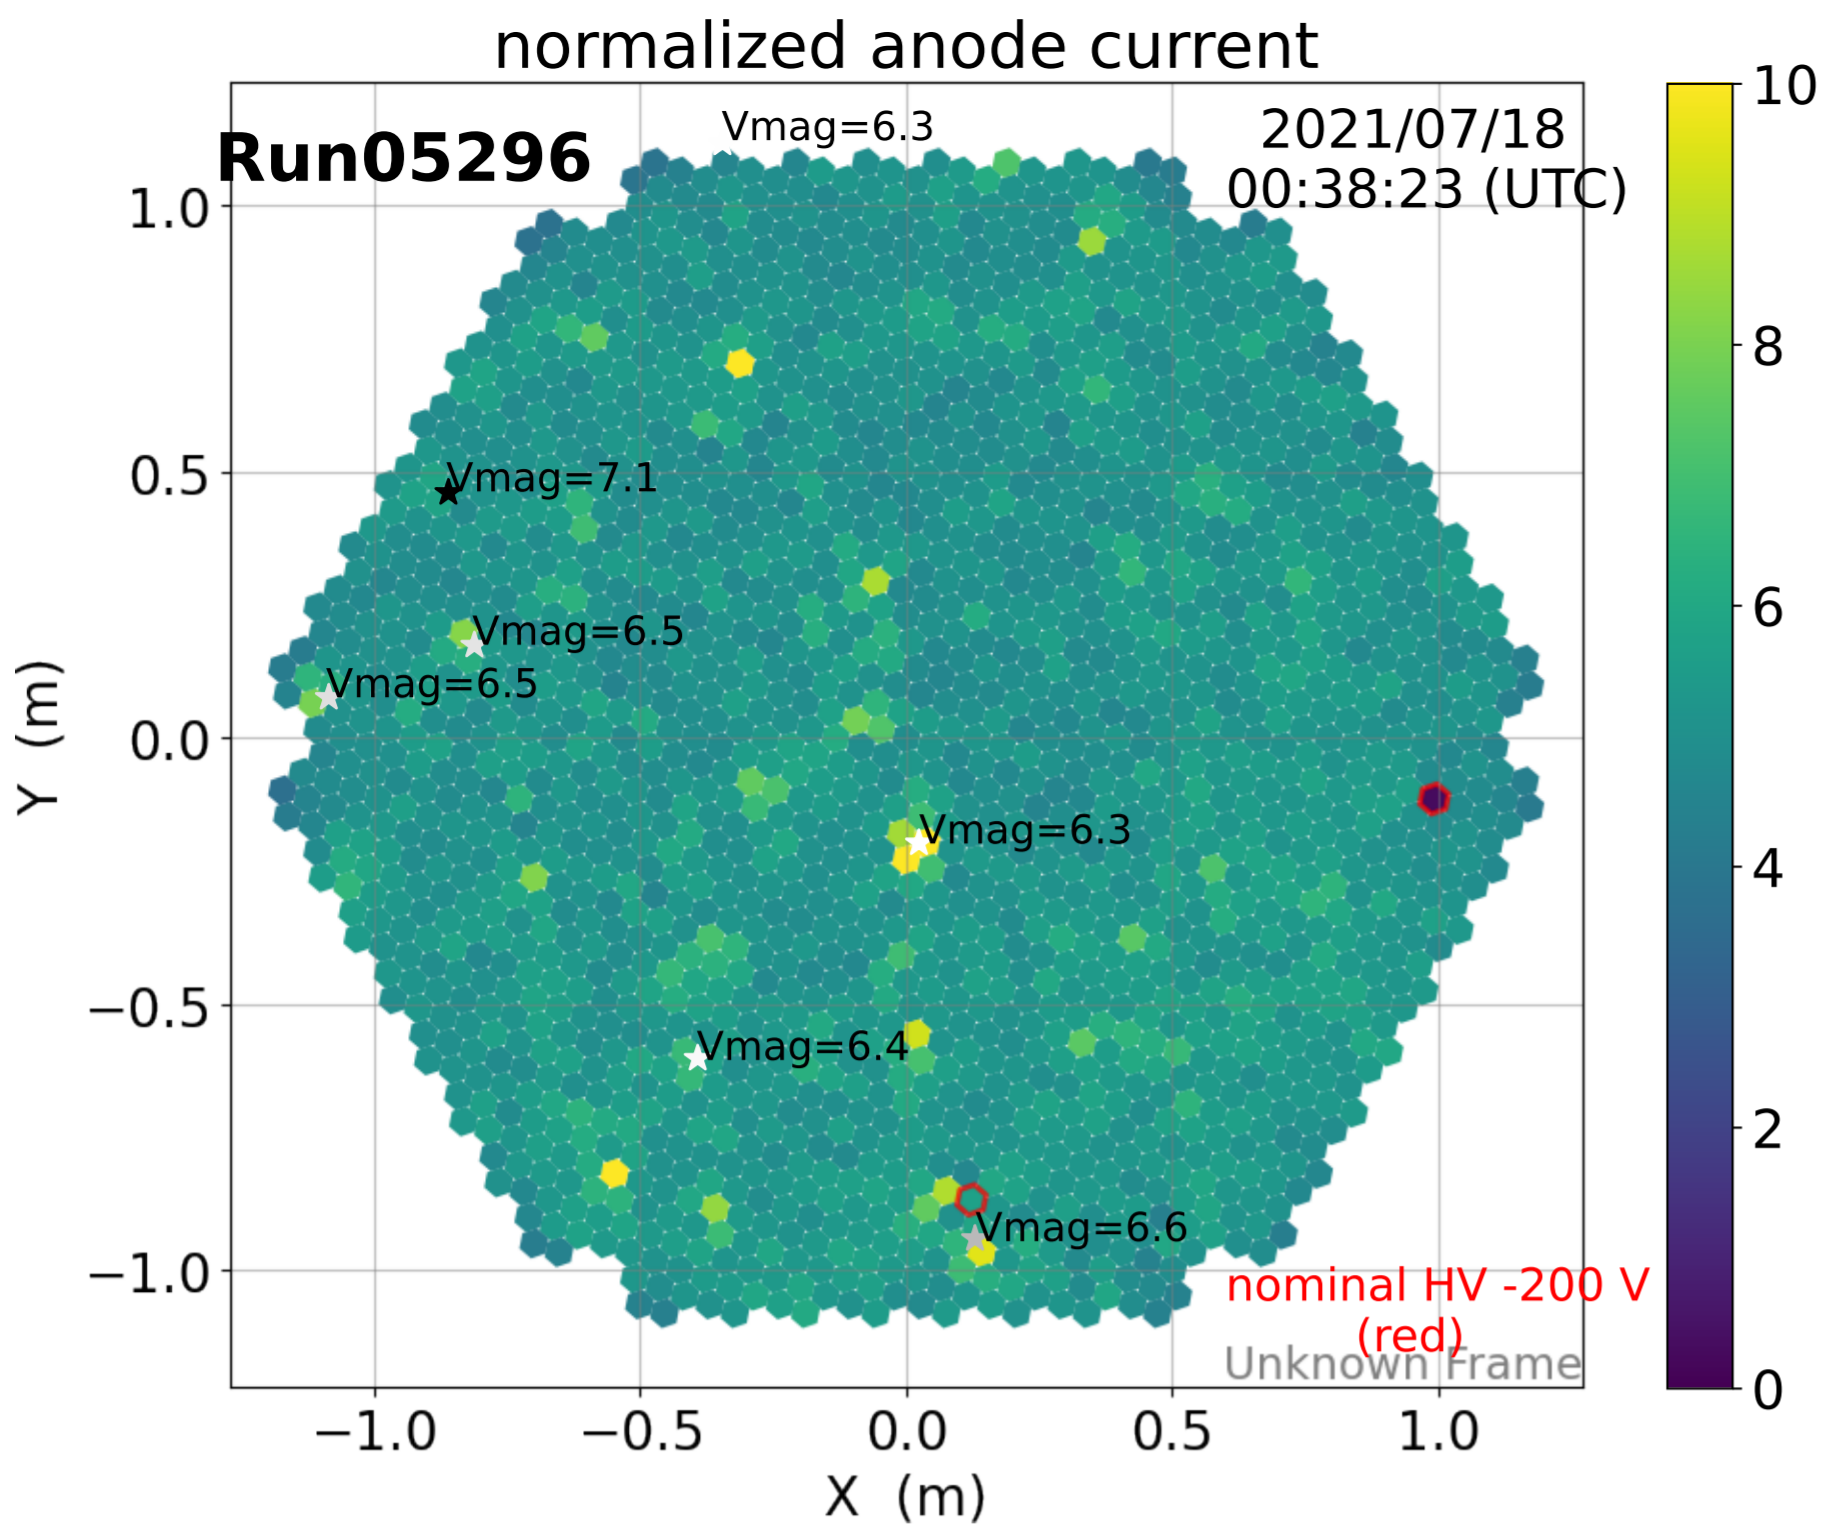









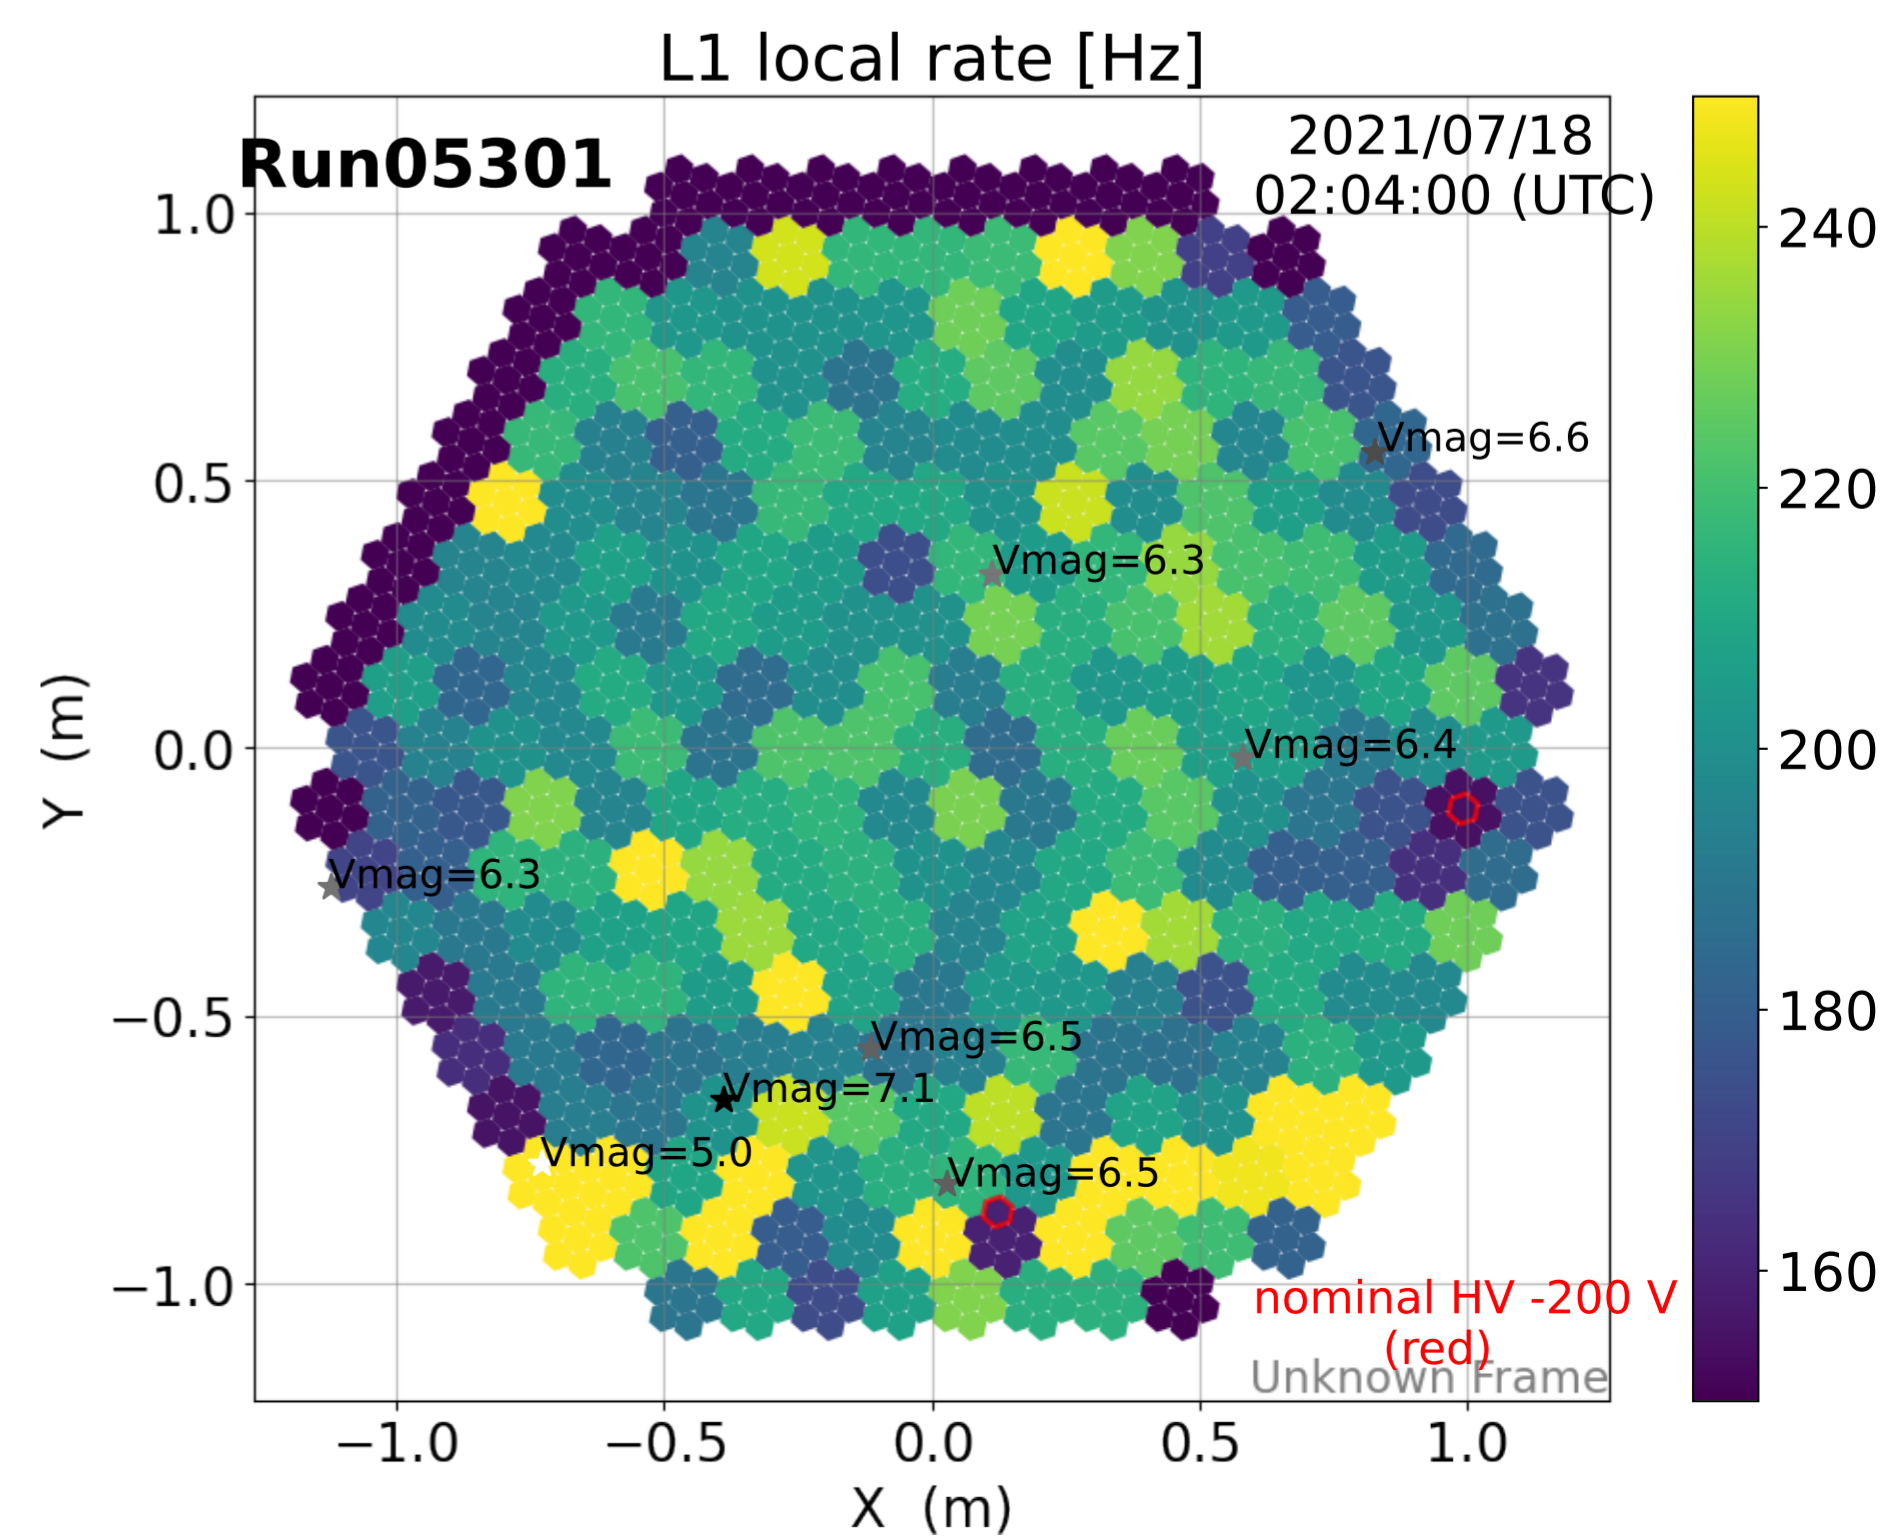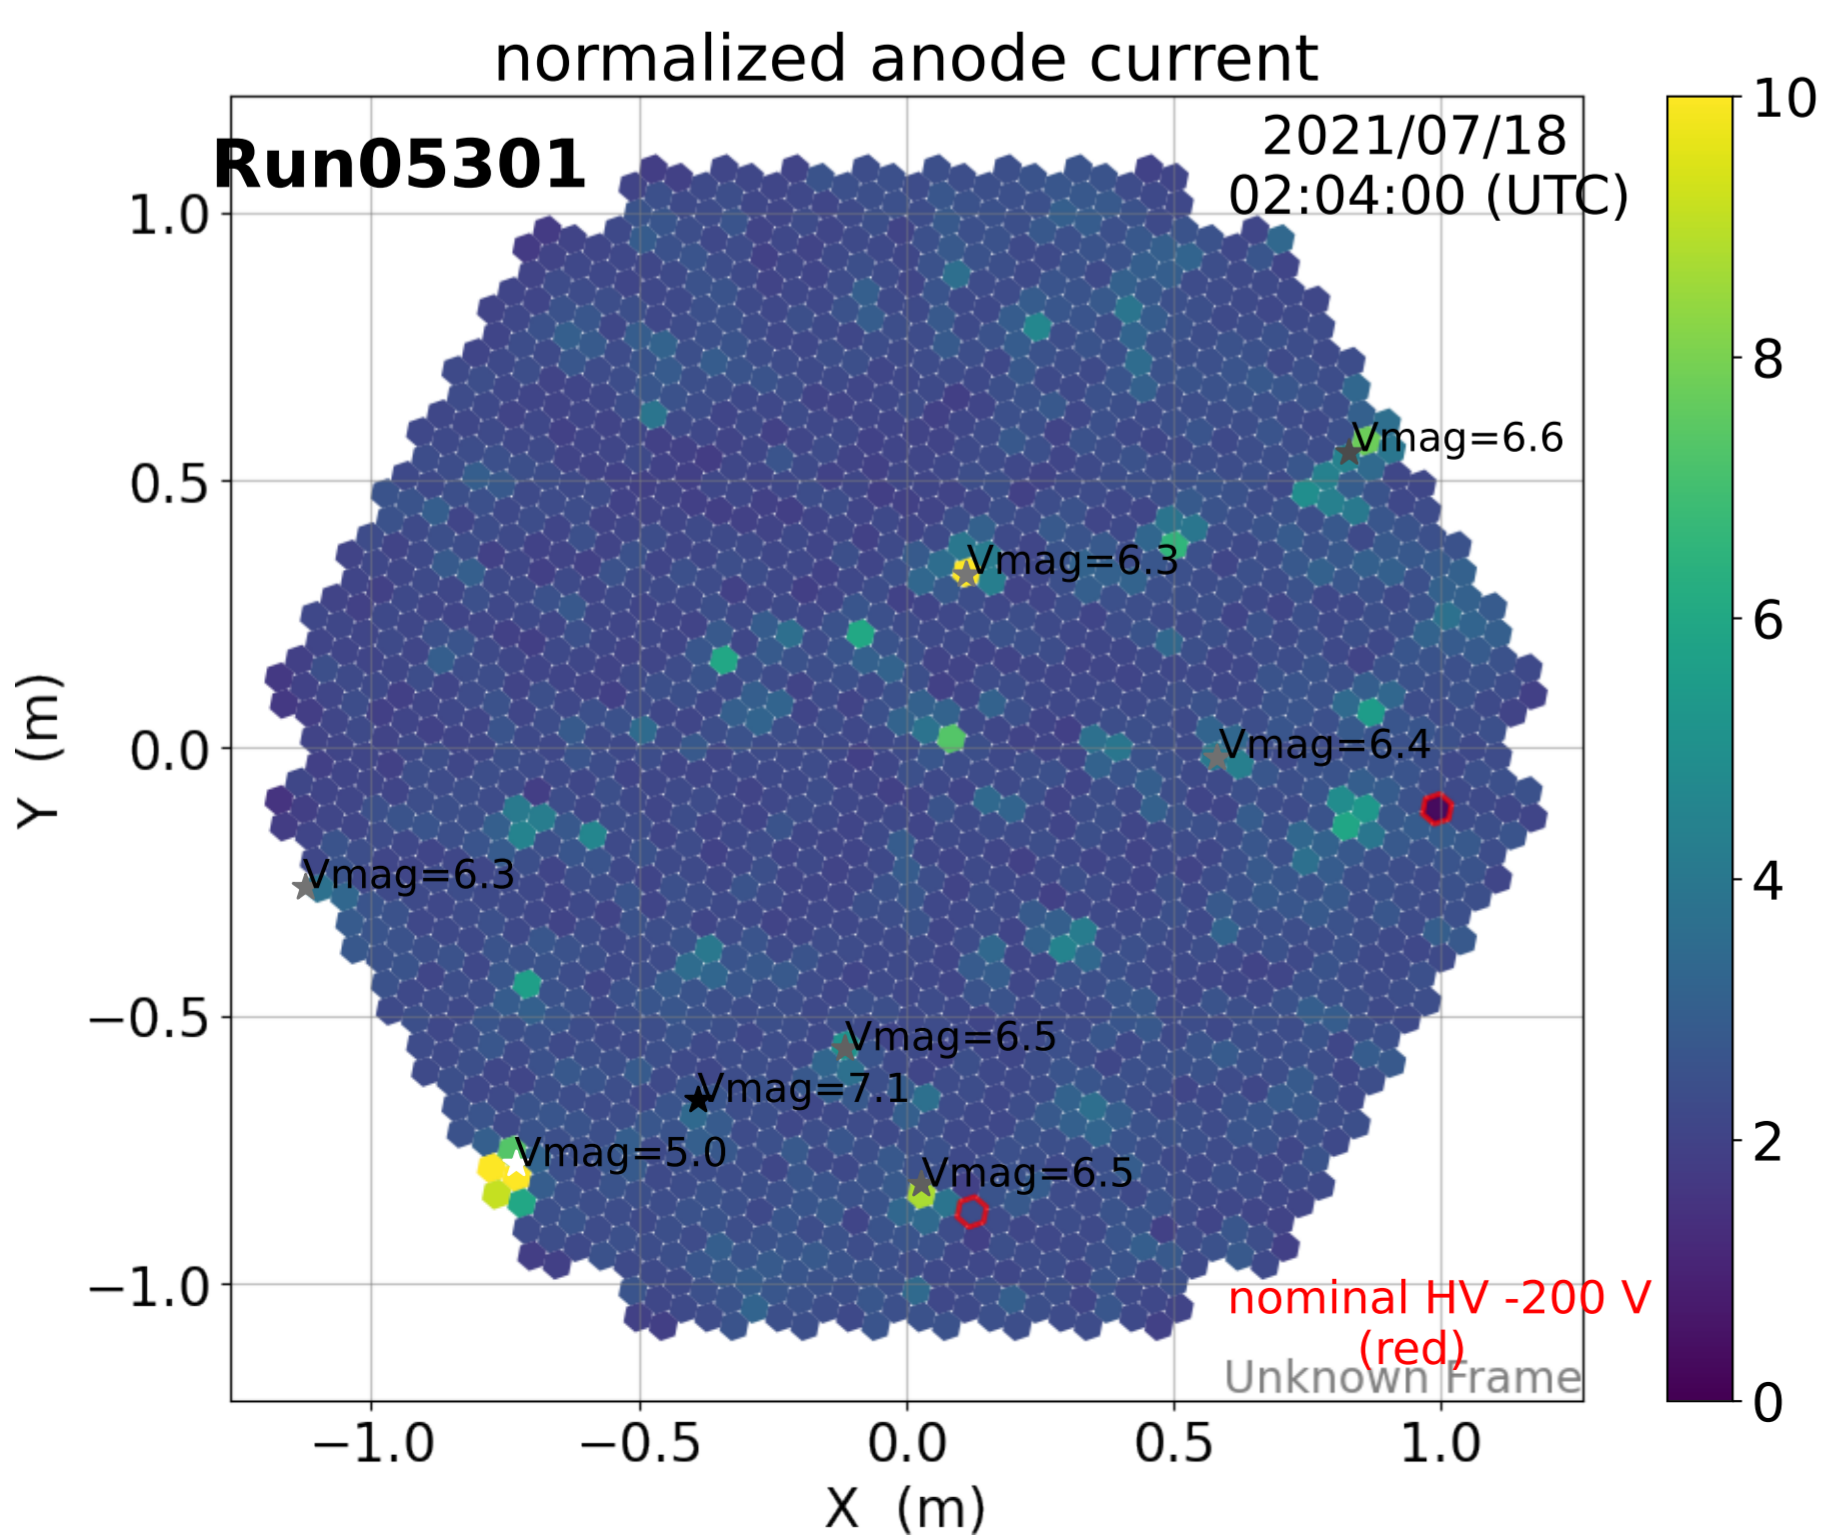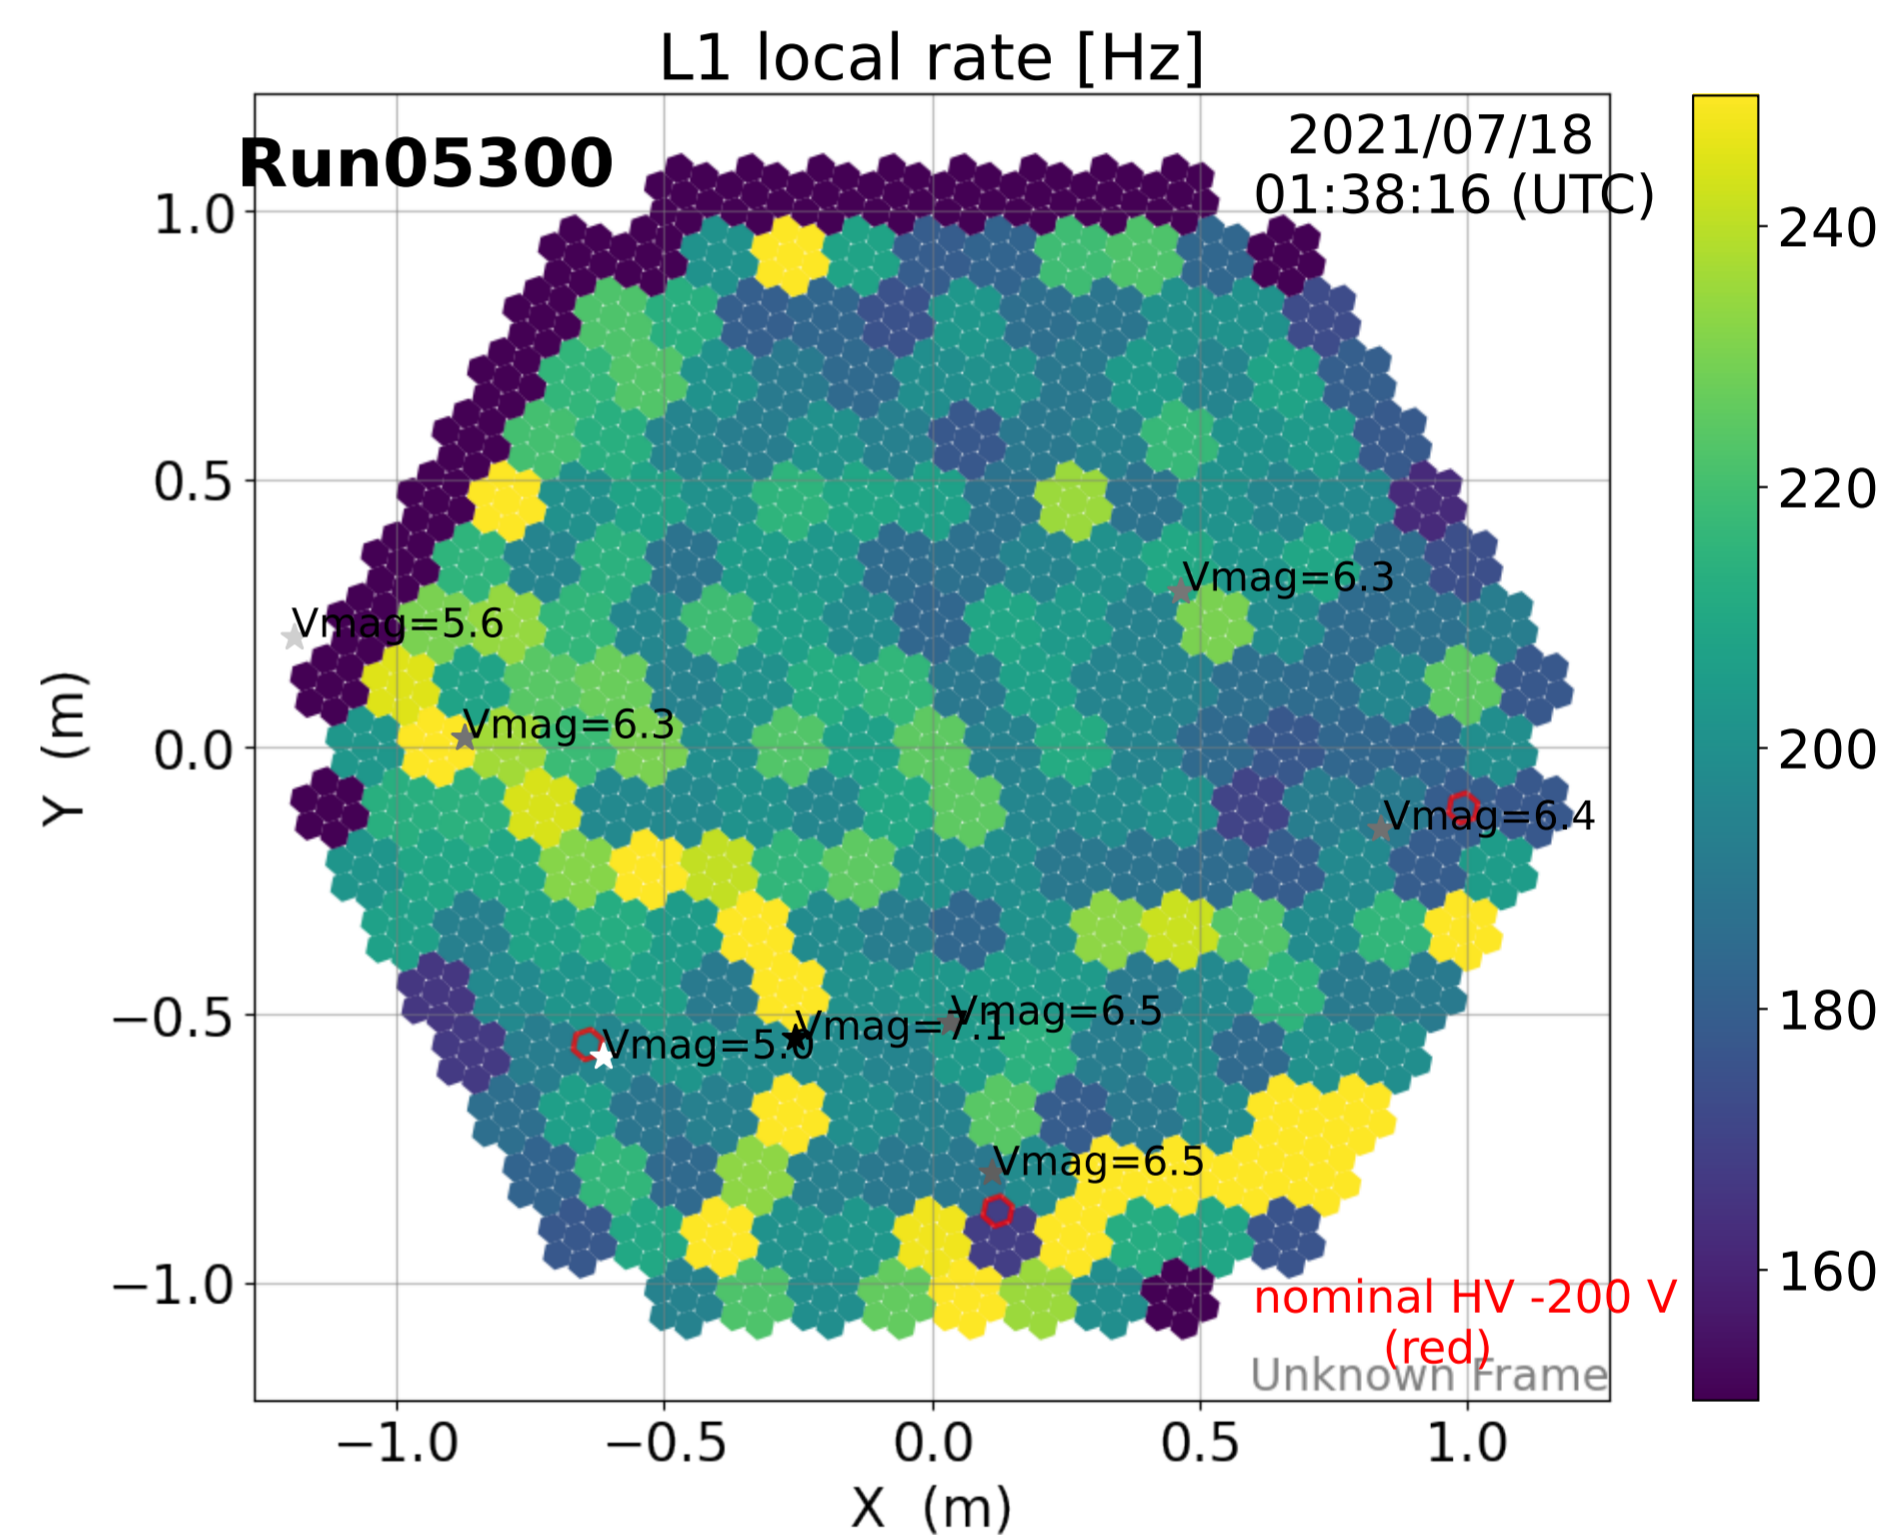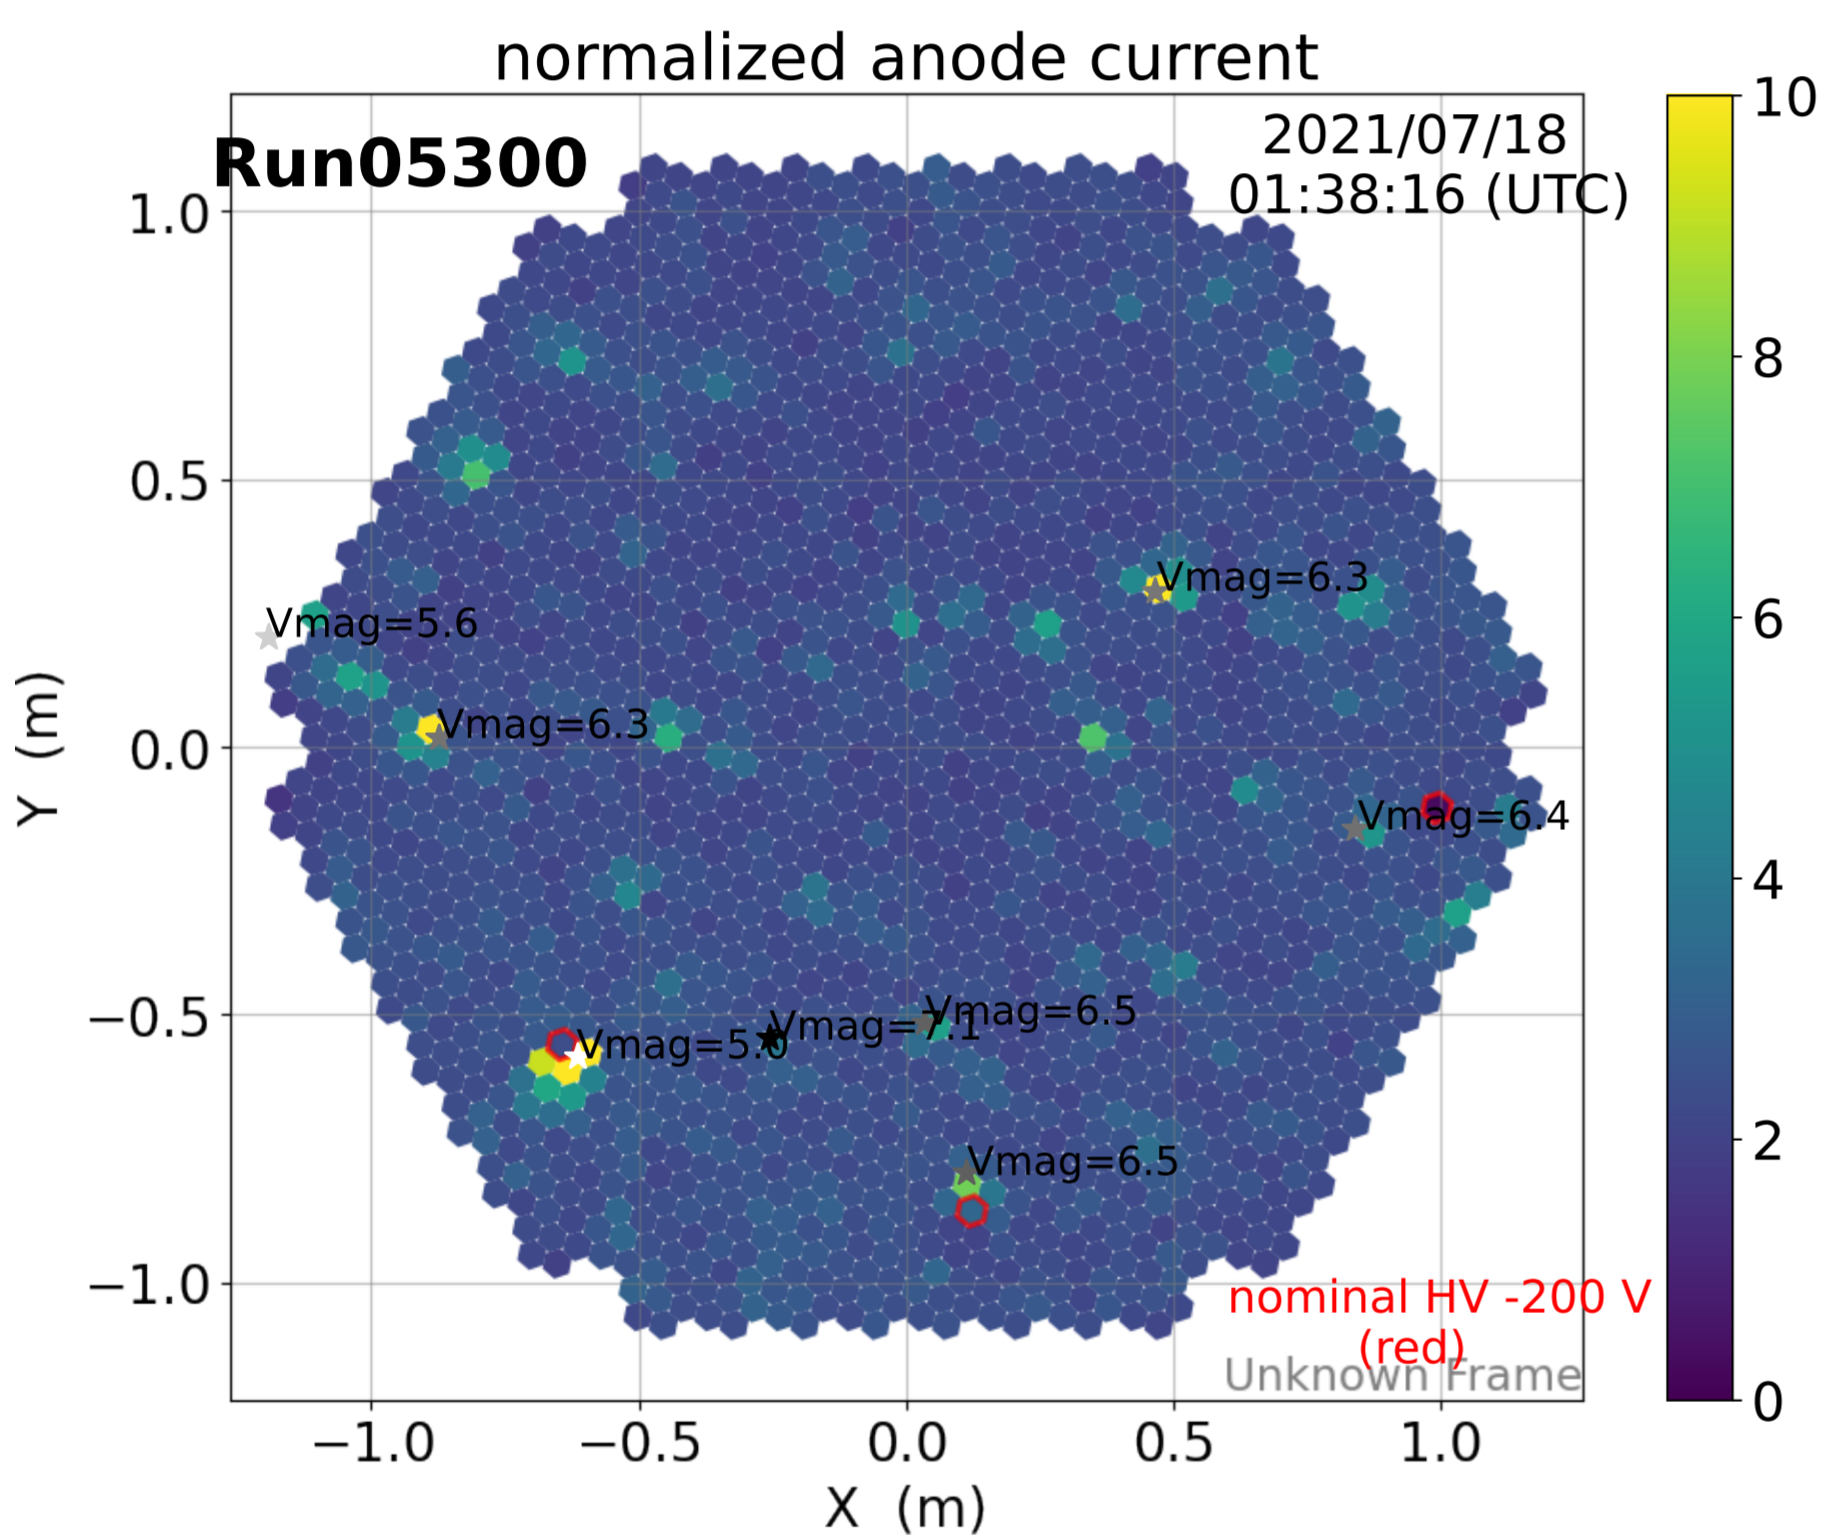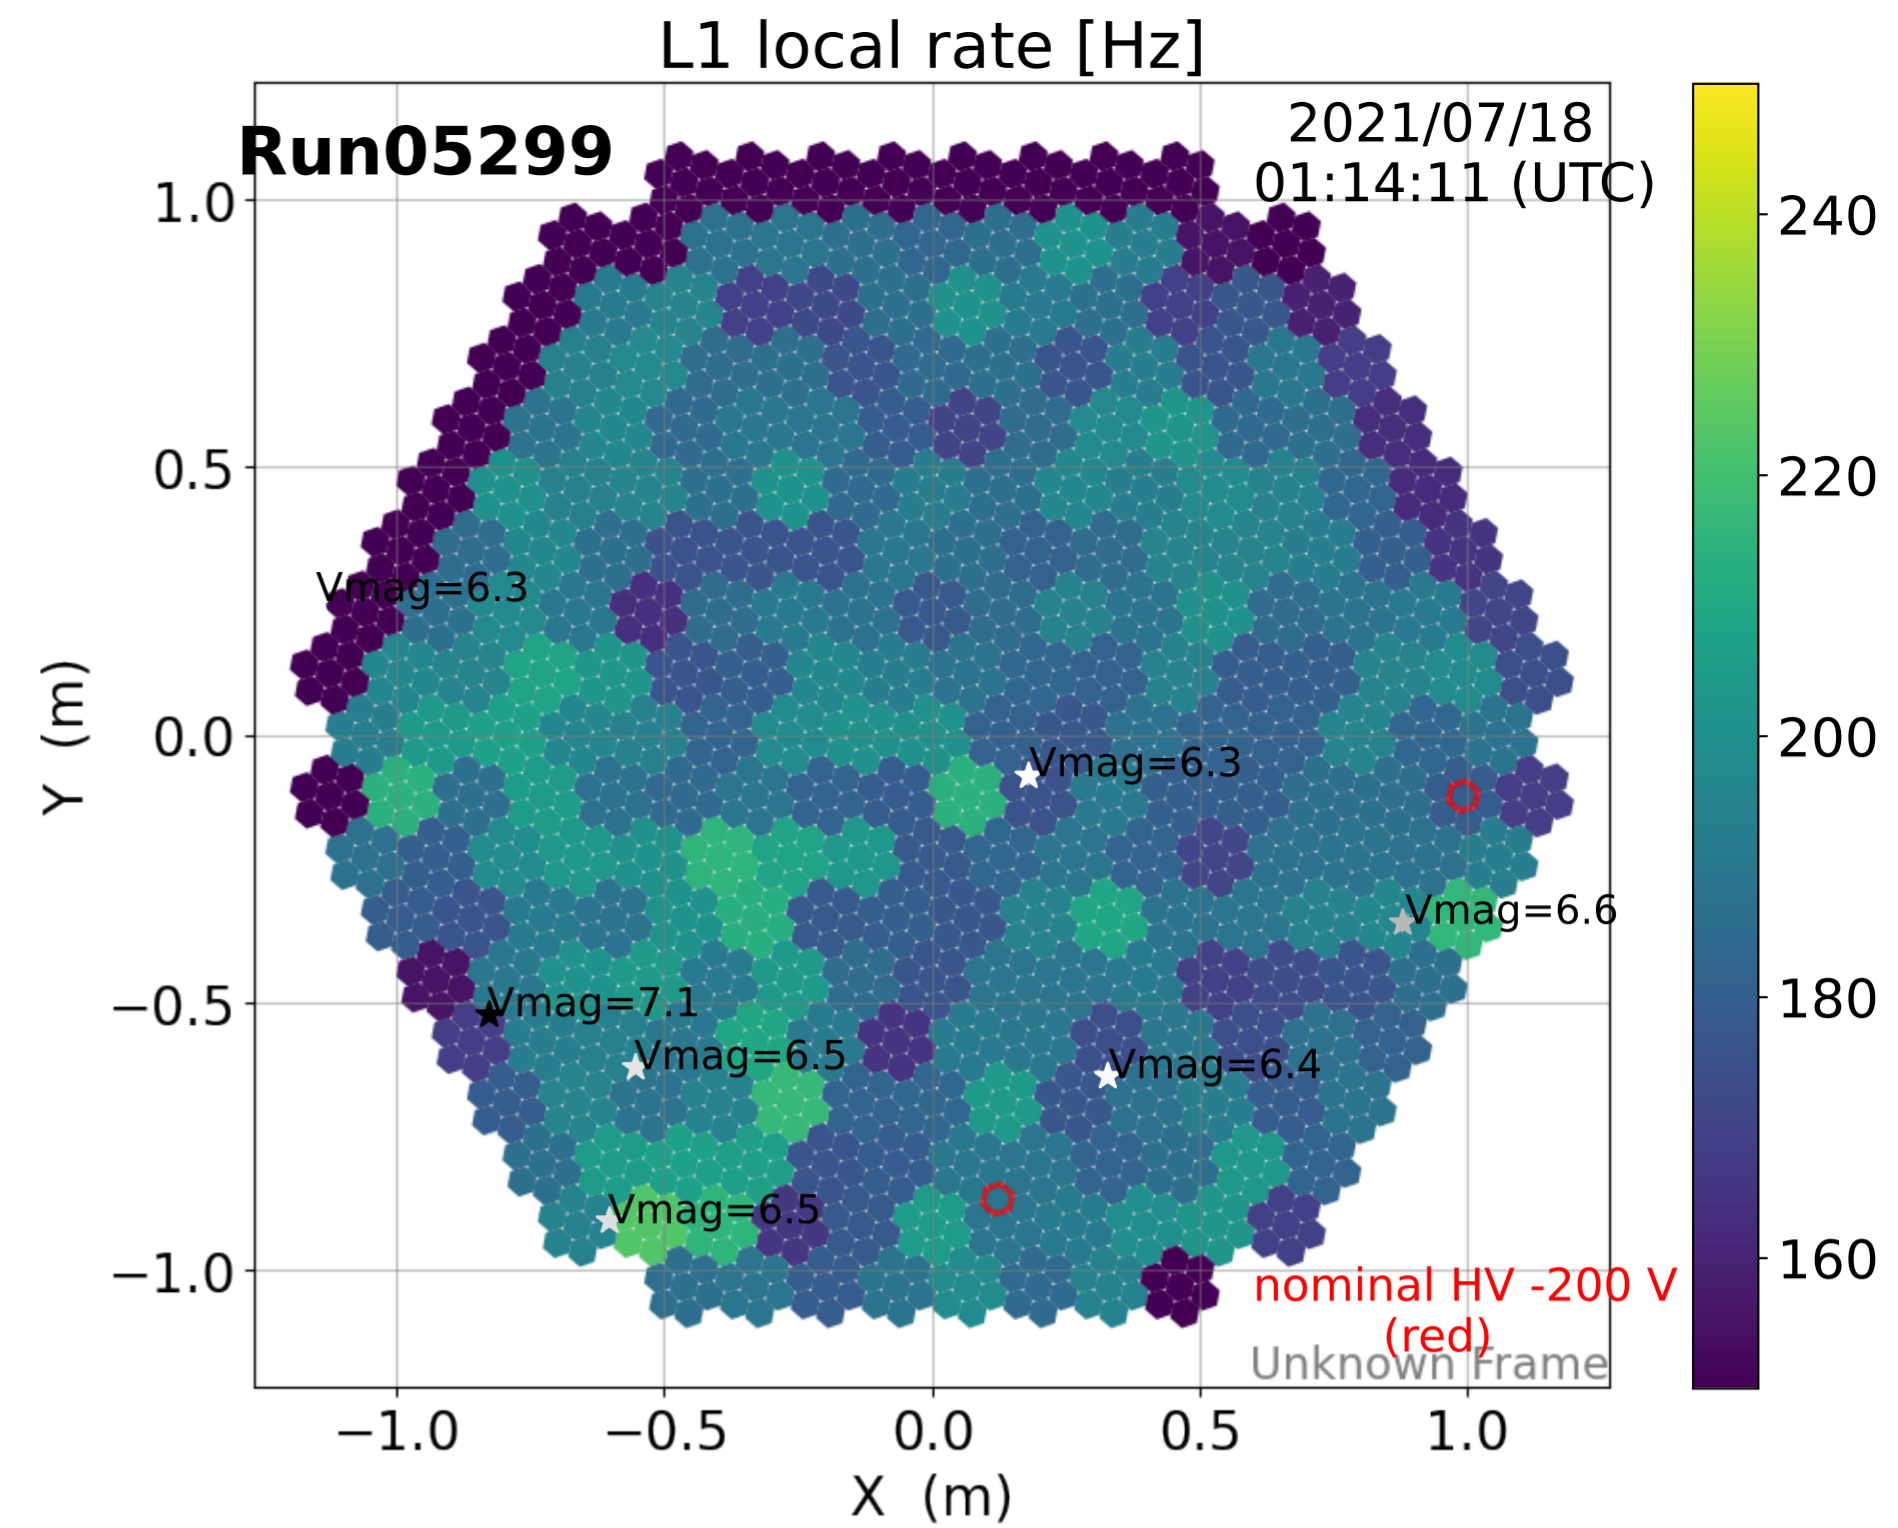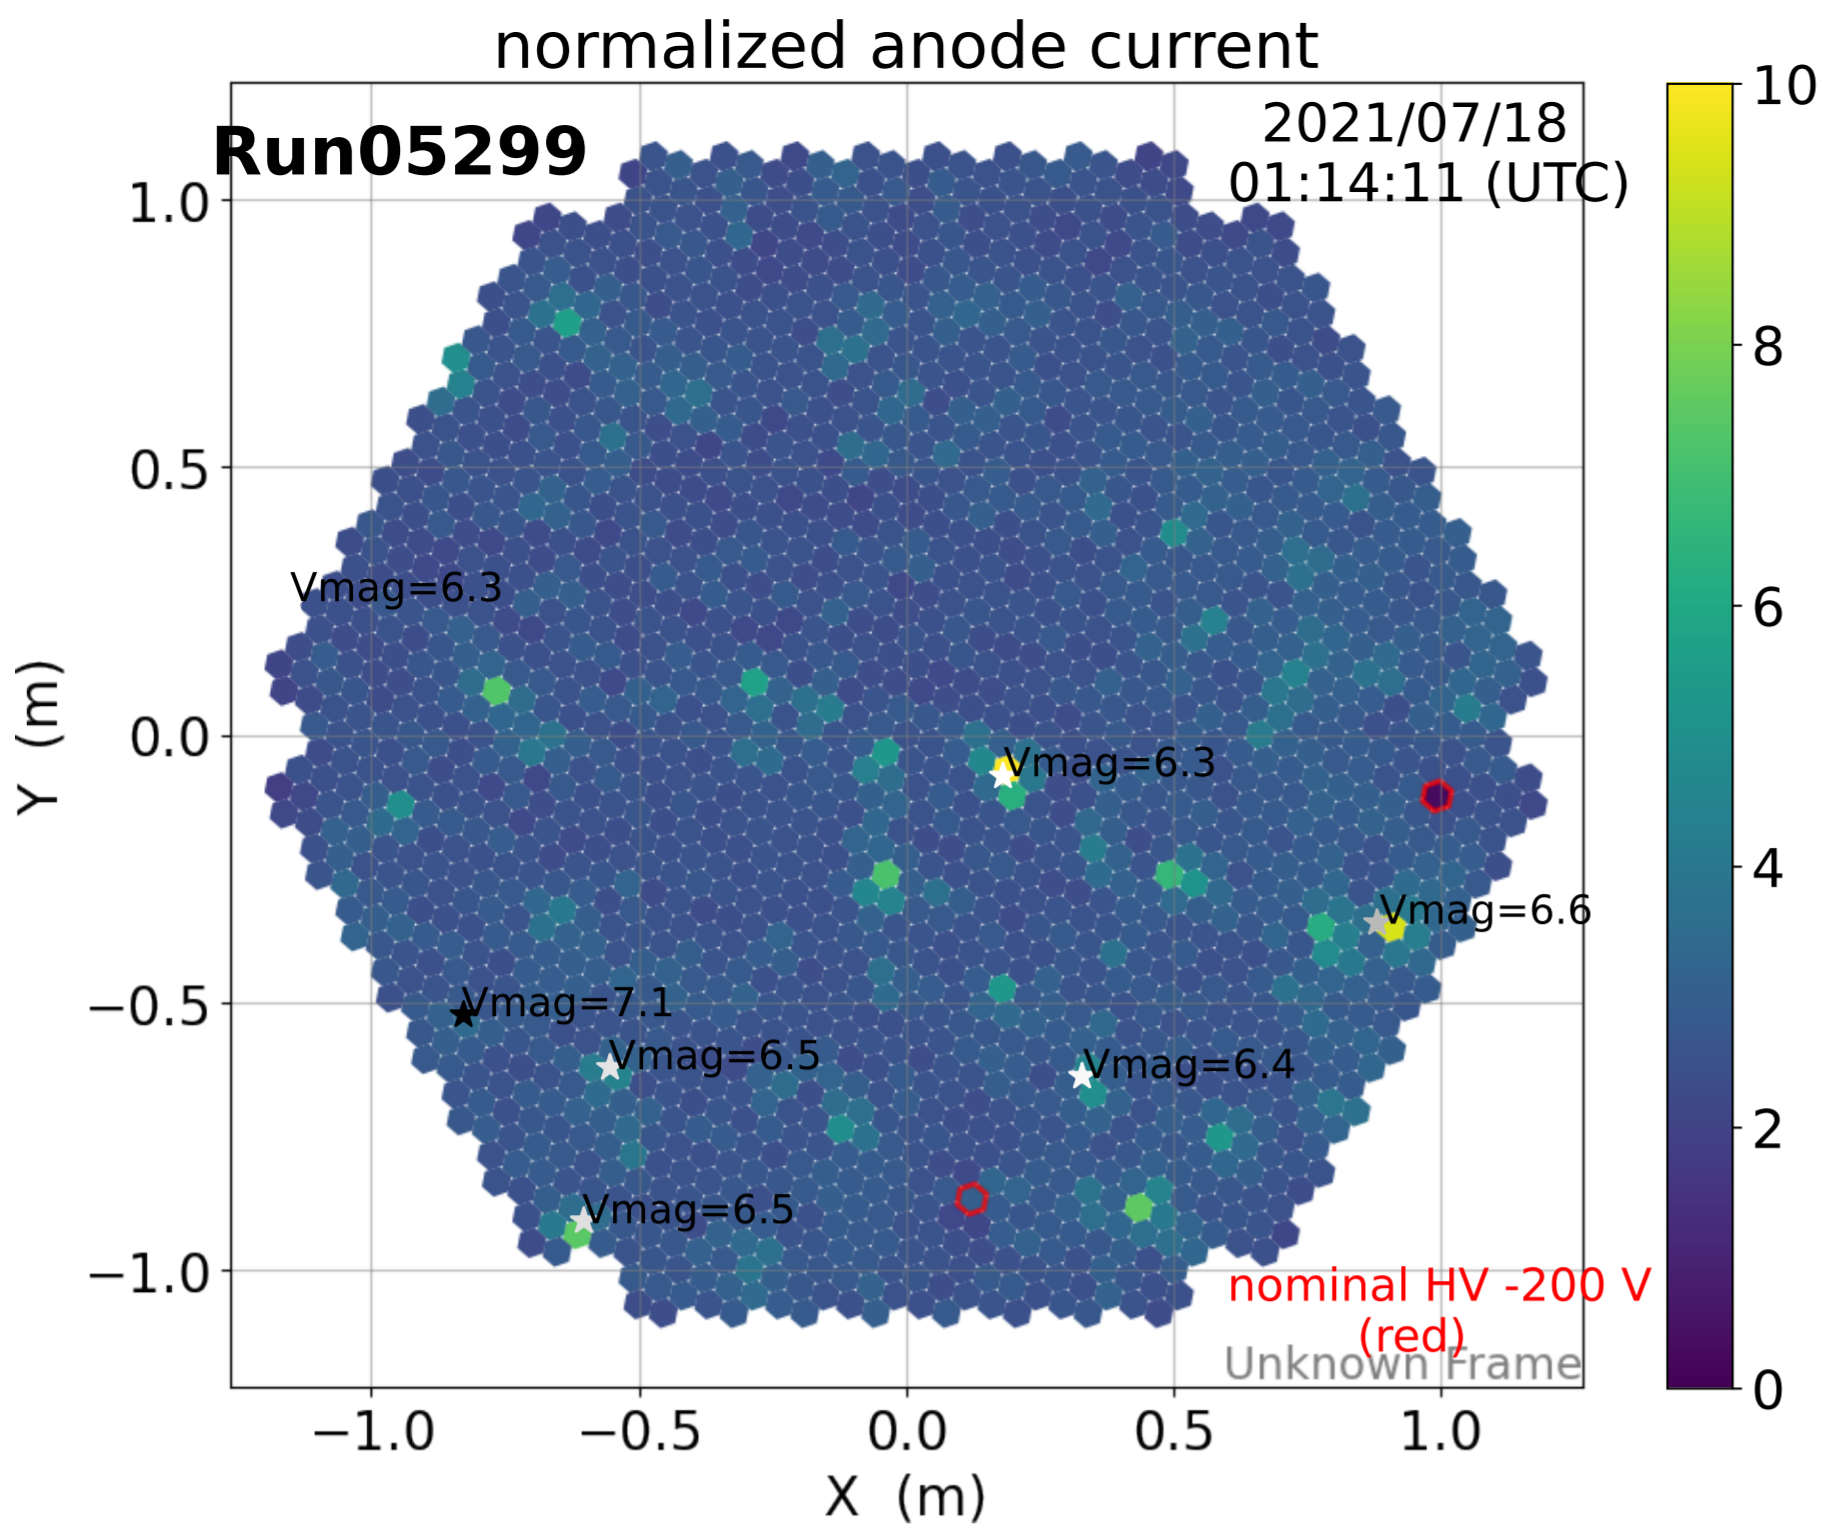









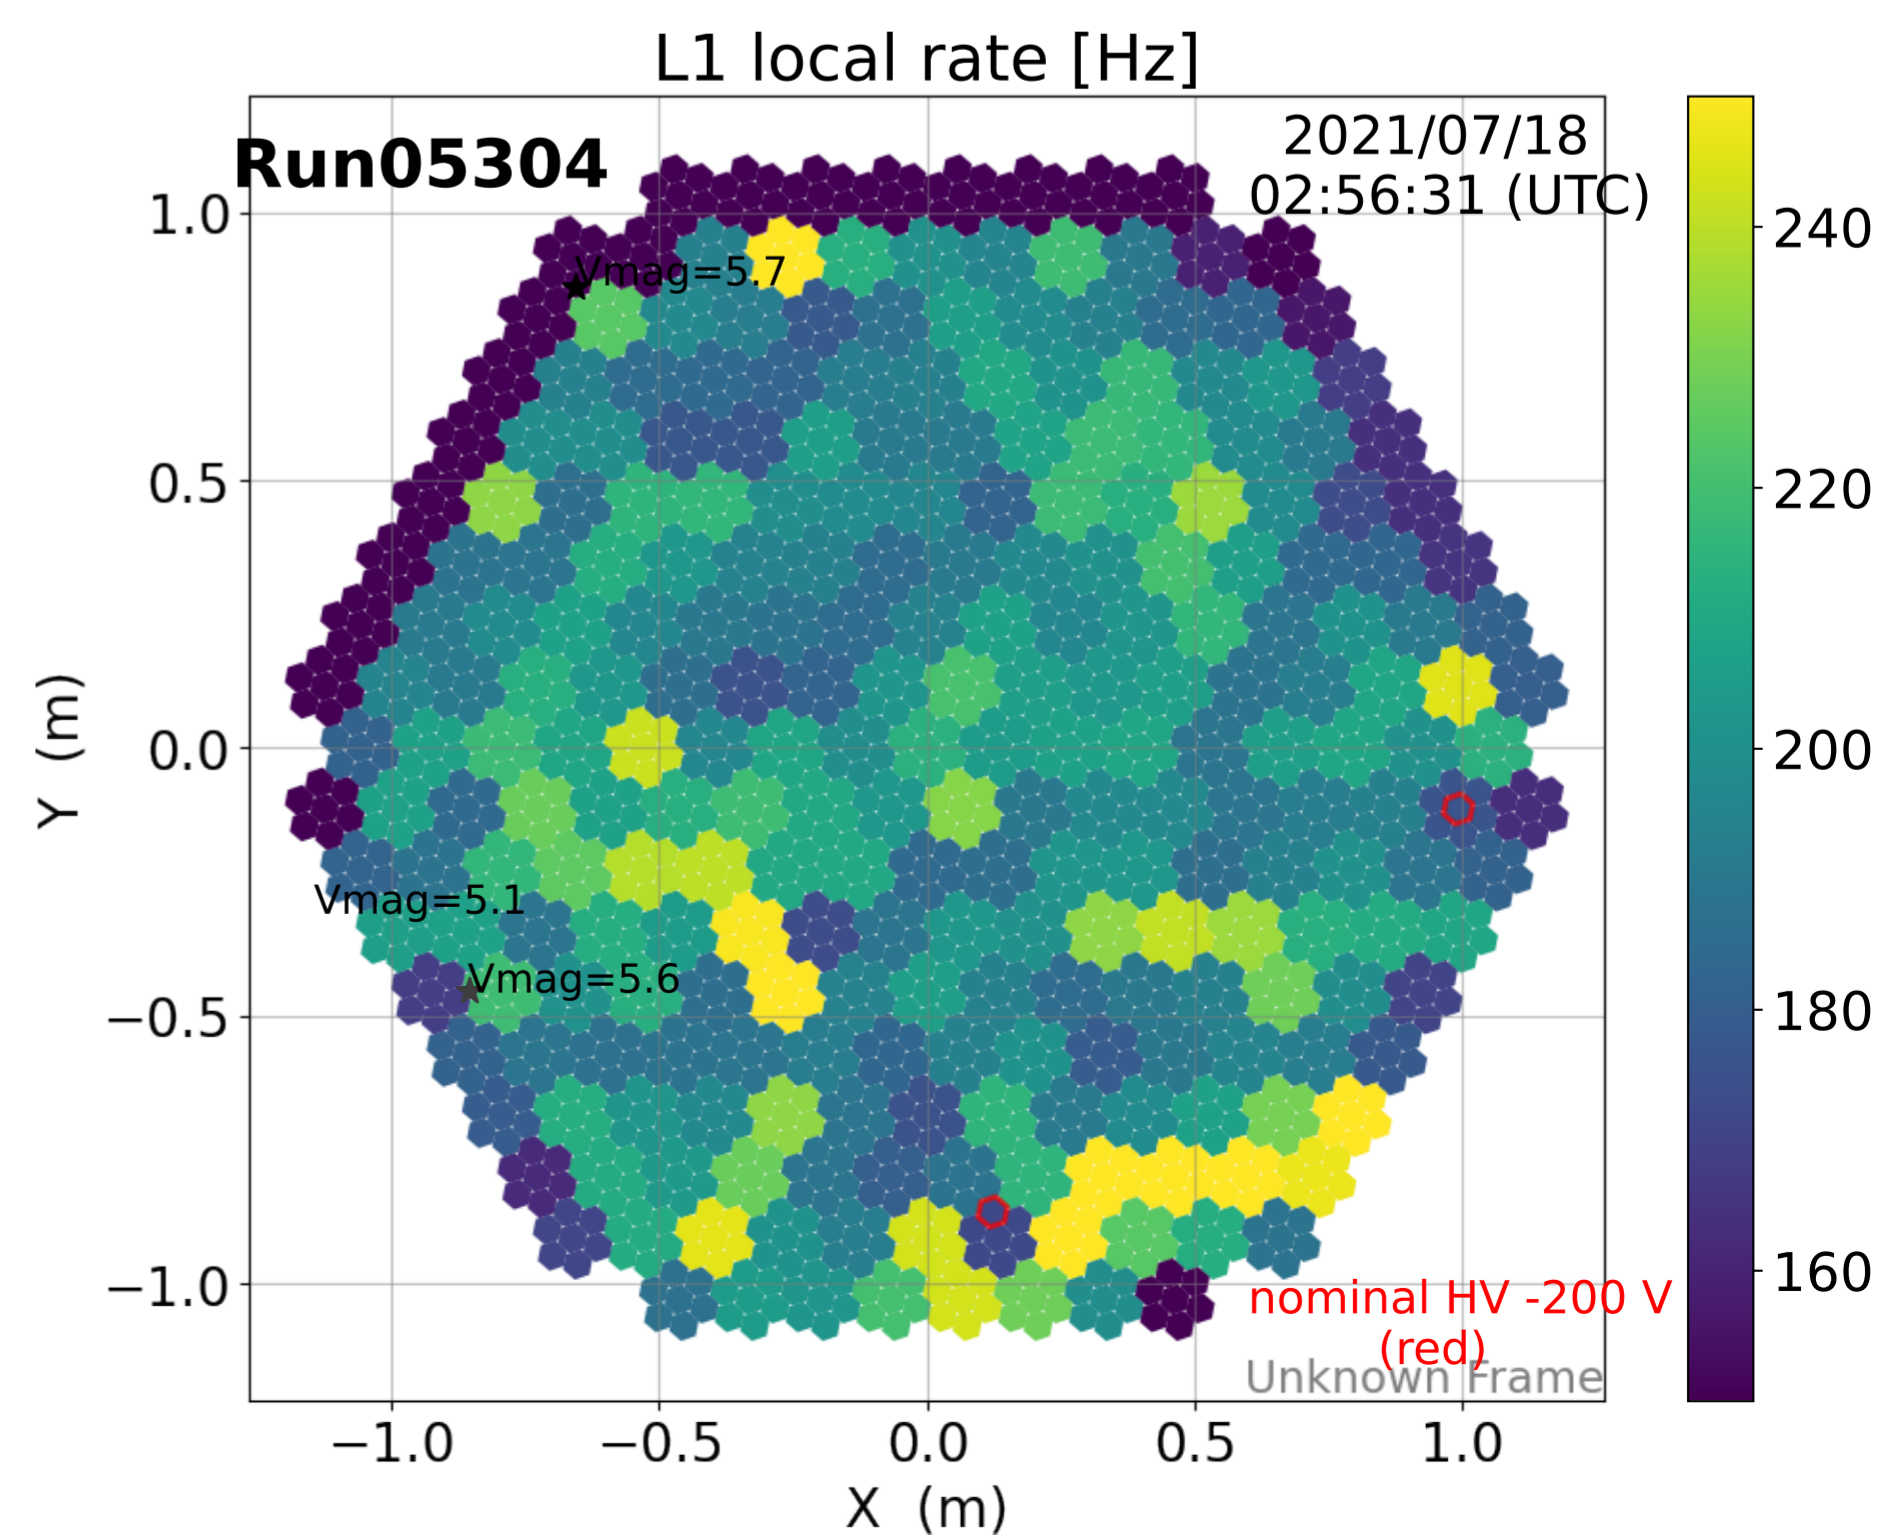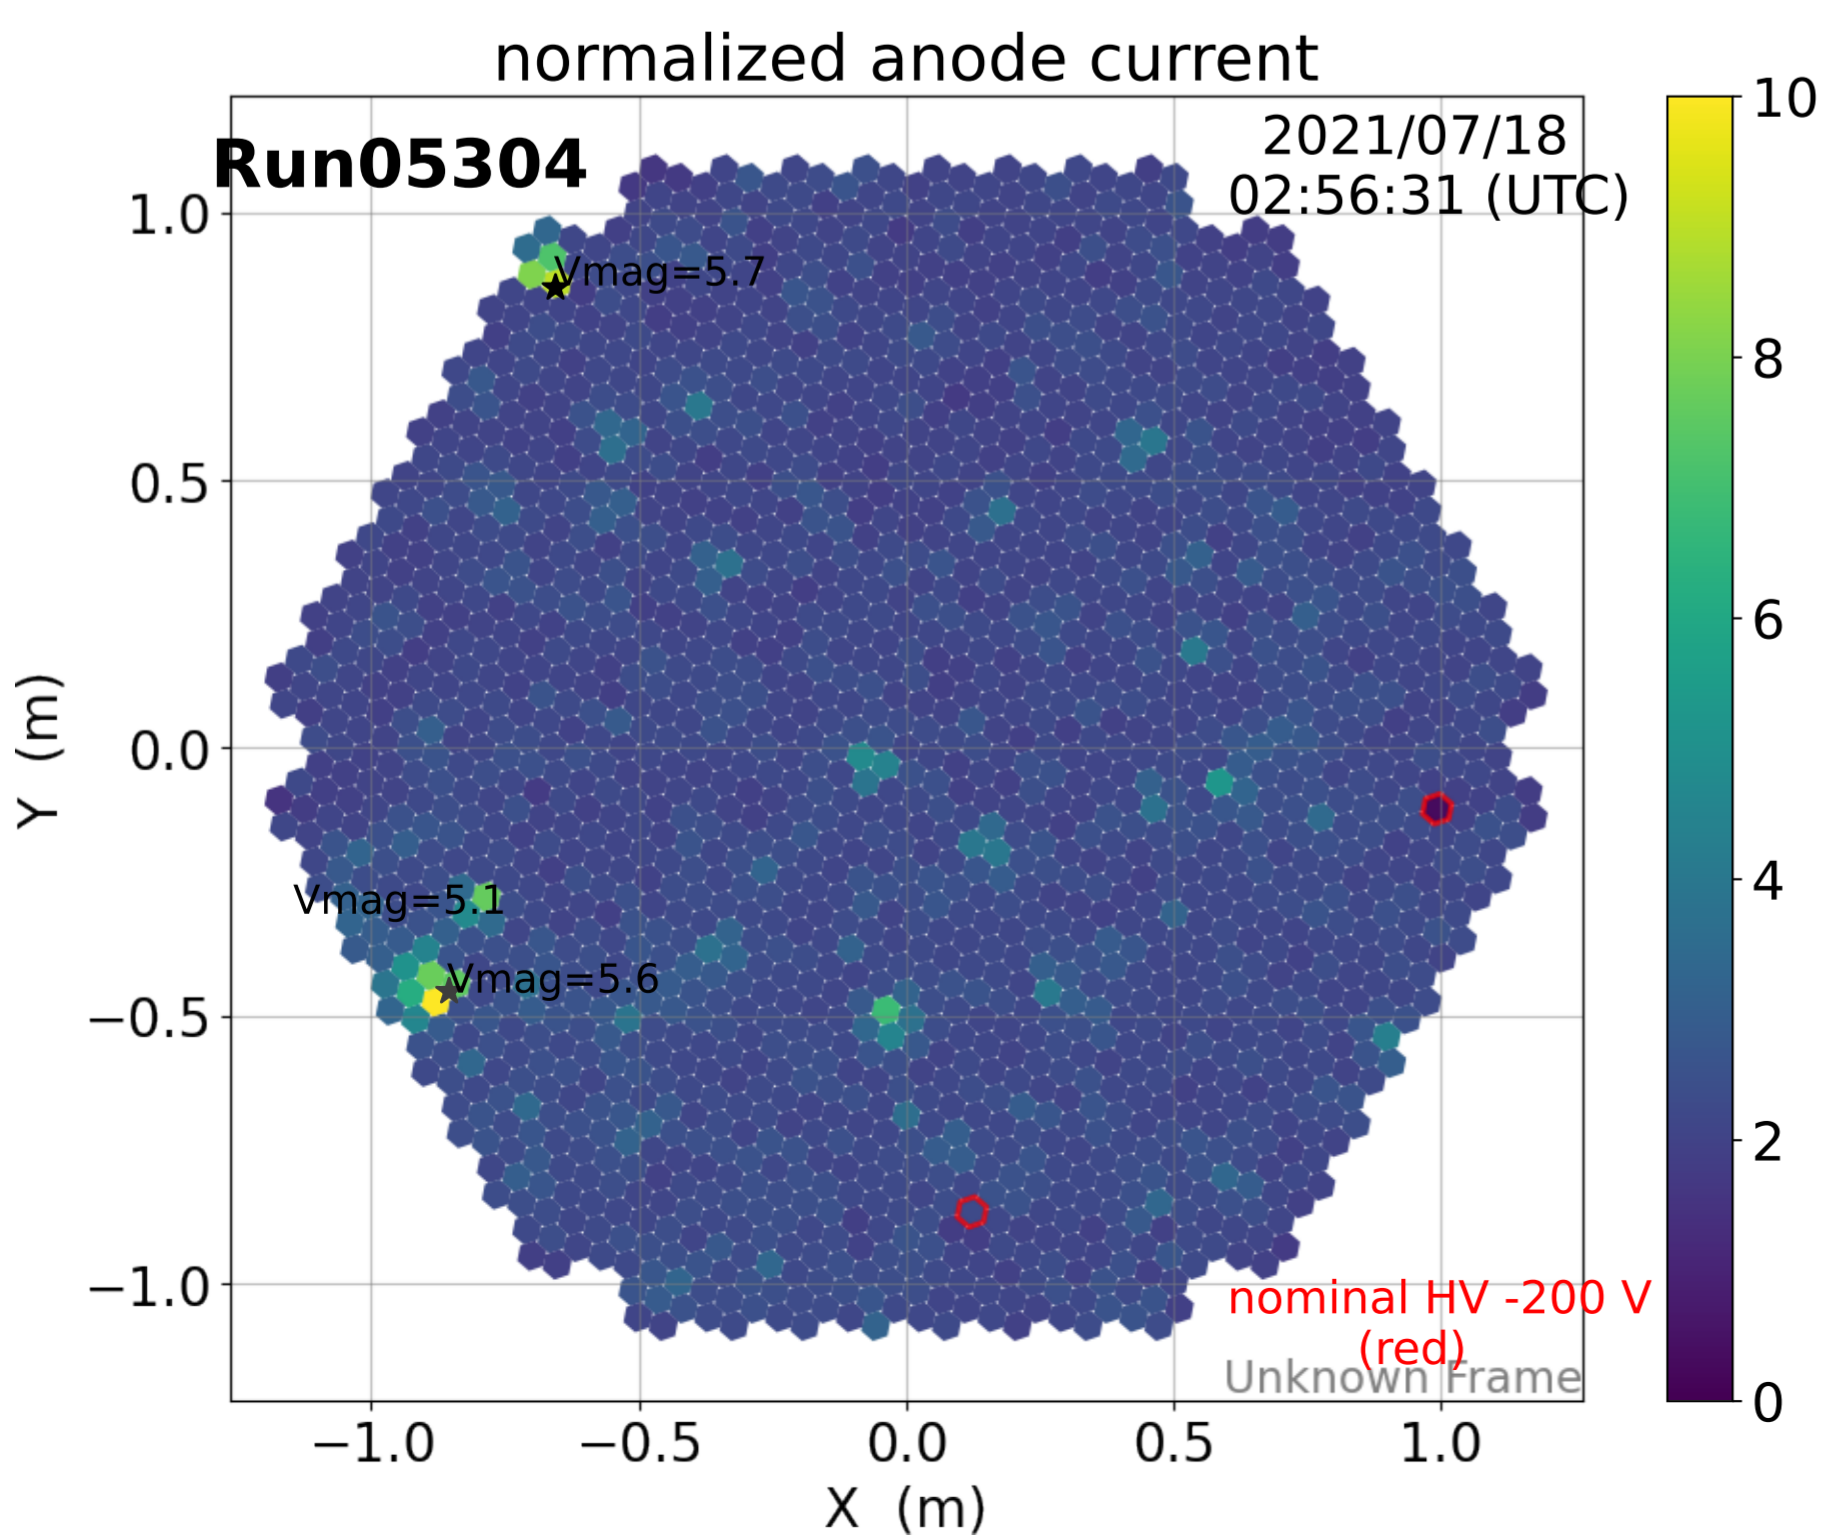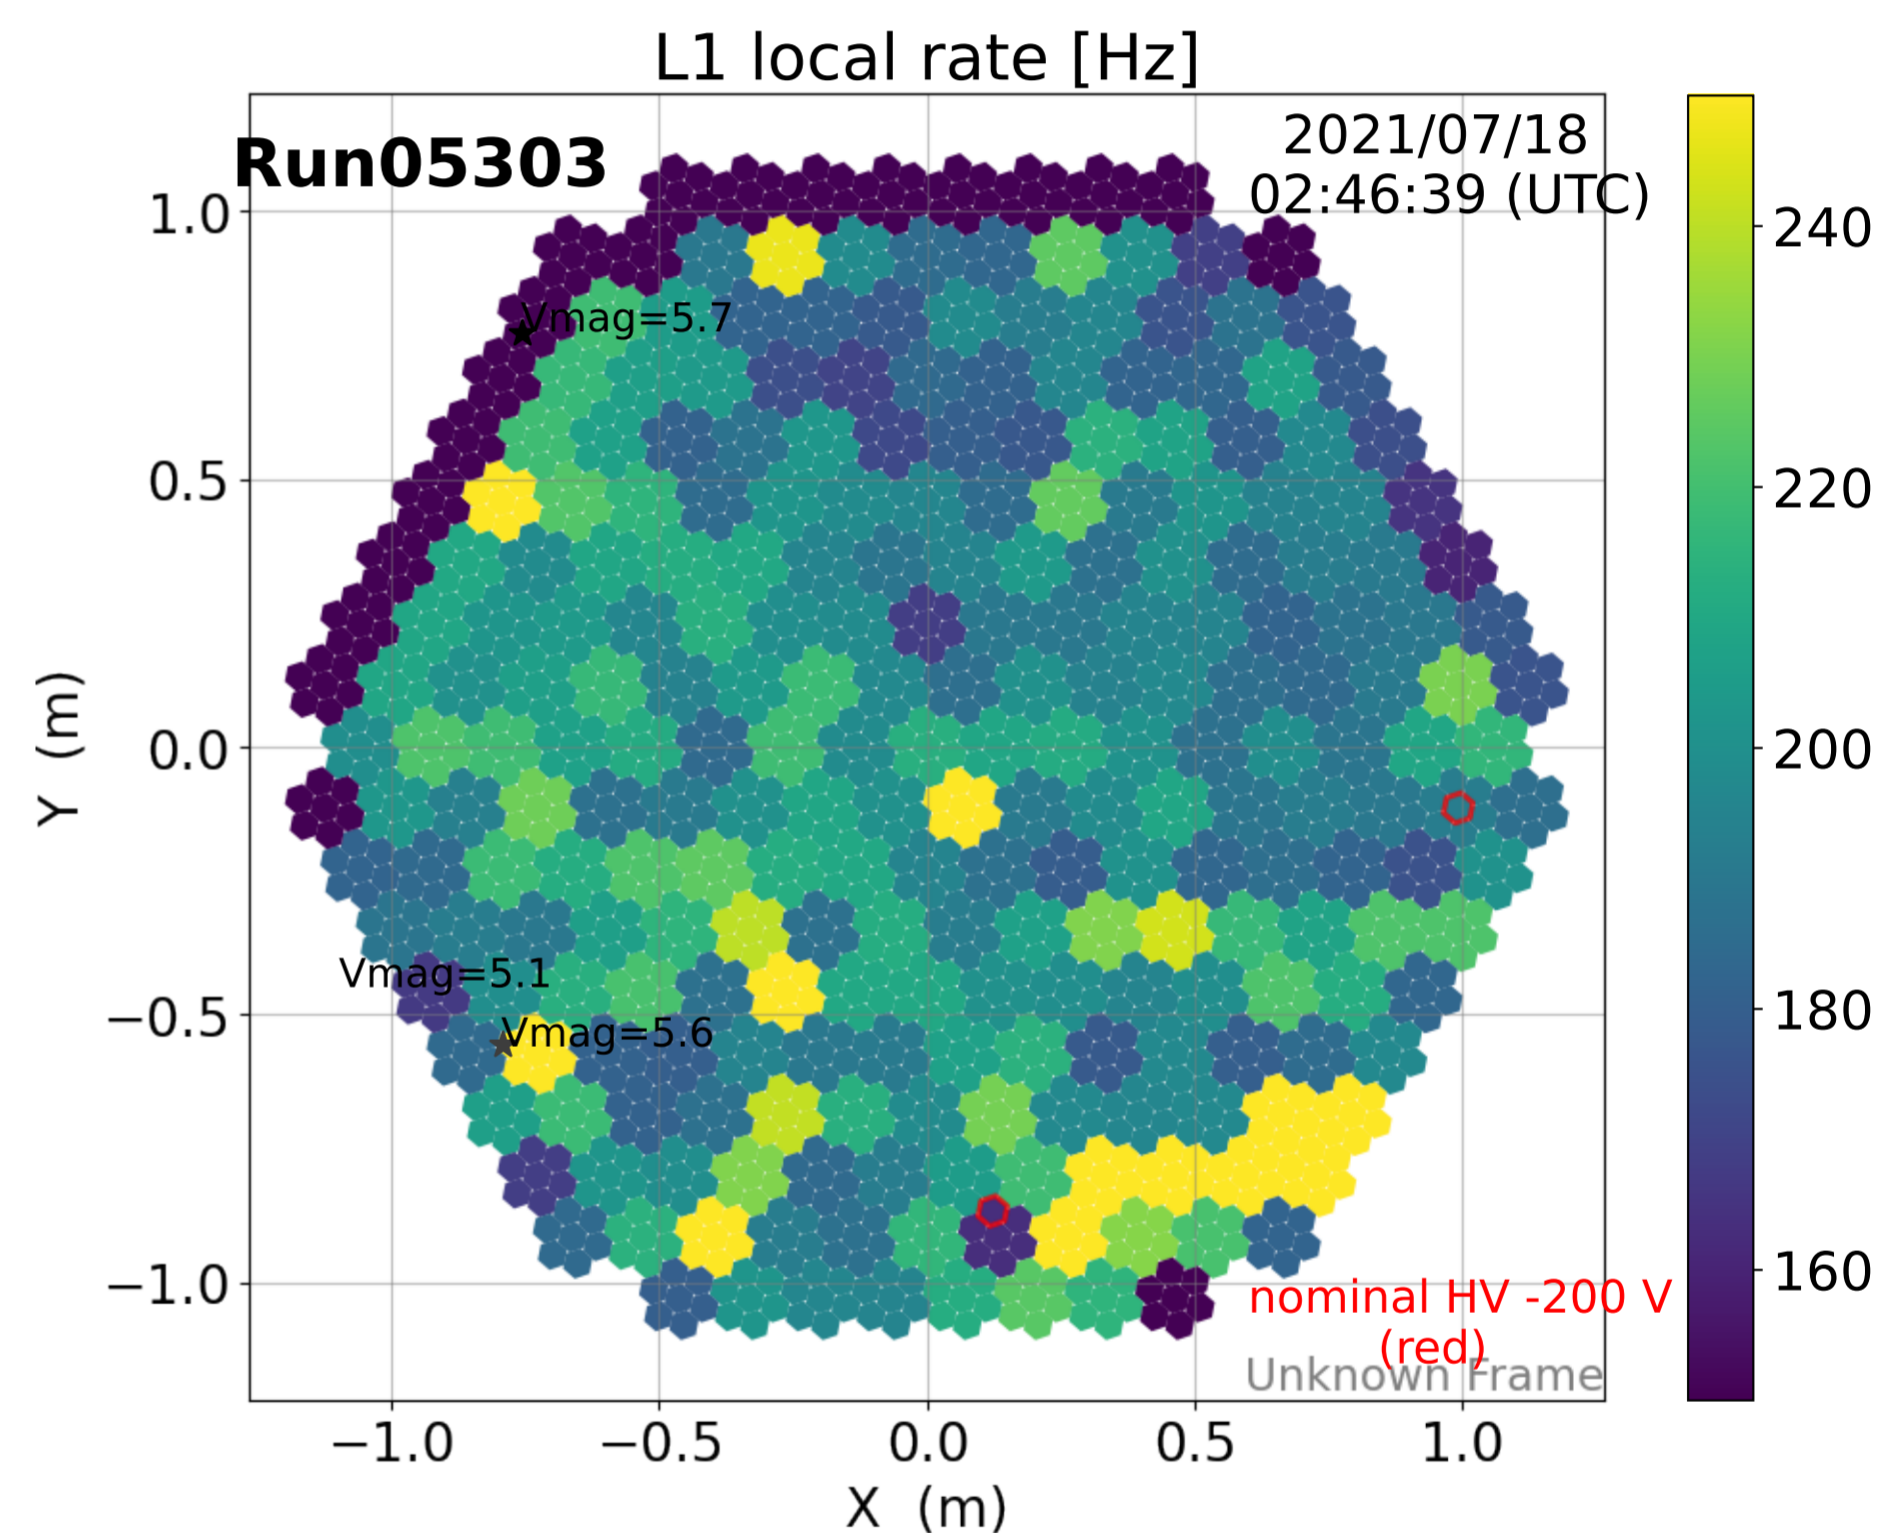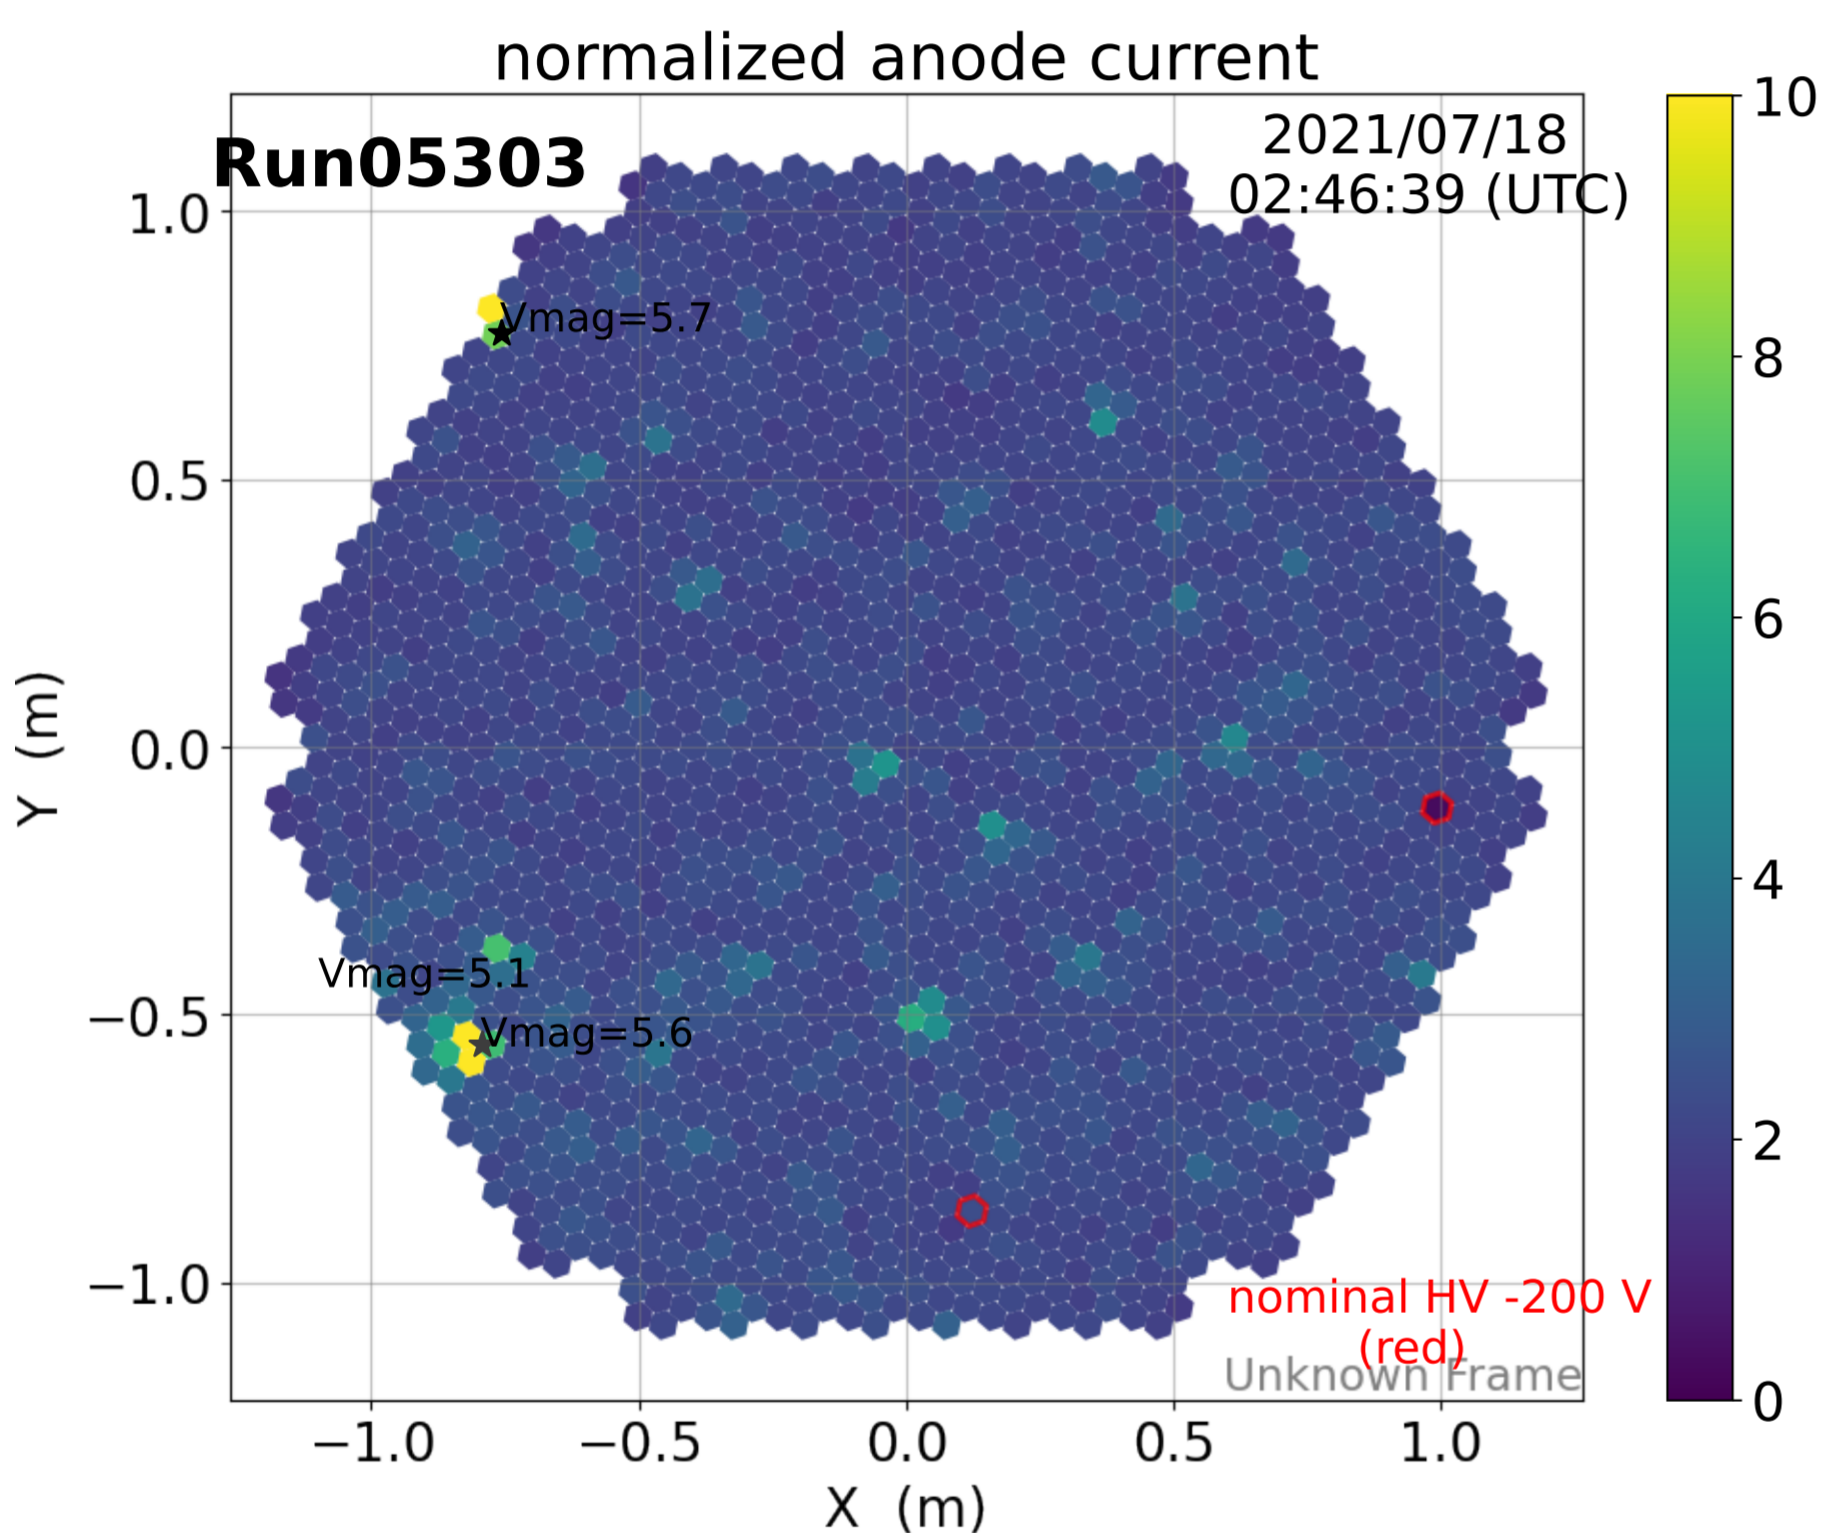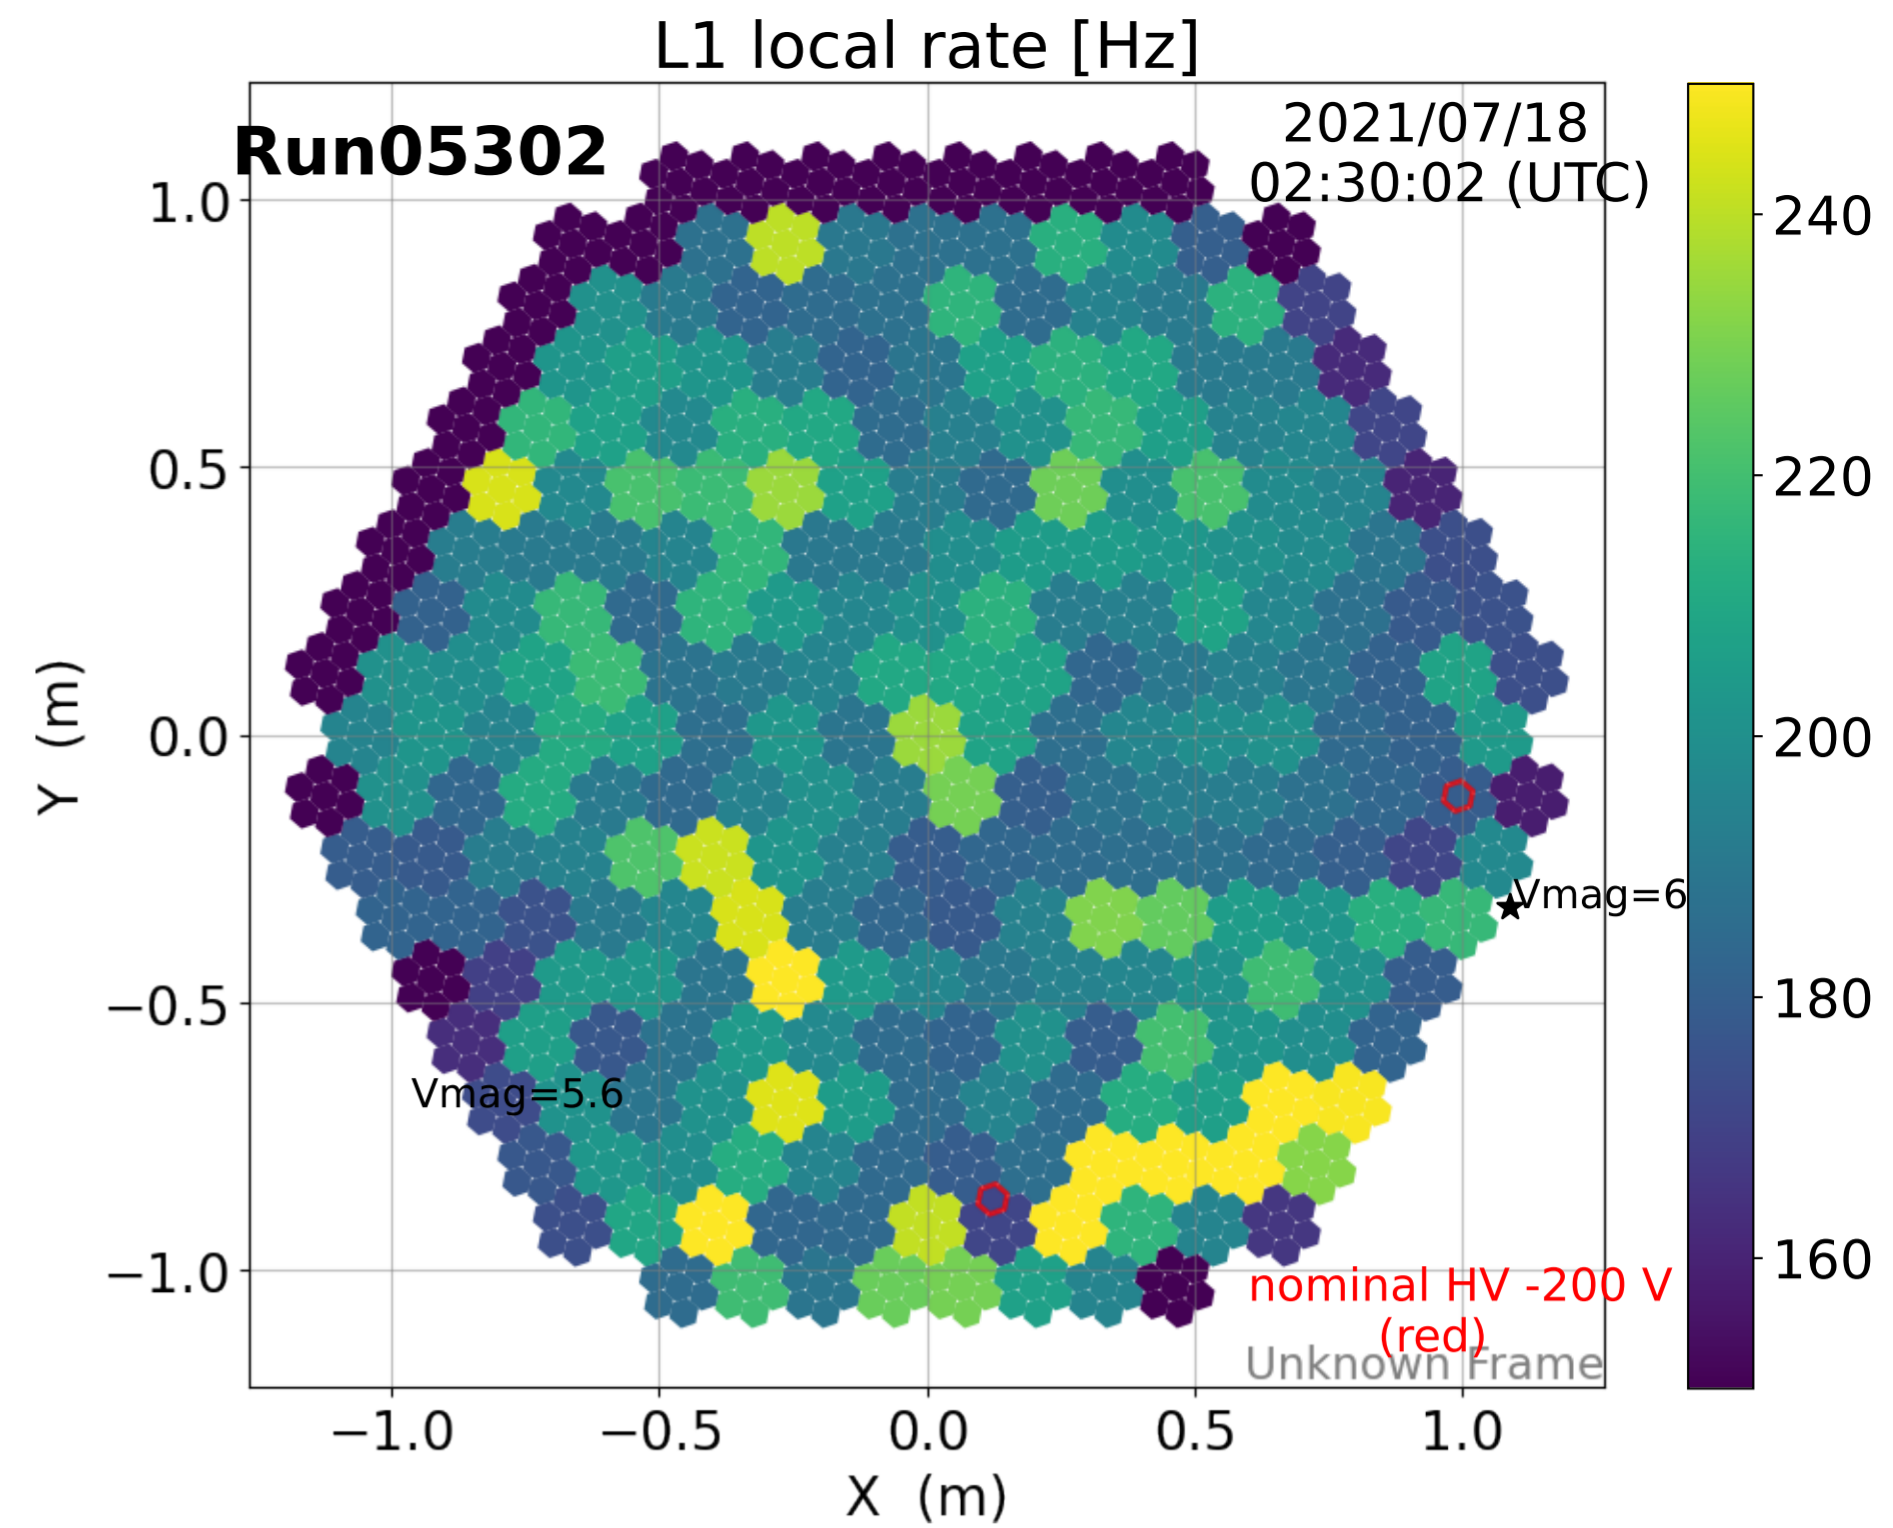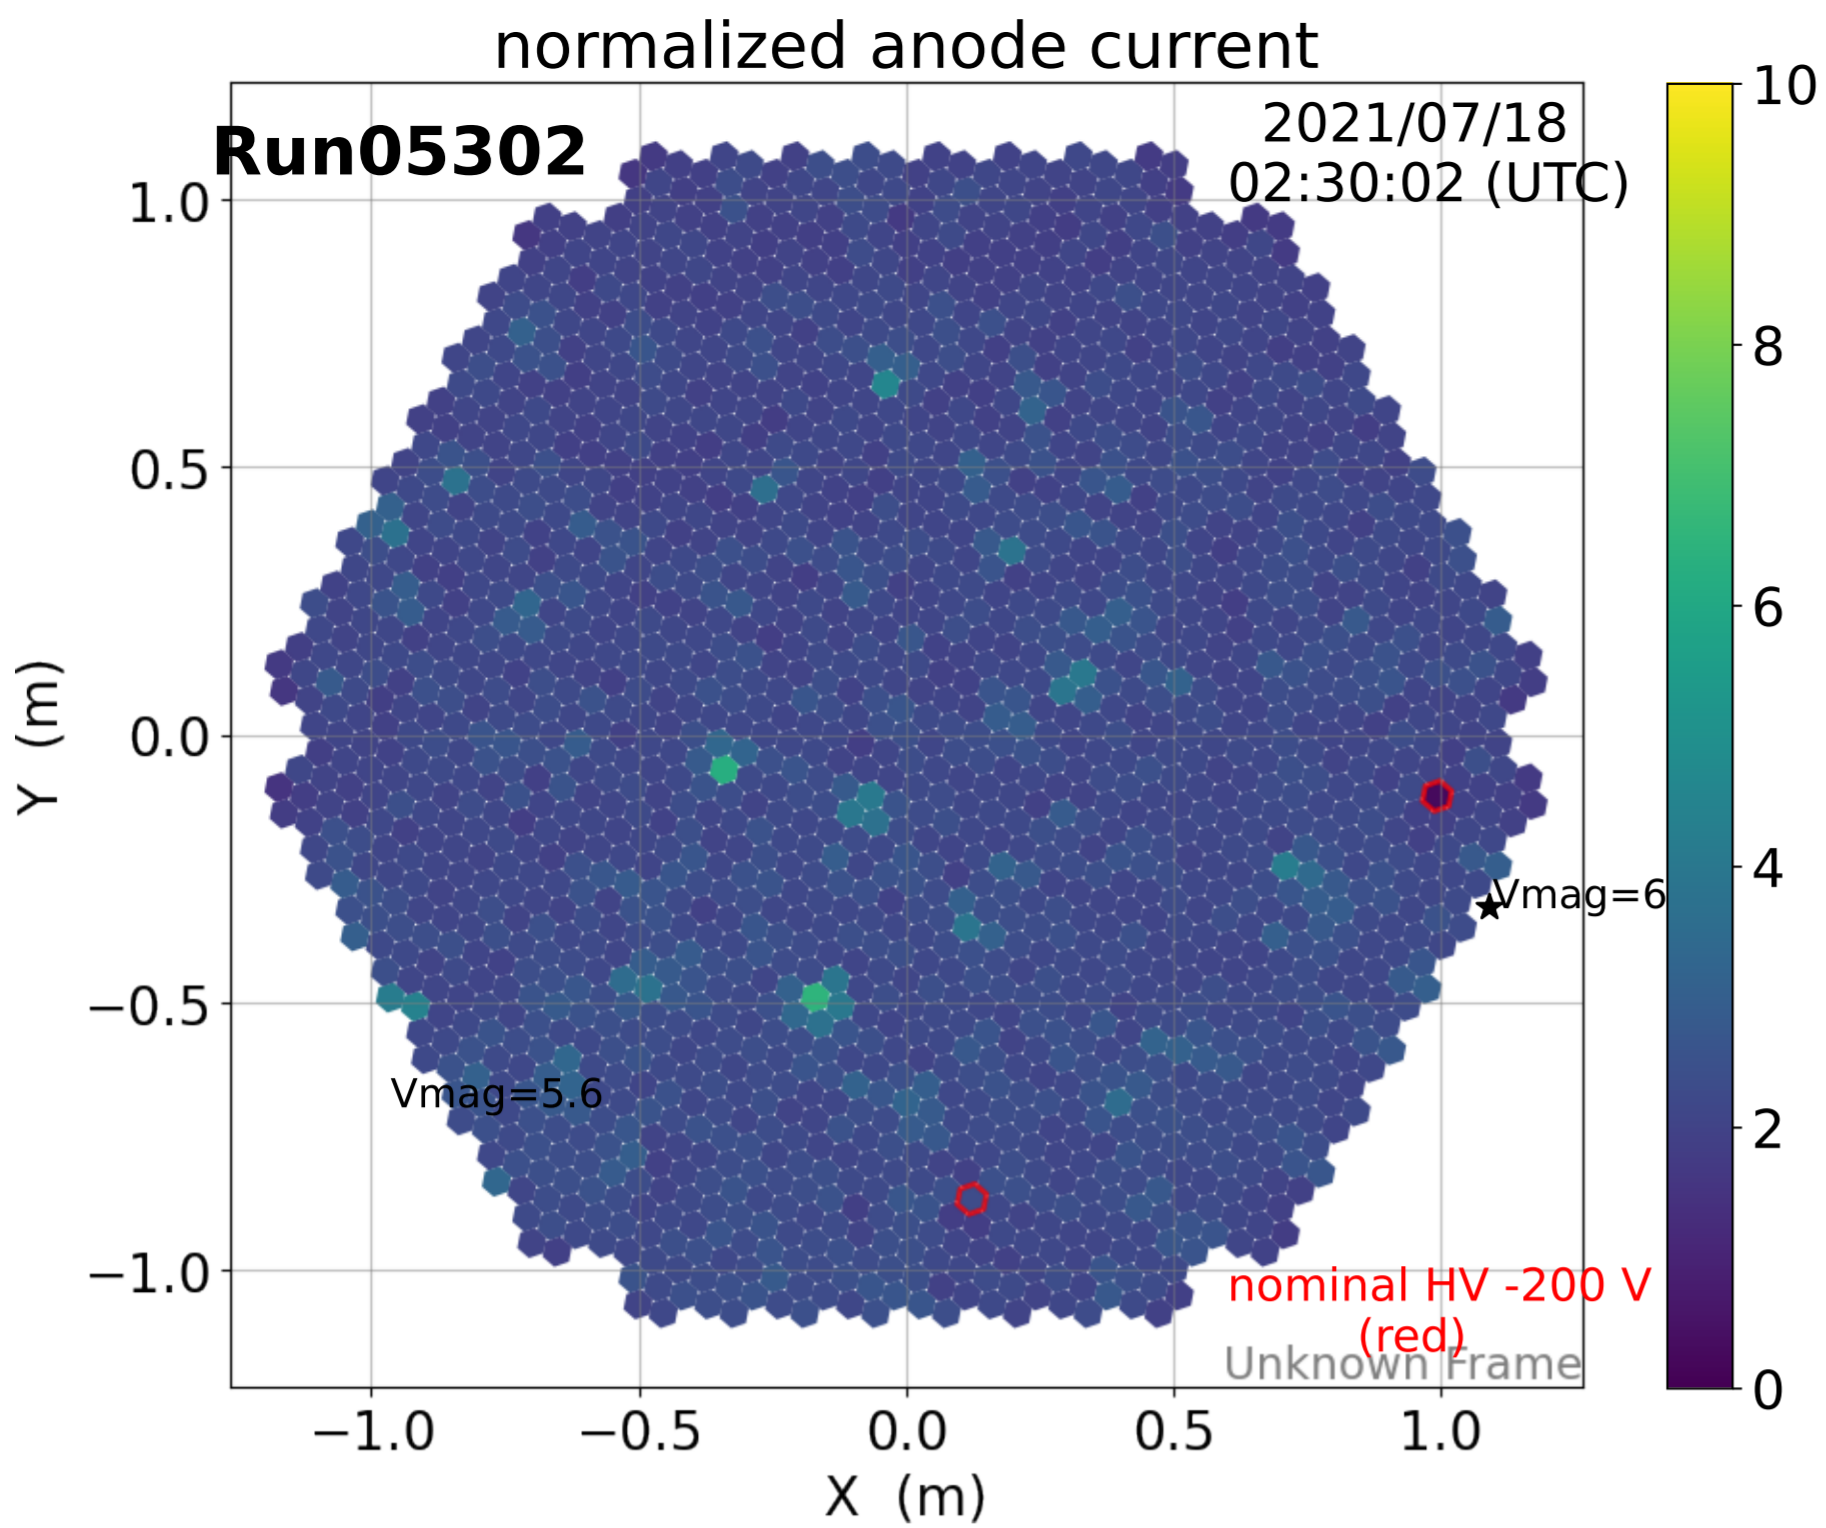









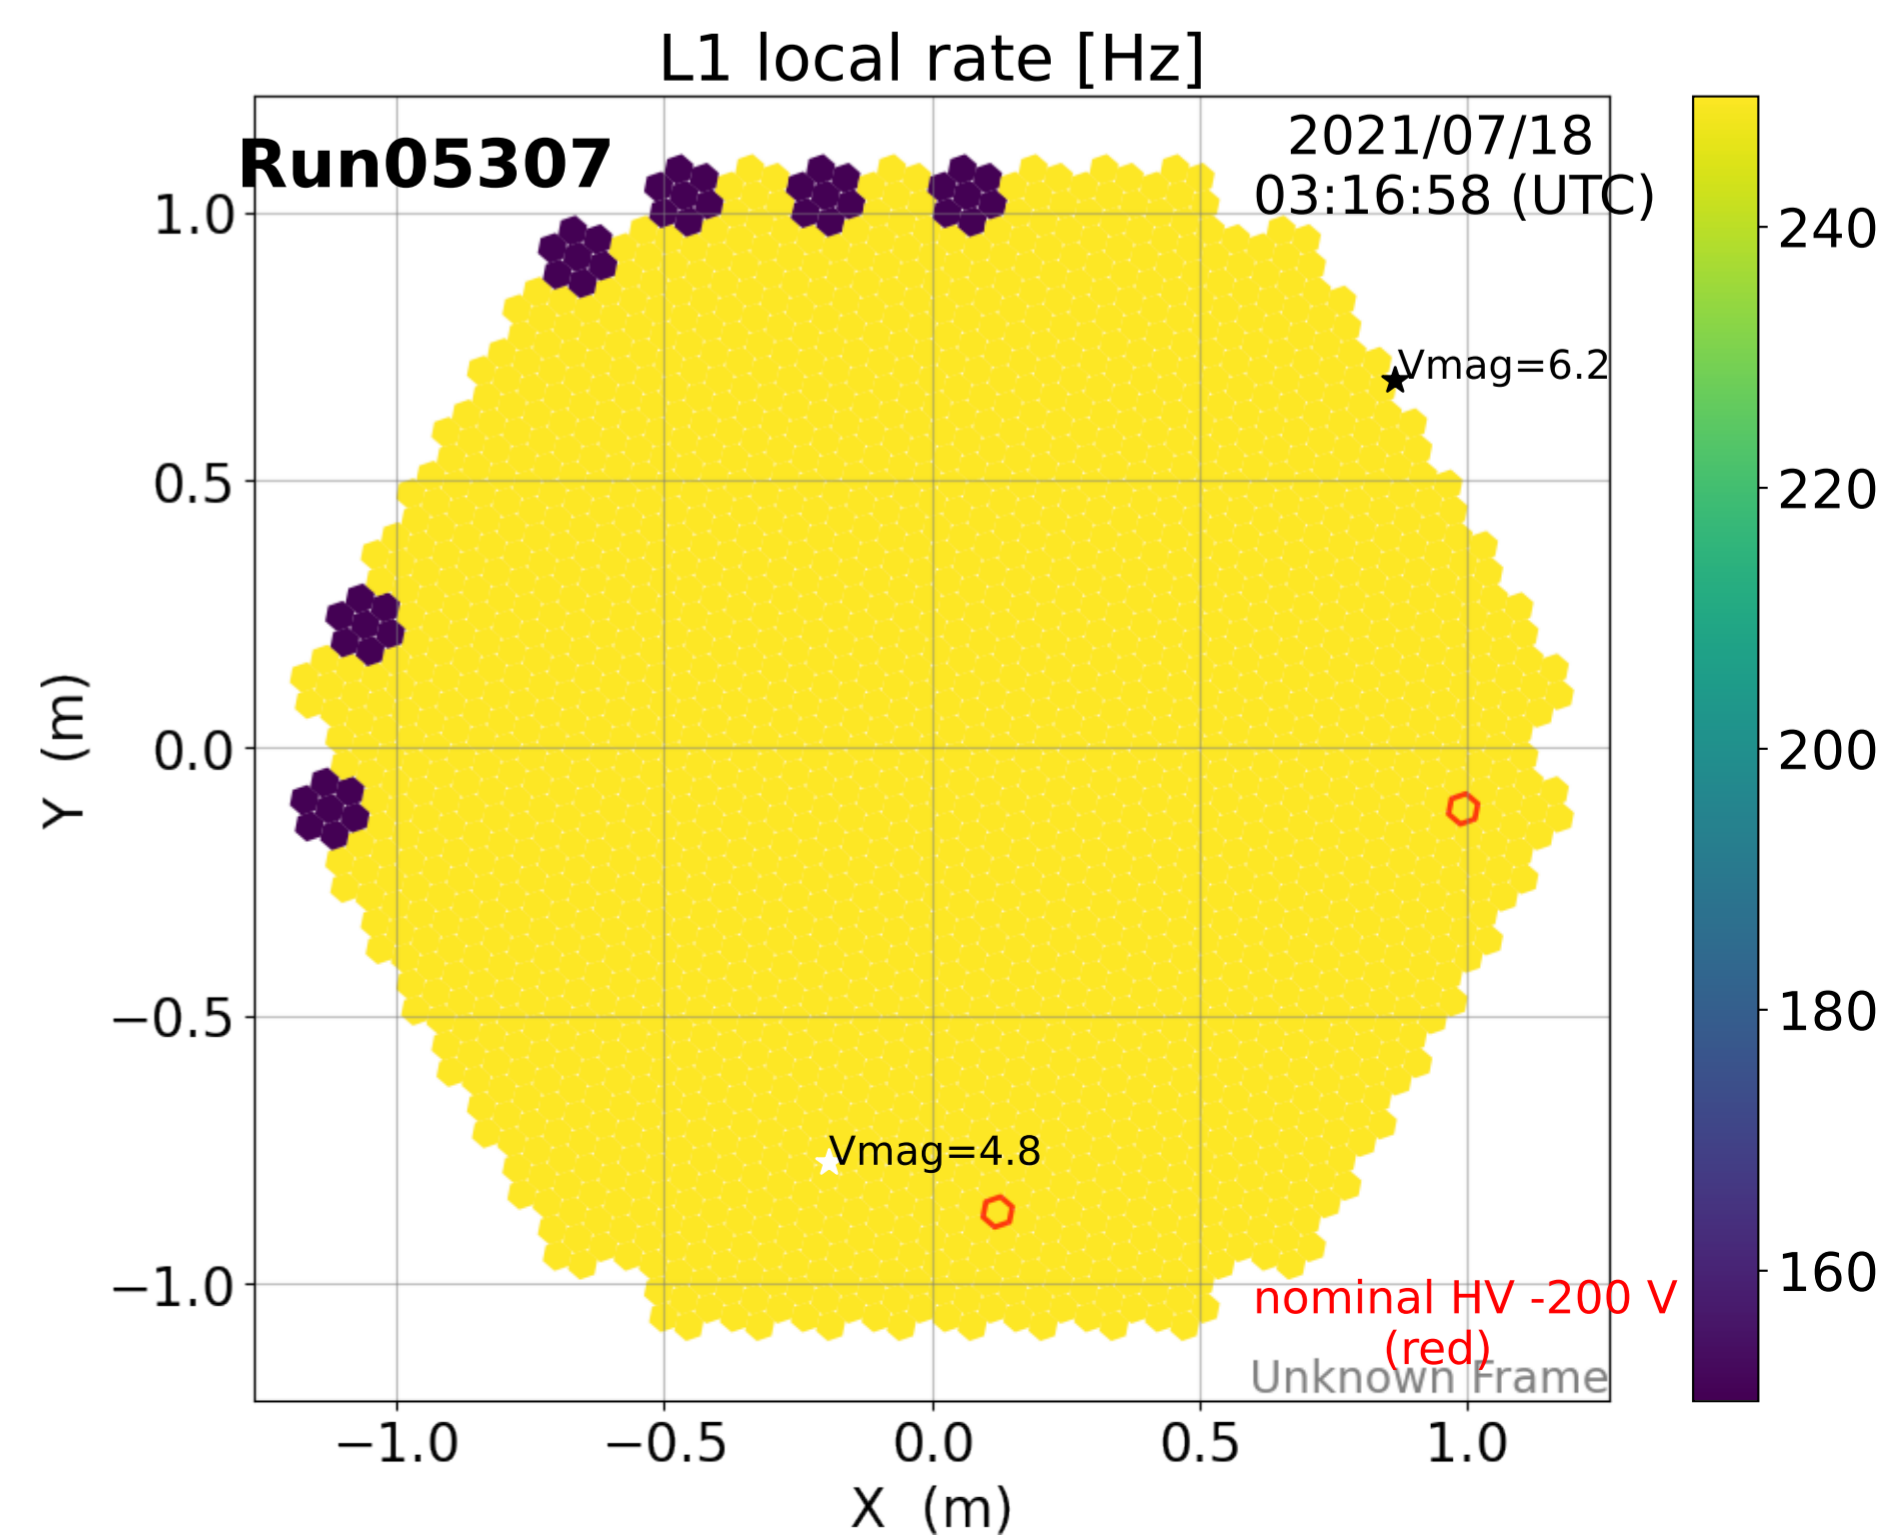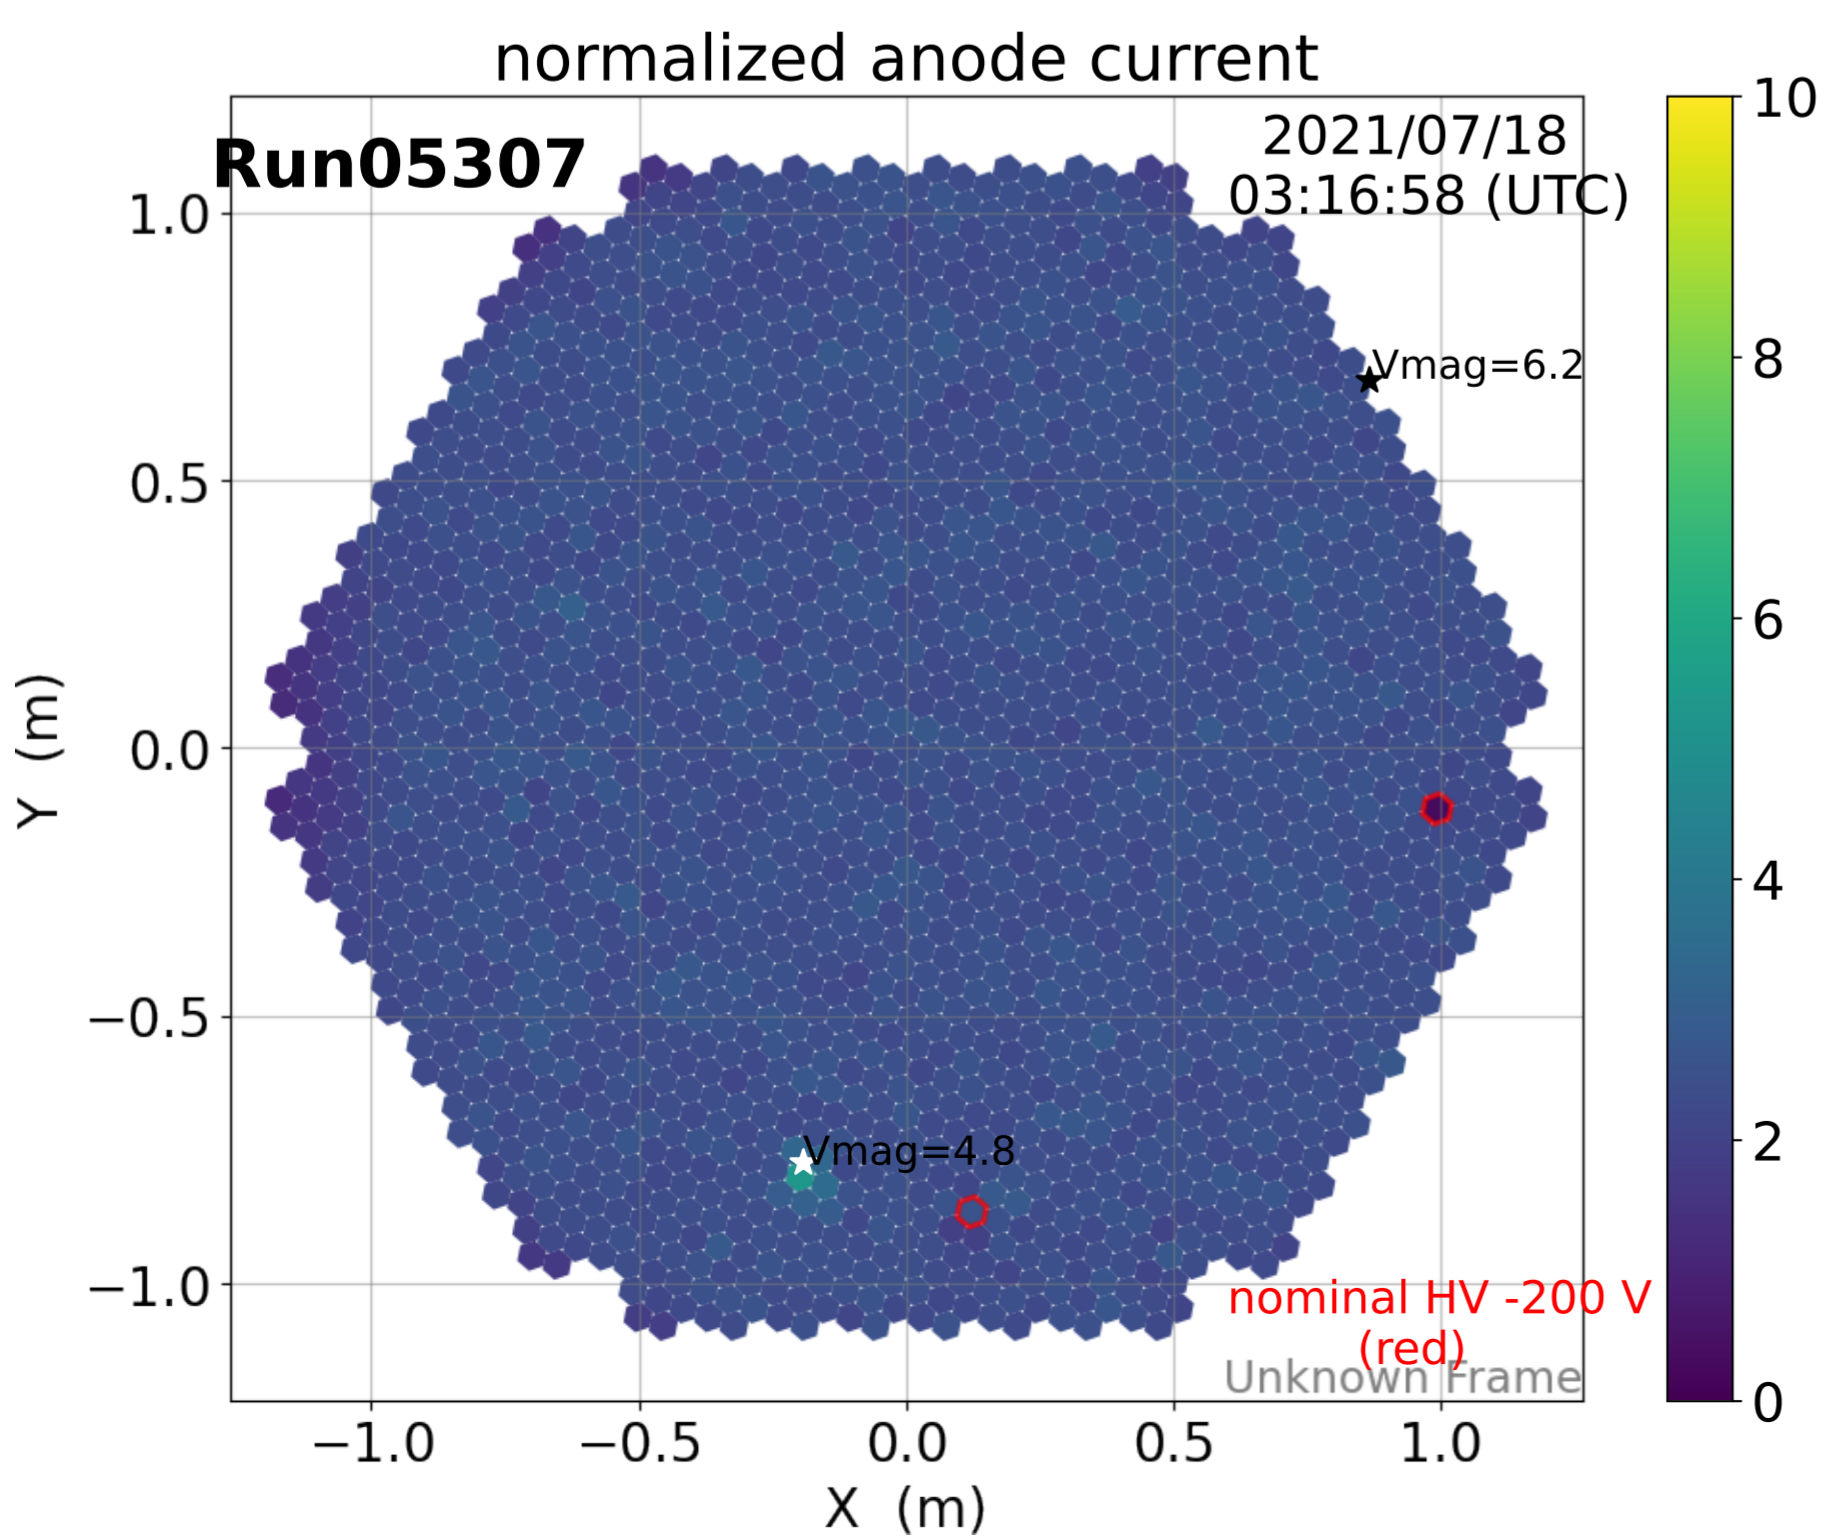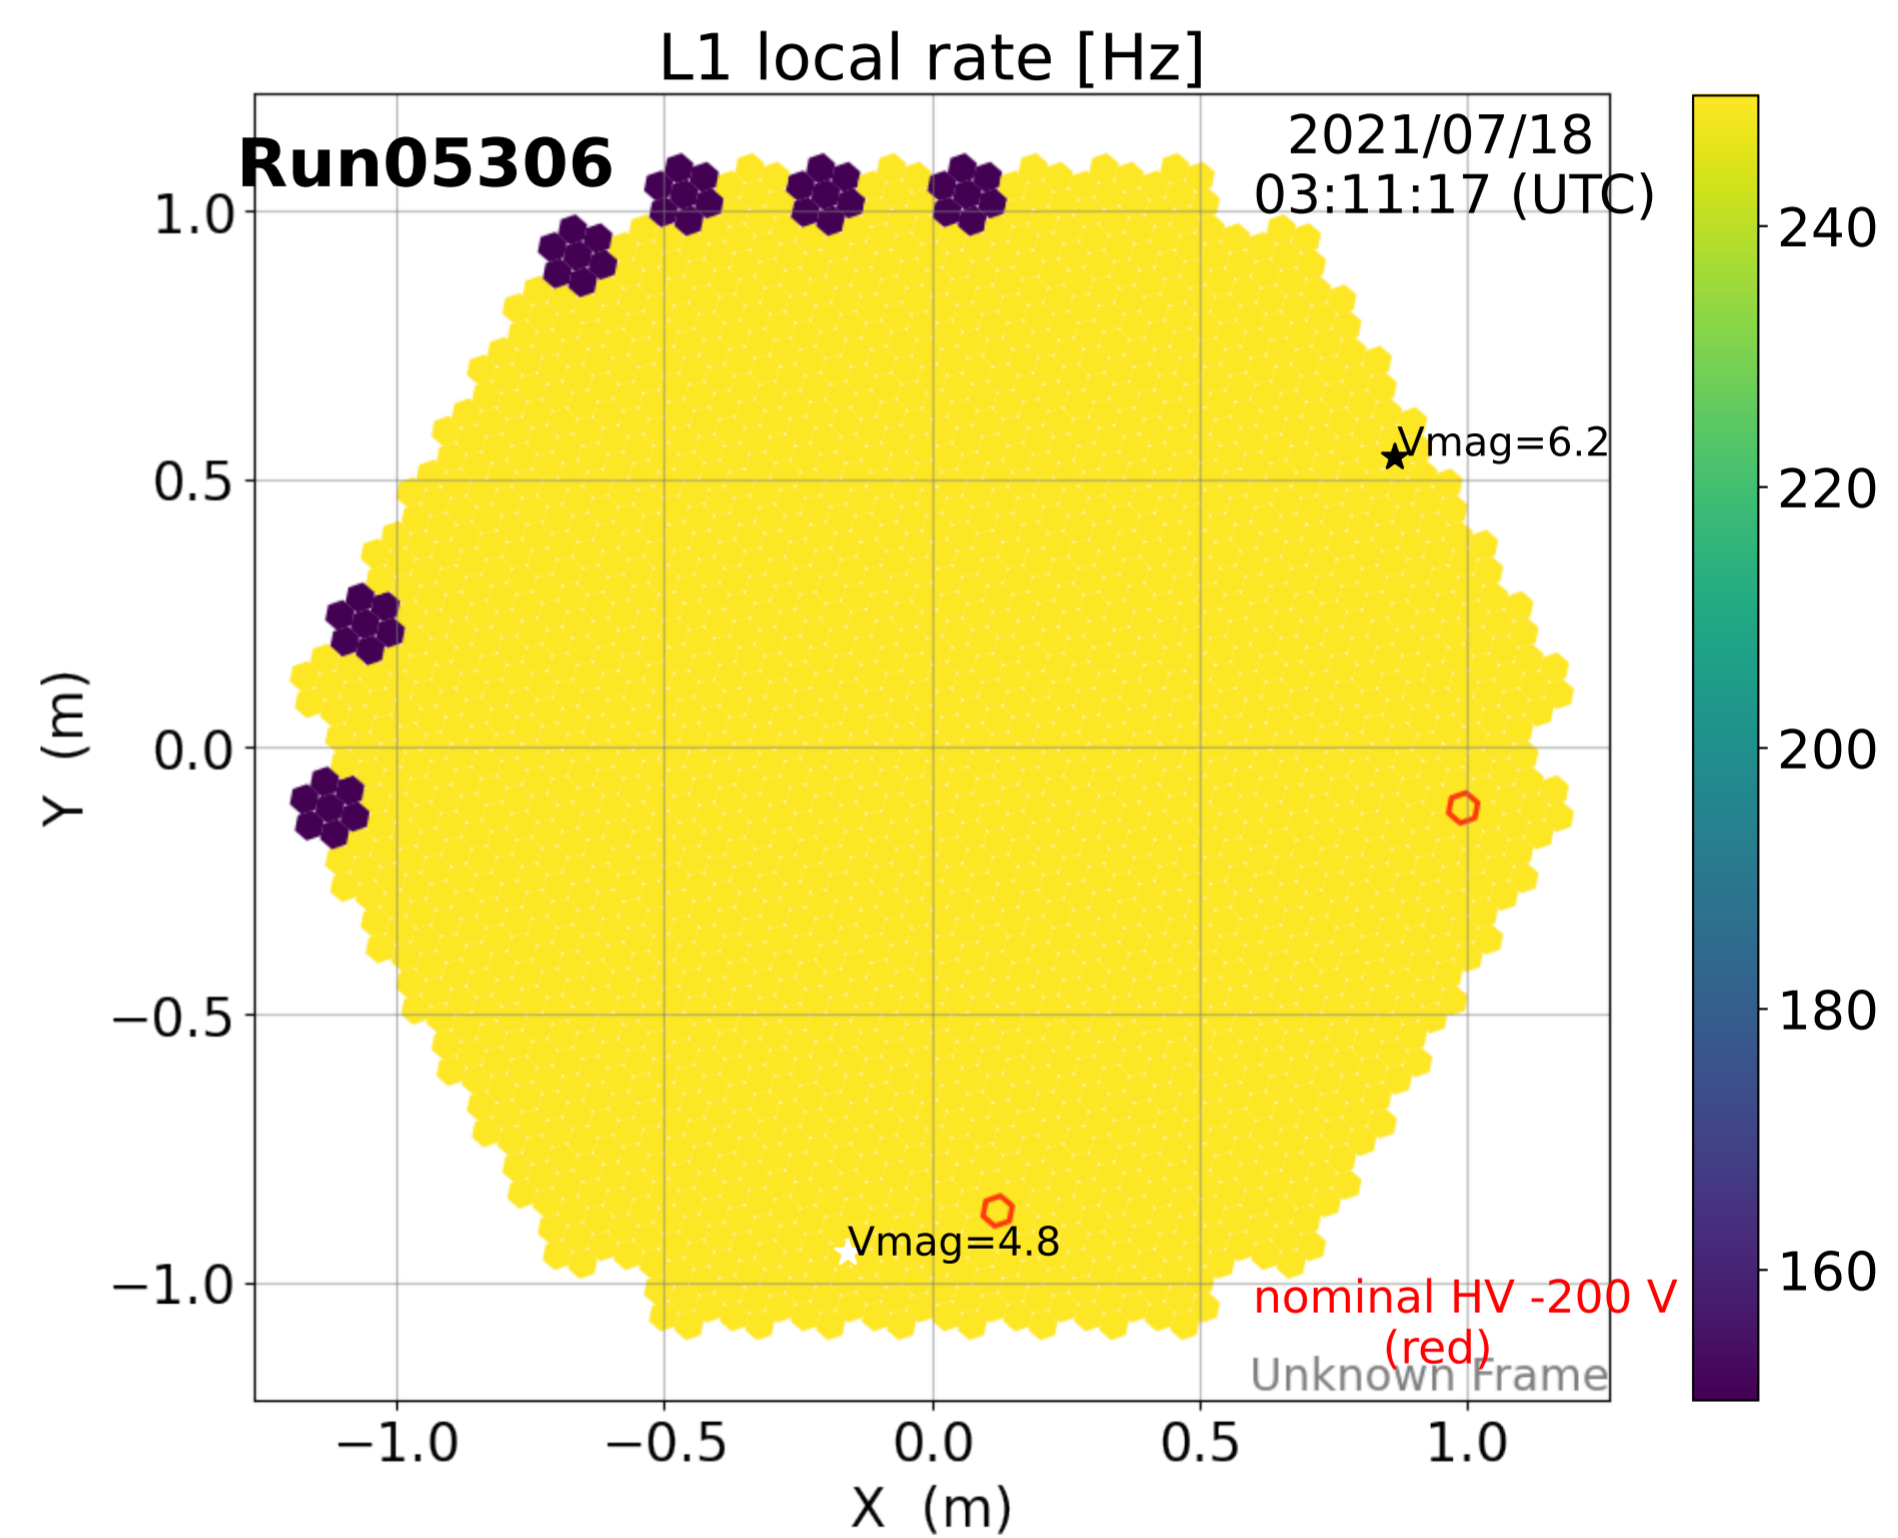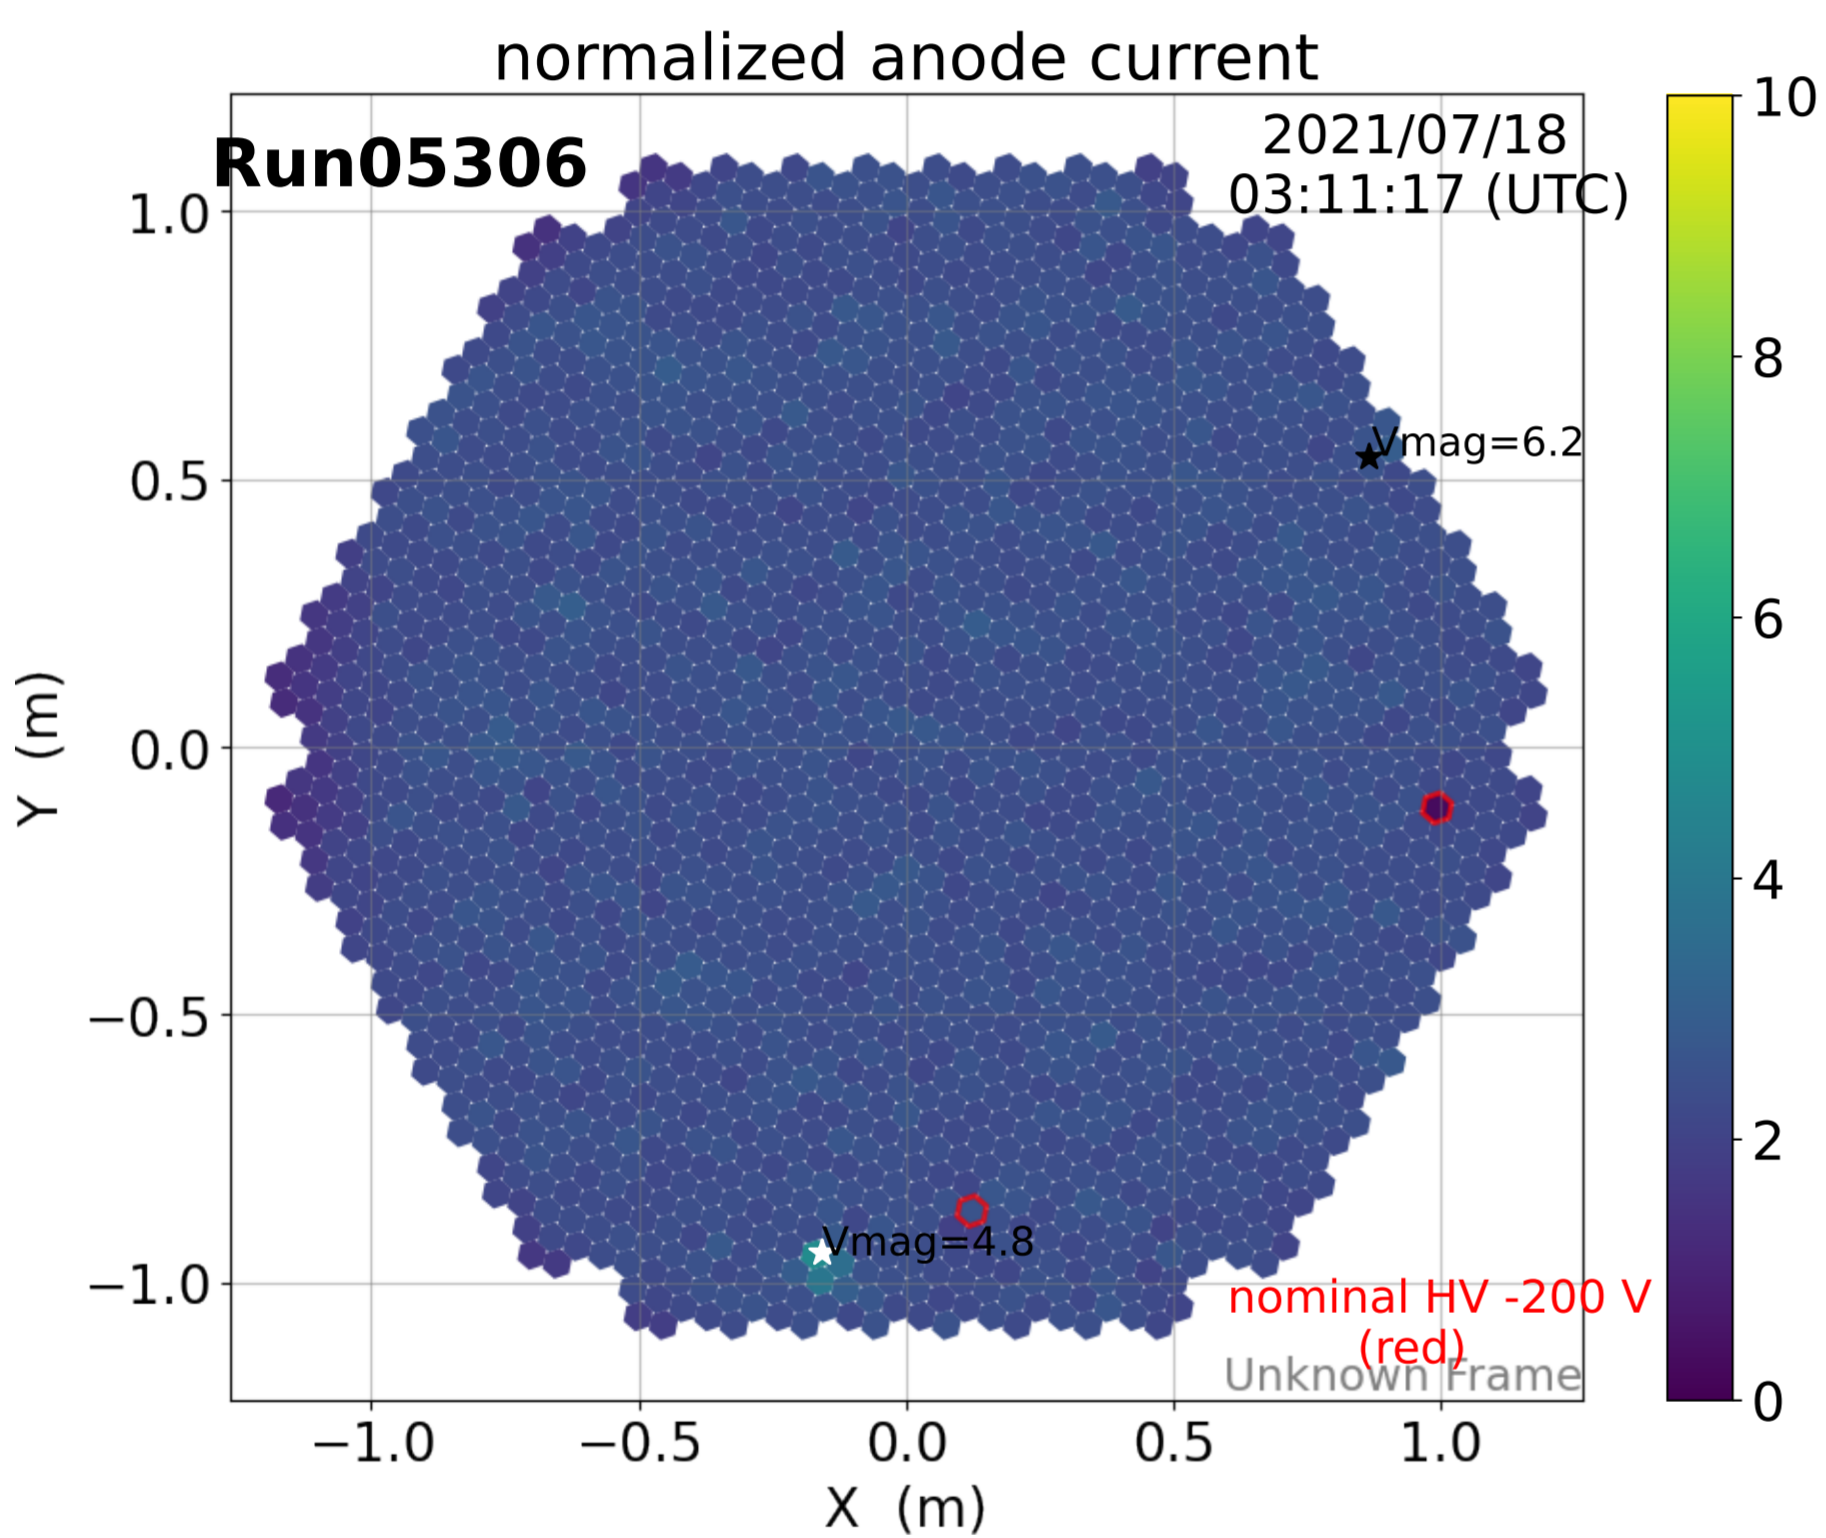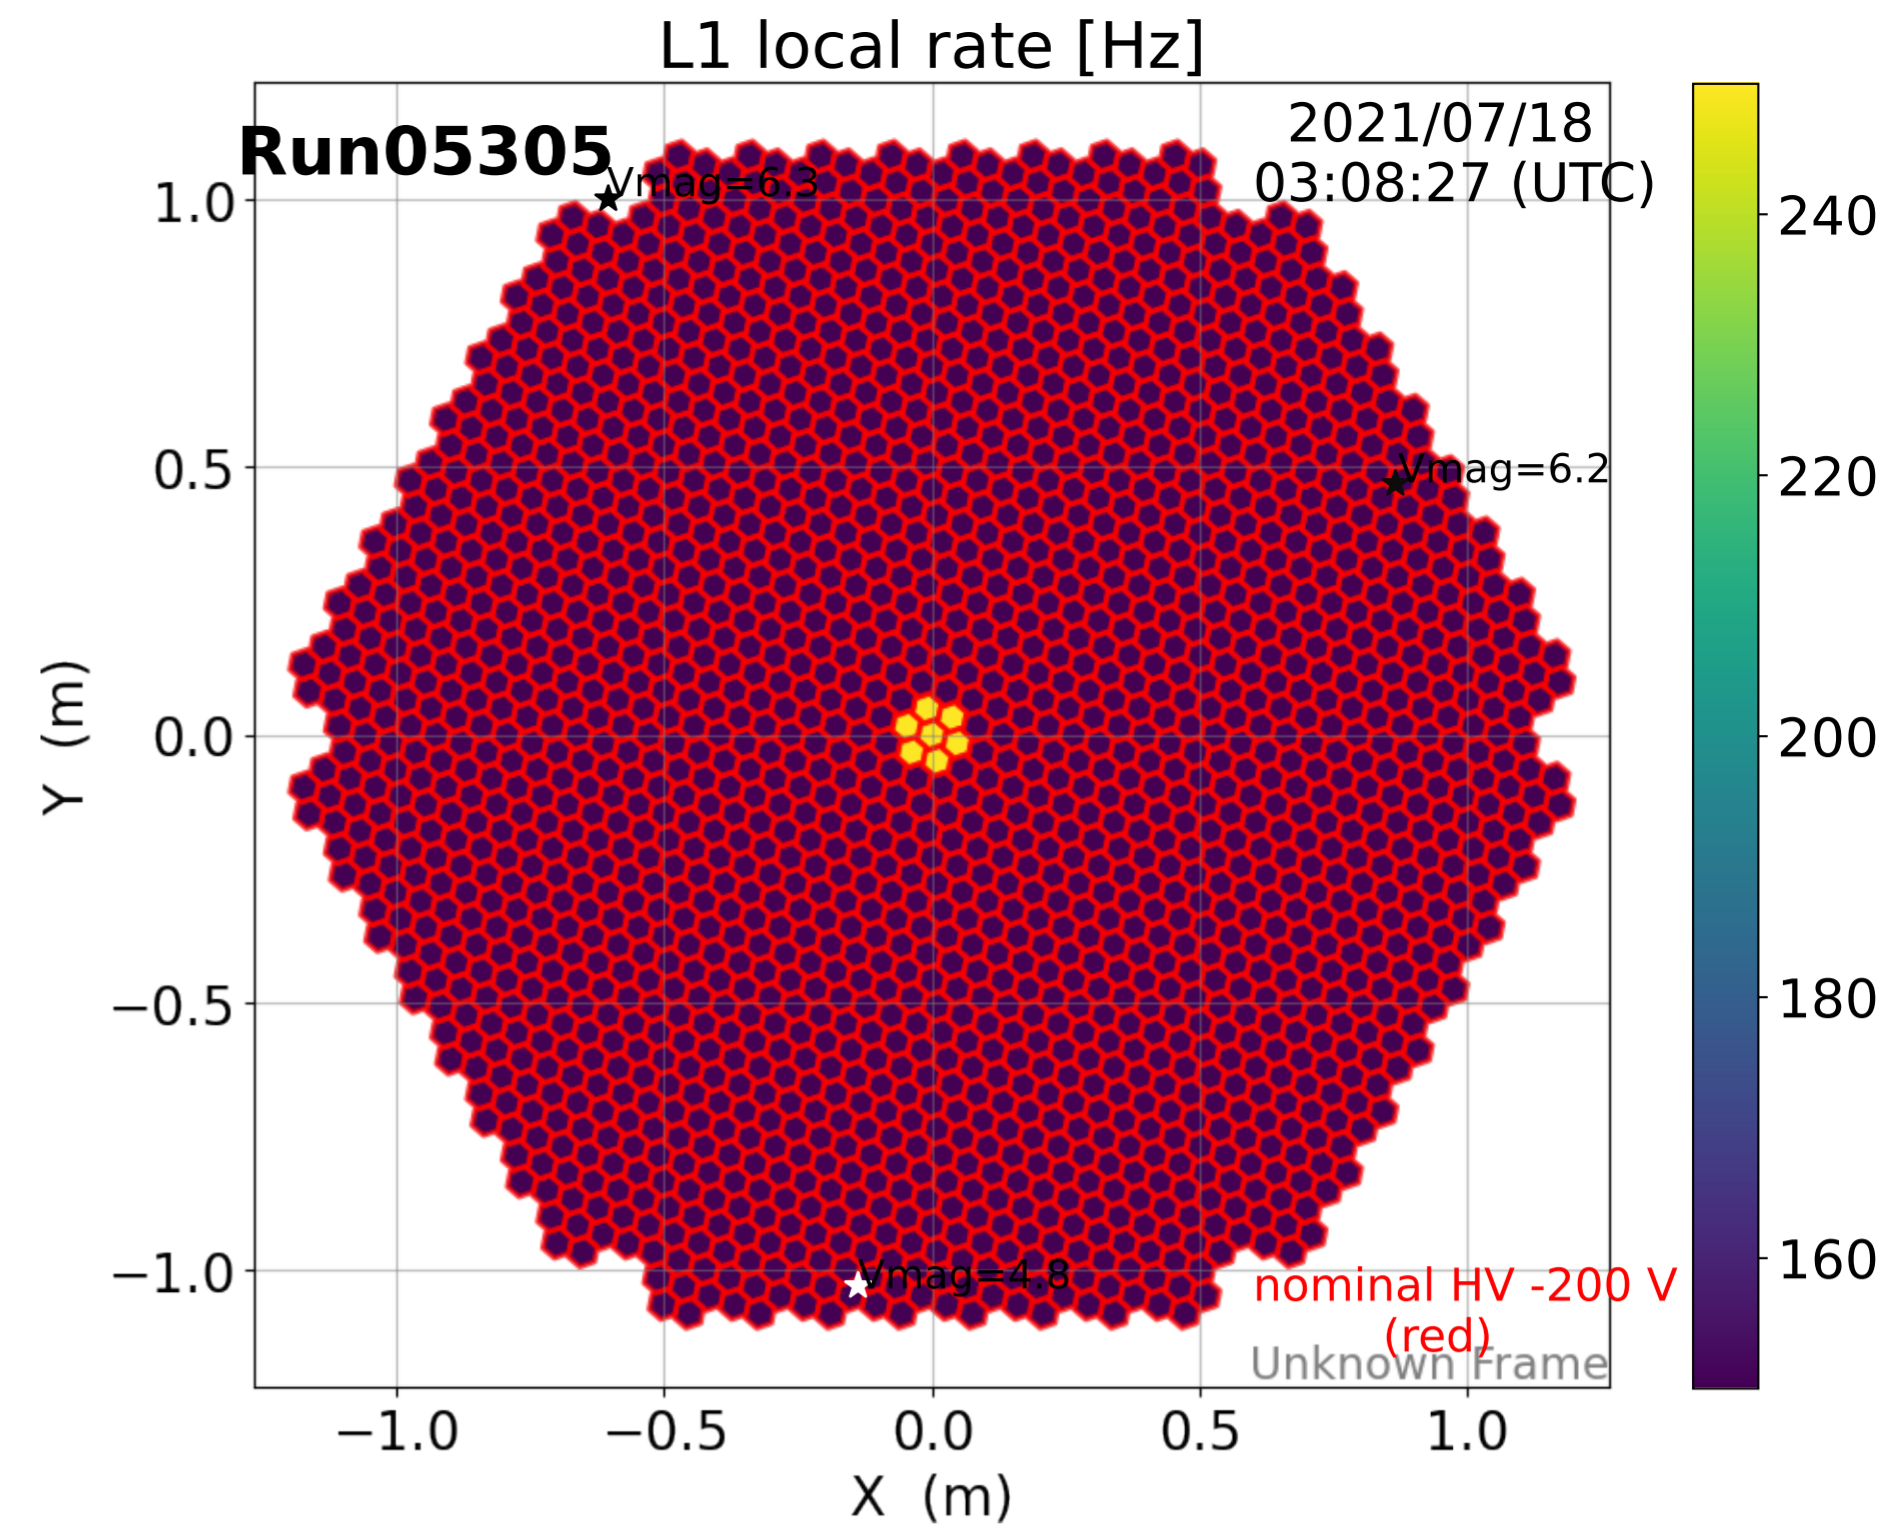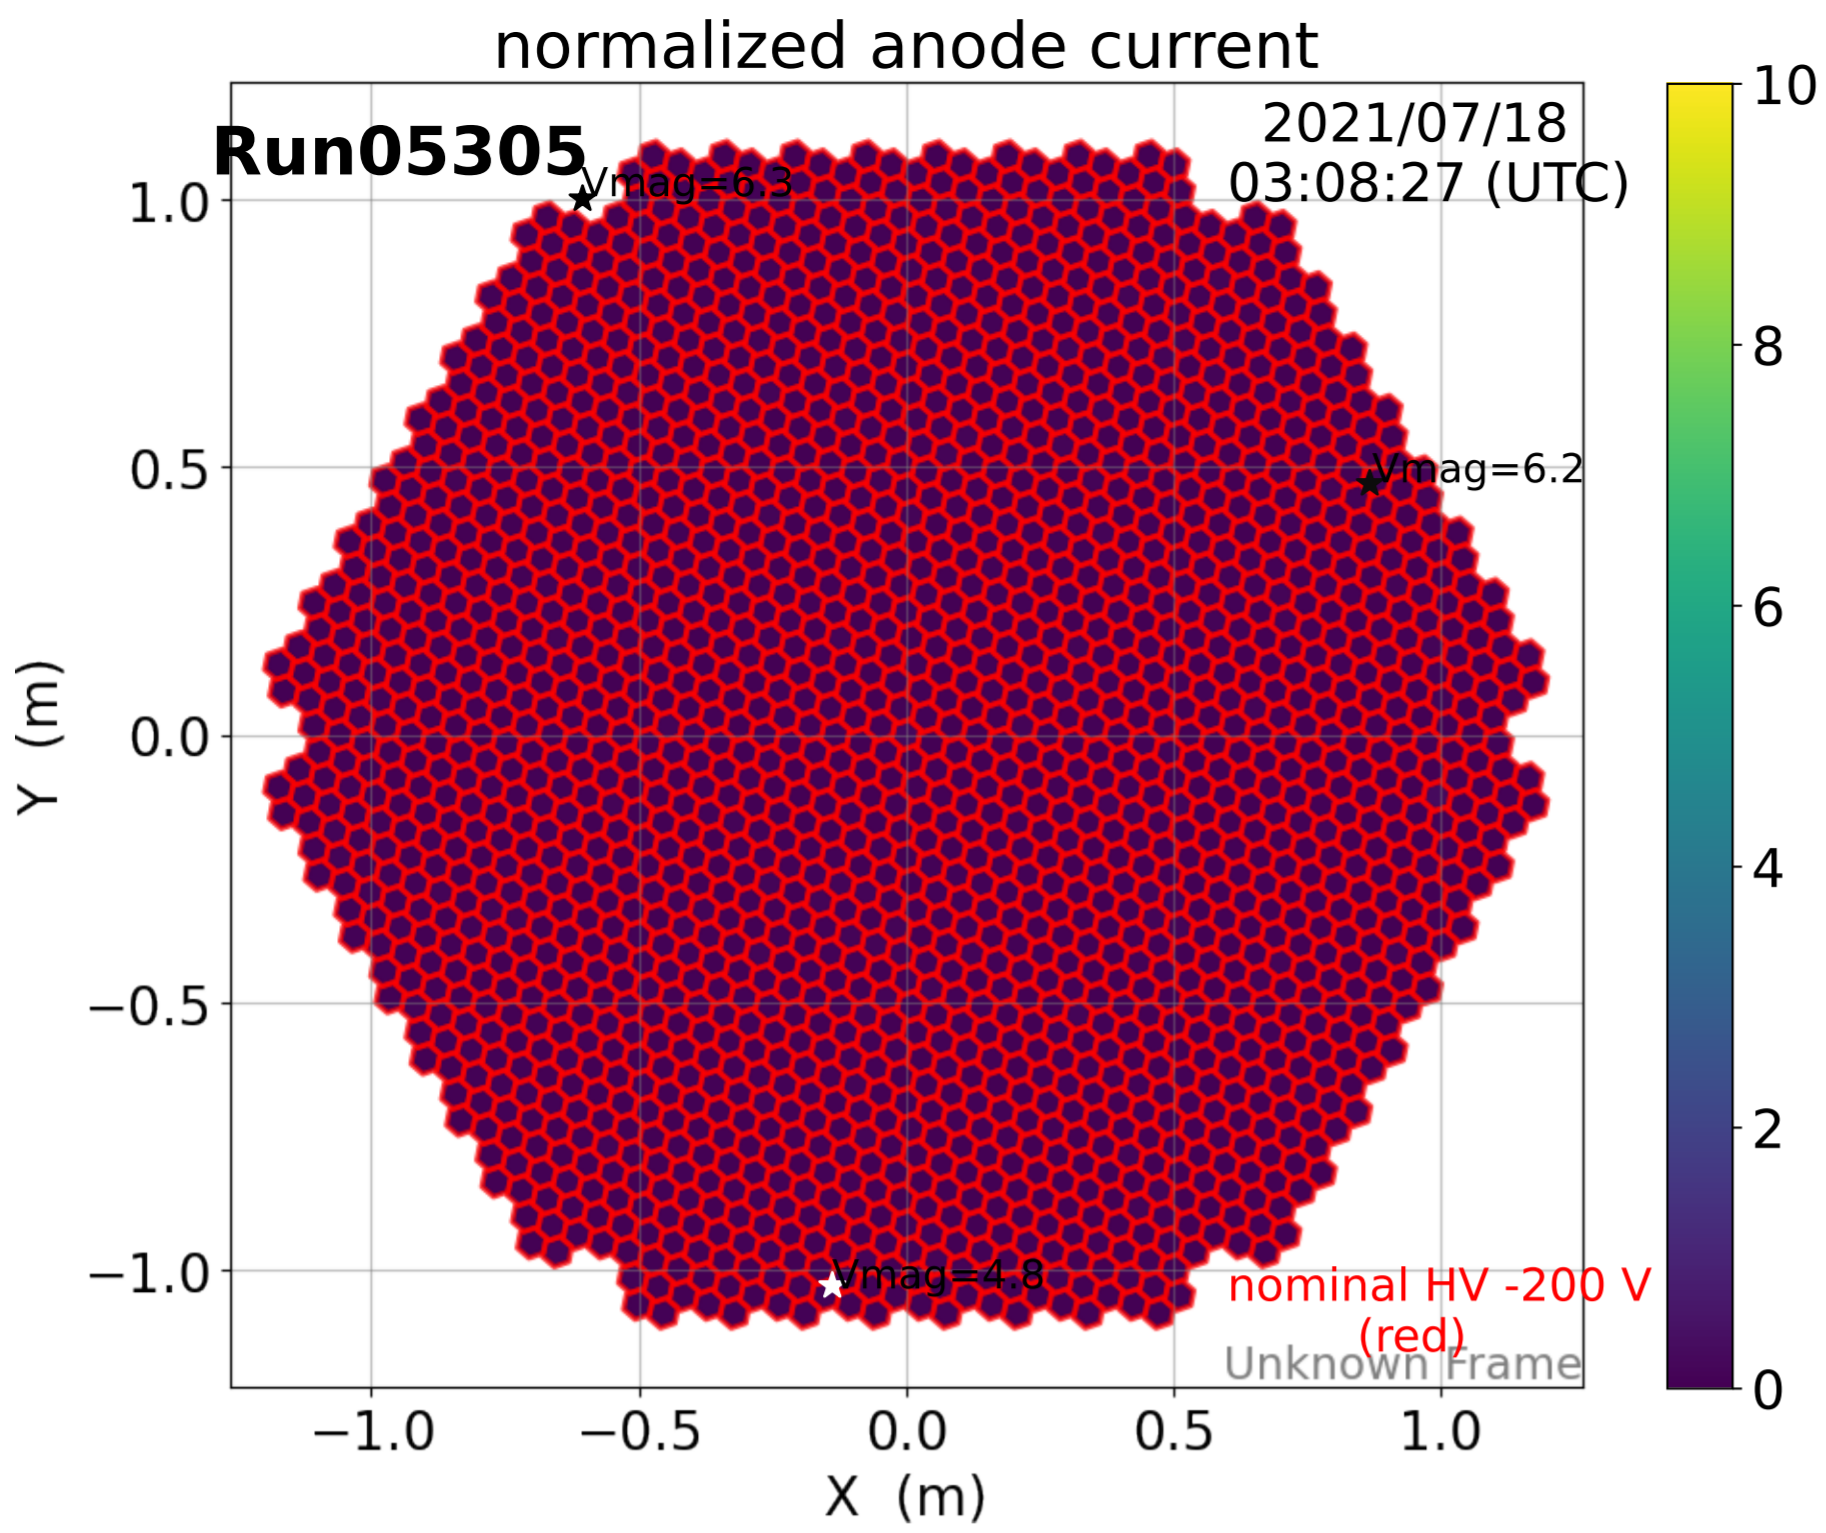









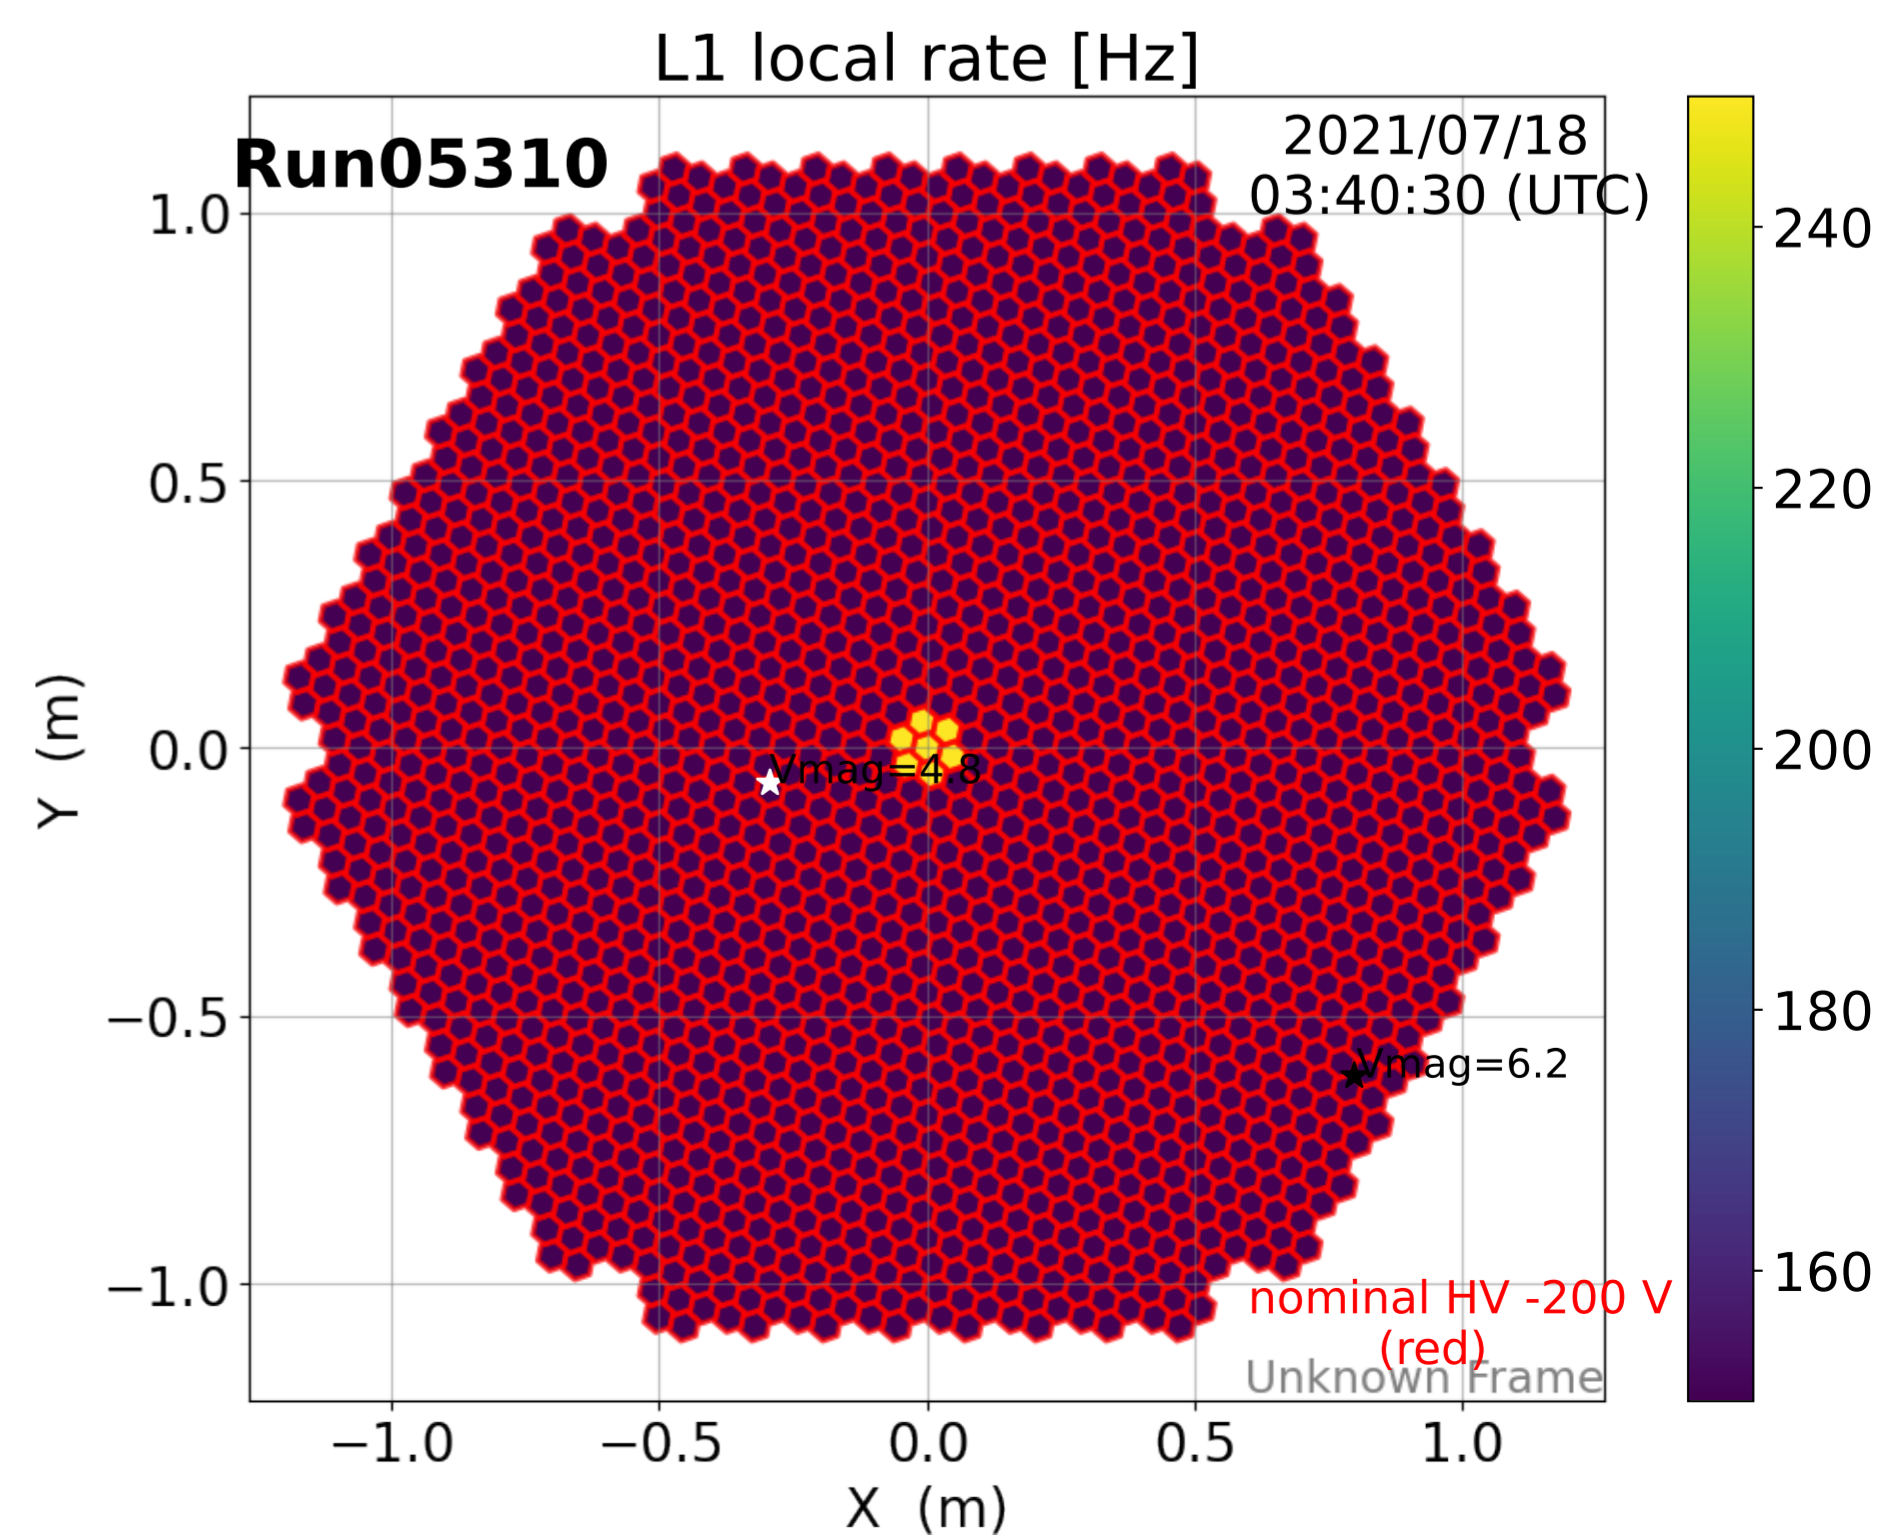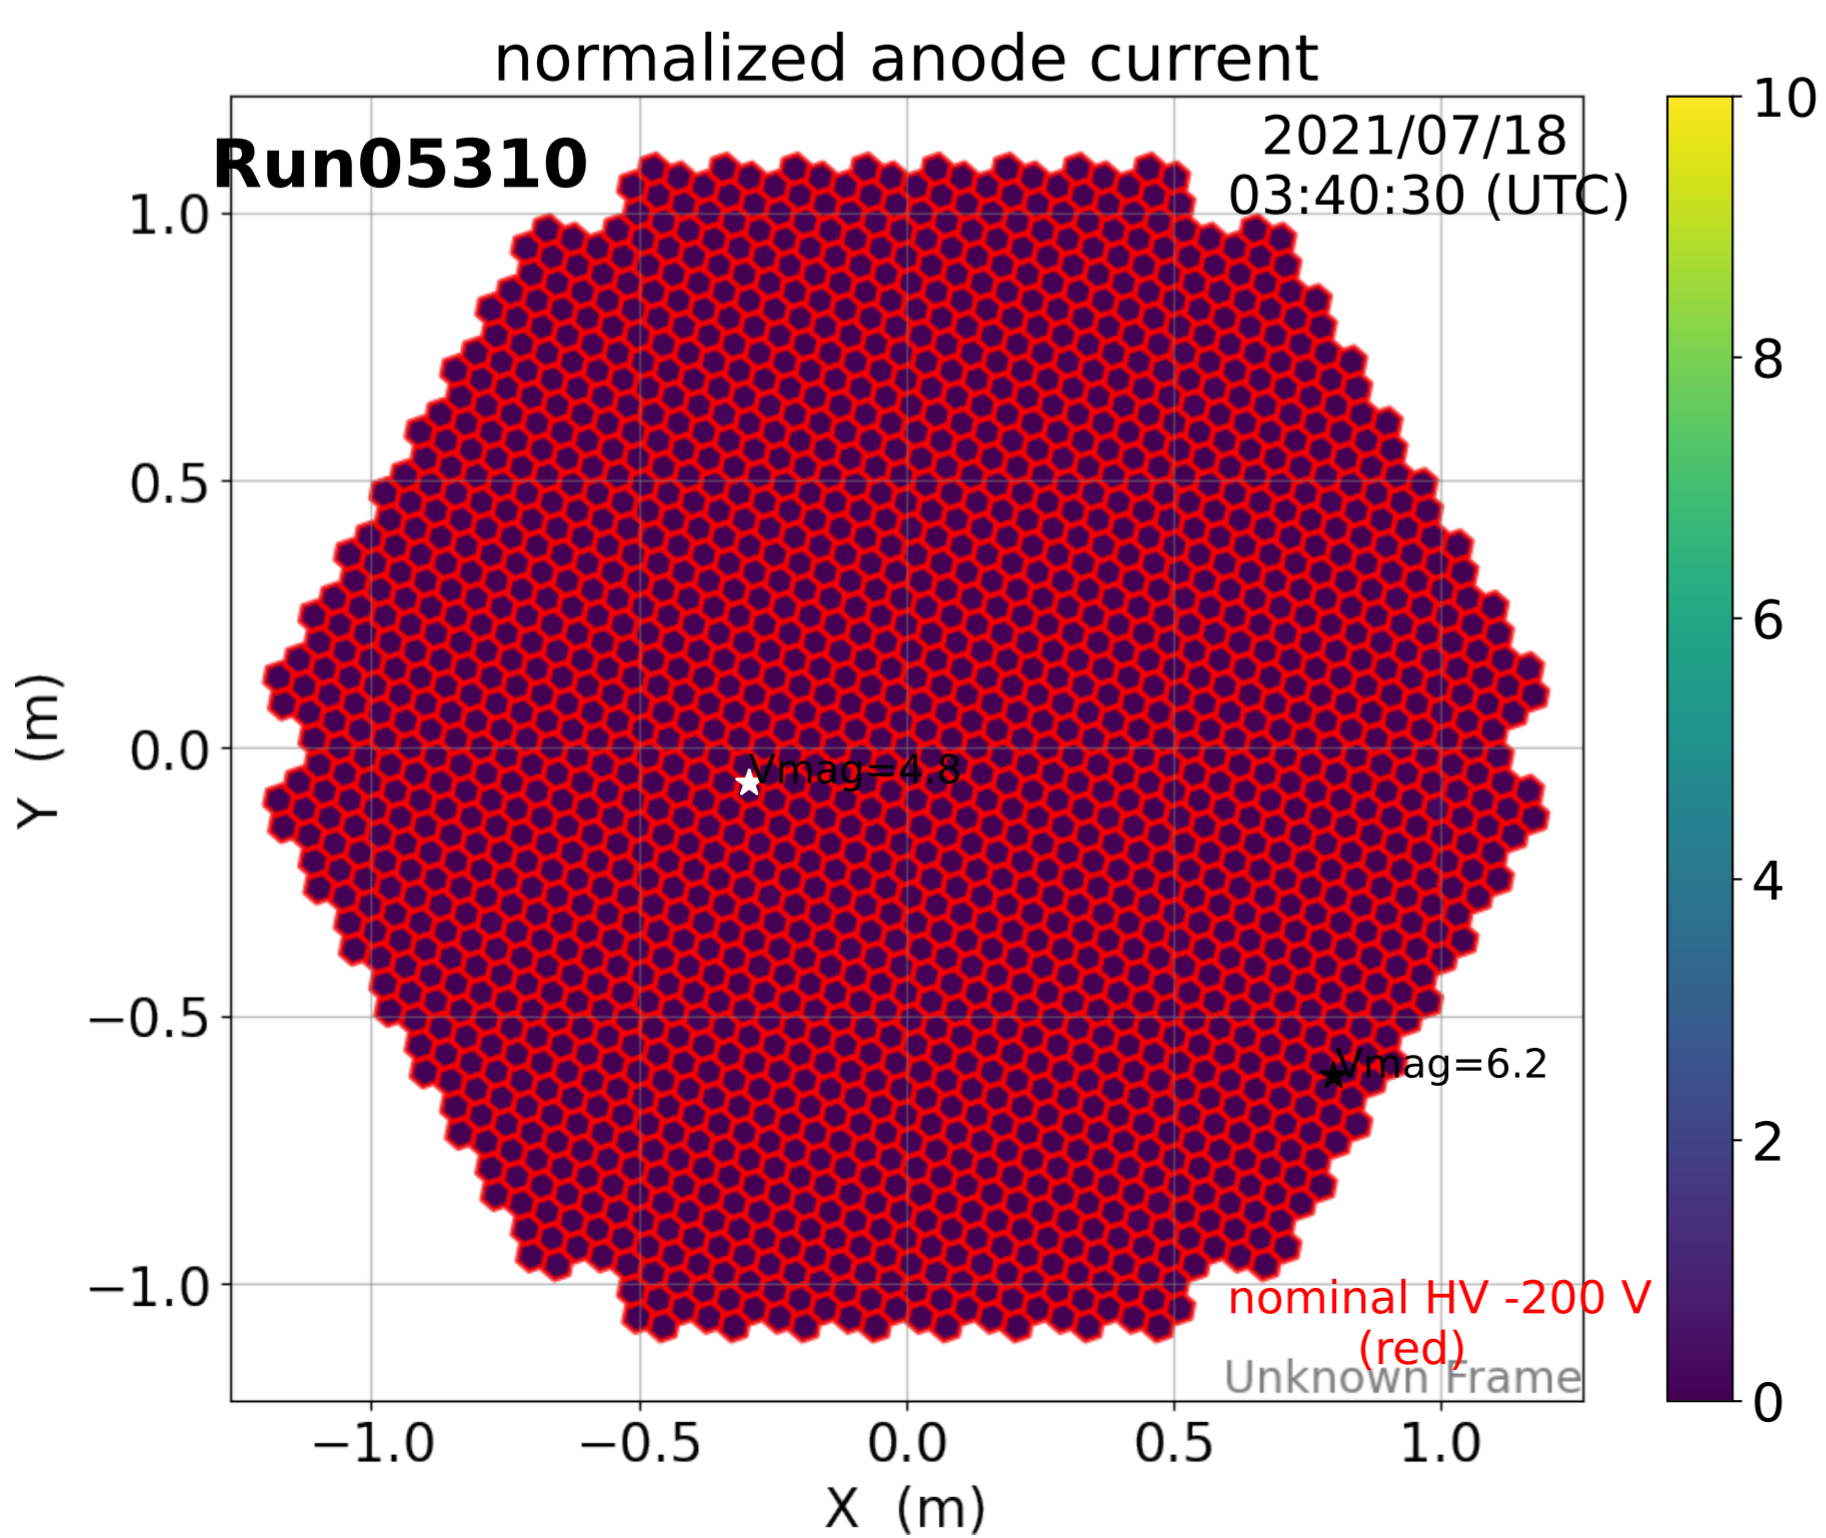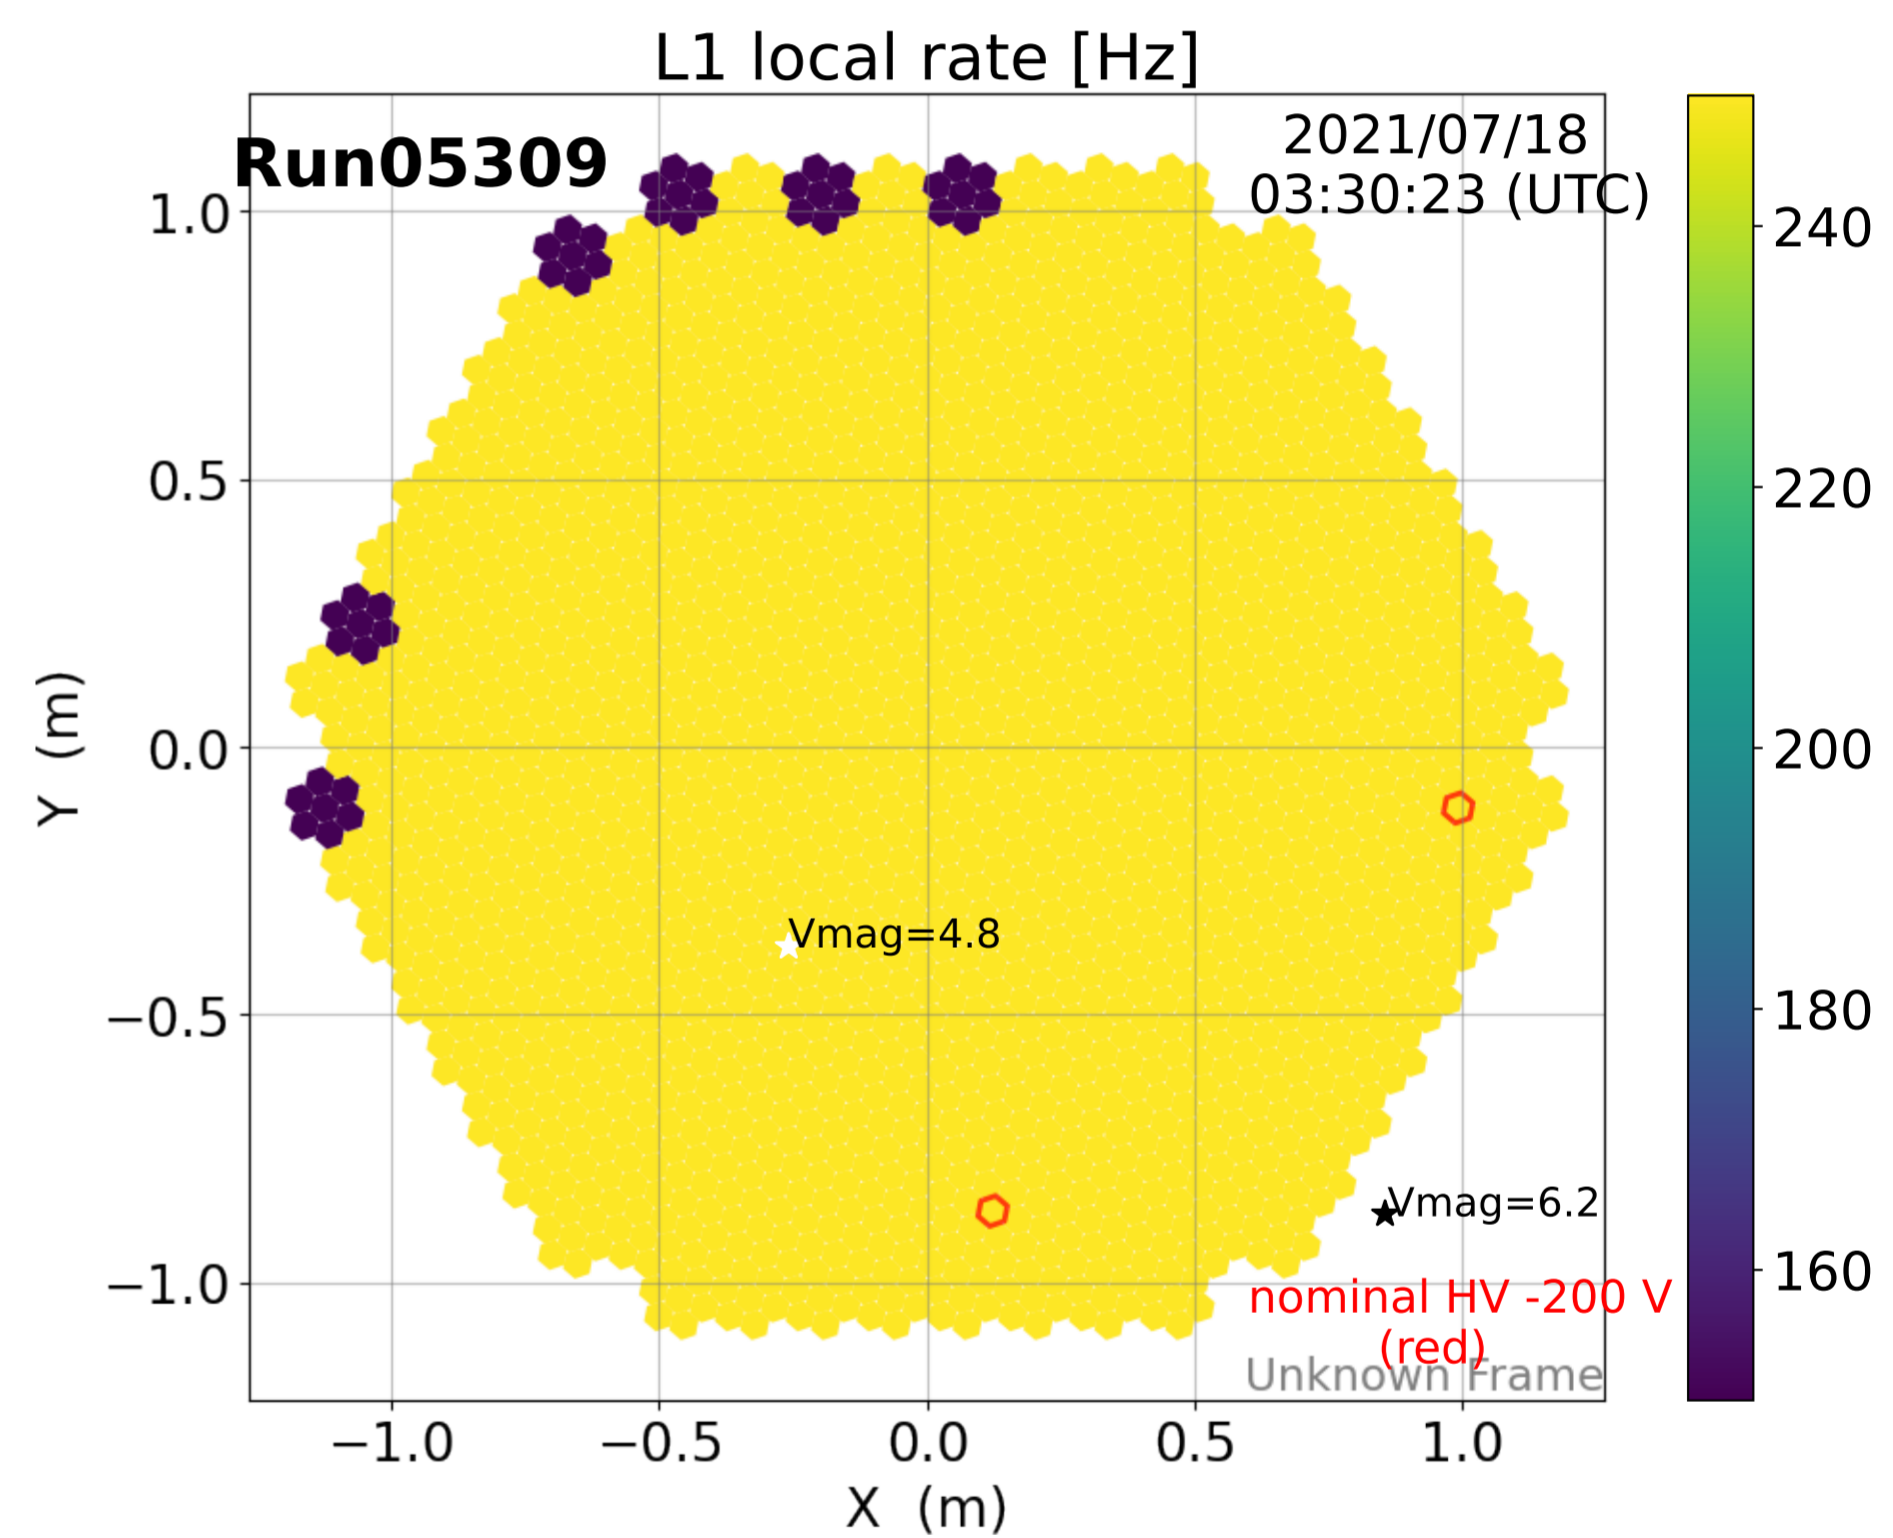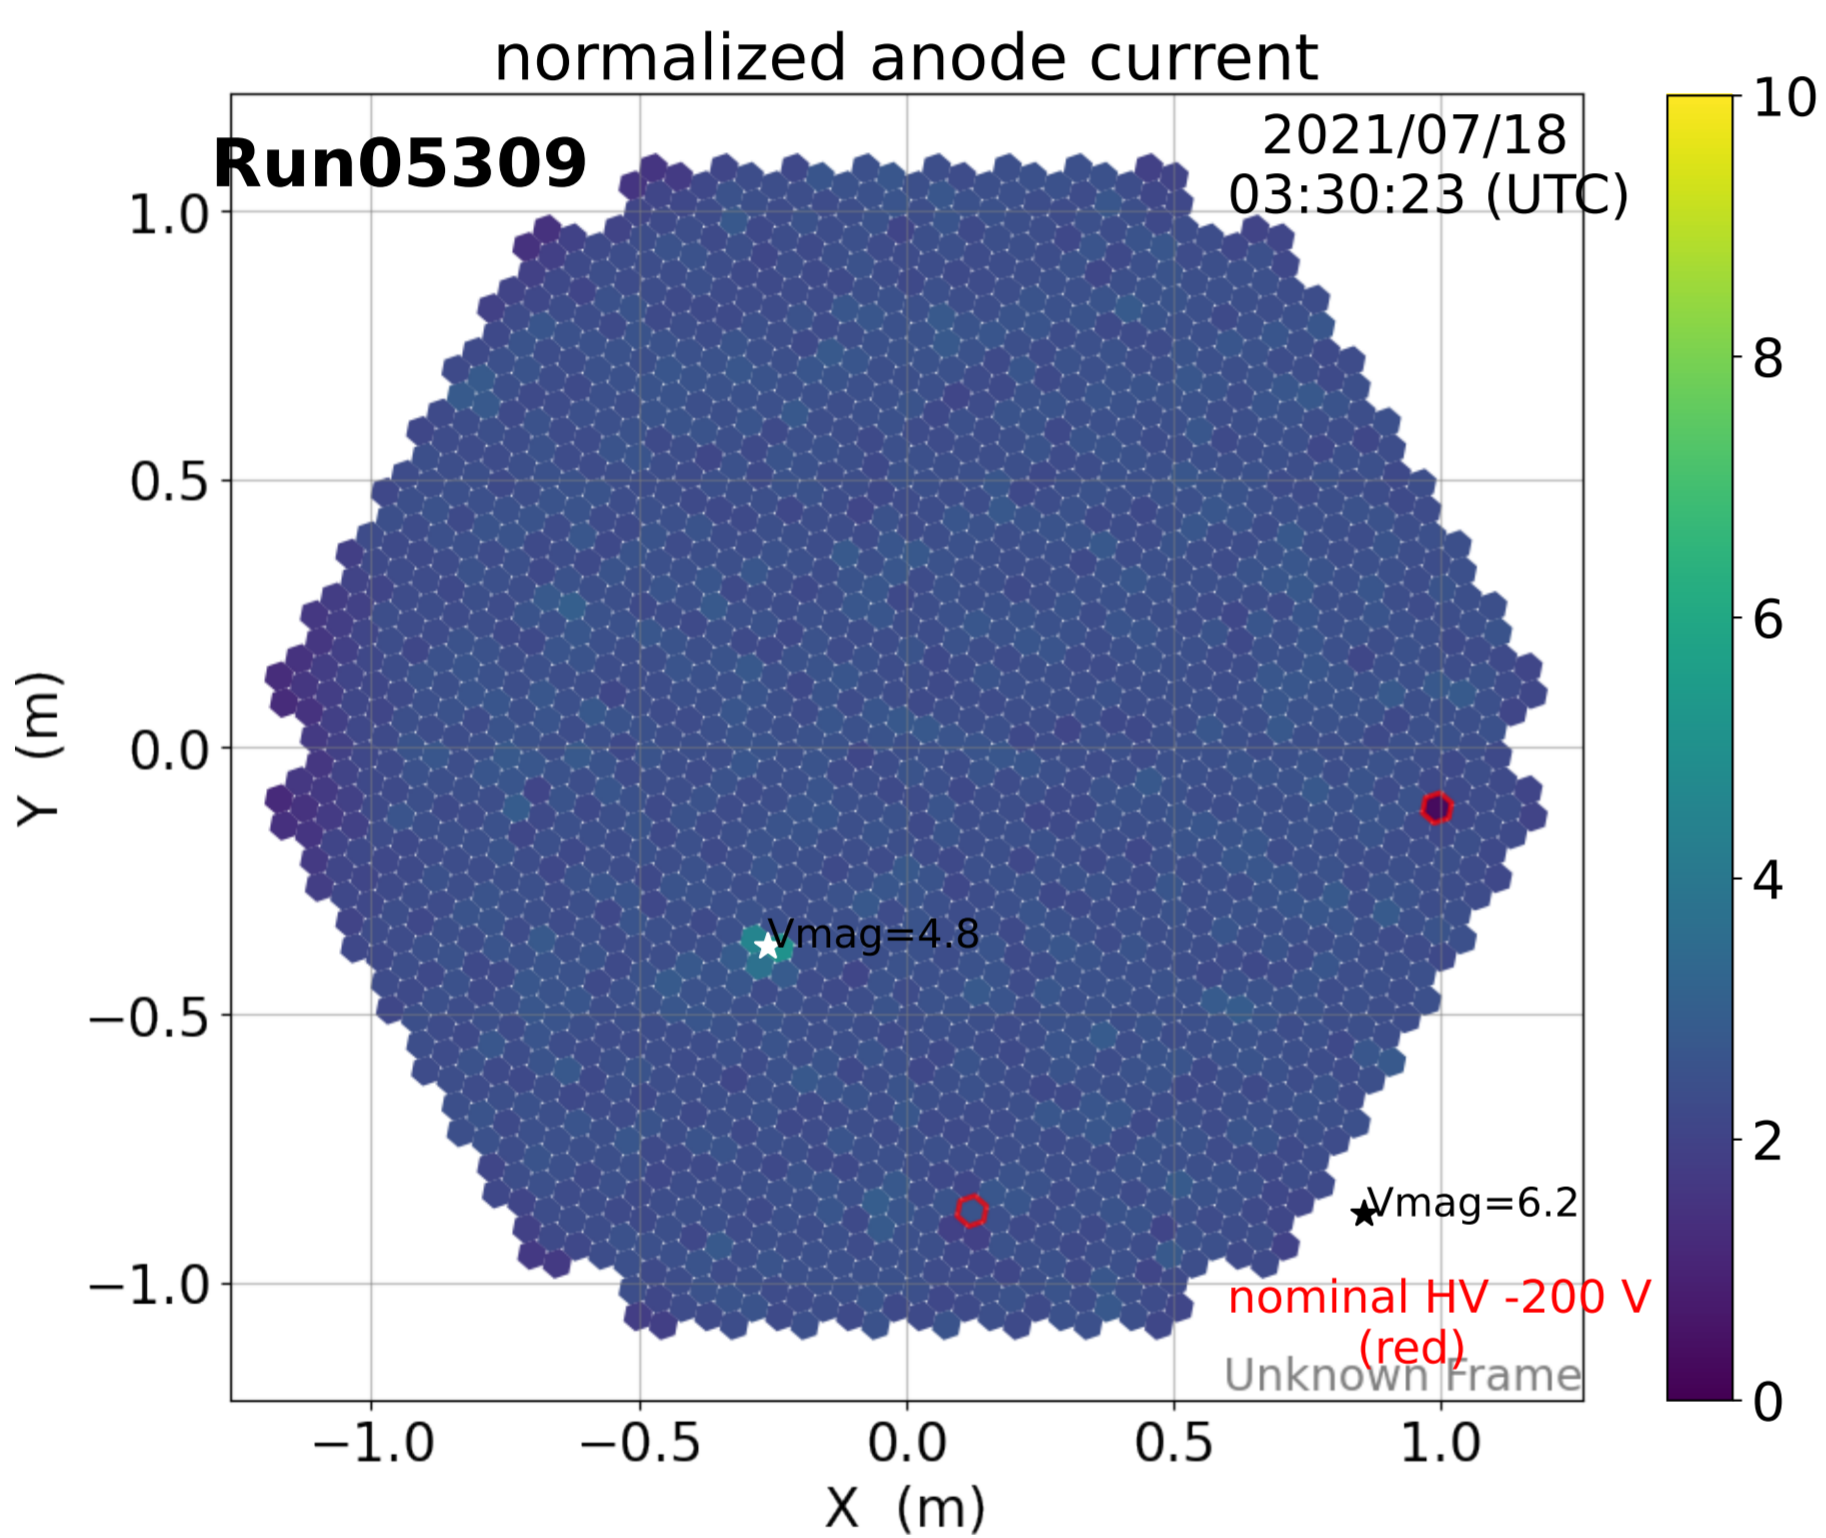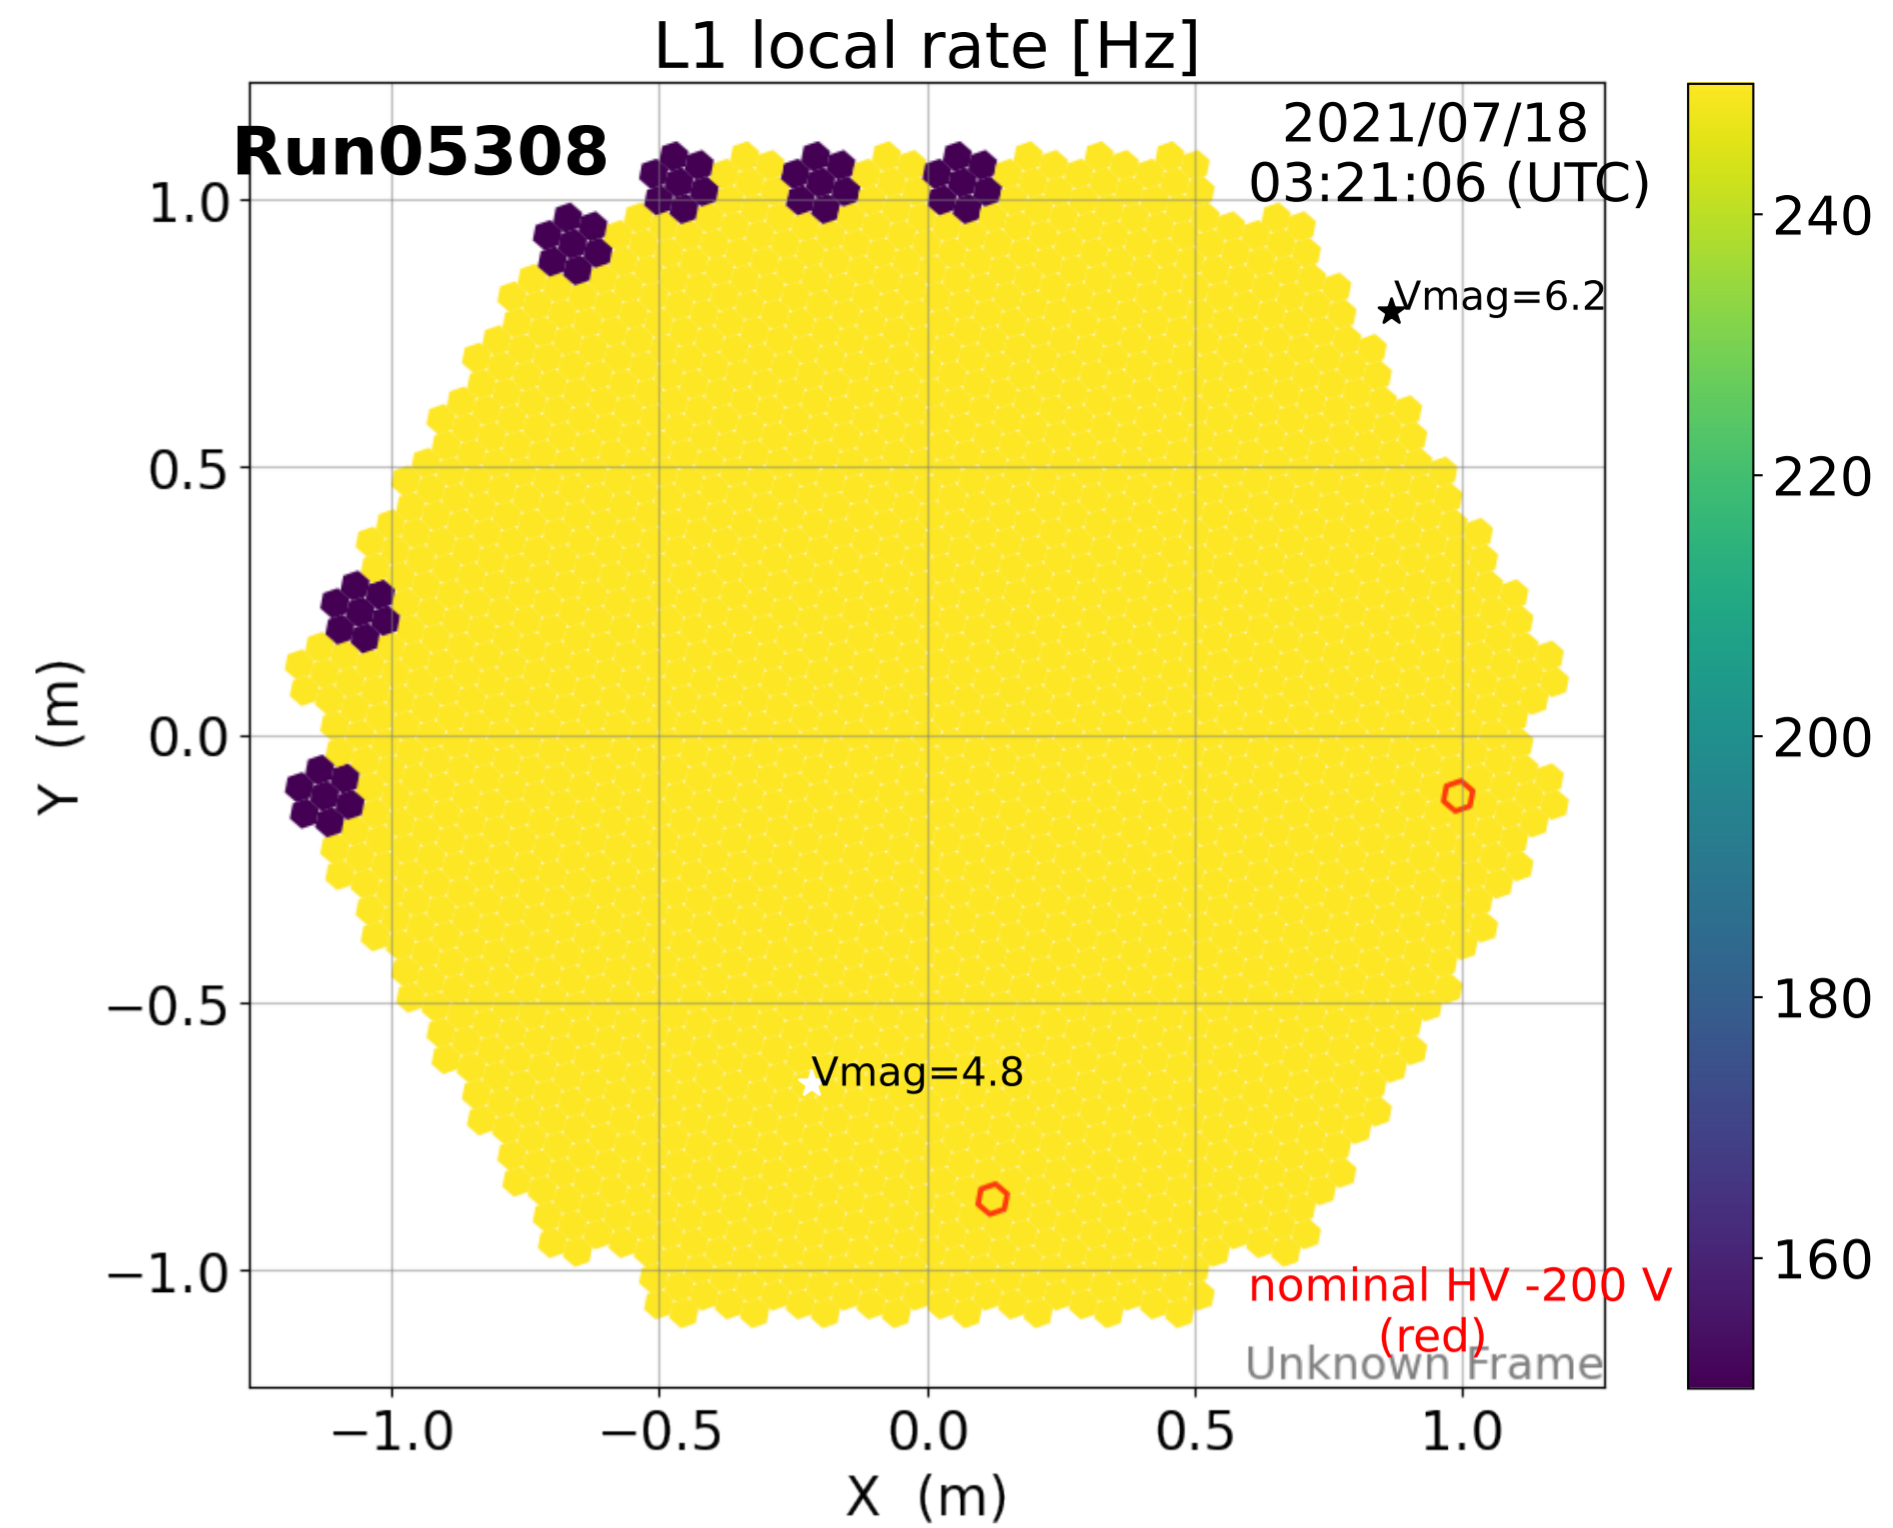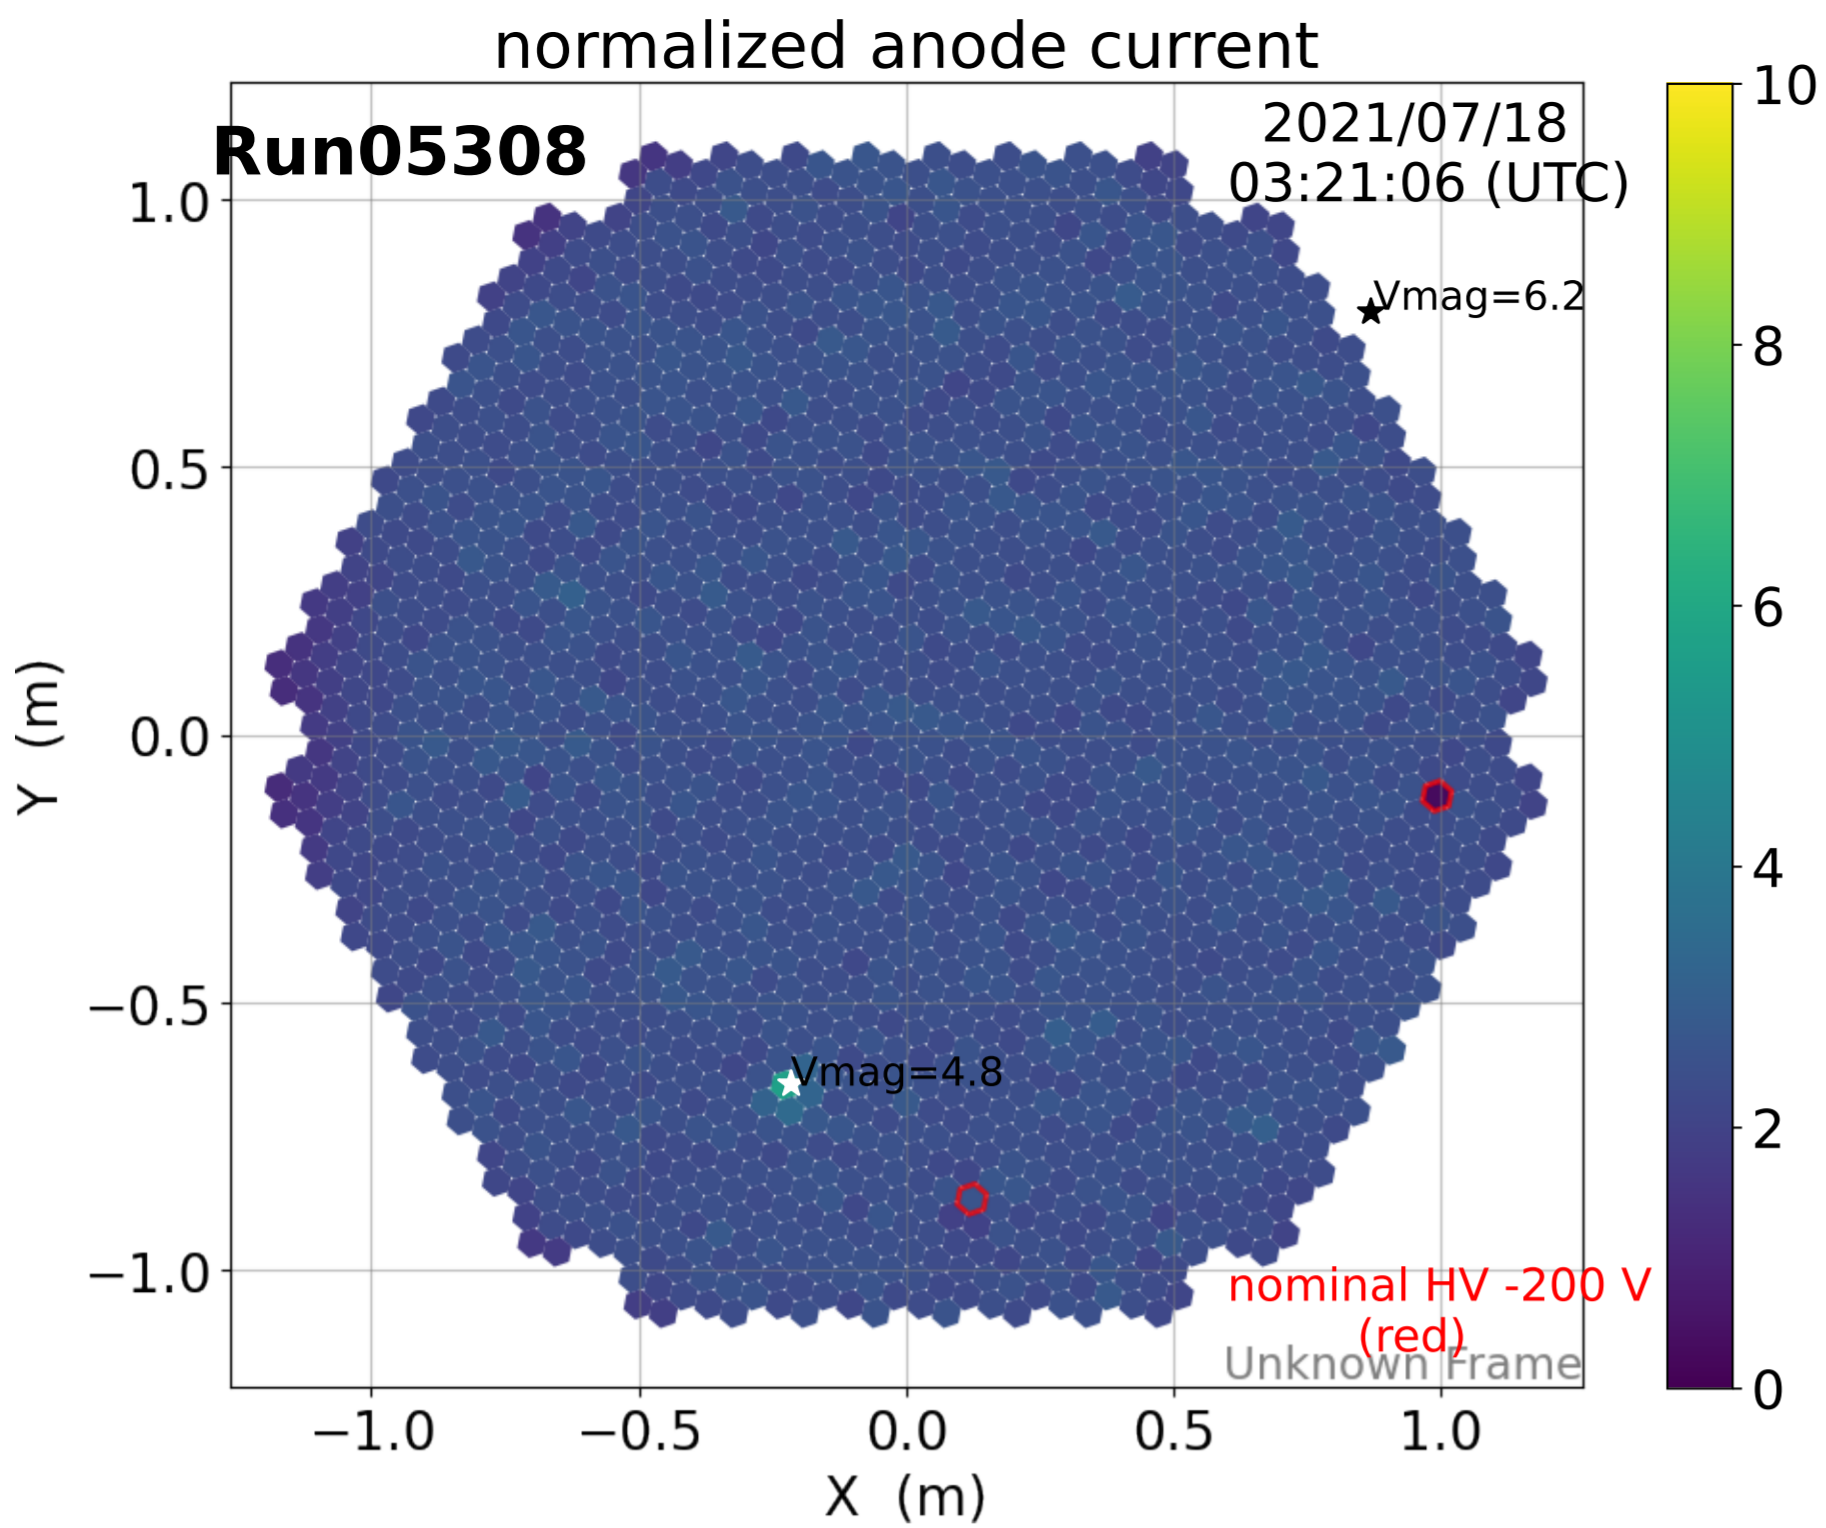



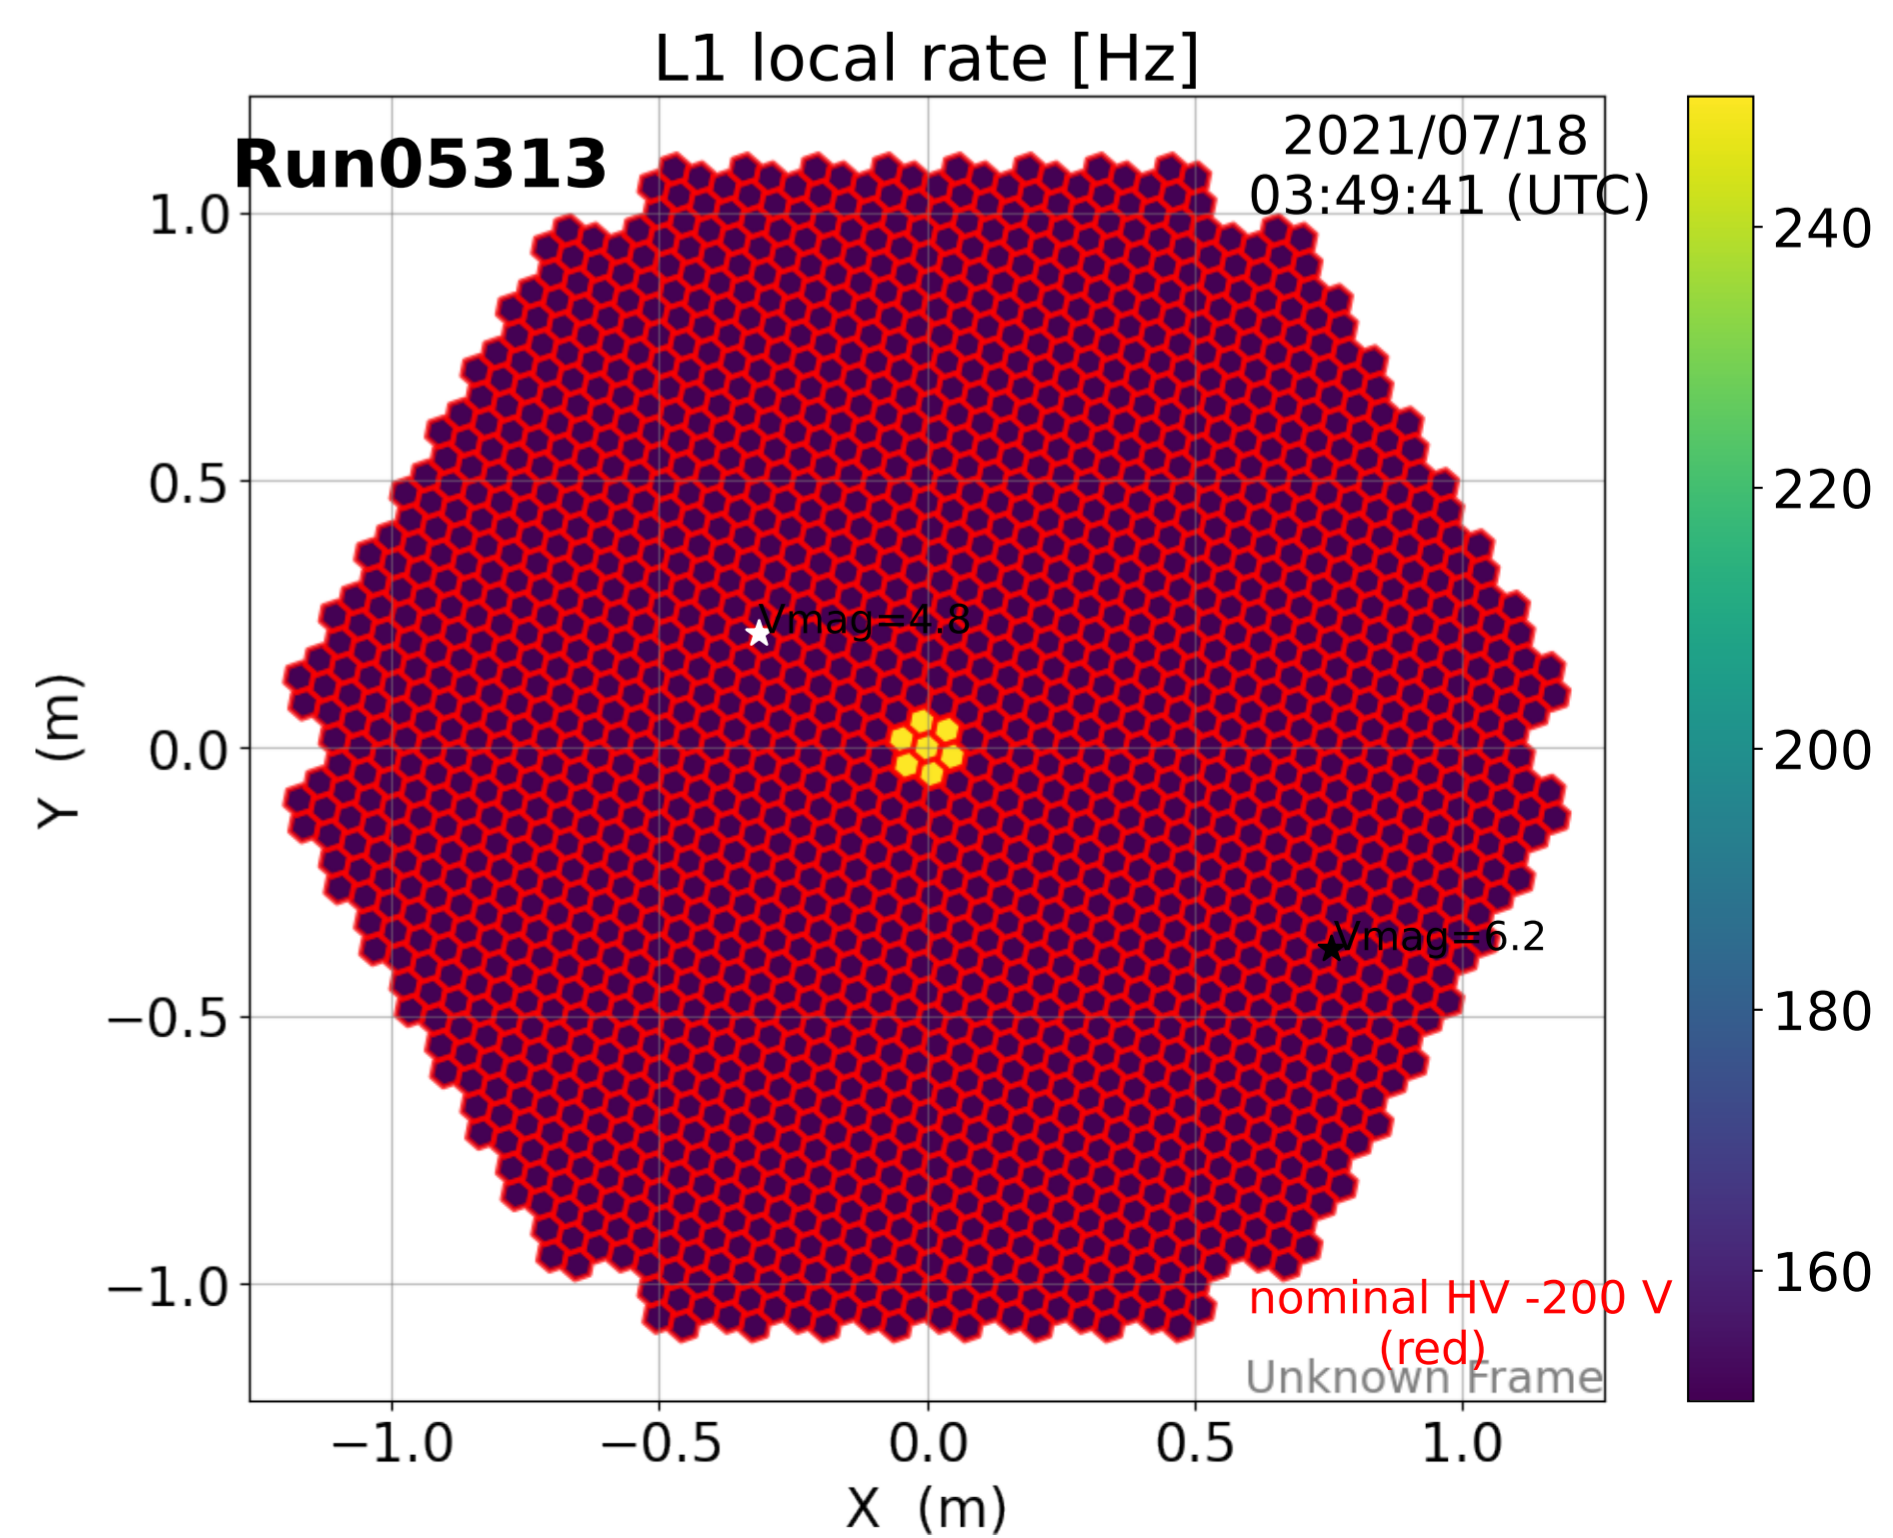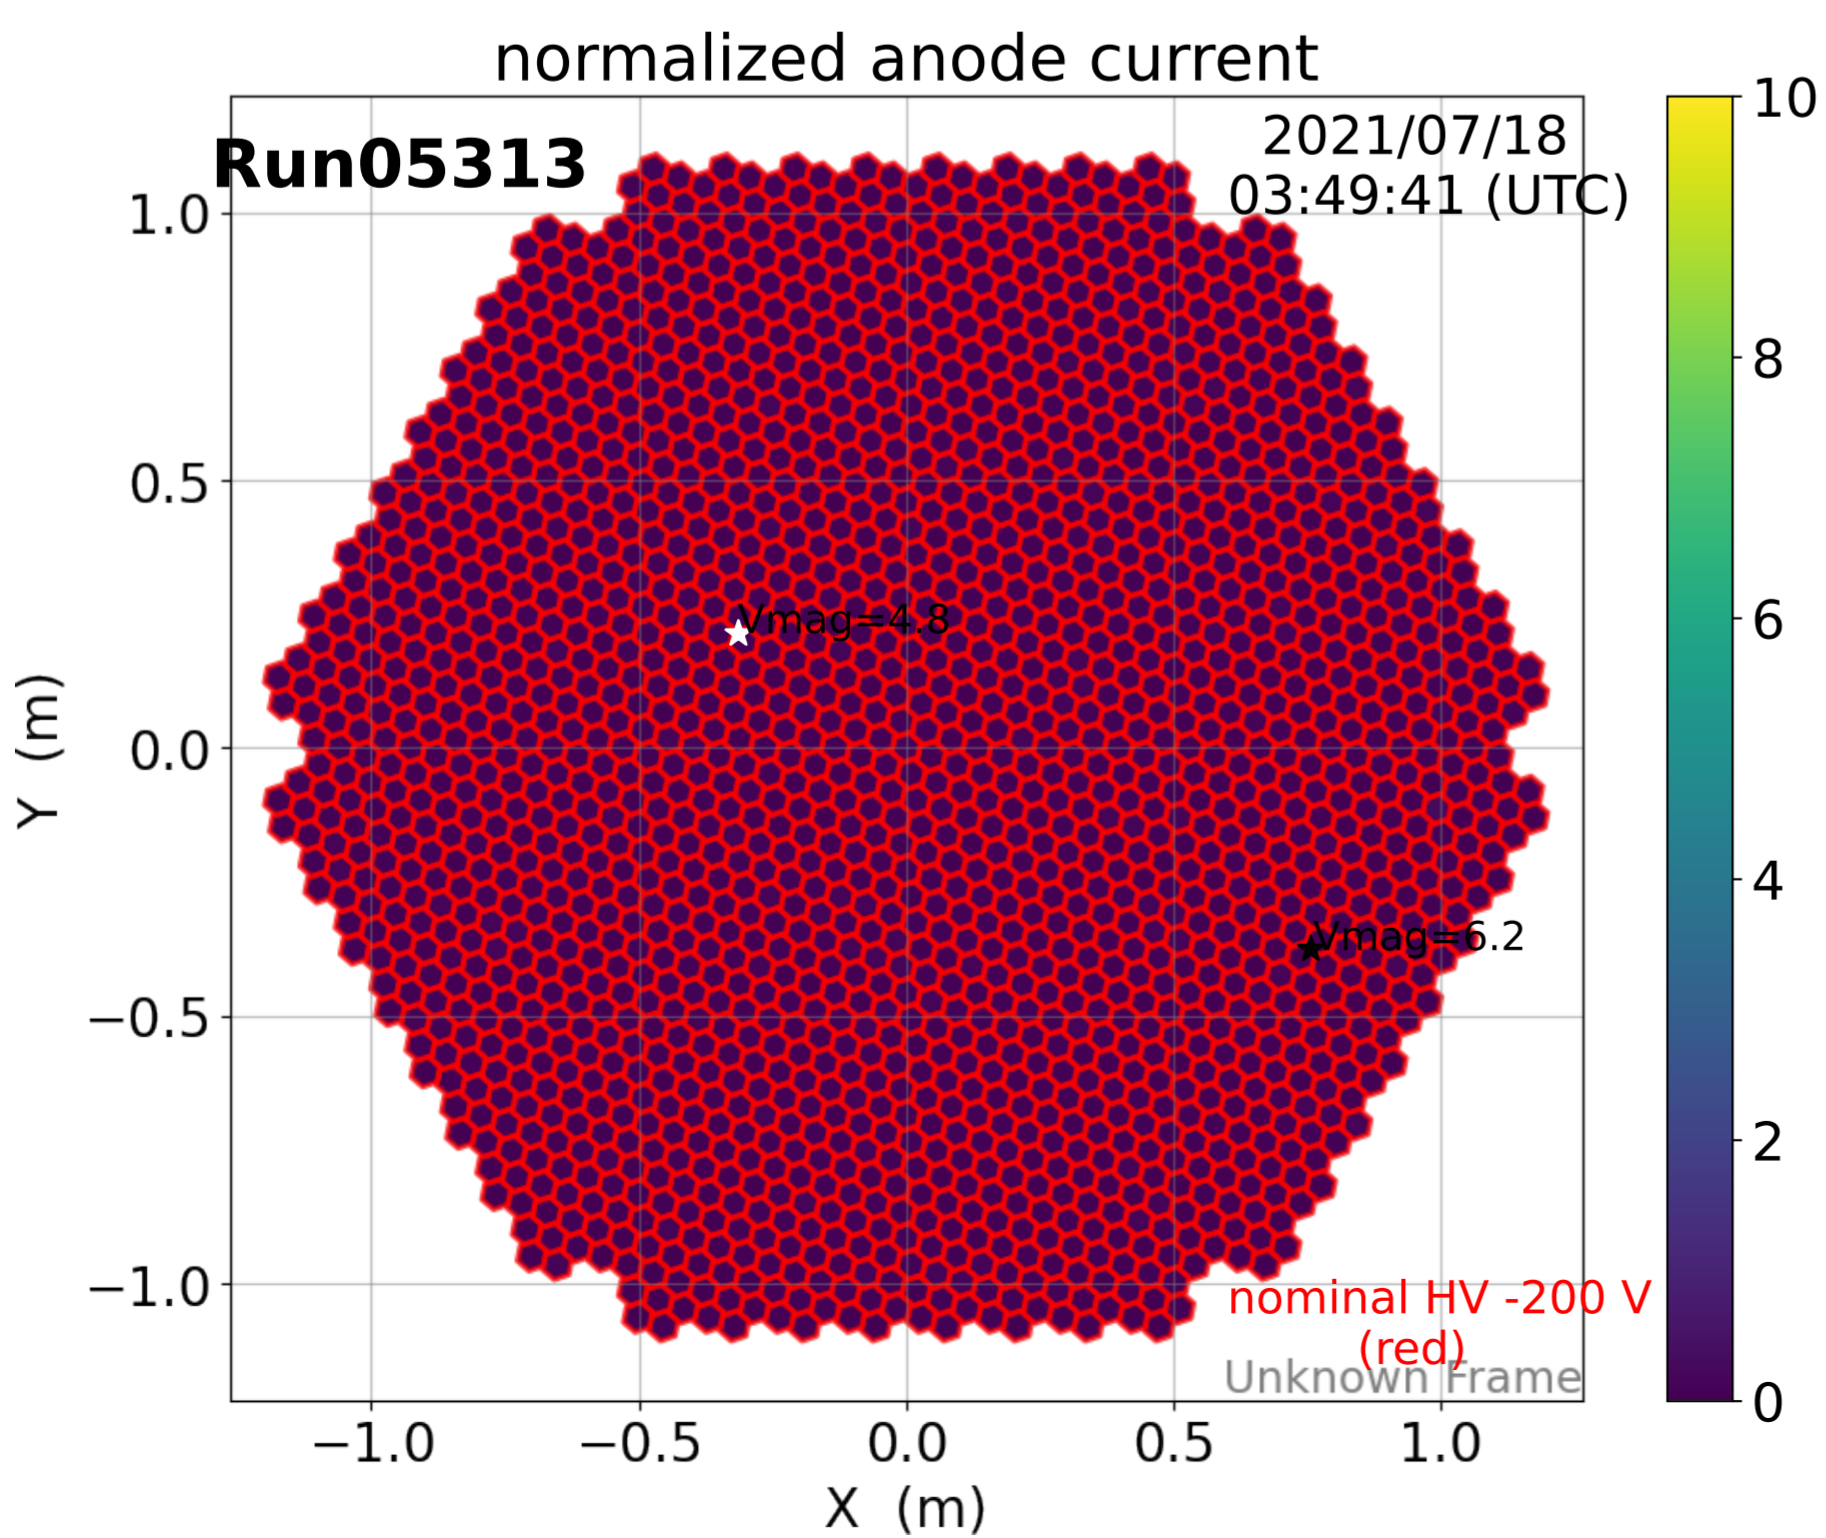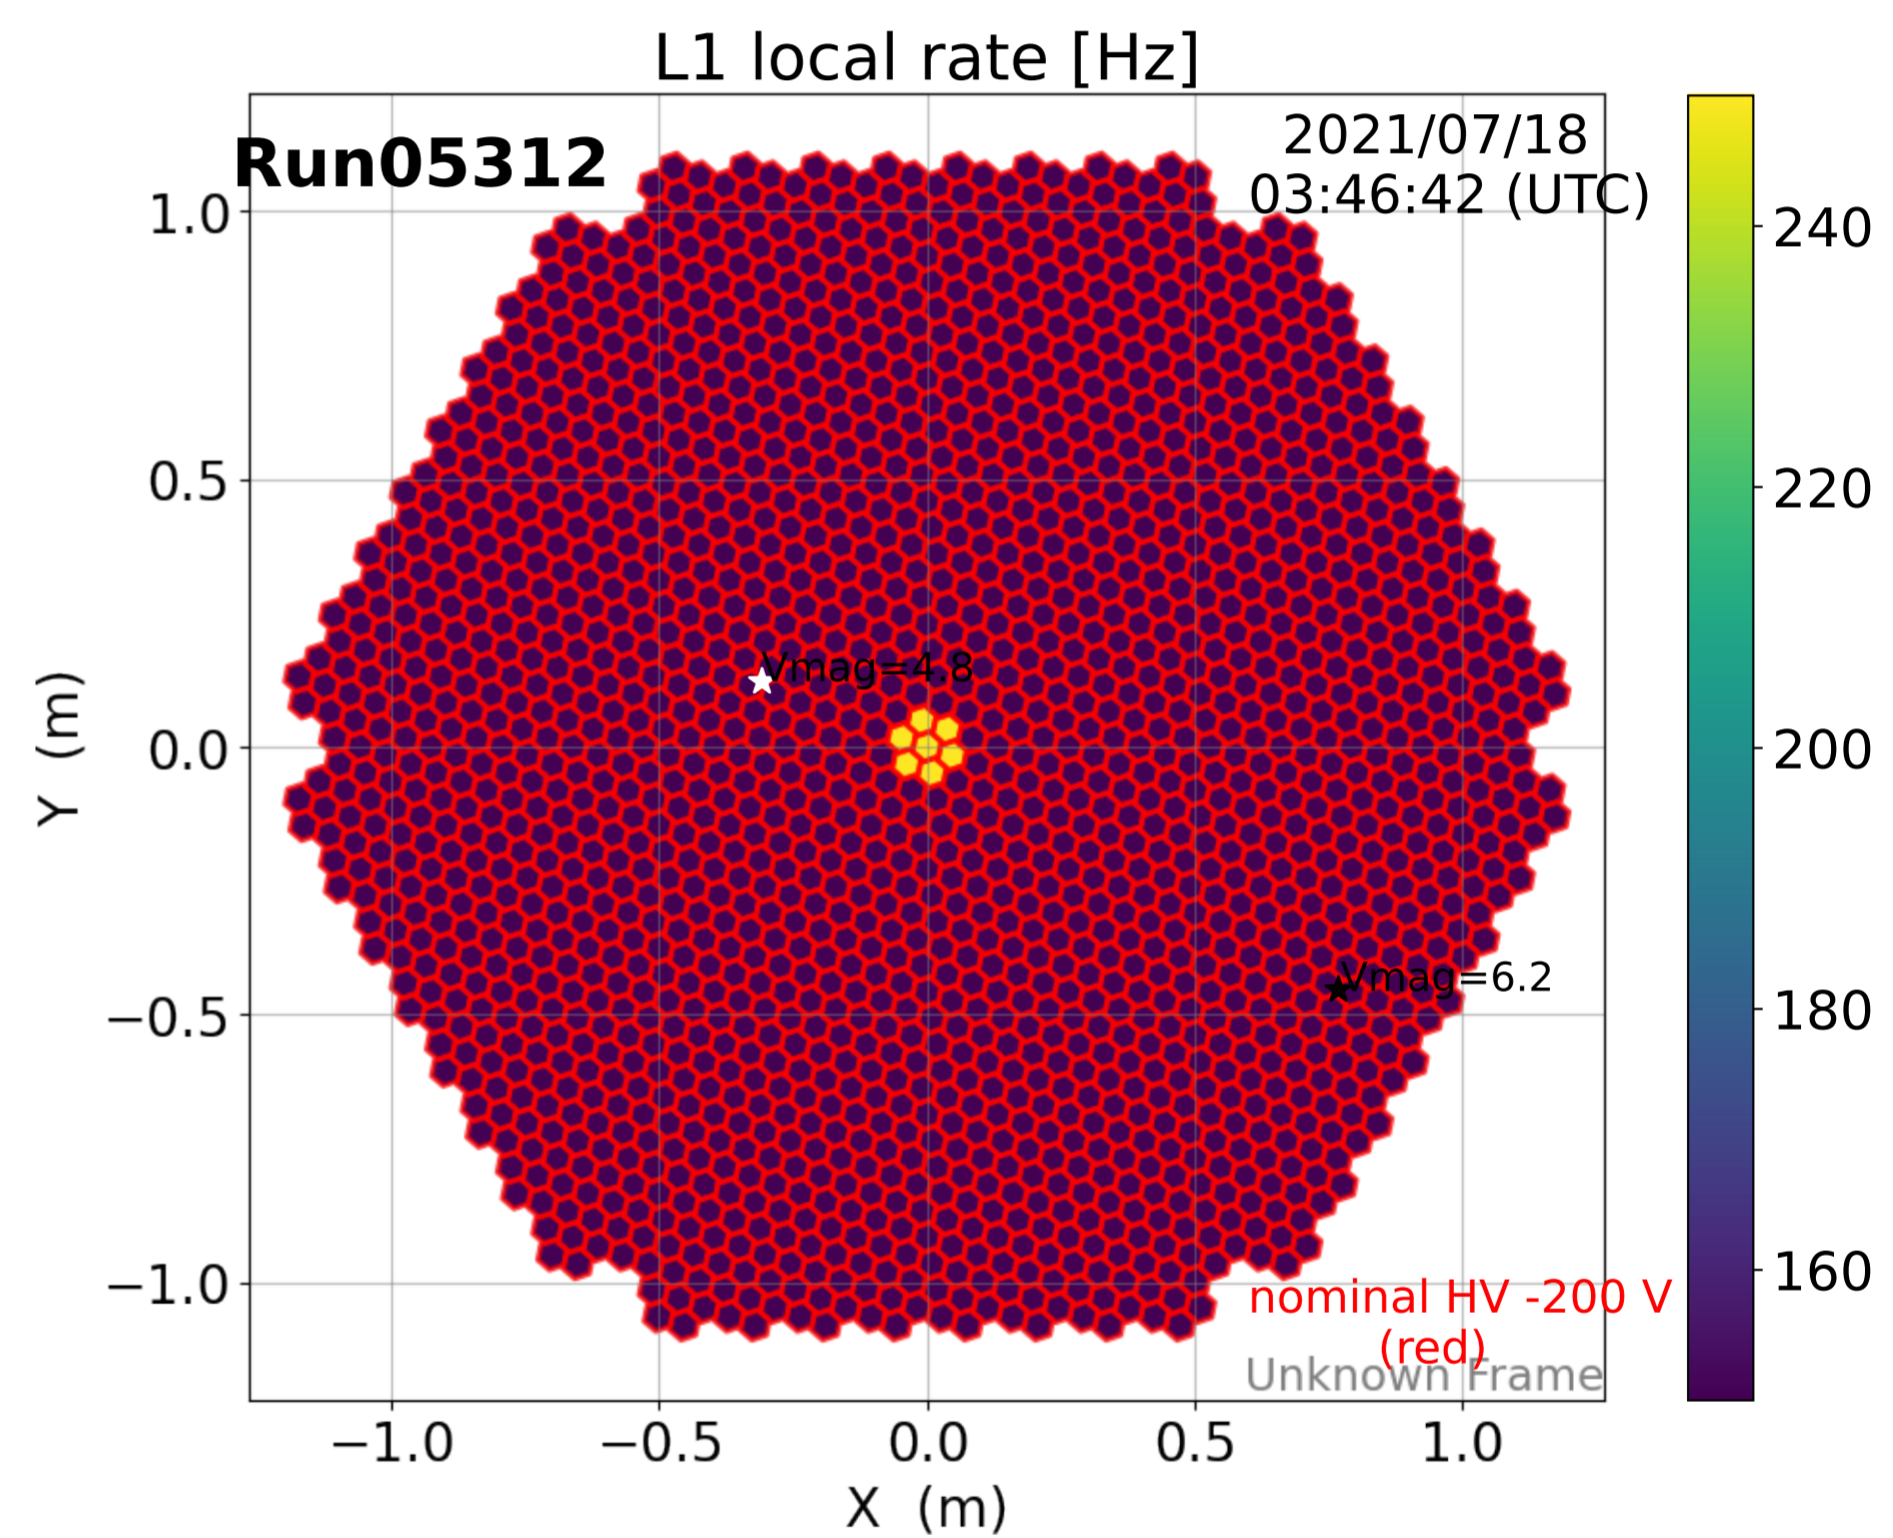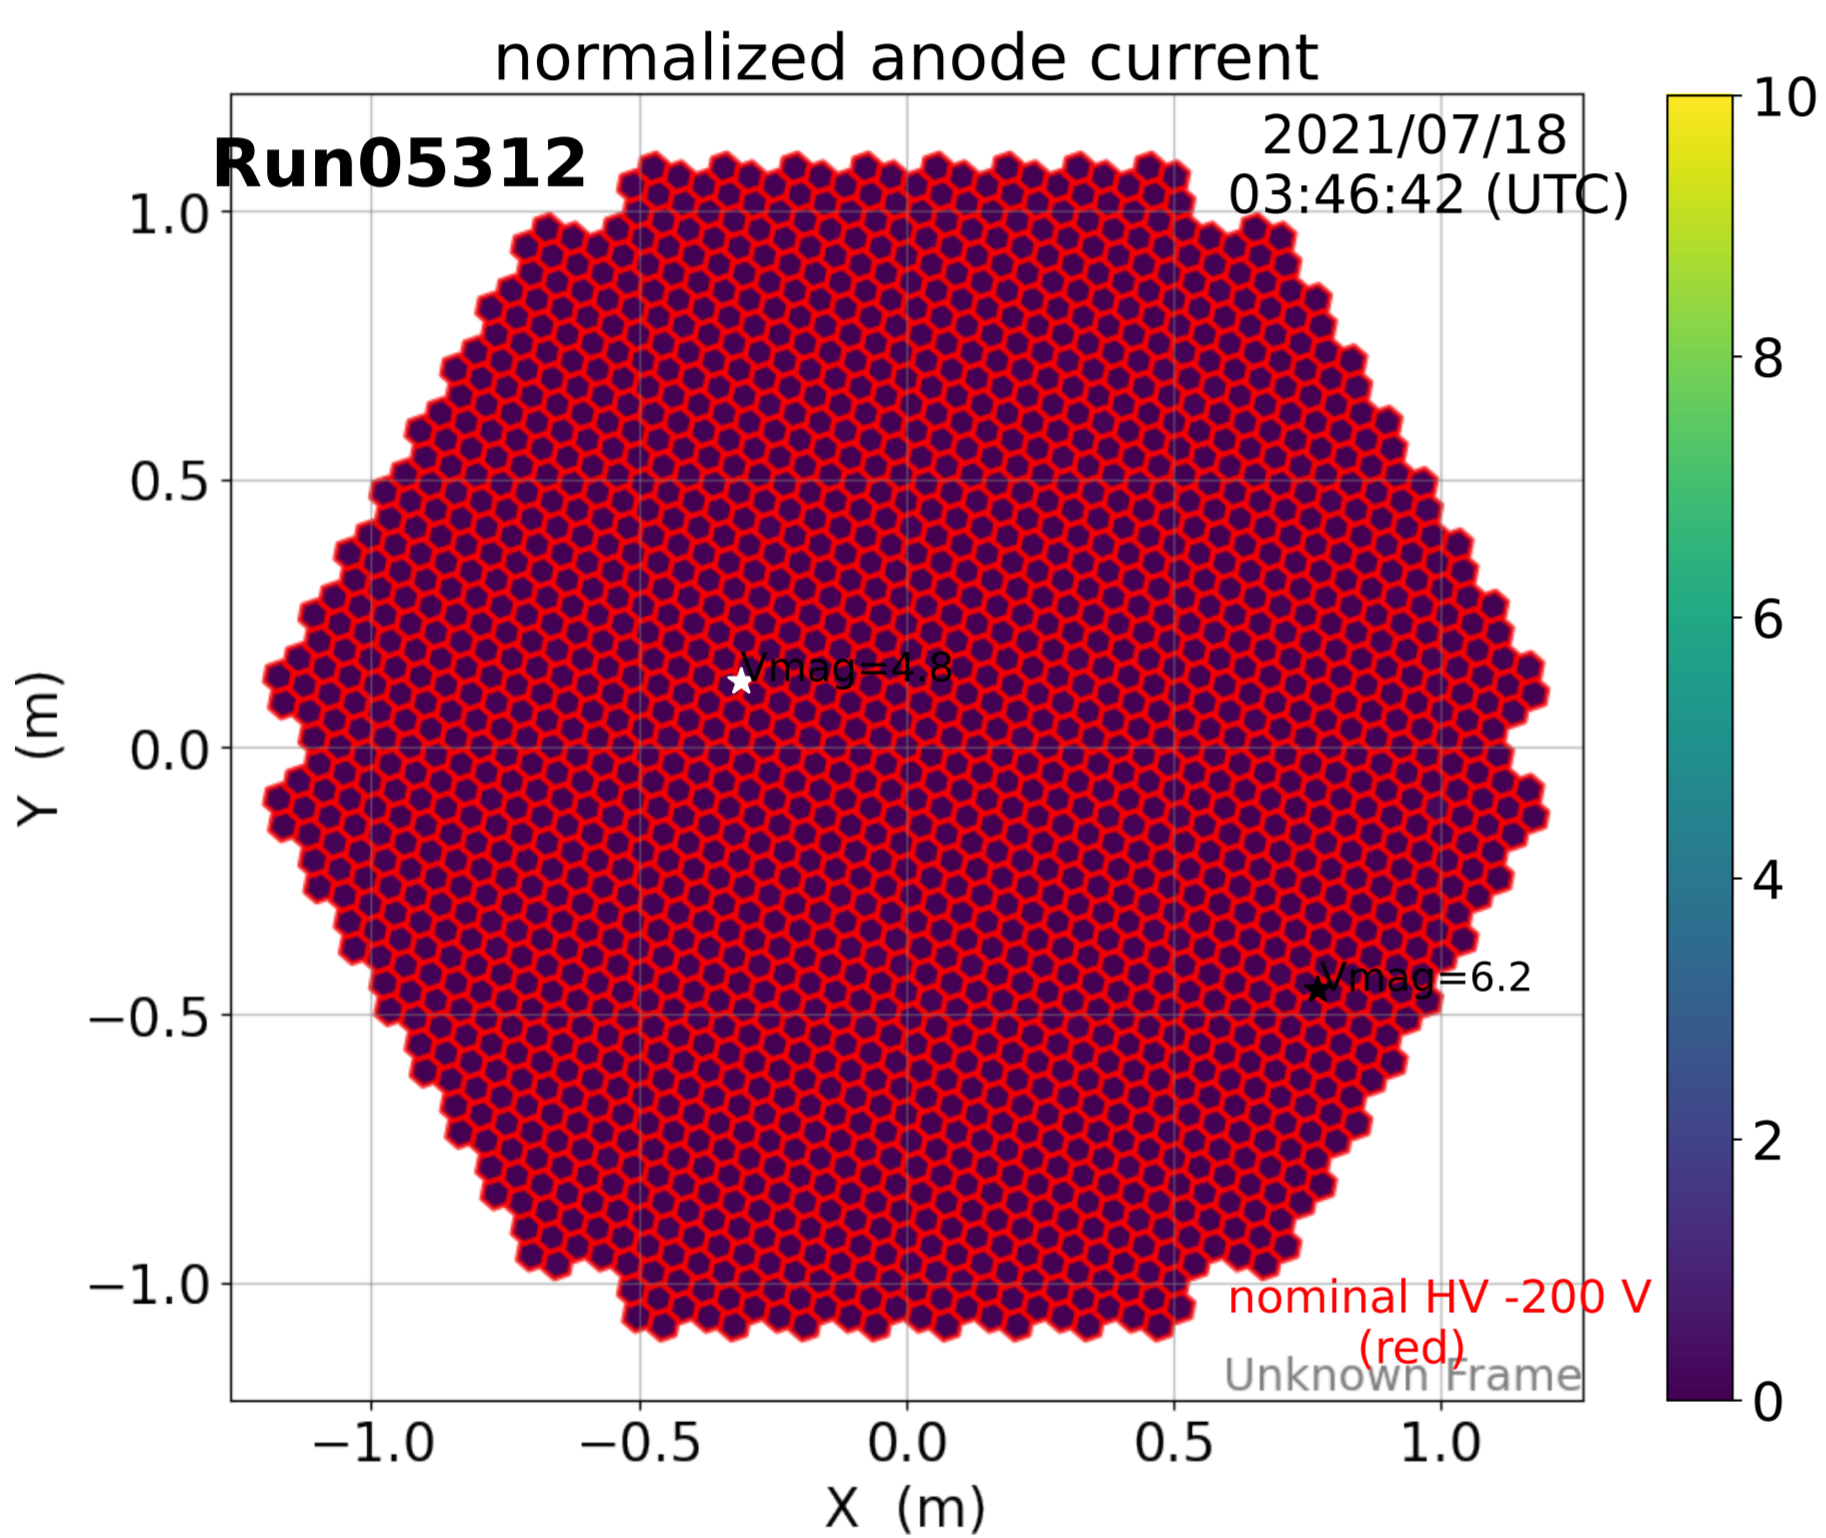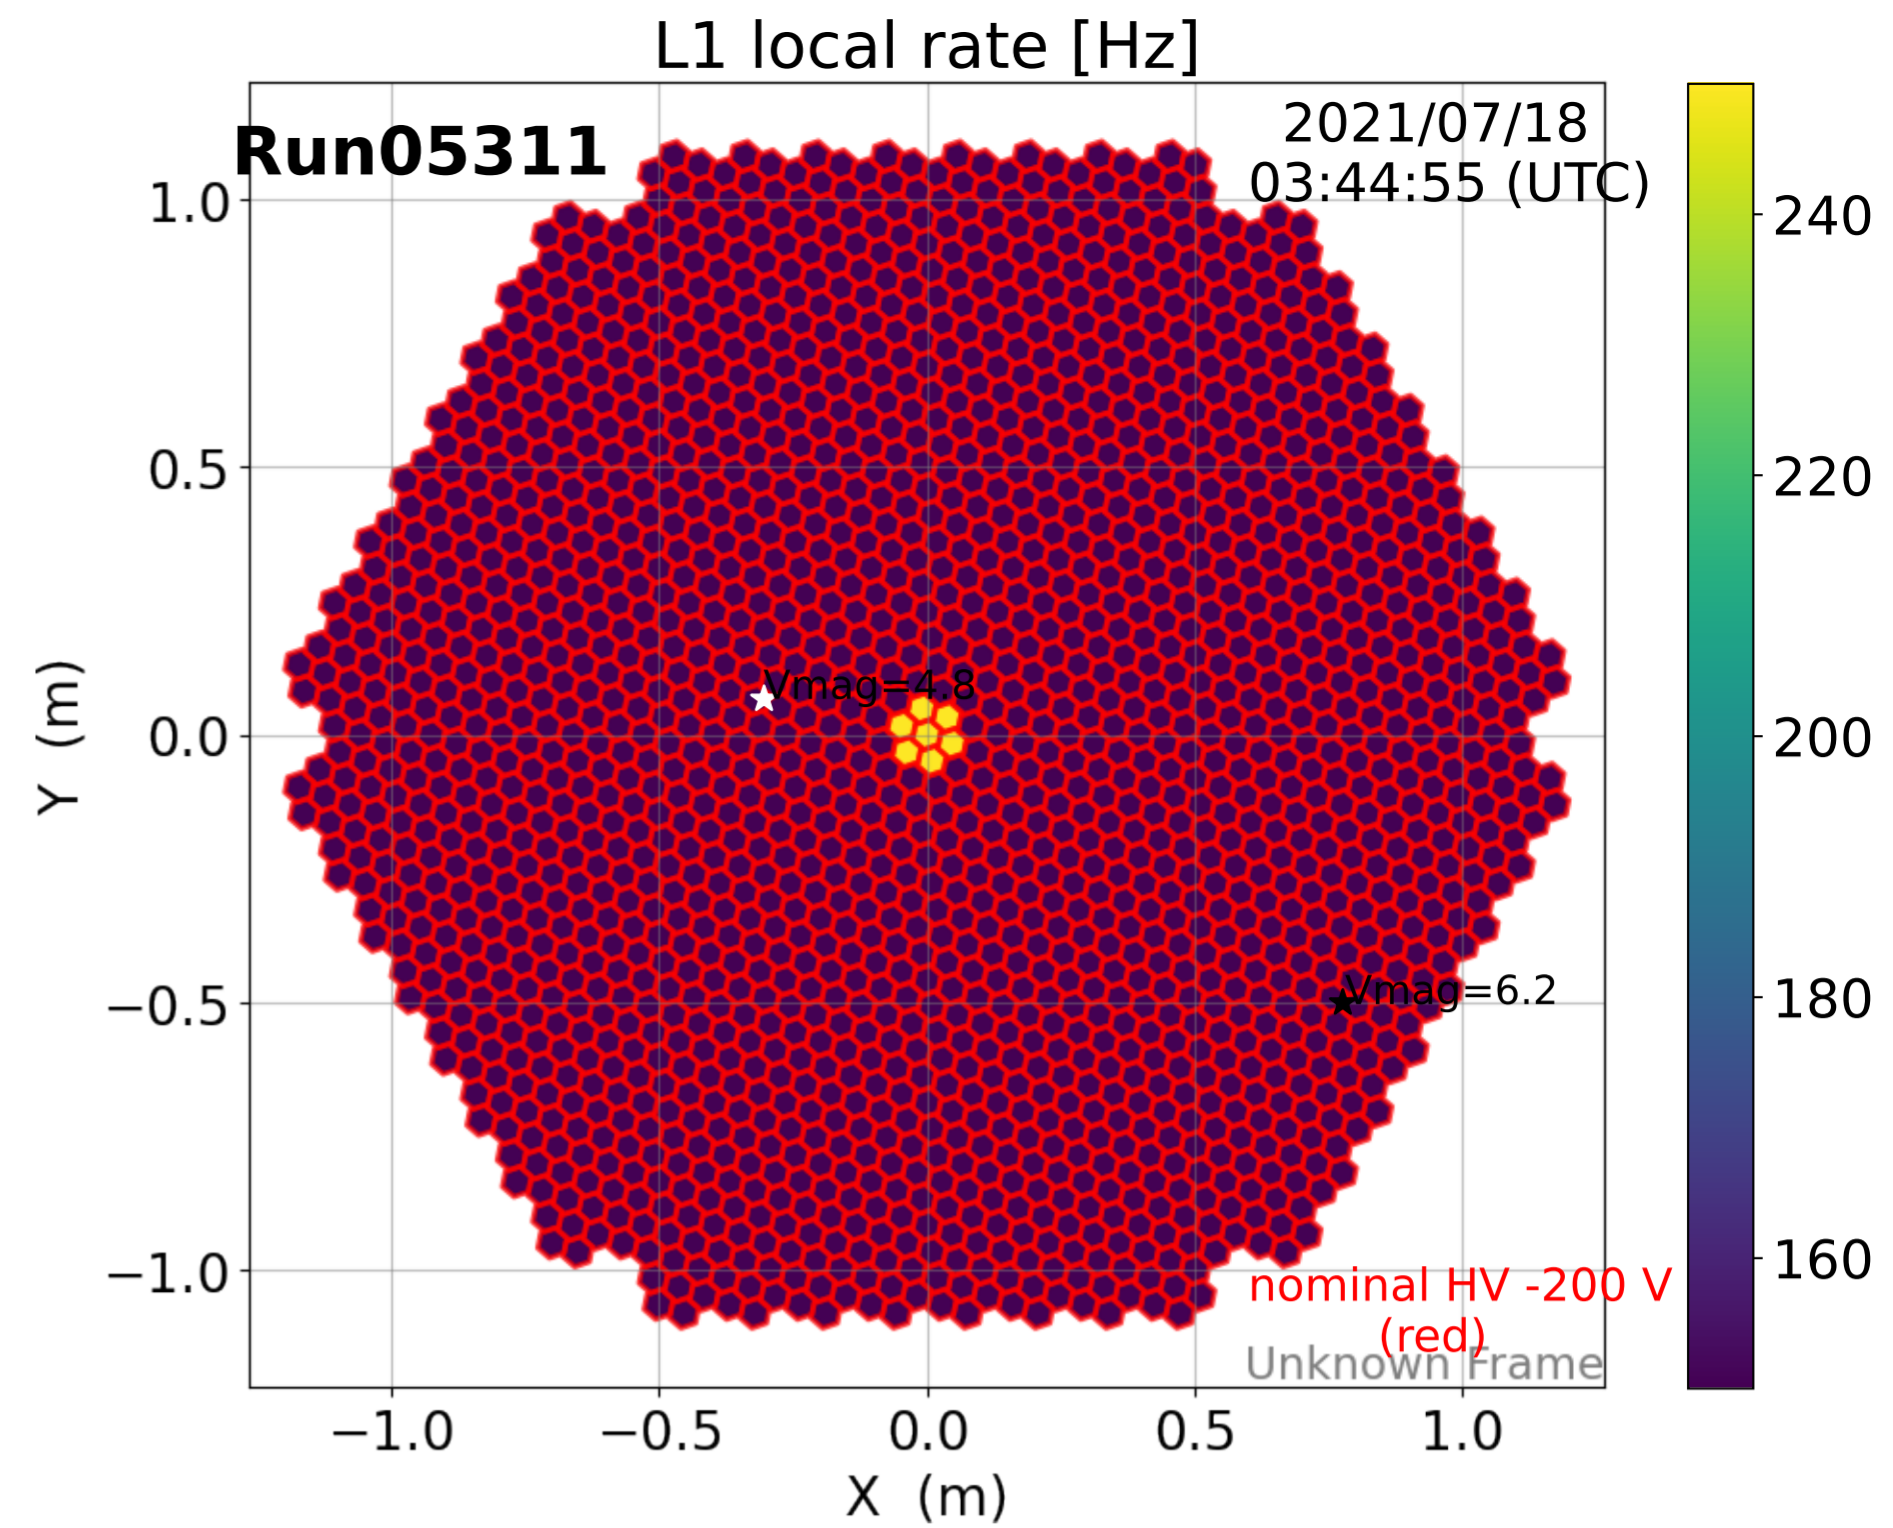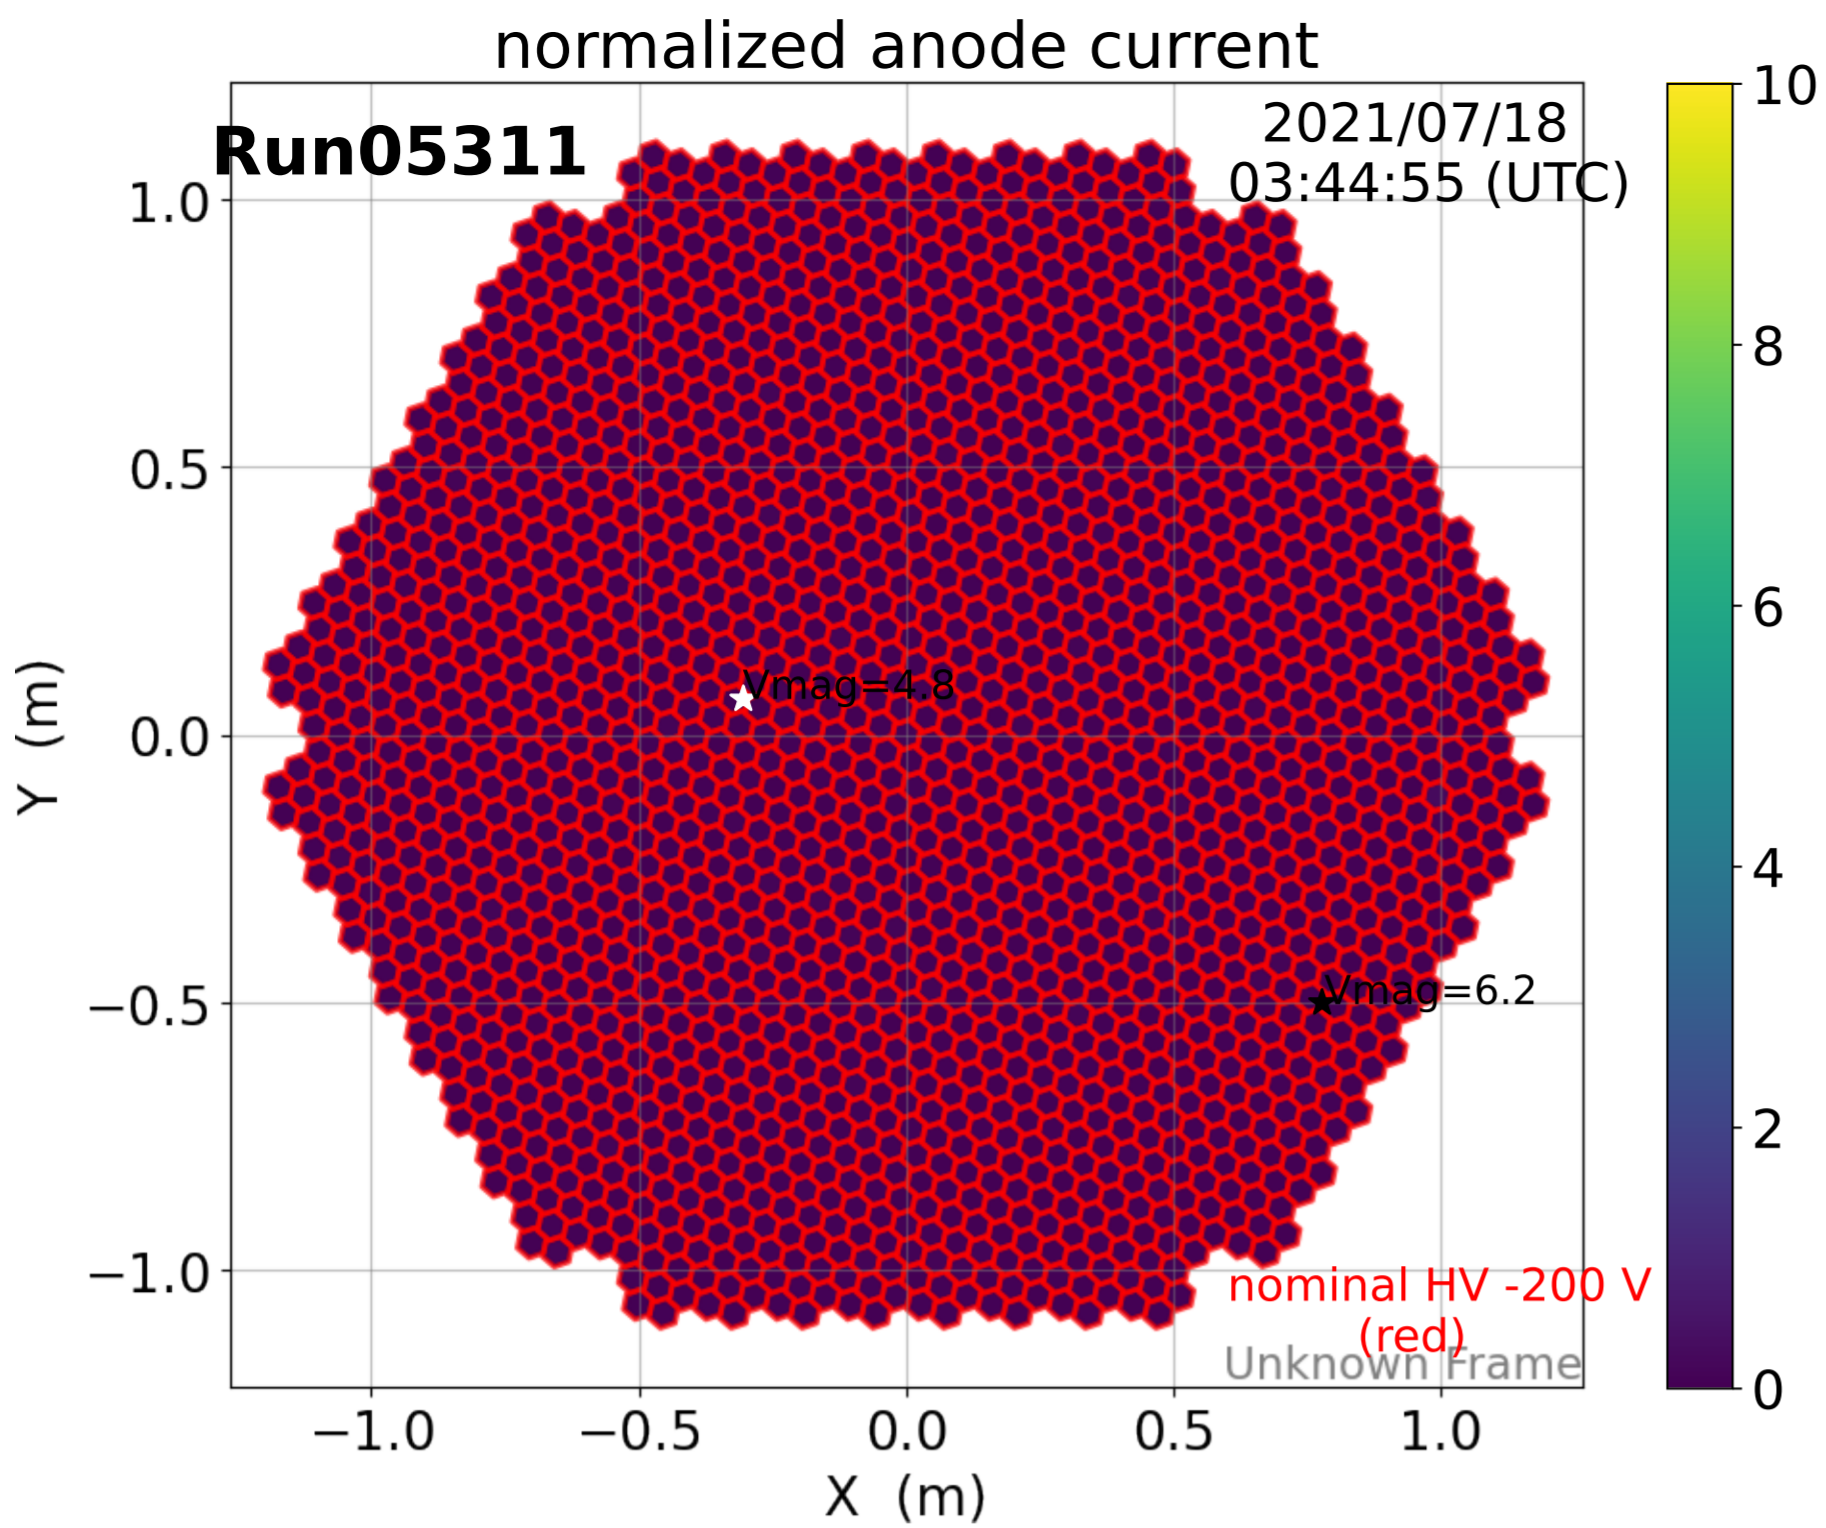




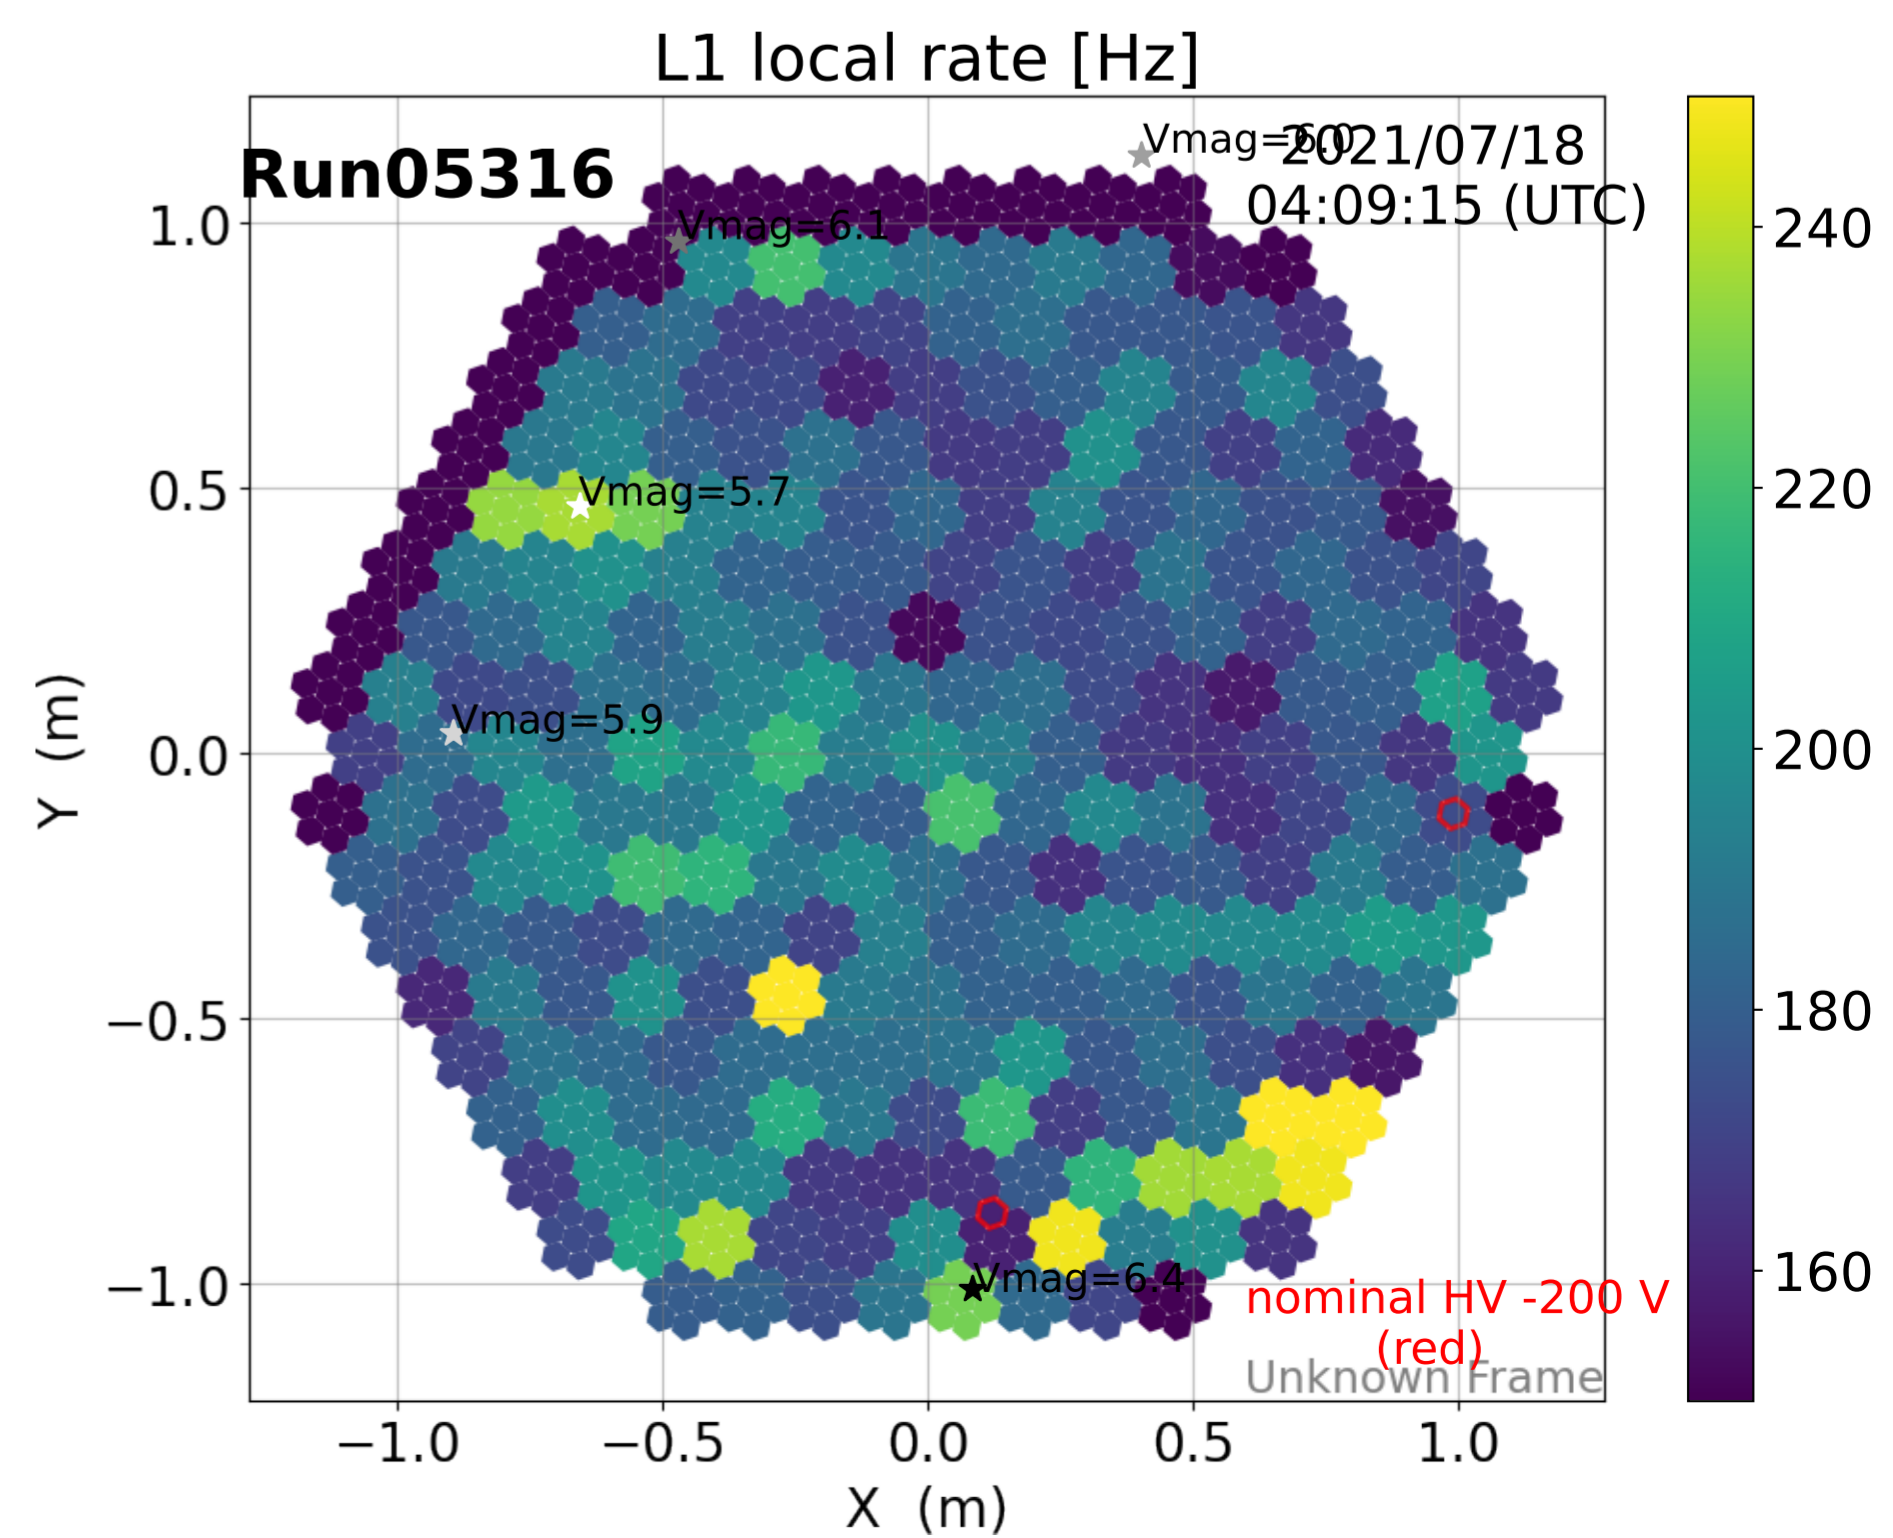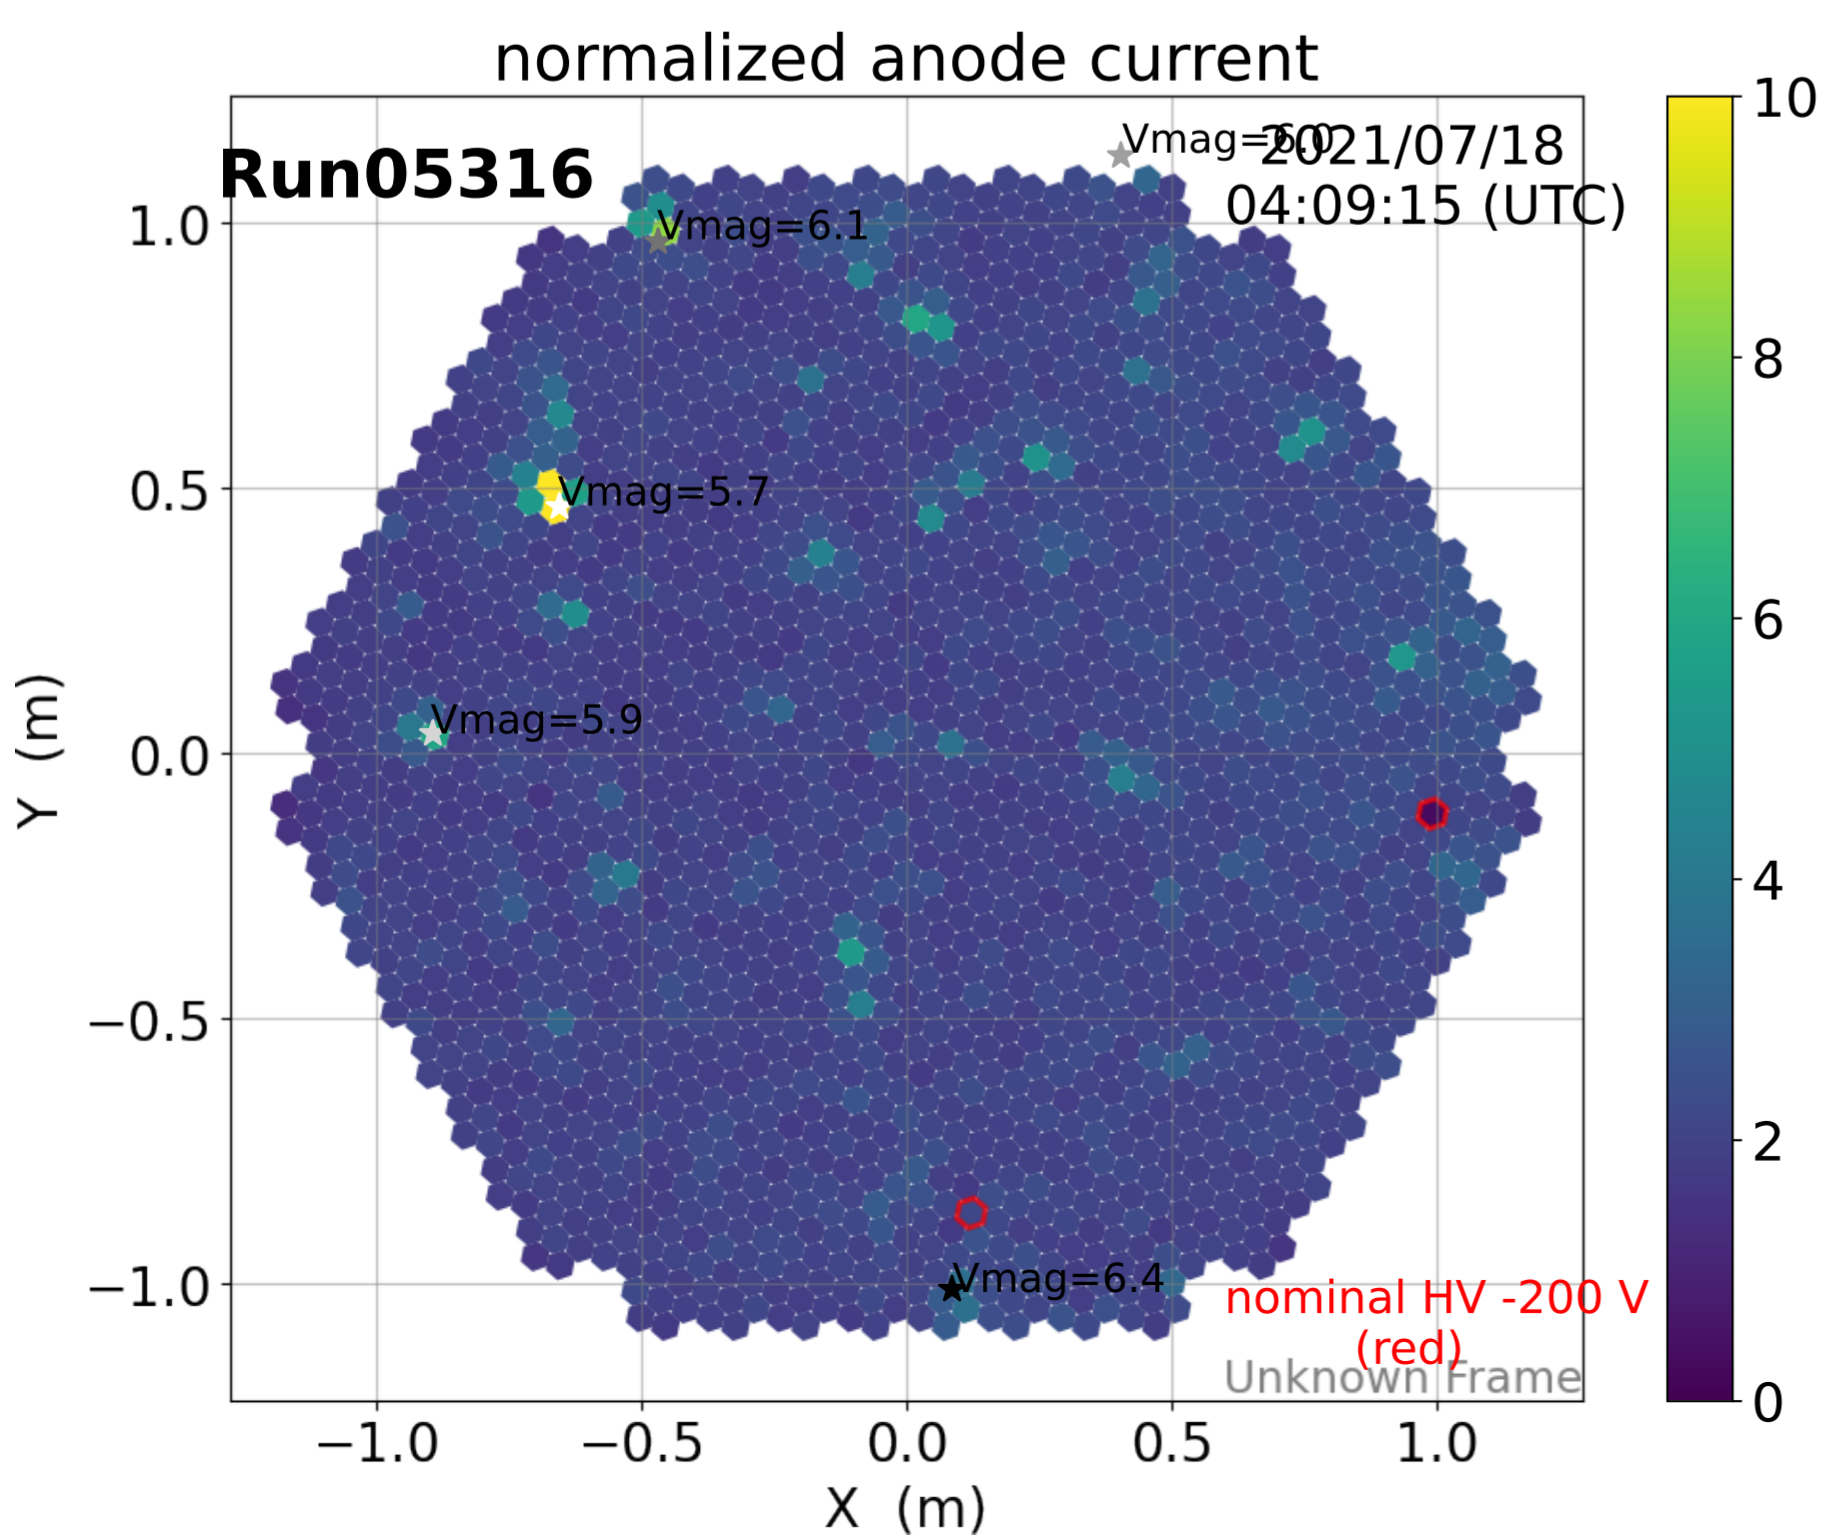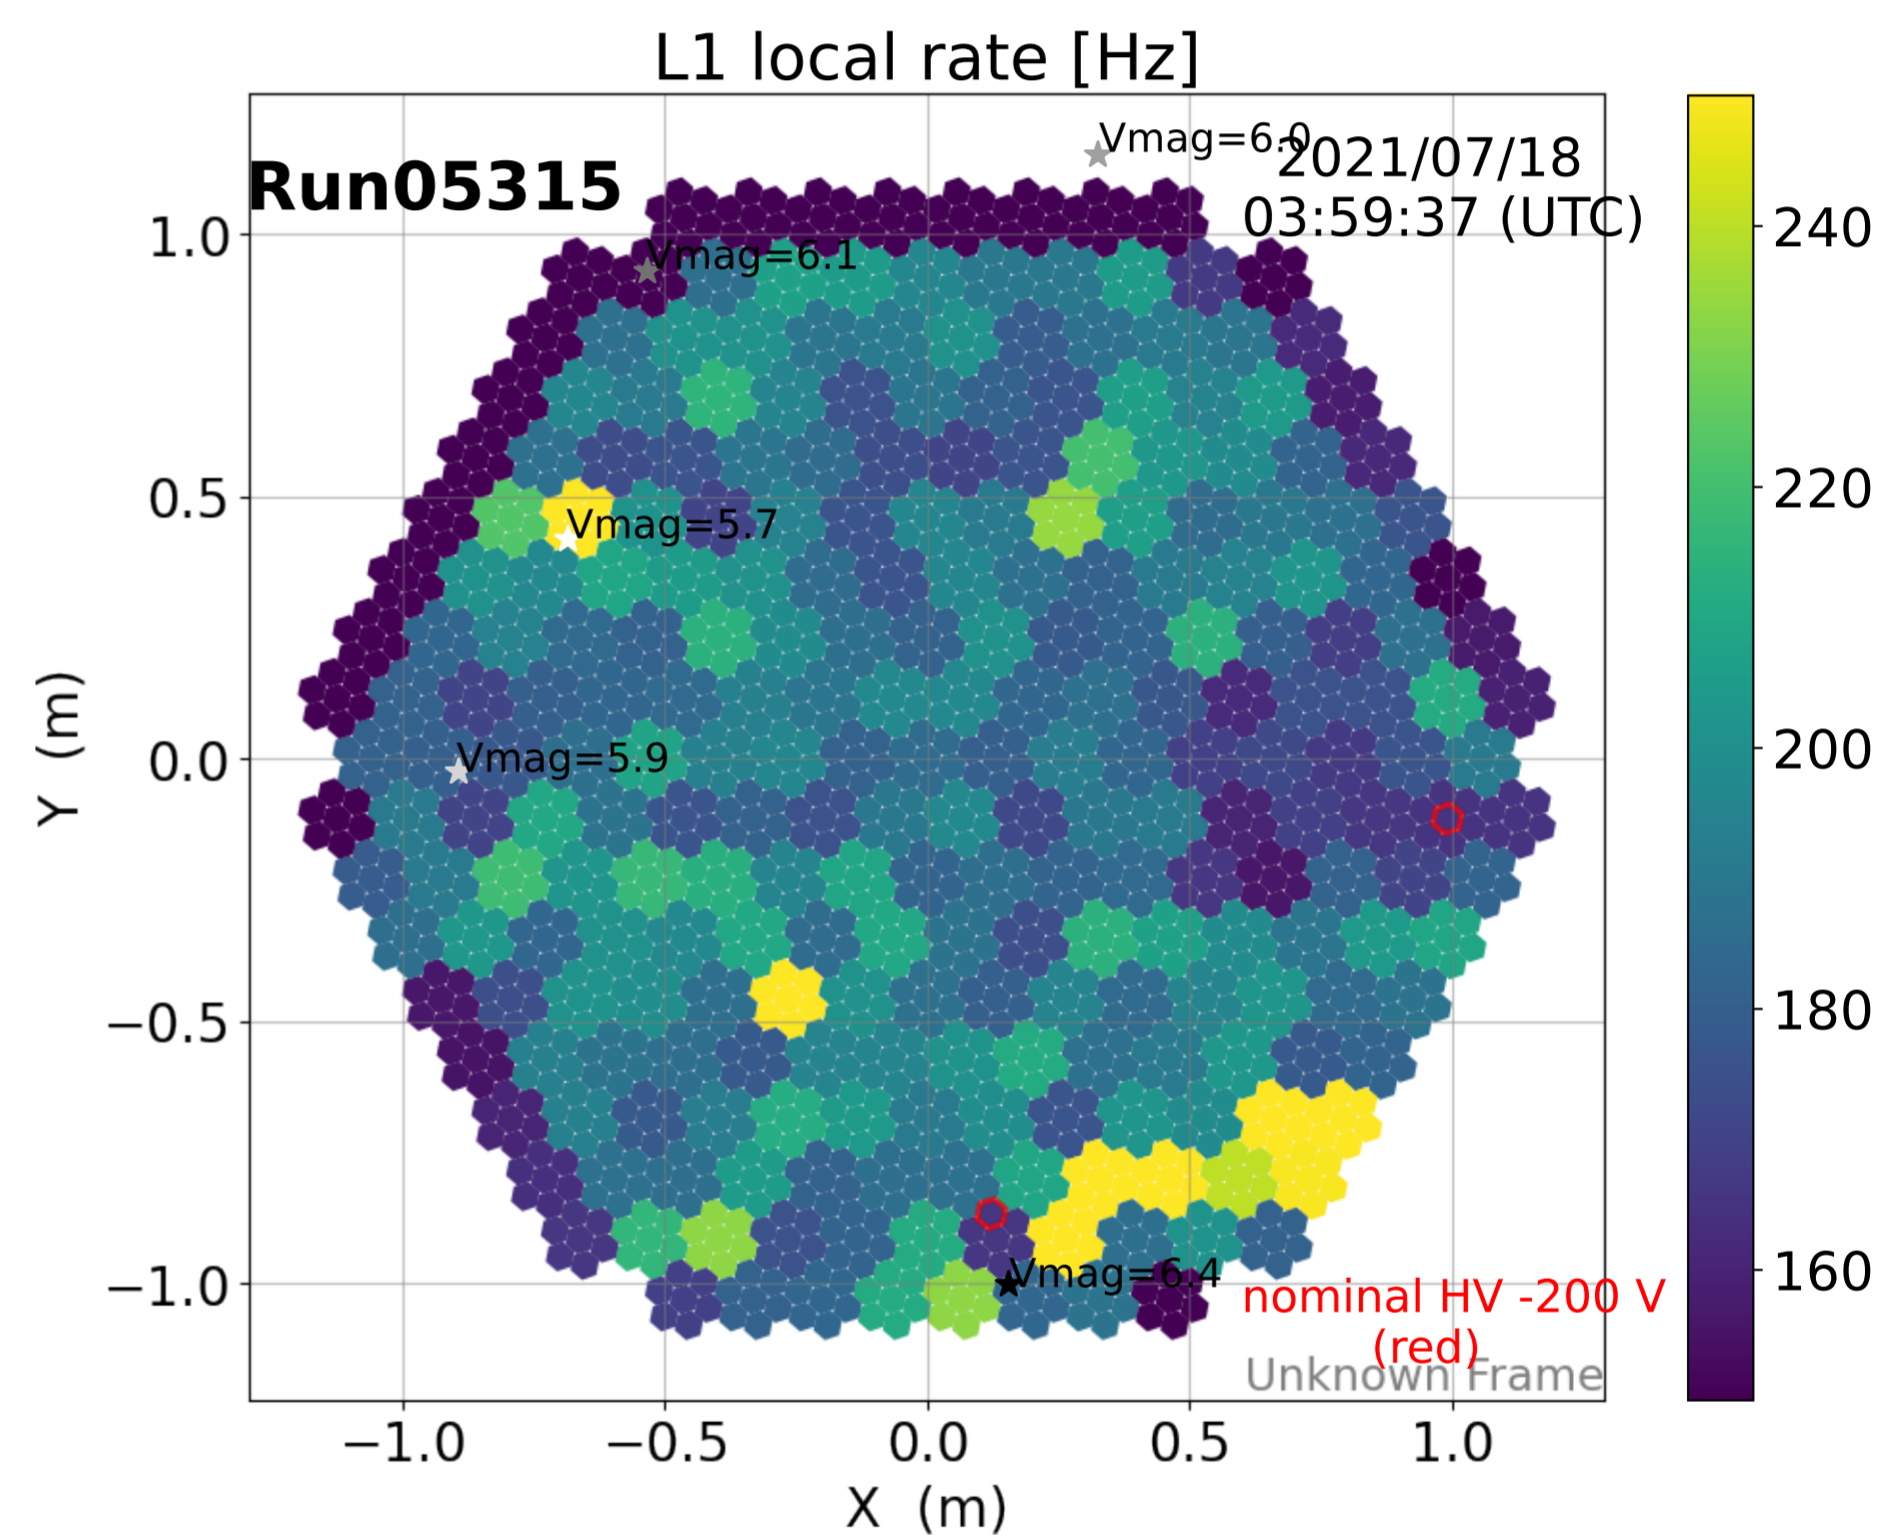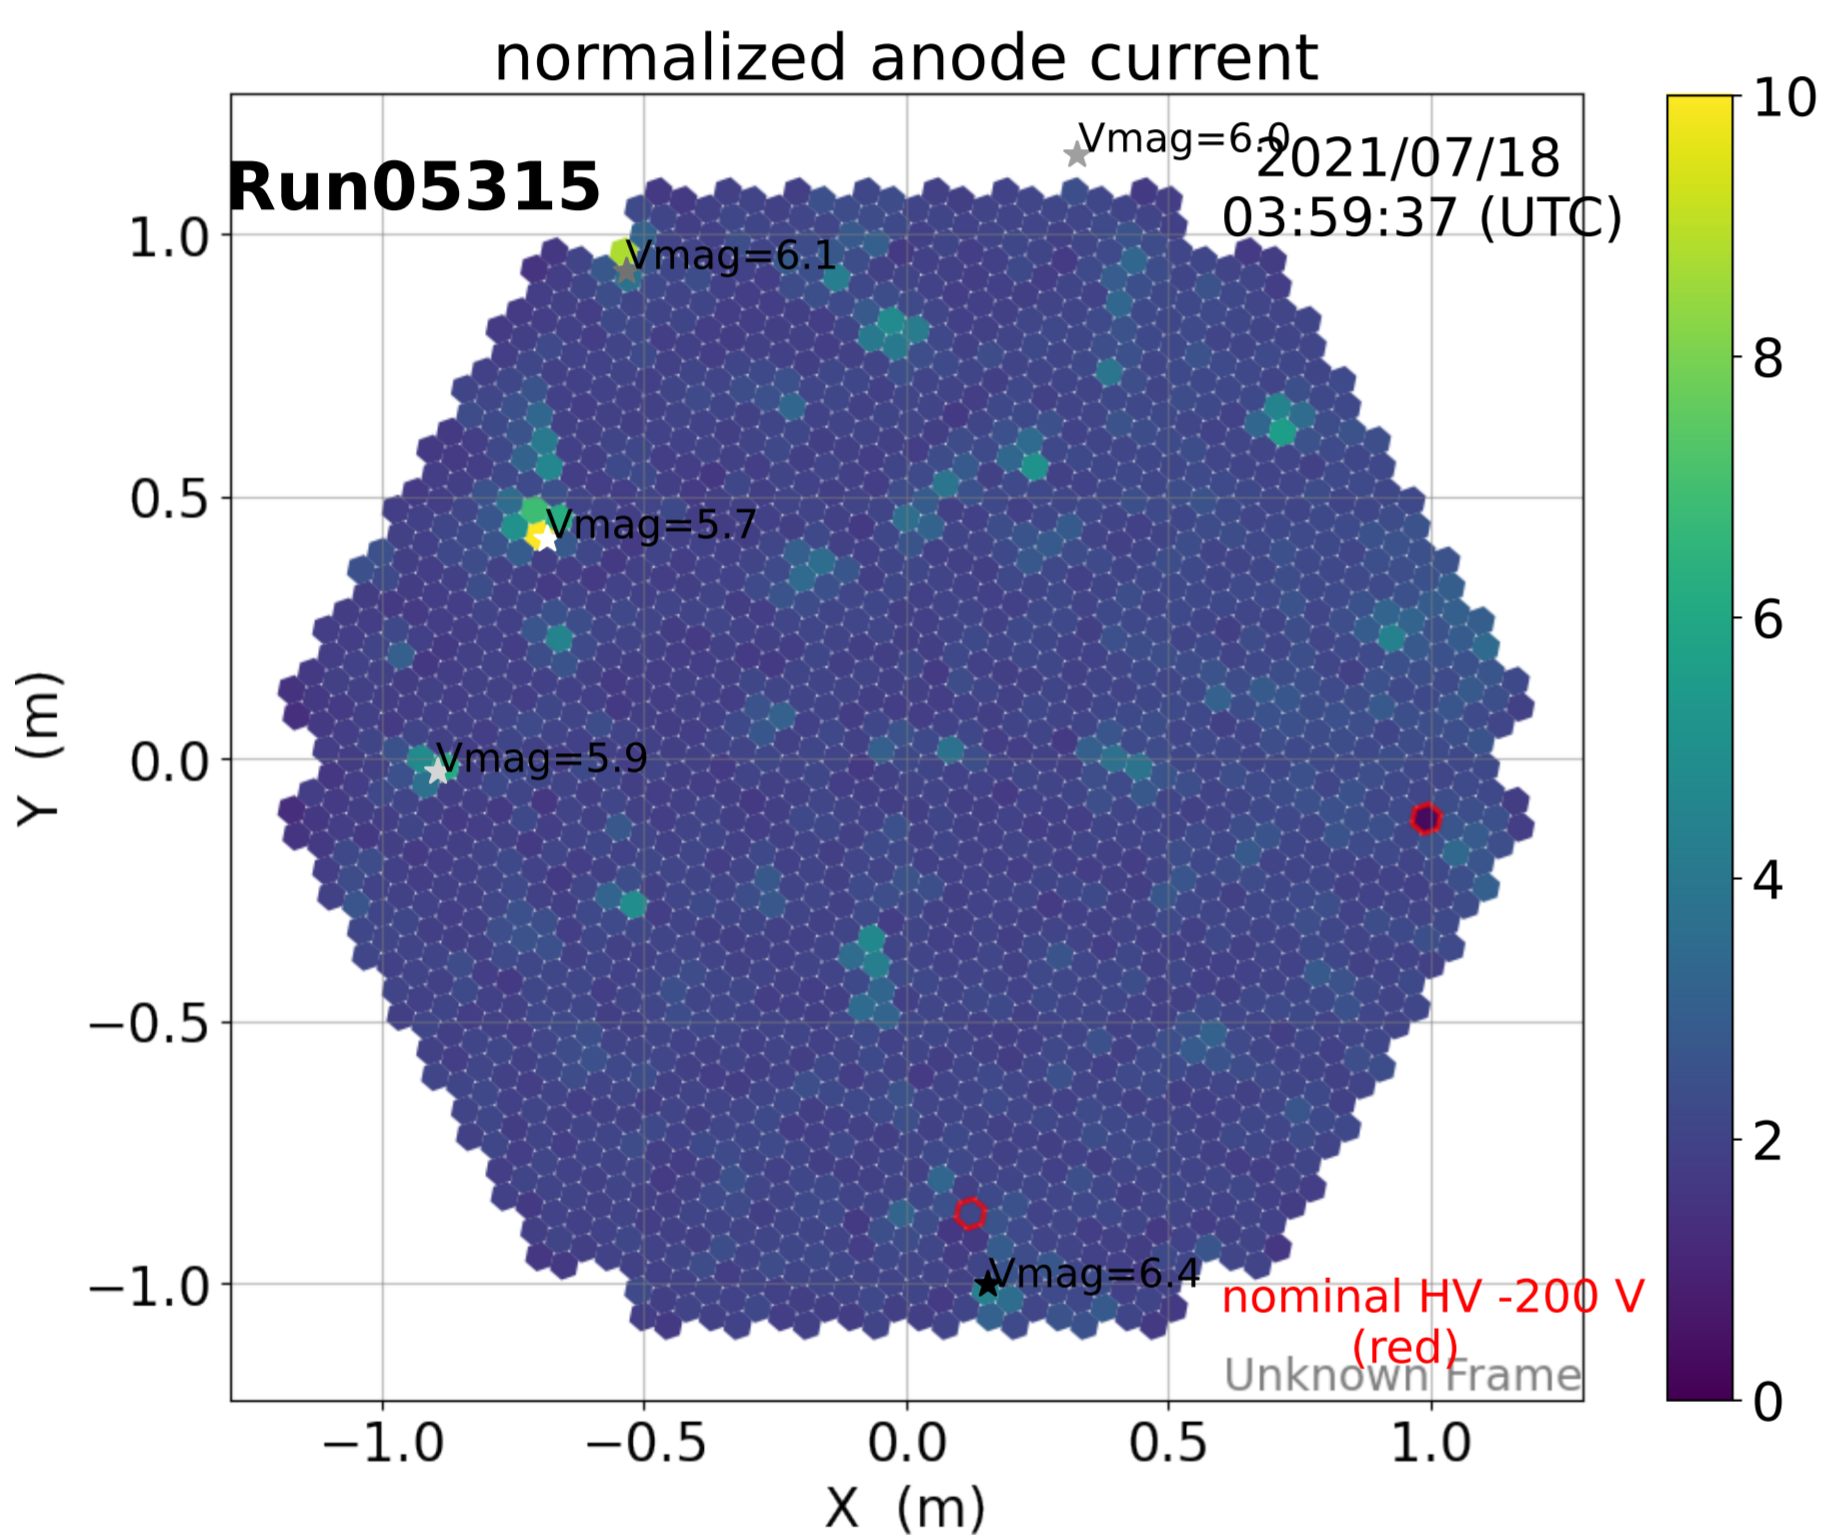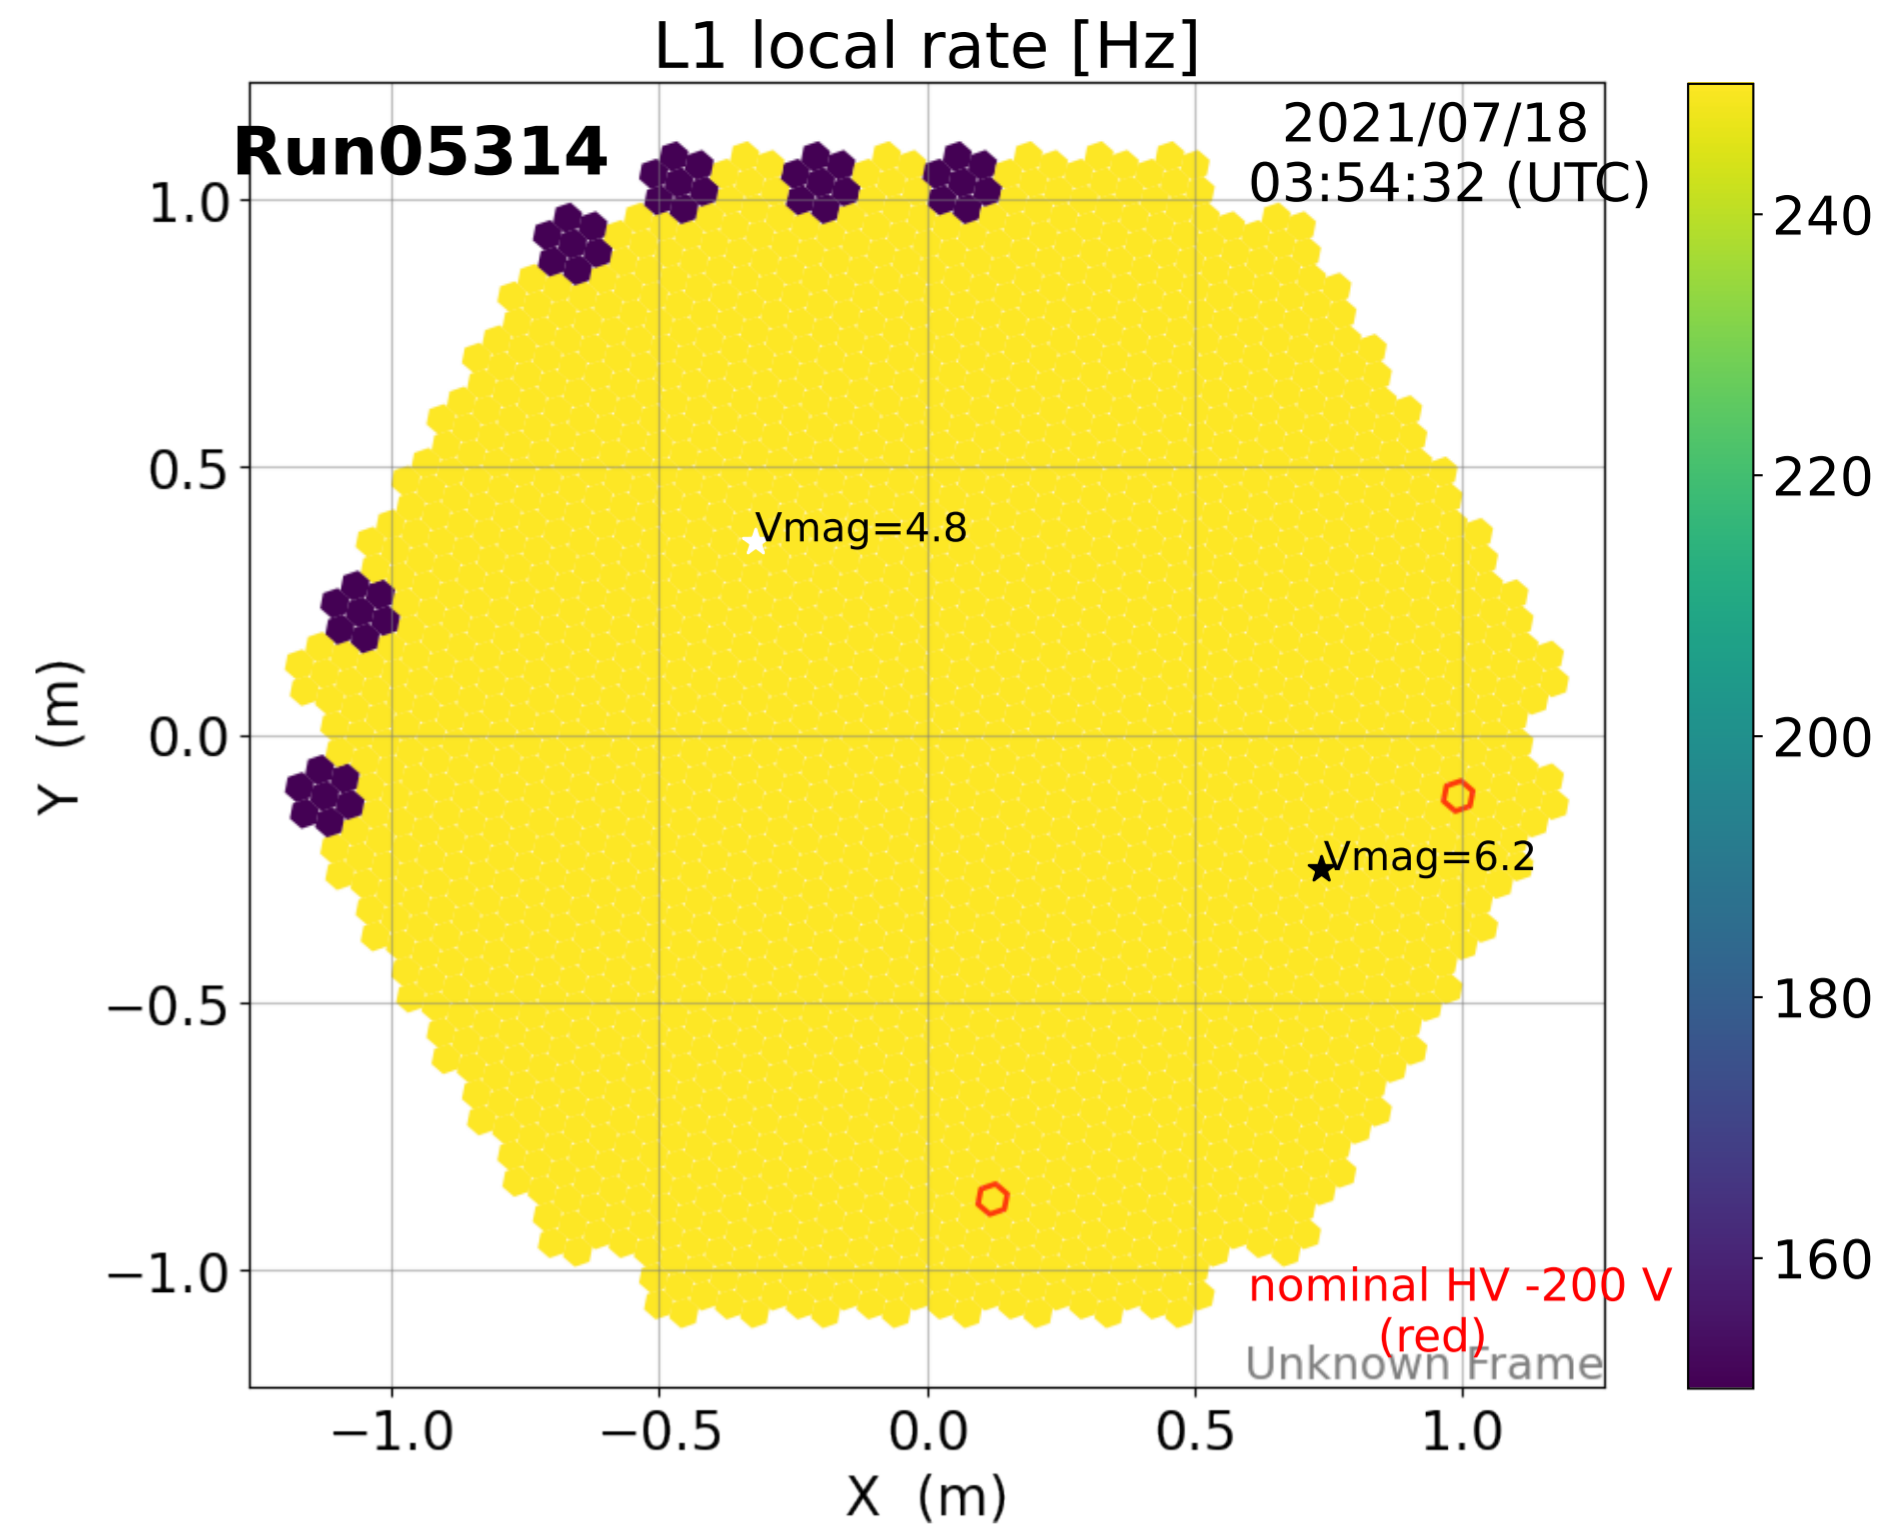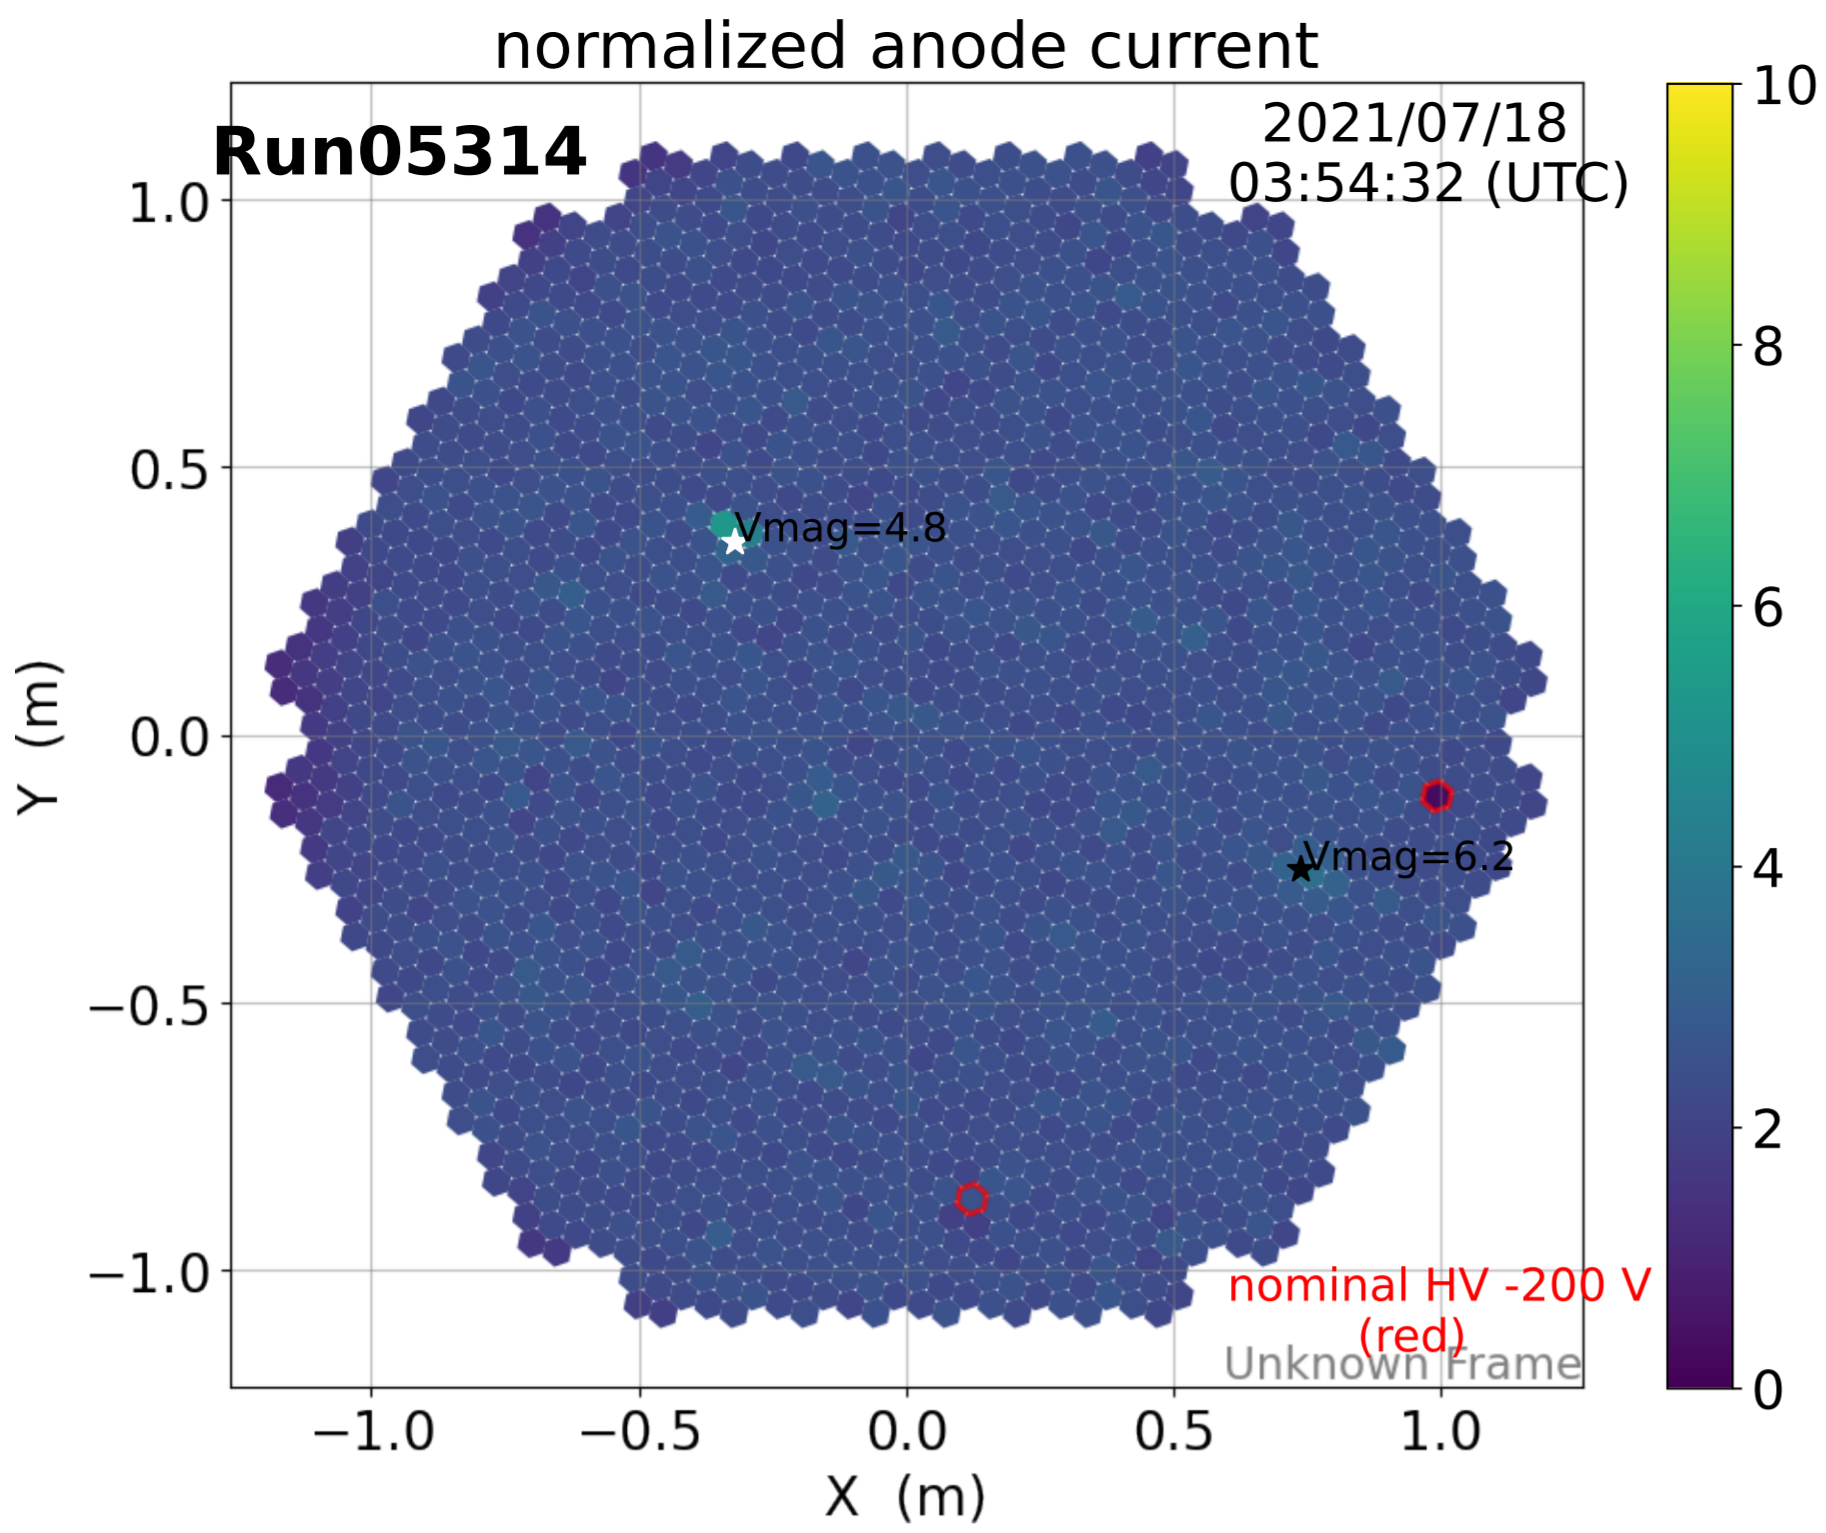





normalized anode current

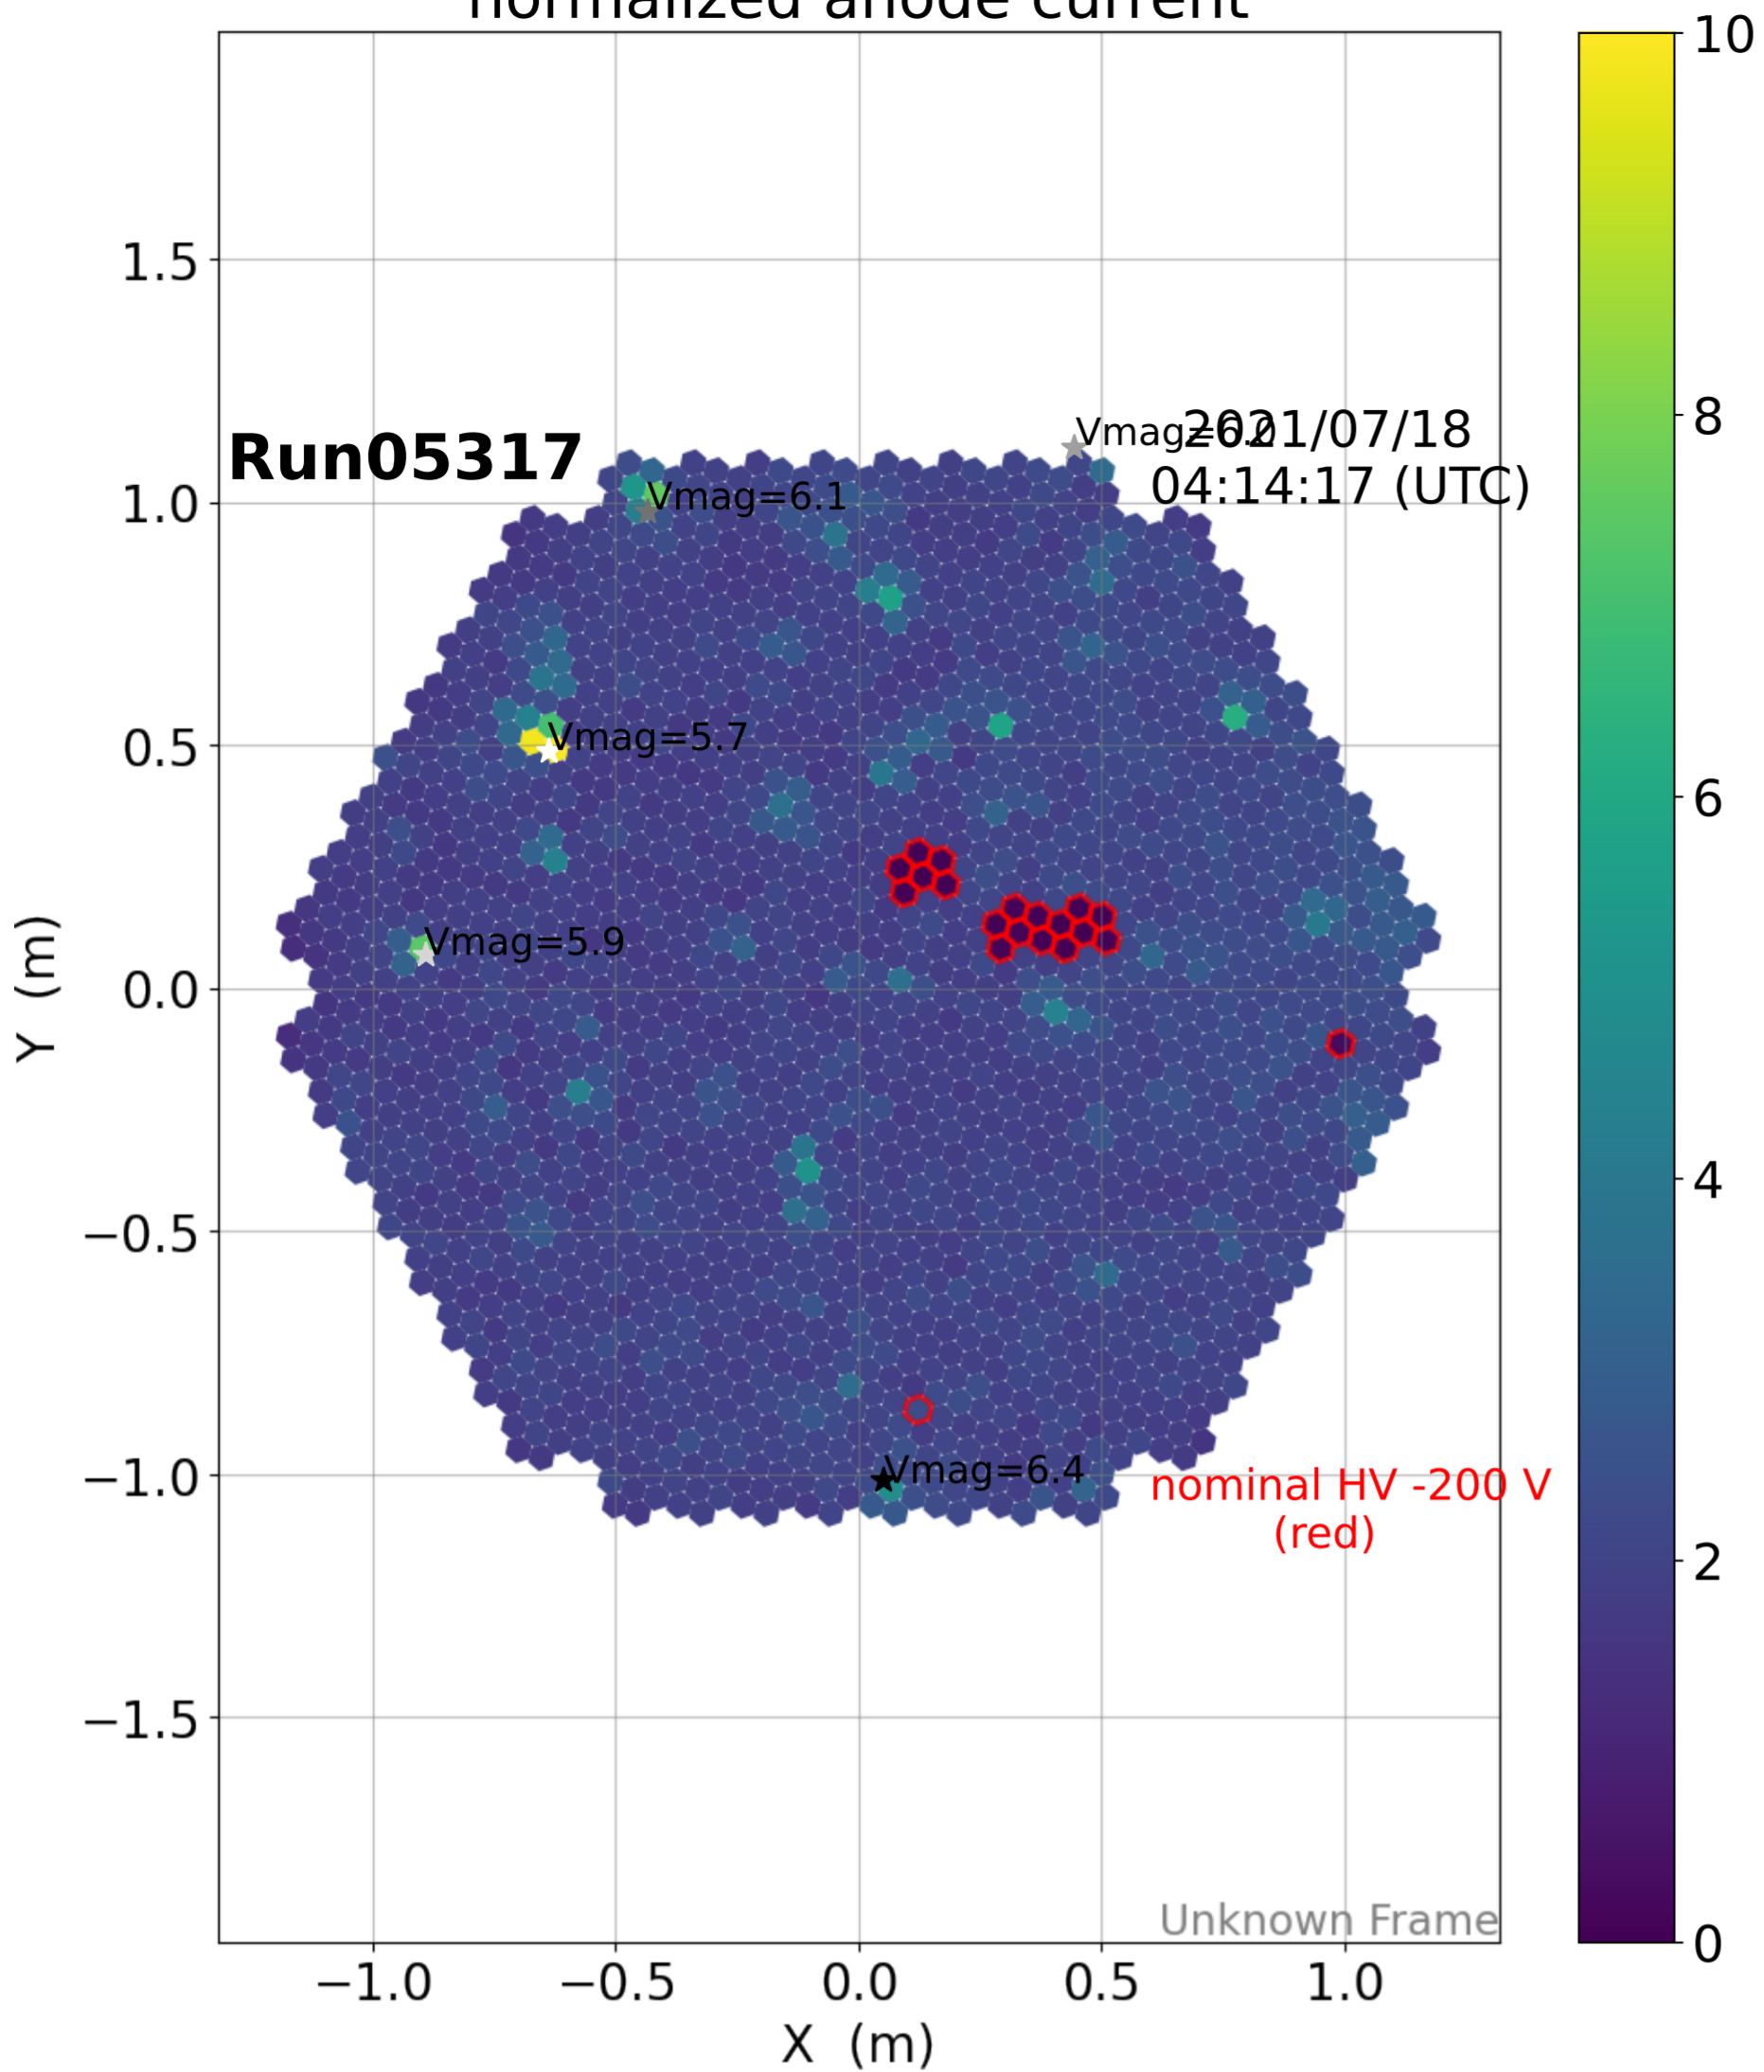

L1 local rate [Hz]

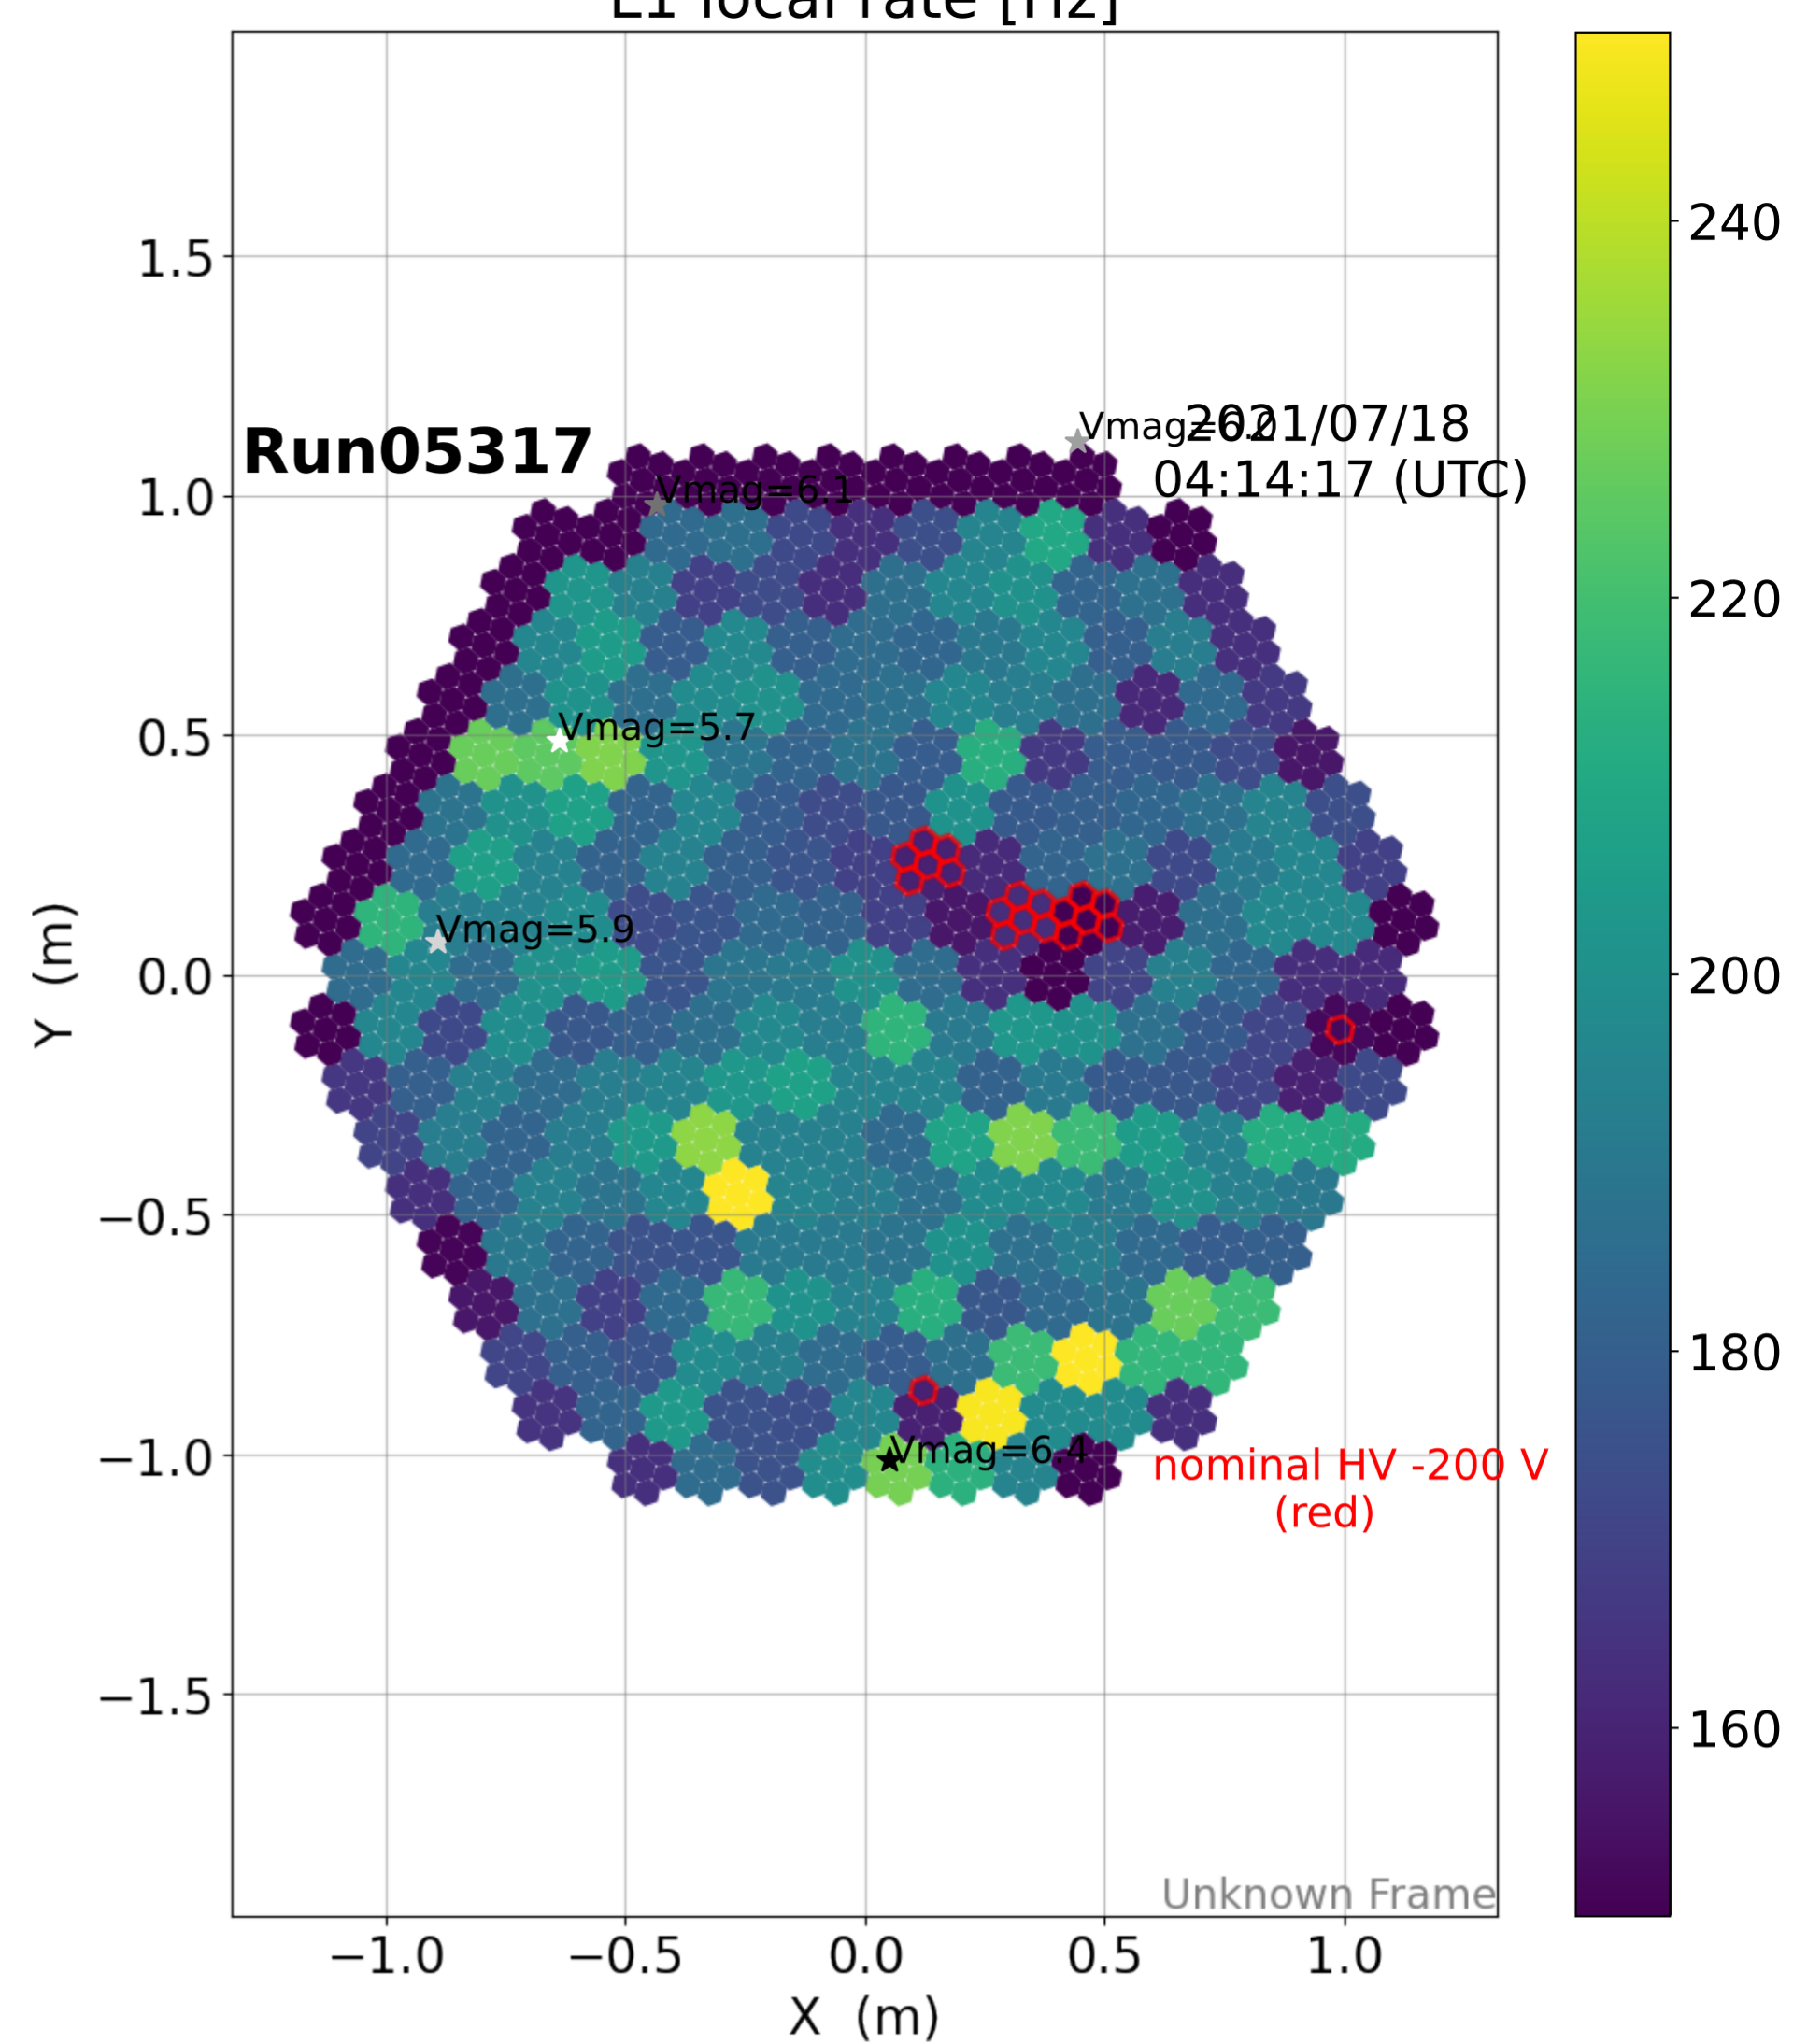

normalized anode current

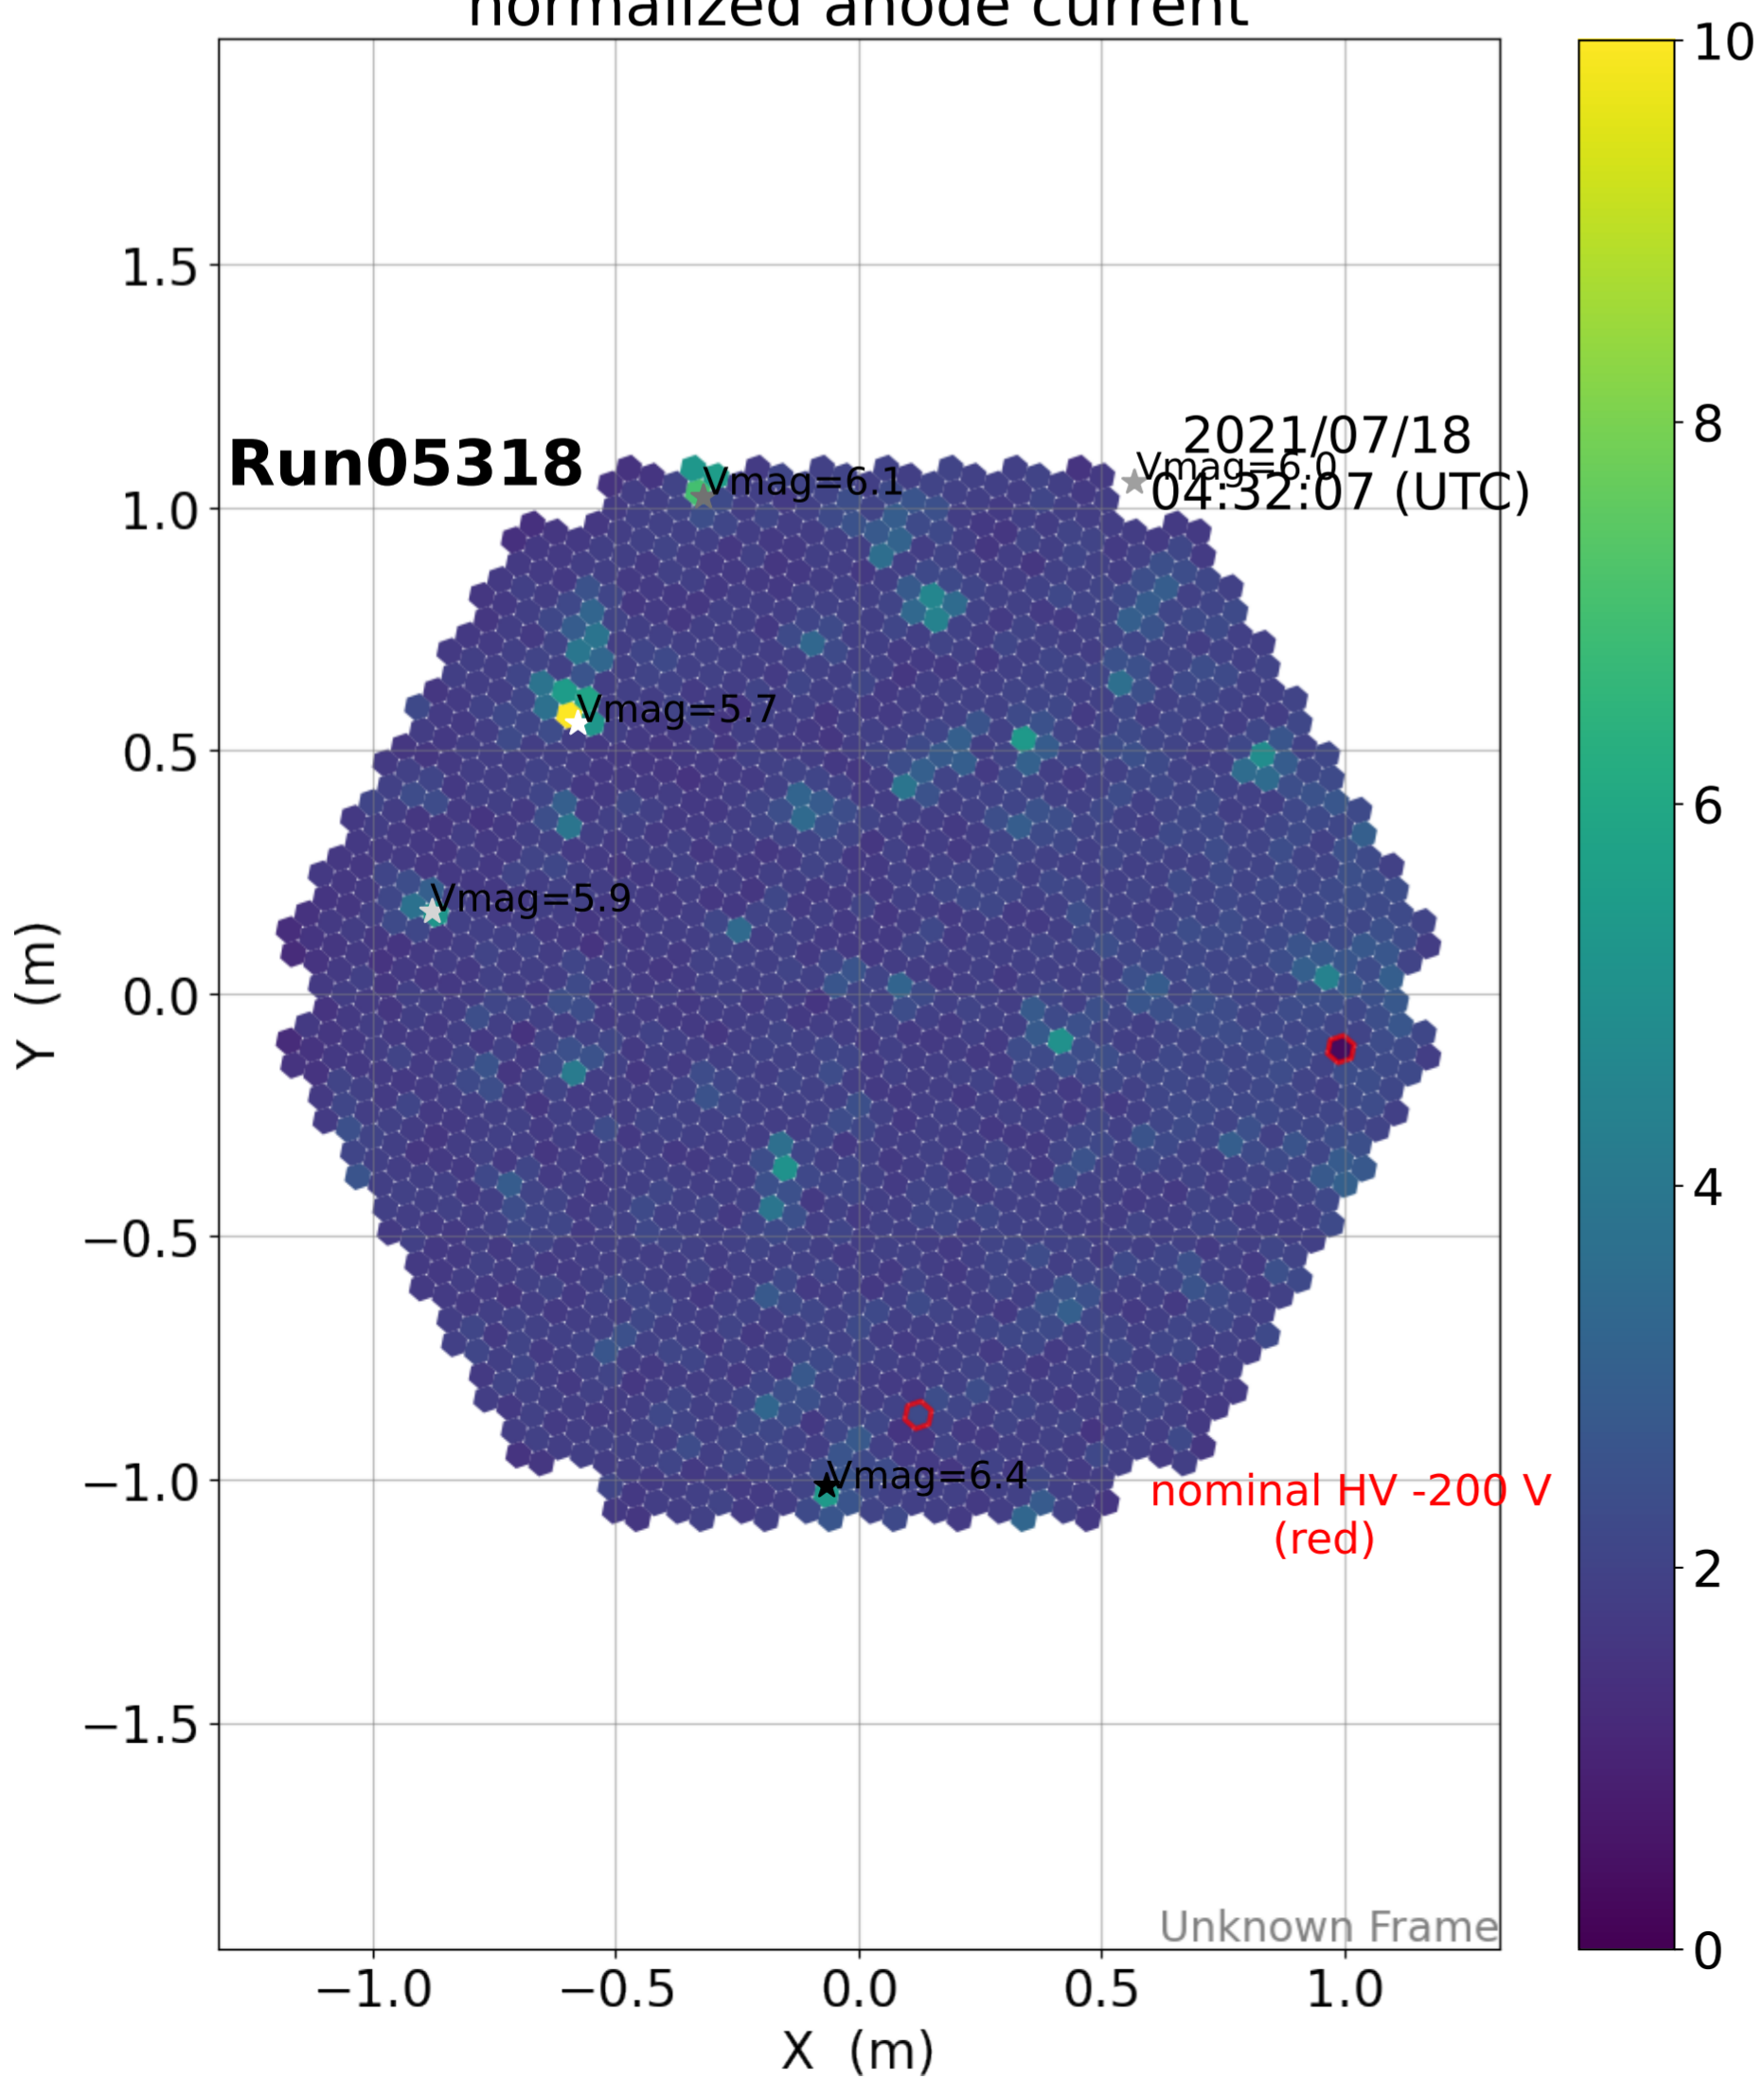

L1 local rate [Hz]

