




2021-8-30

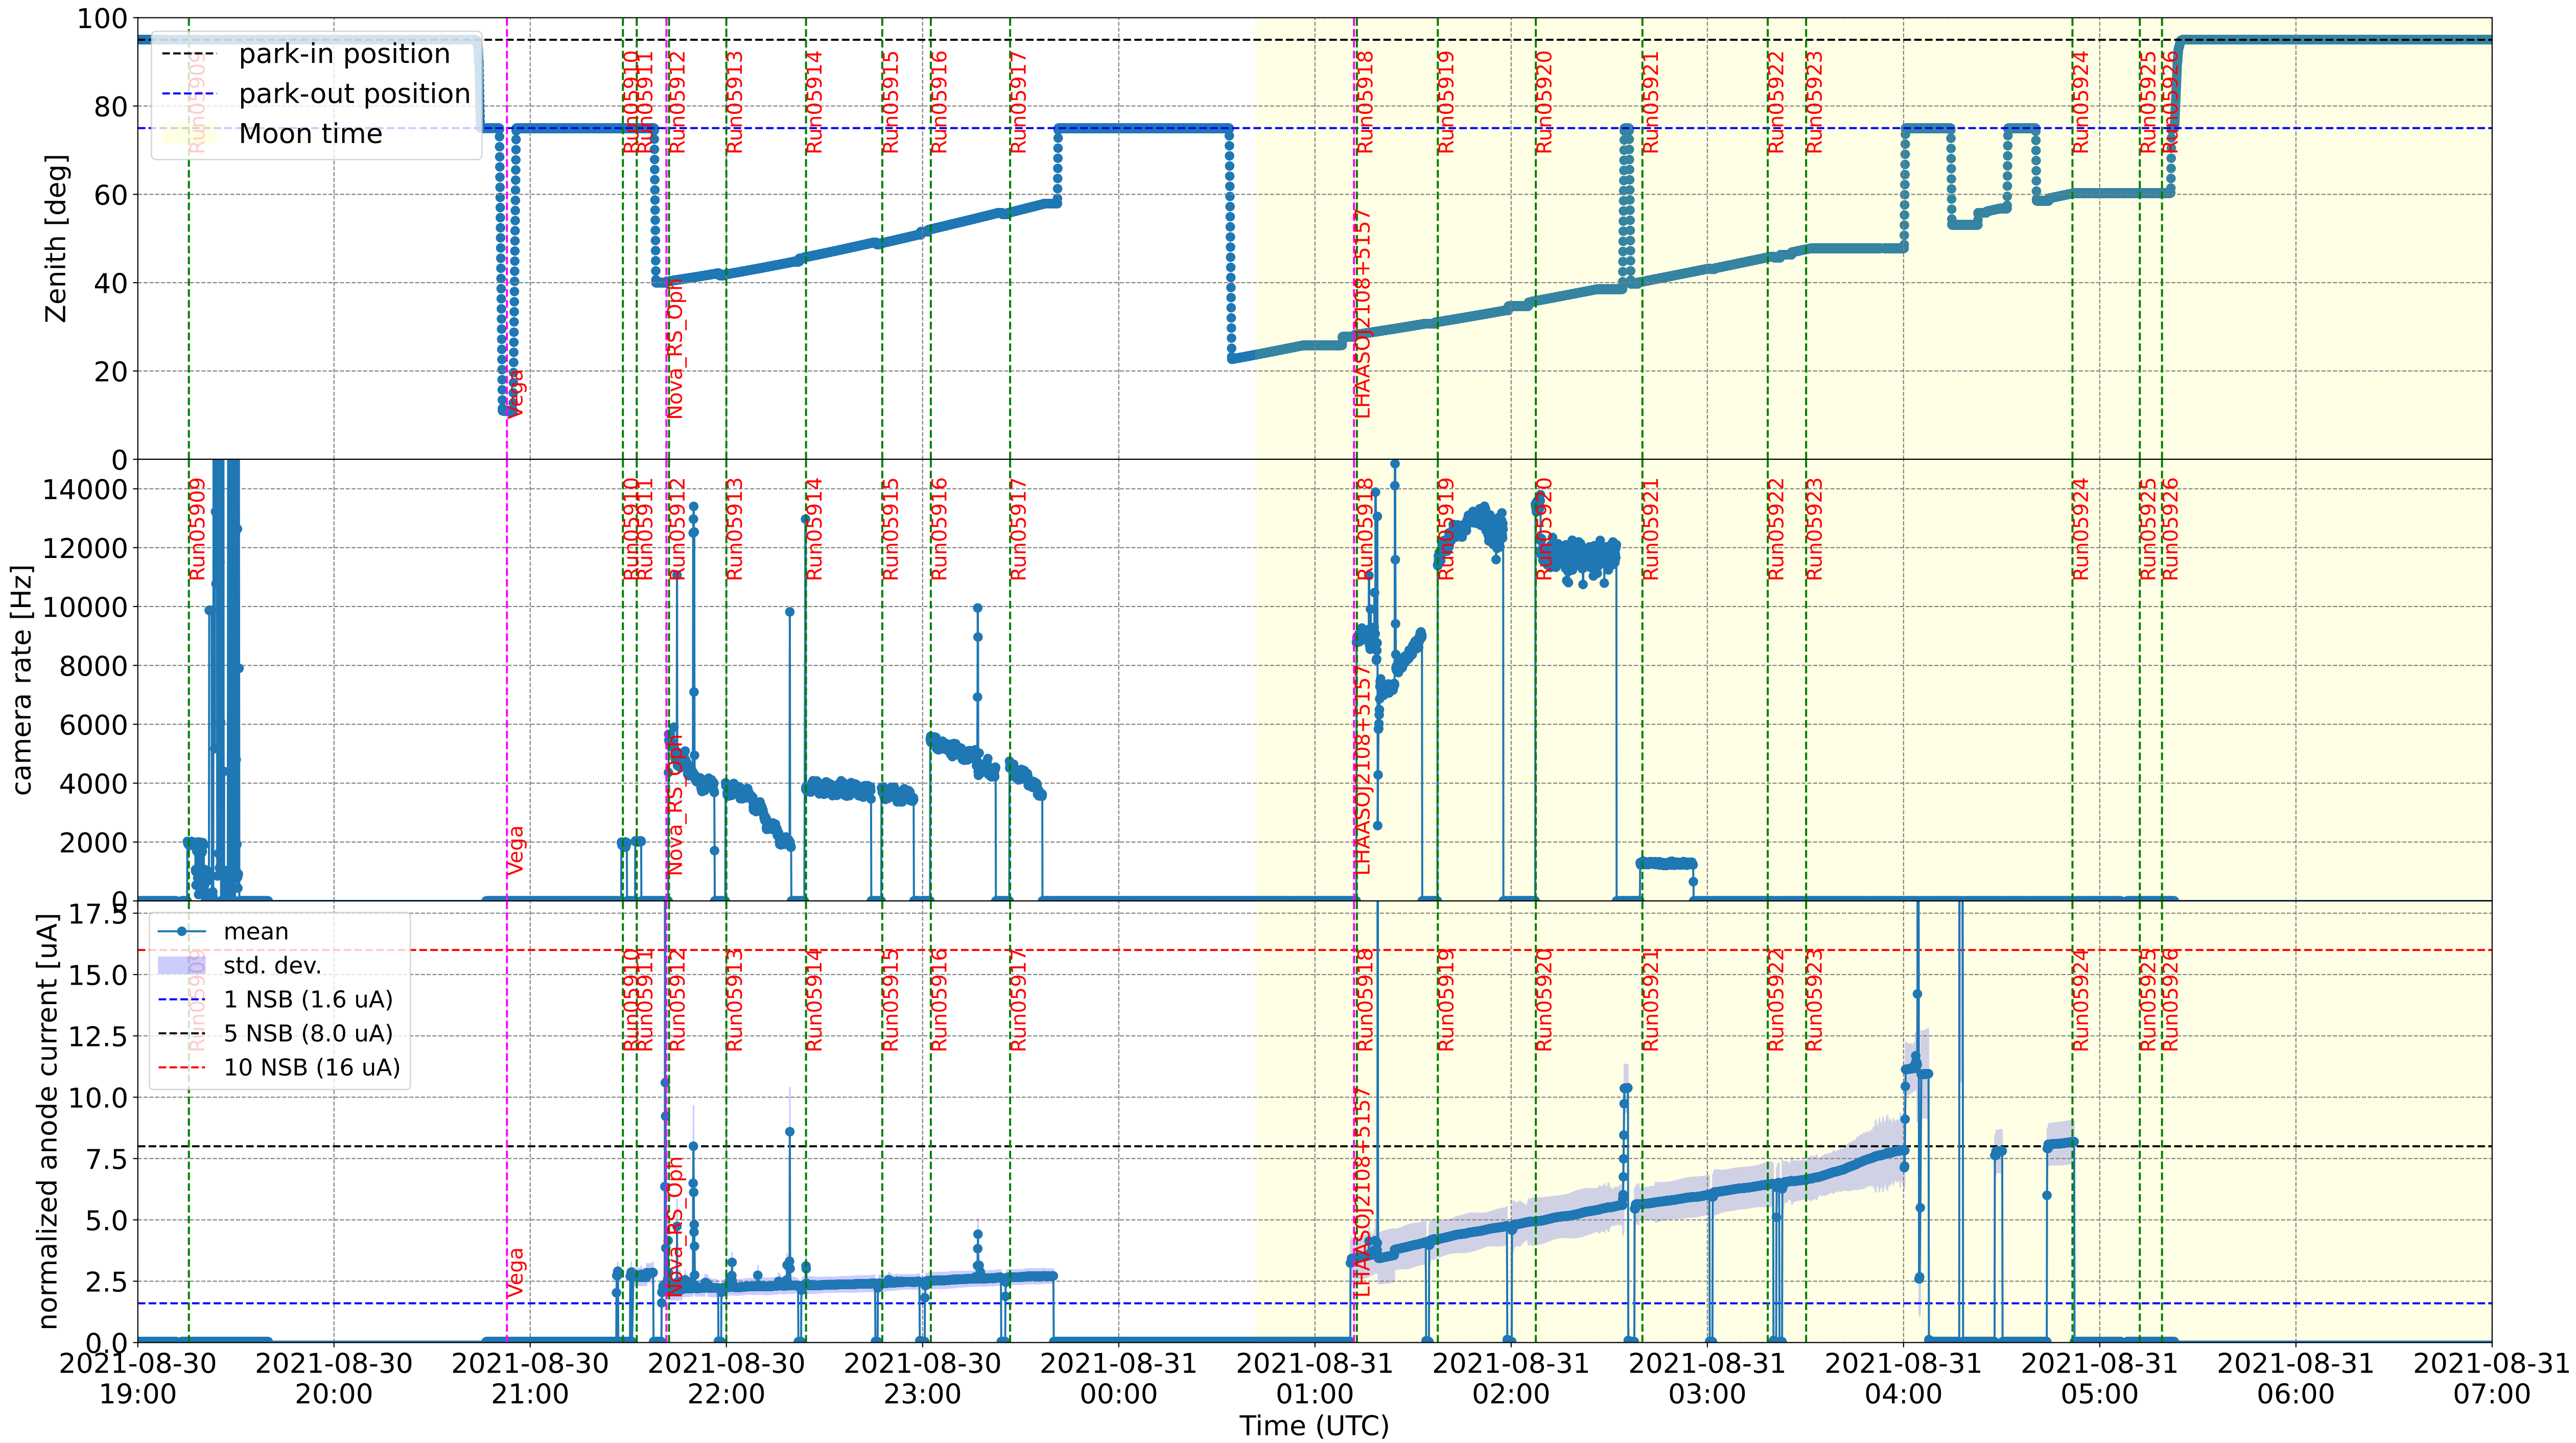







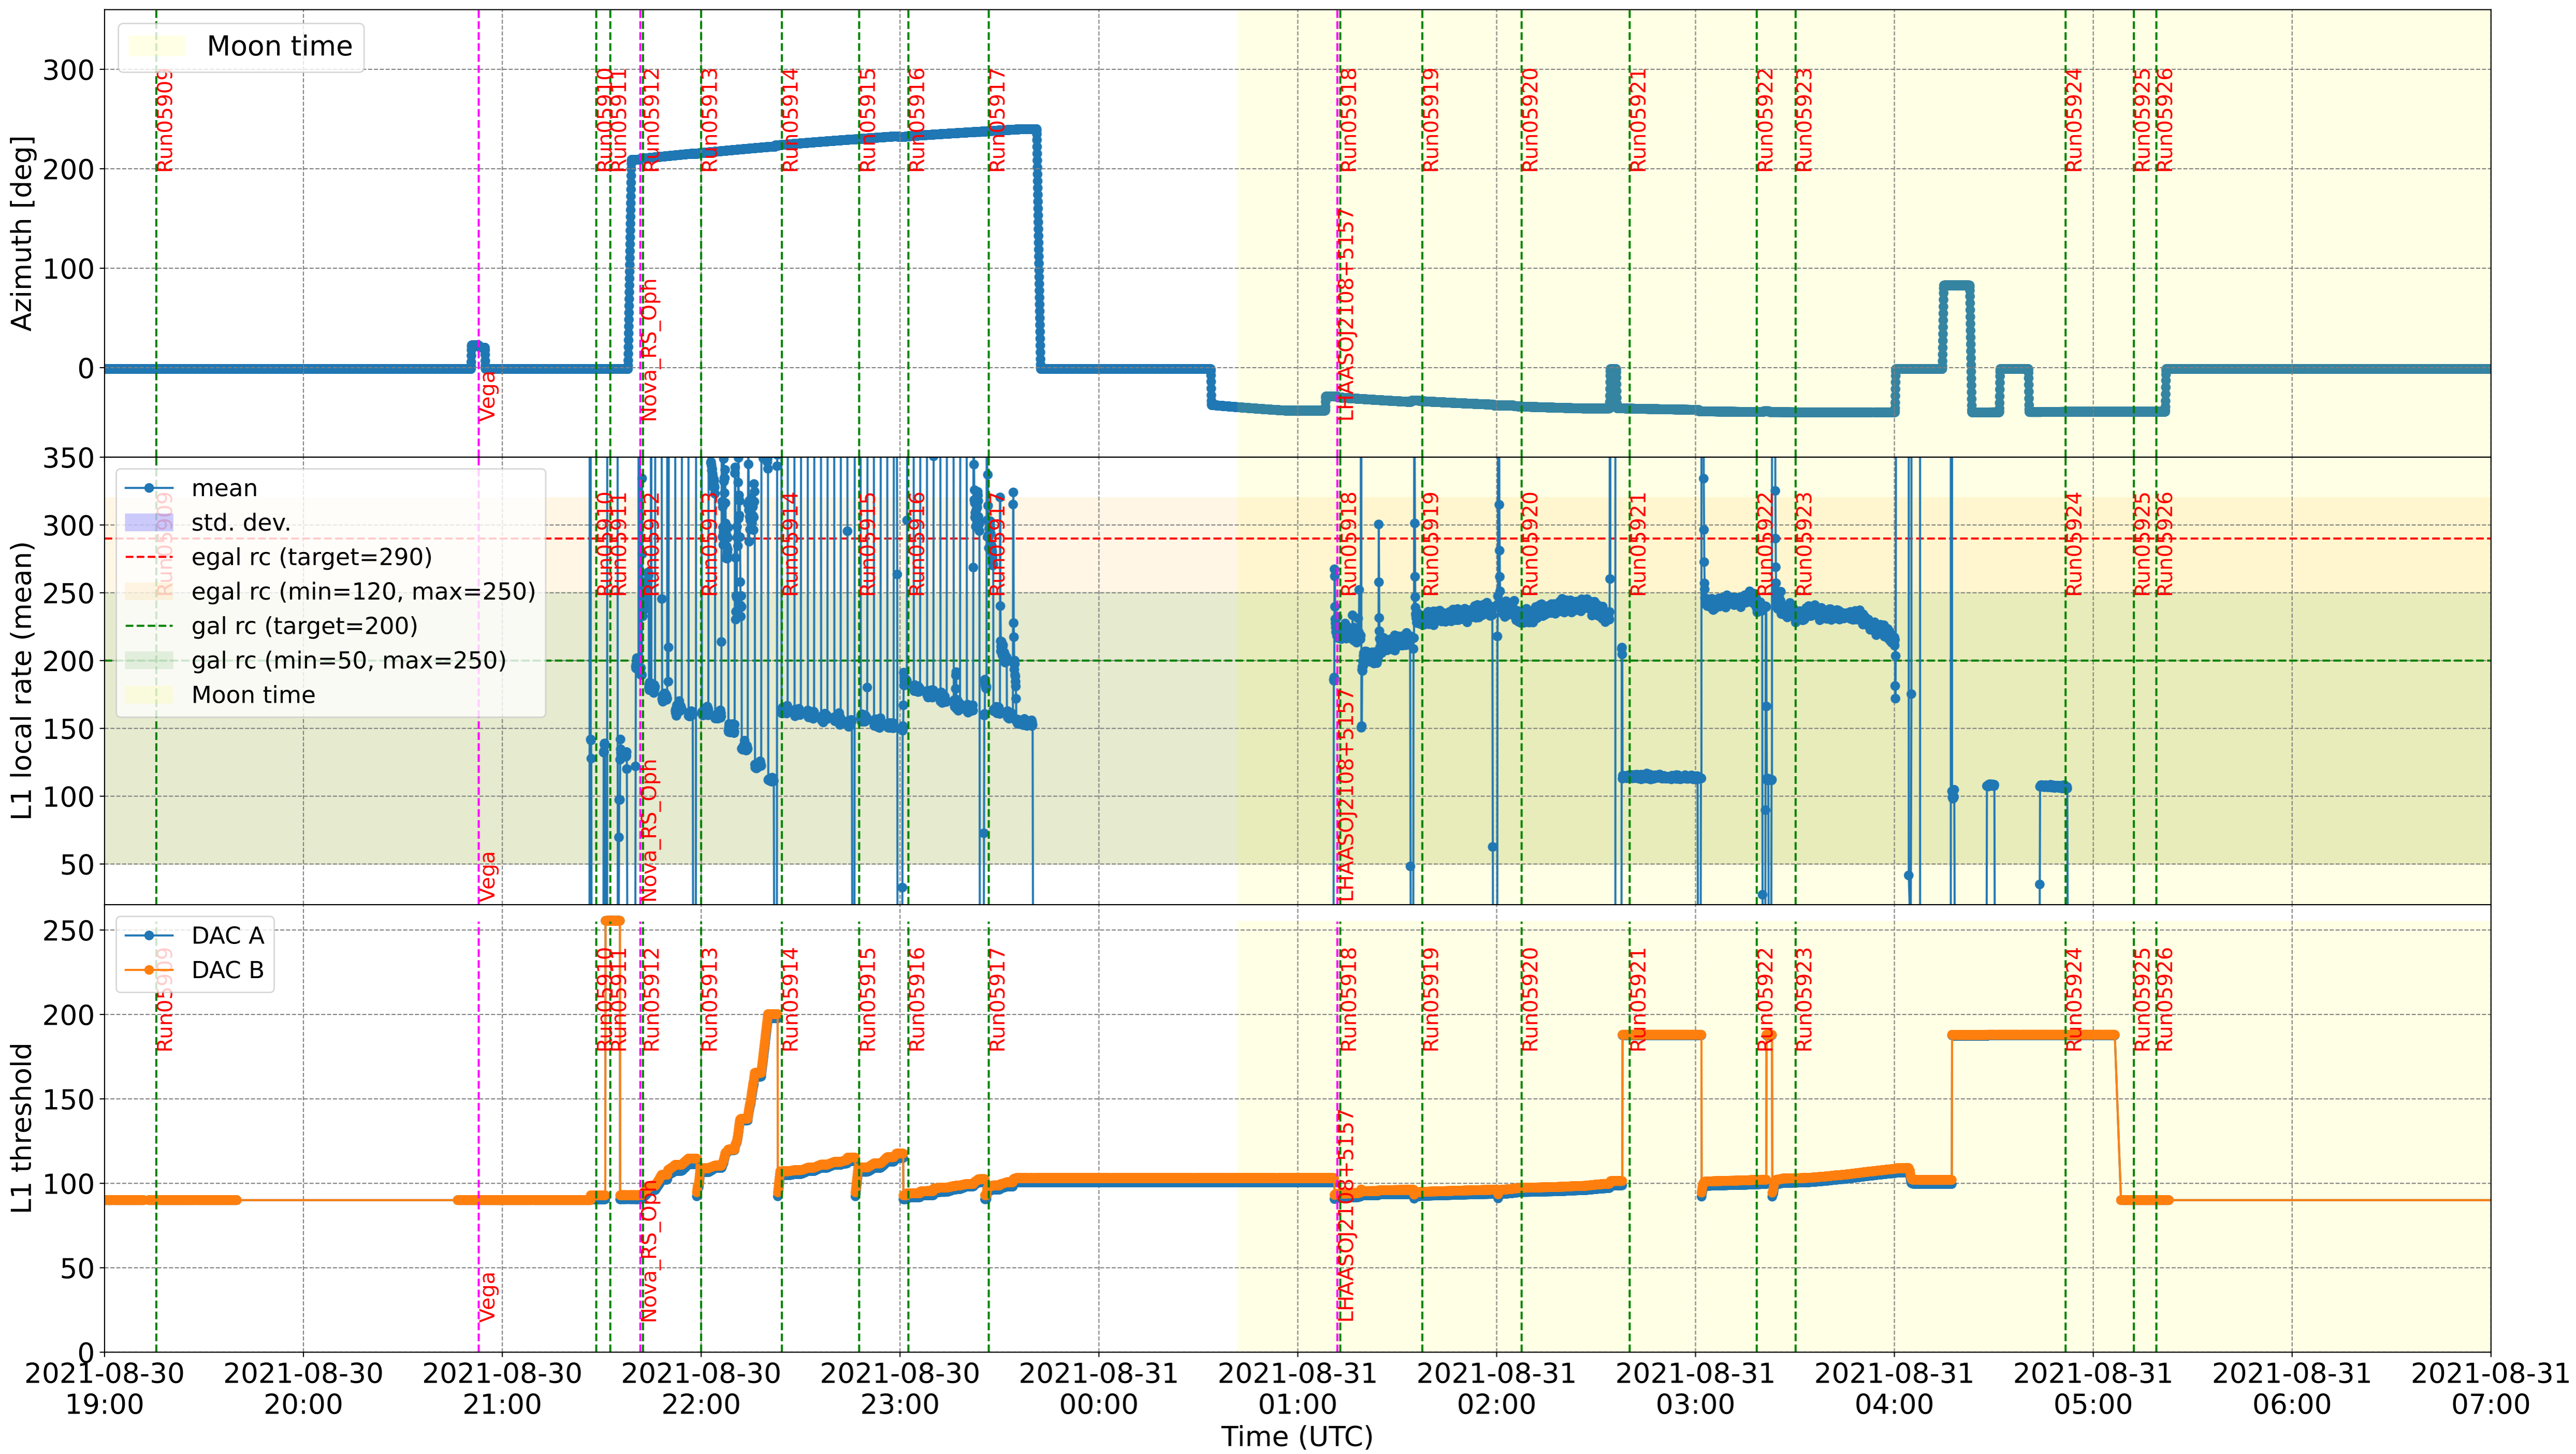








2021-8-30






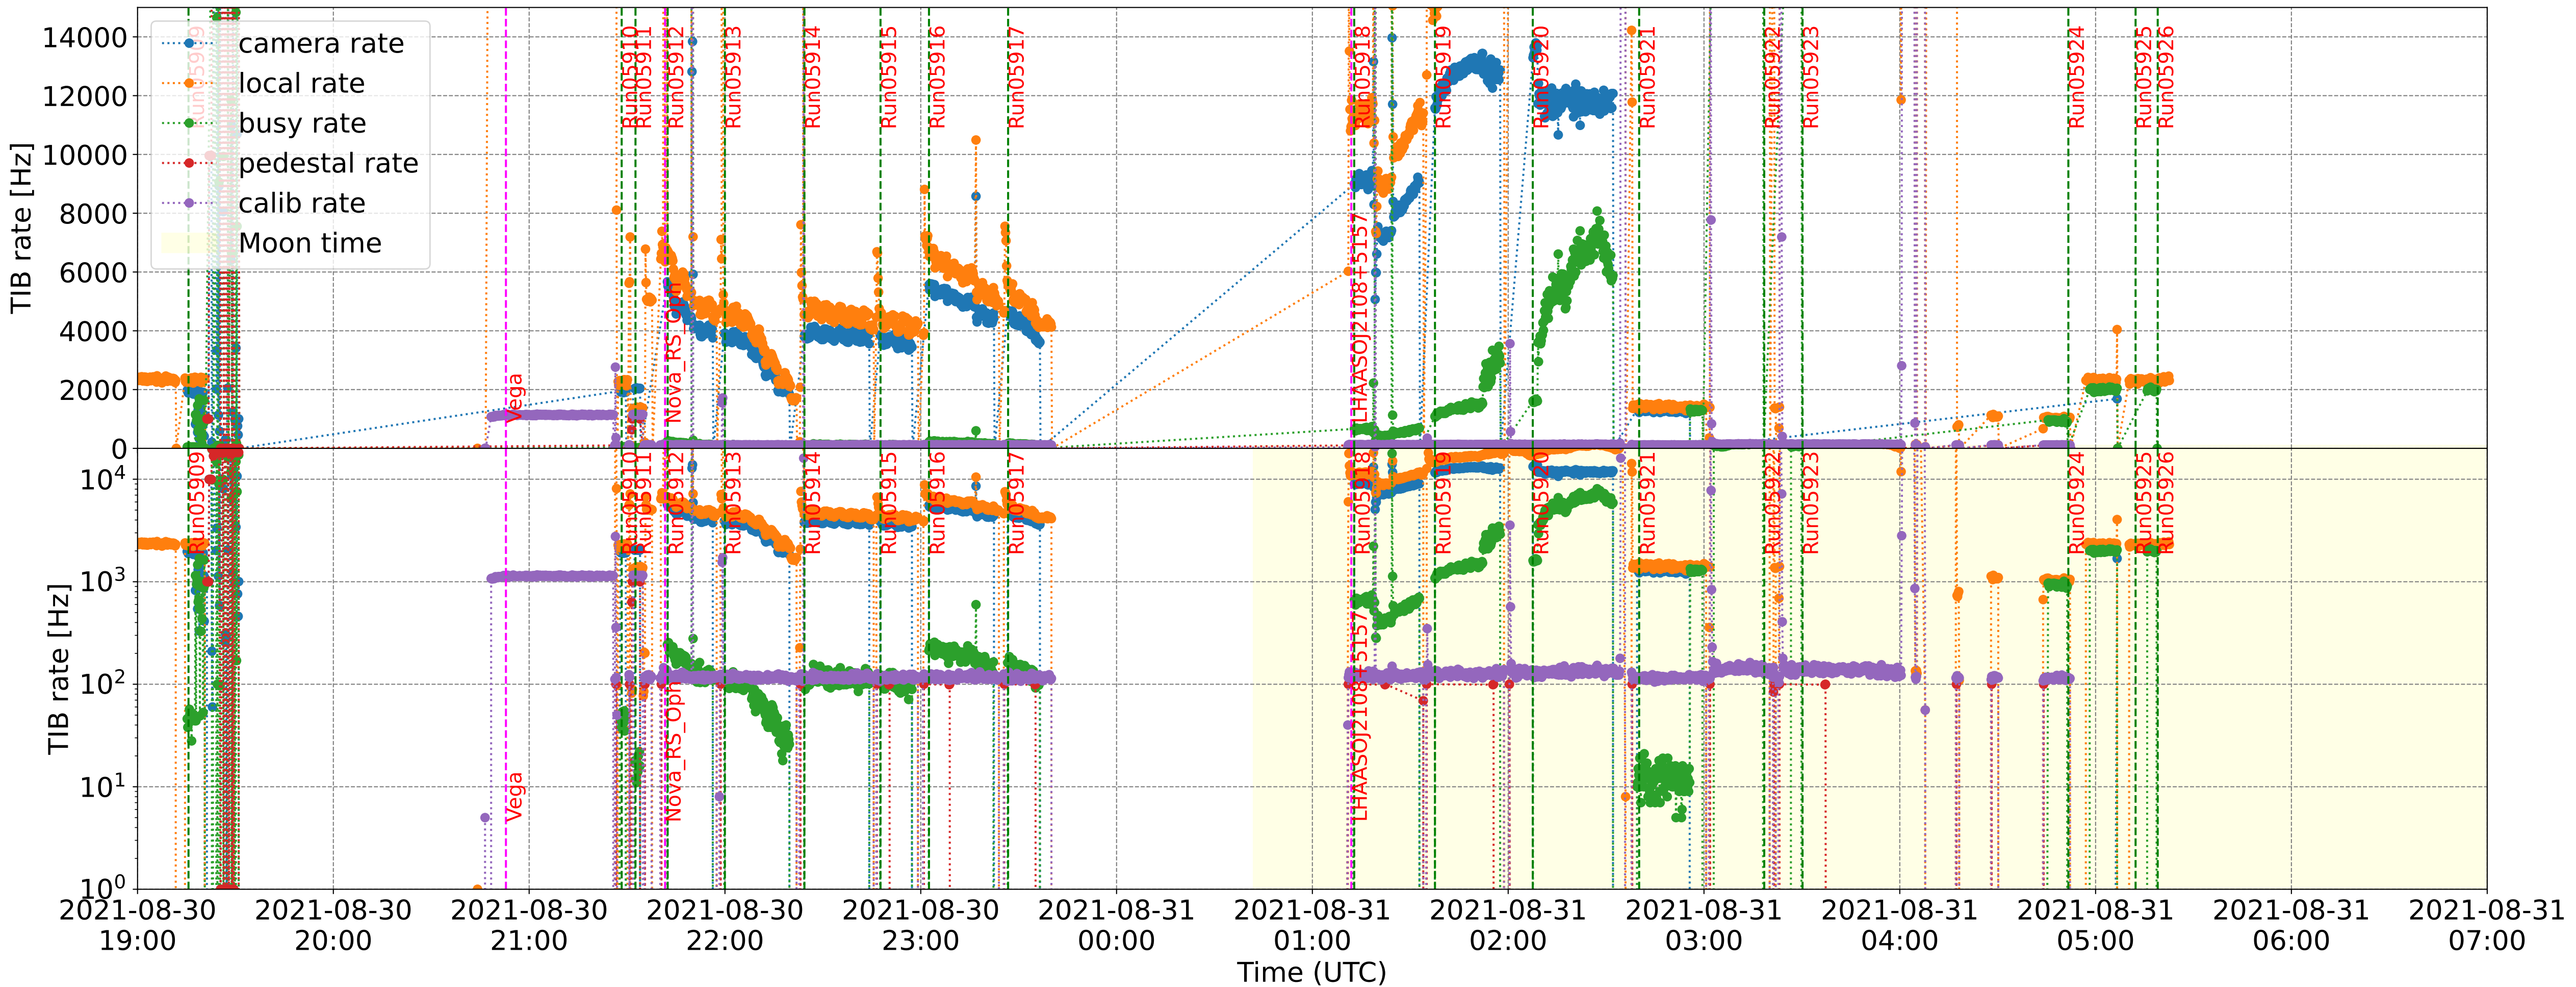








# Calibration Box (2021-8-30)

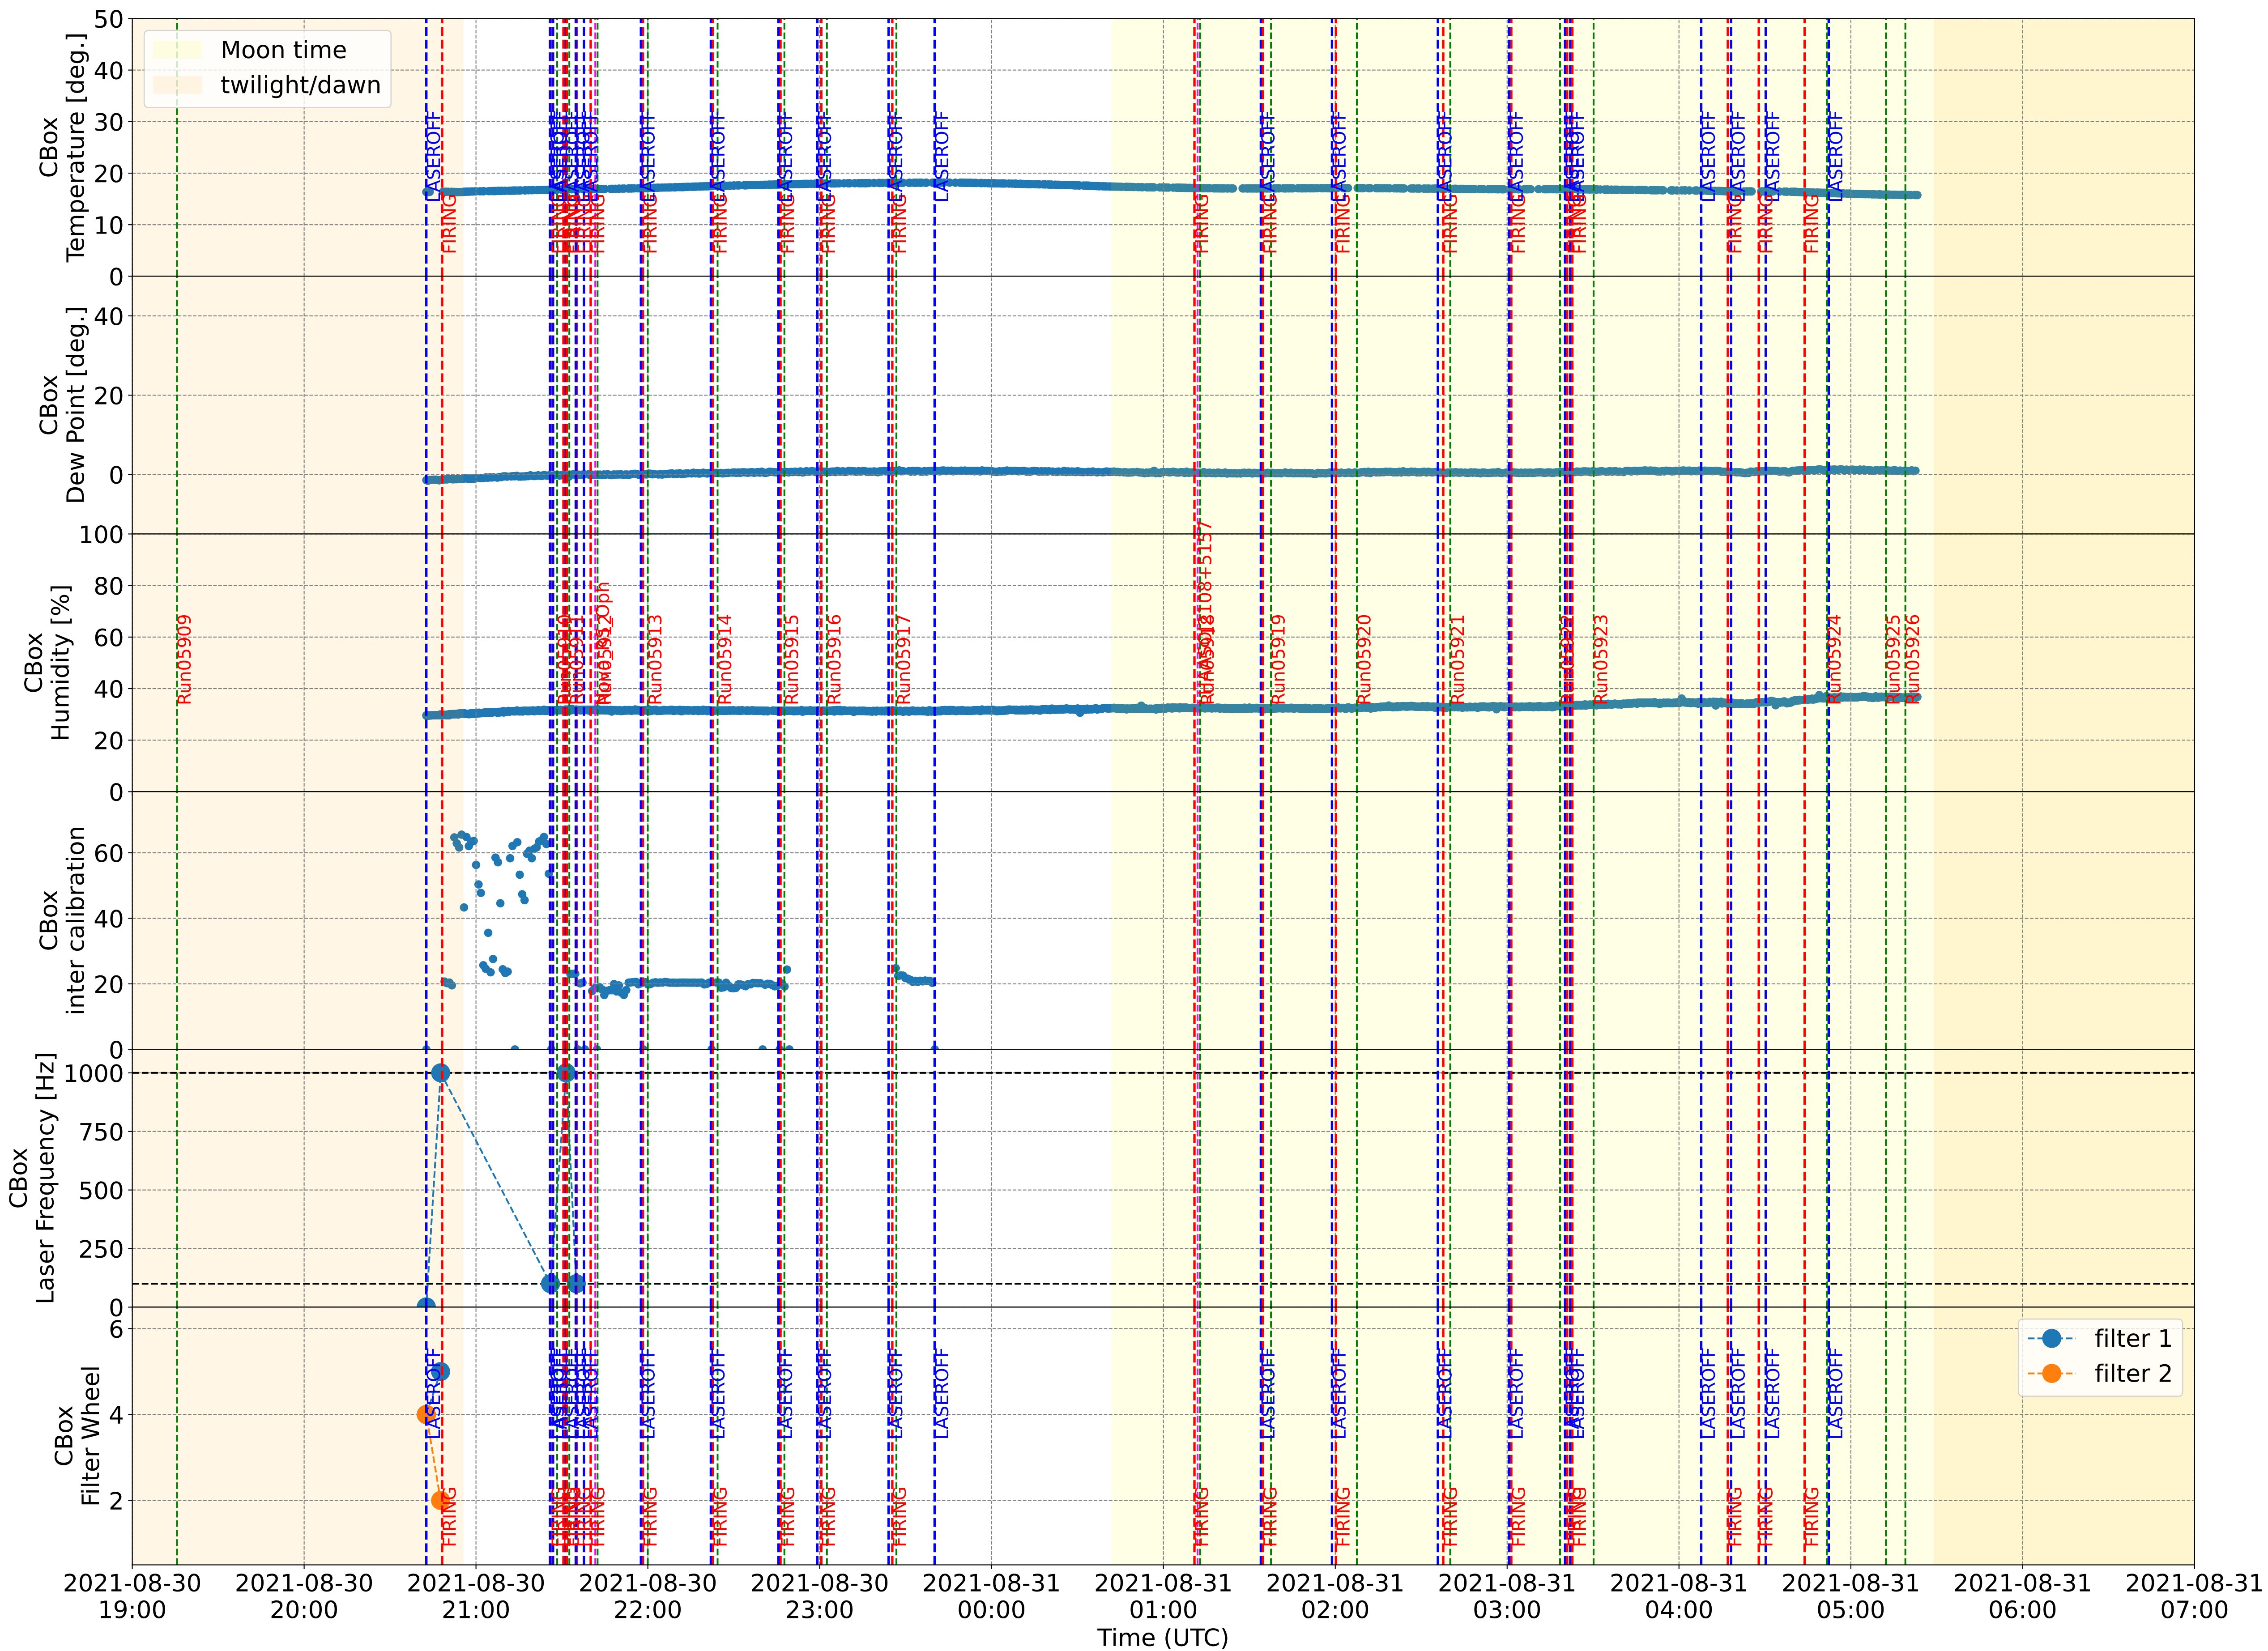

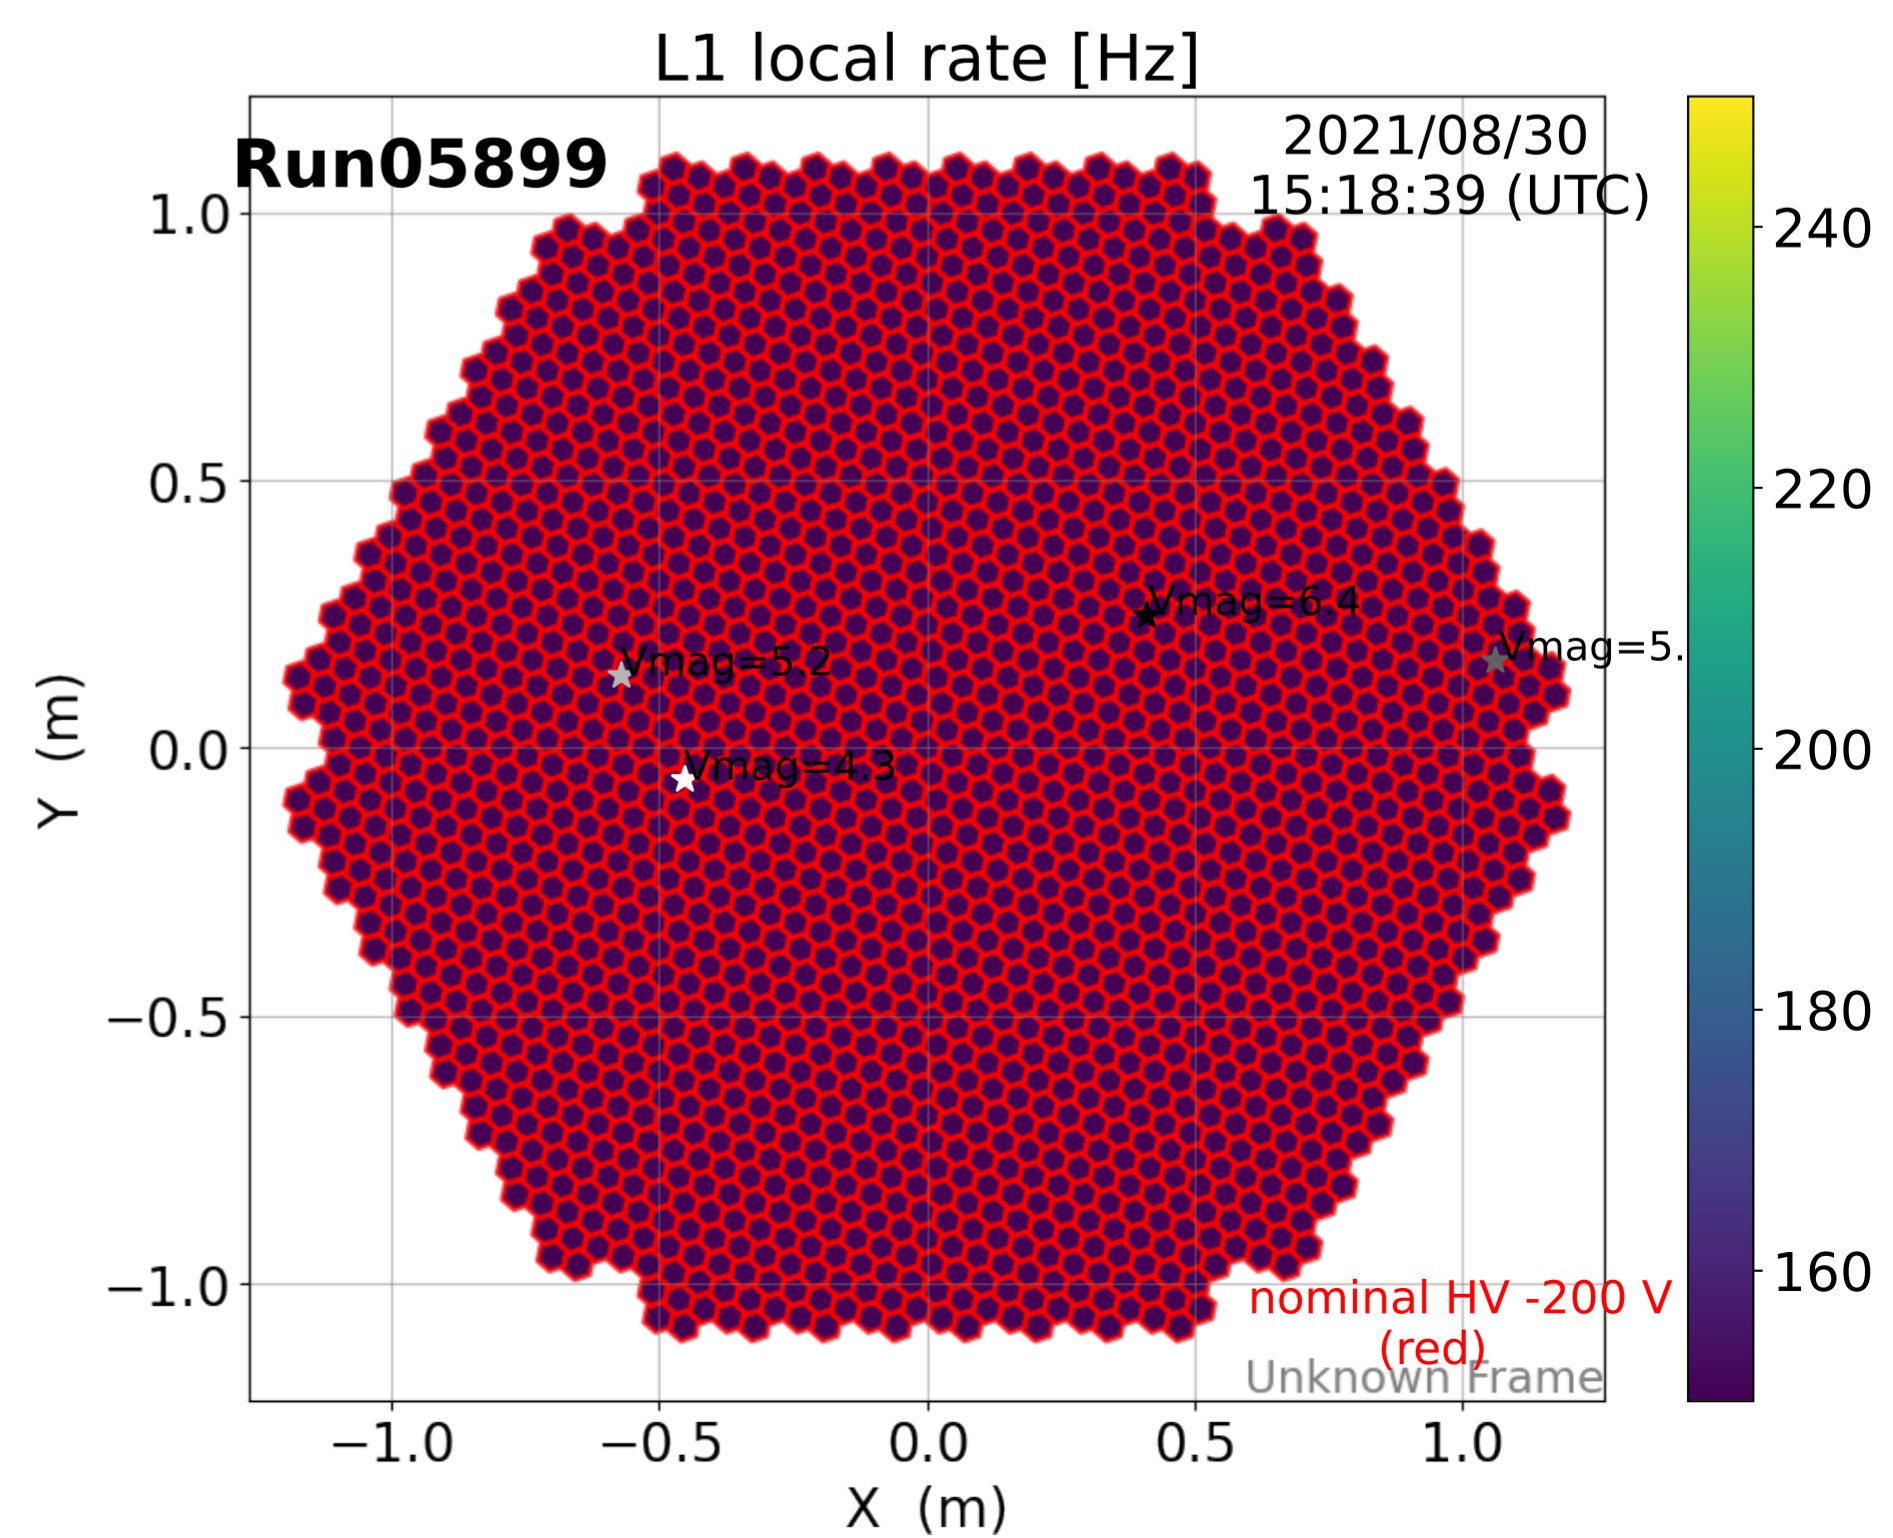
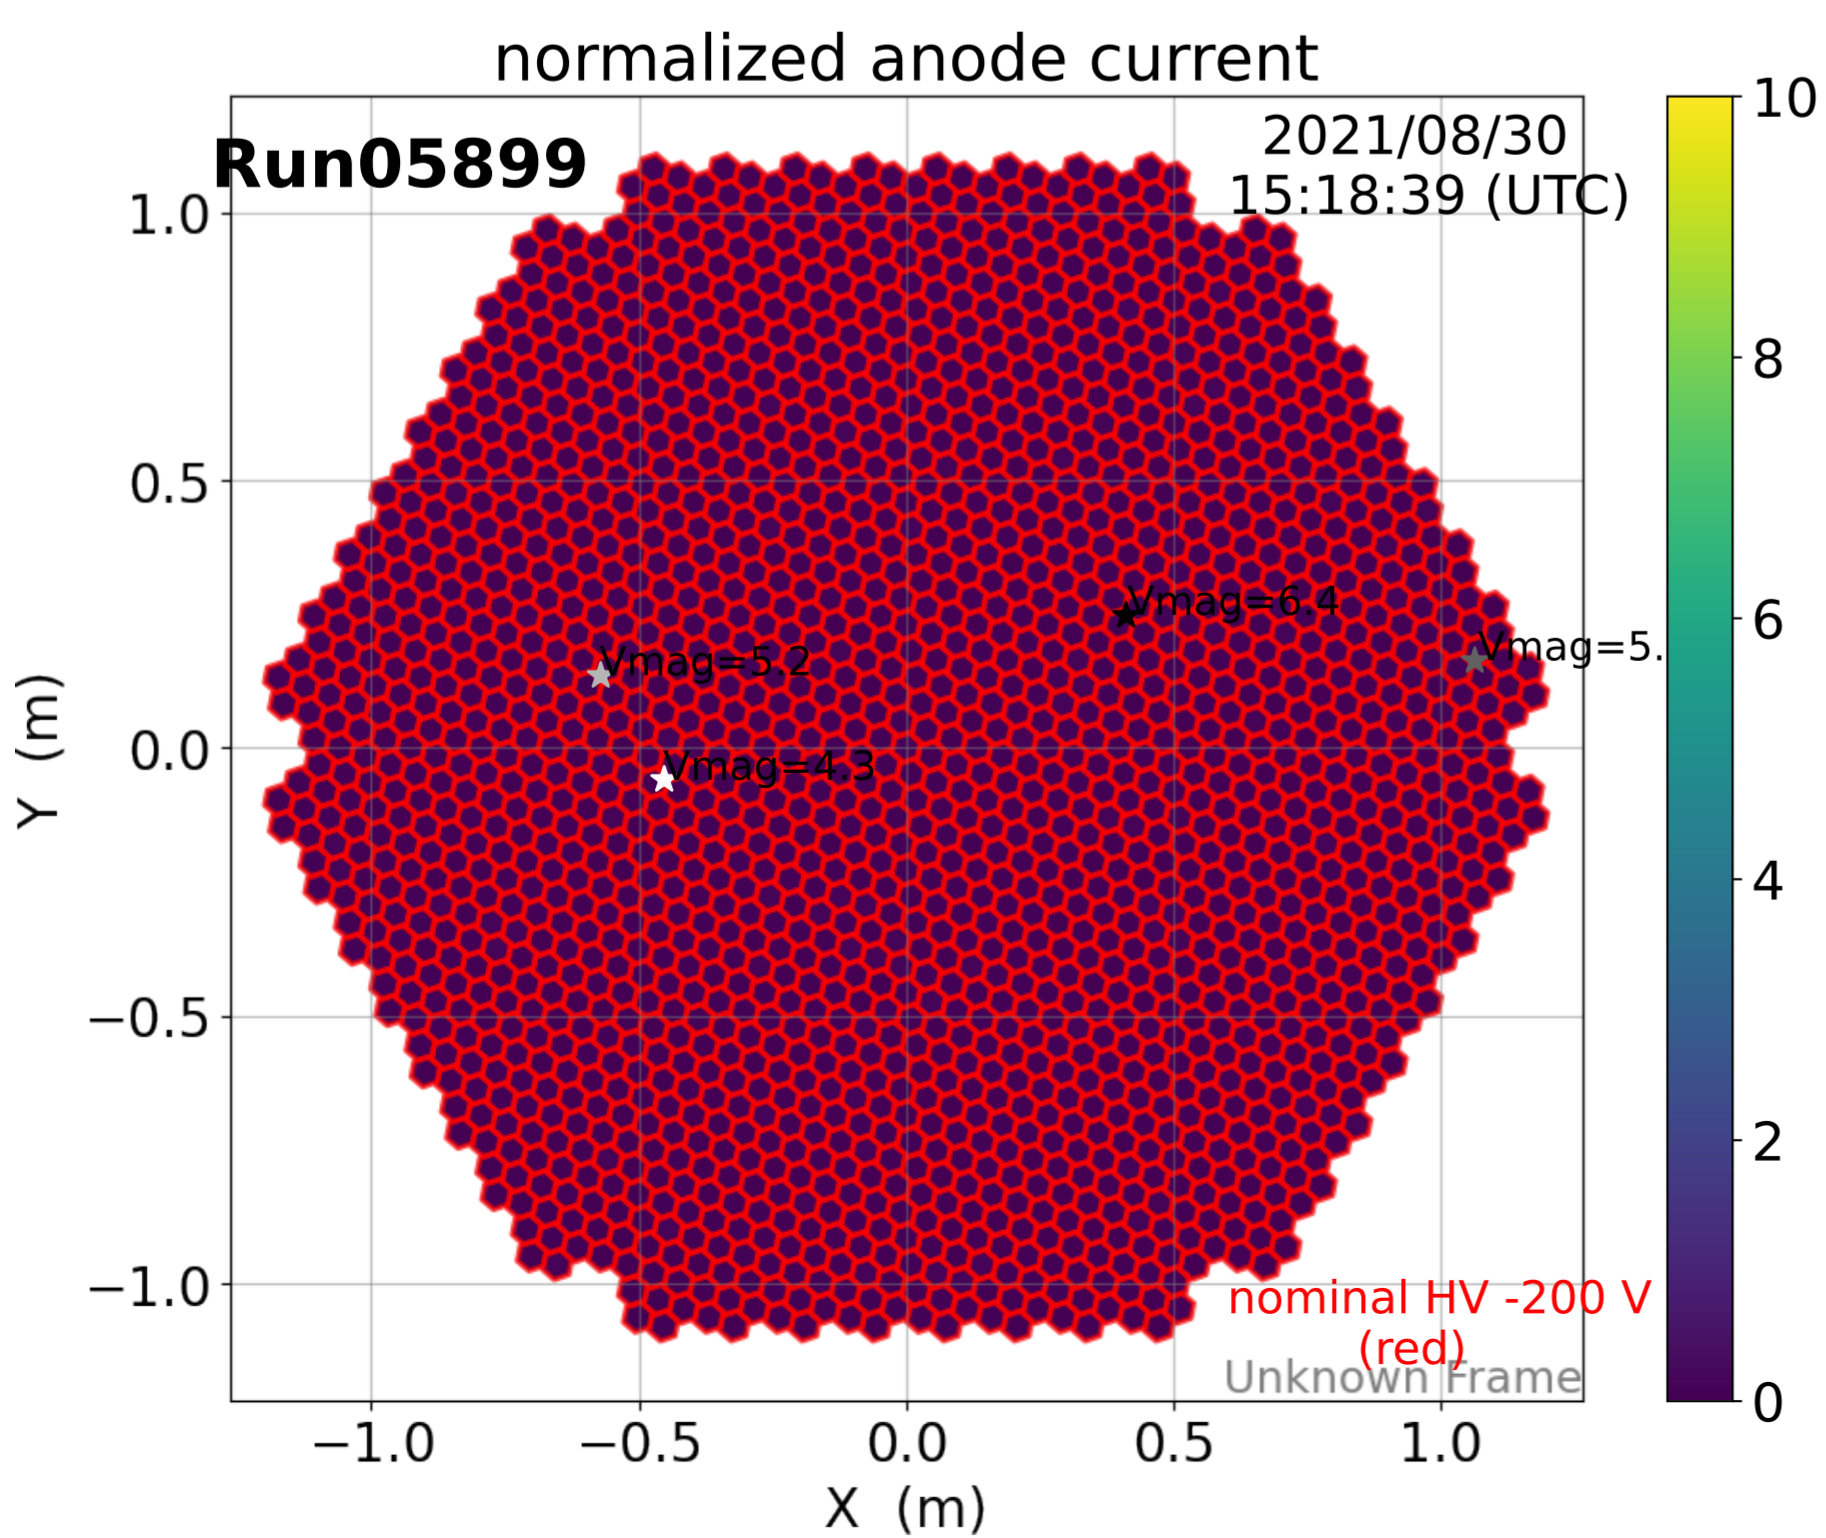
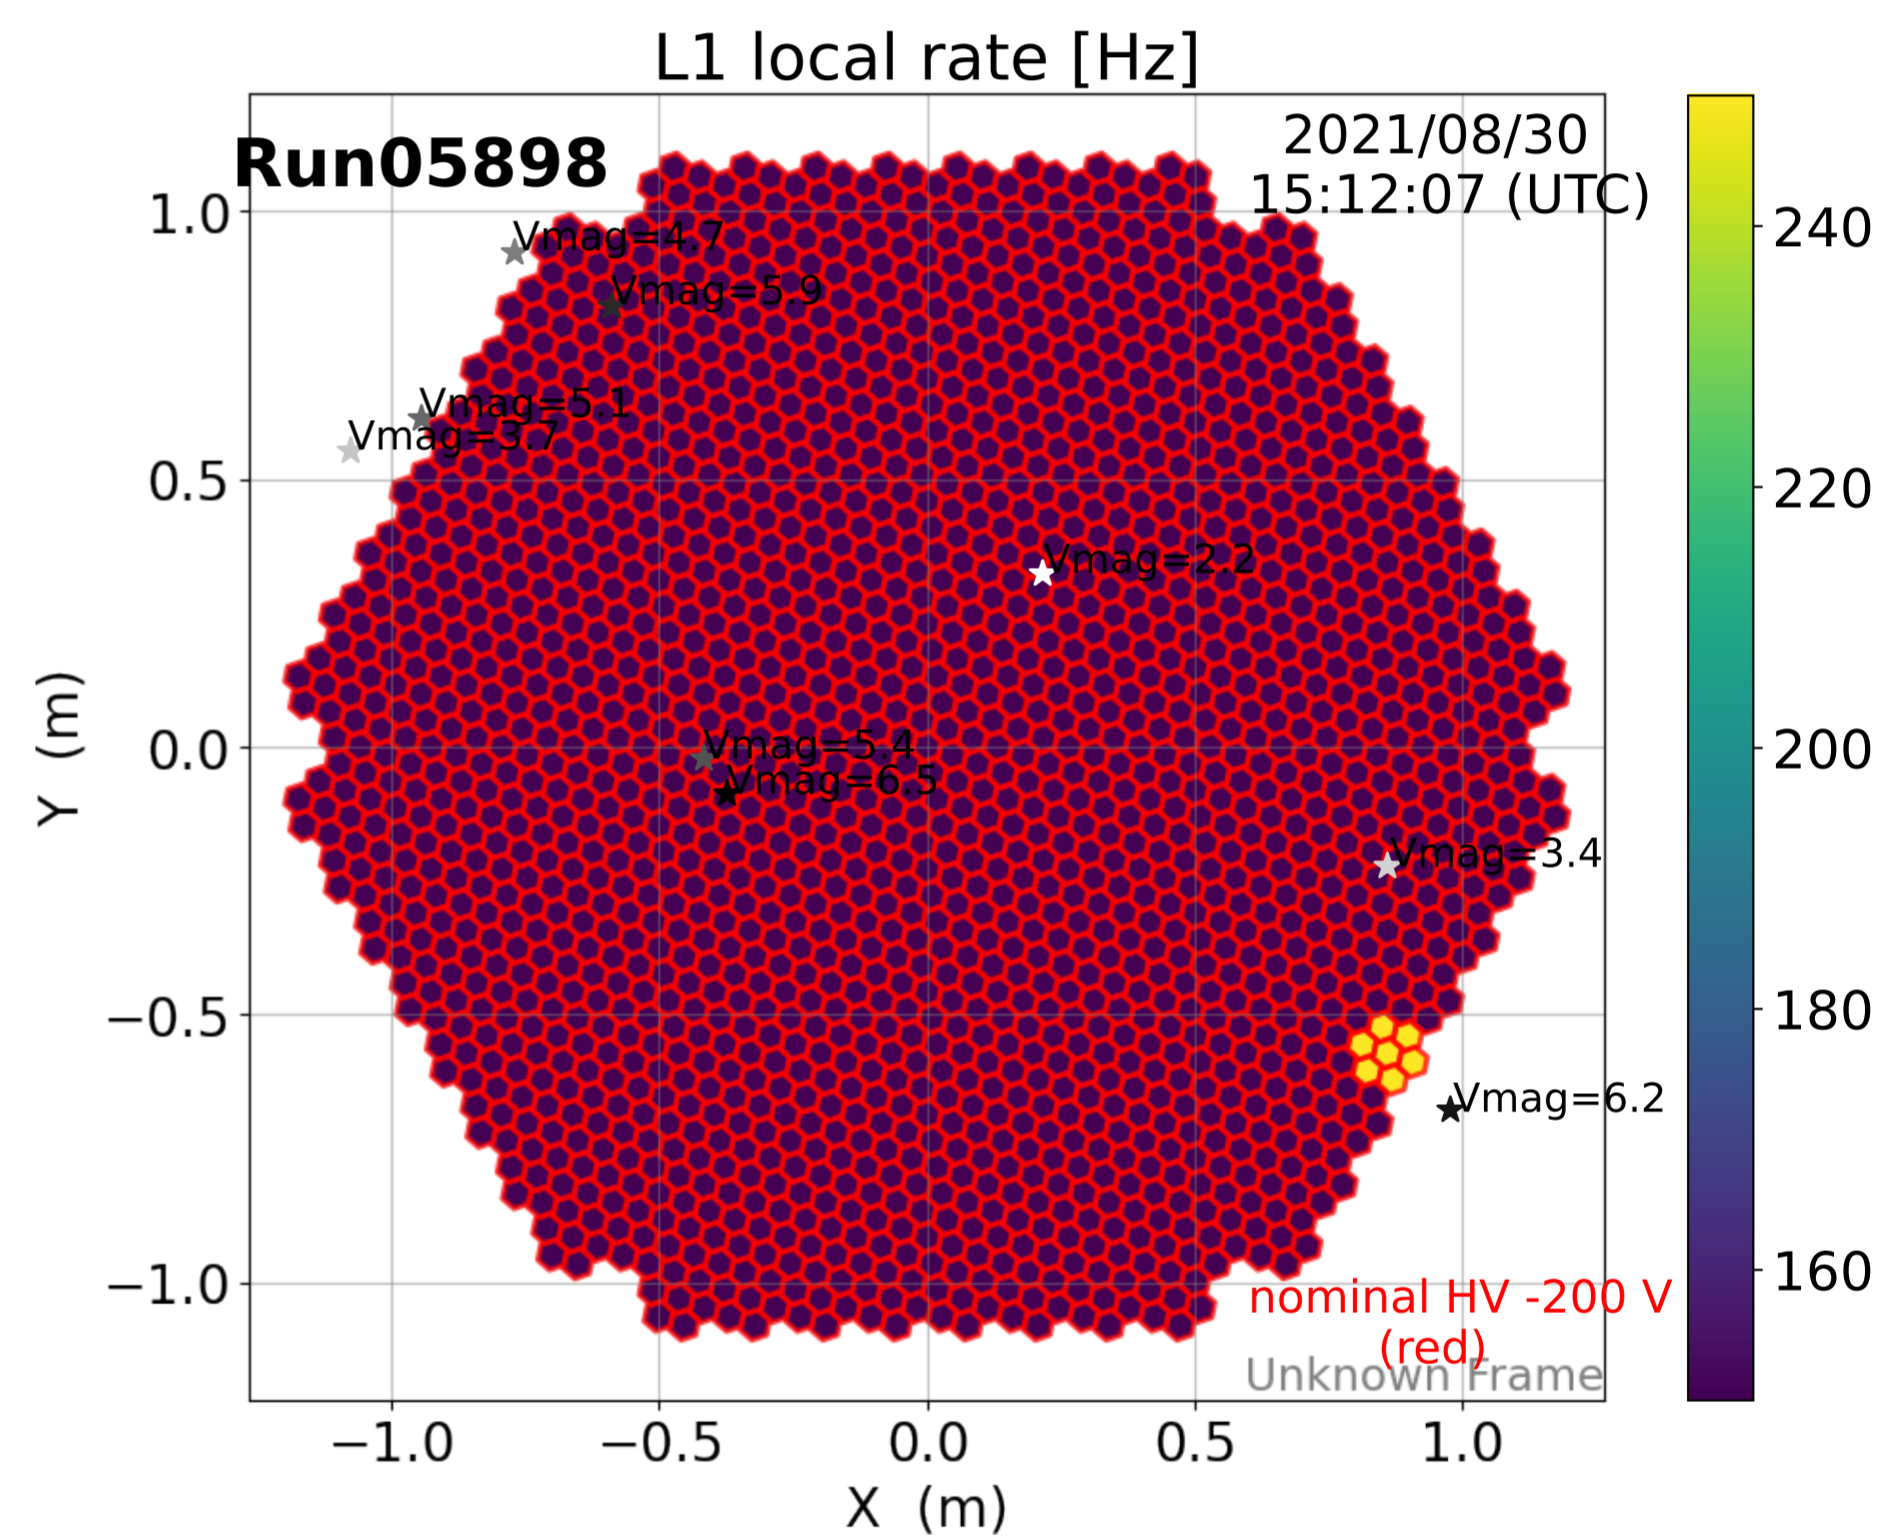
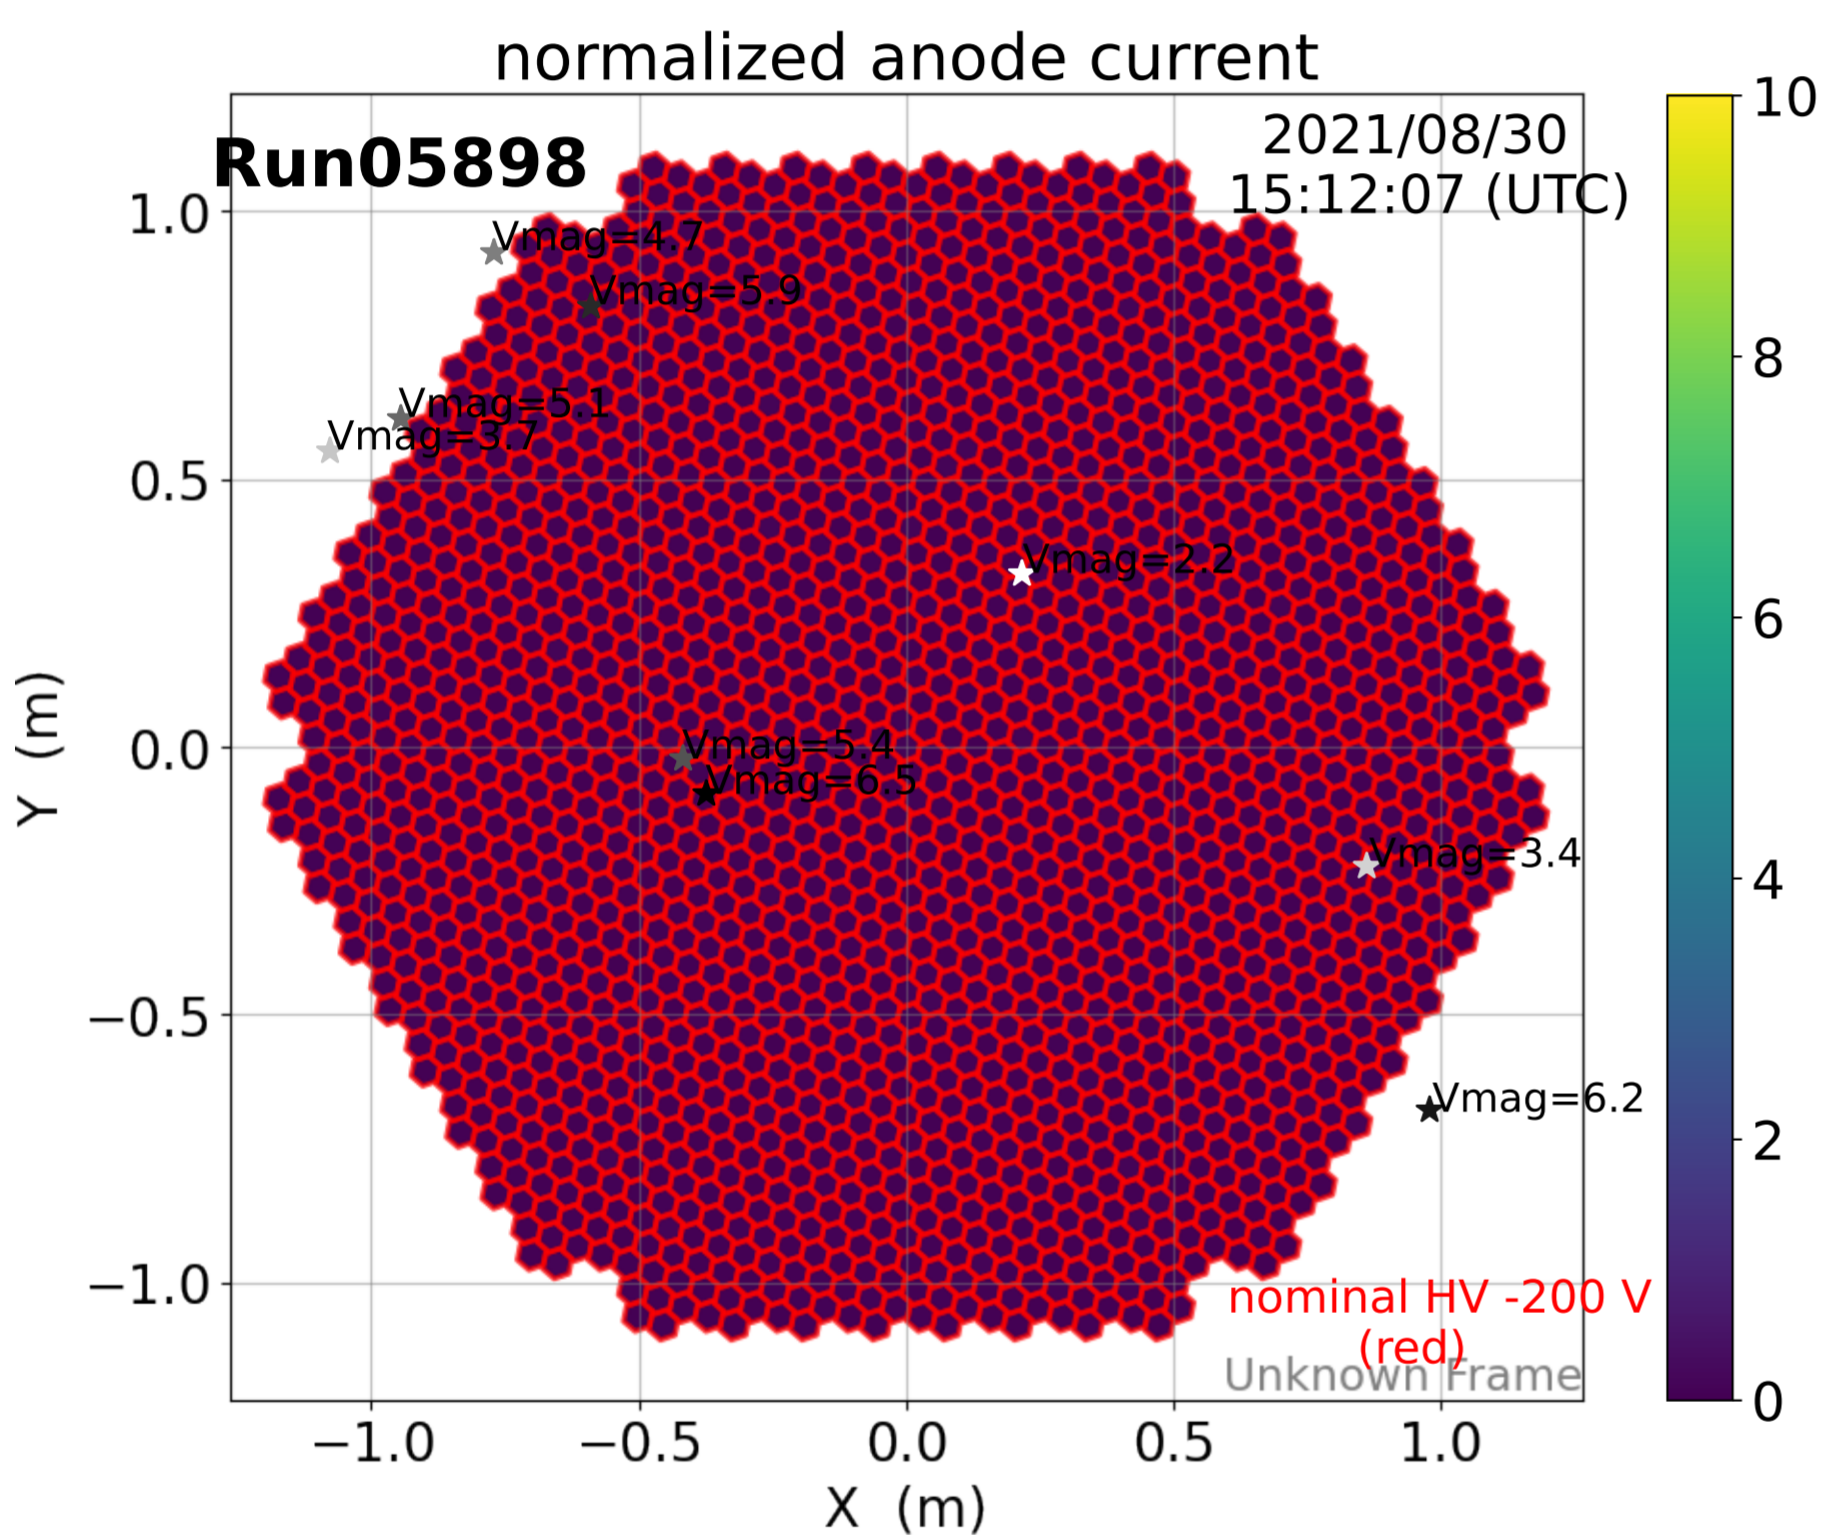
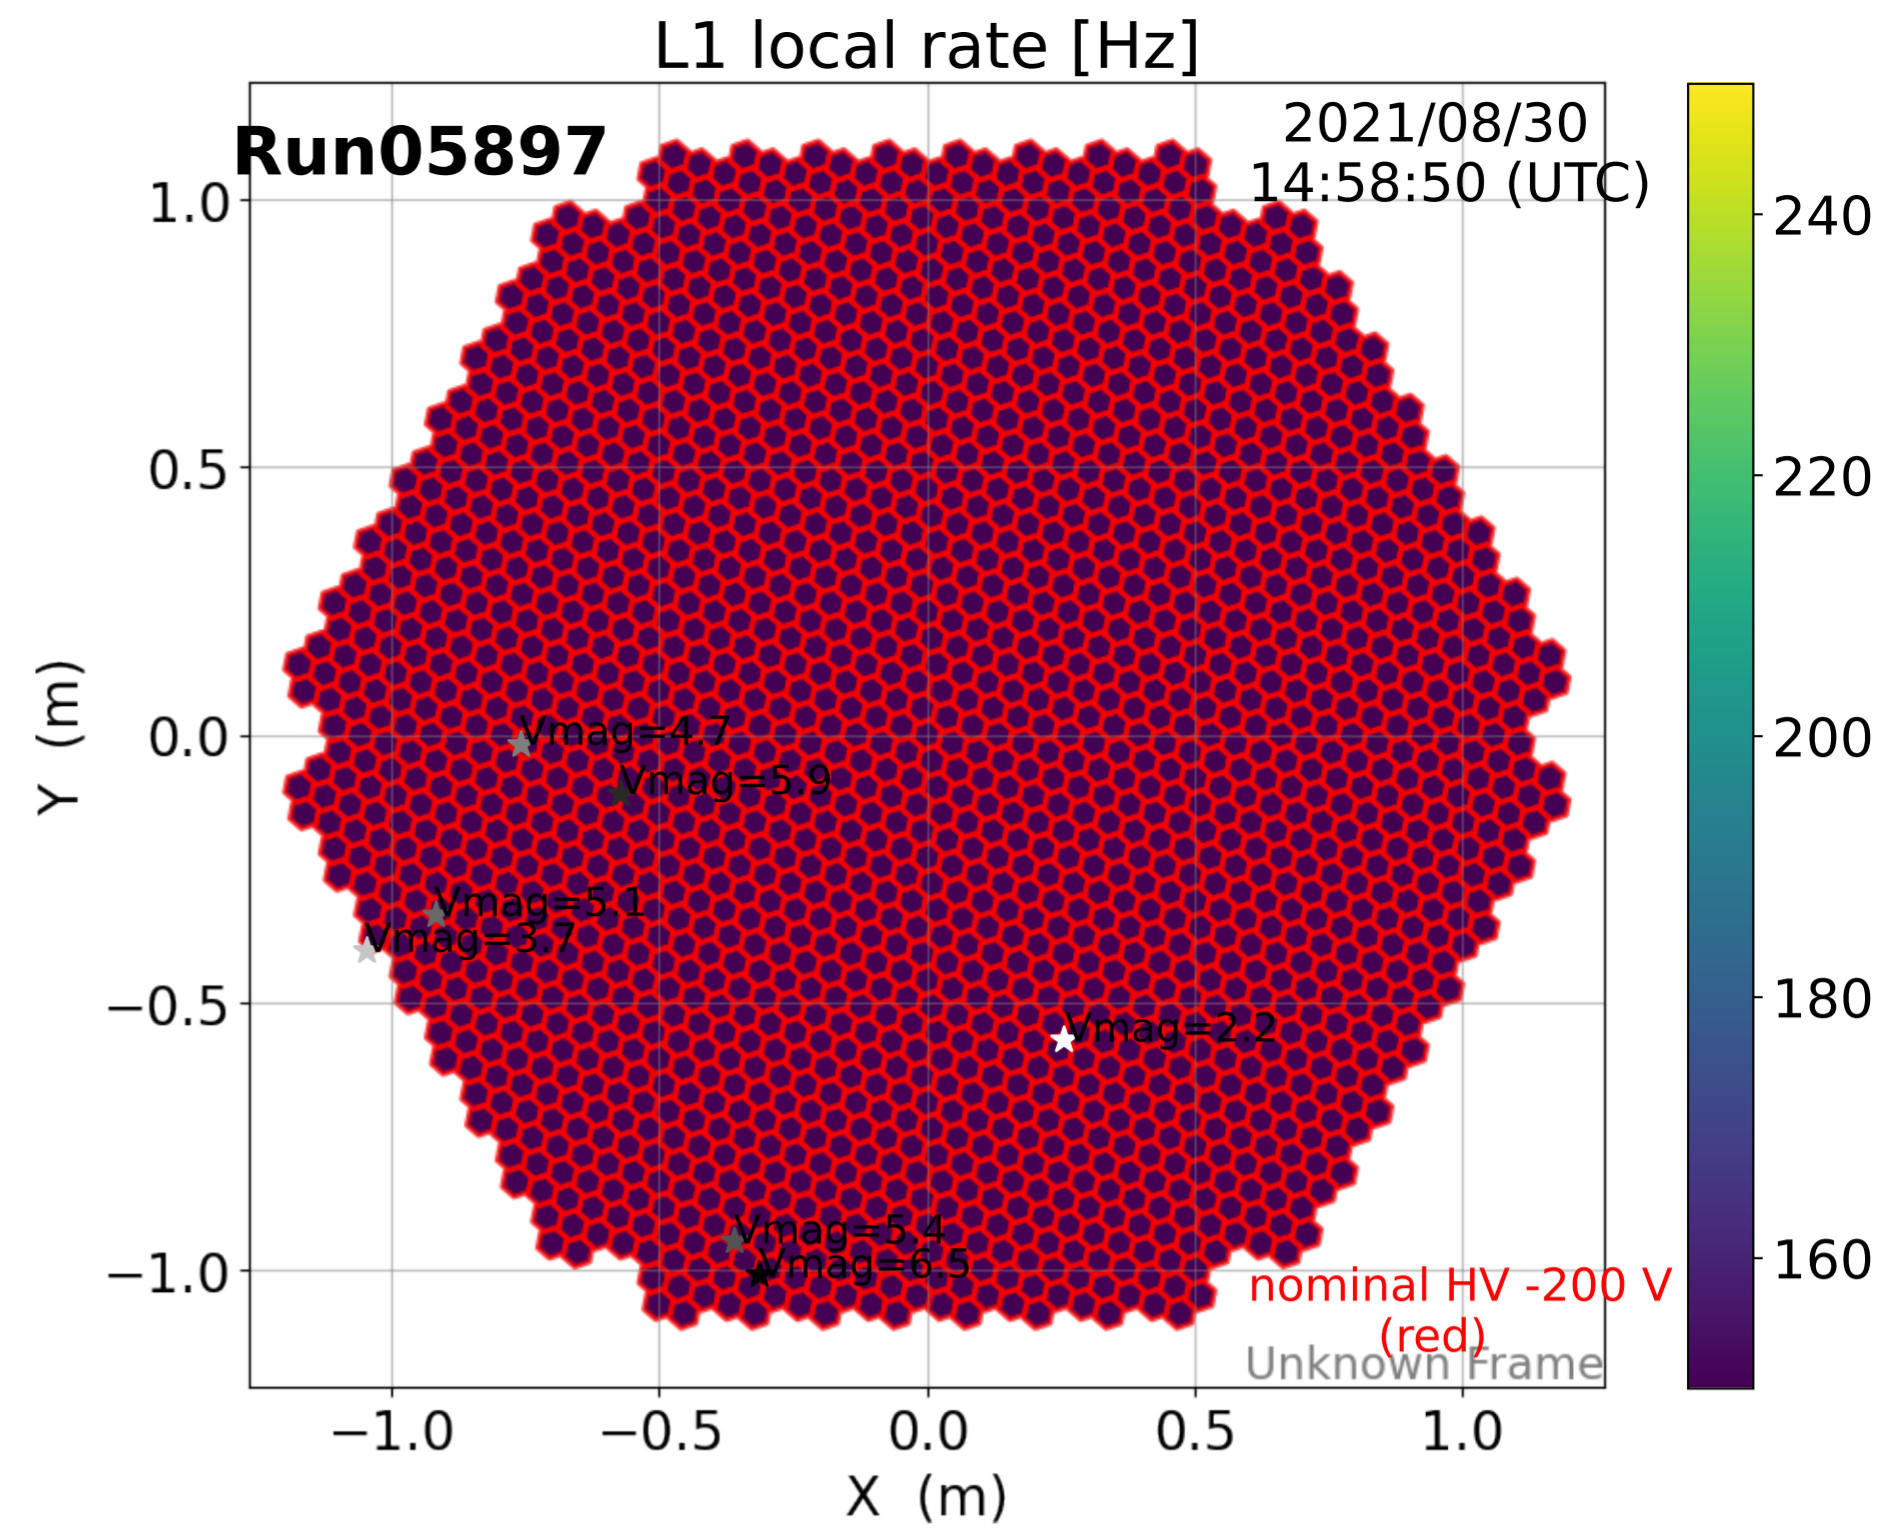
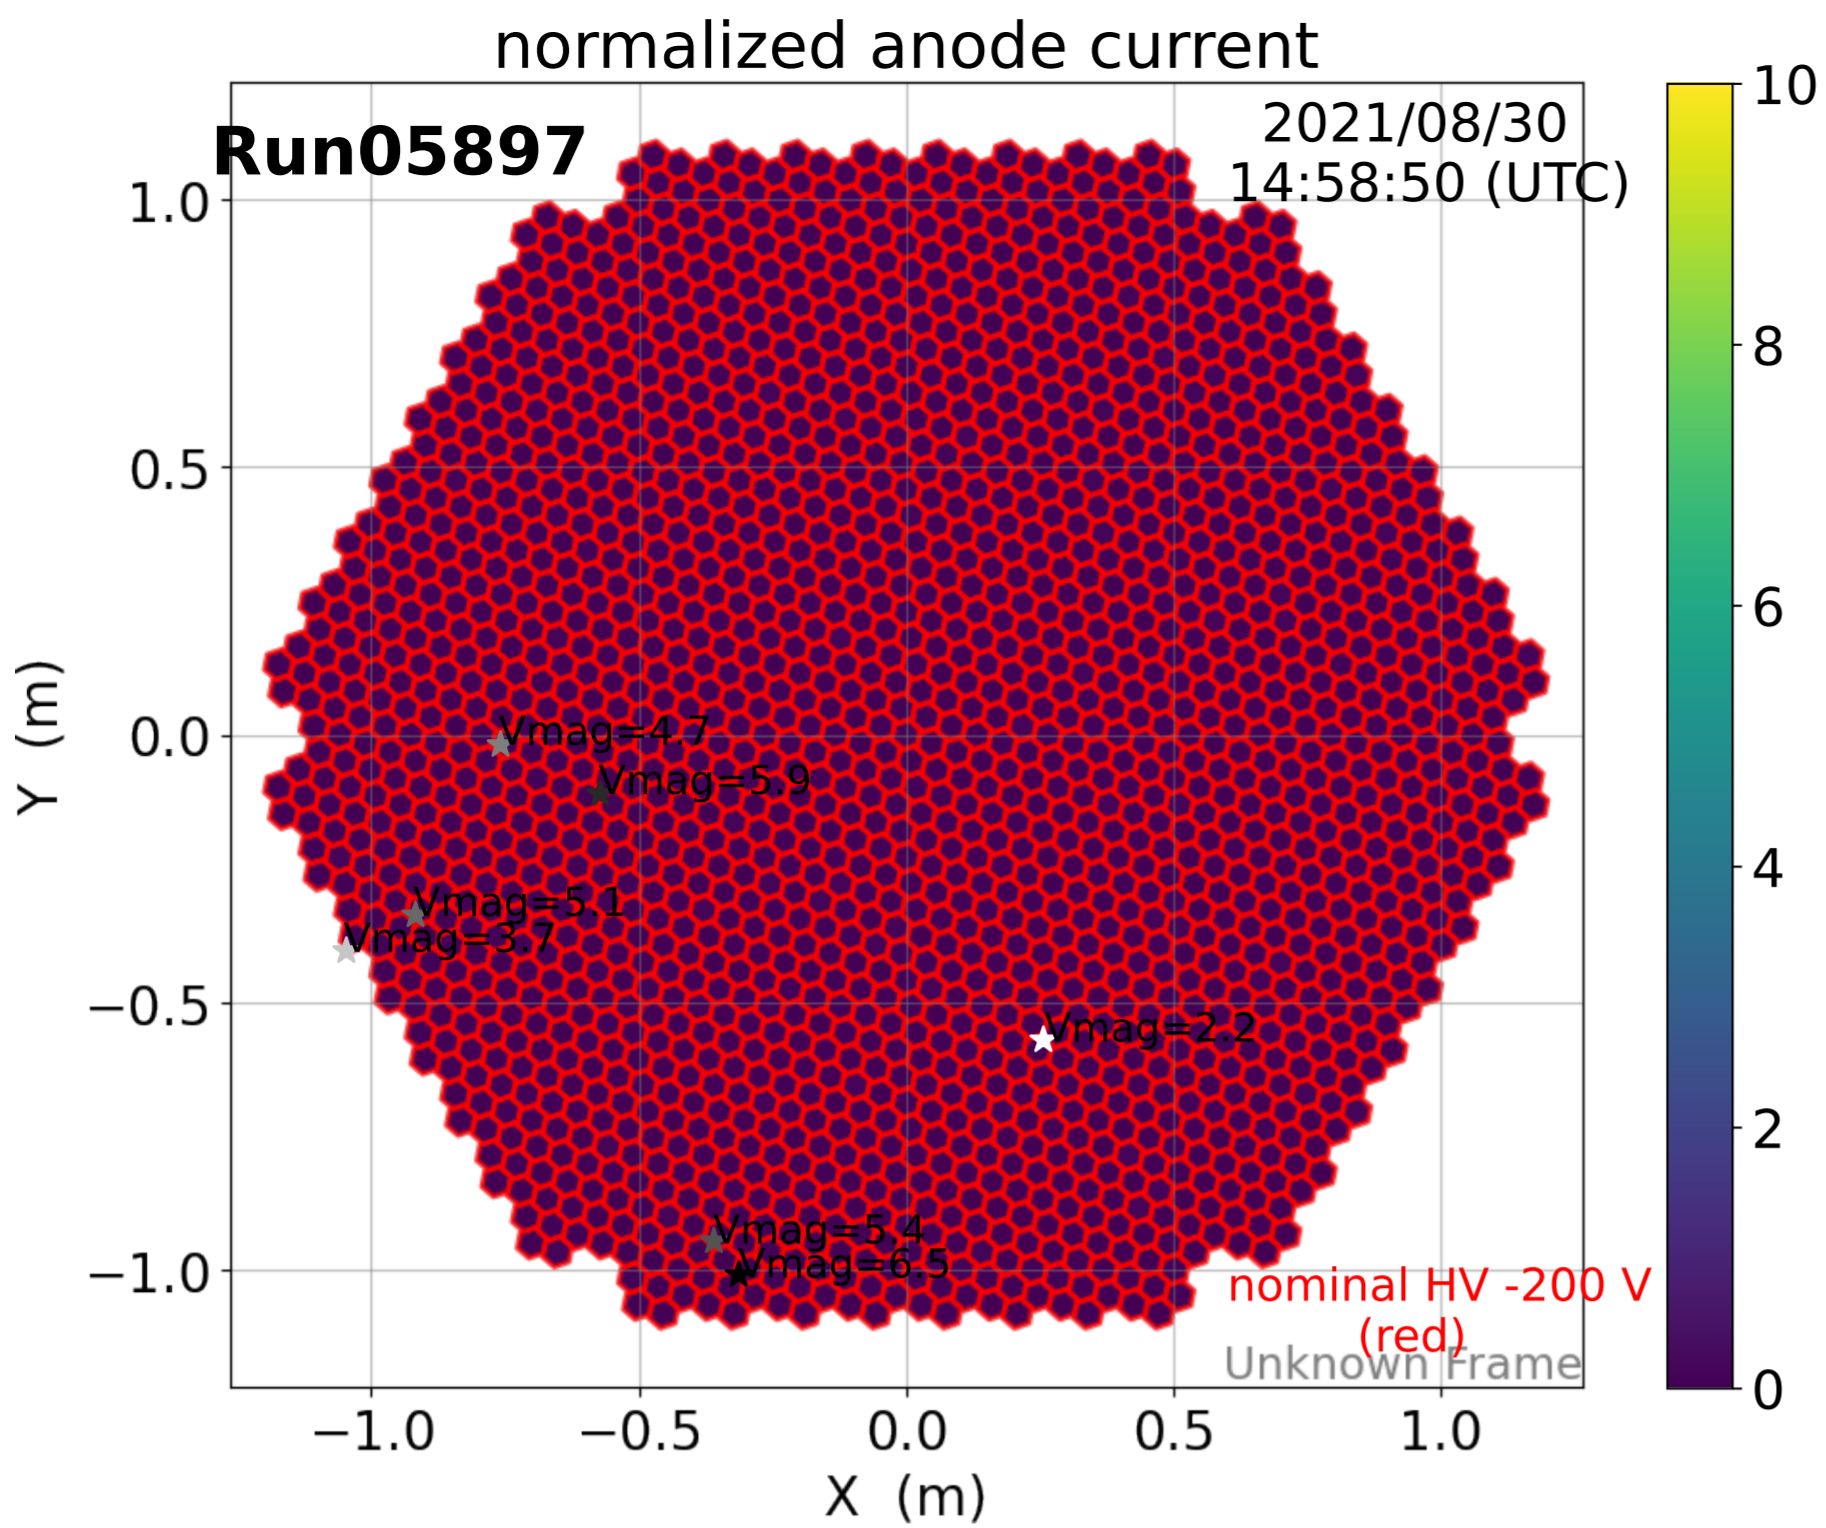


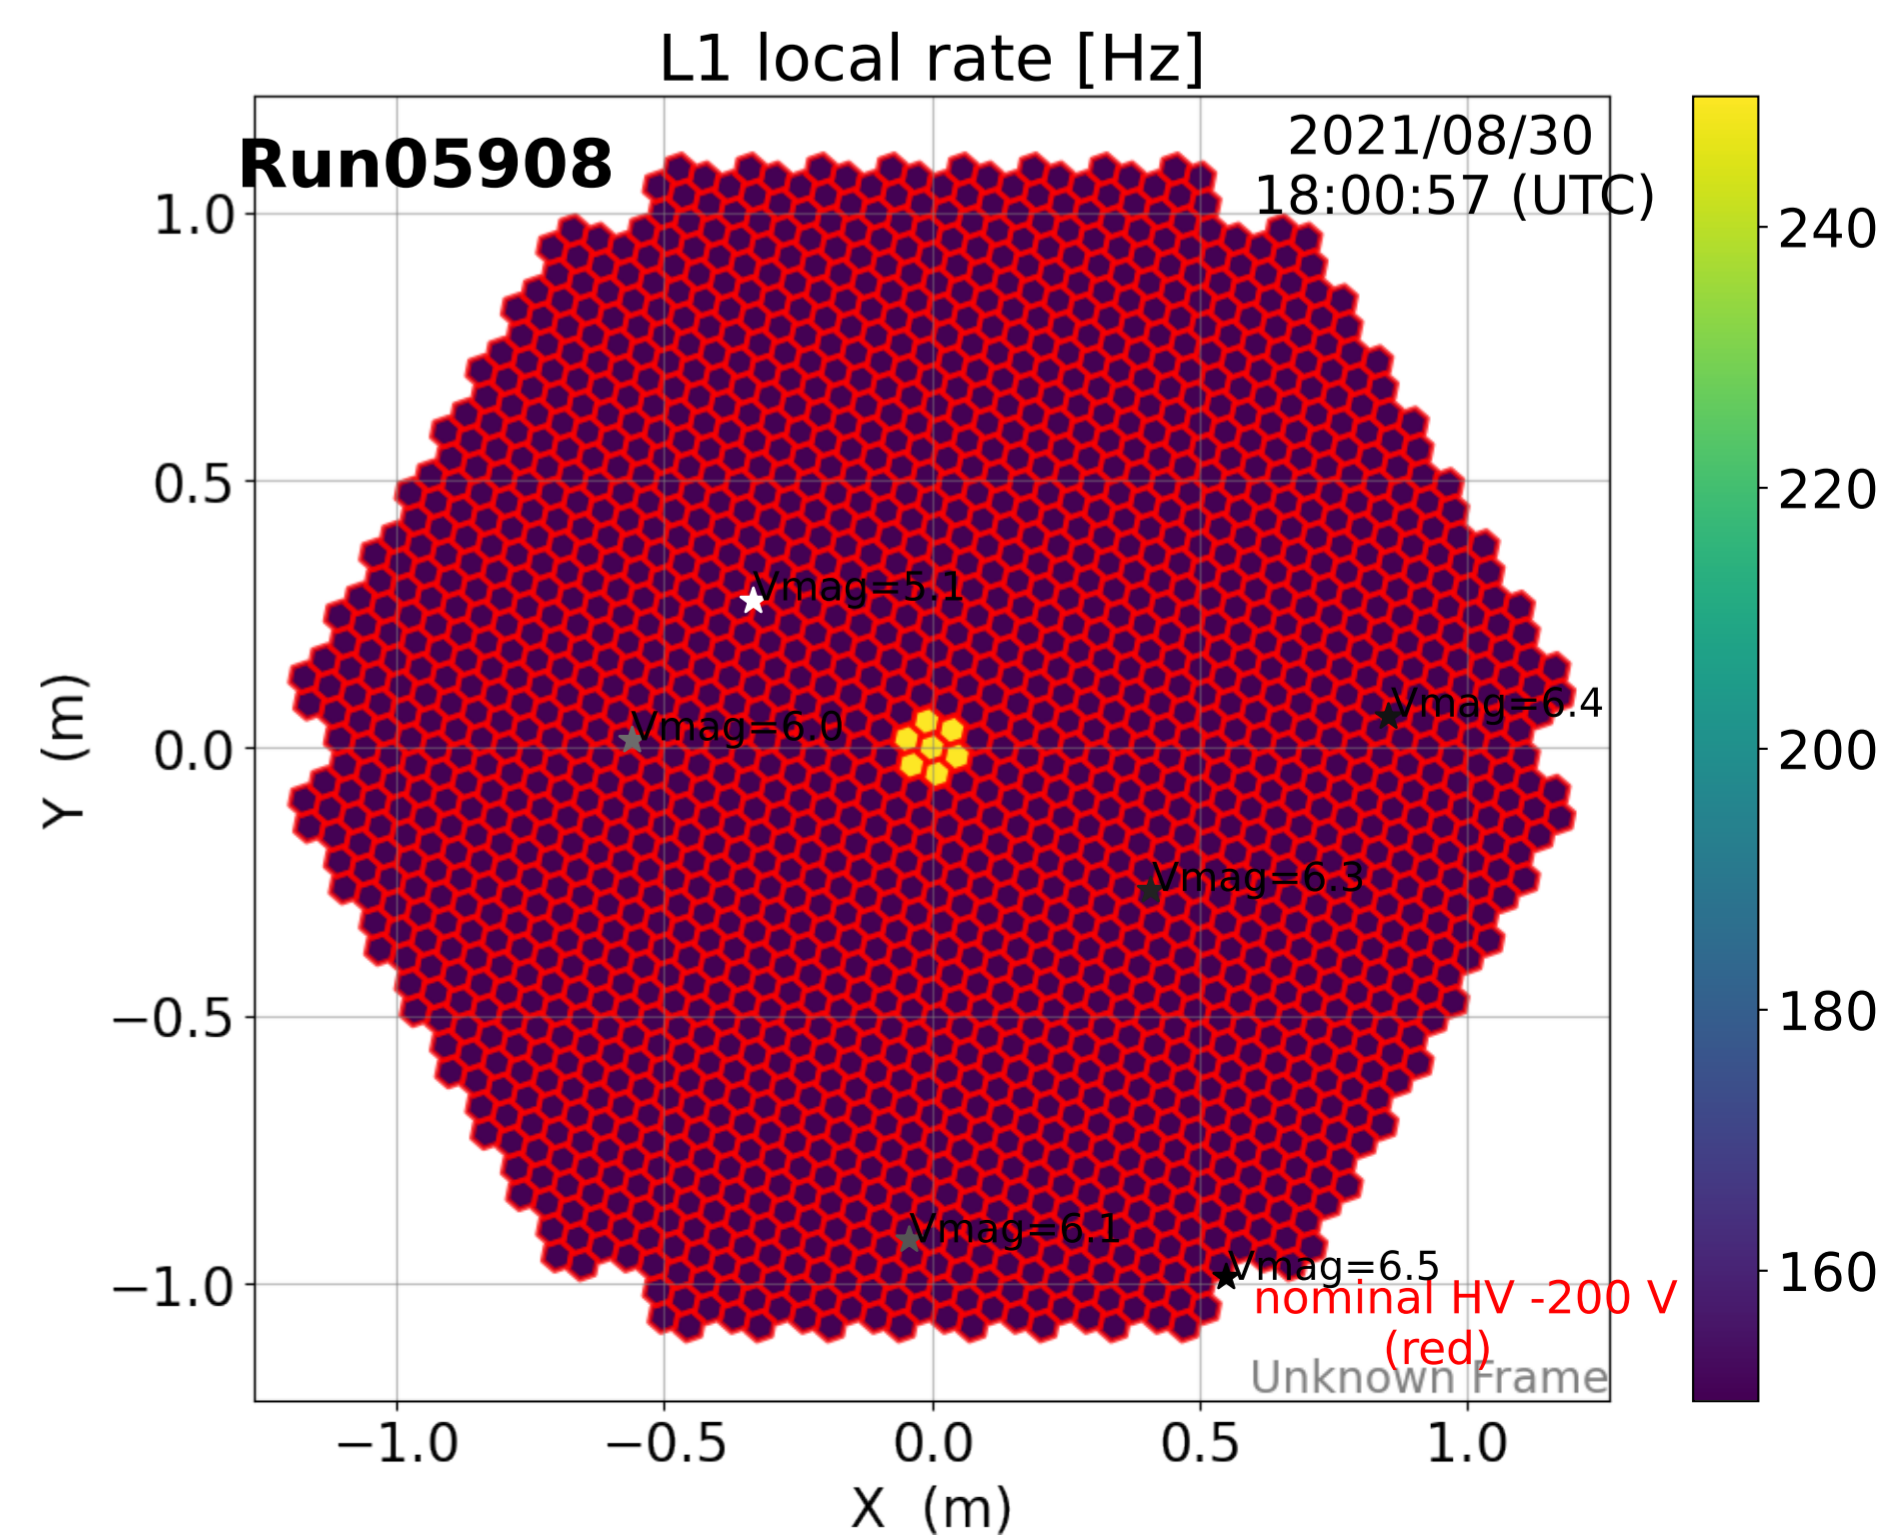
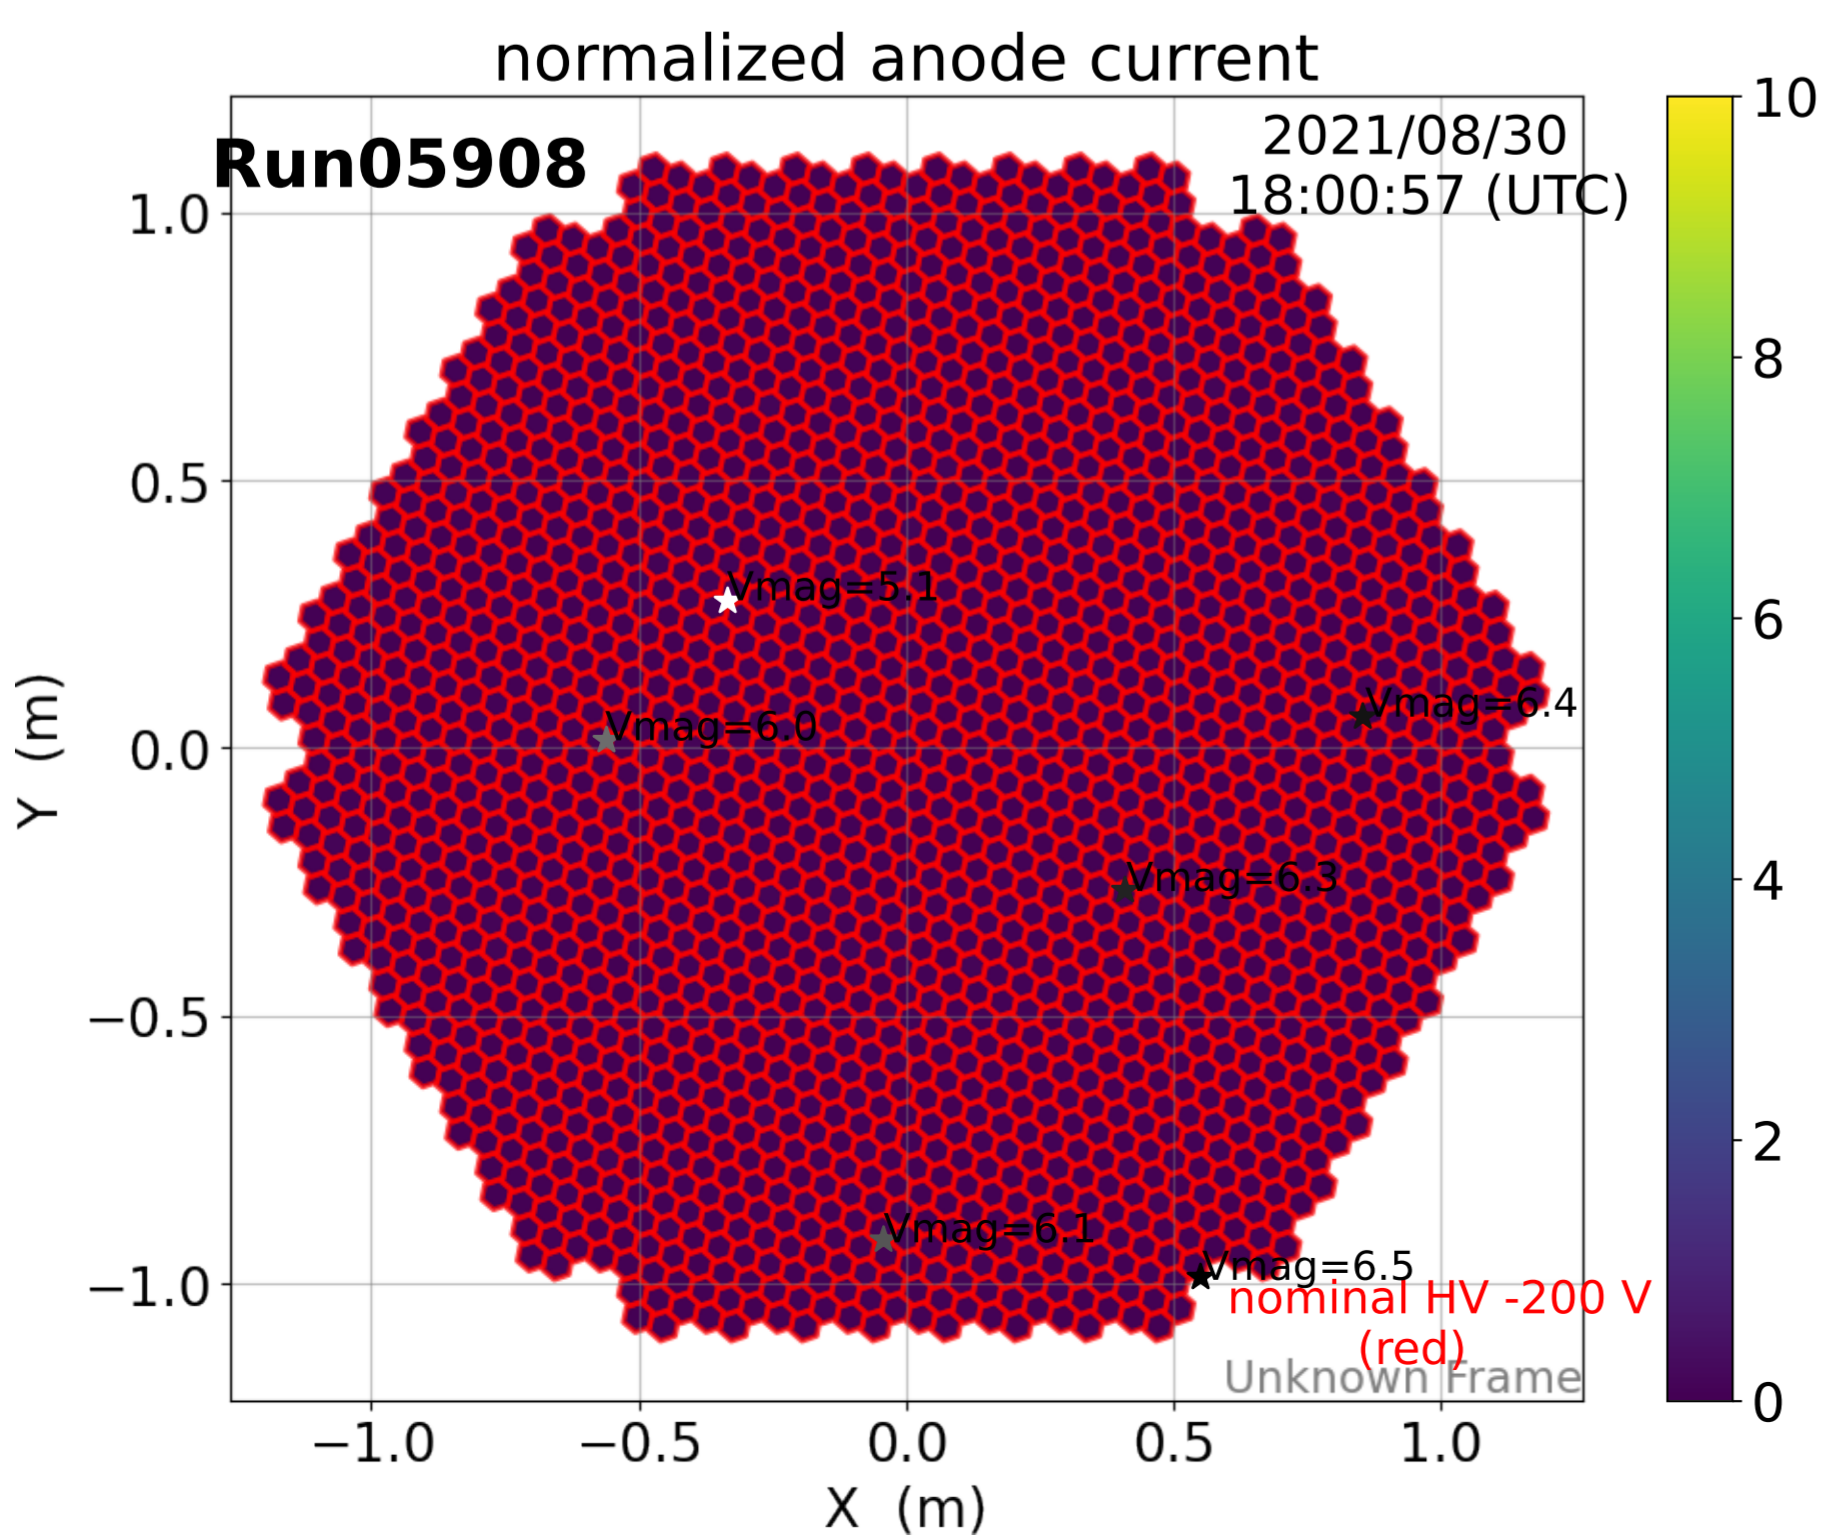
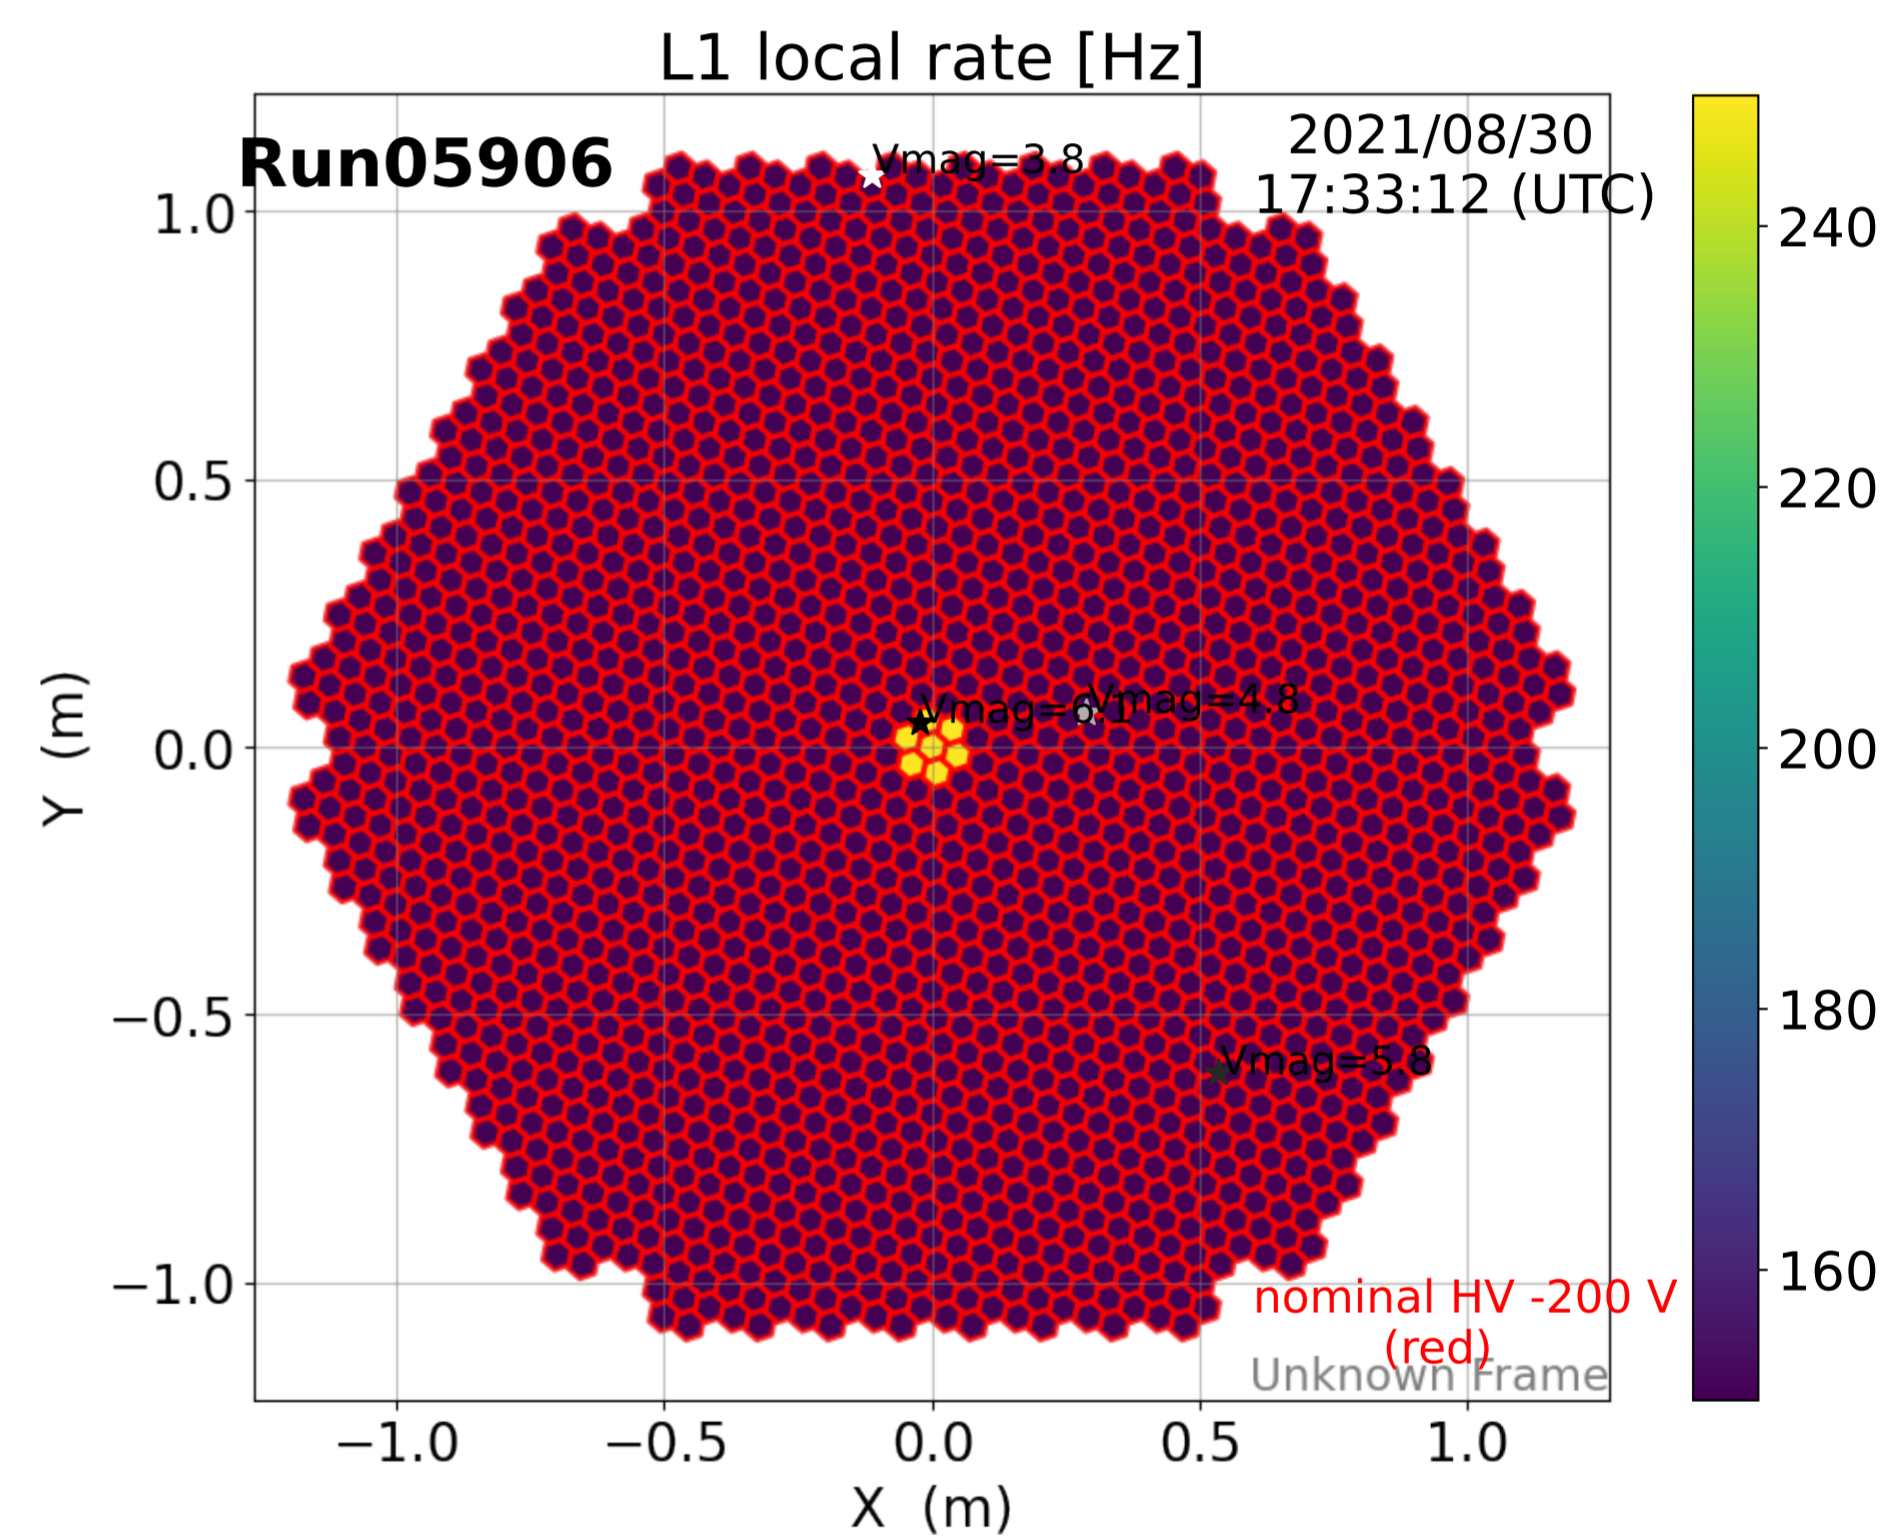
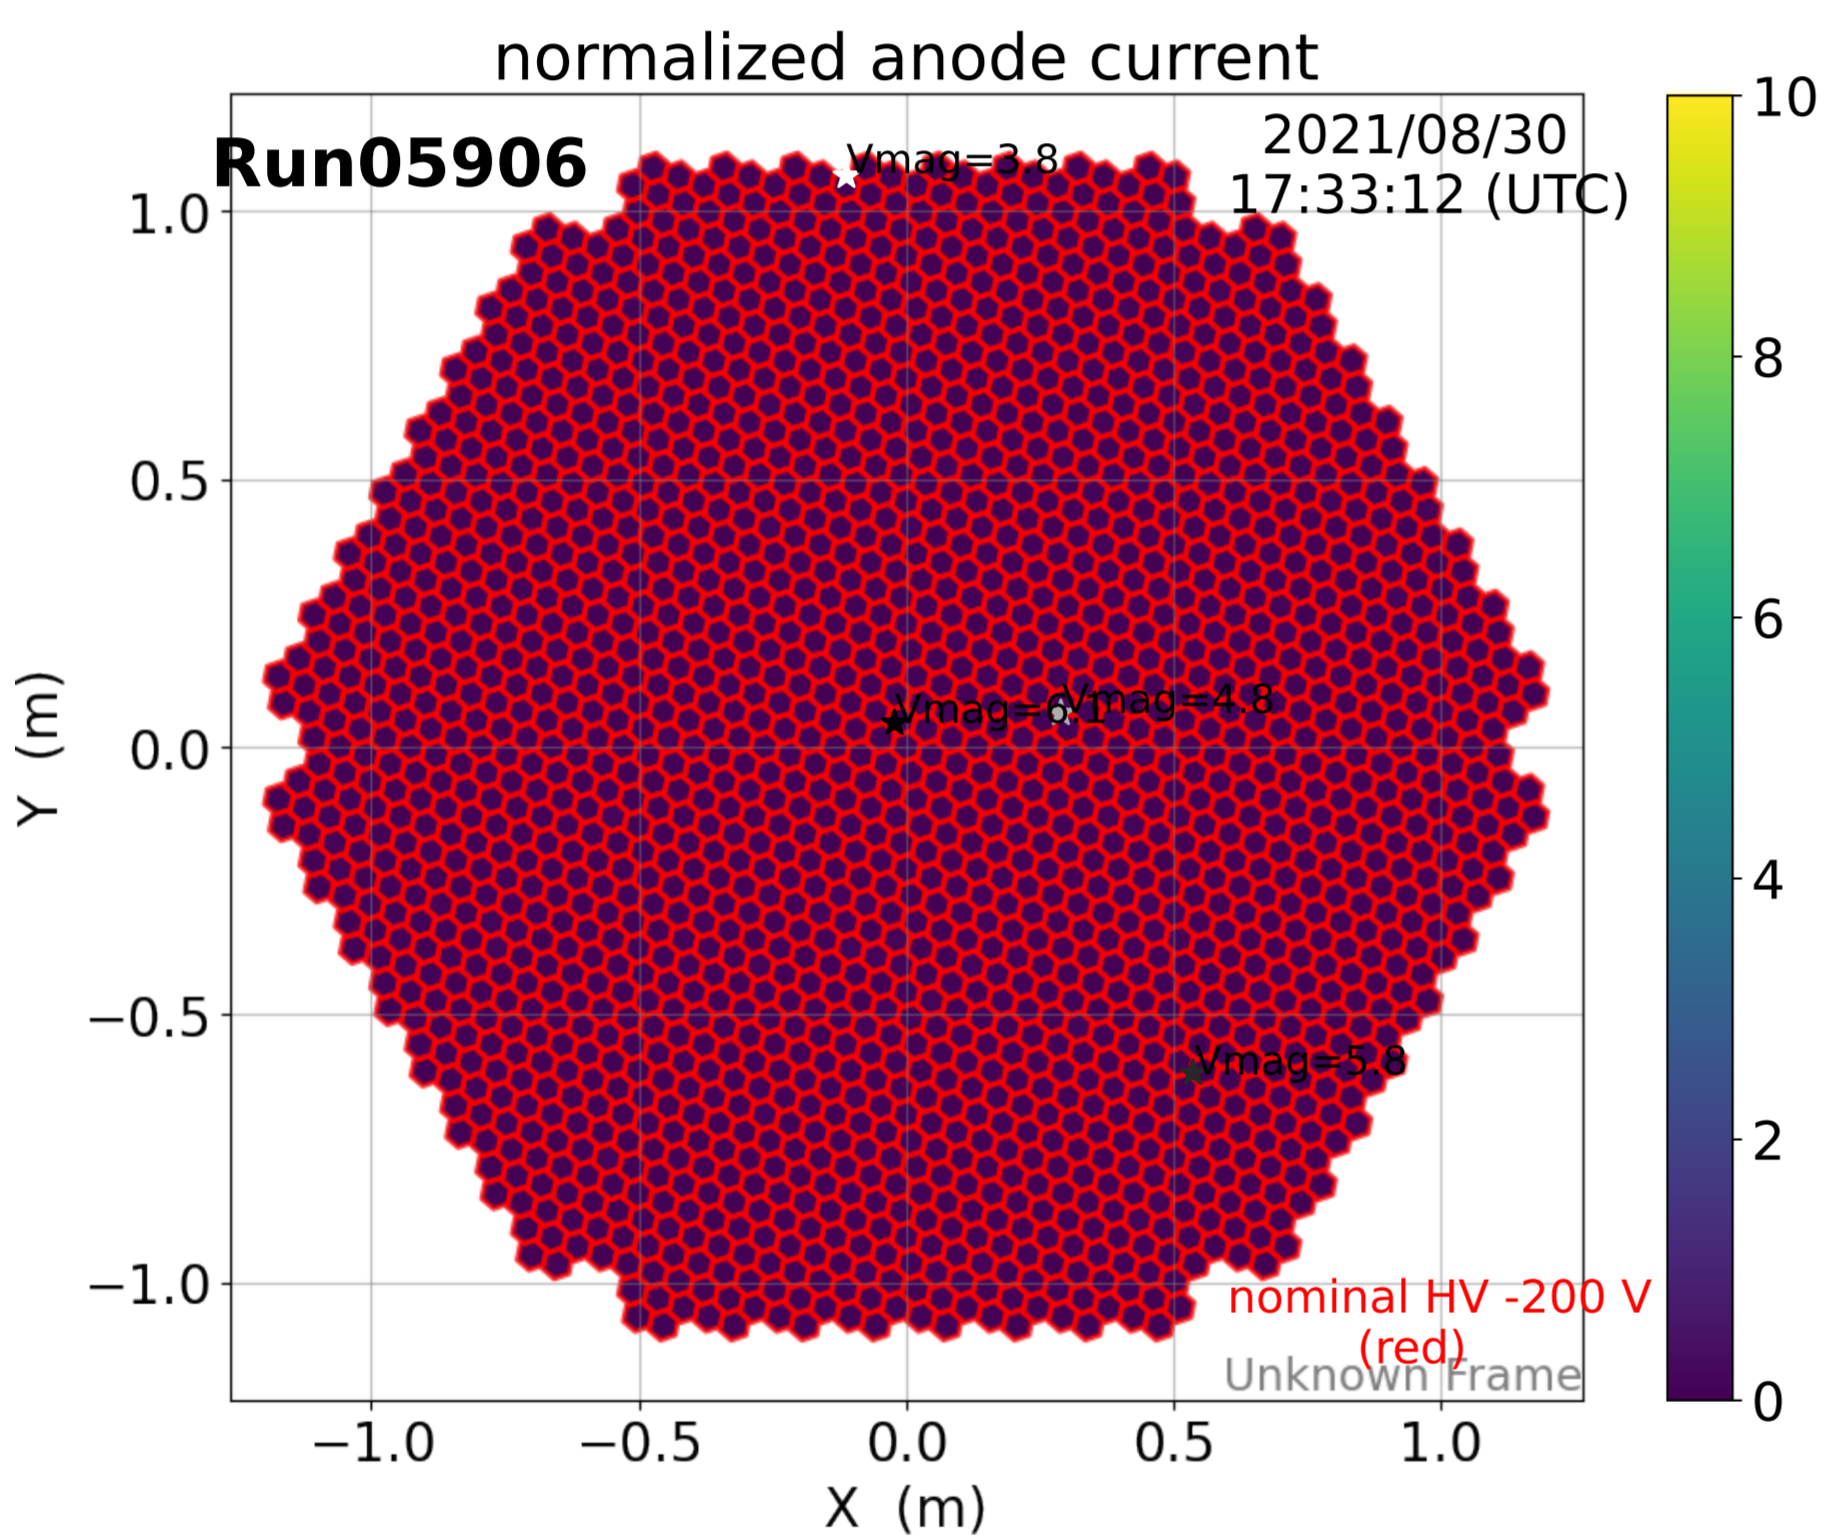
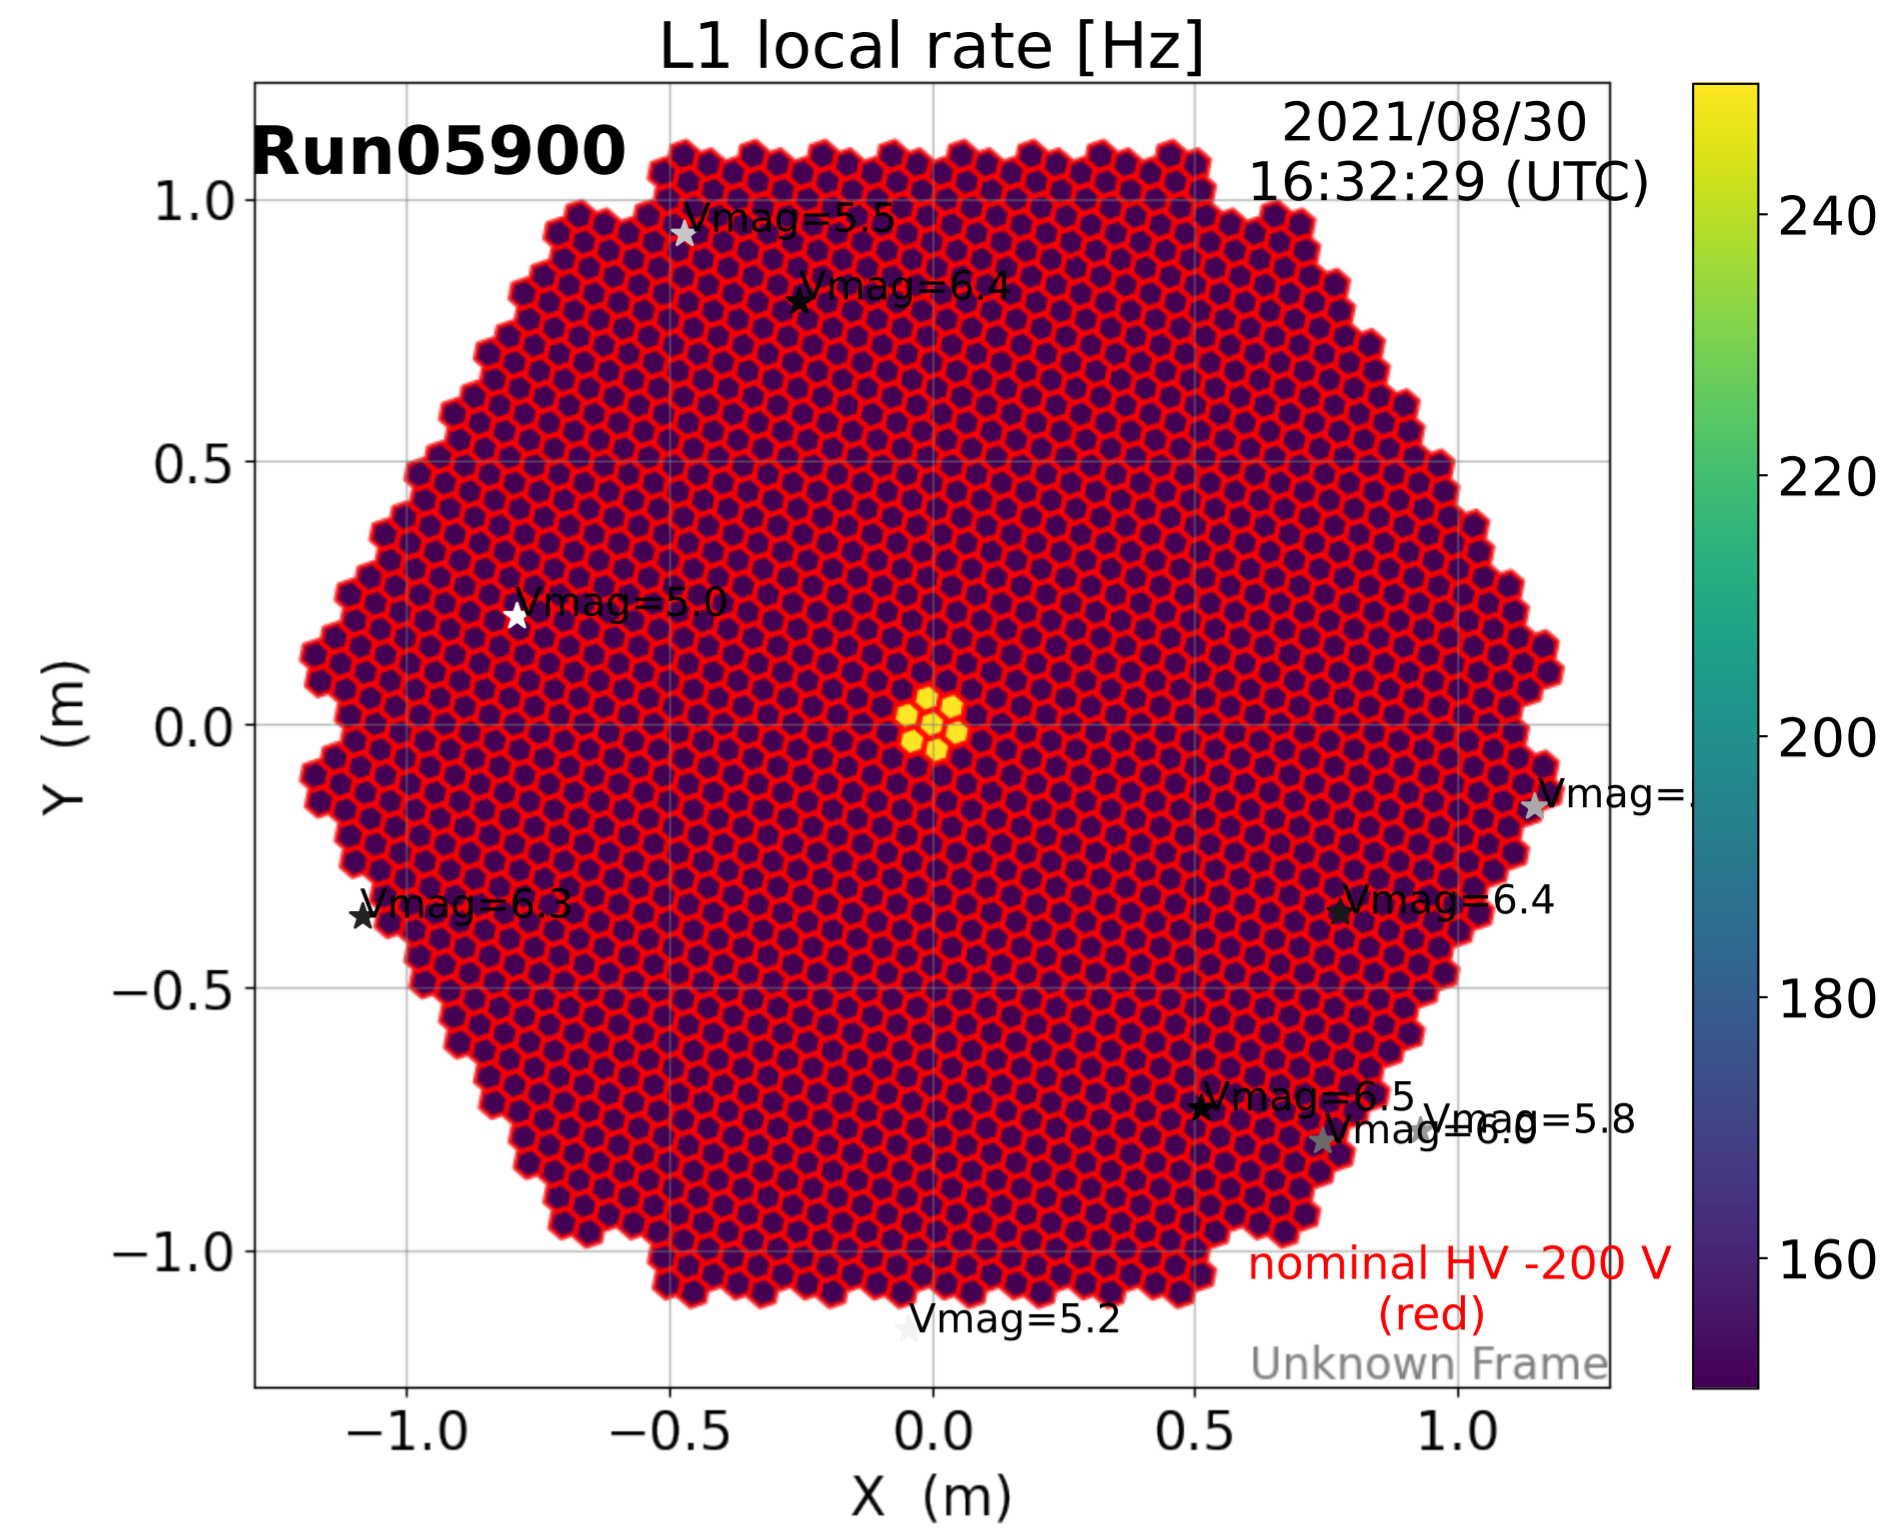
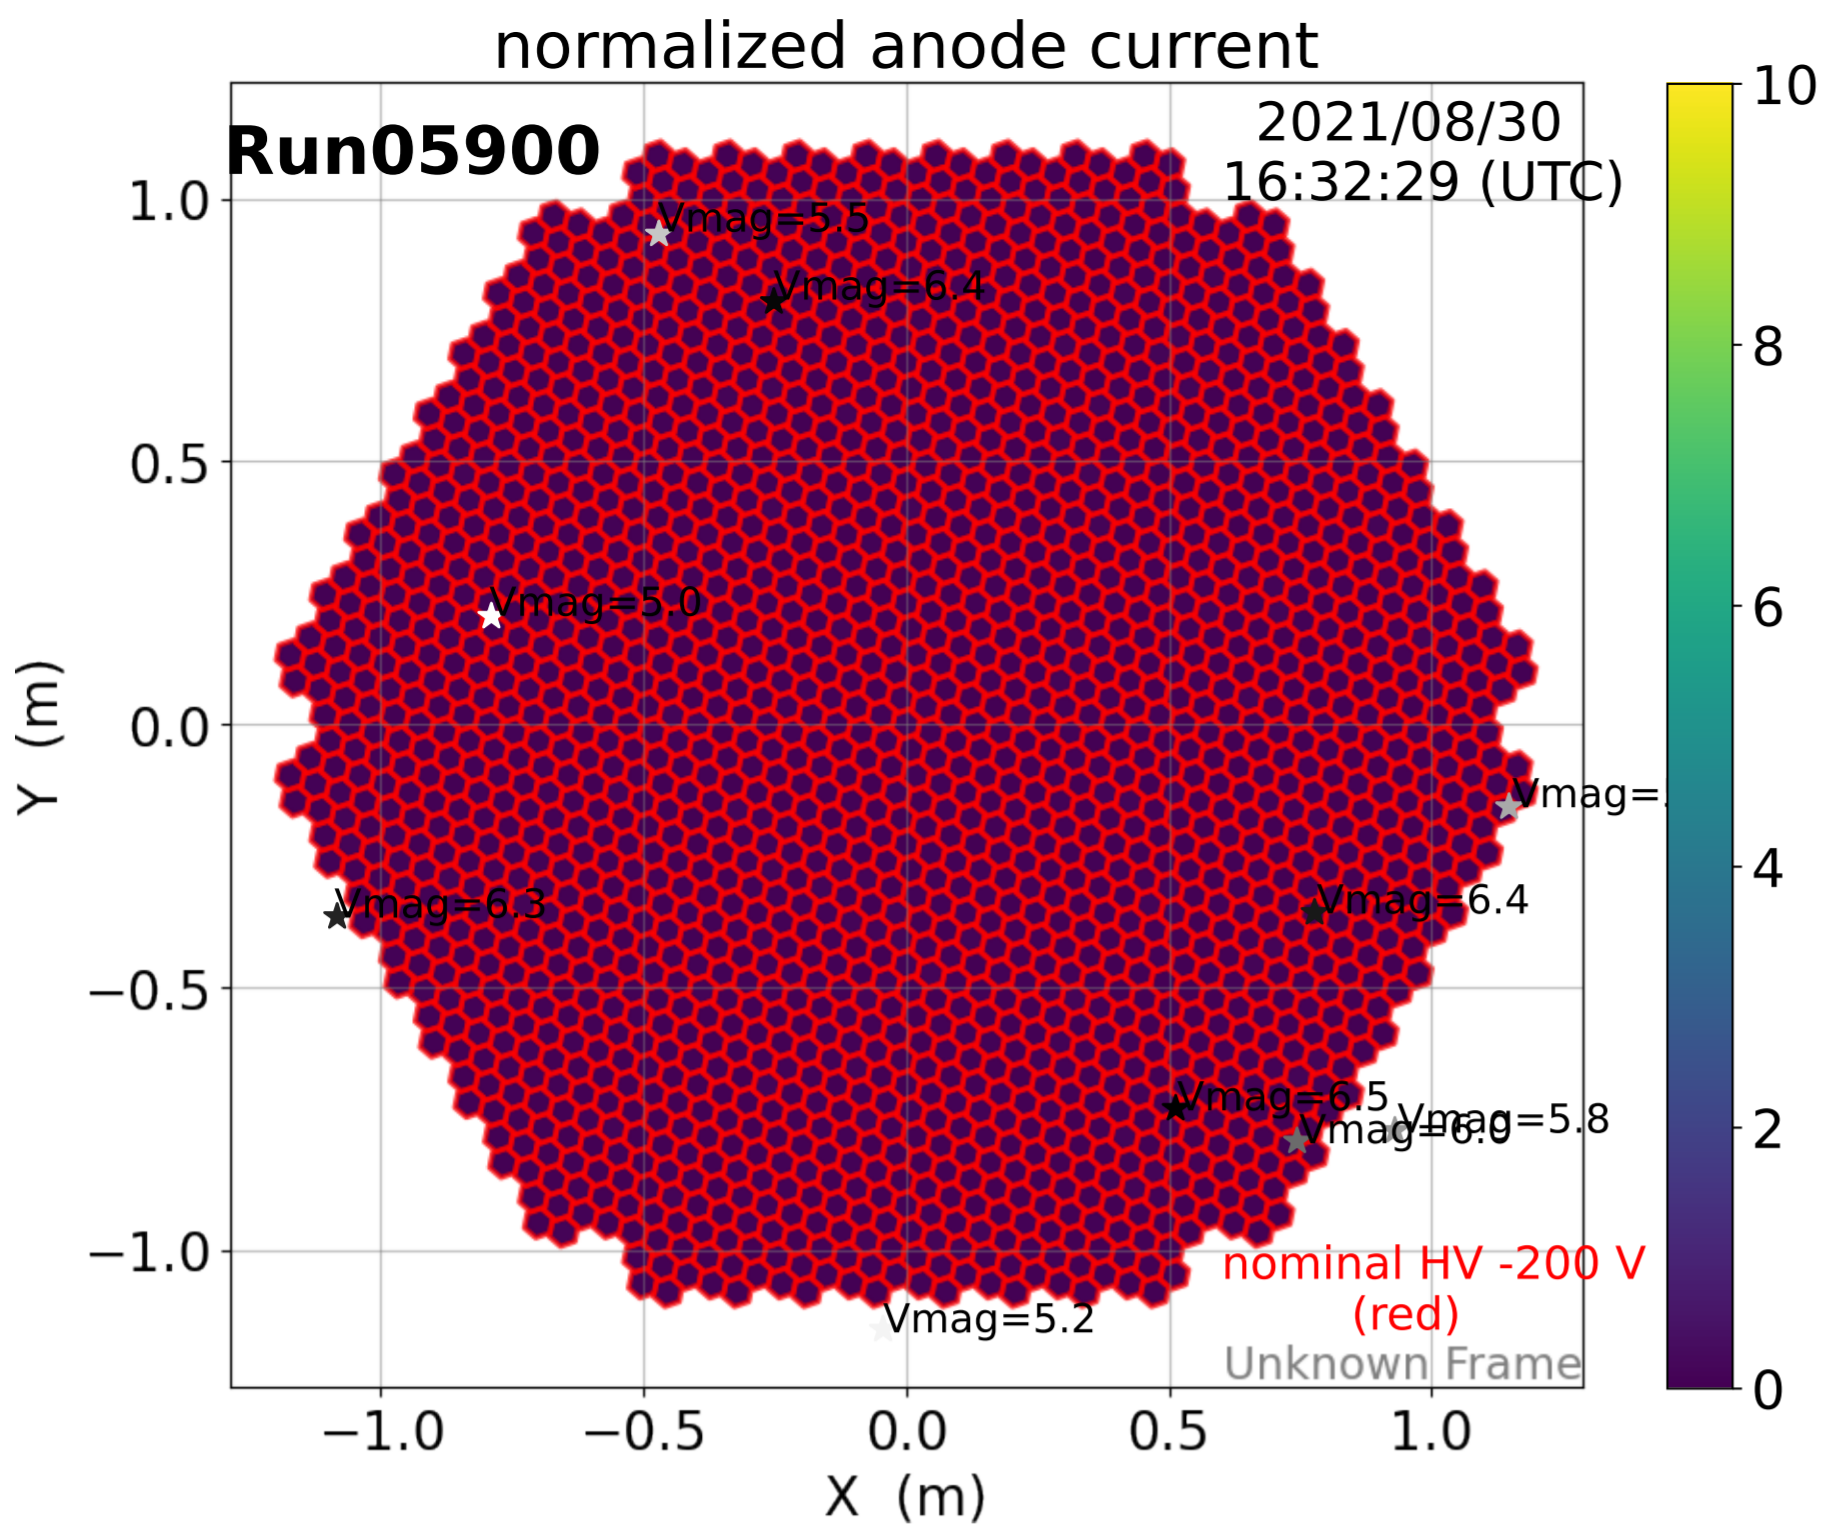


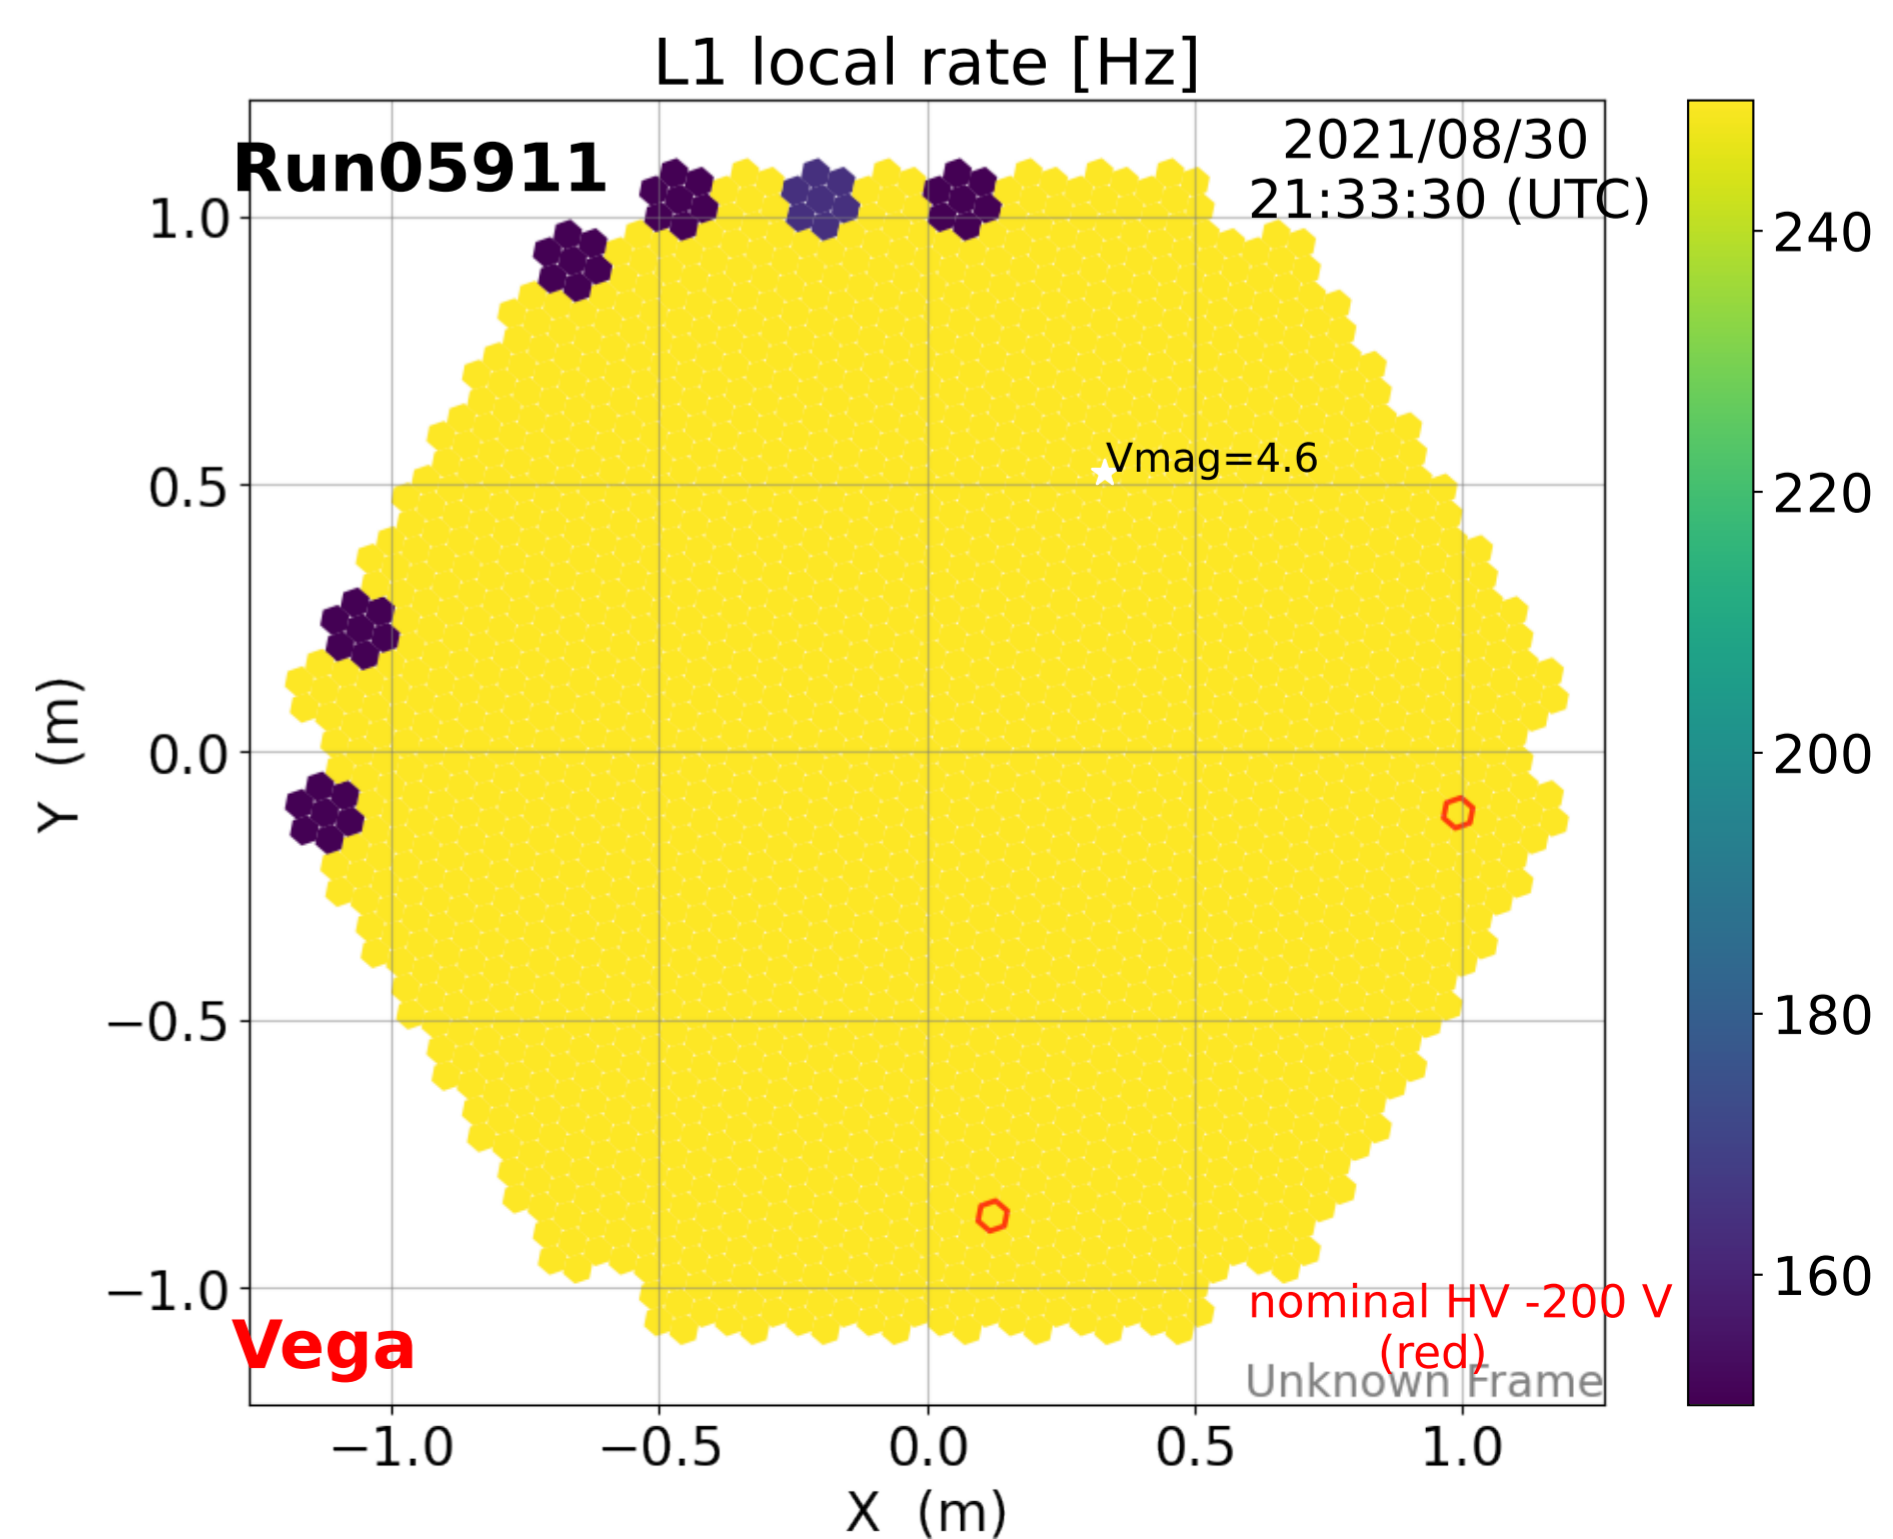
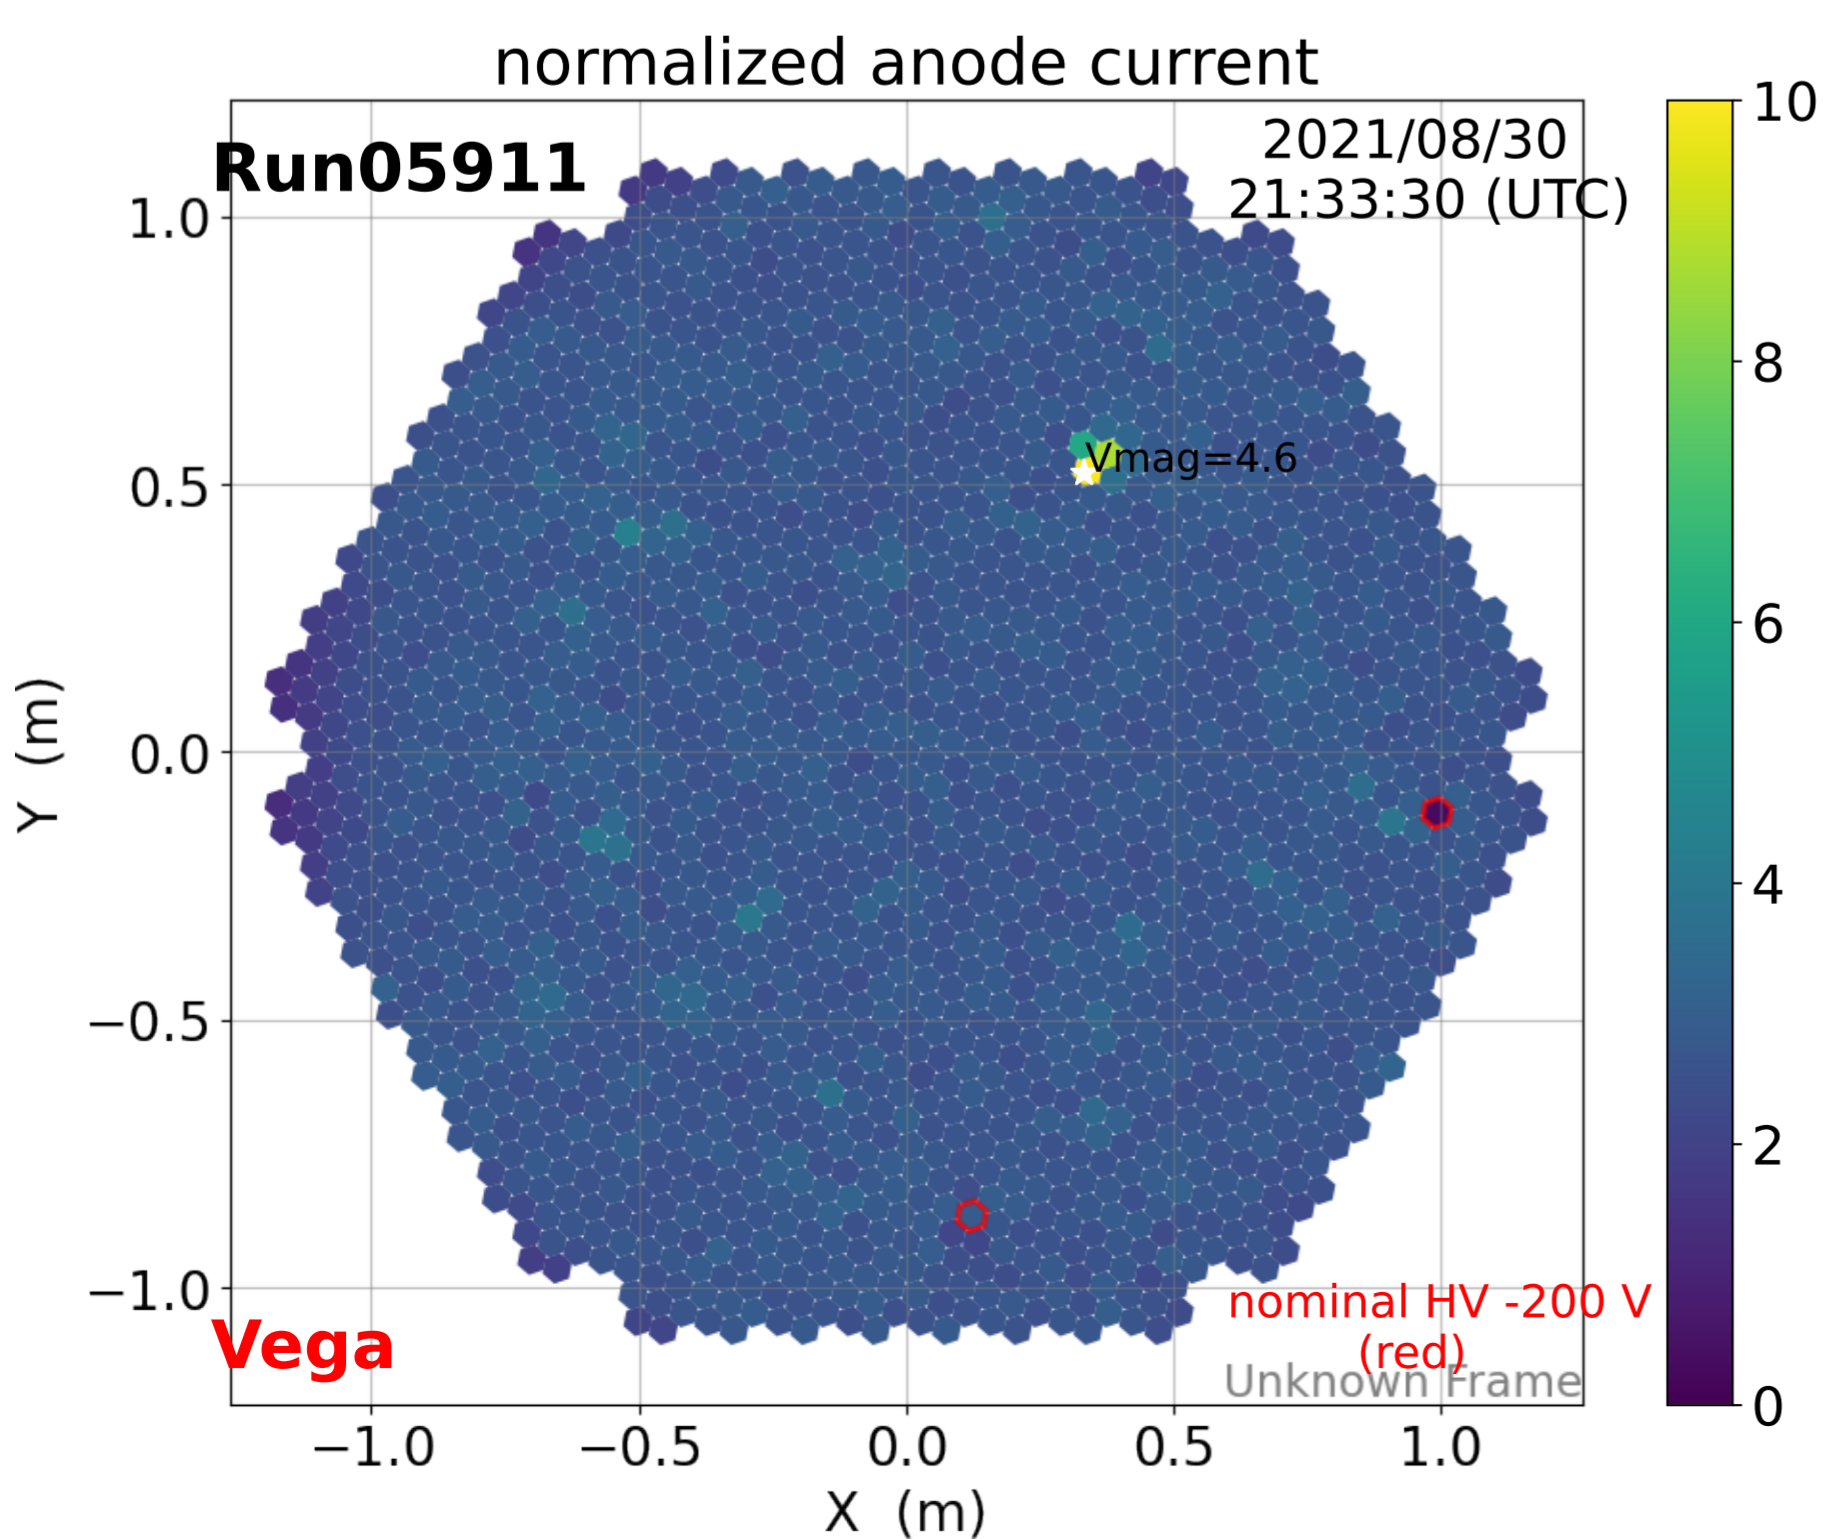
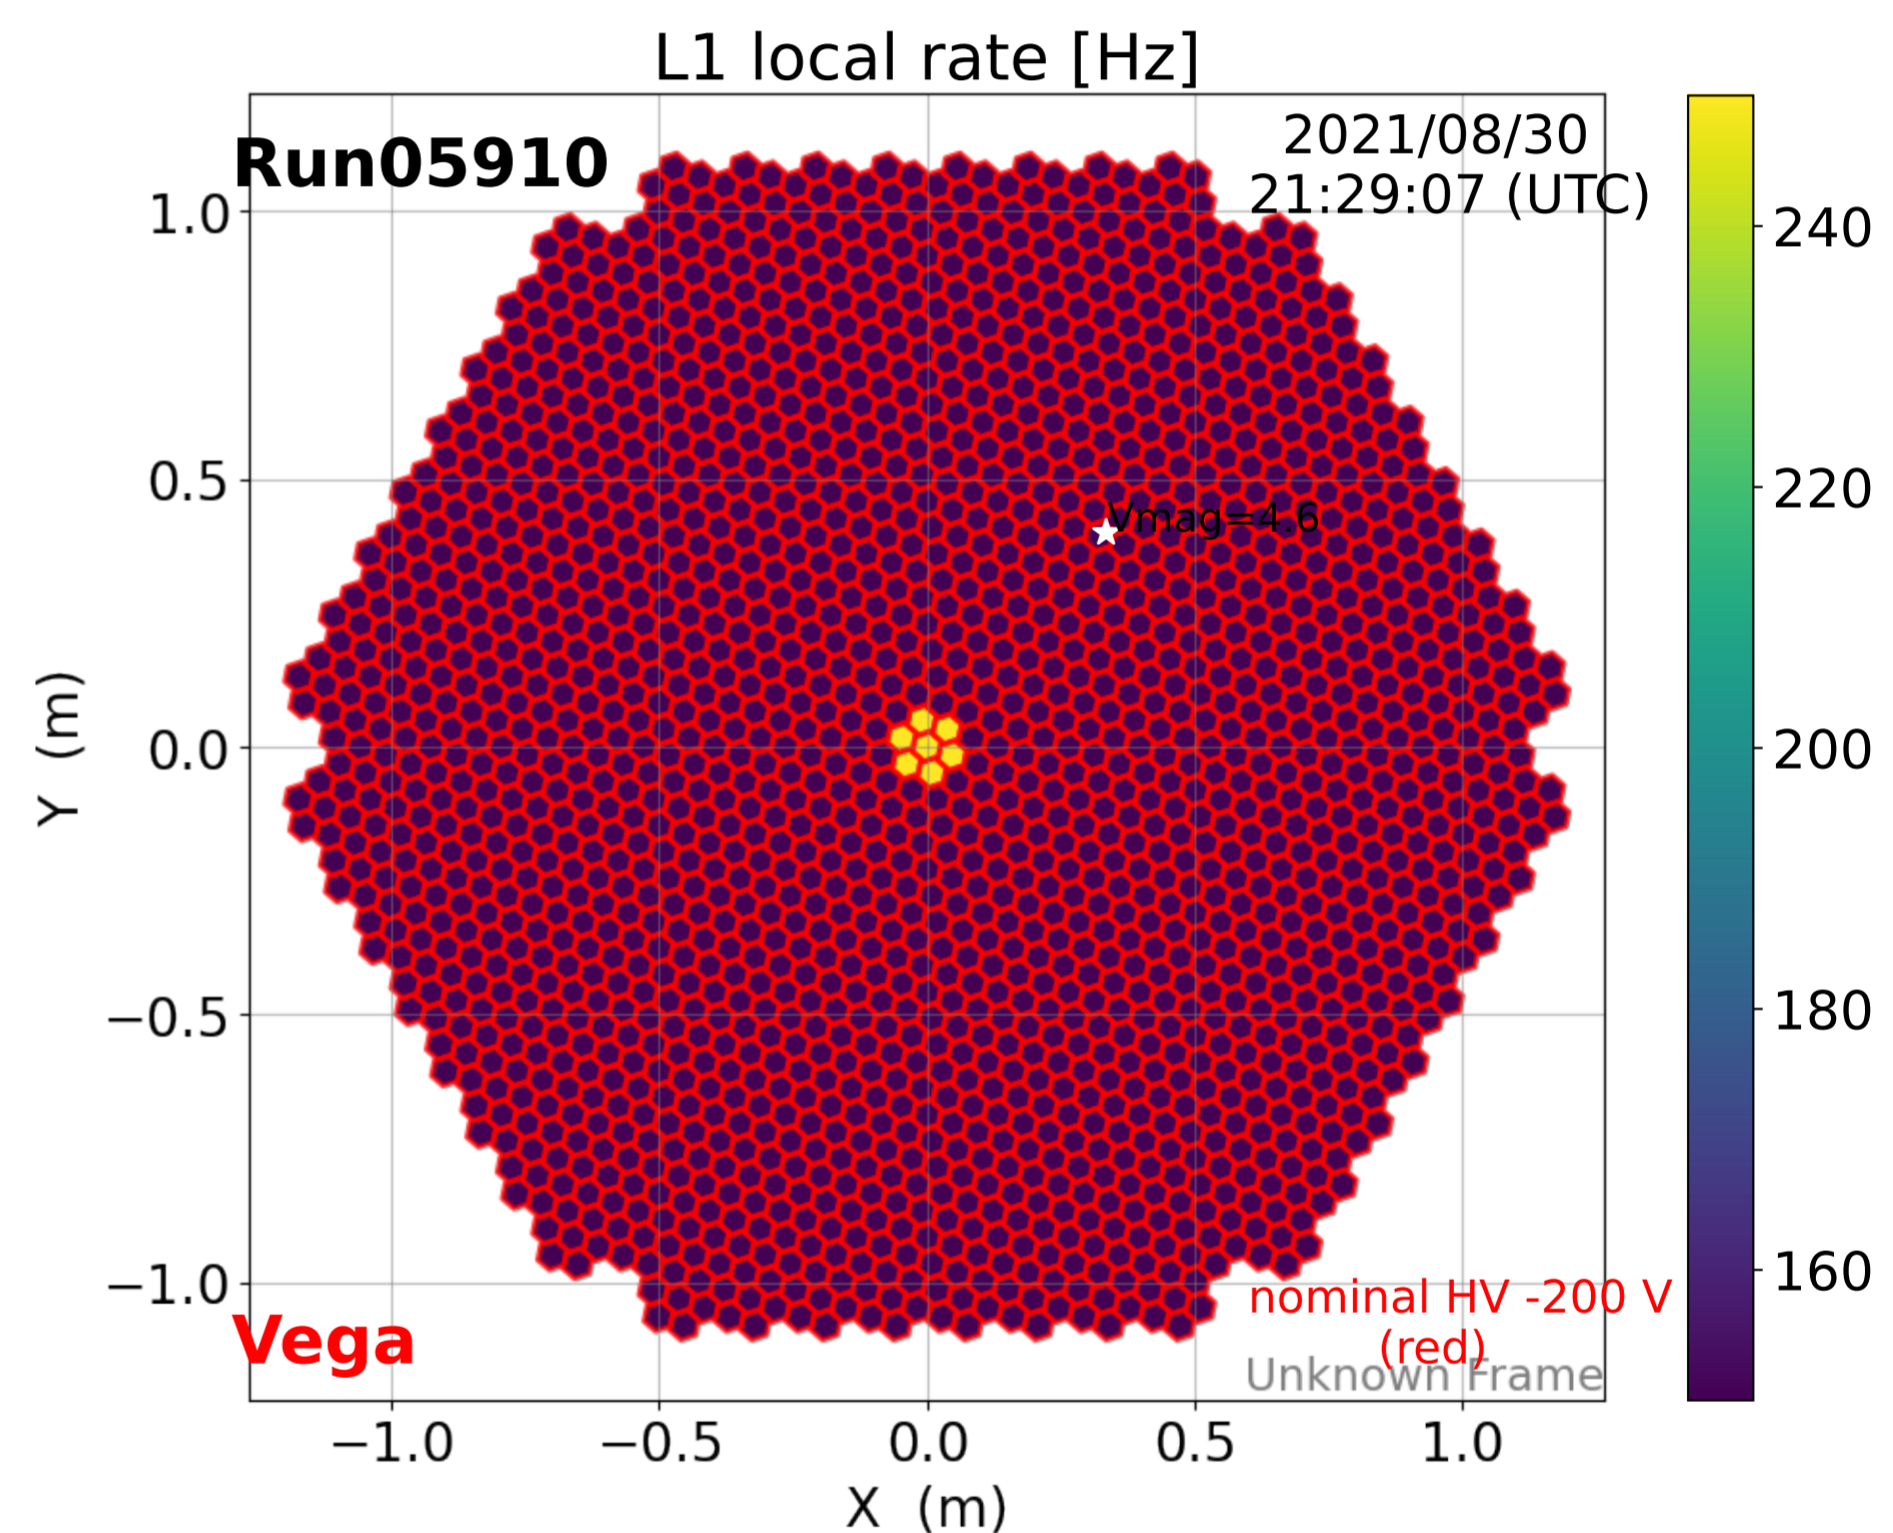
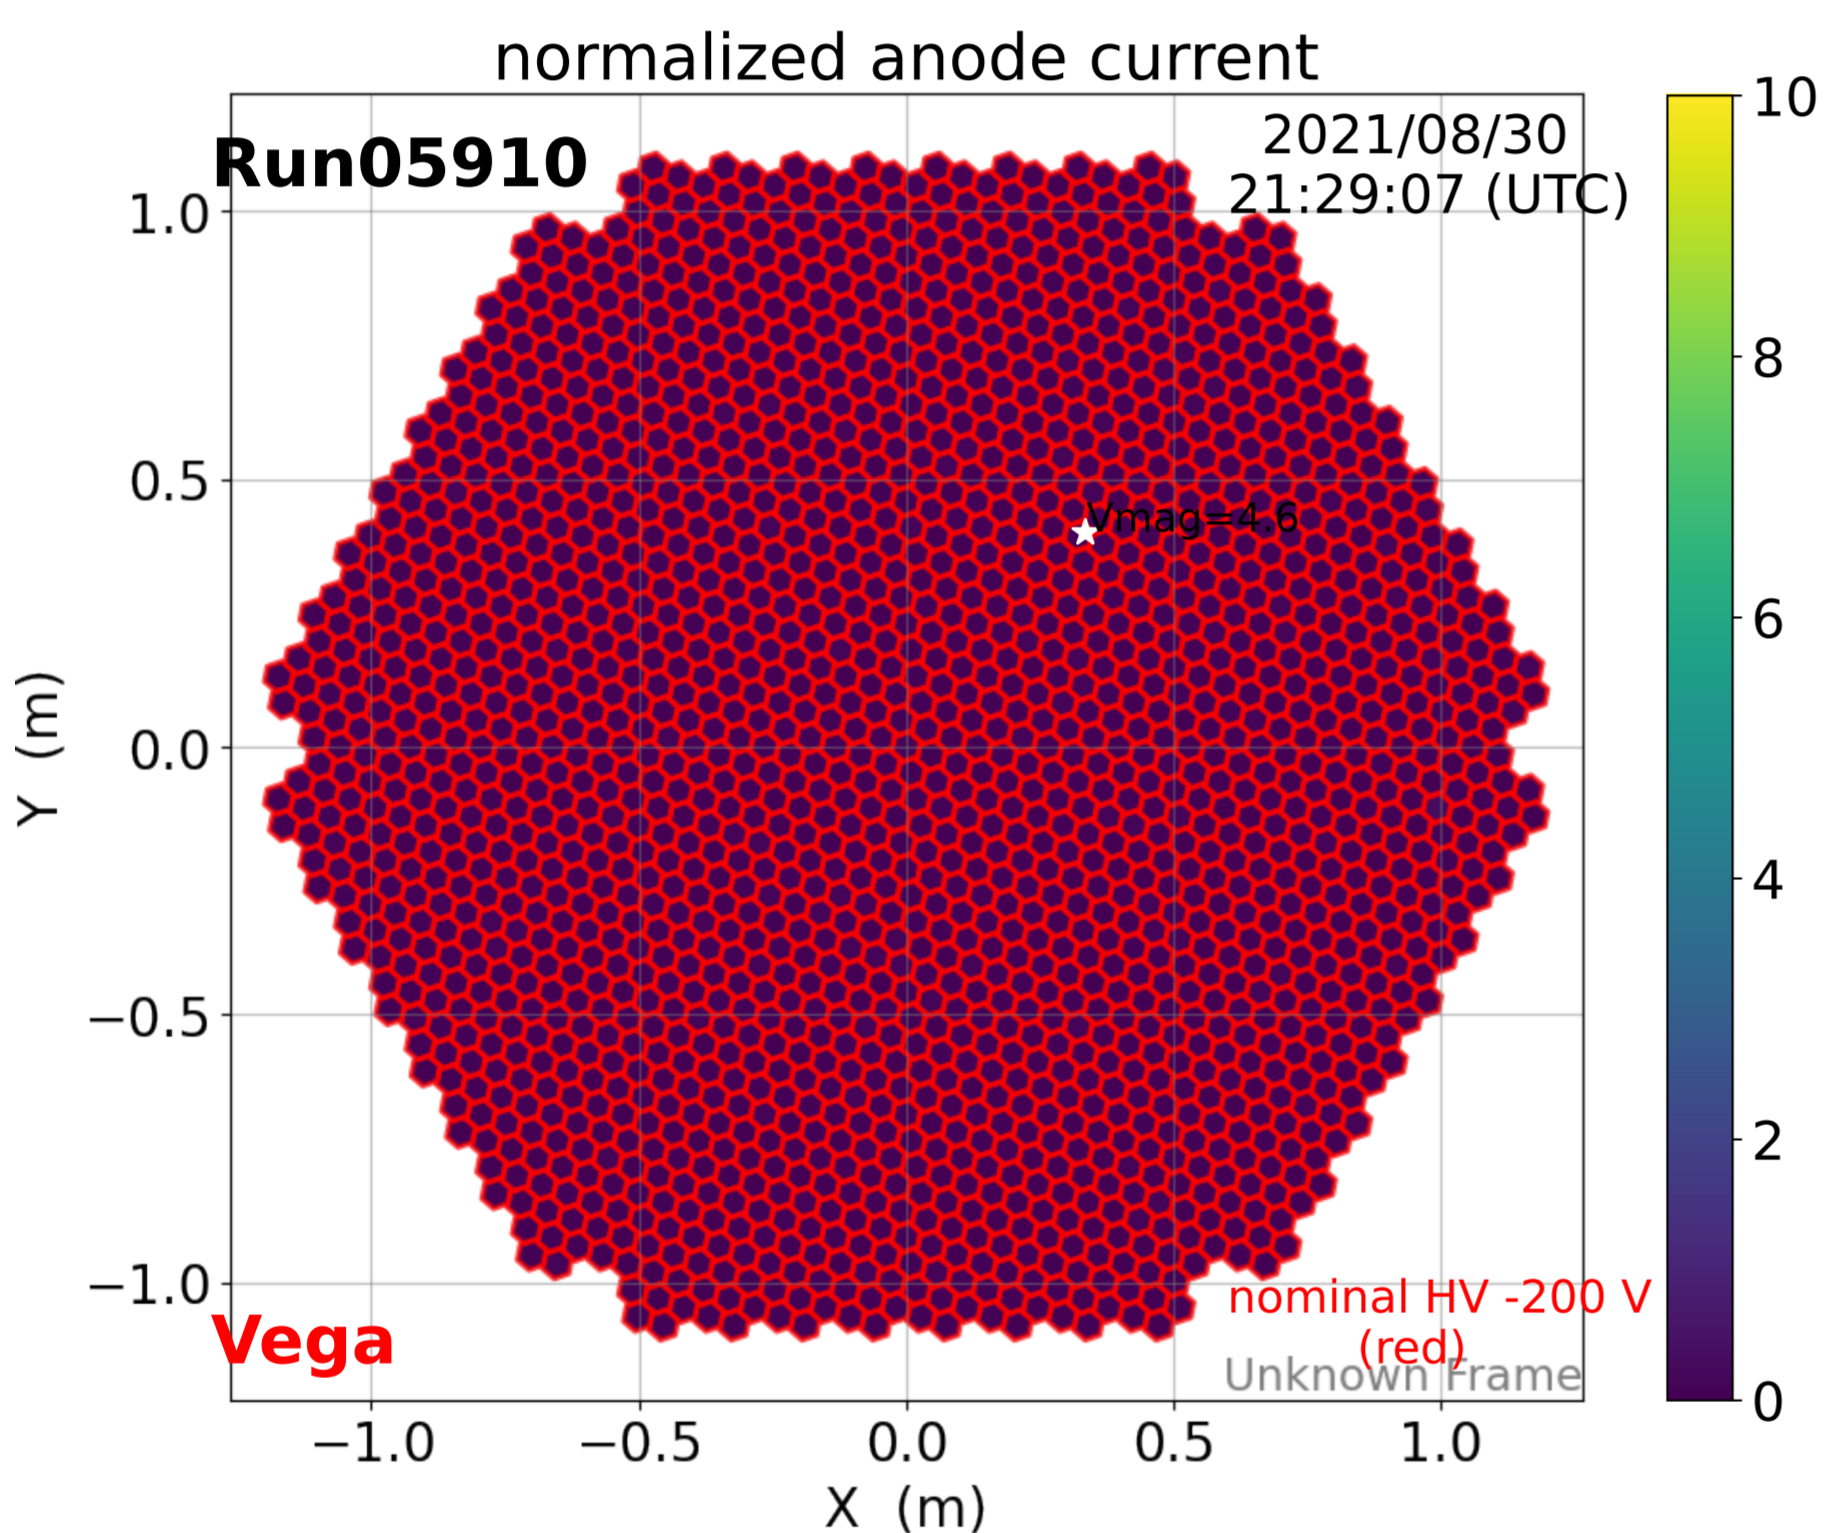
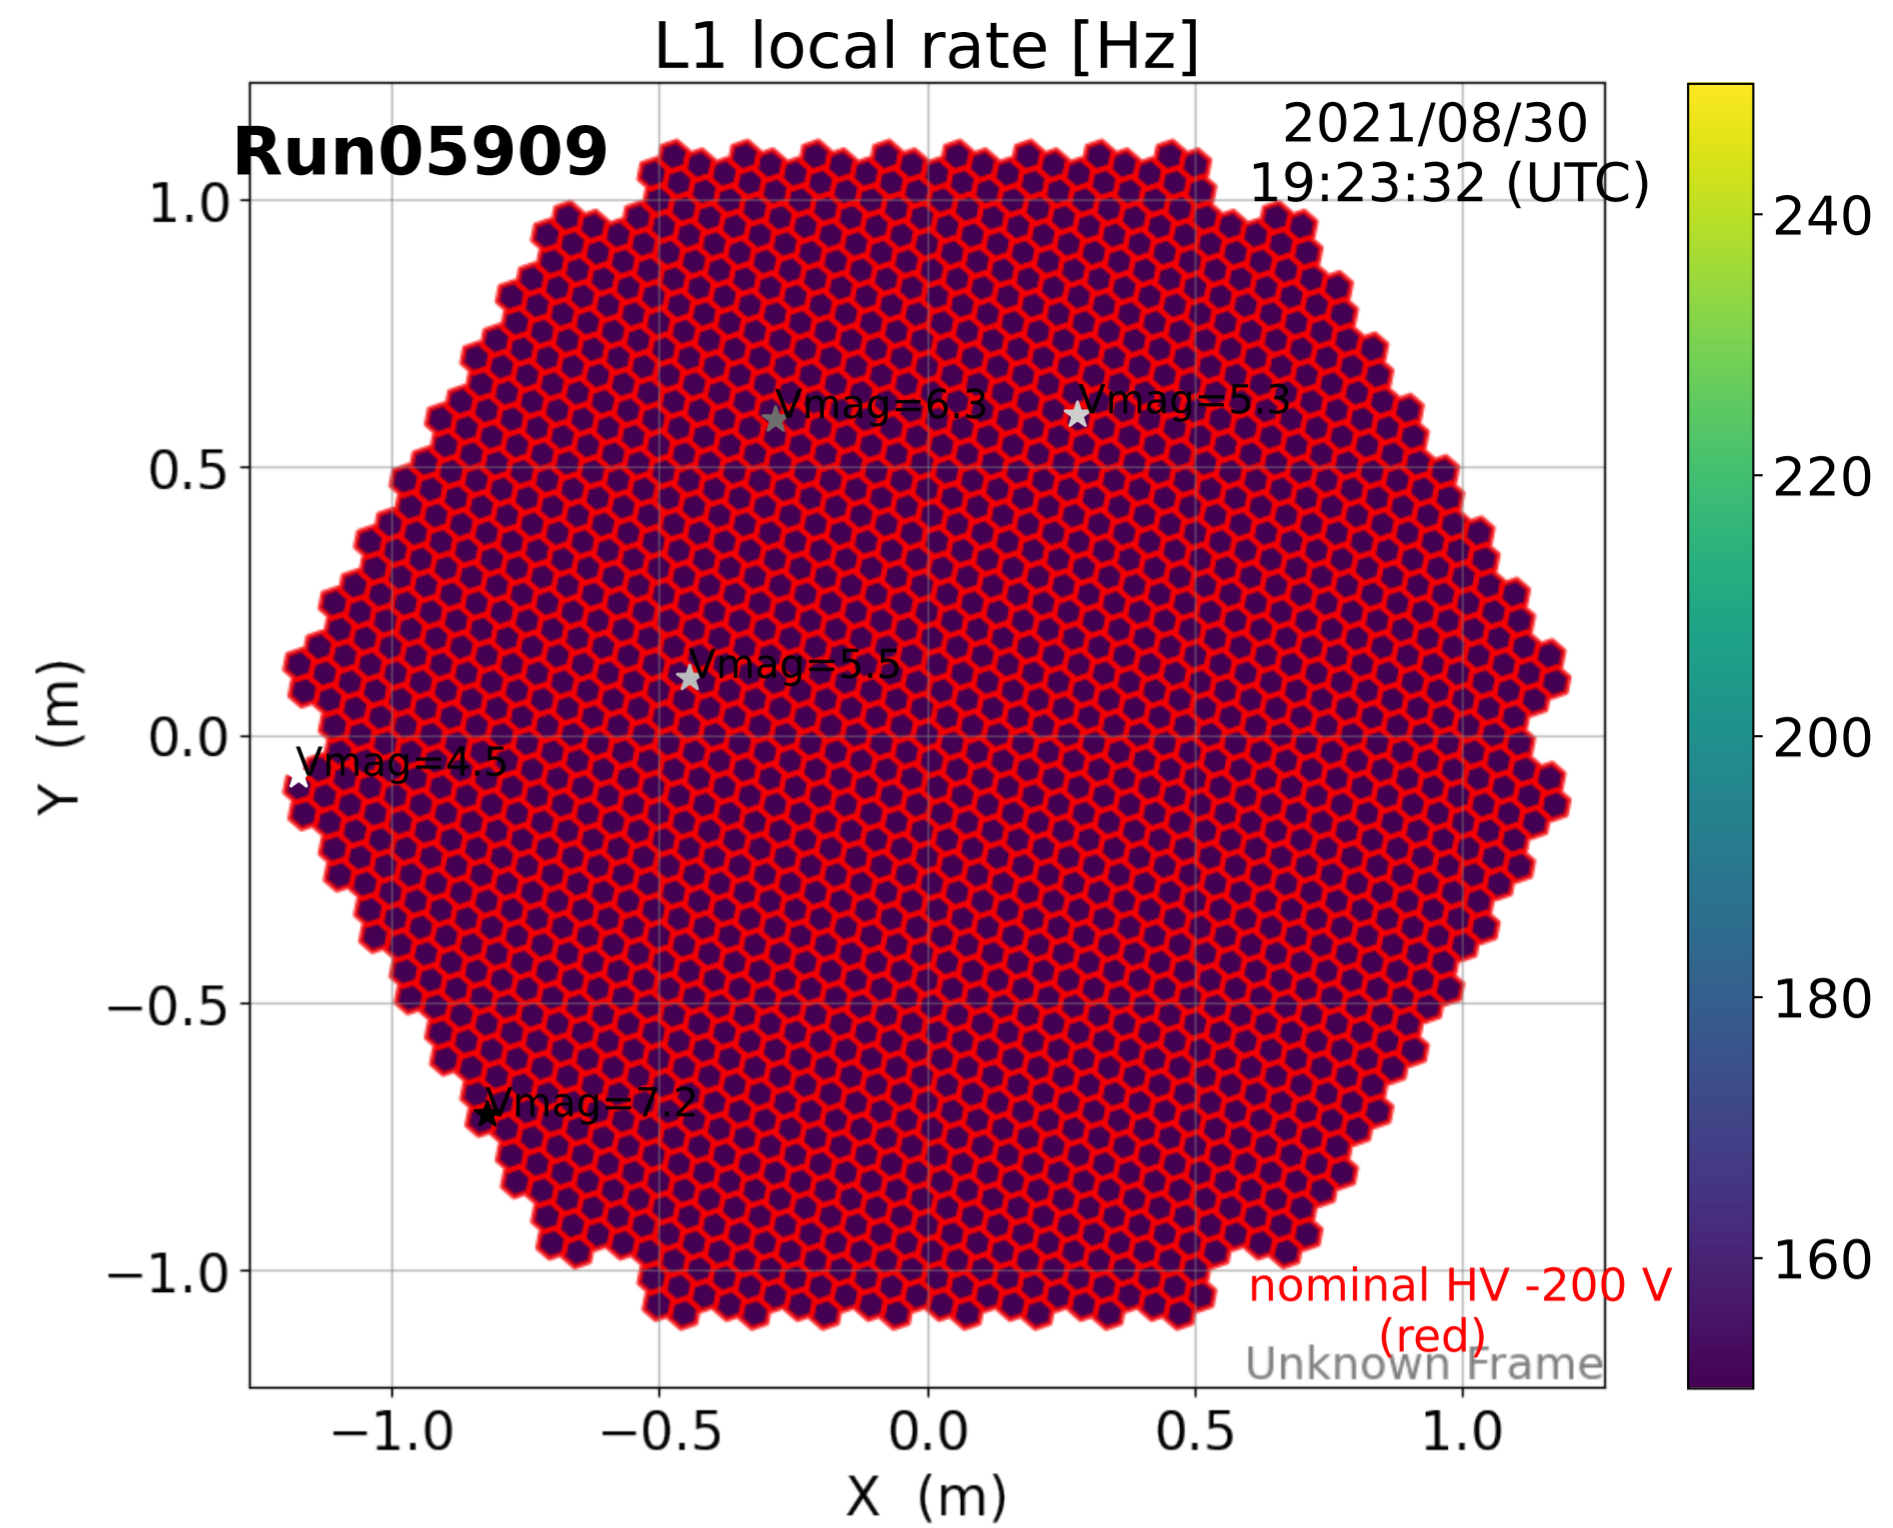
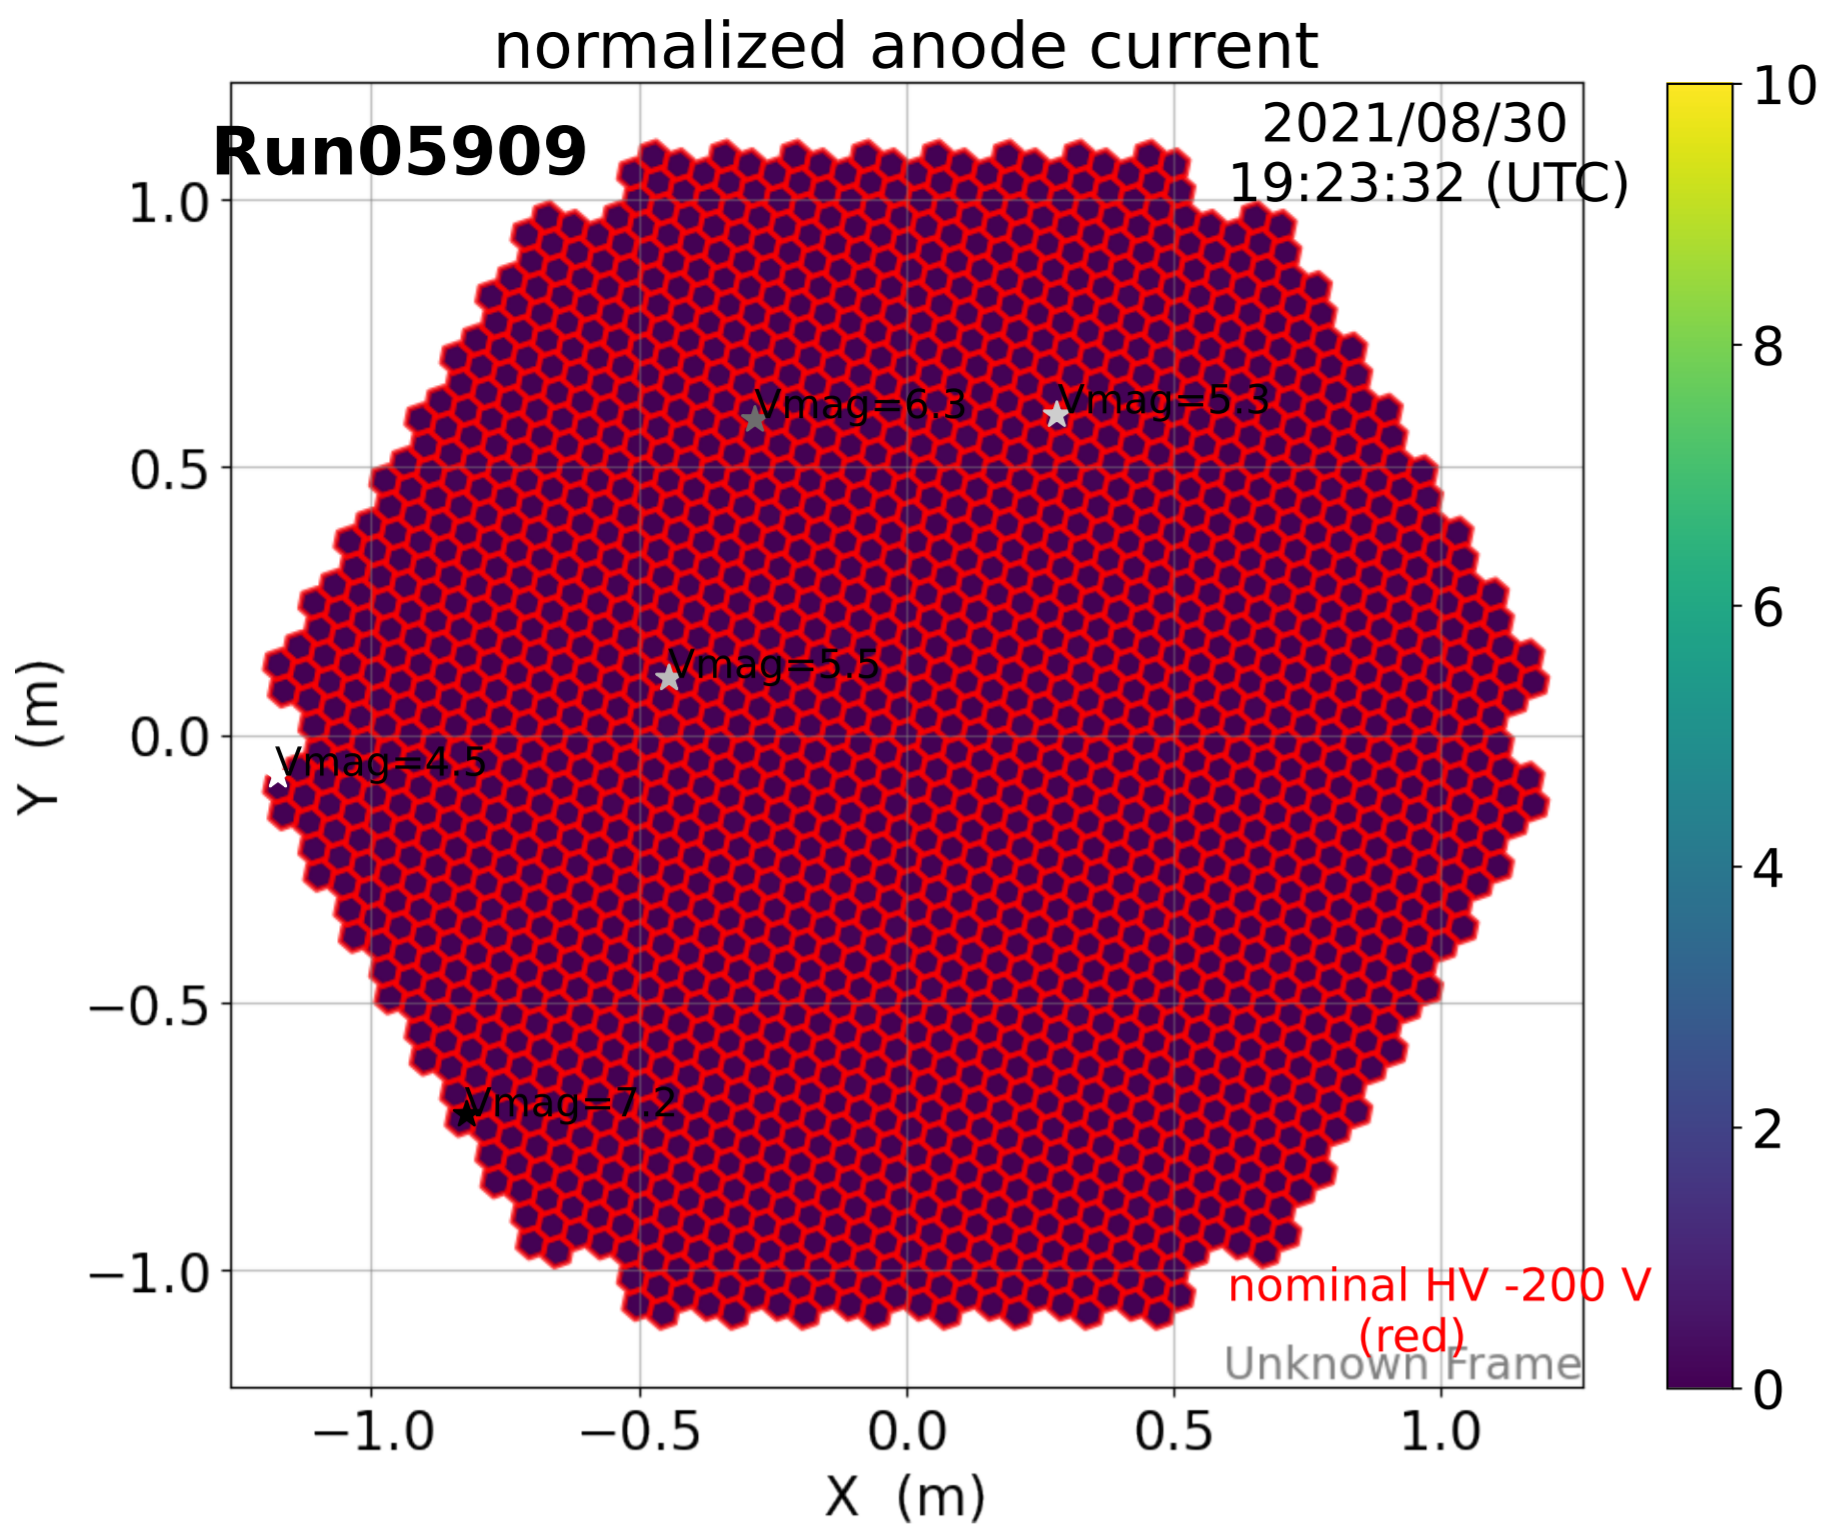


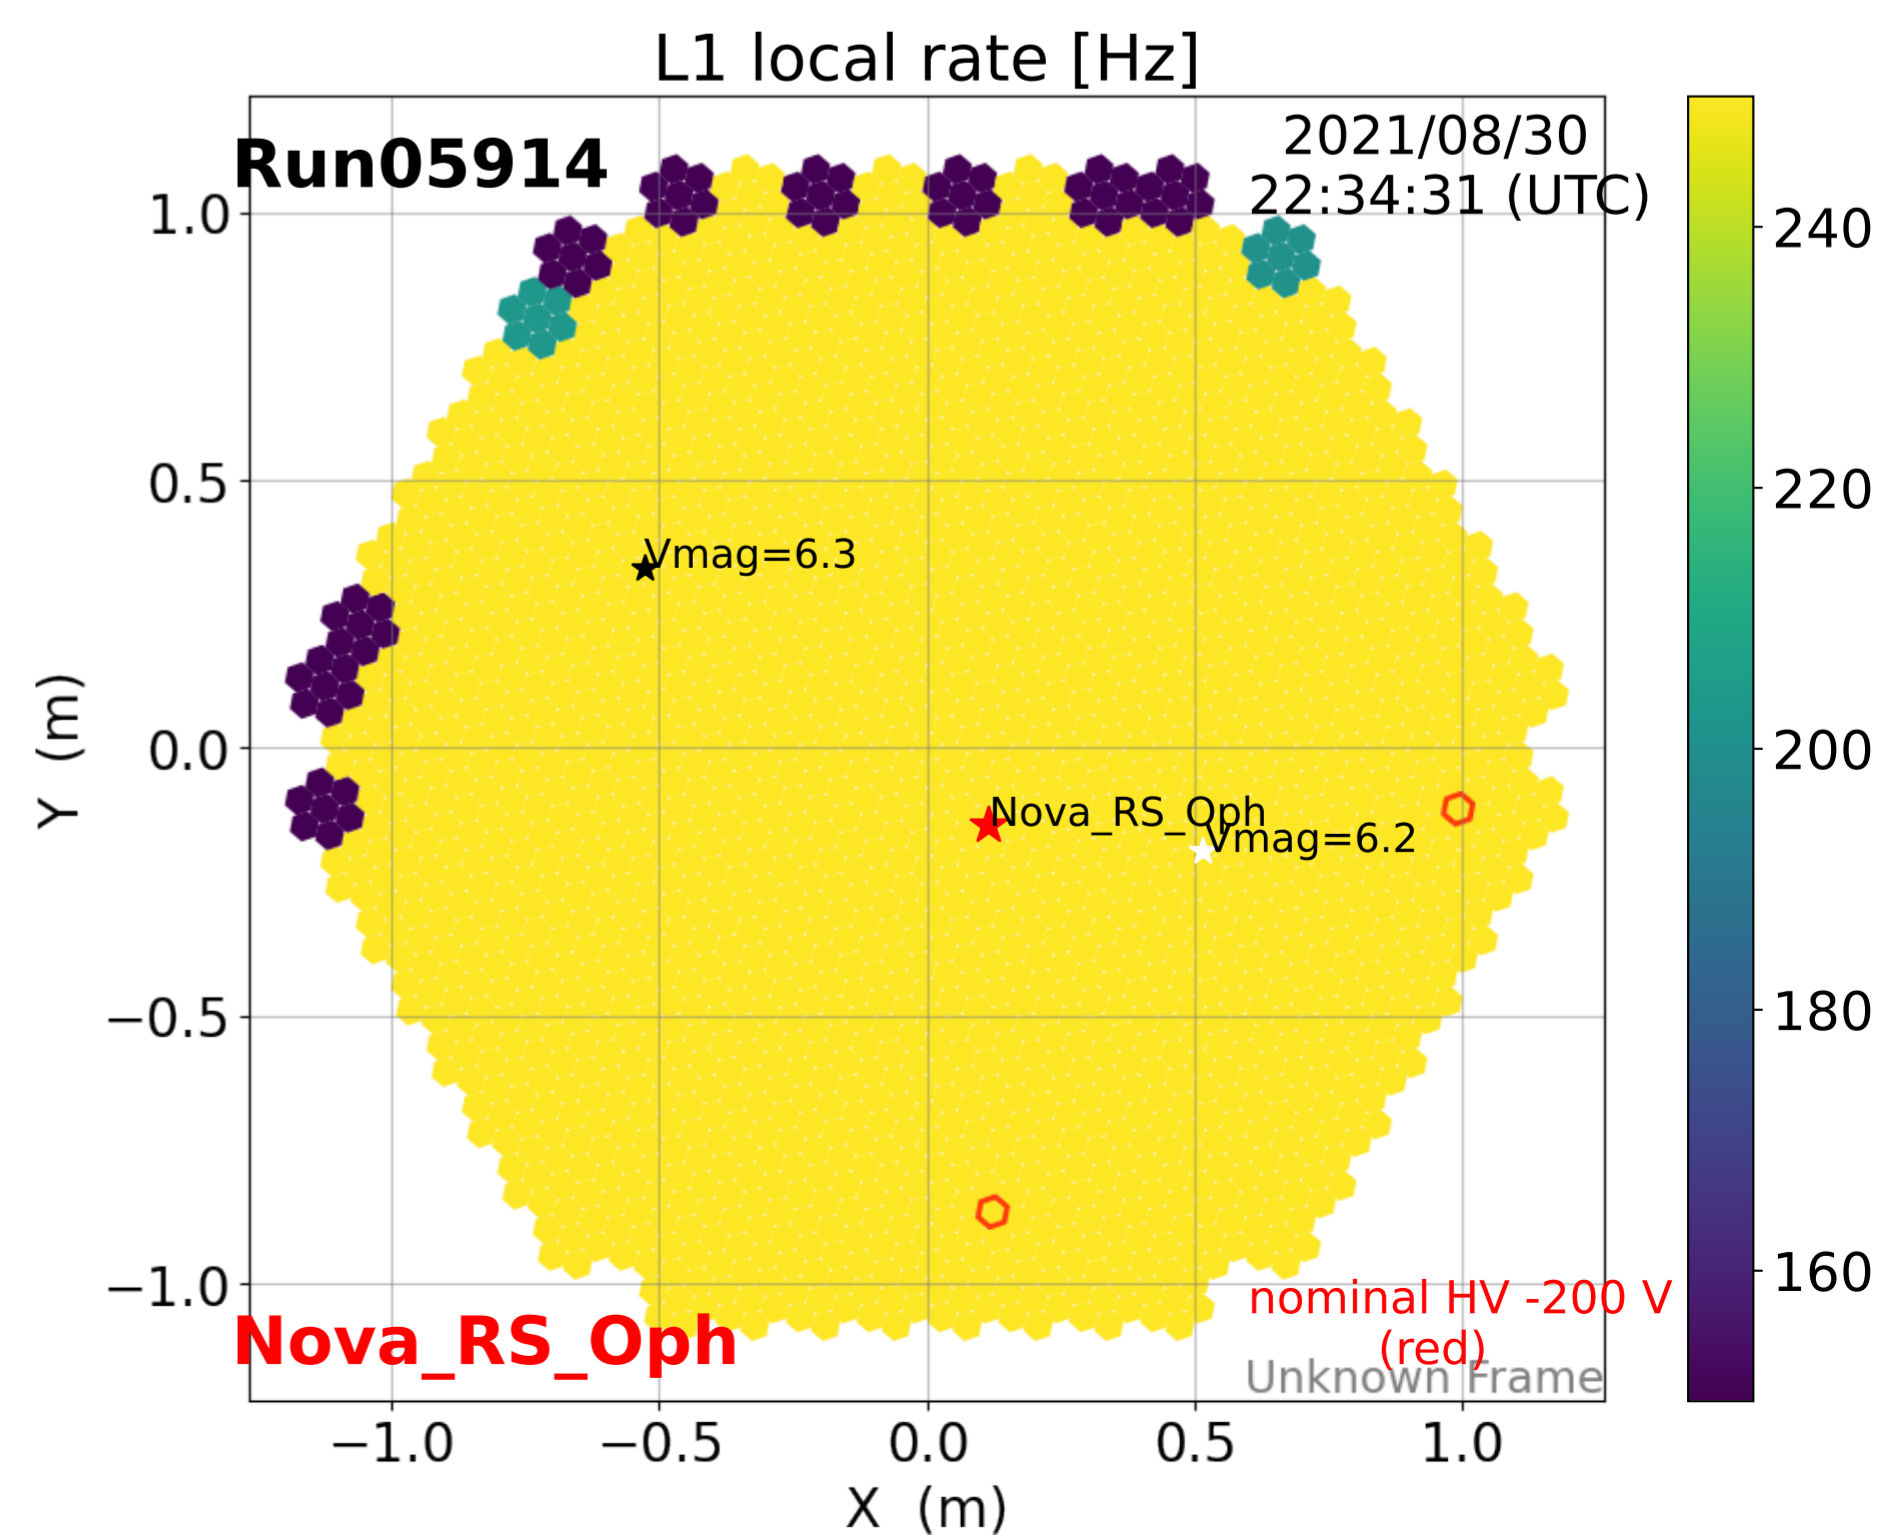
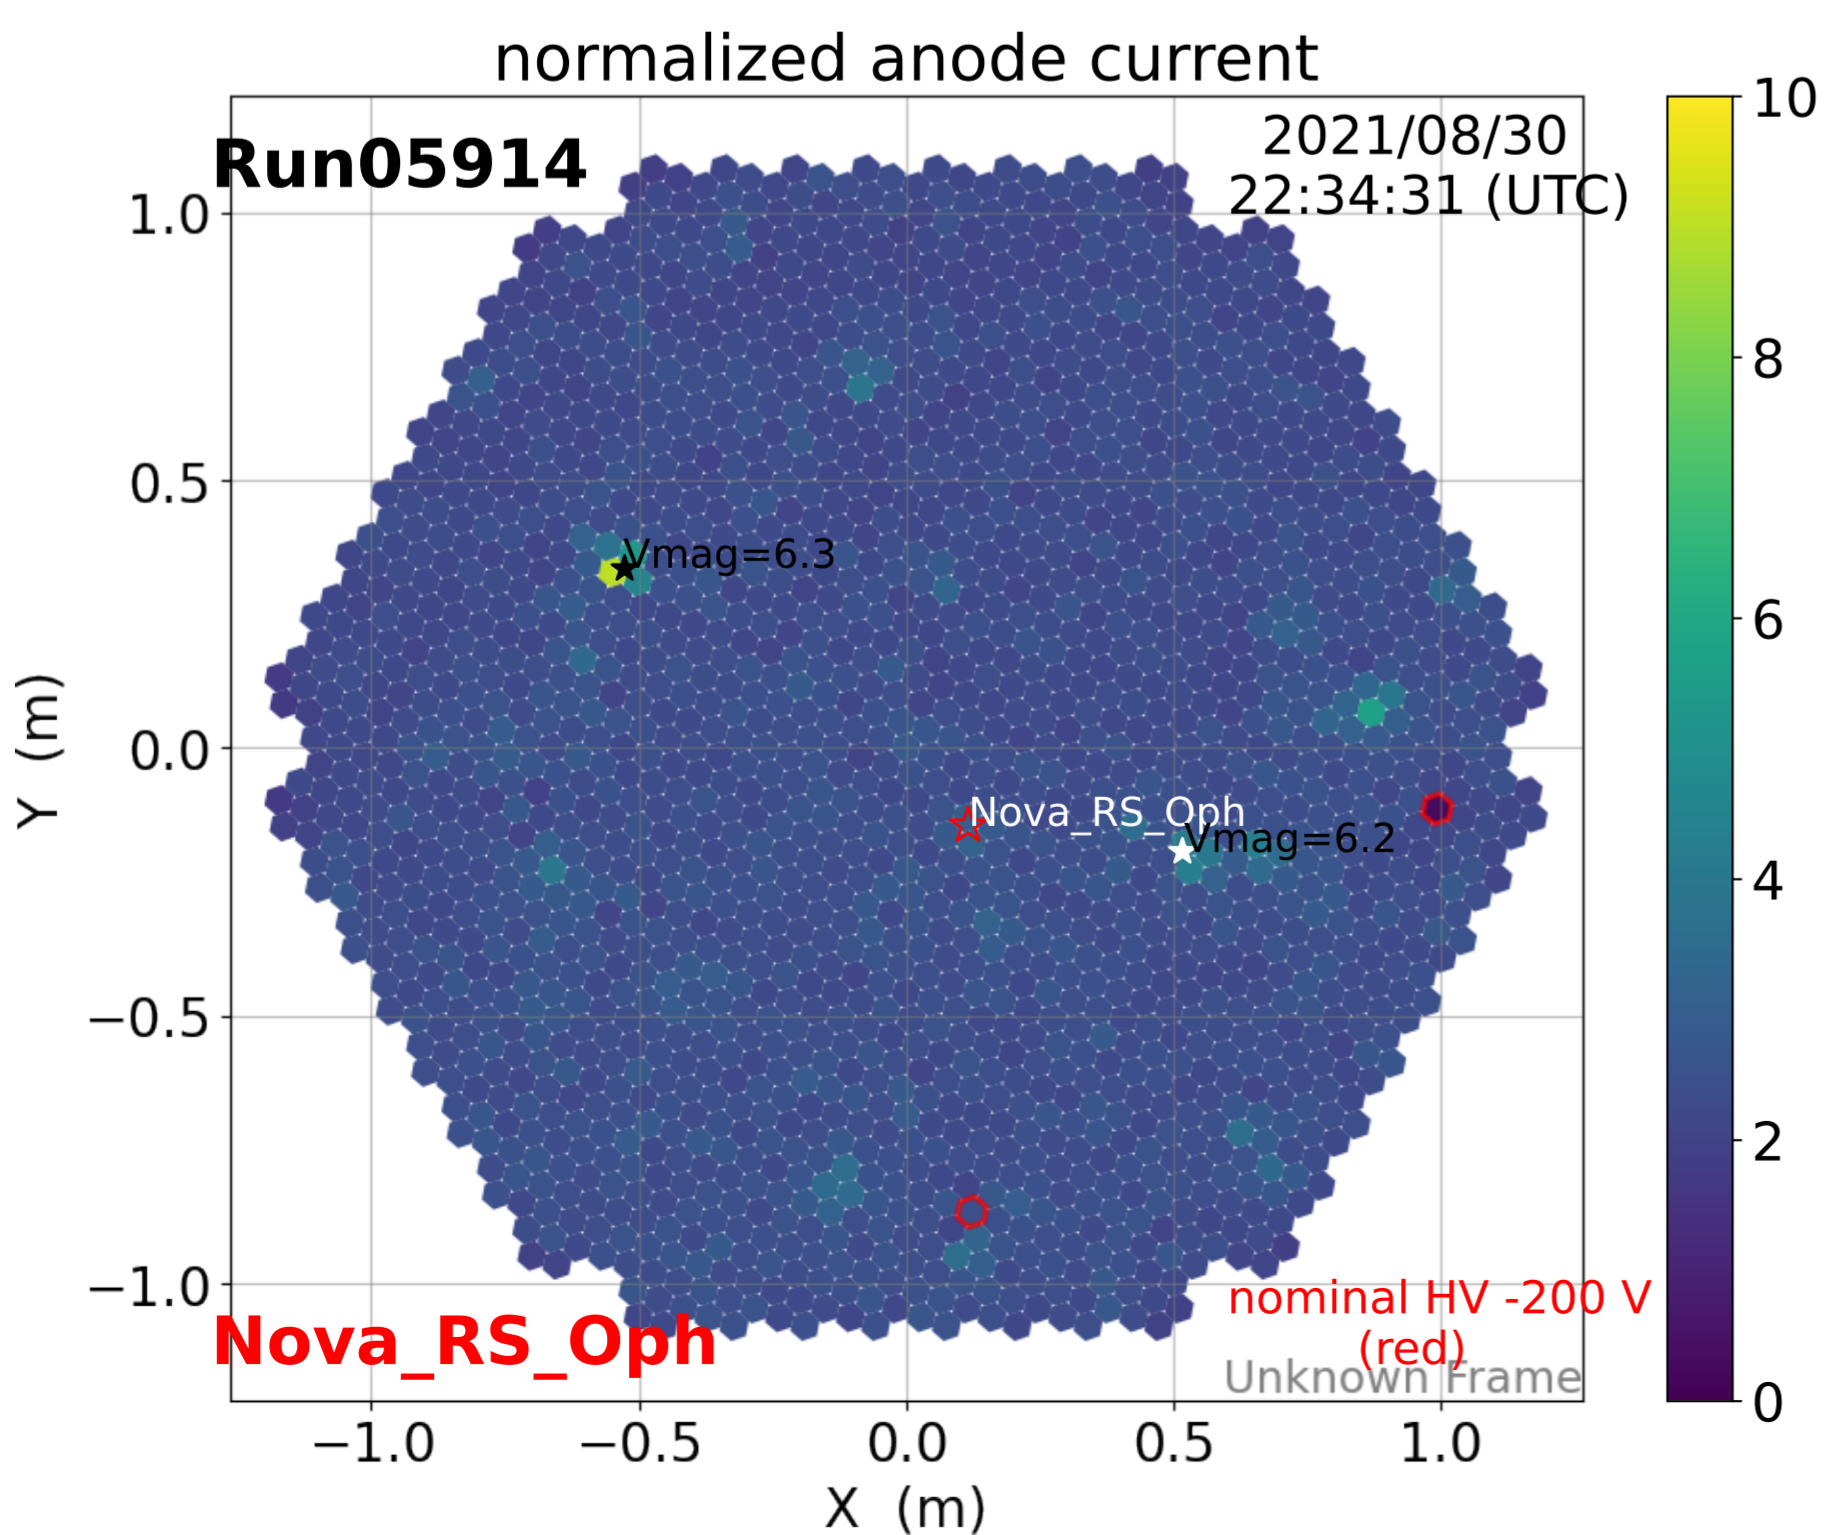
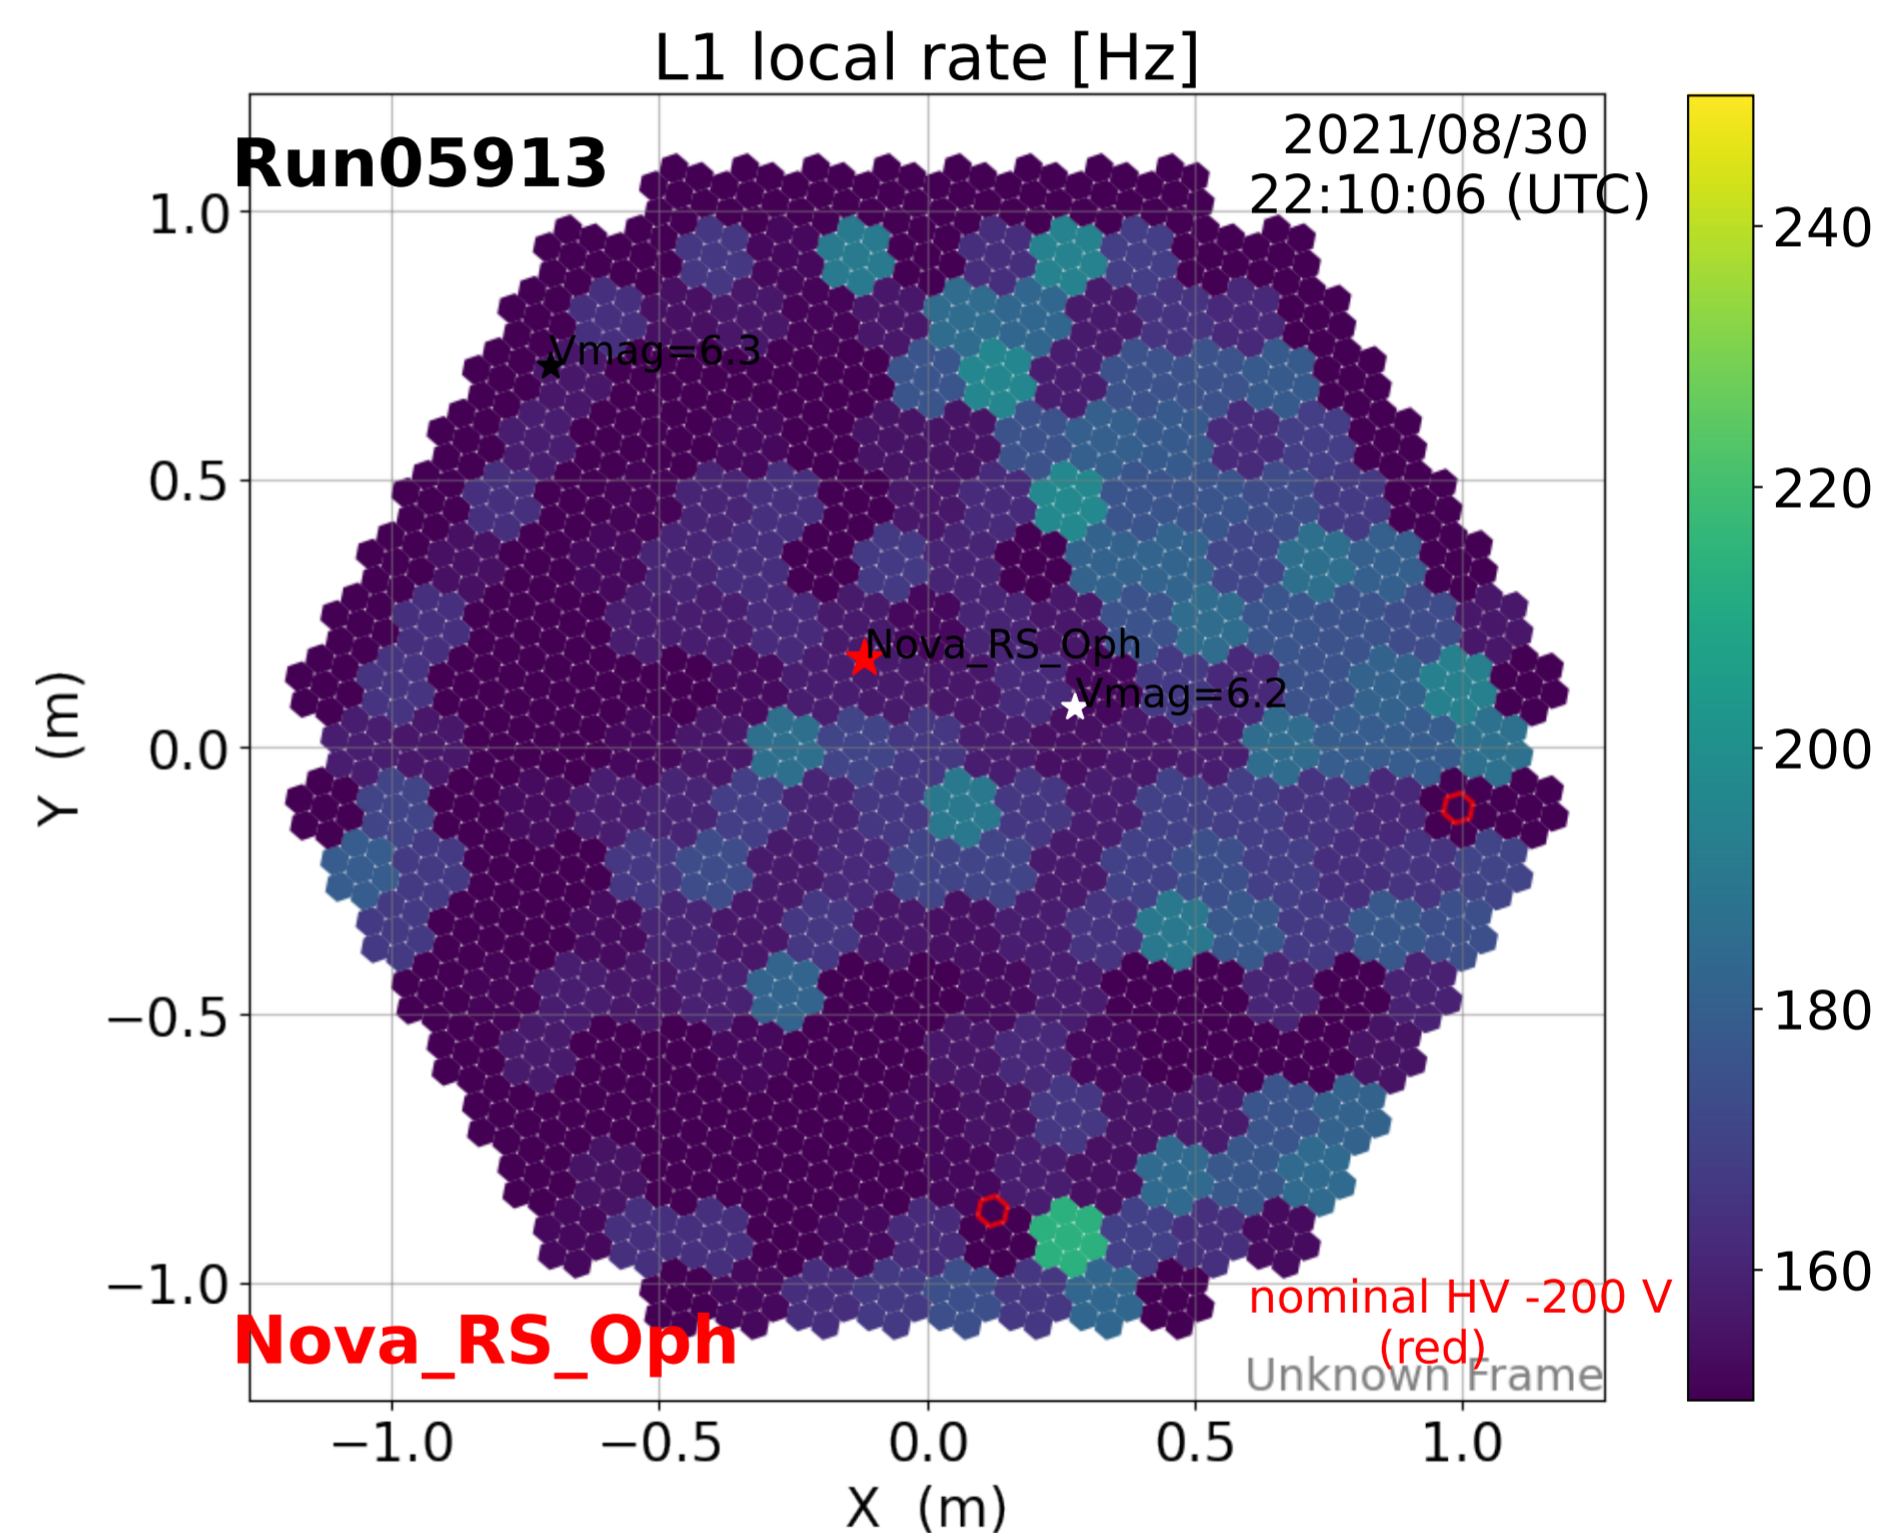
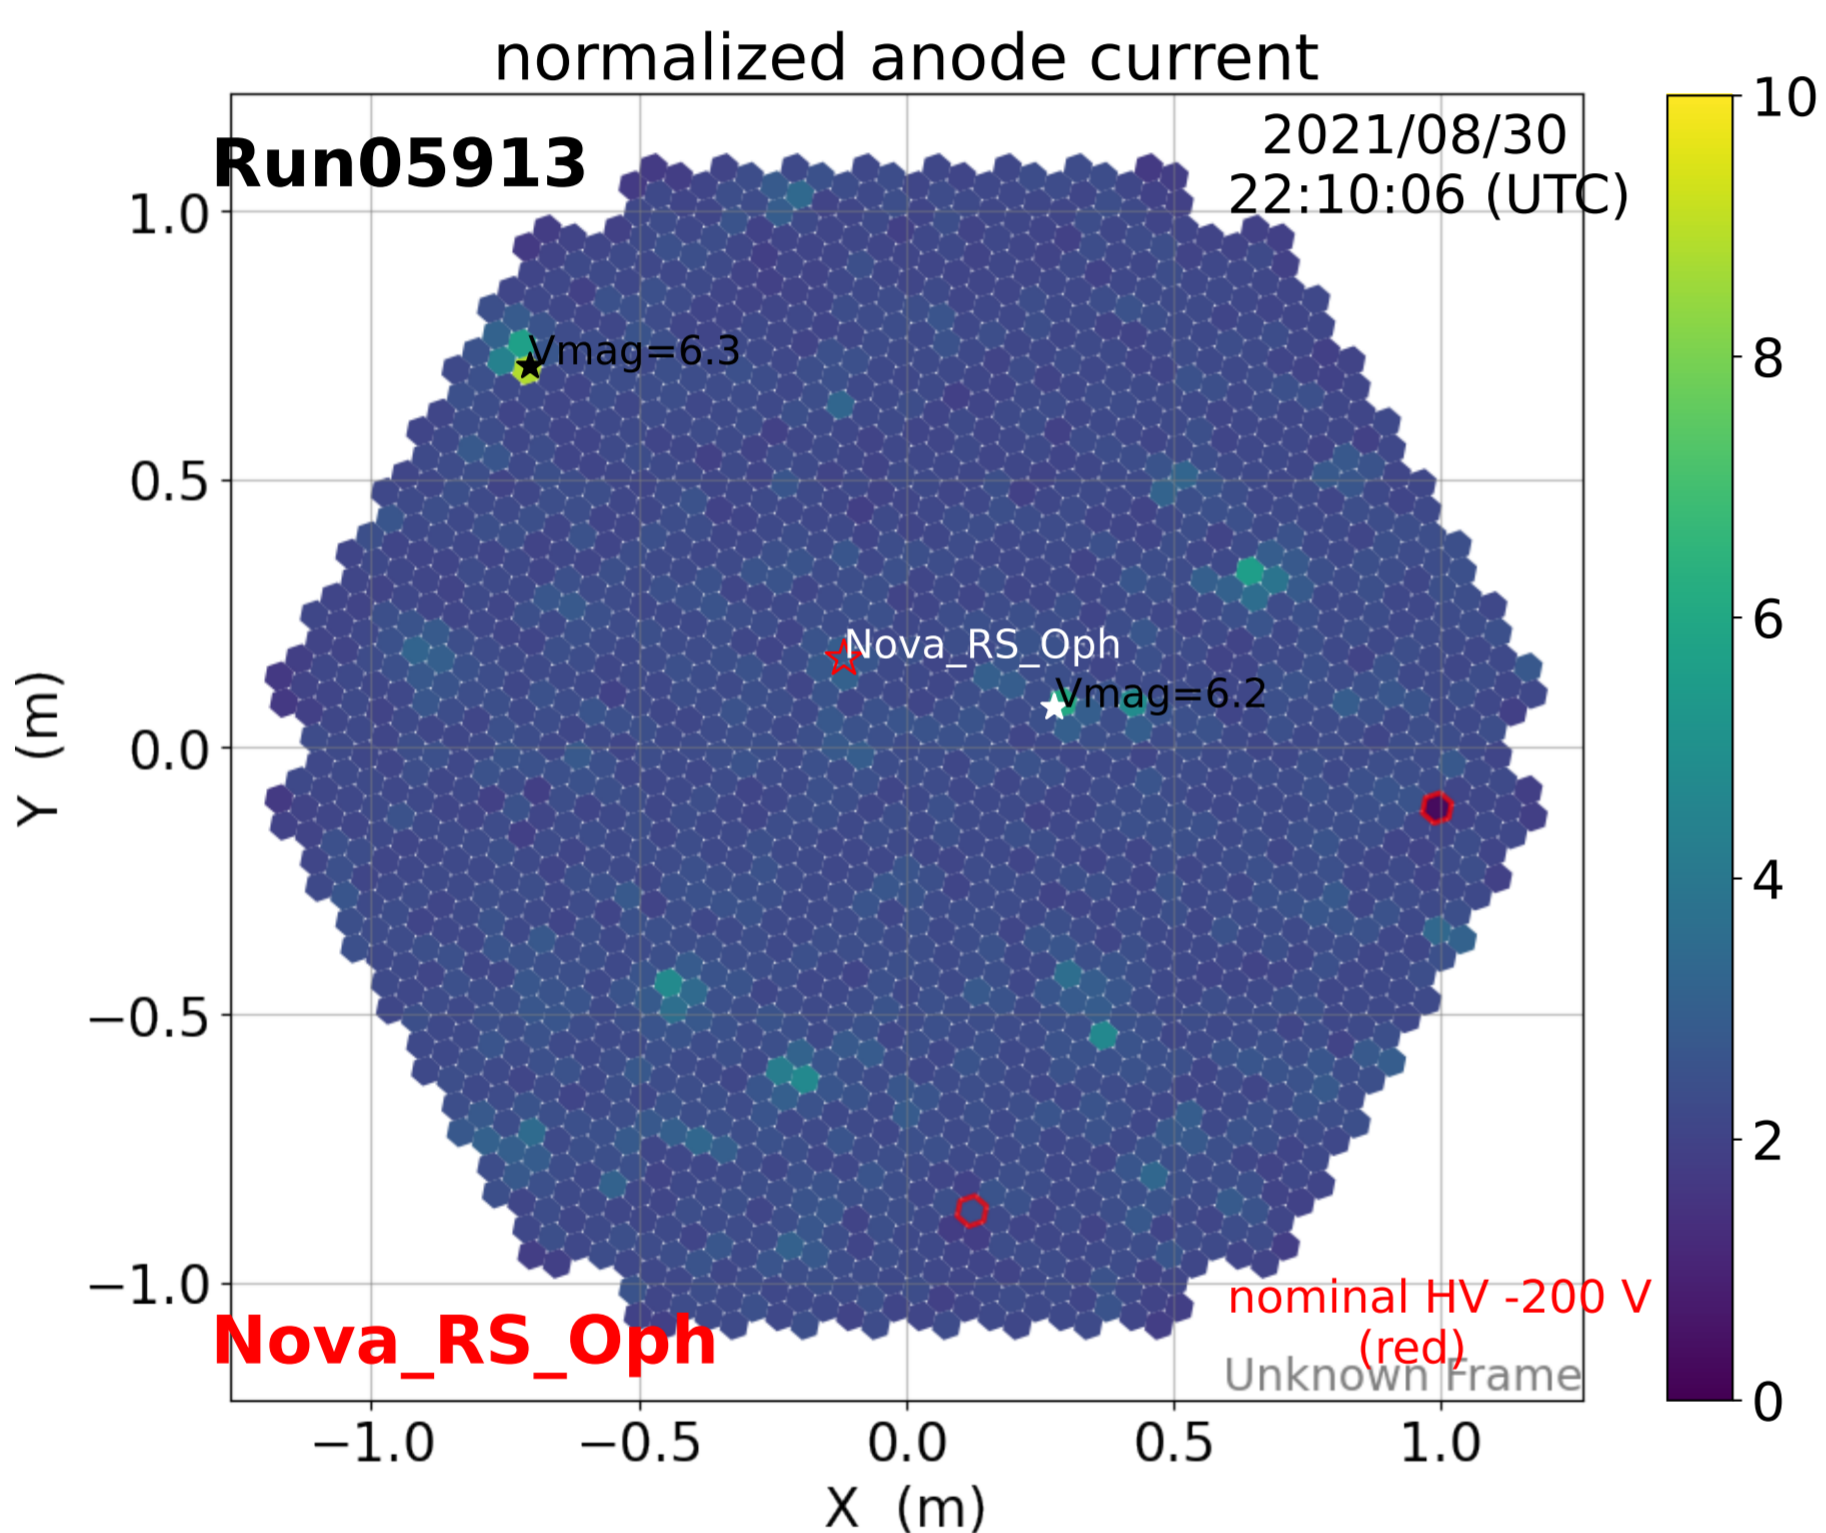
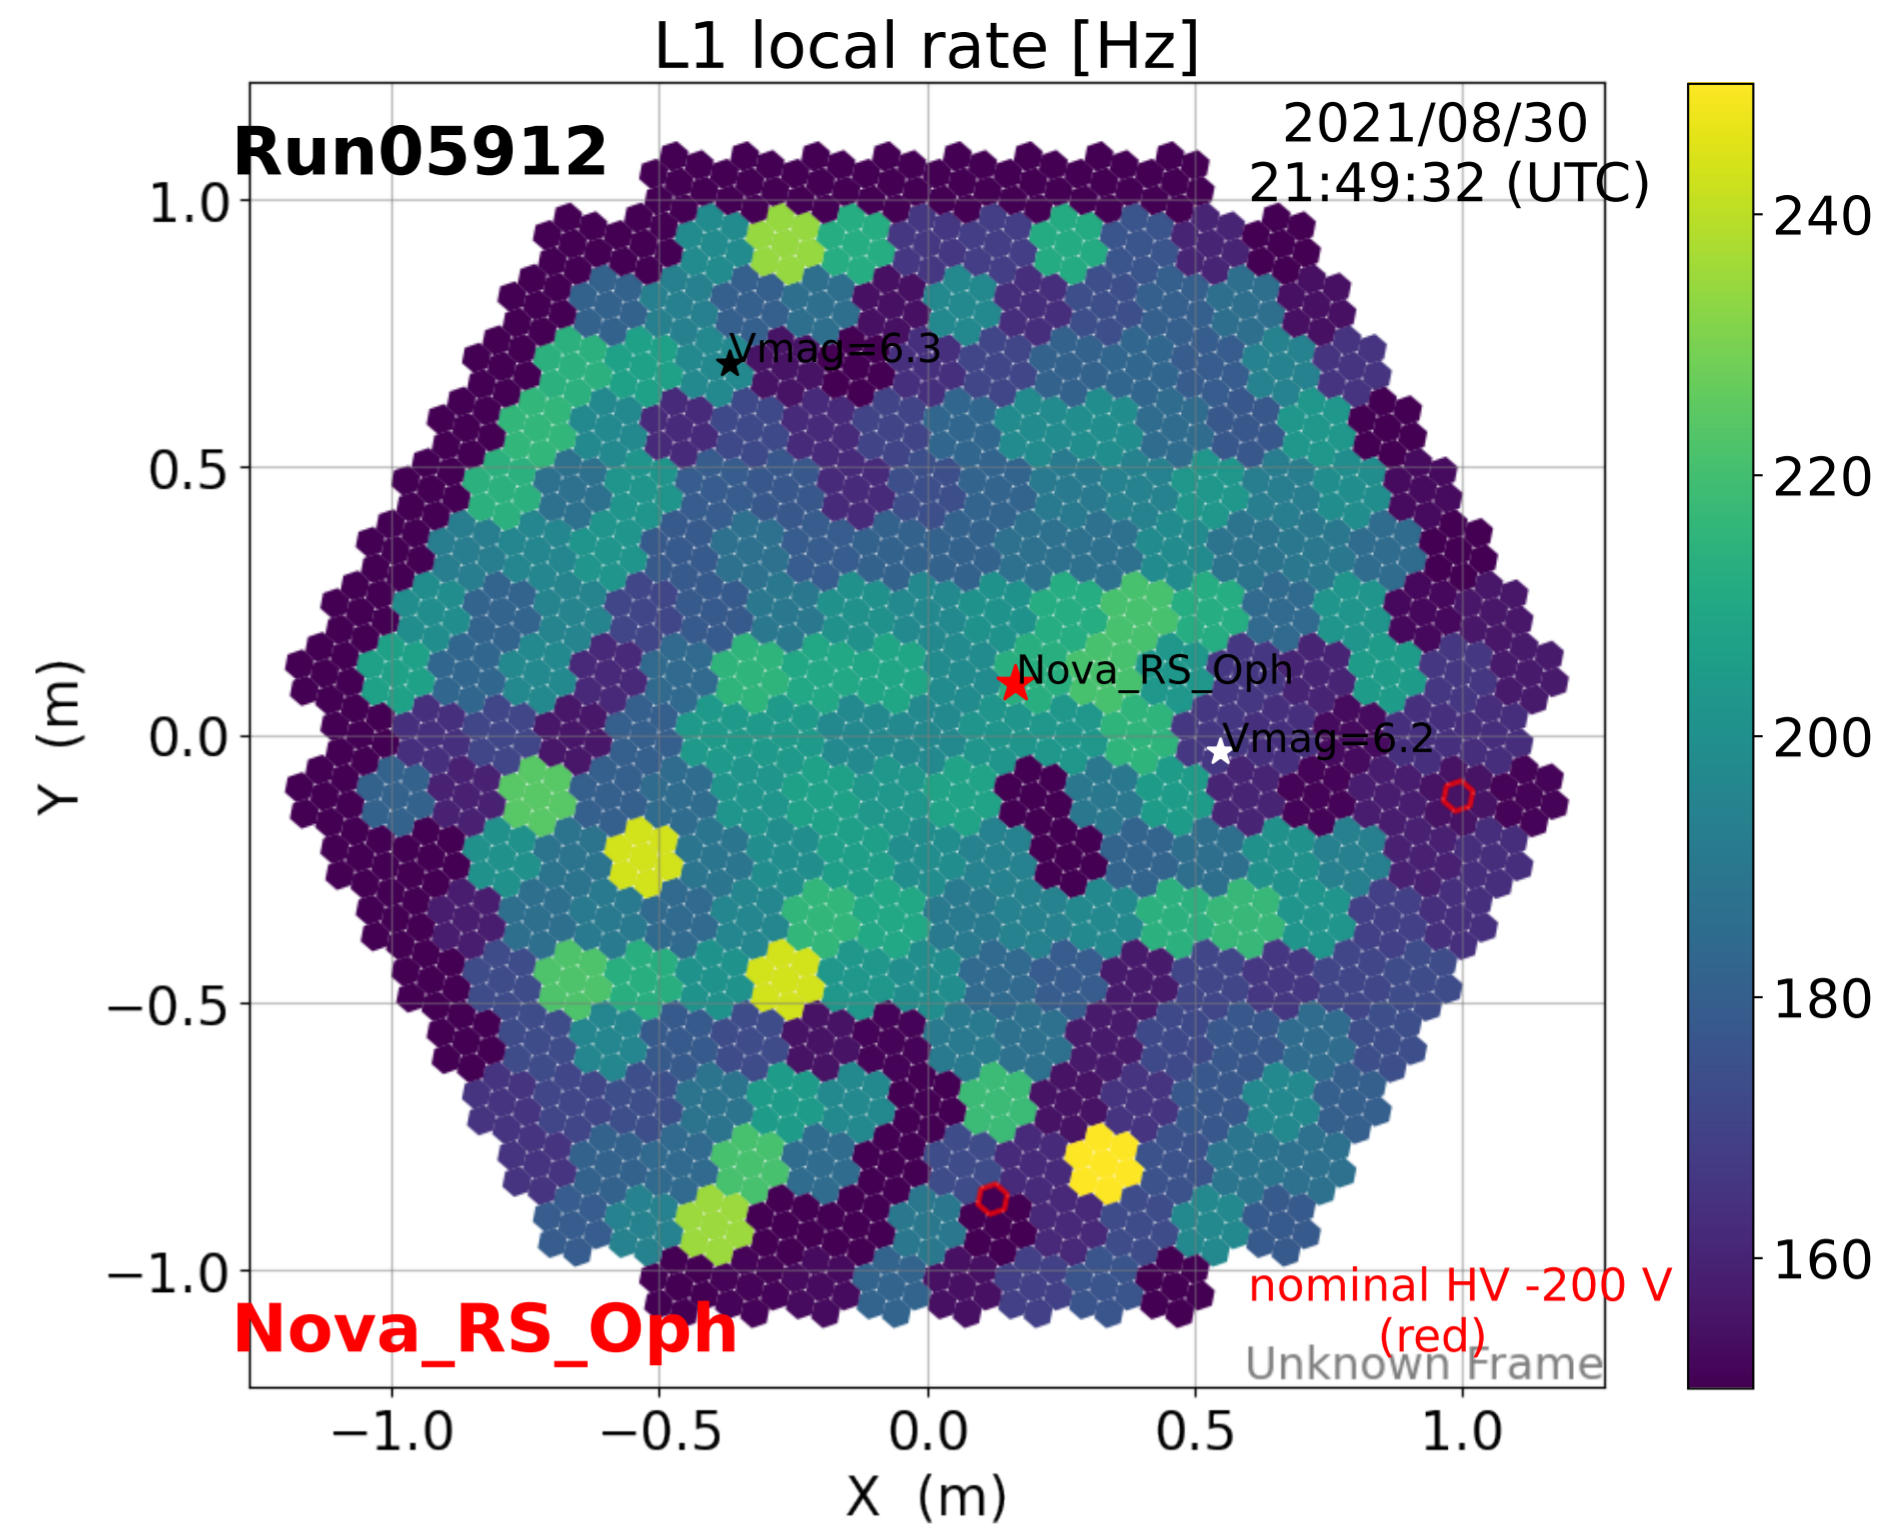
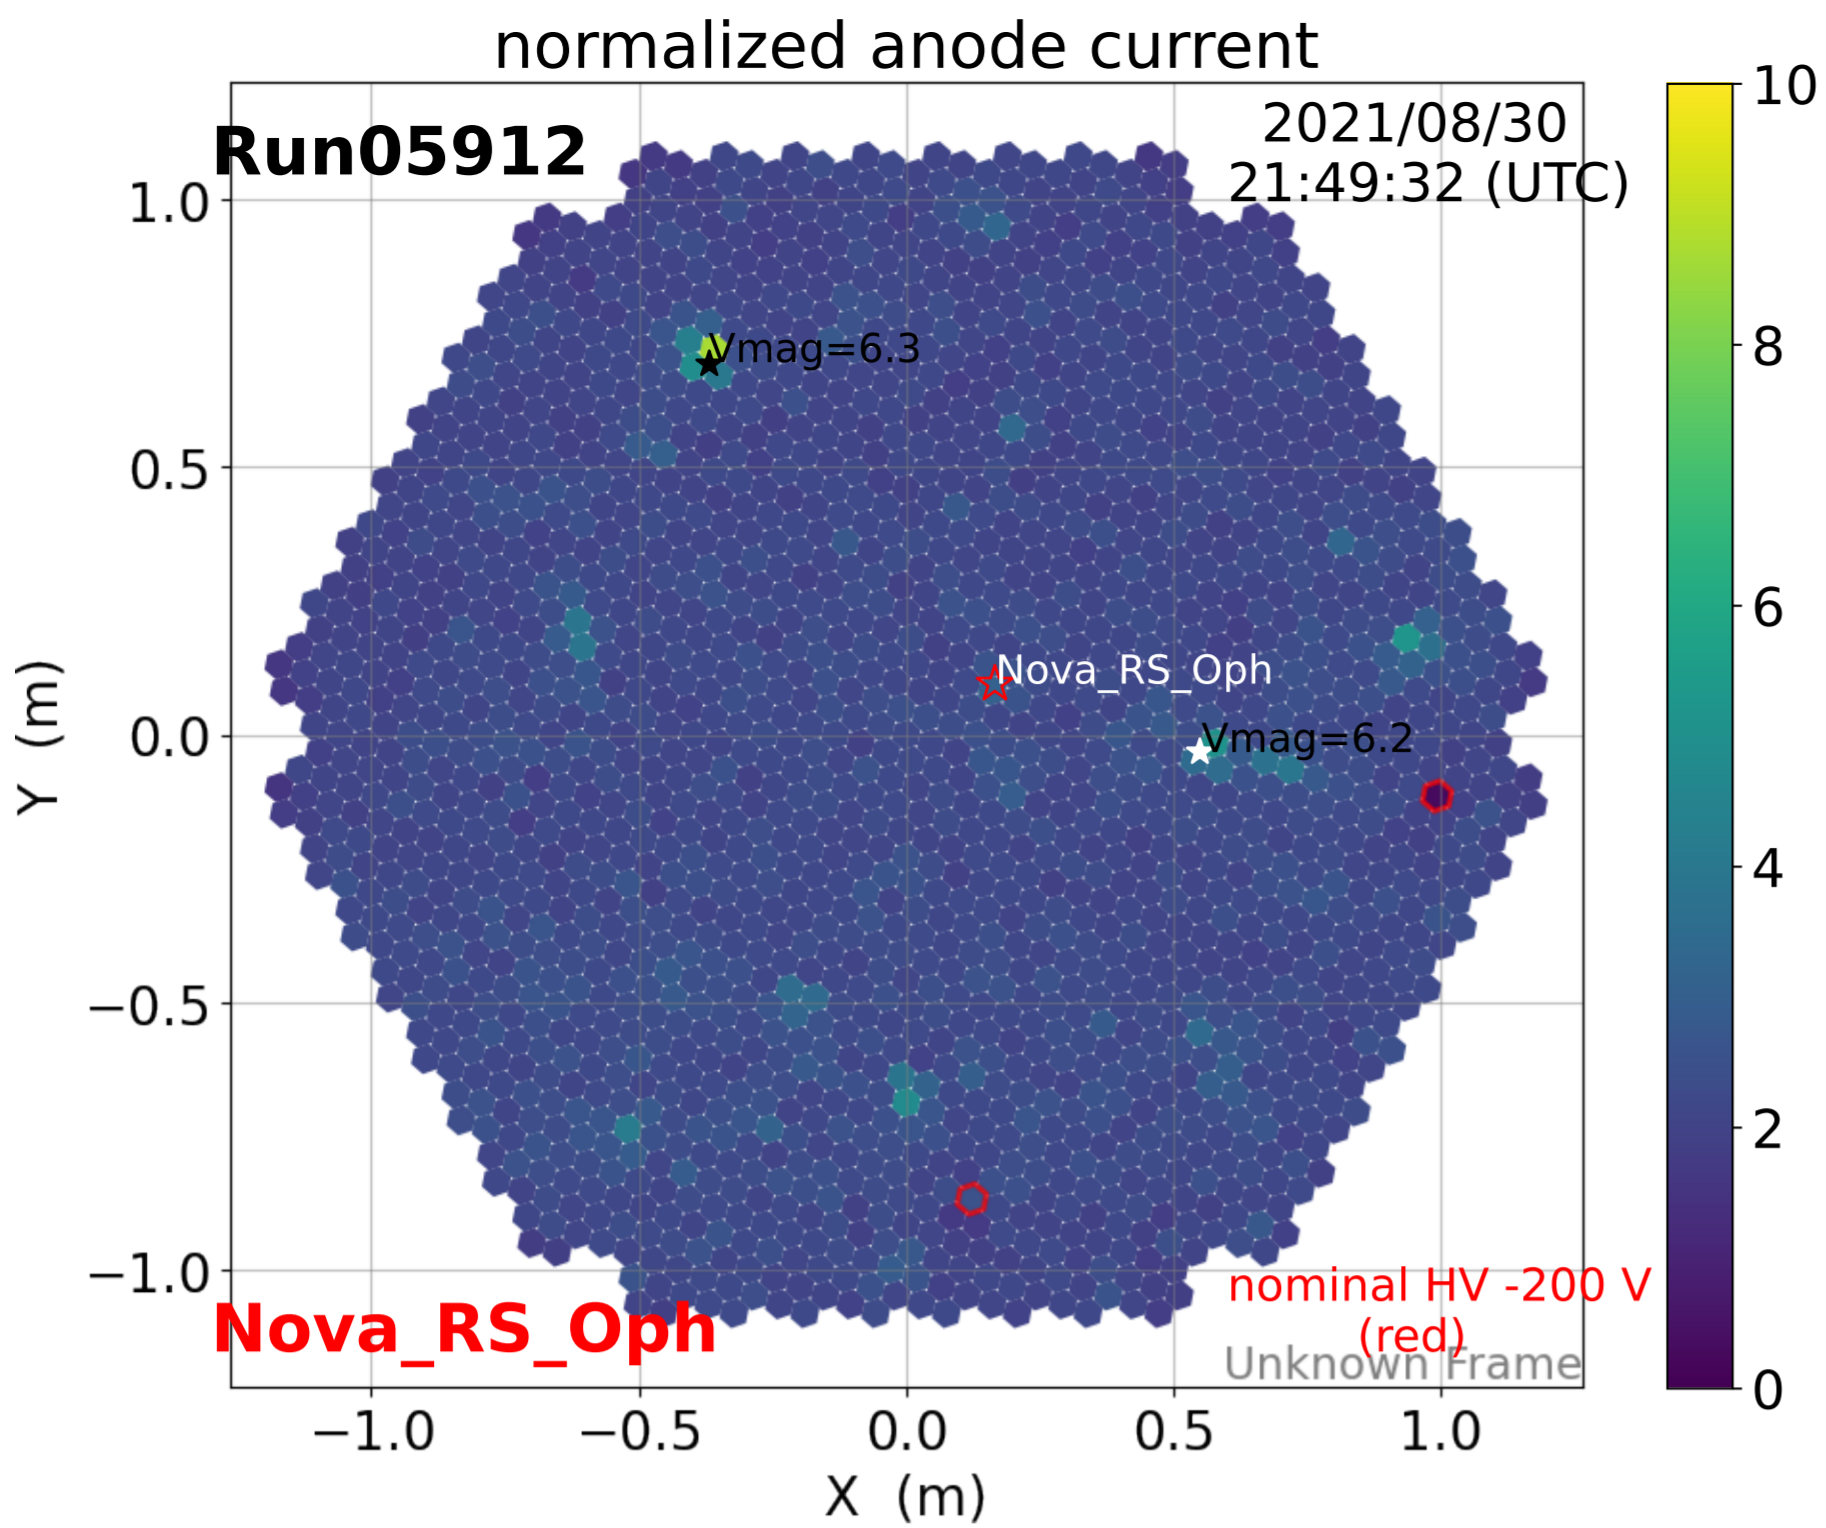




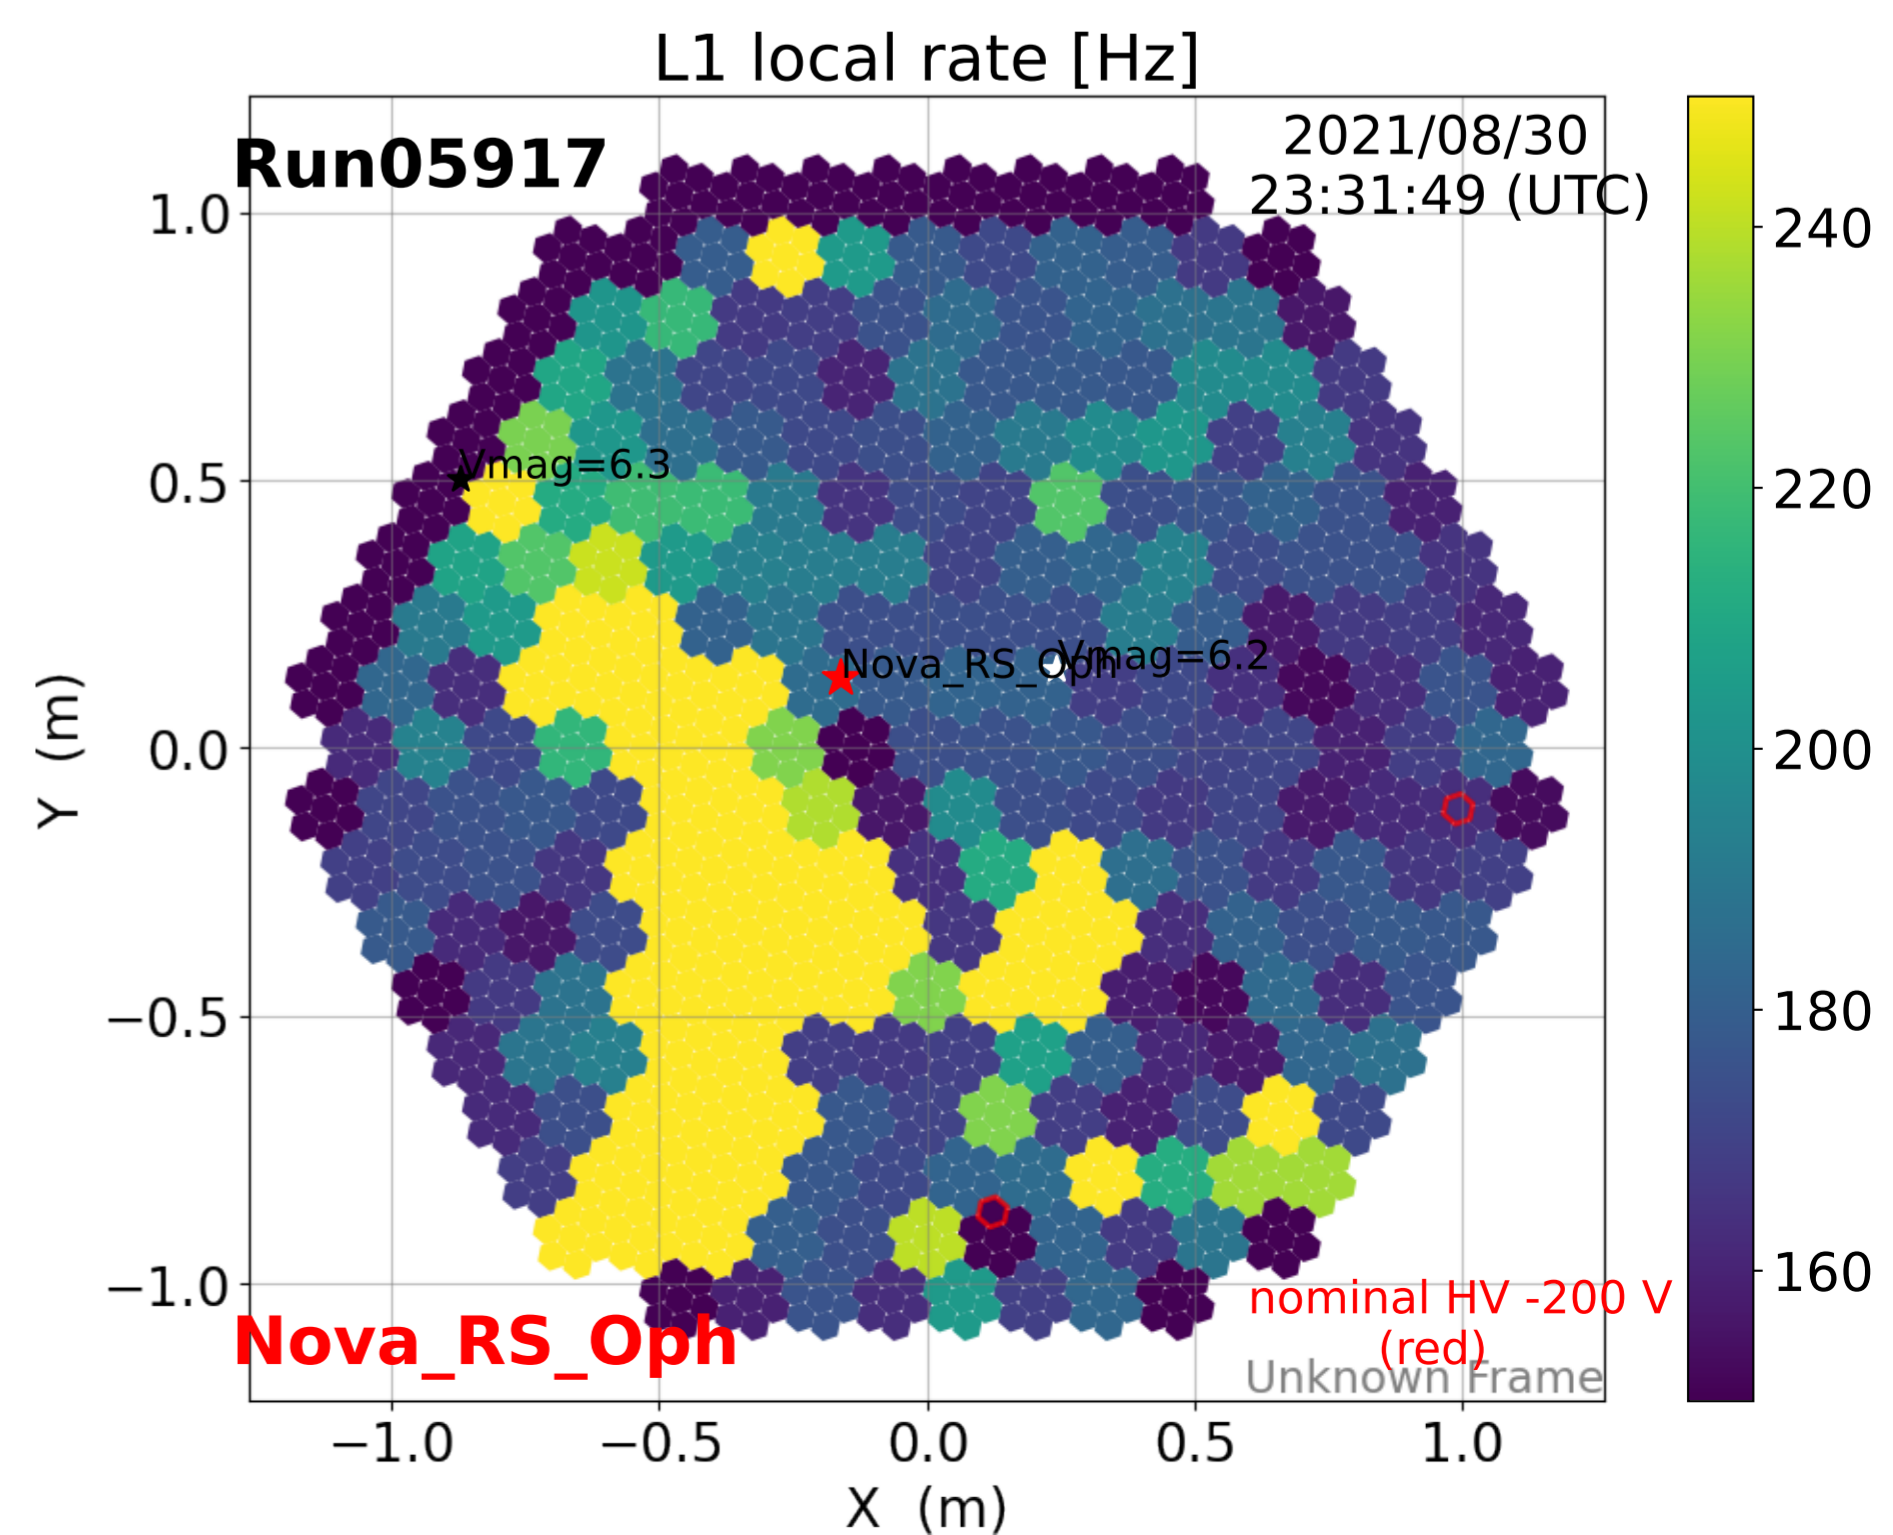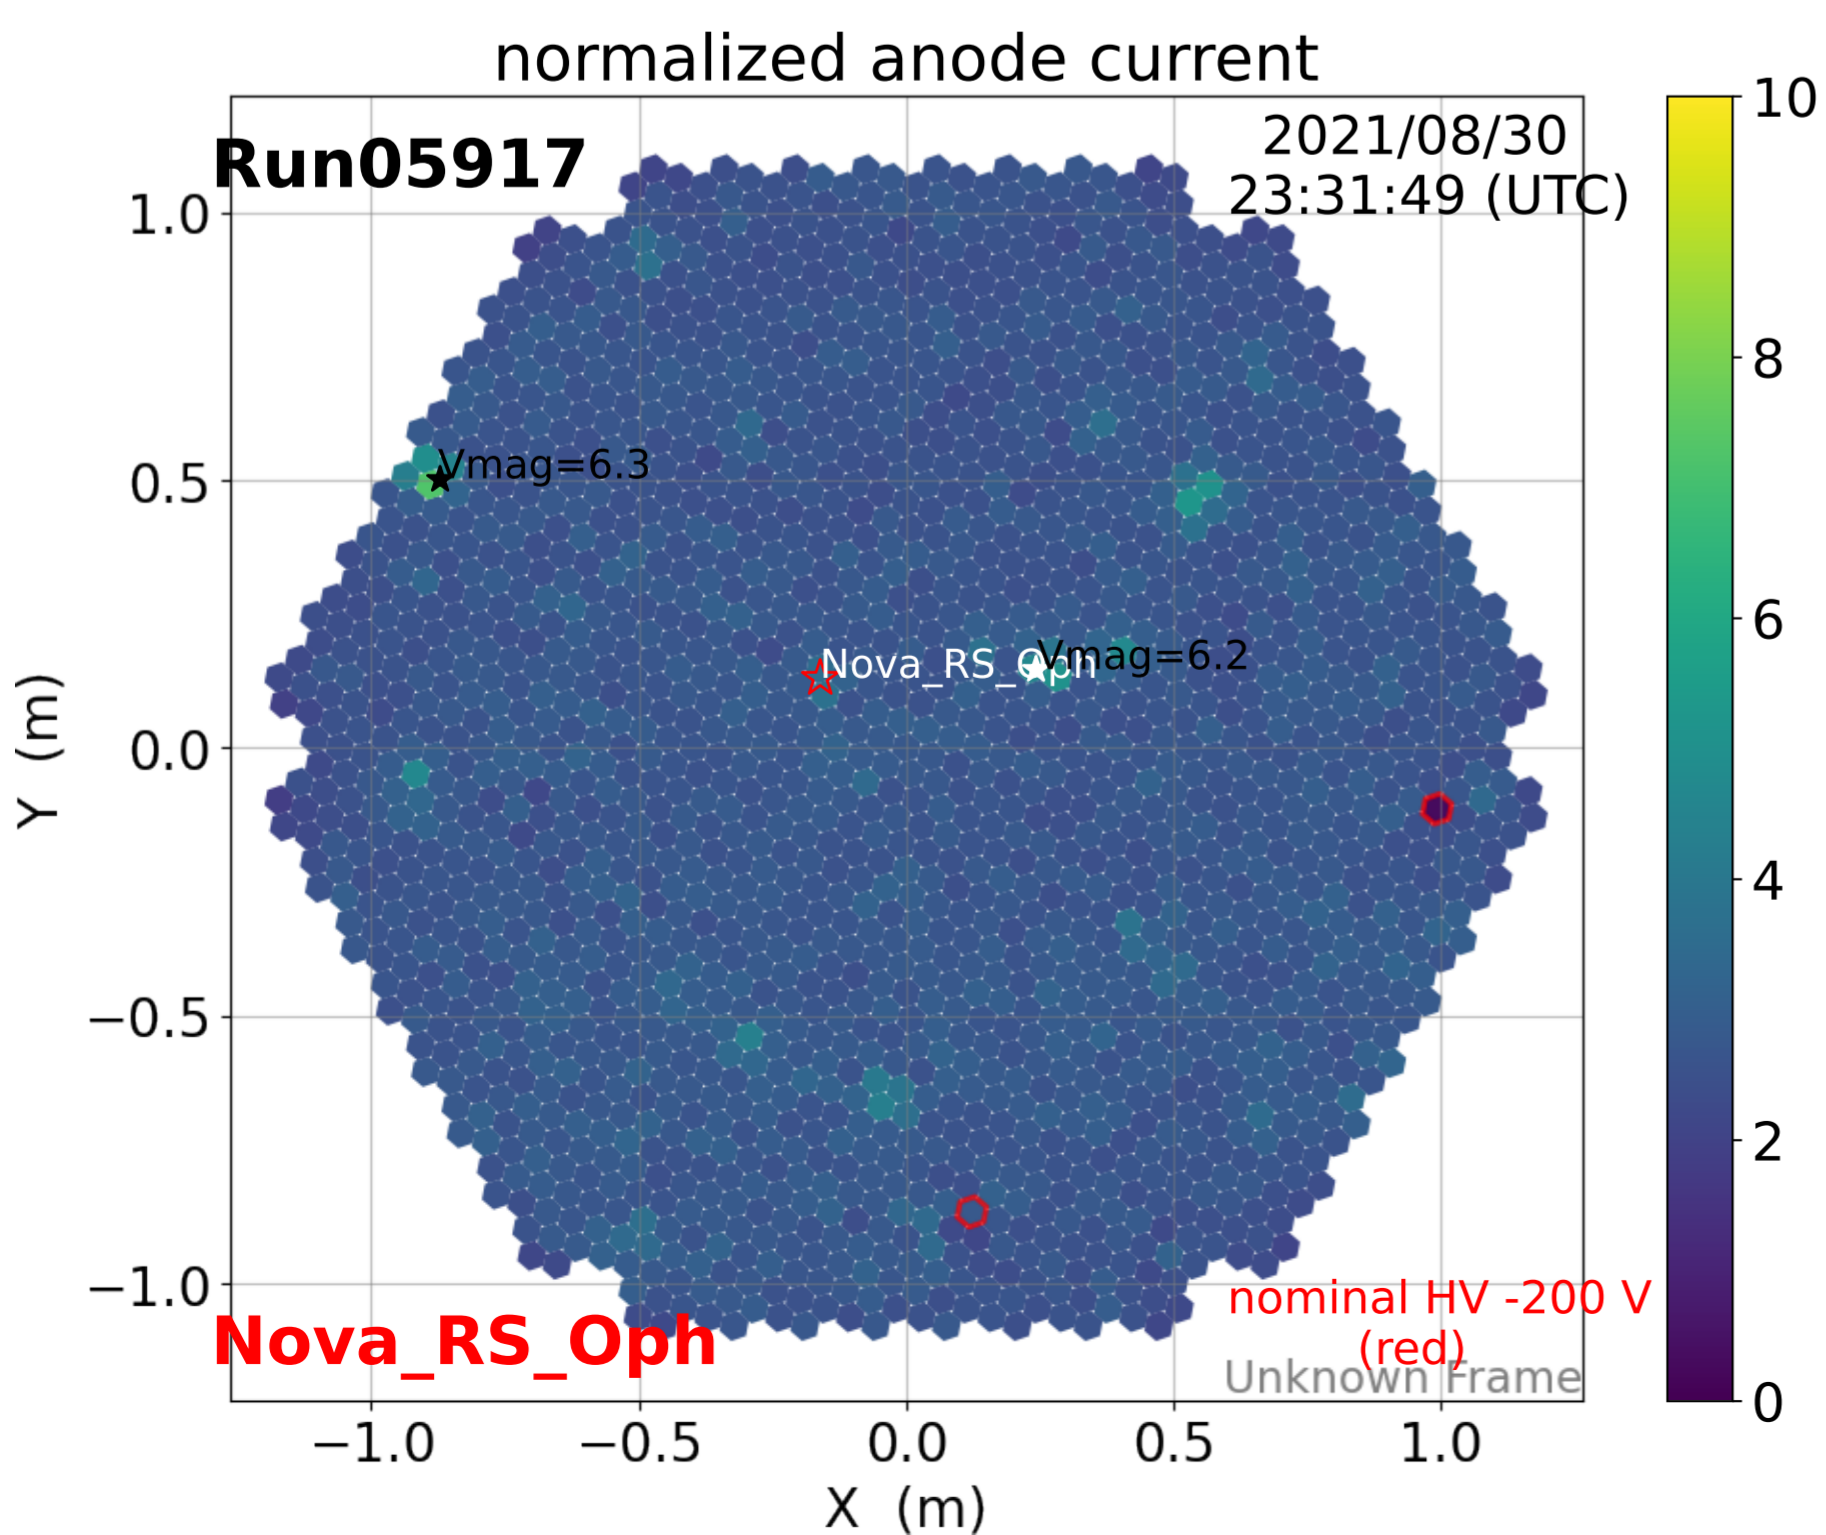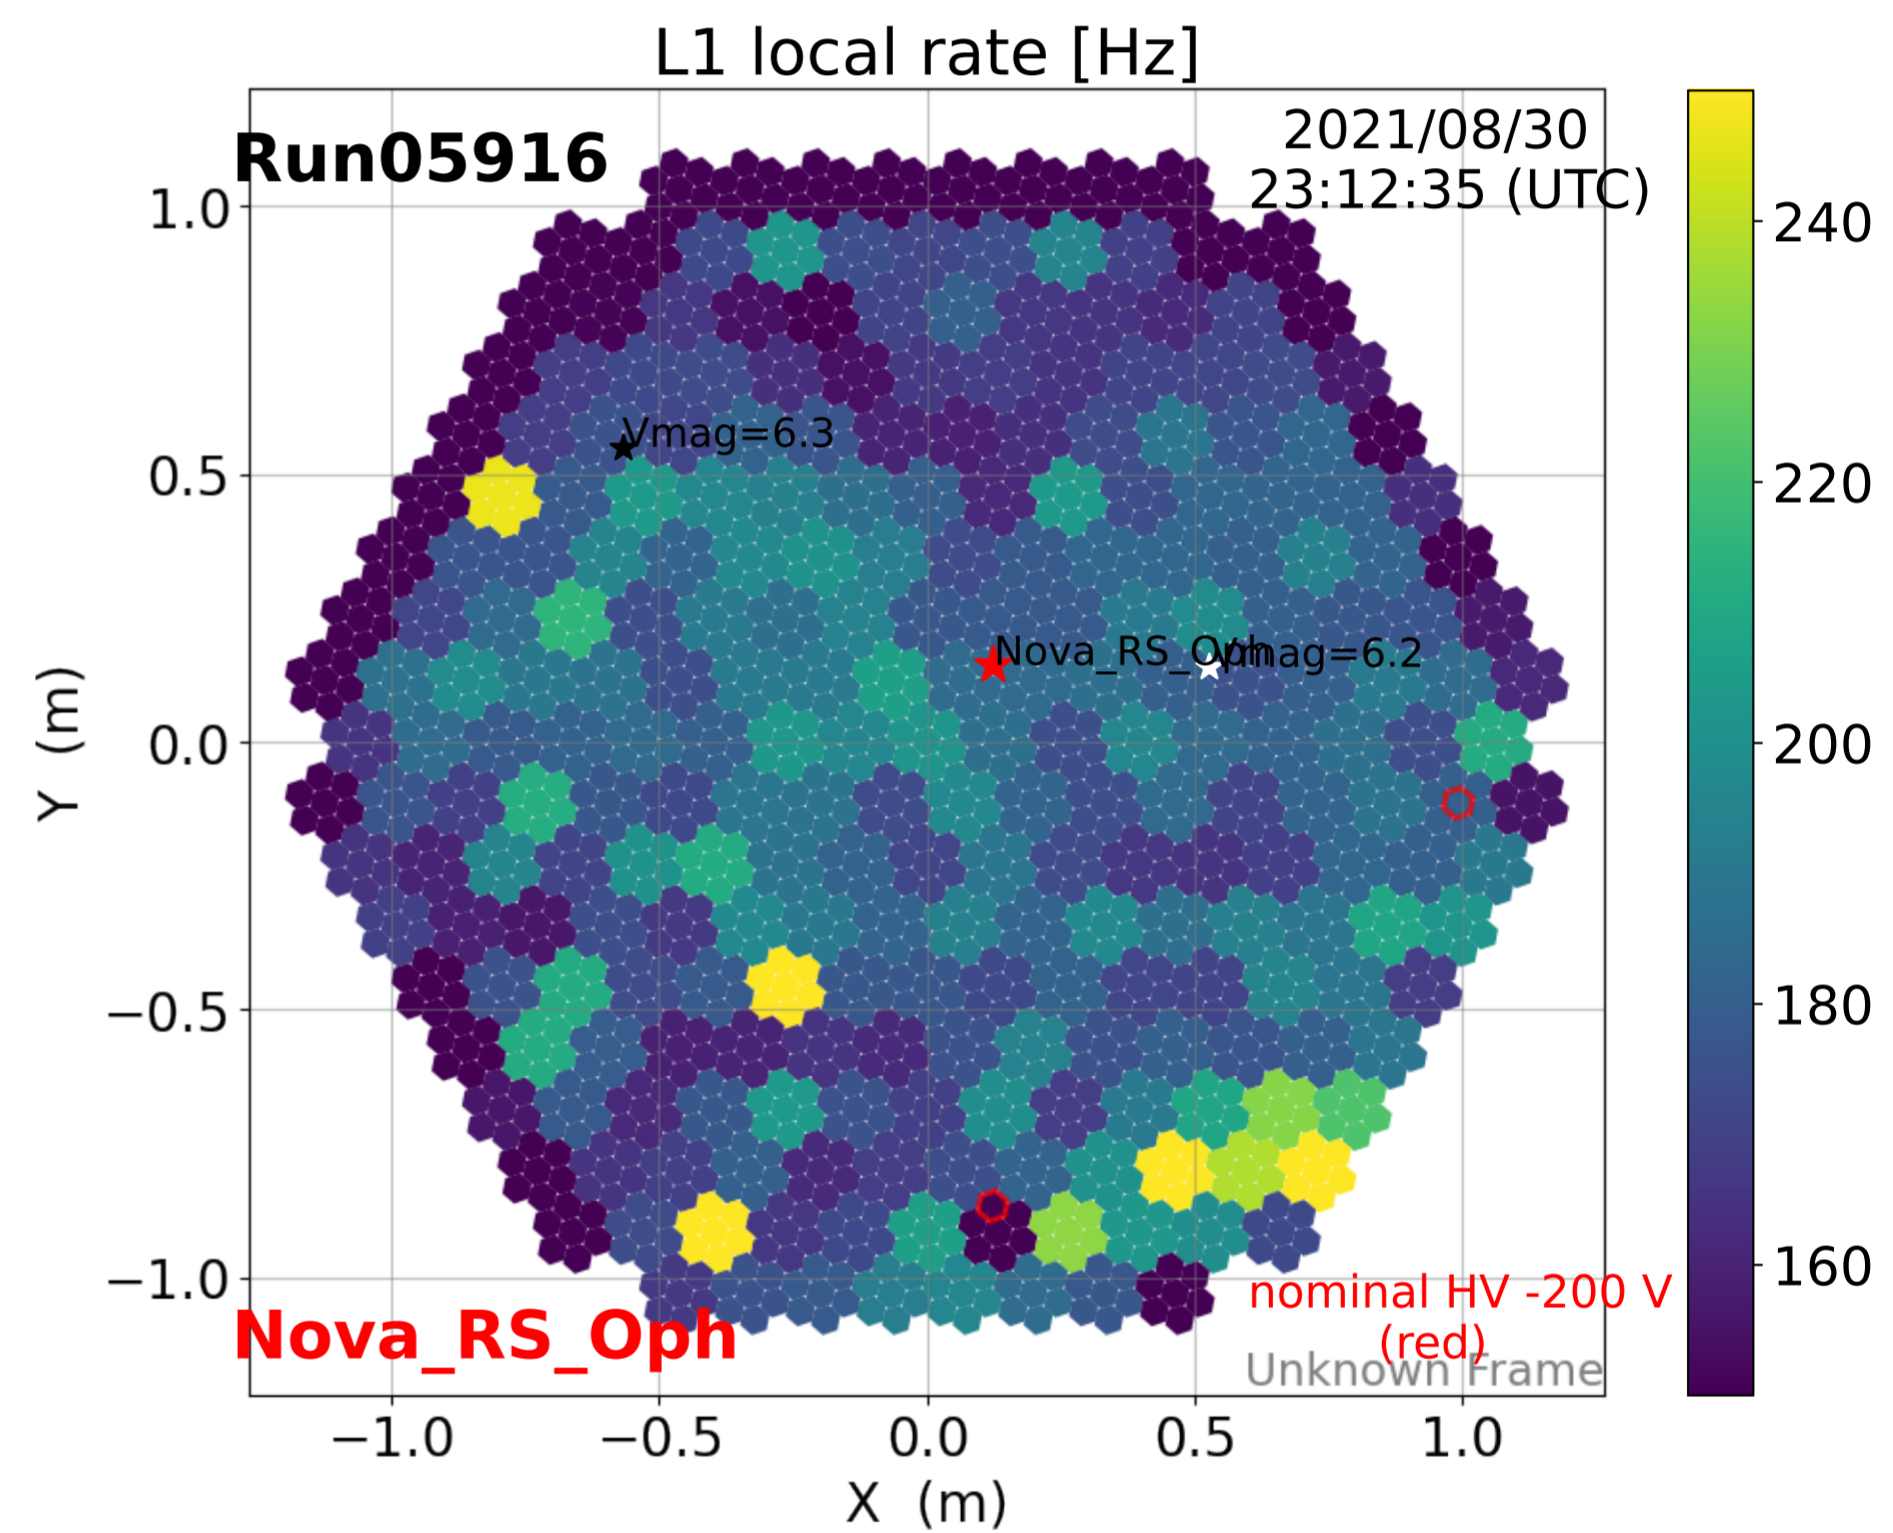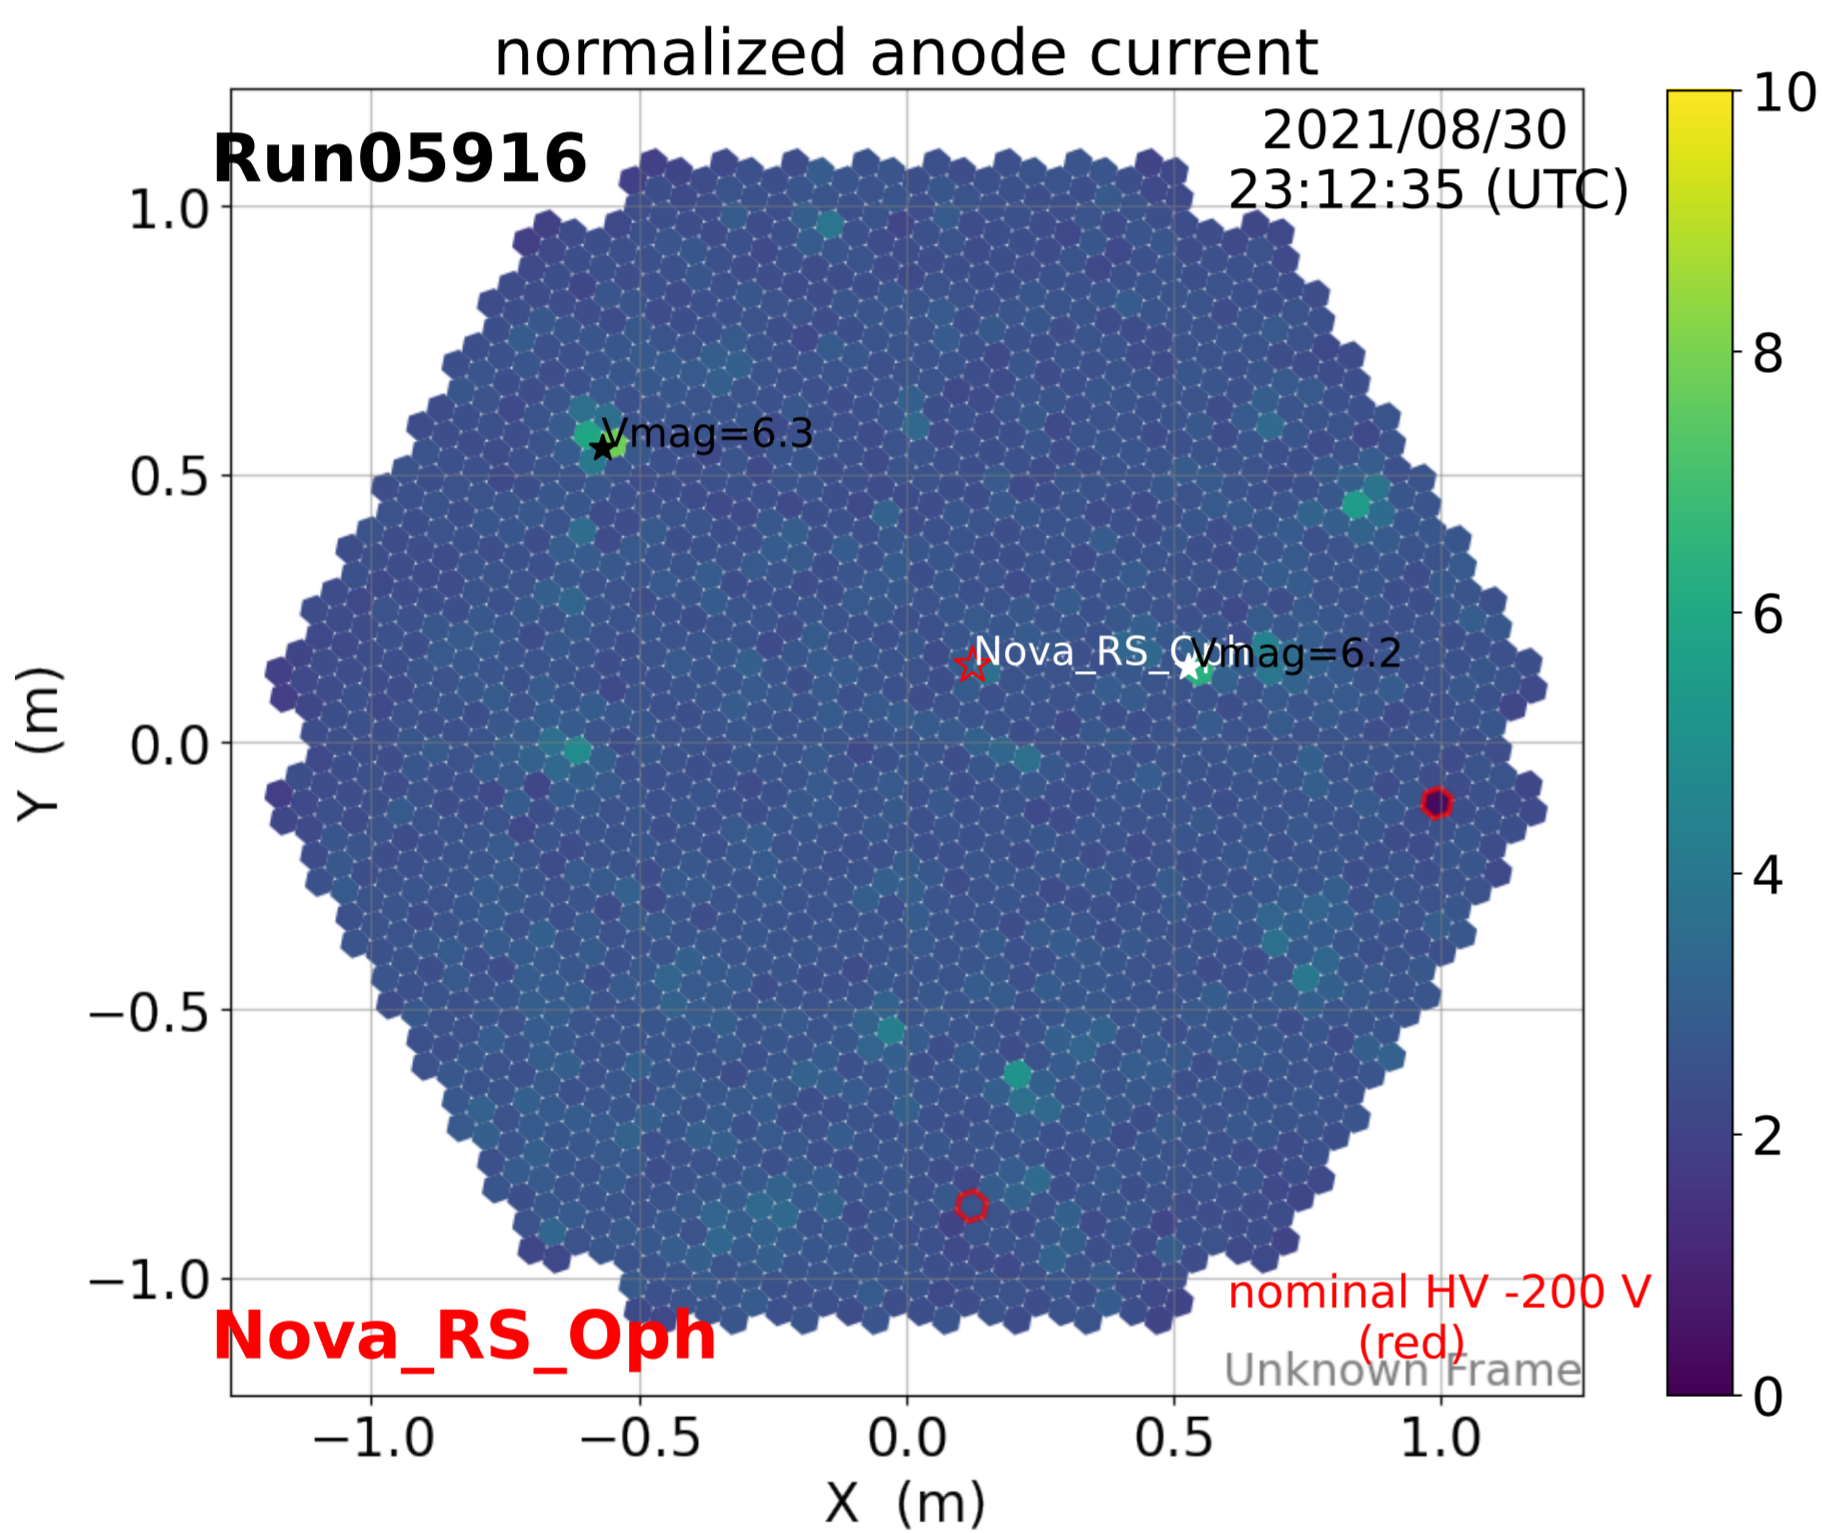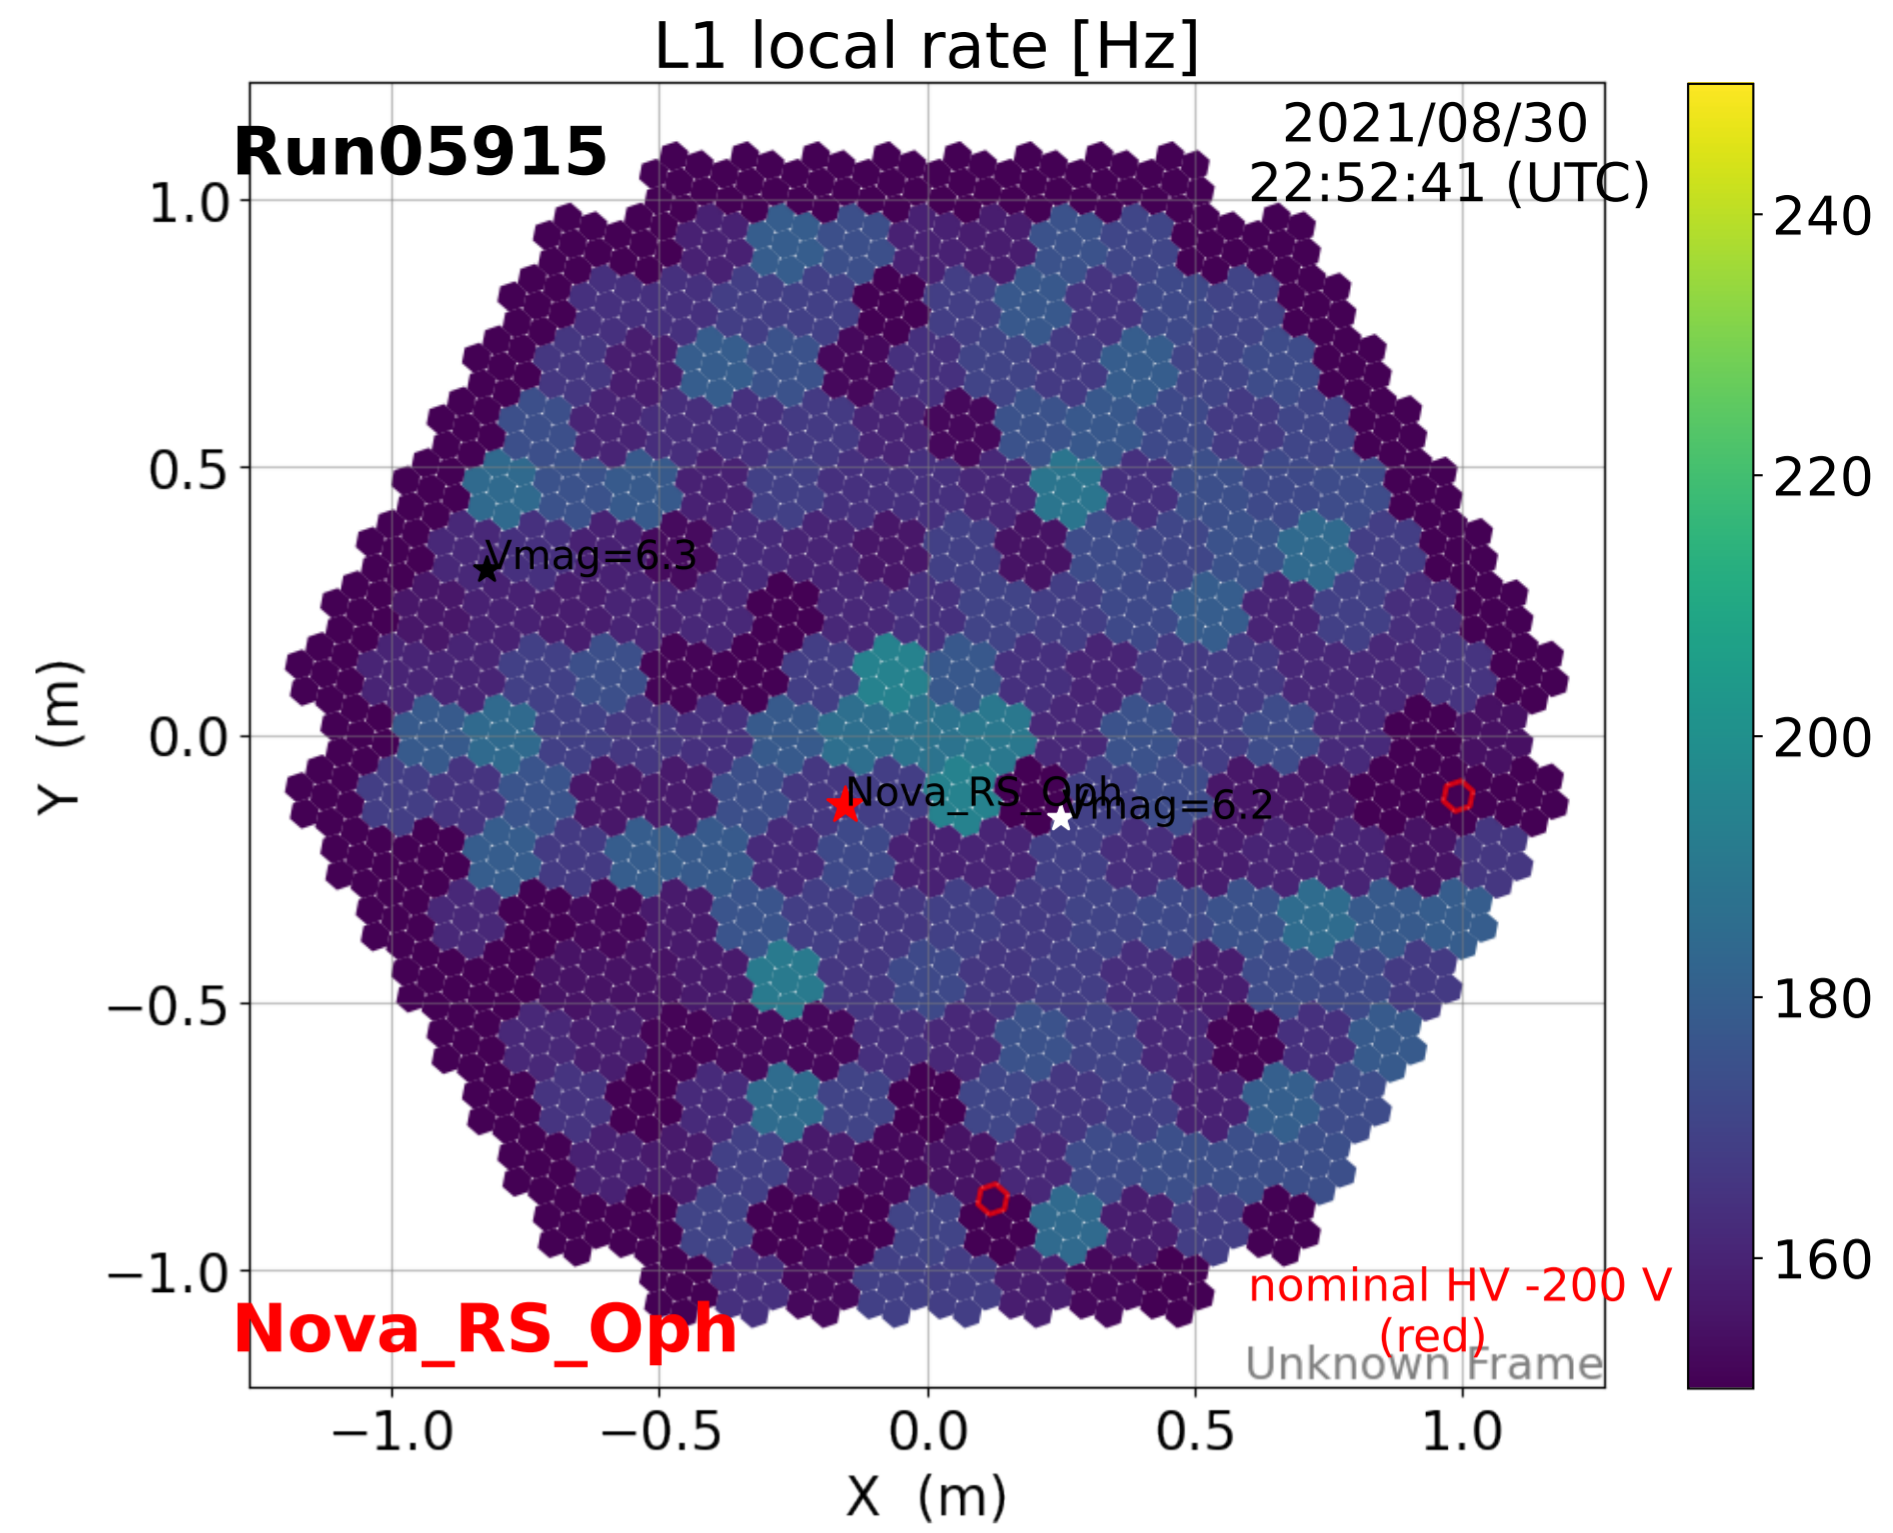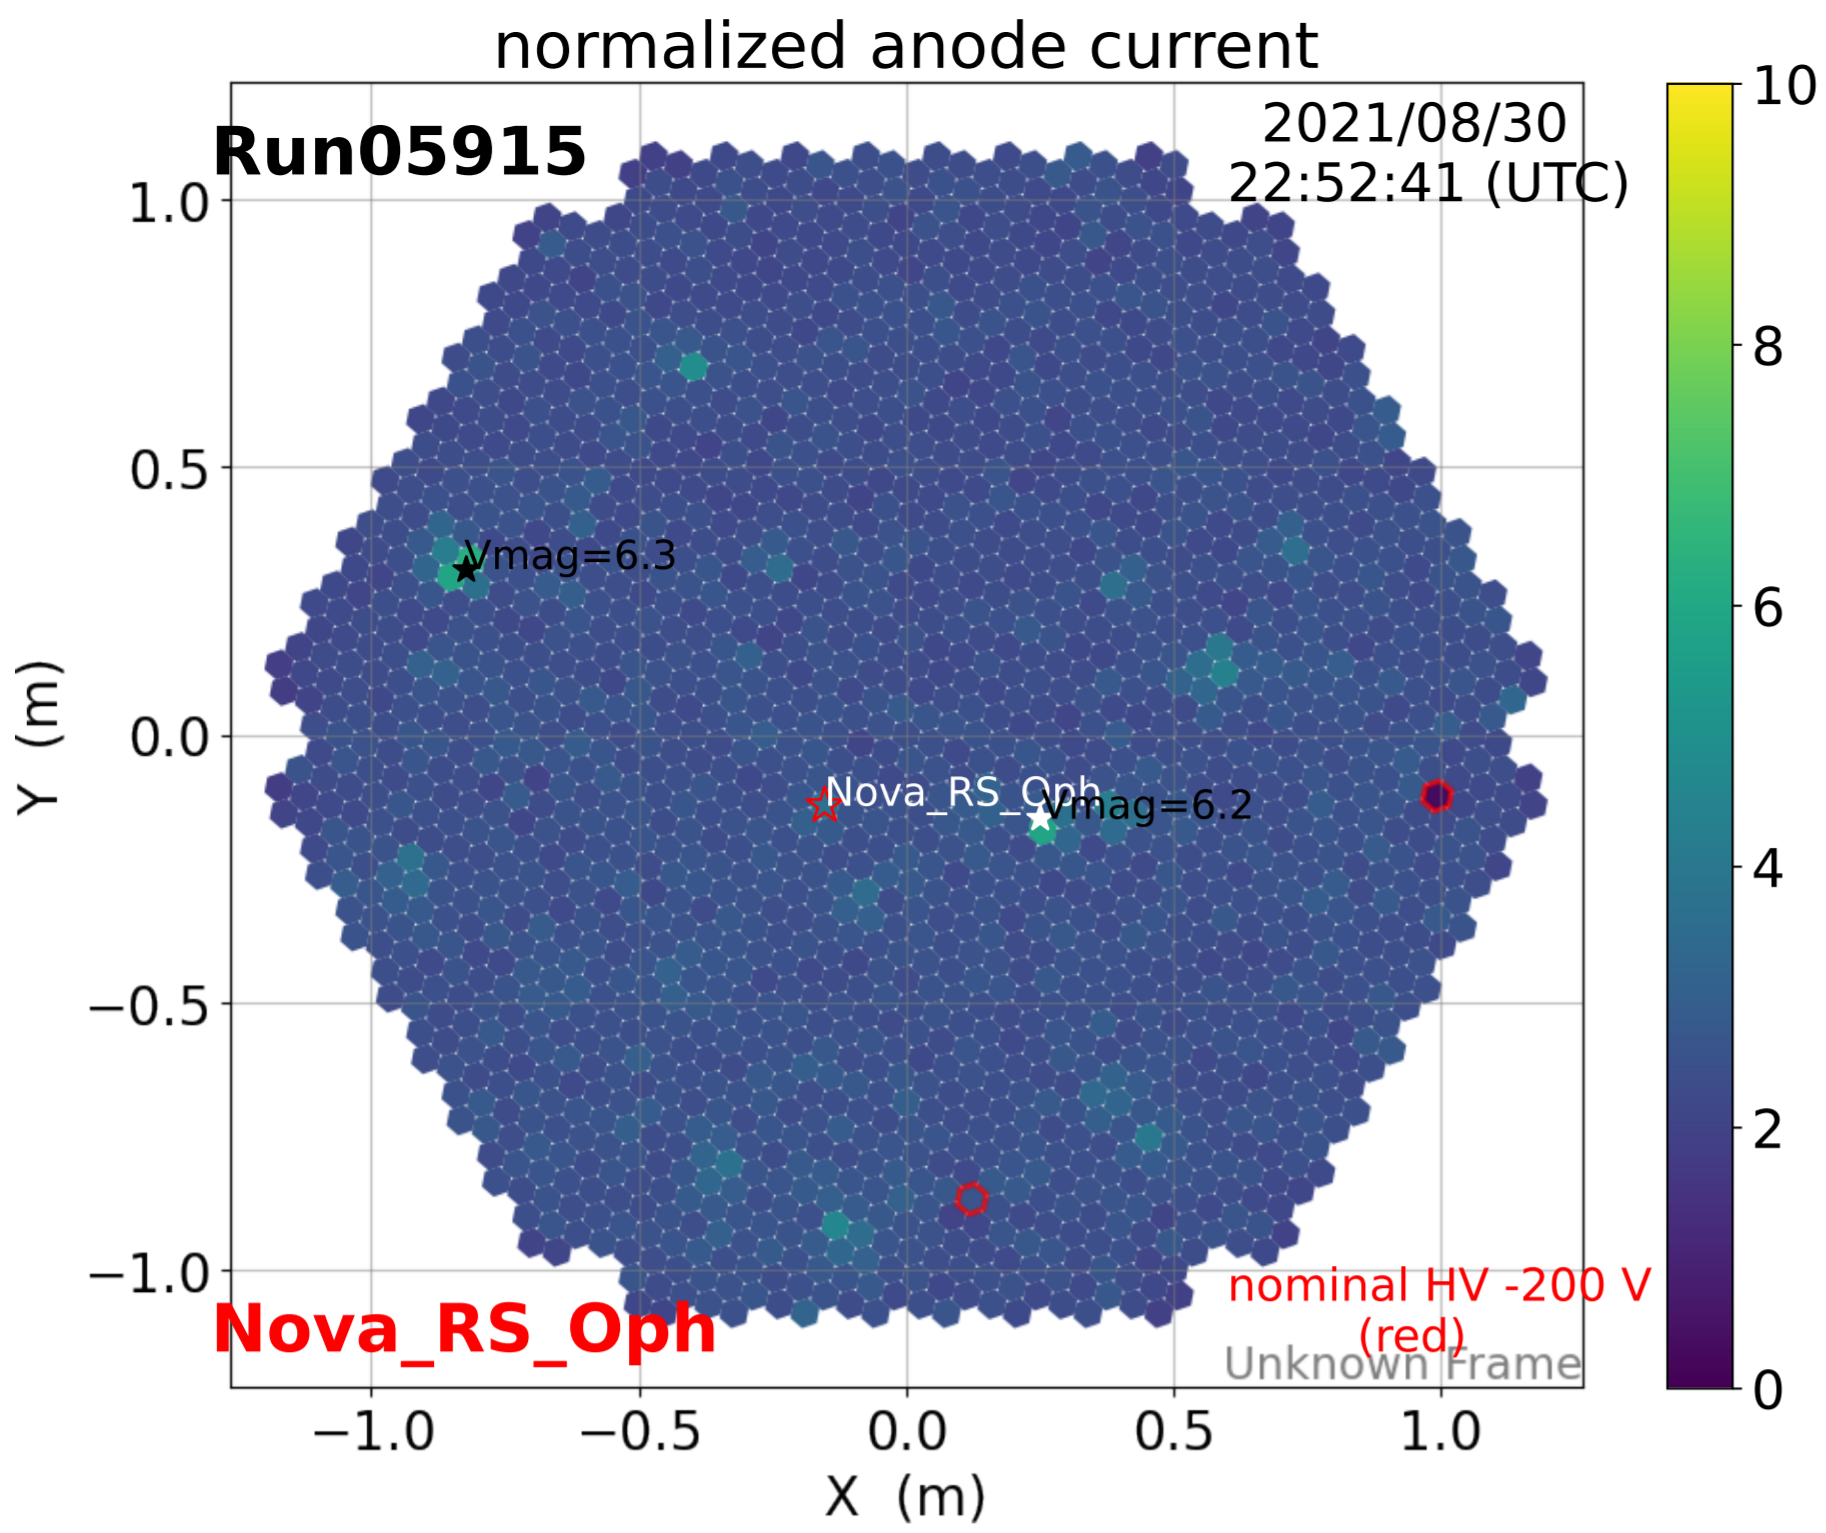


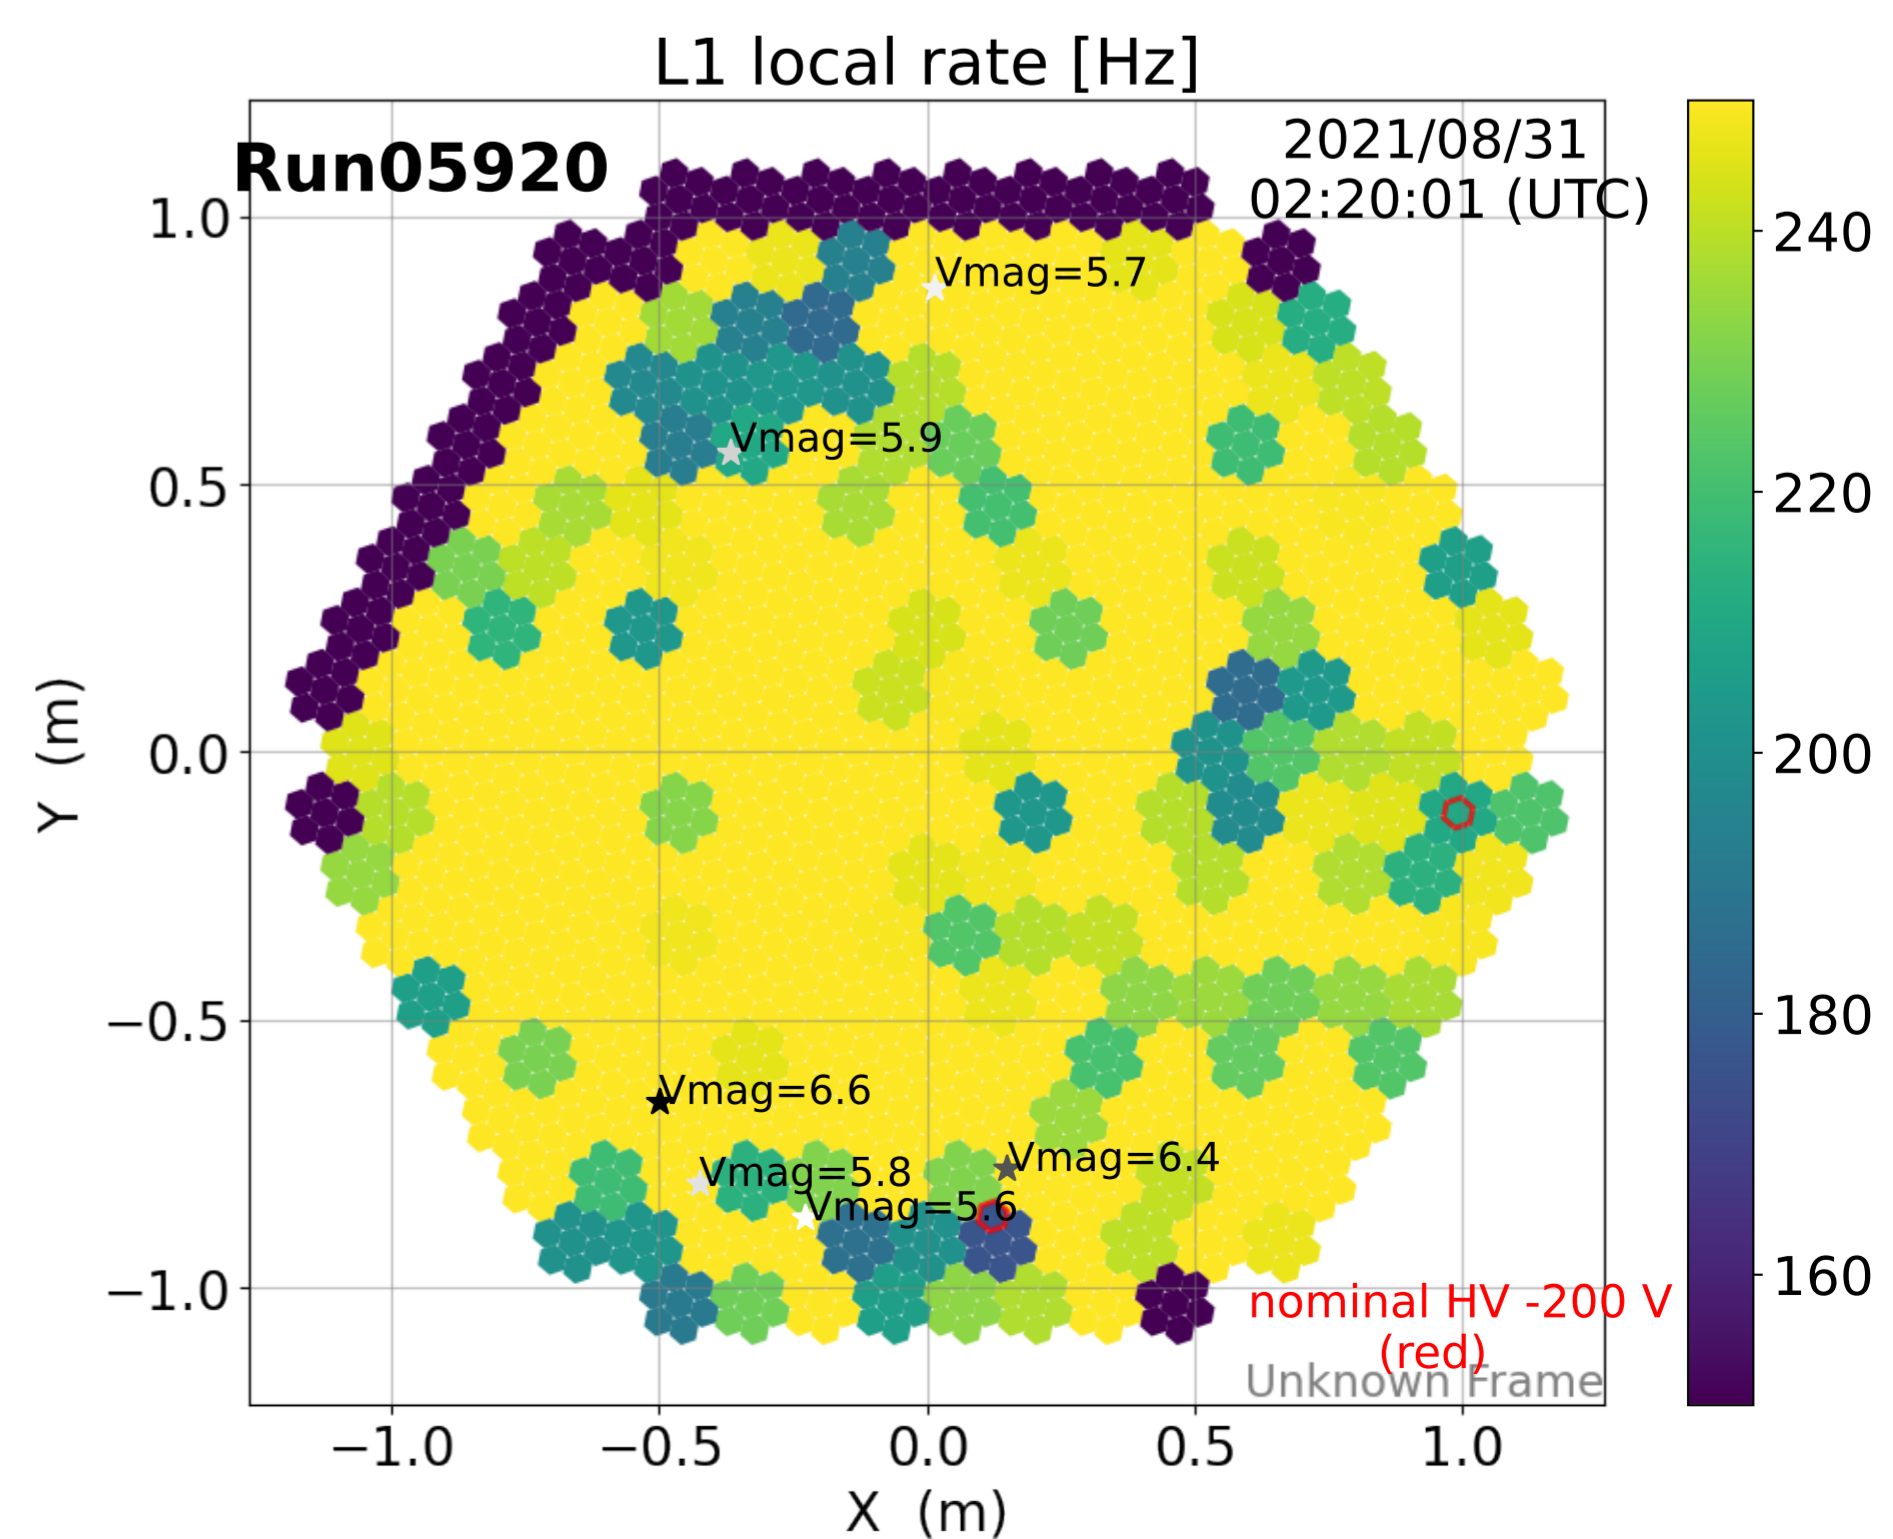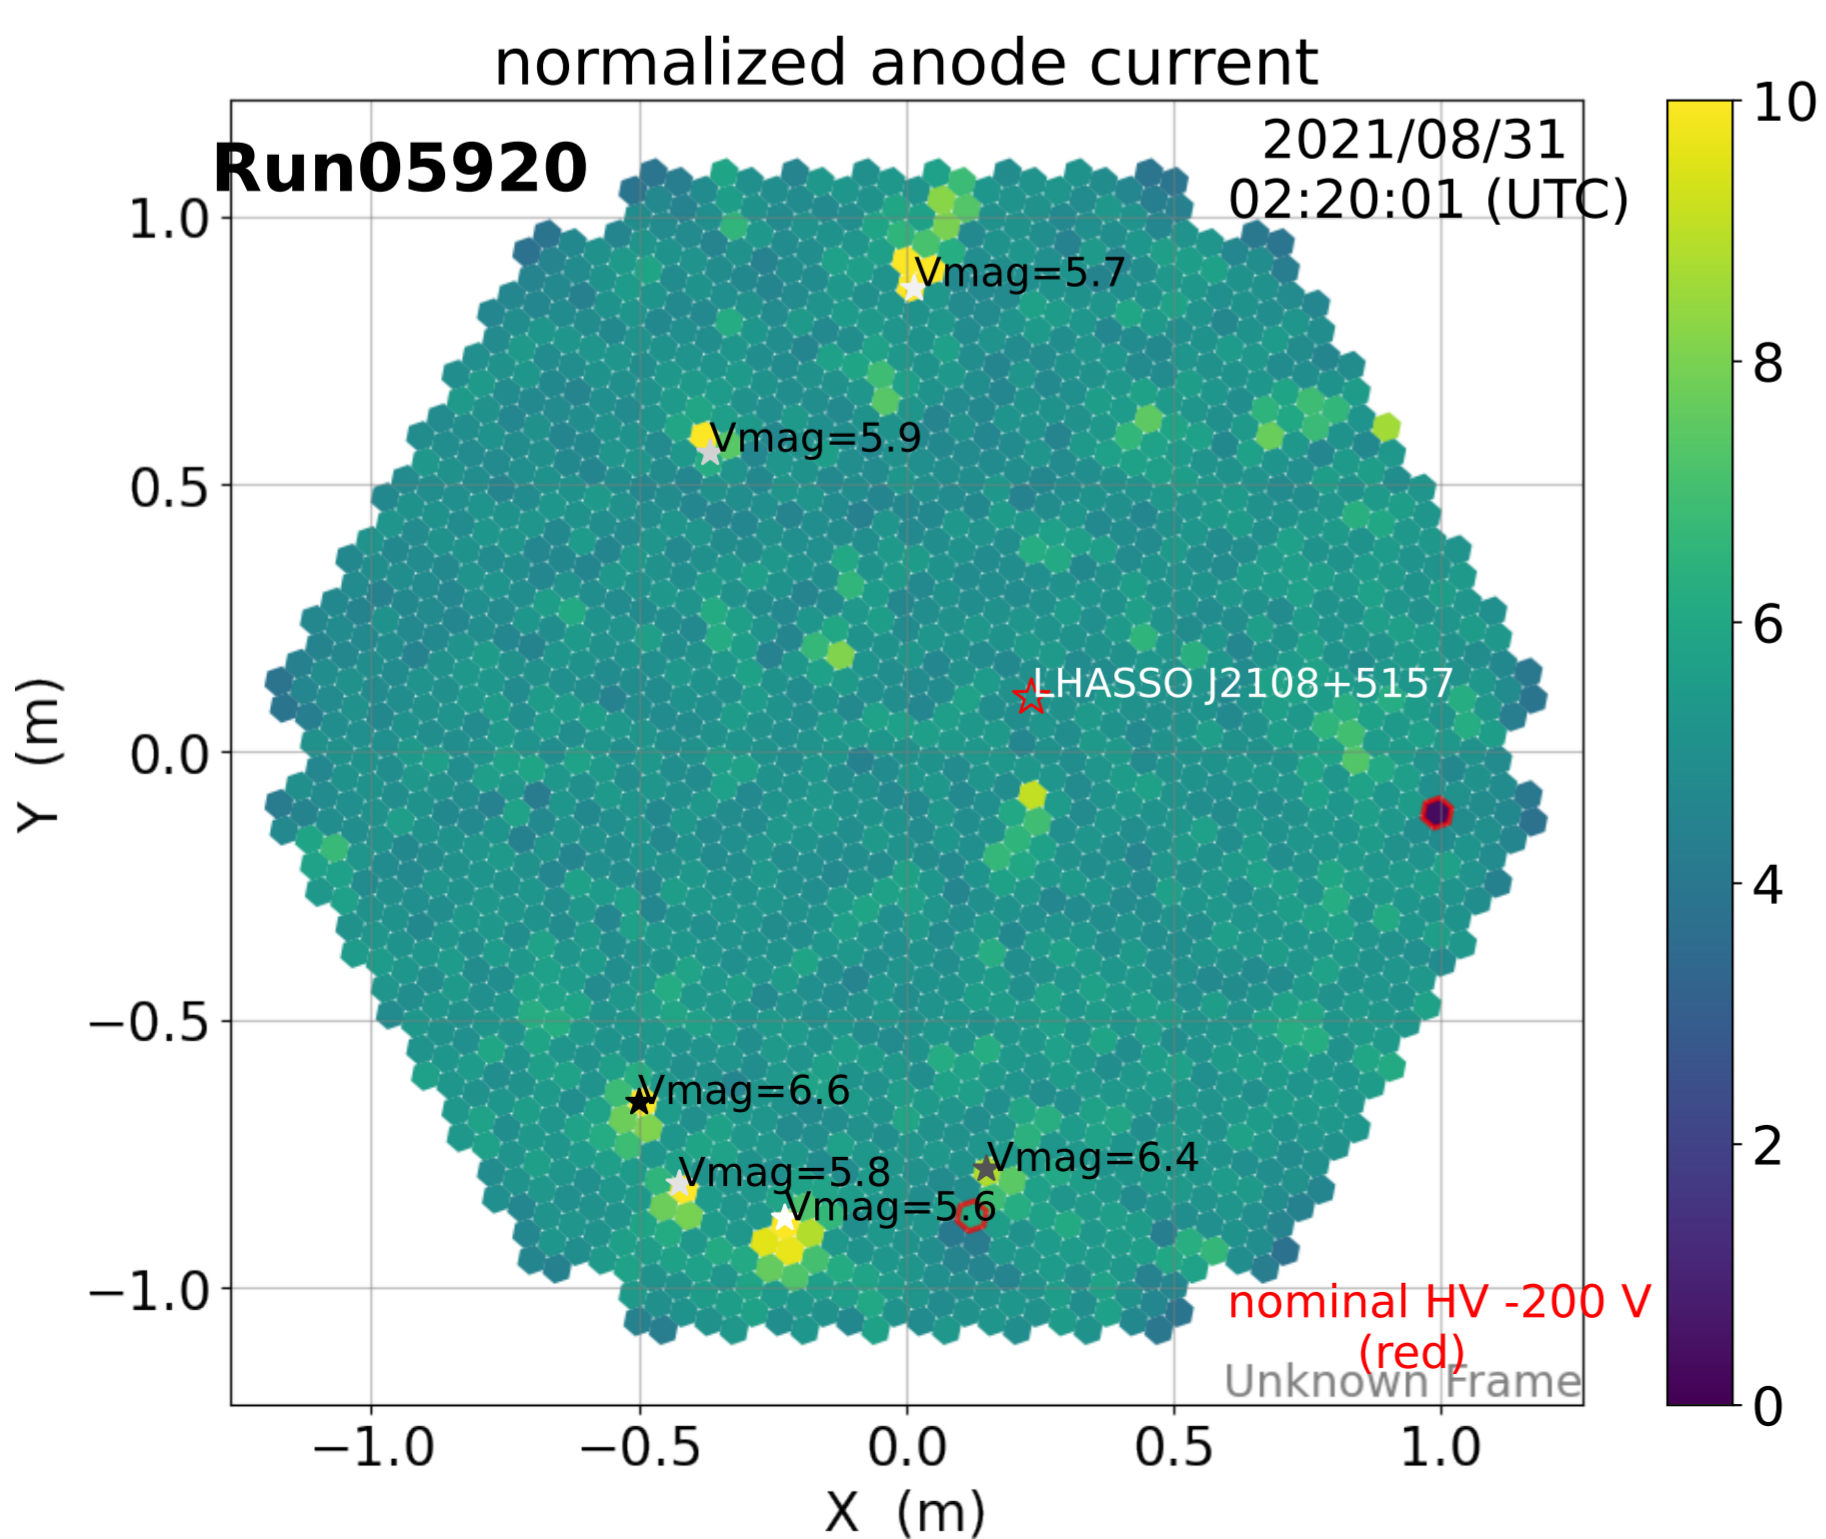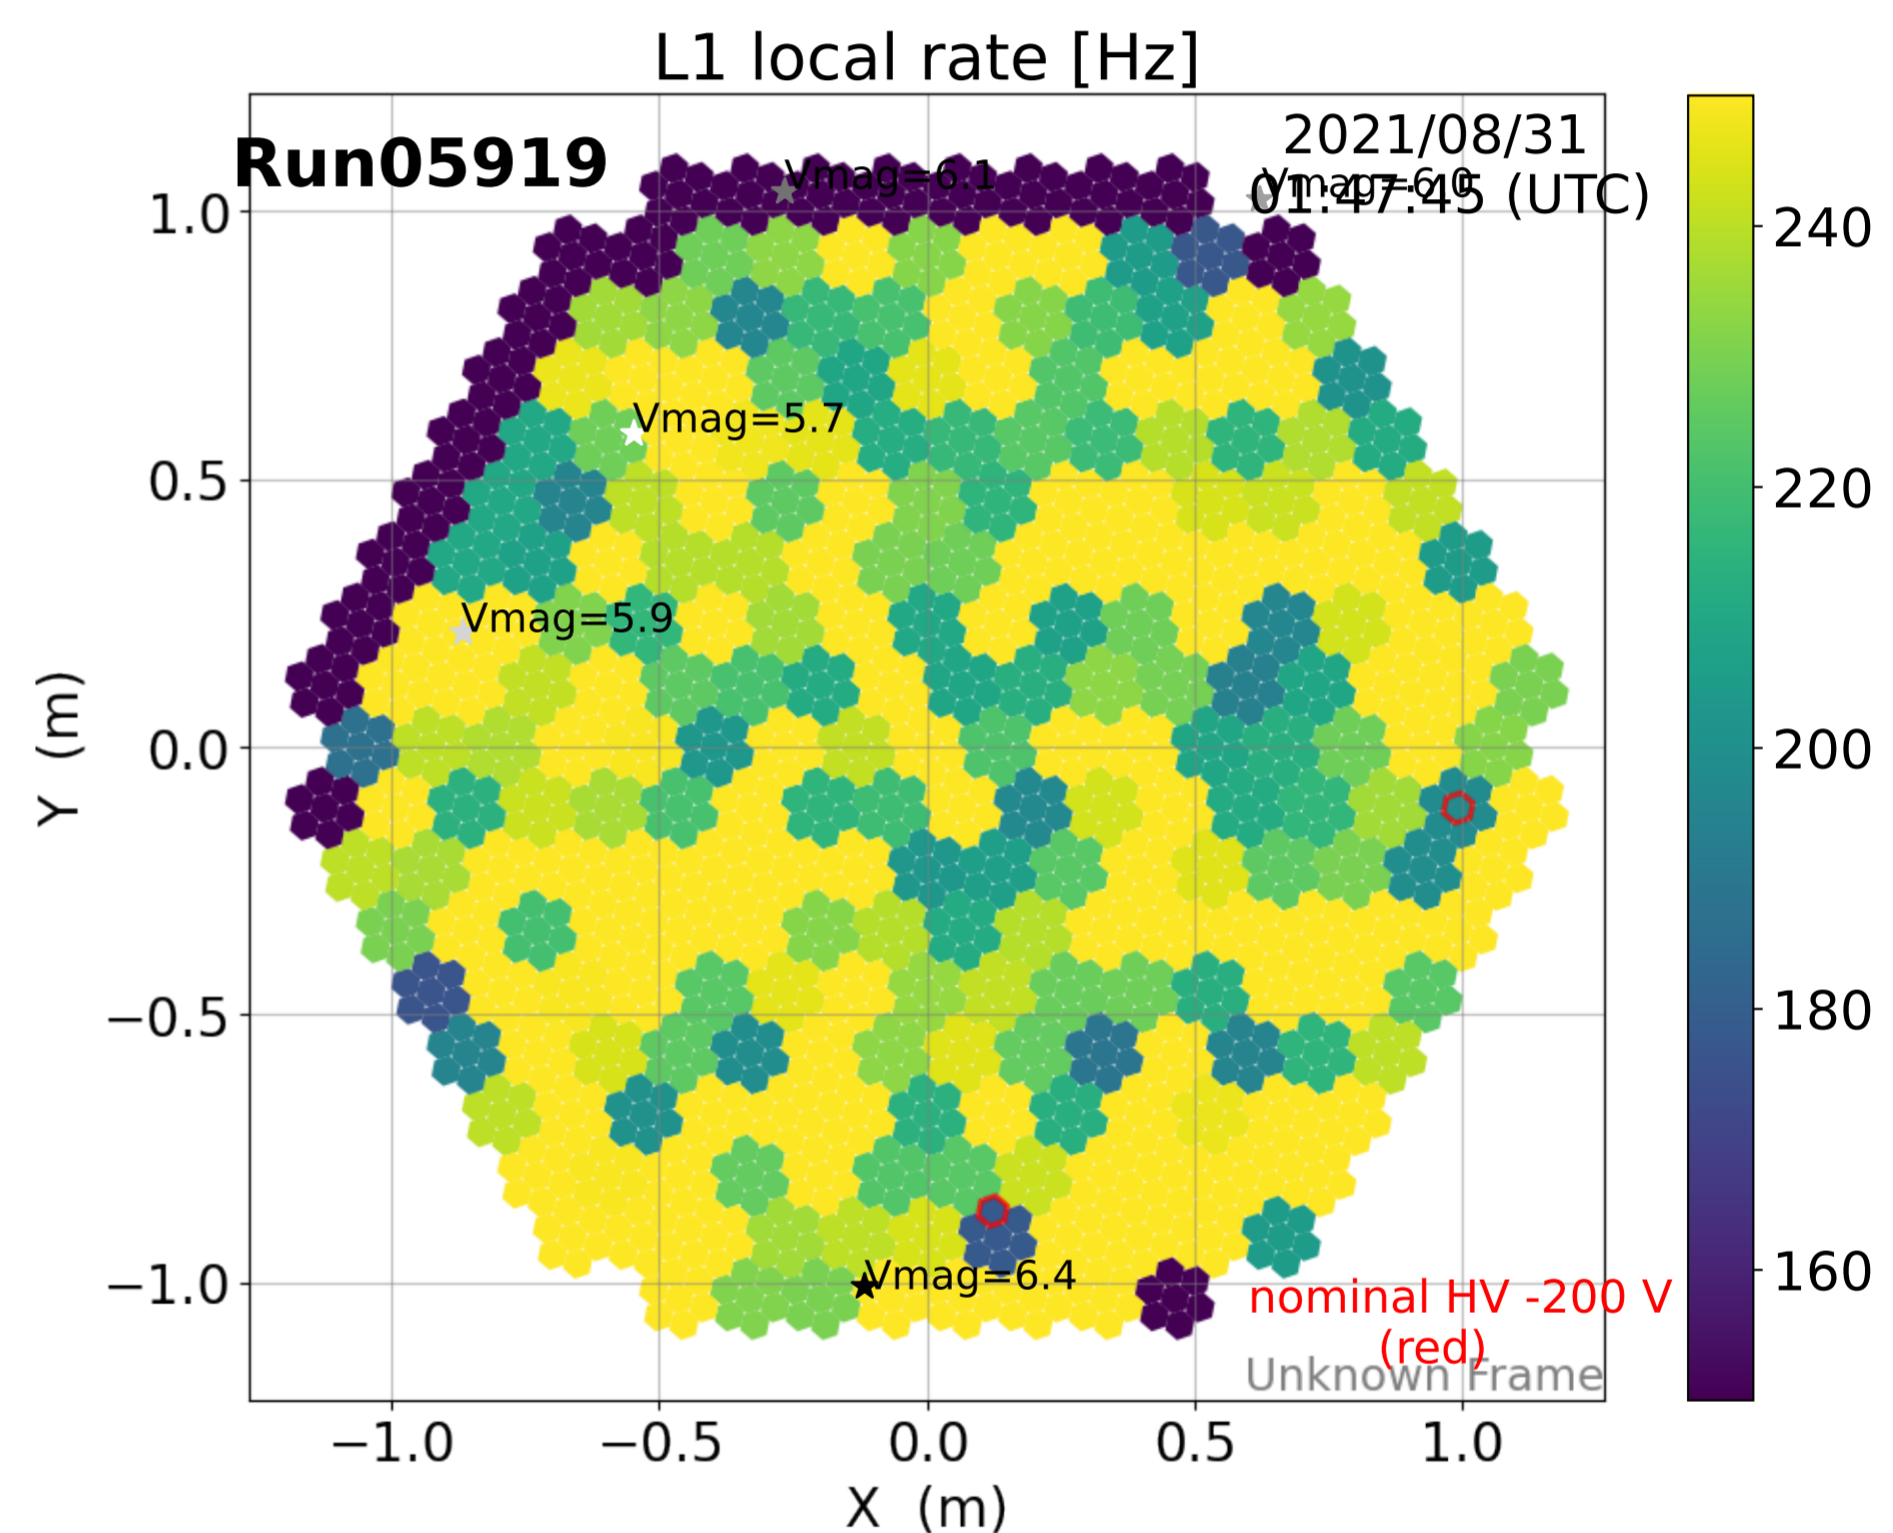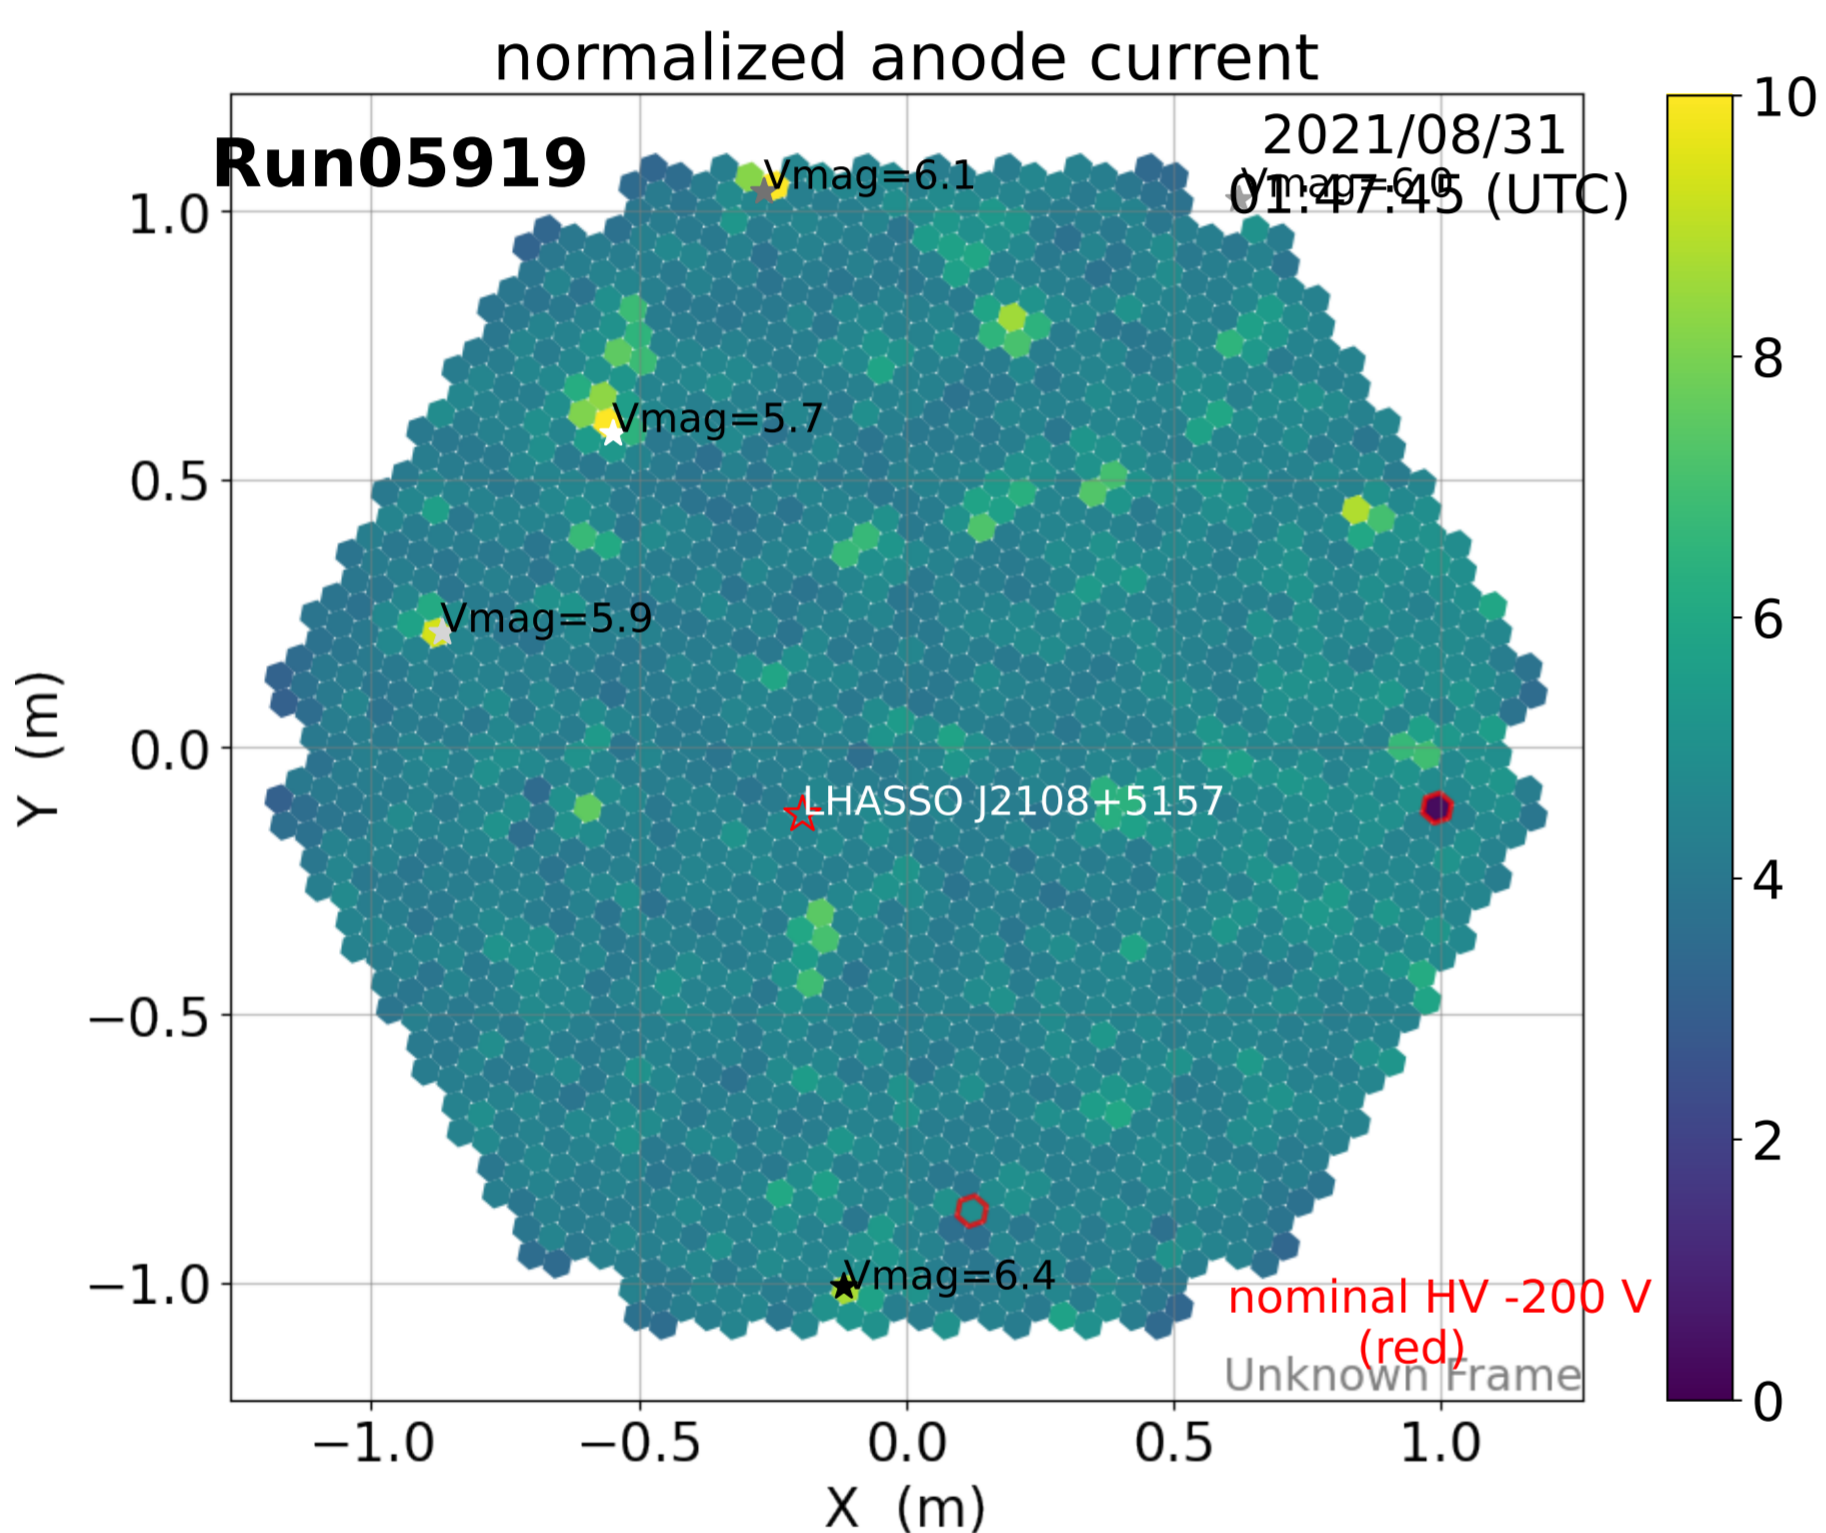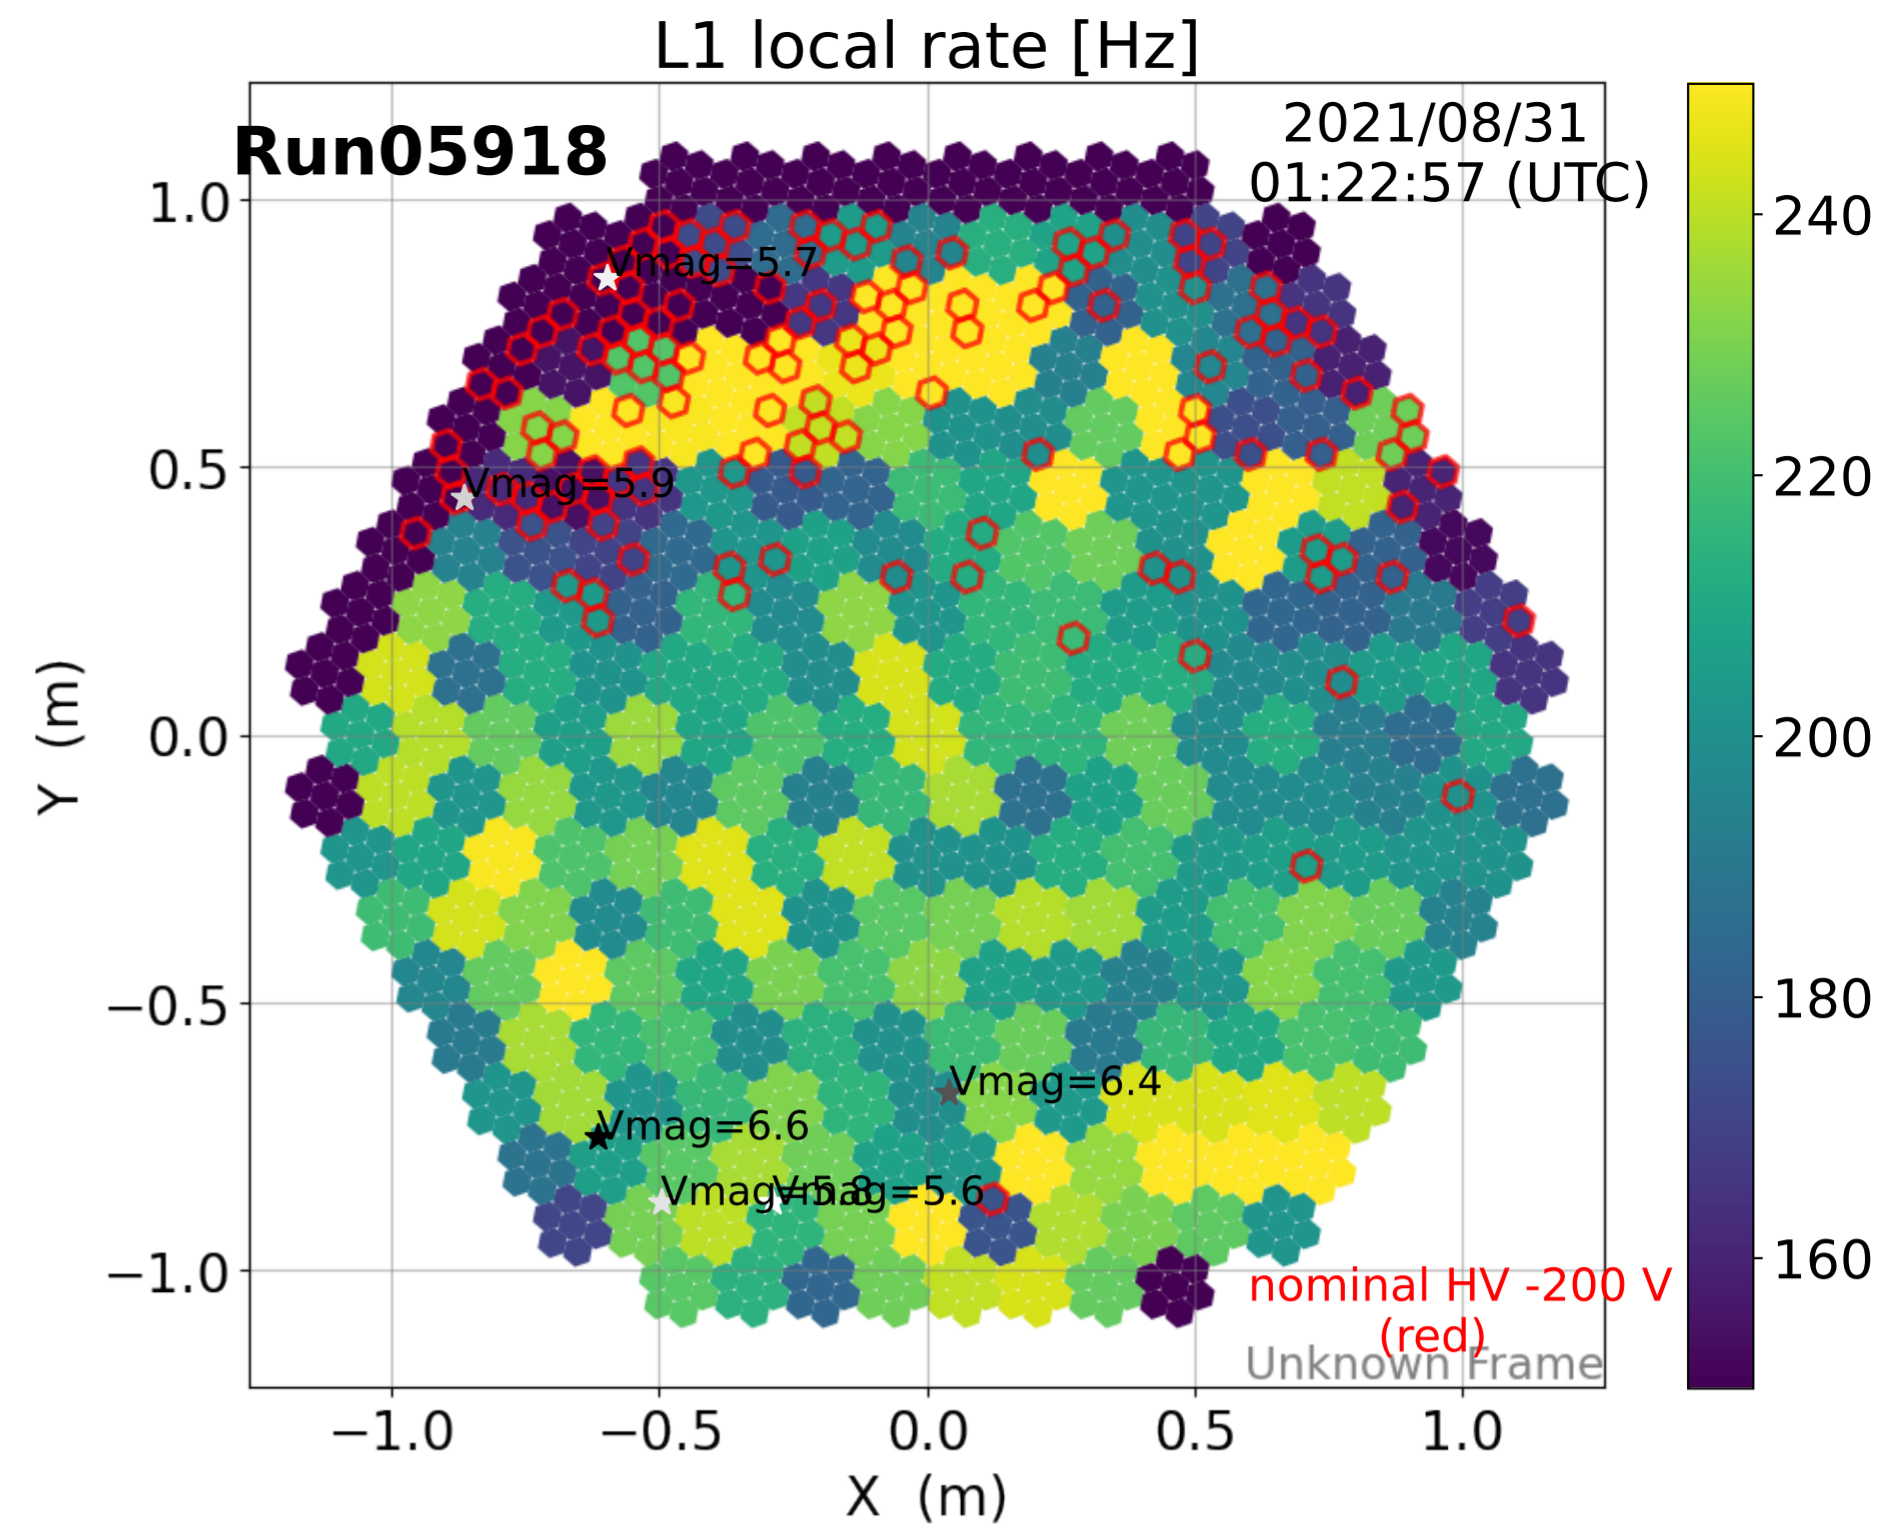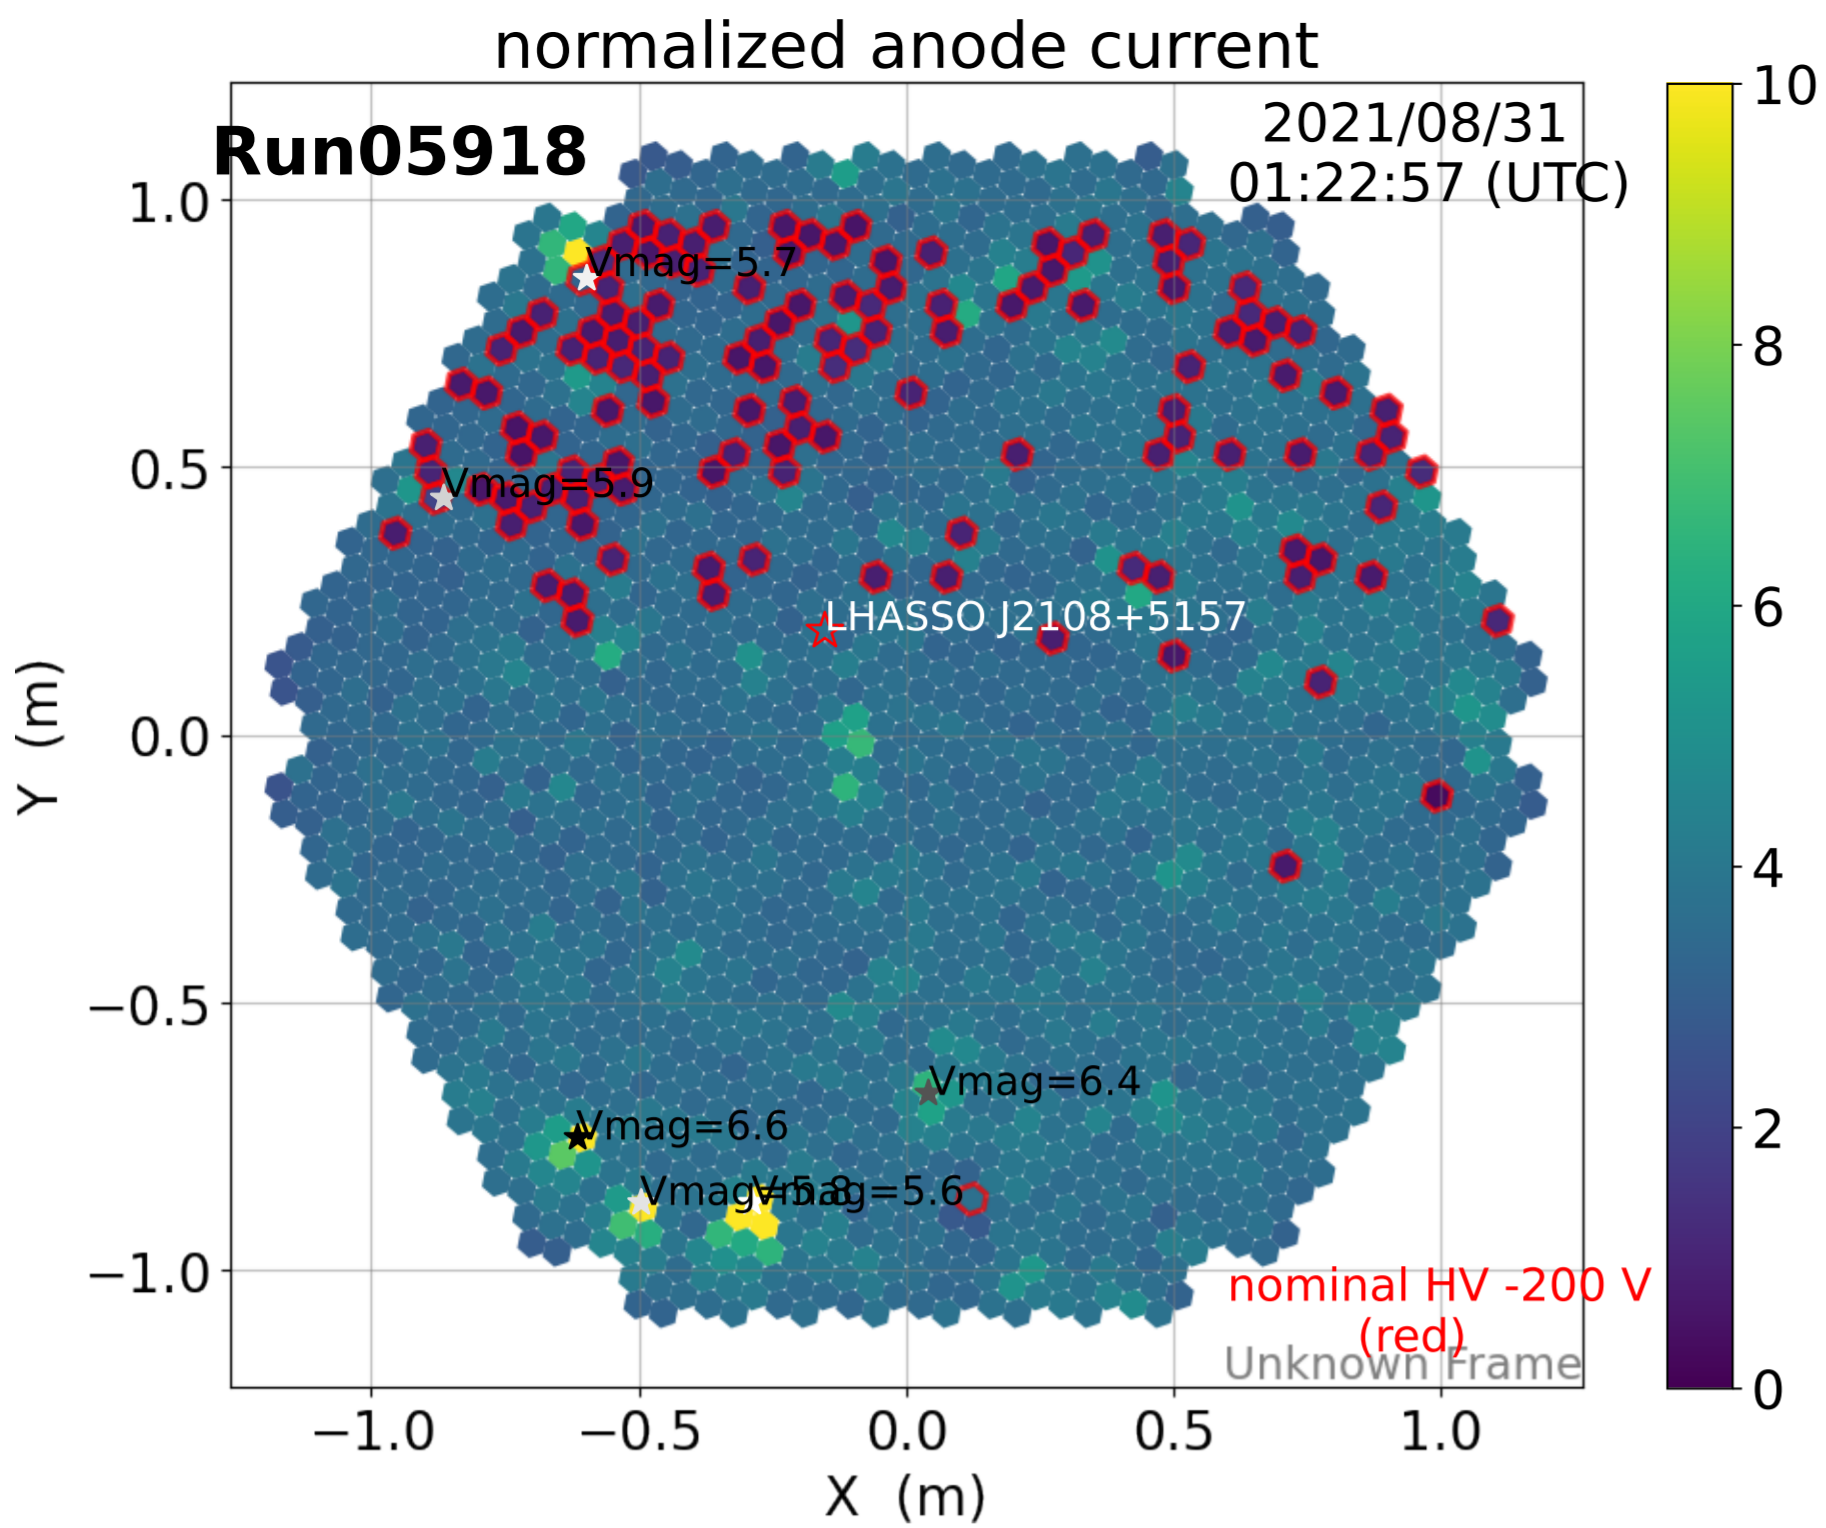

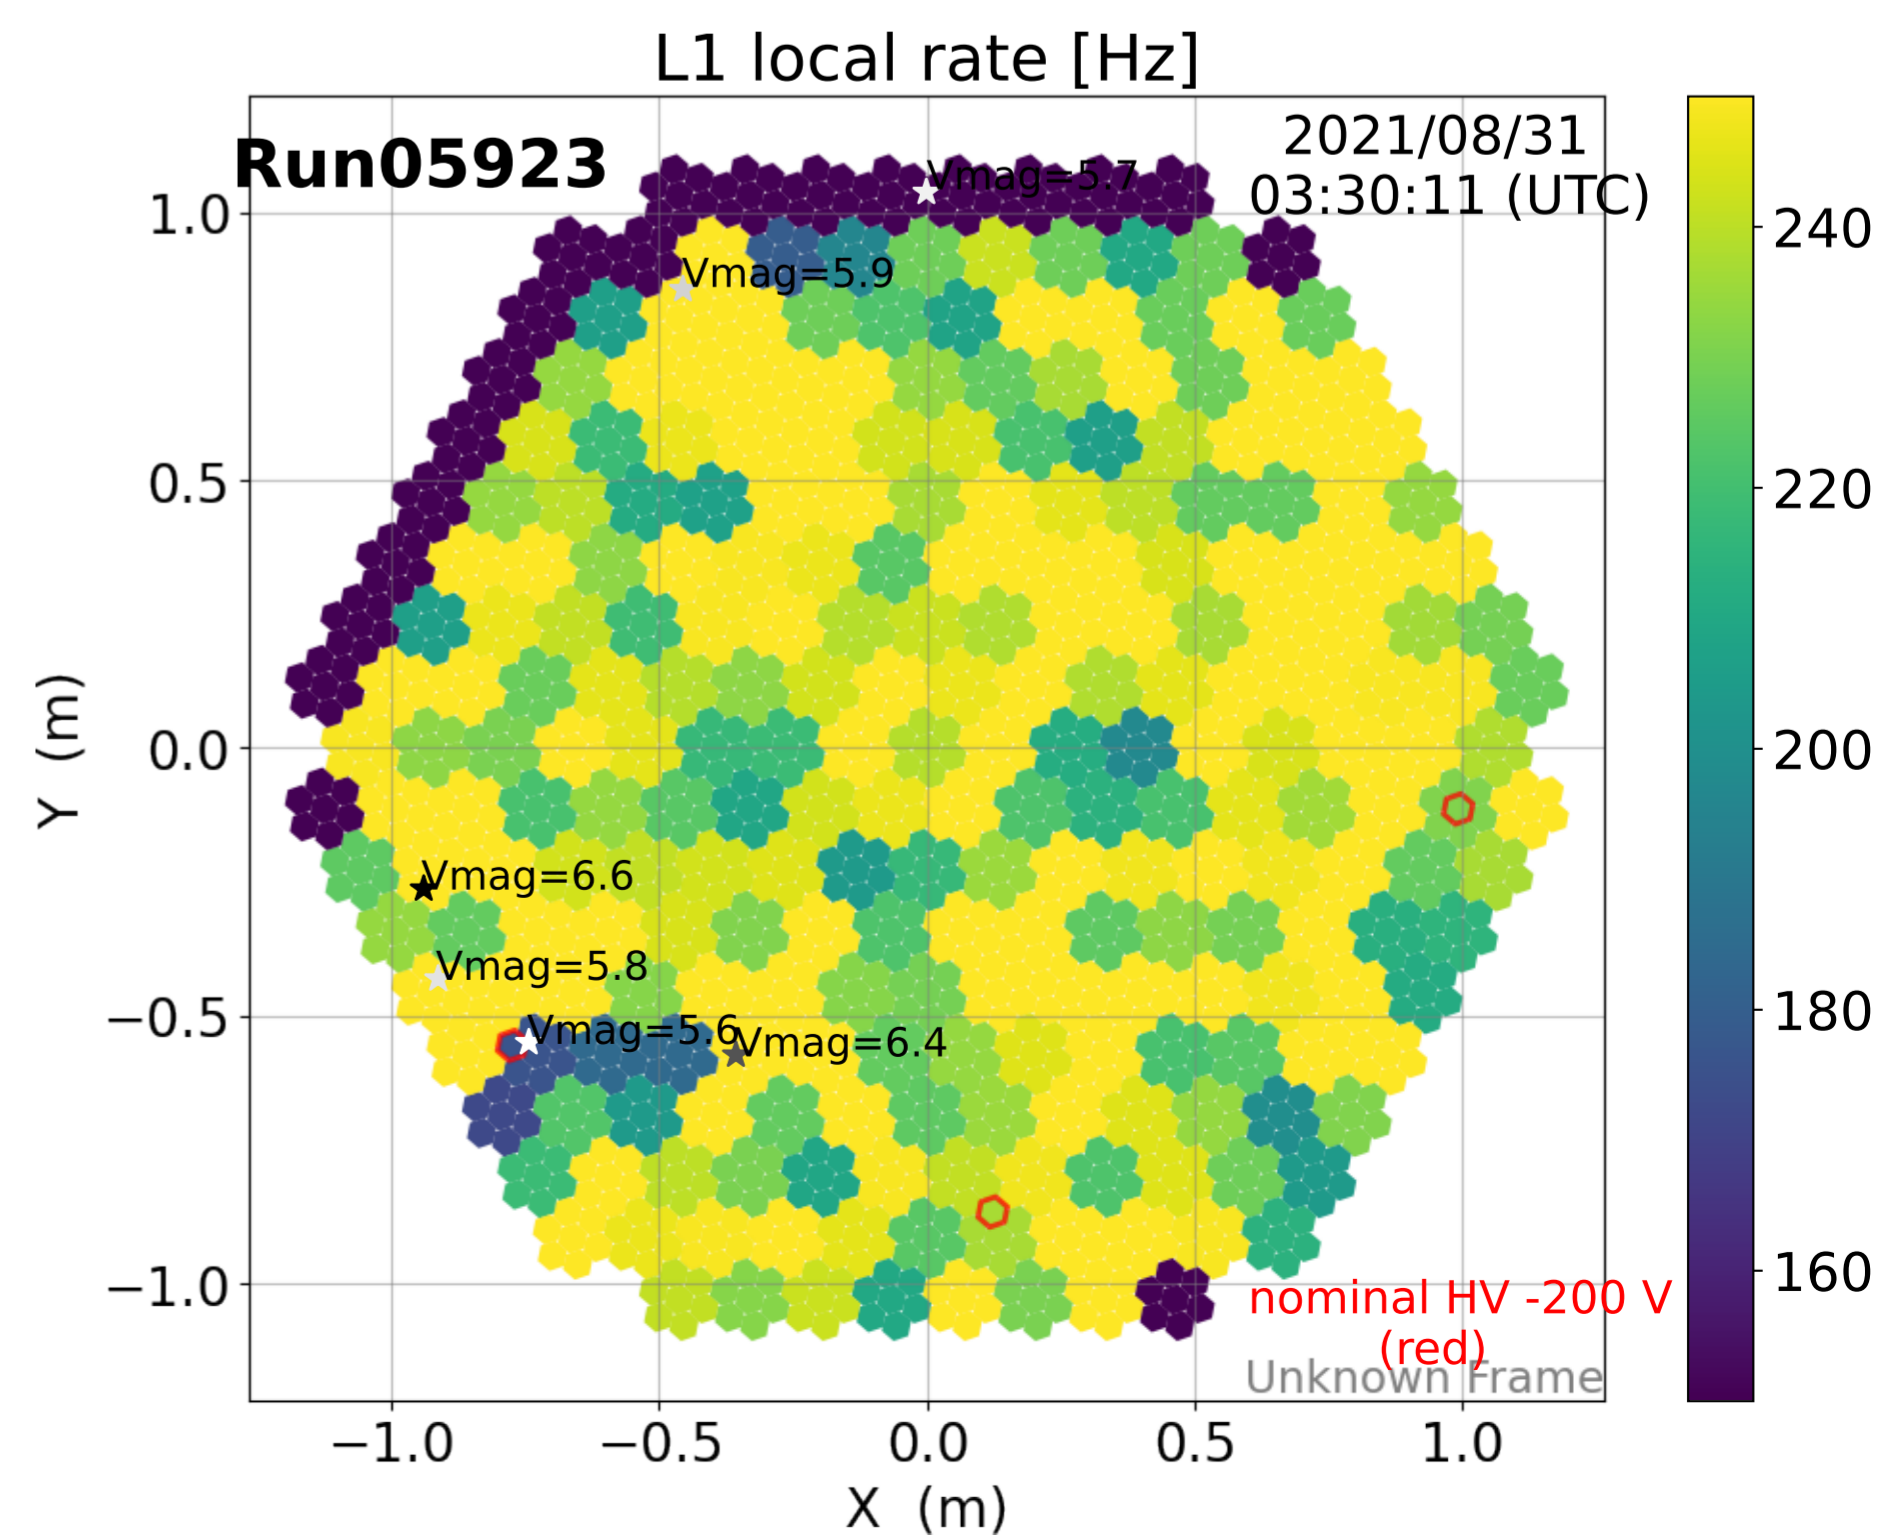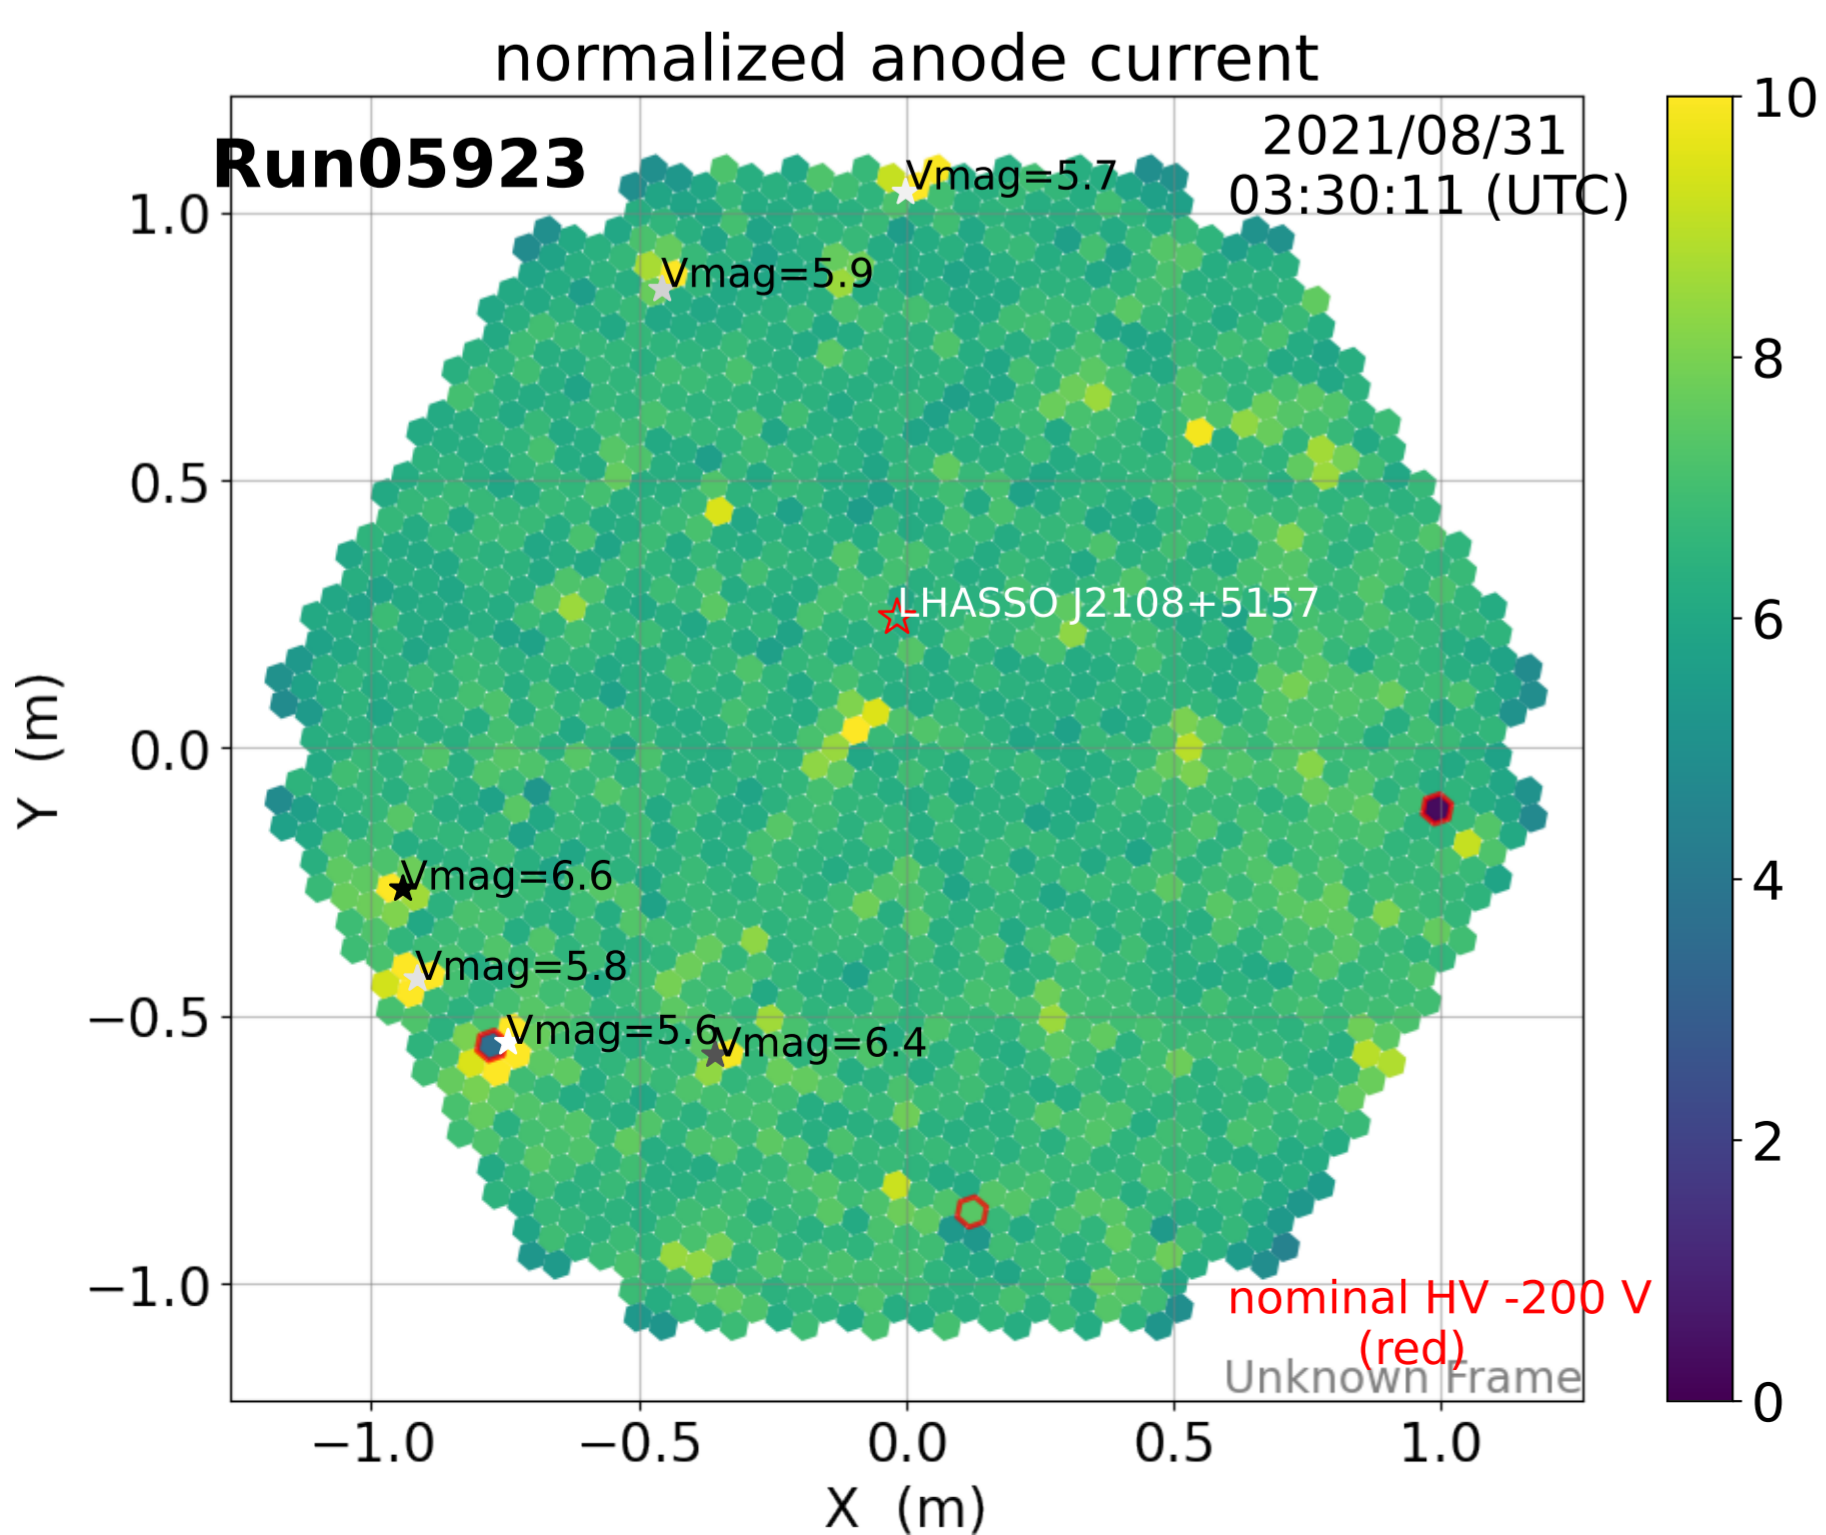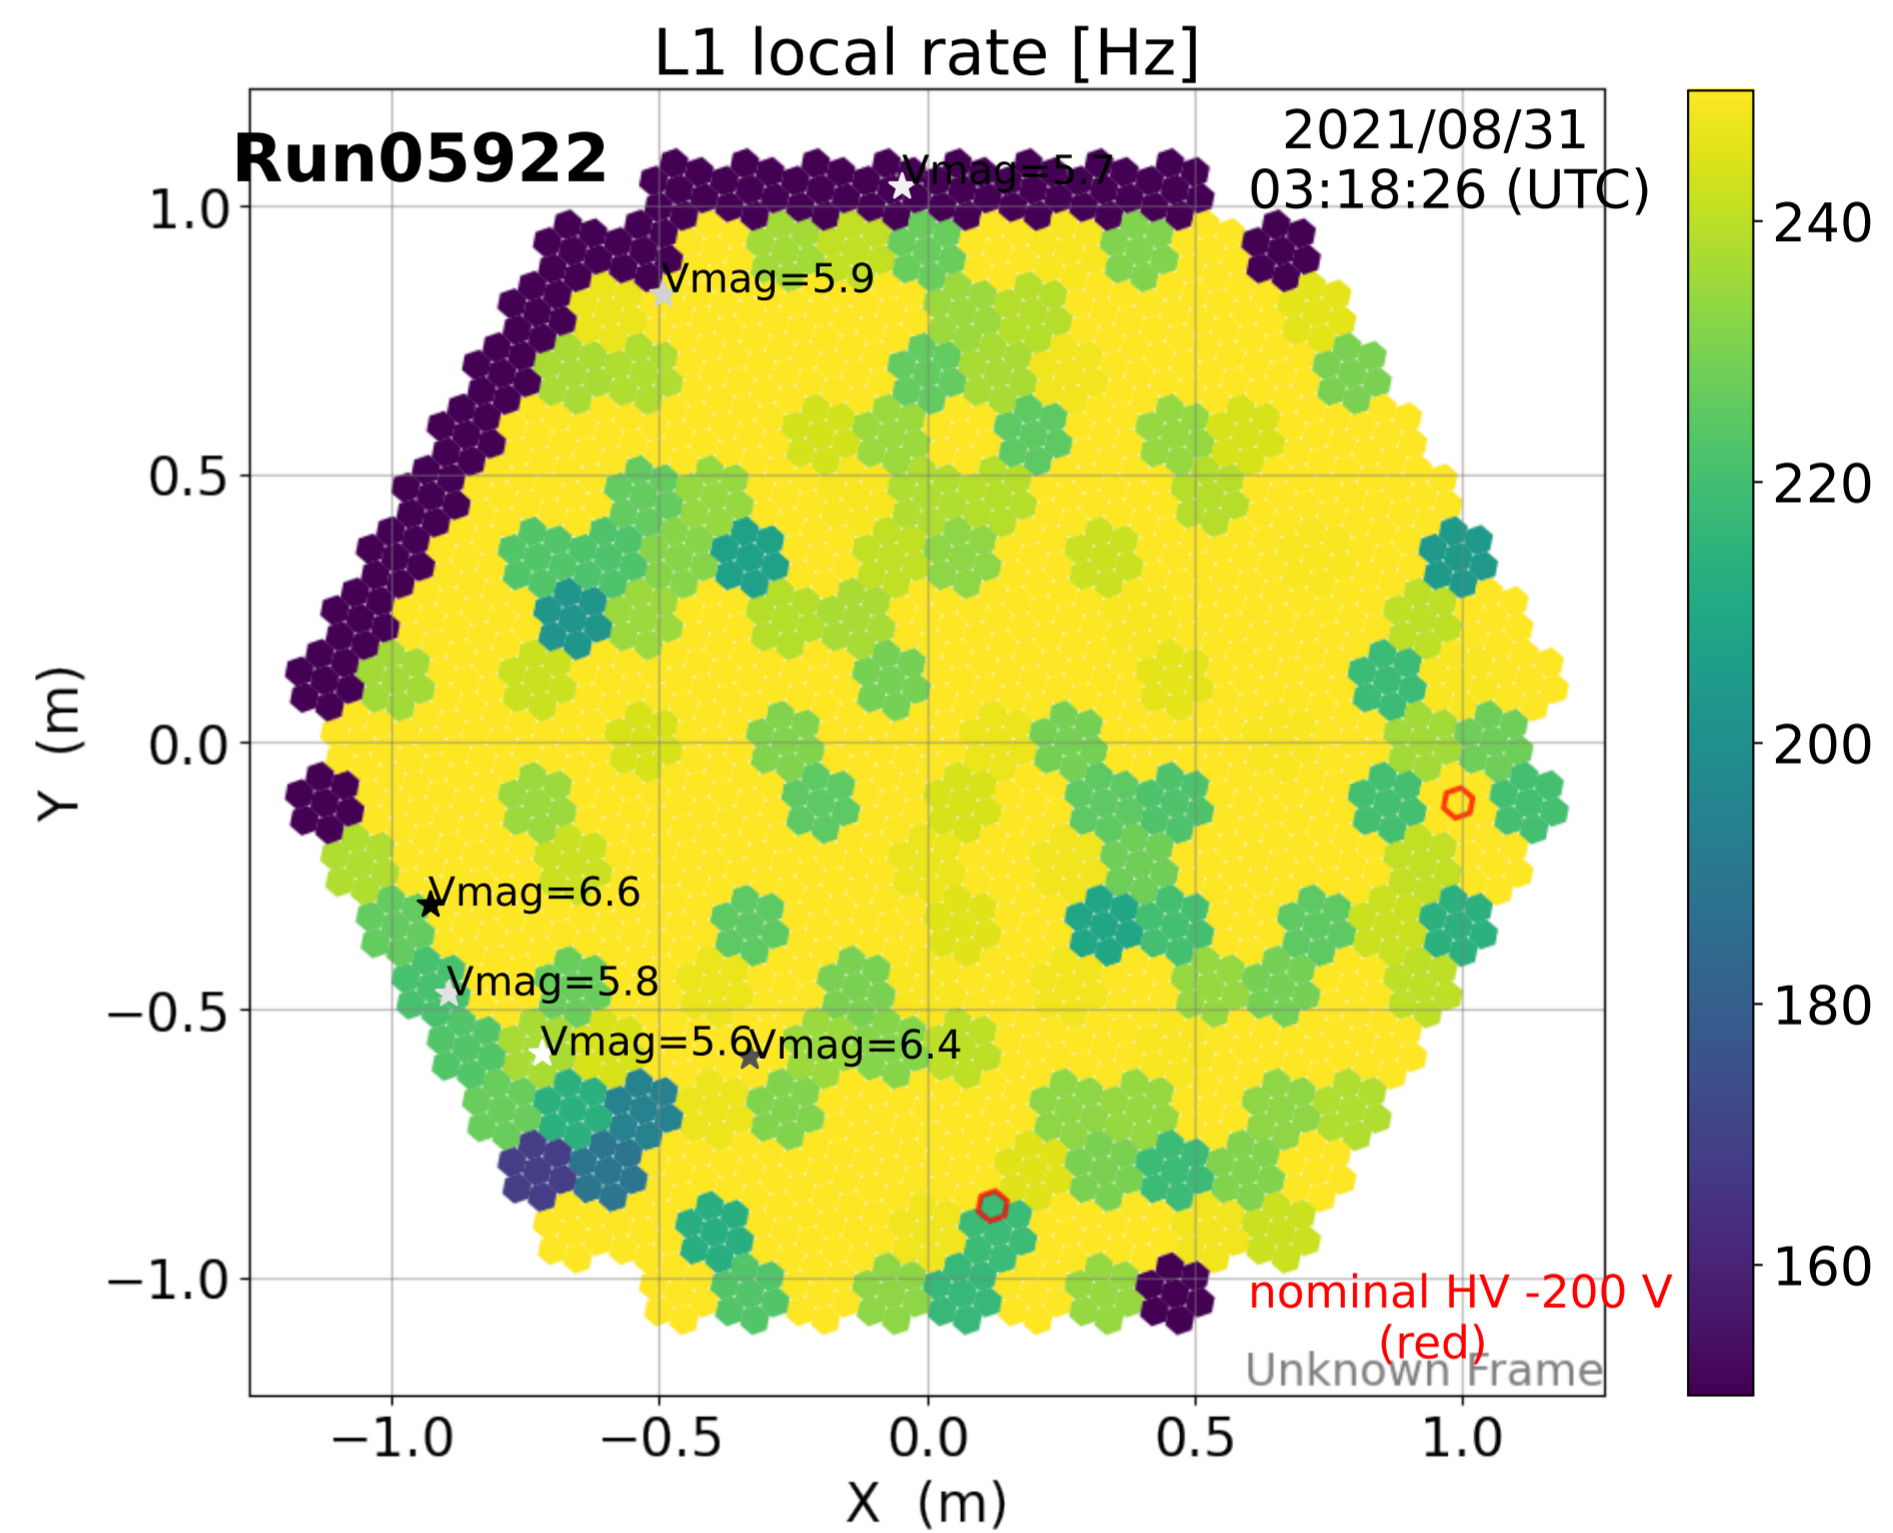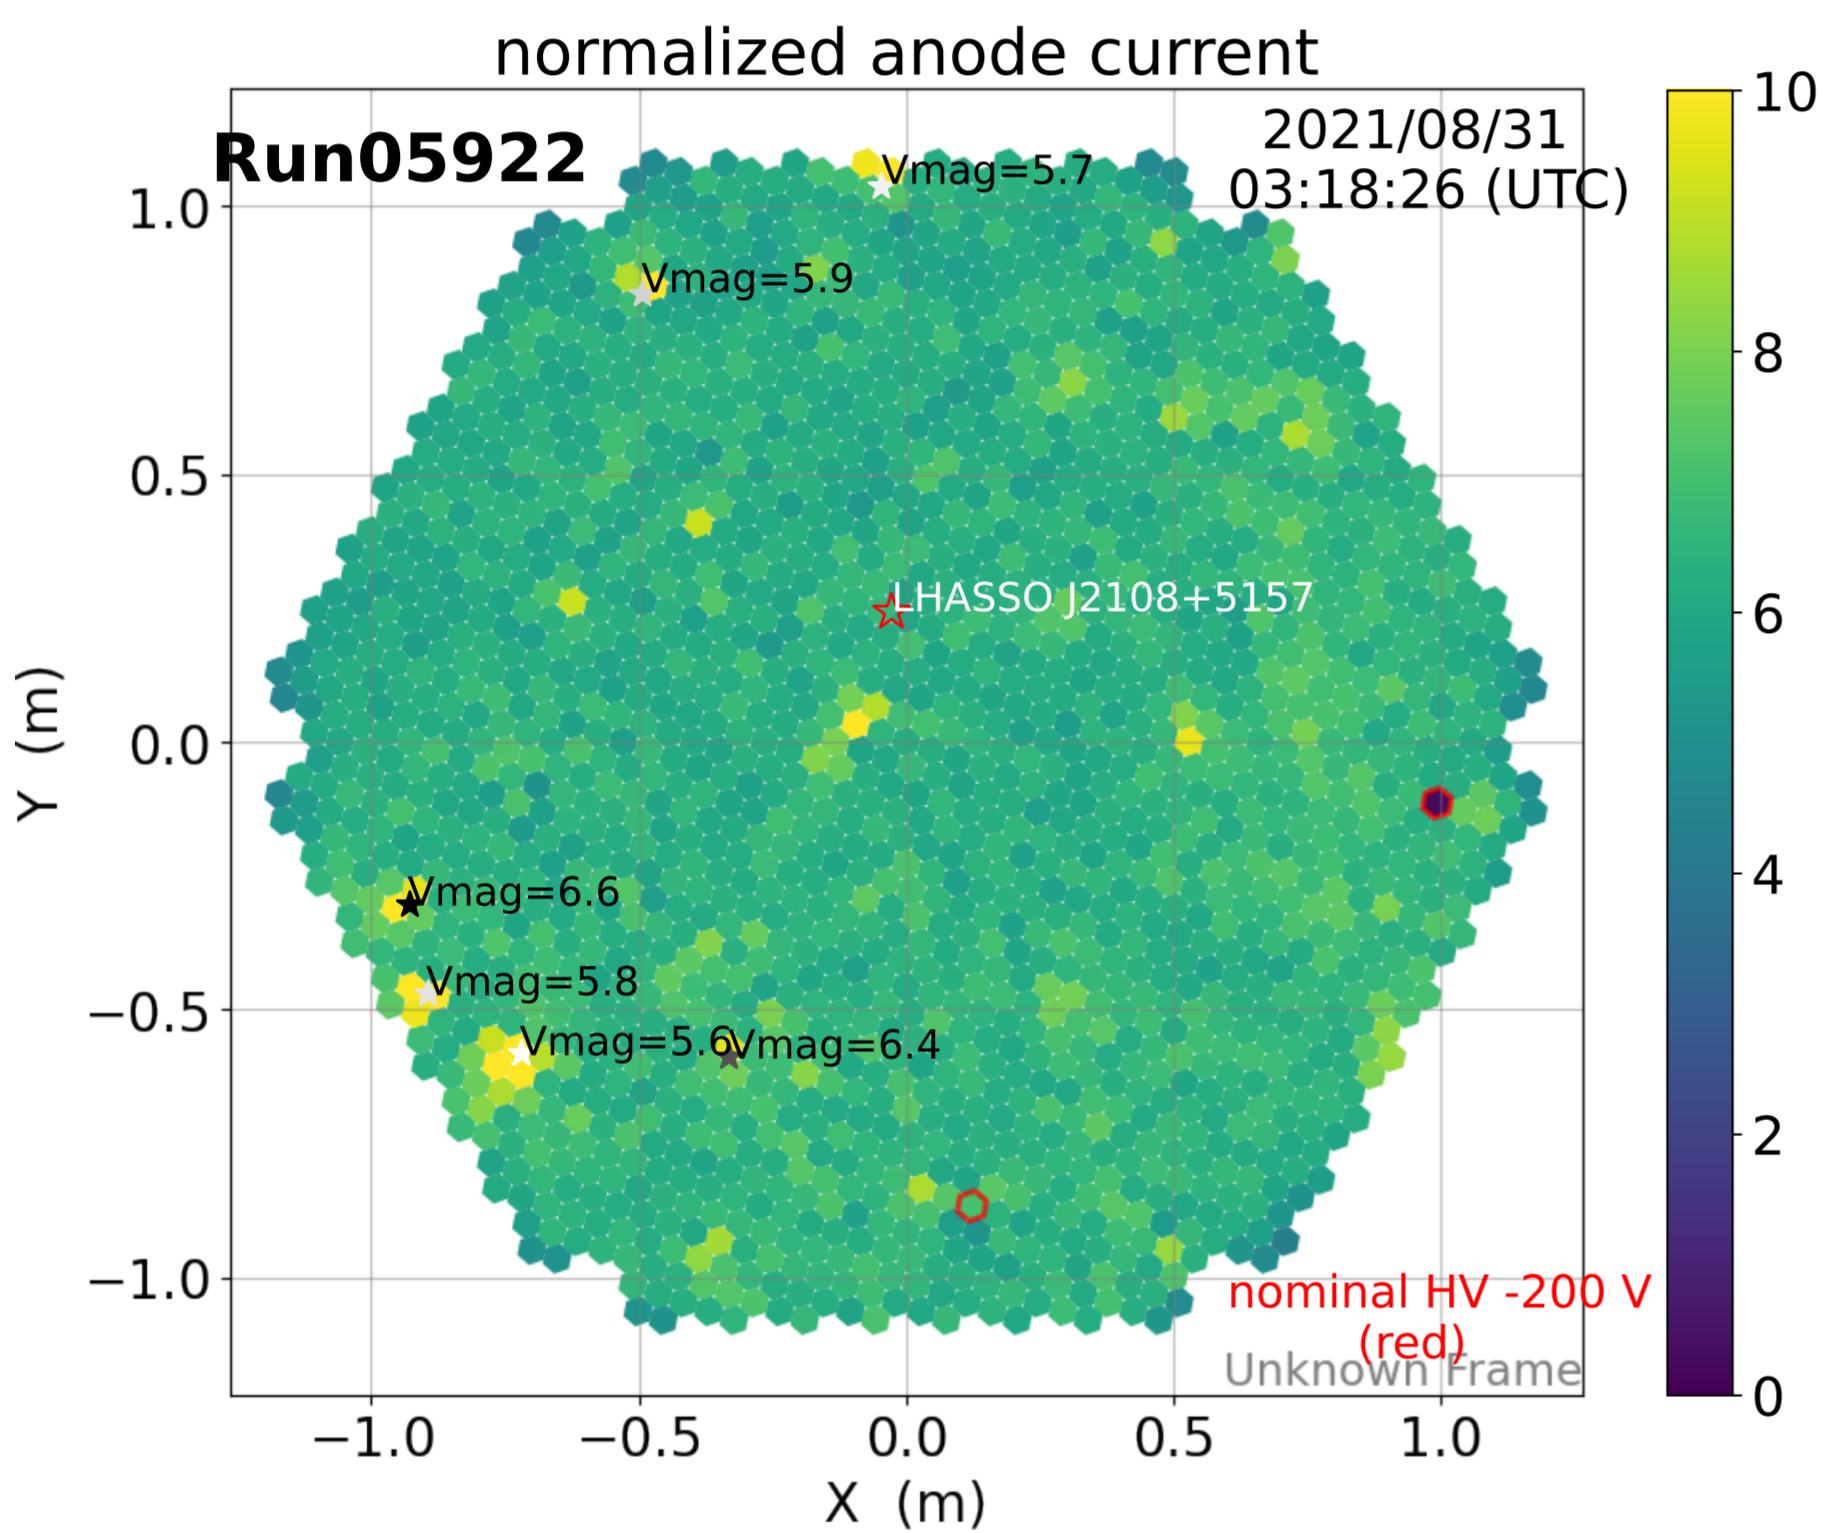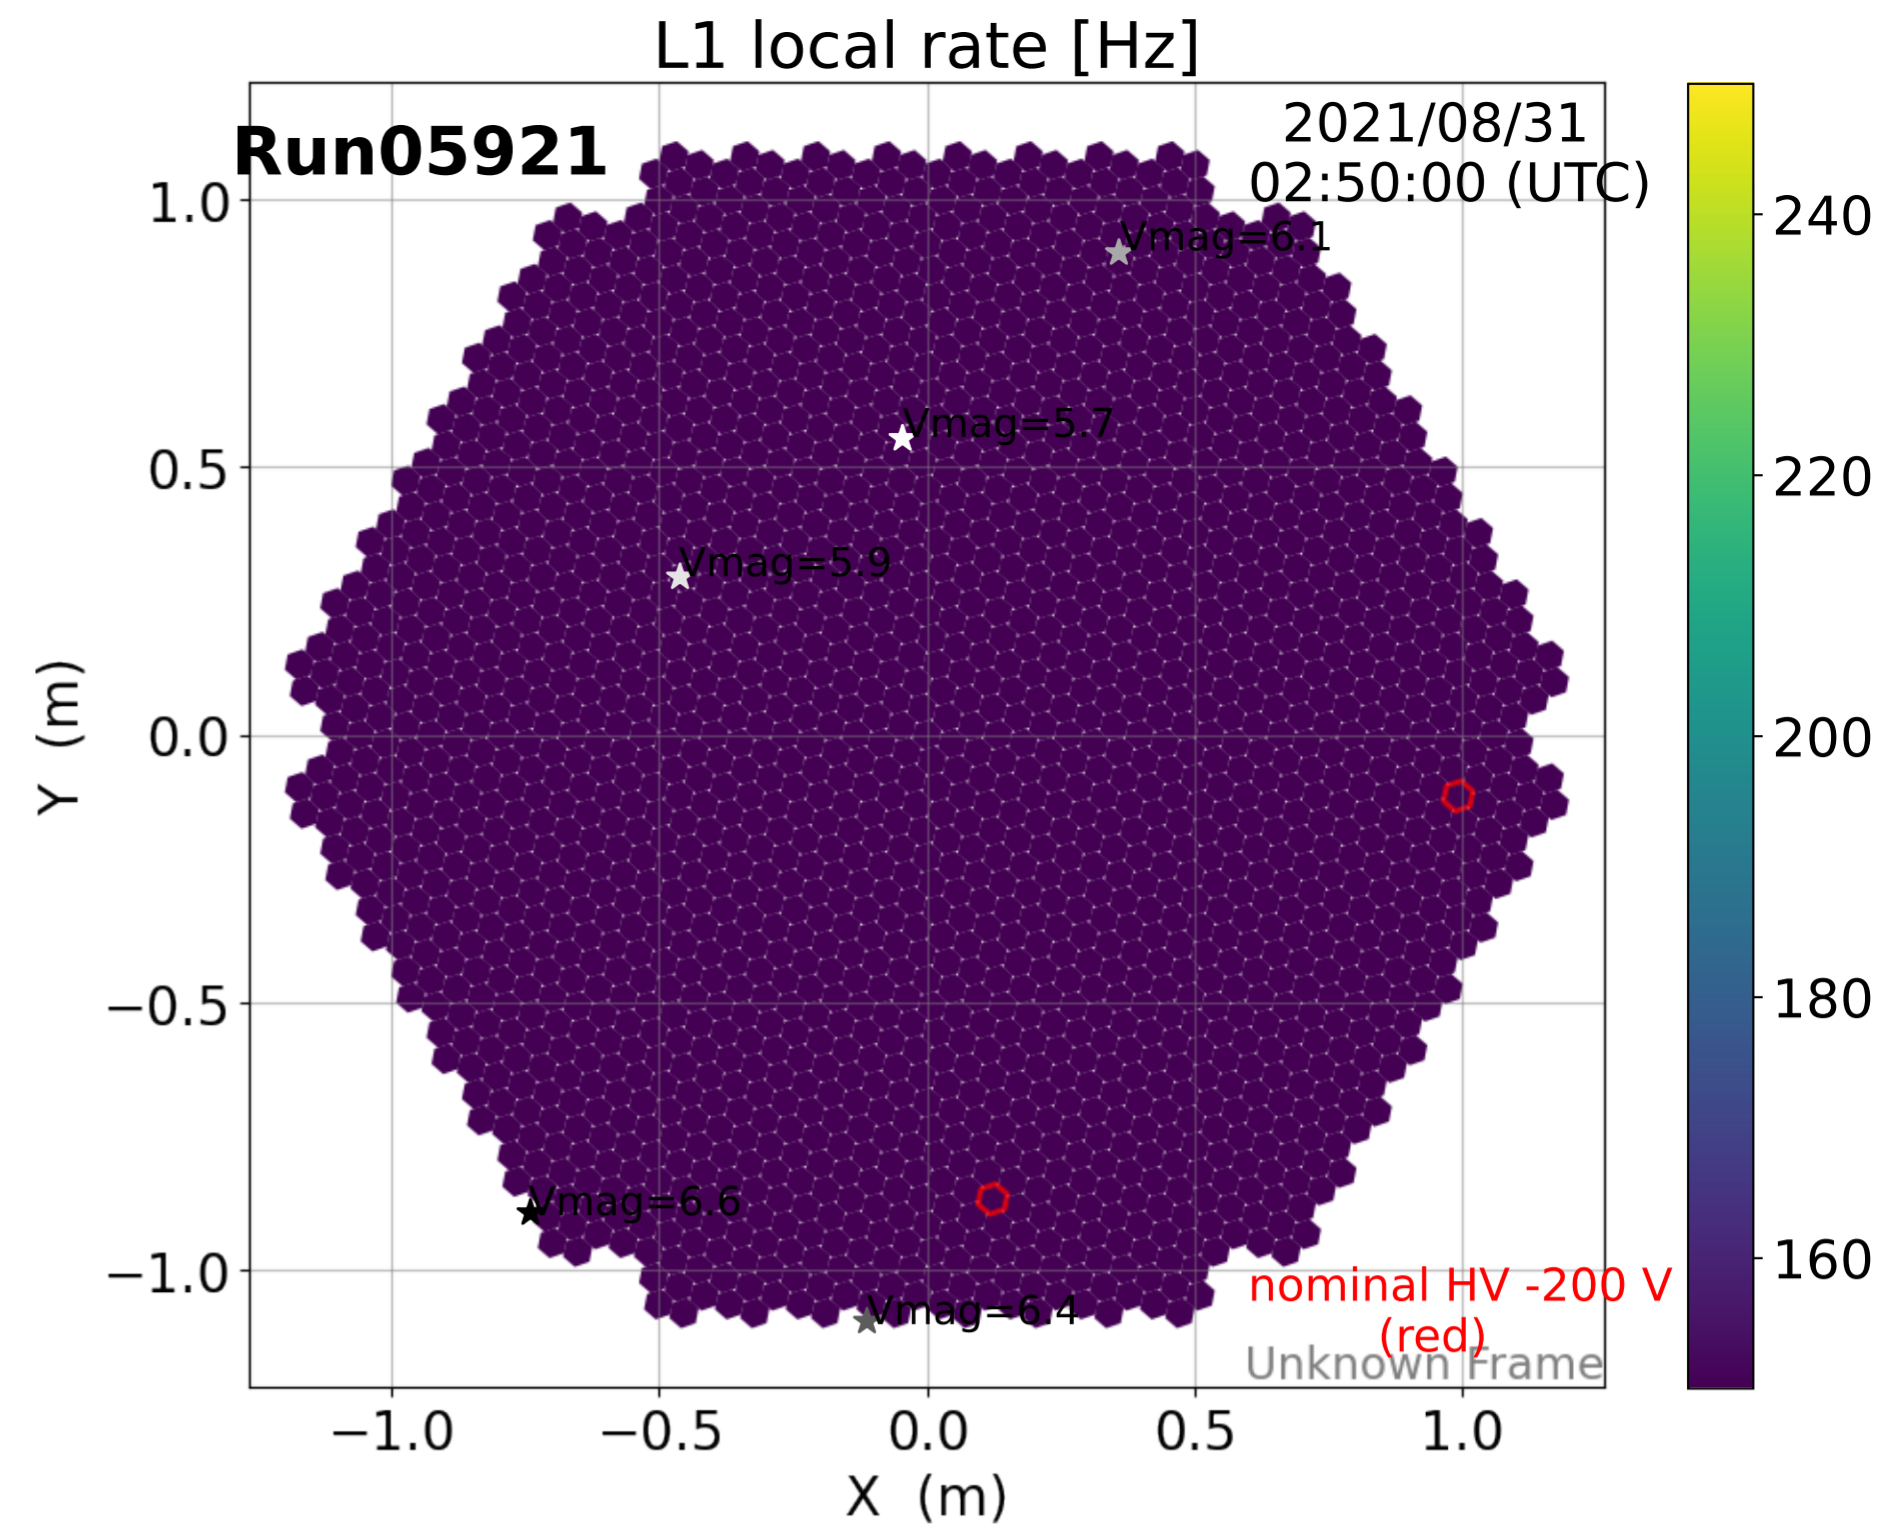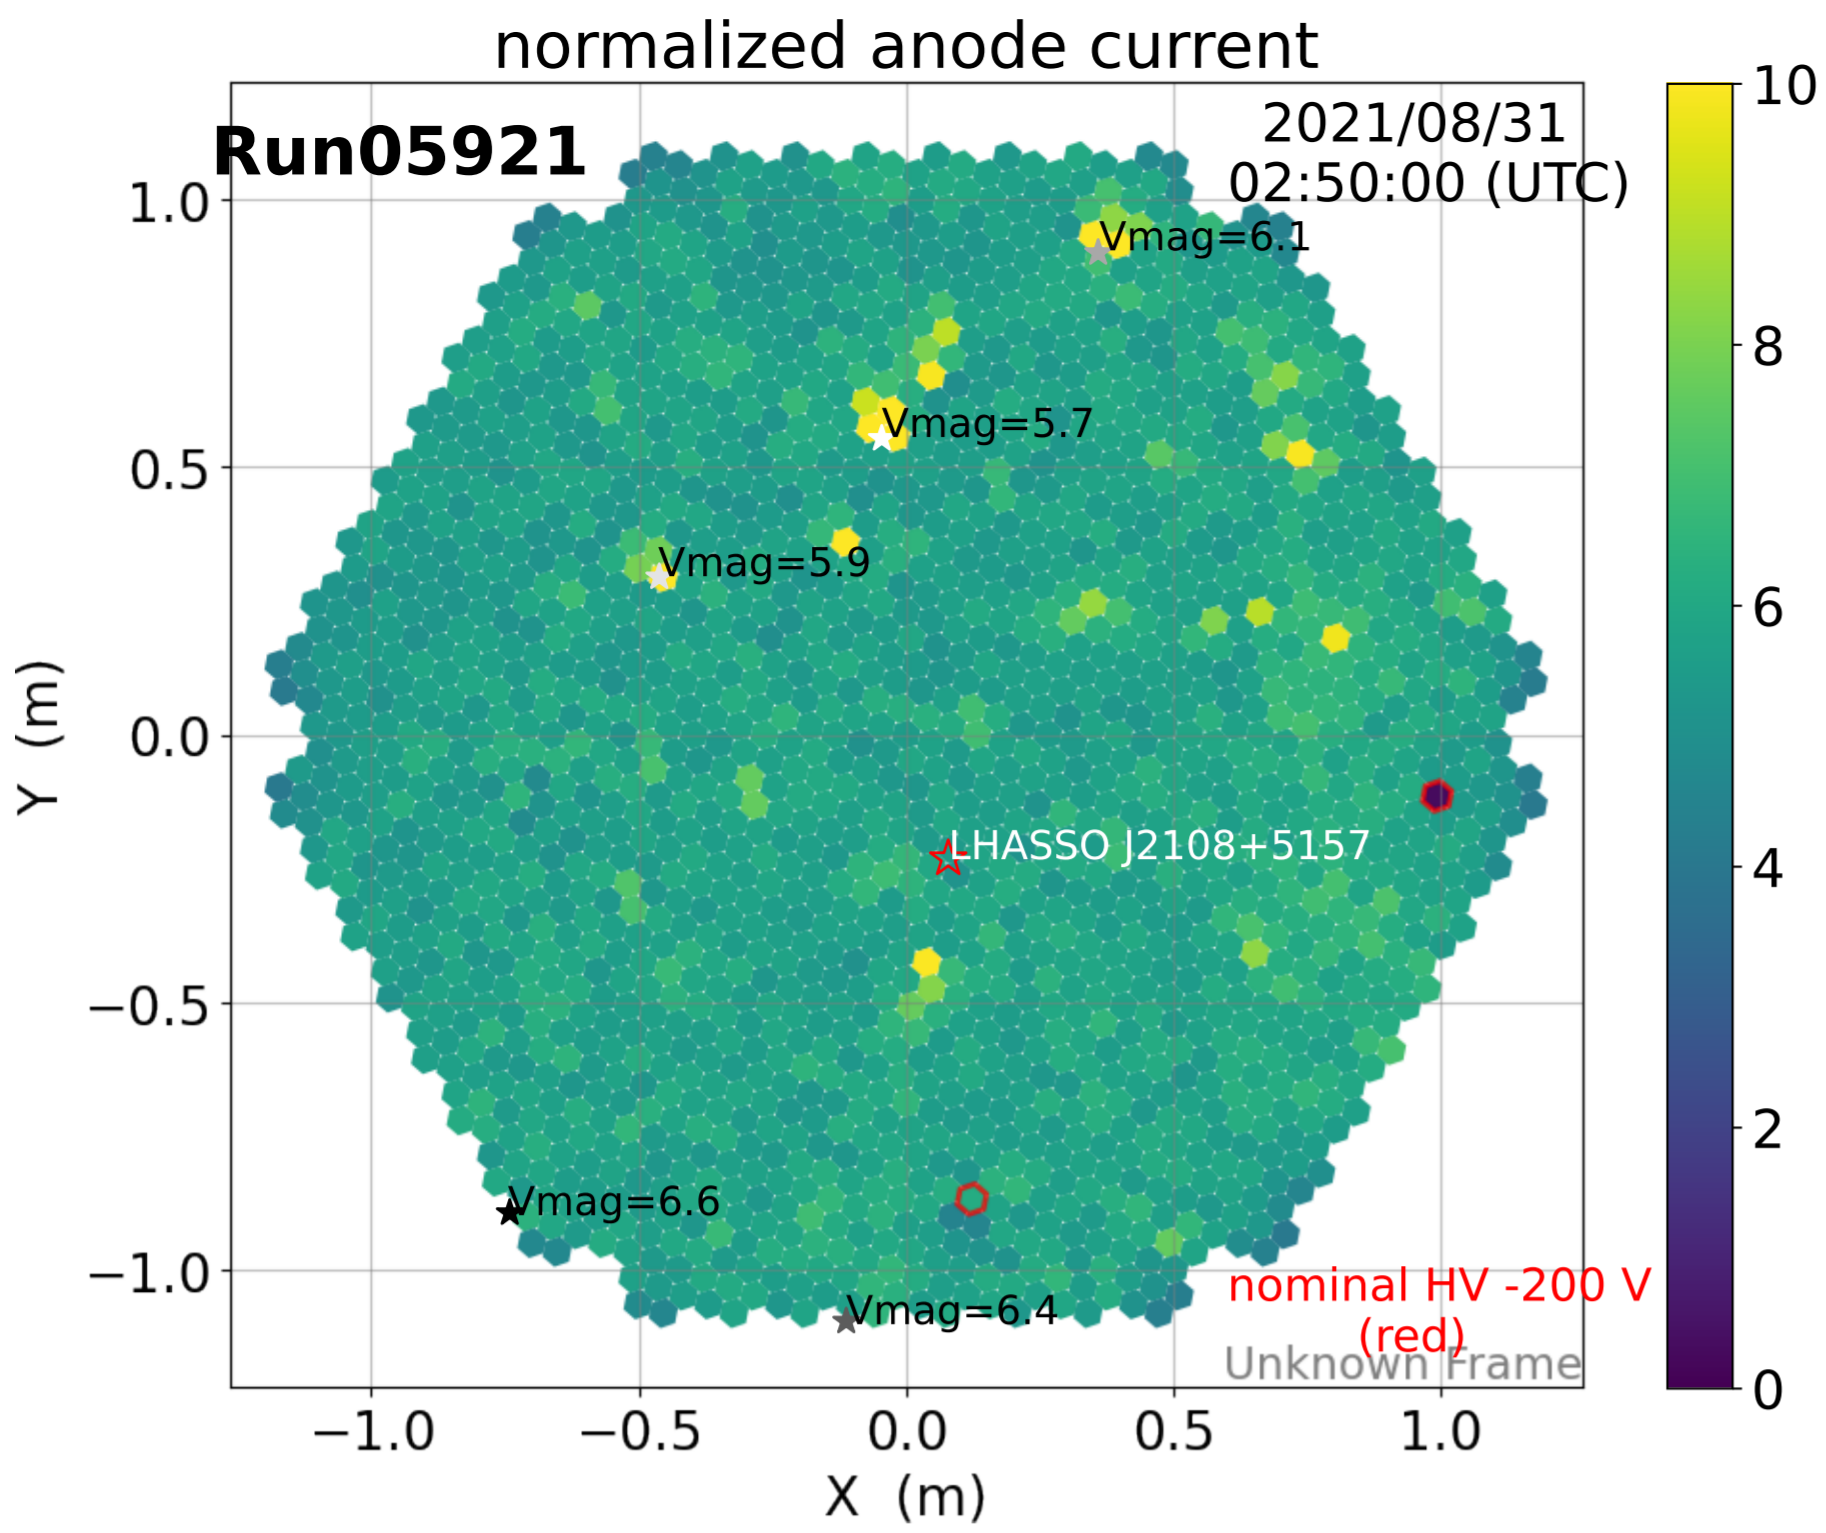


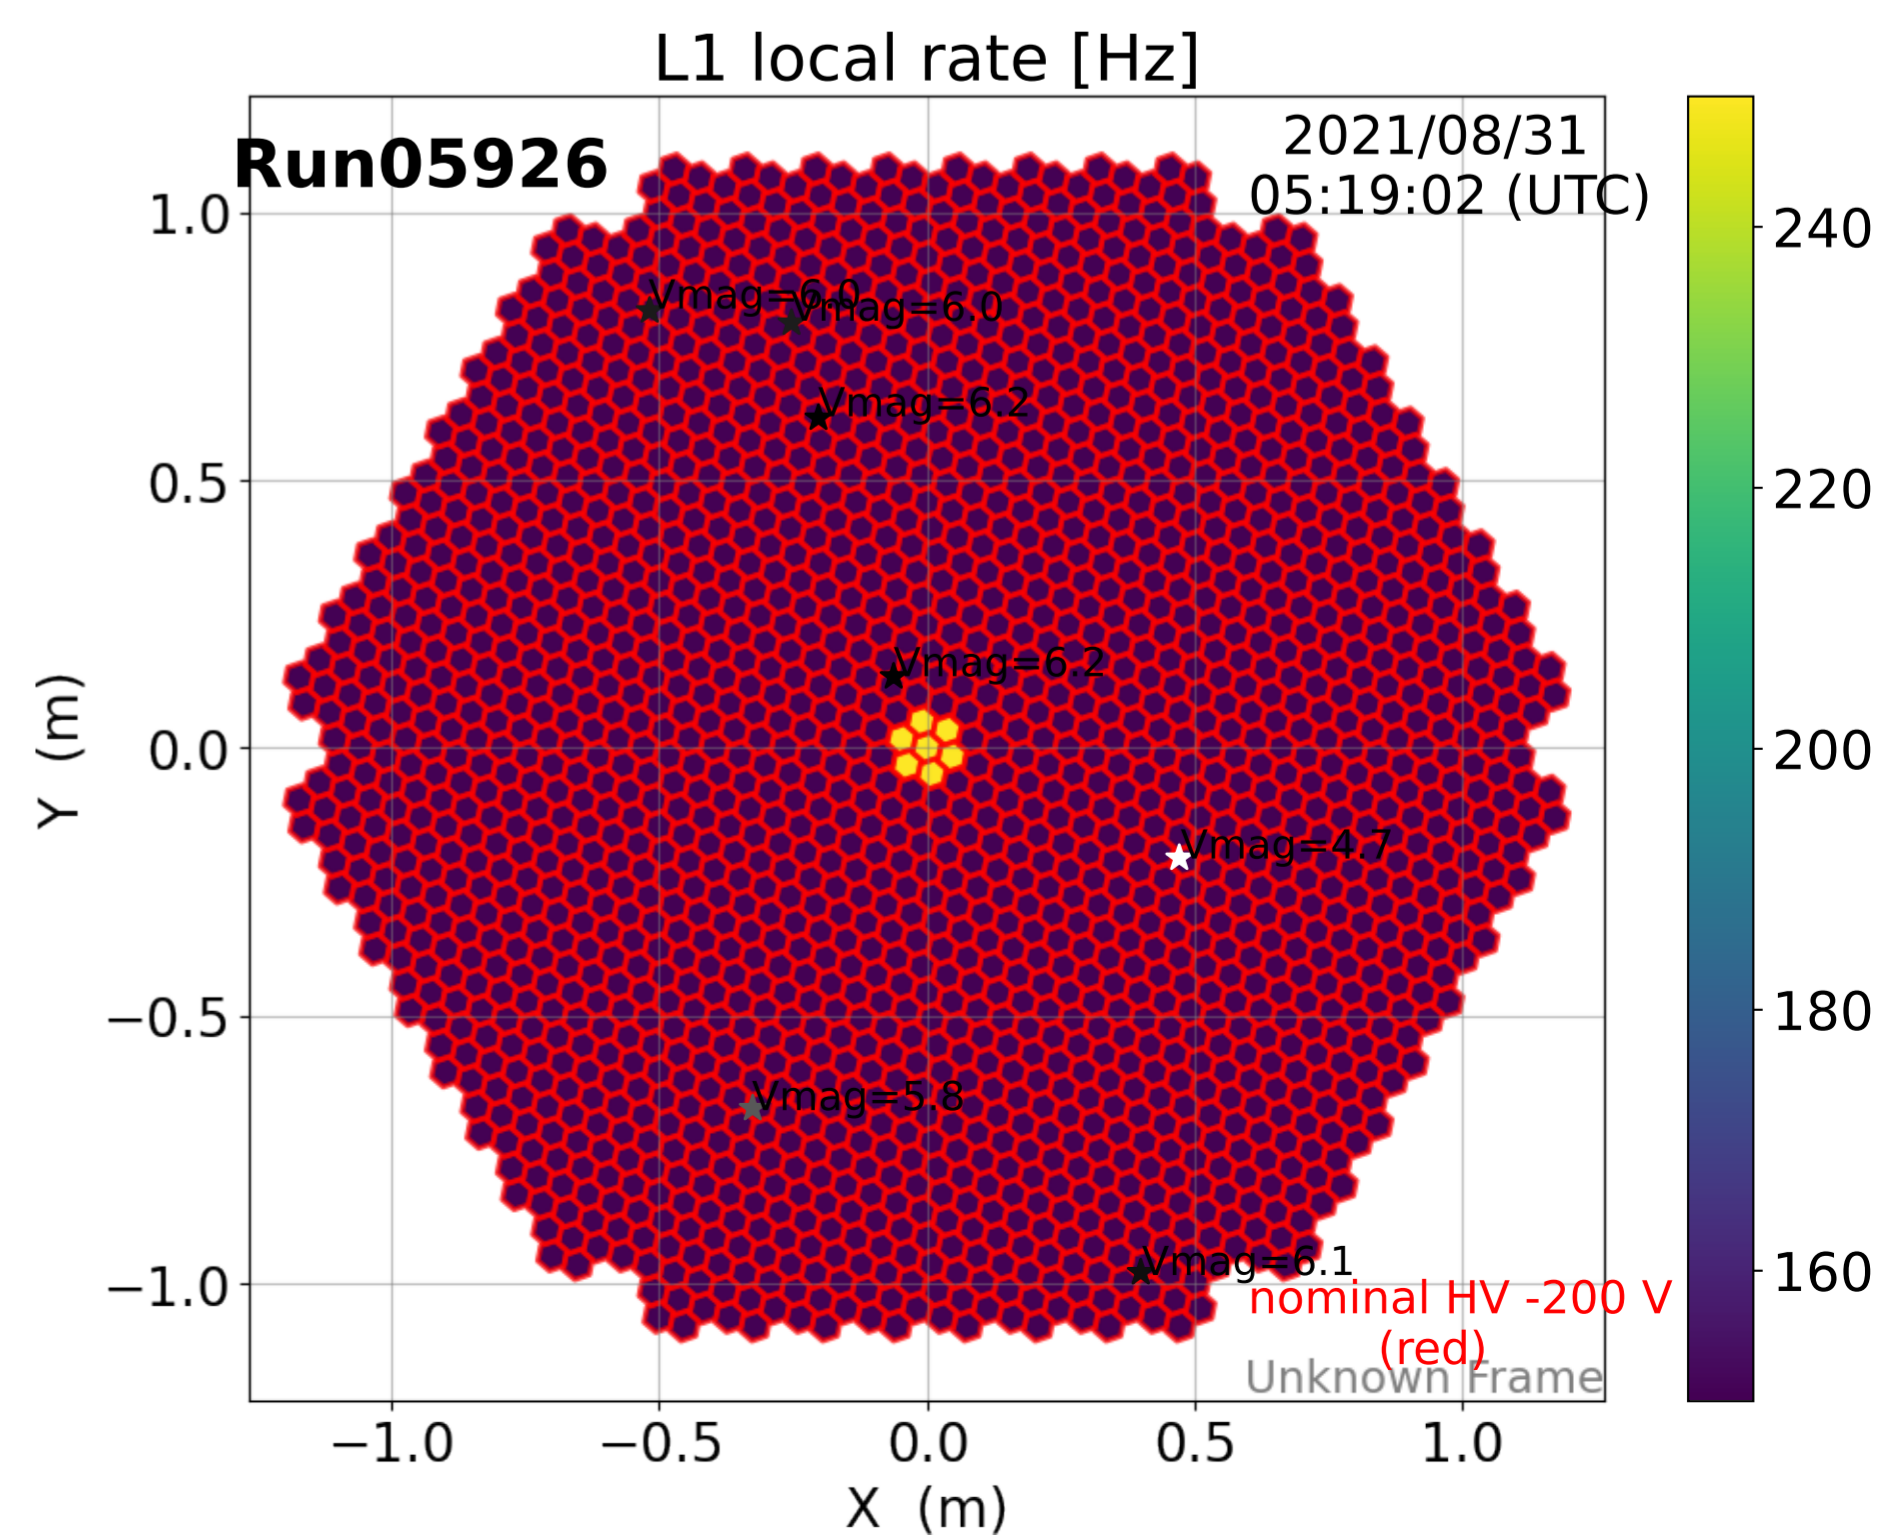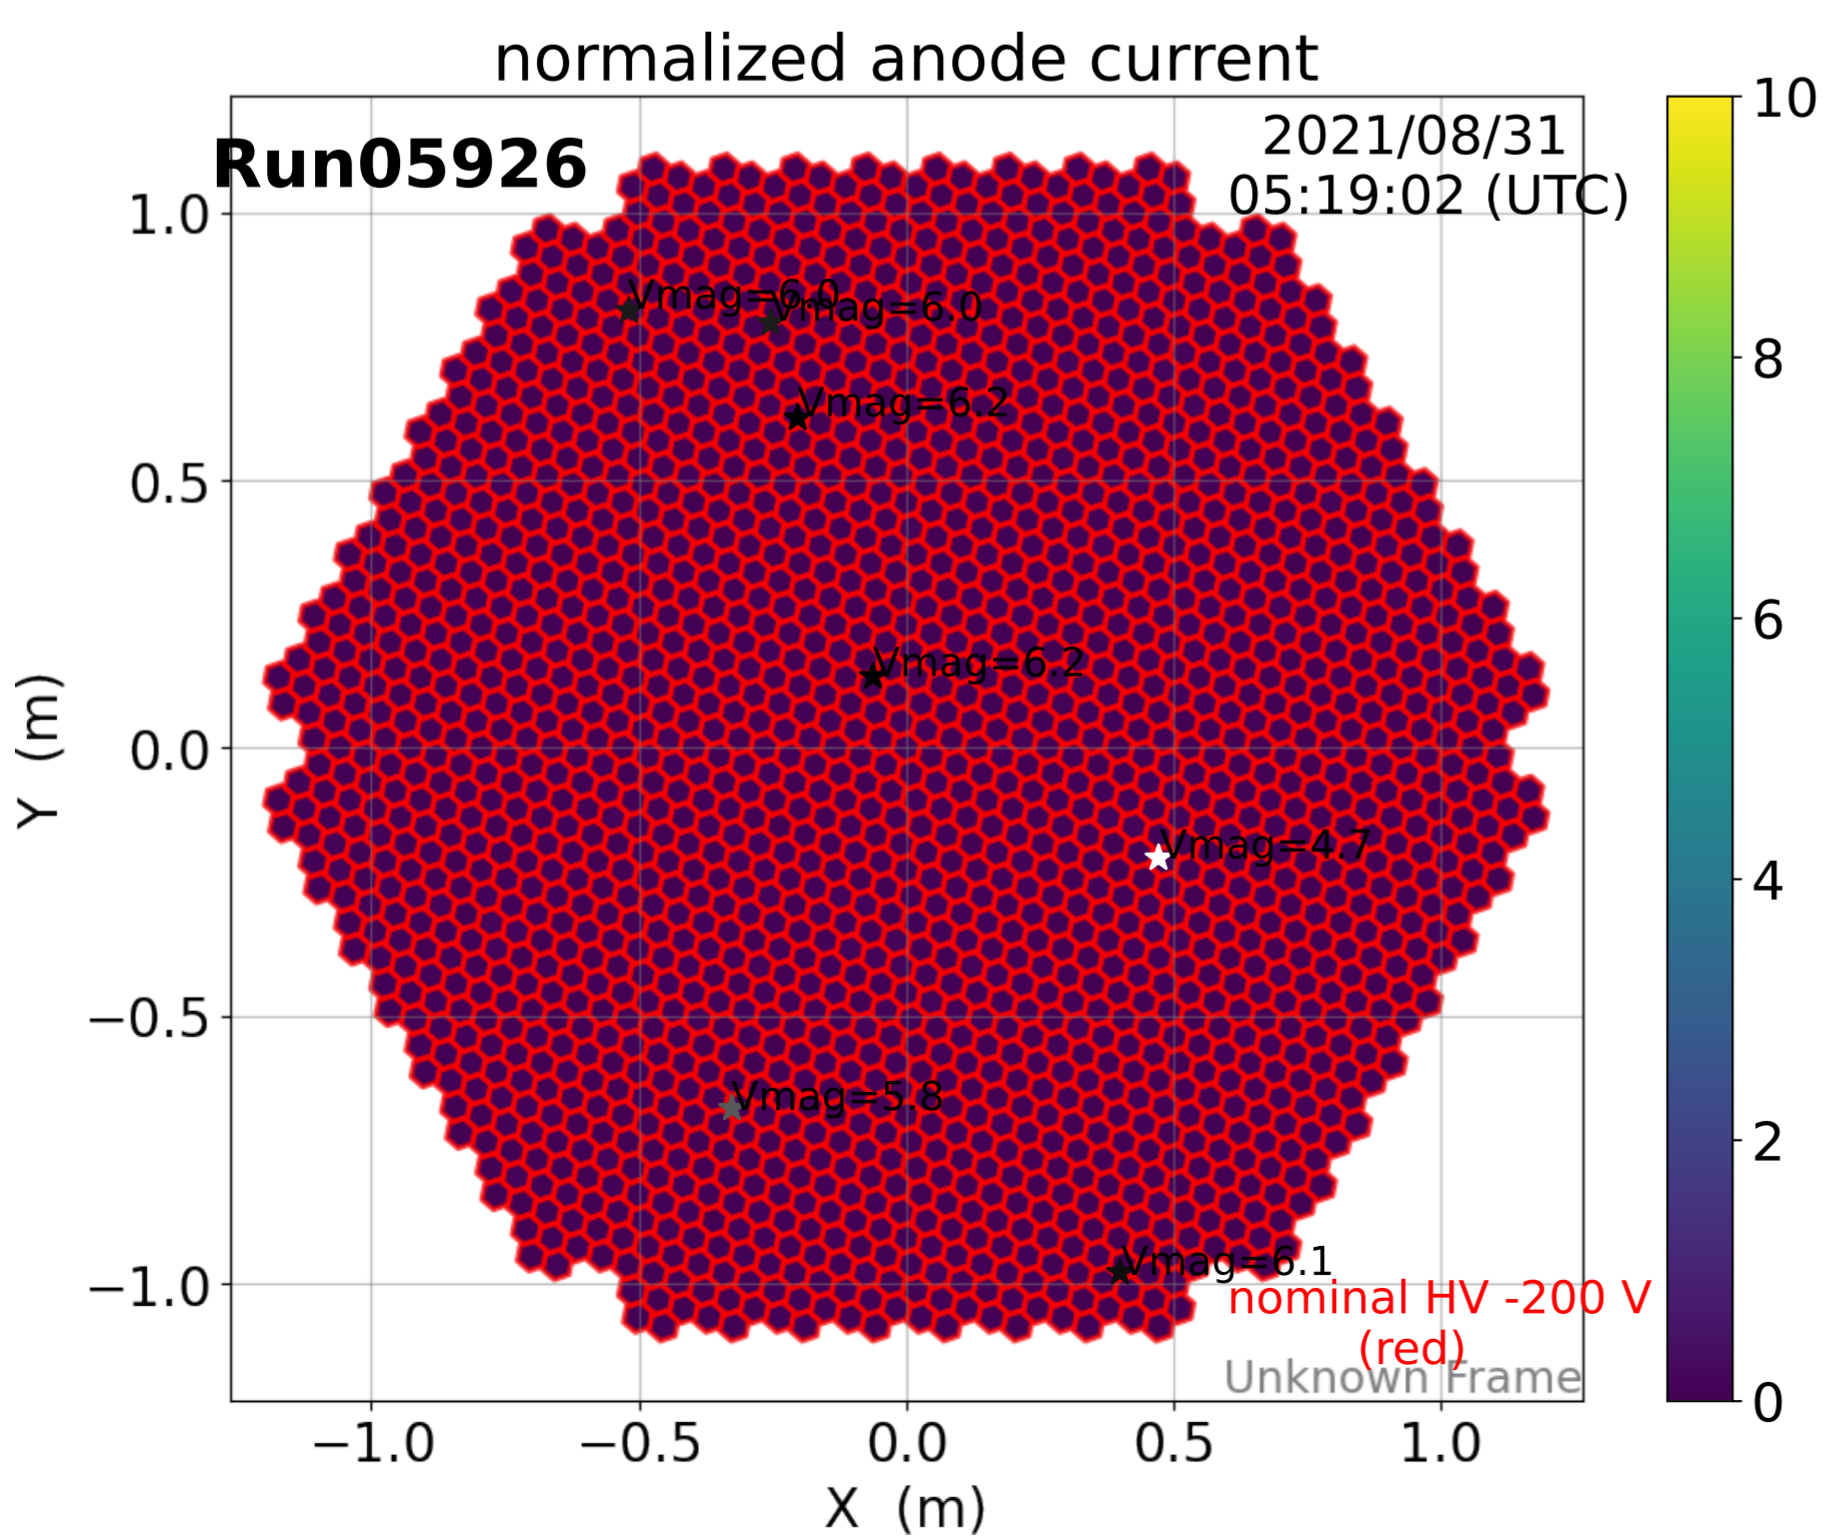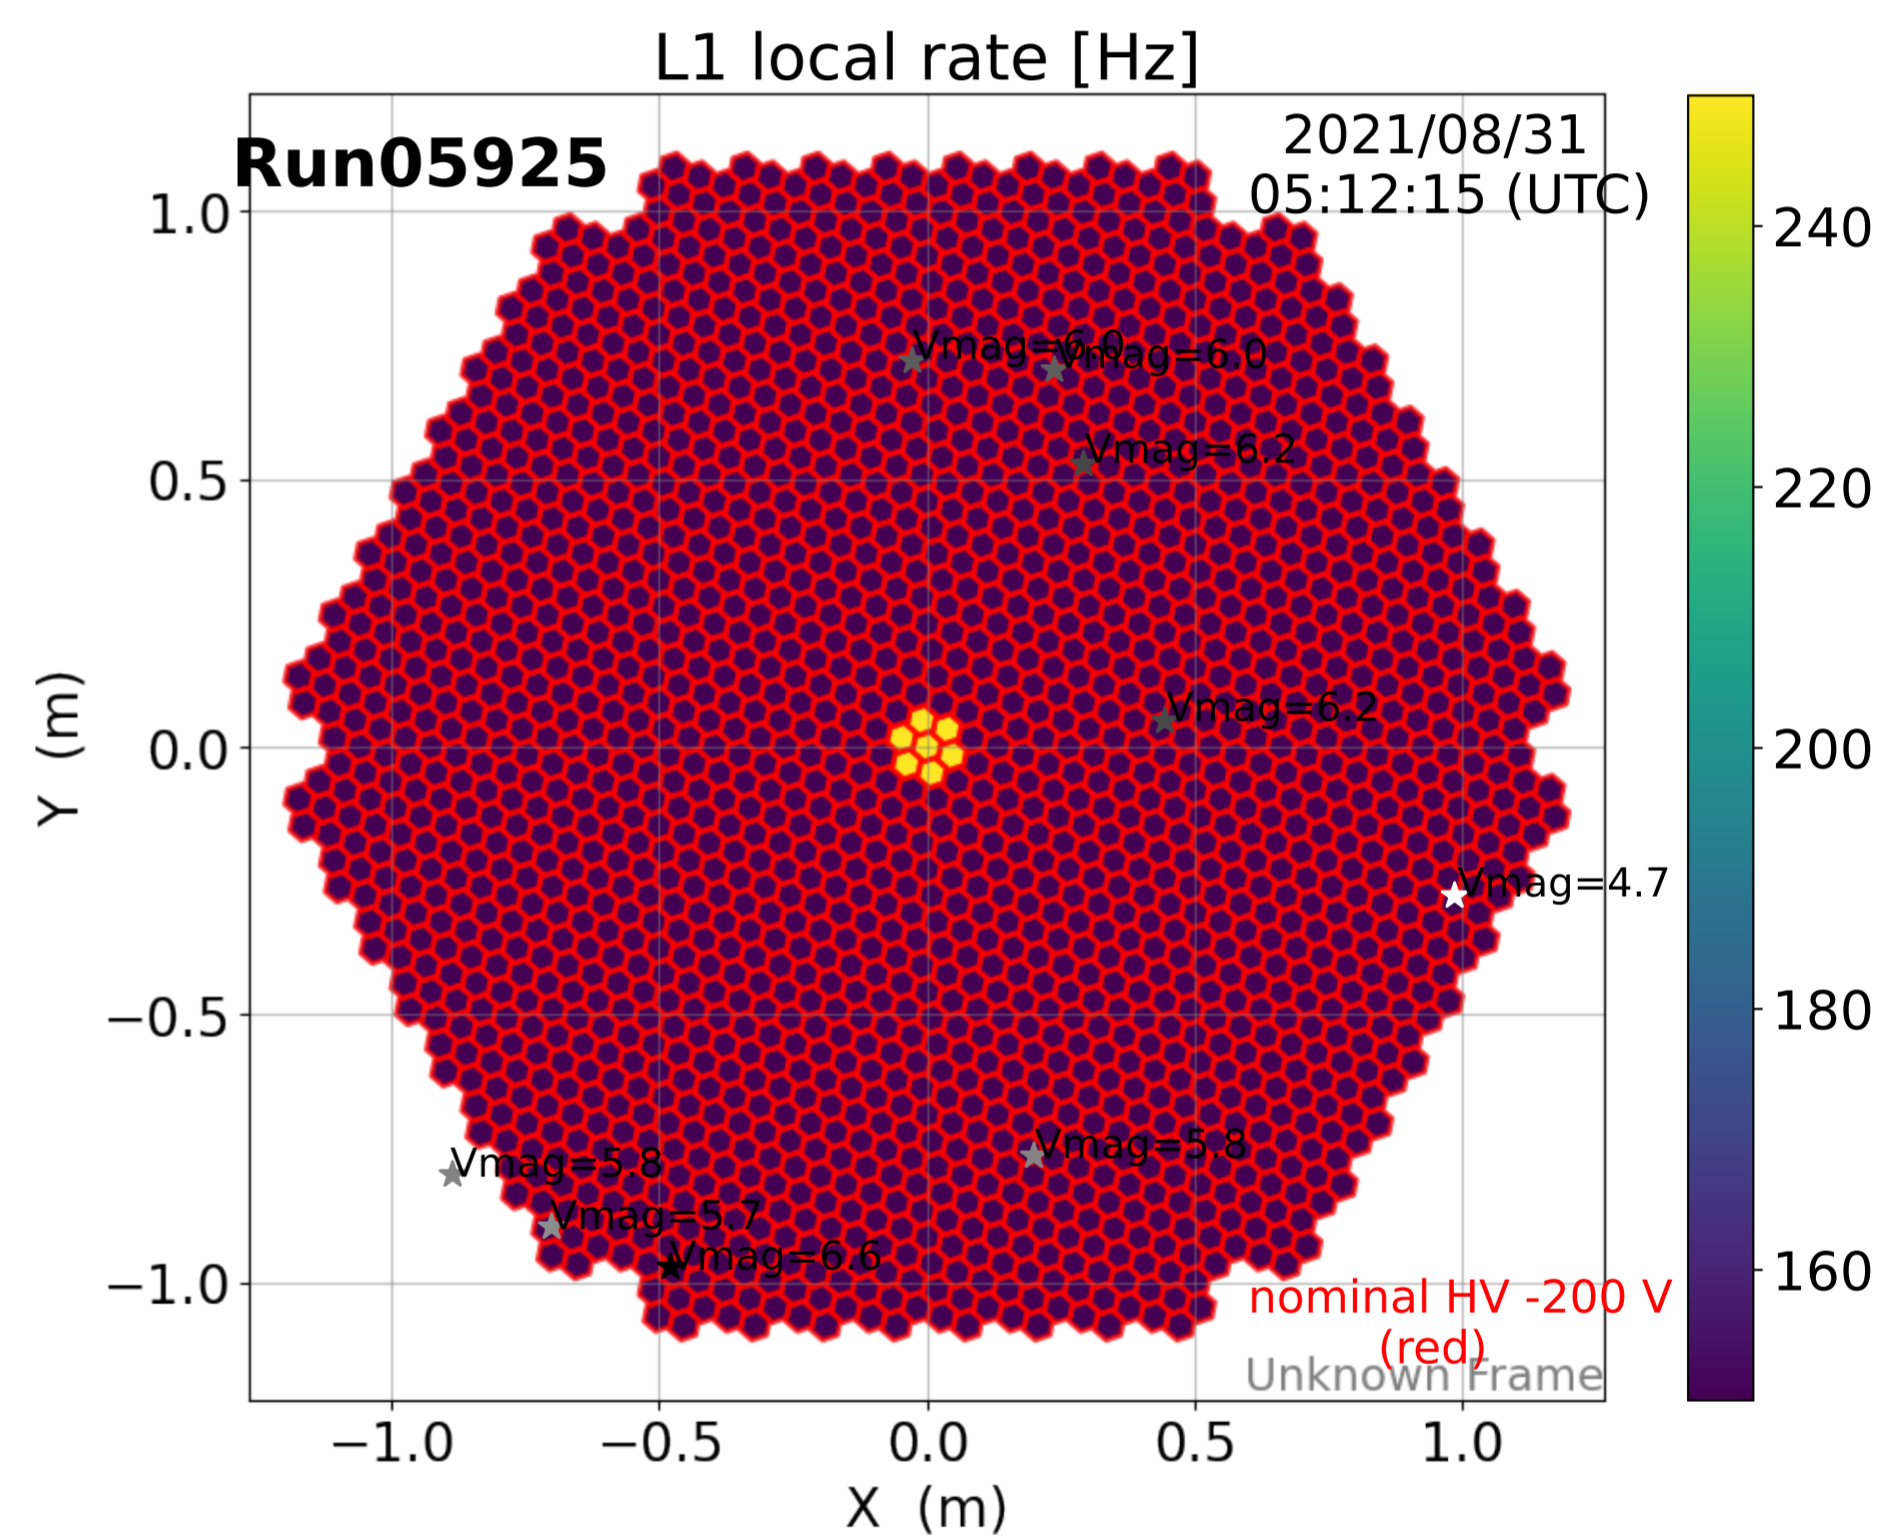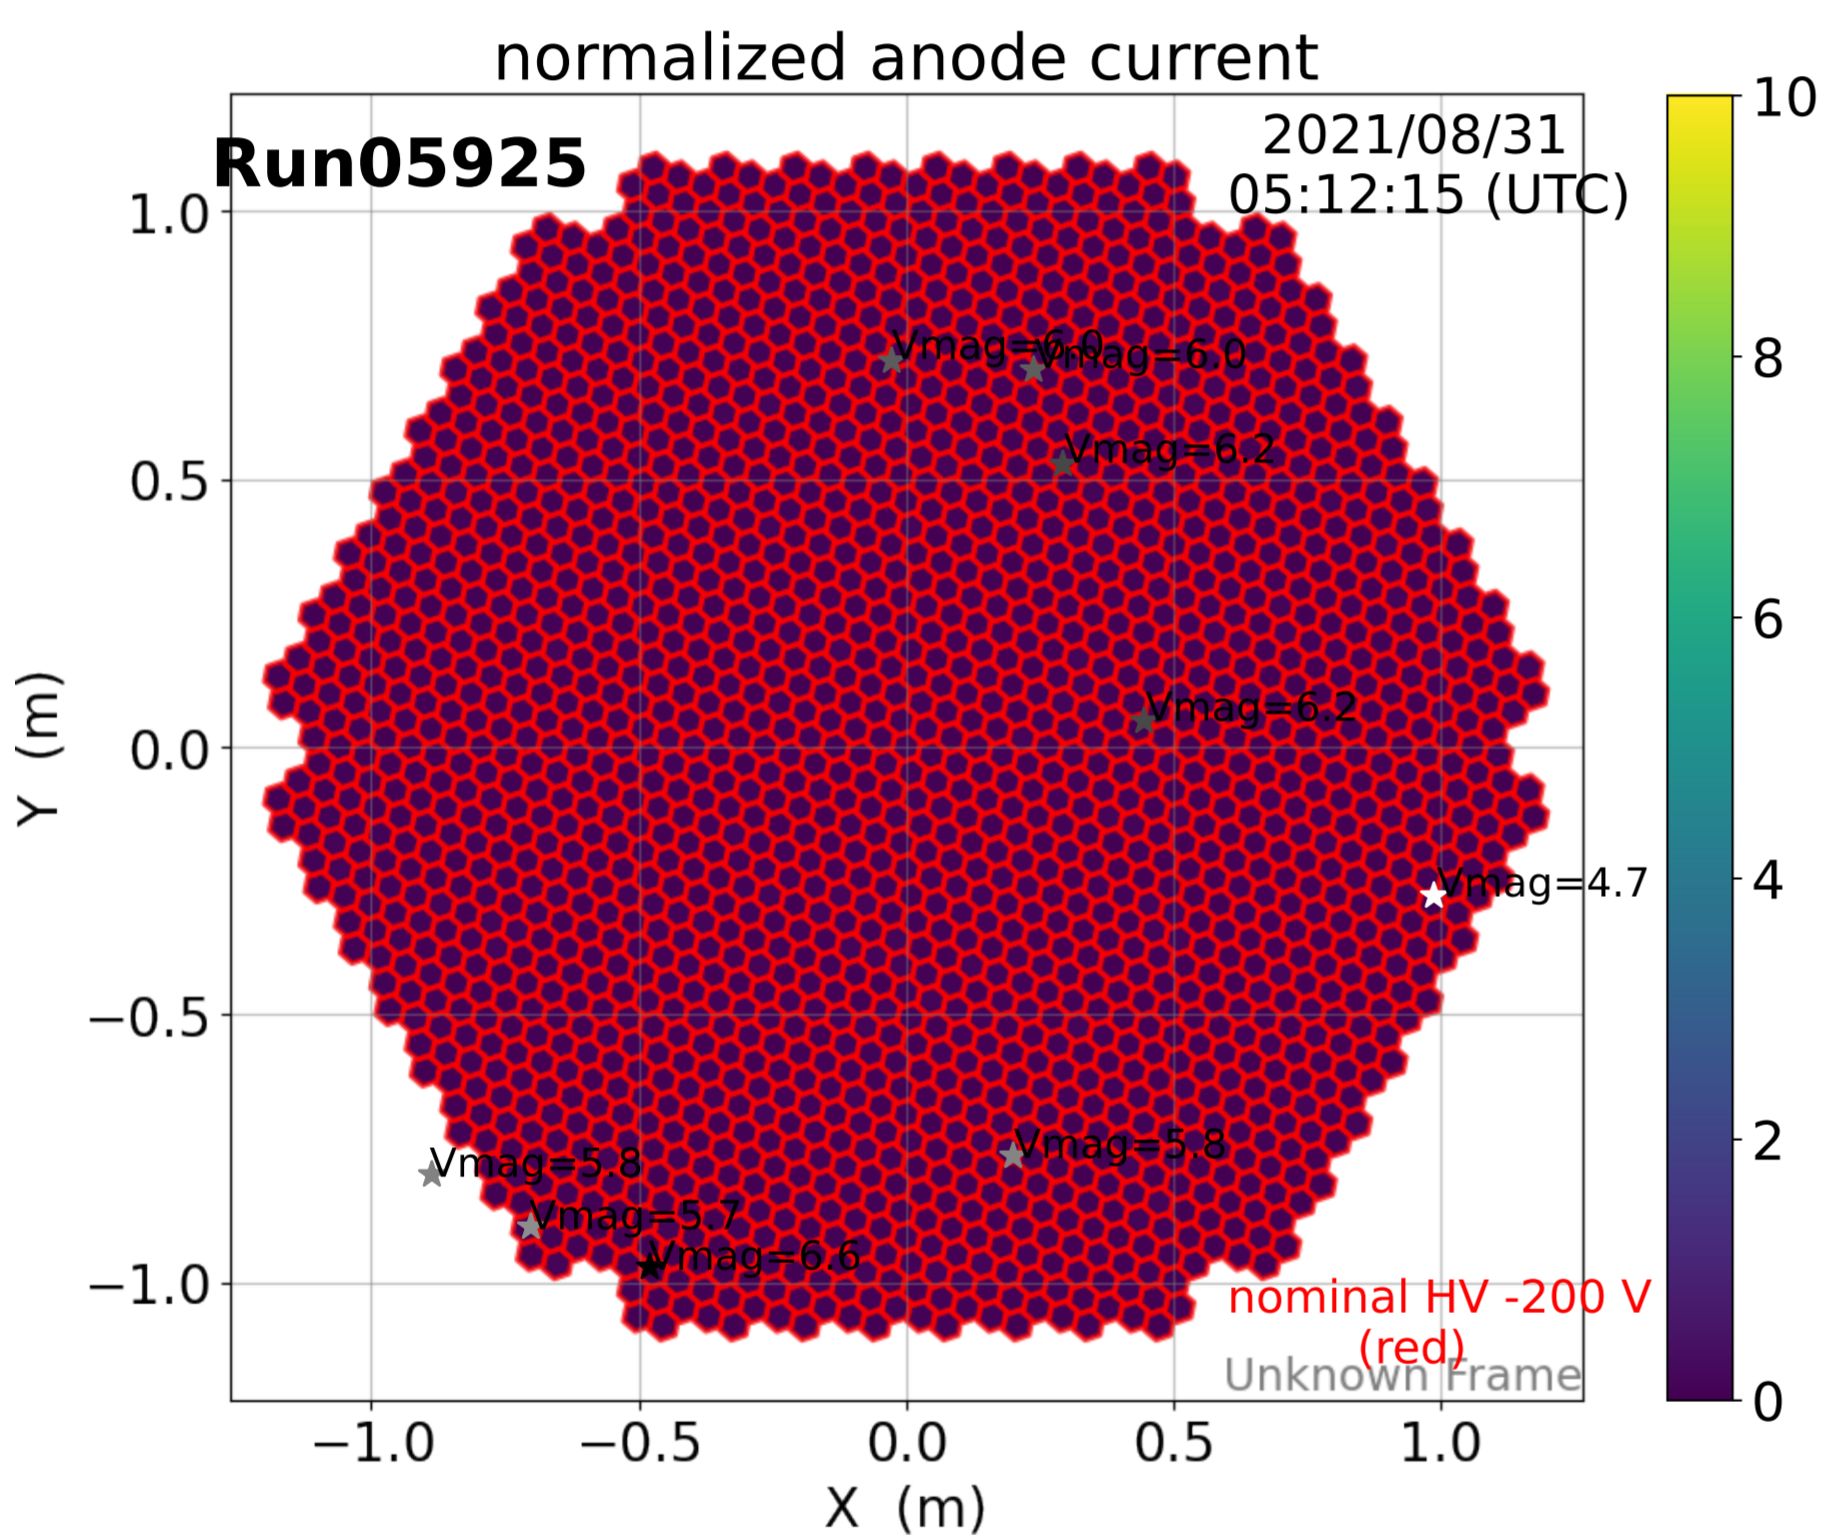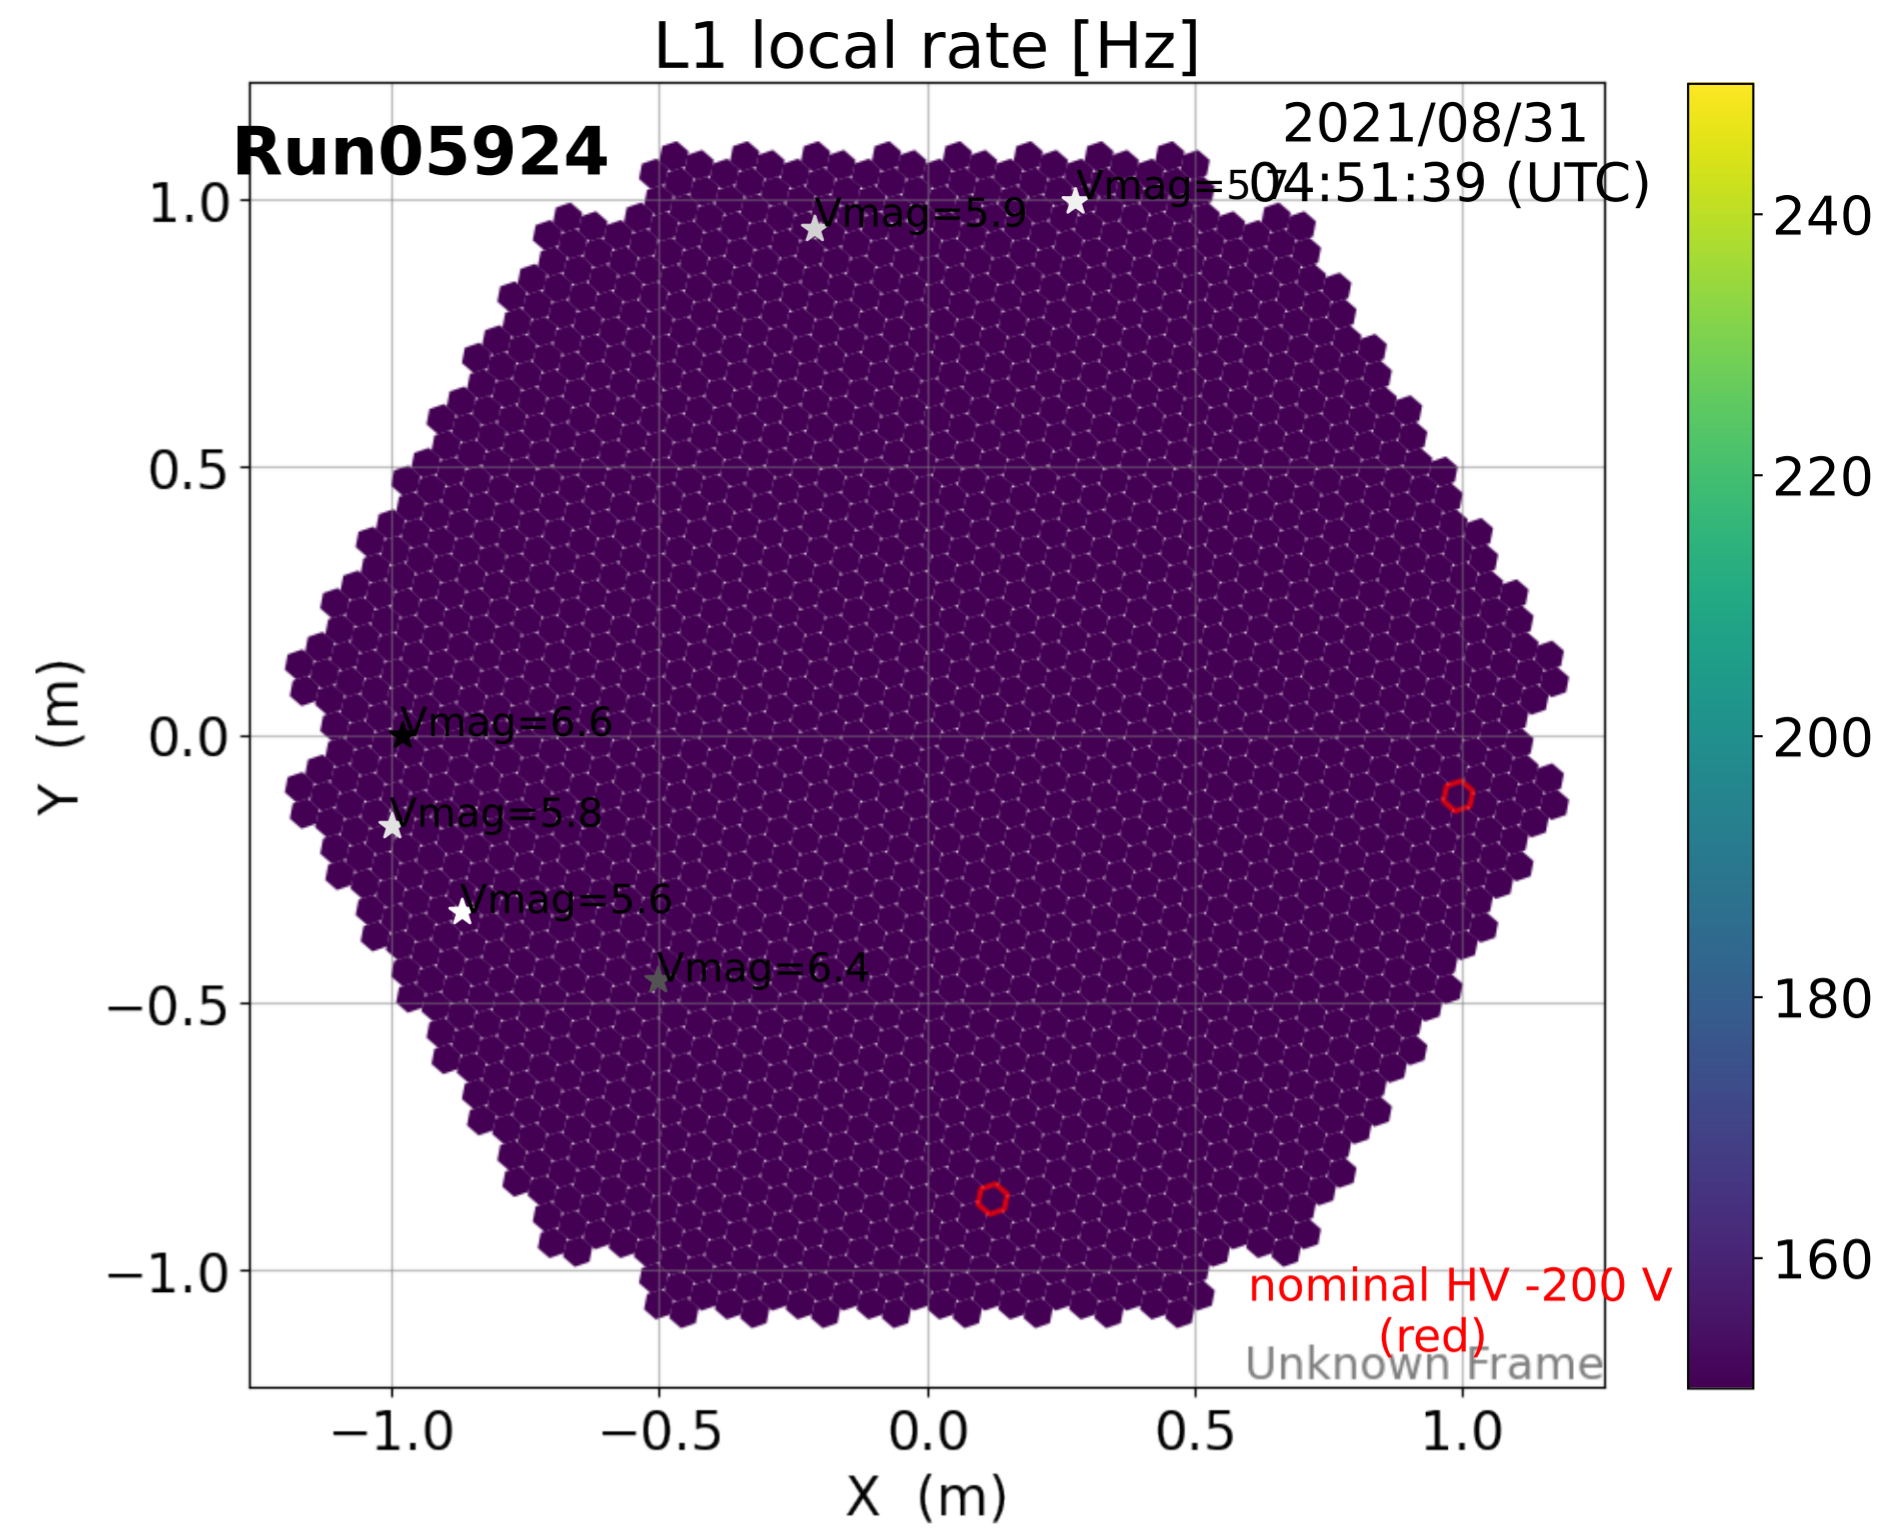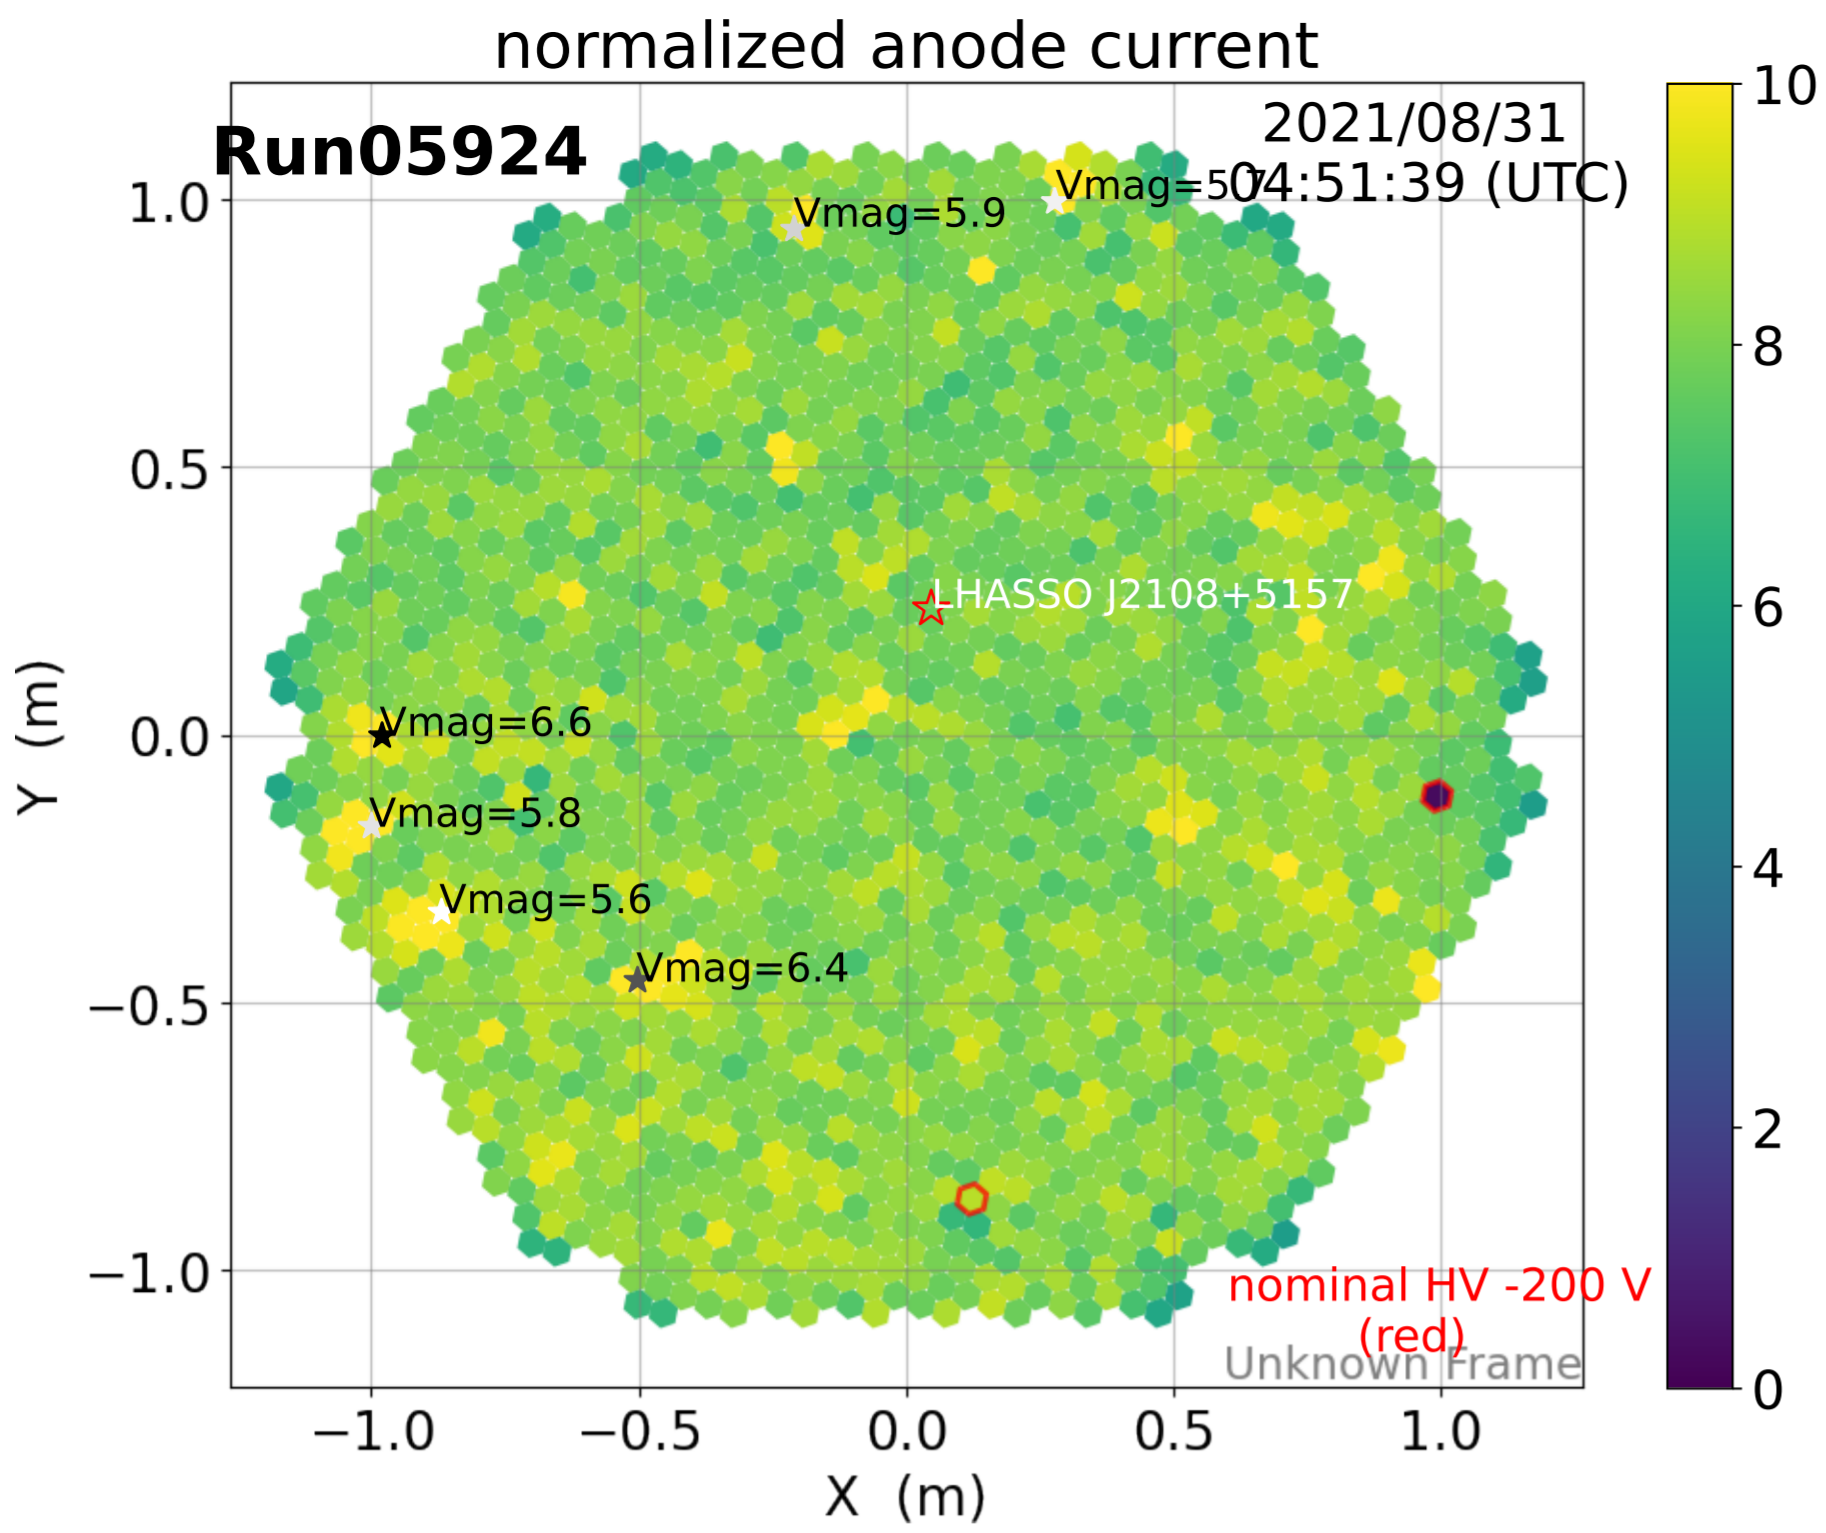


normalized anode current

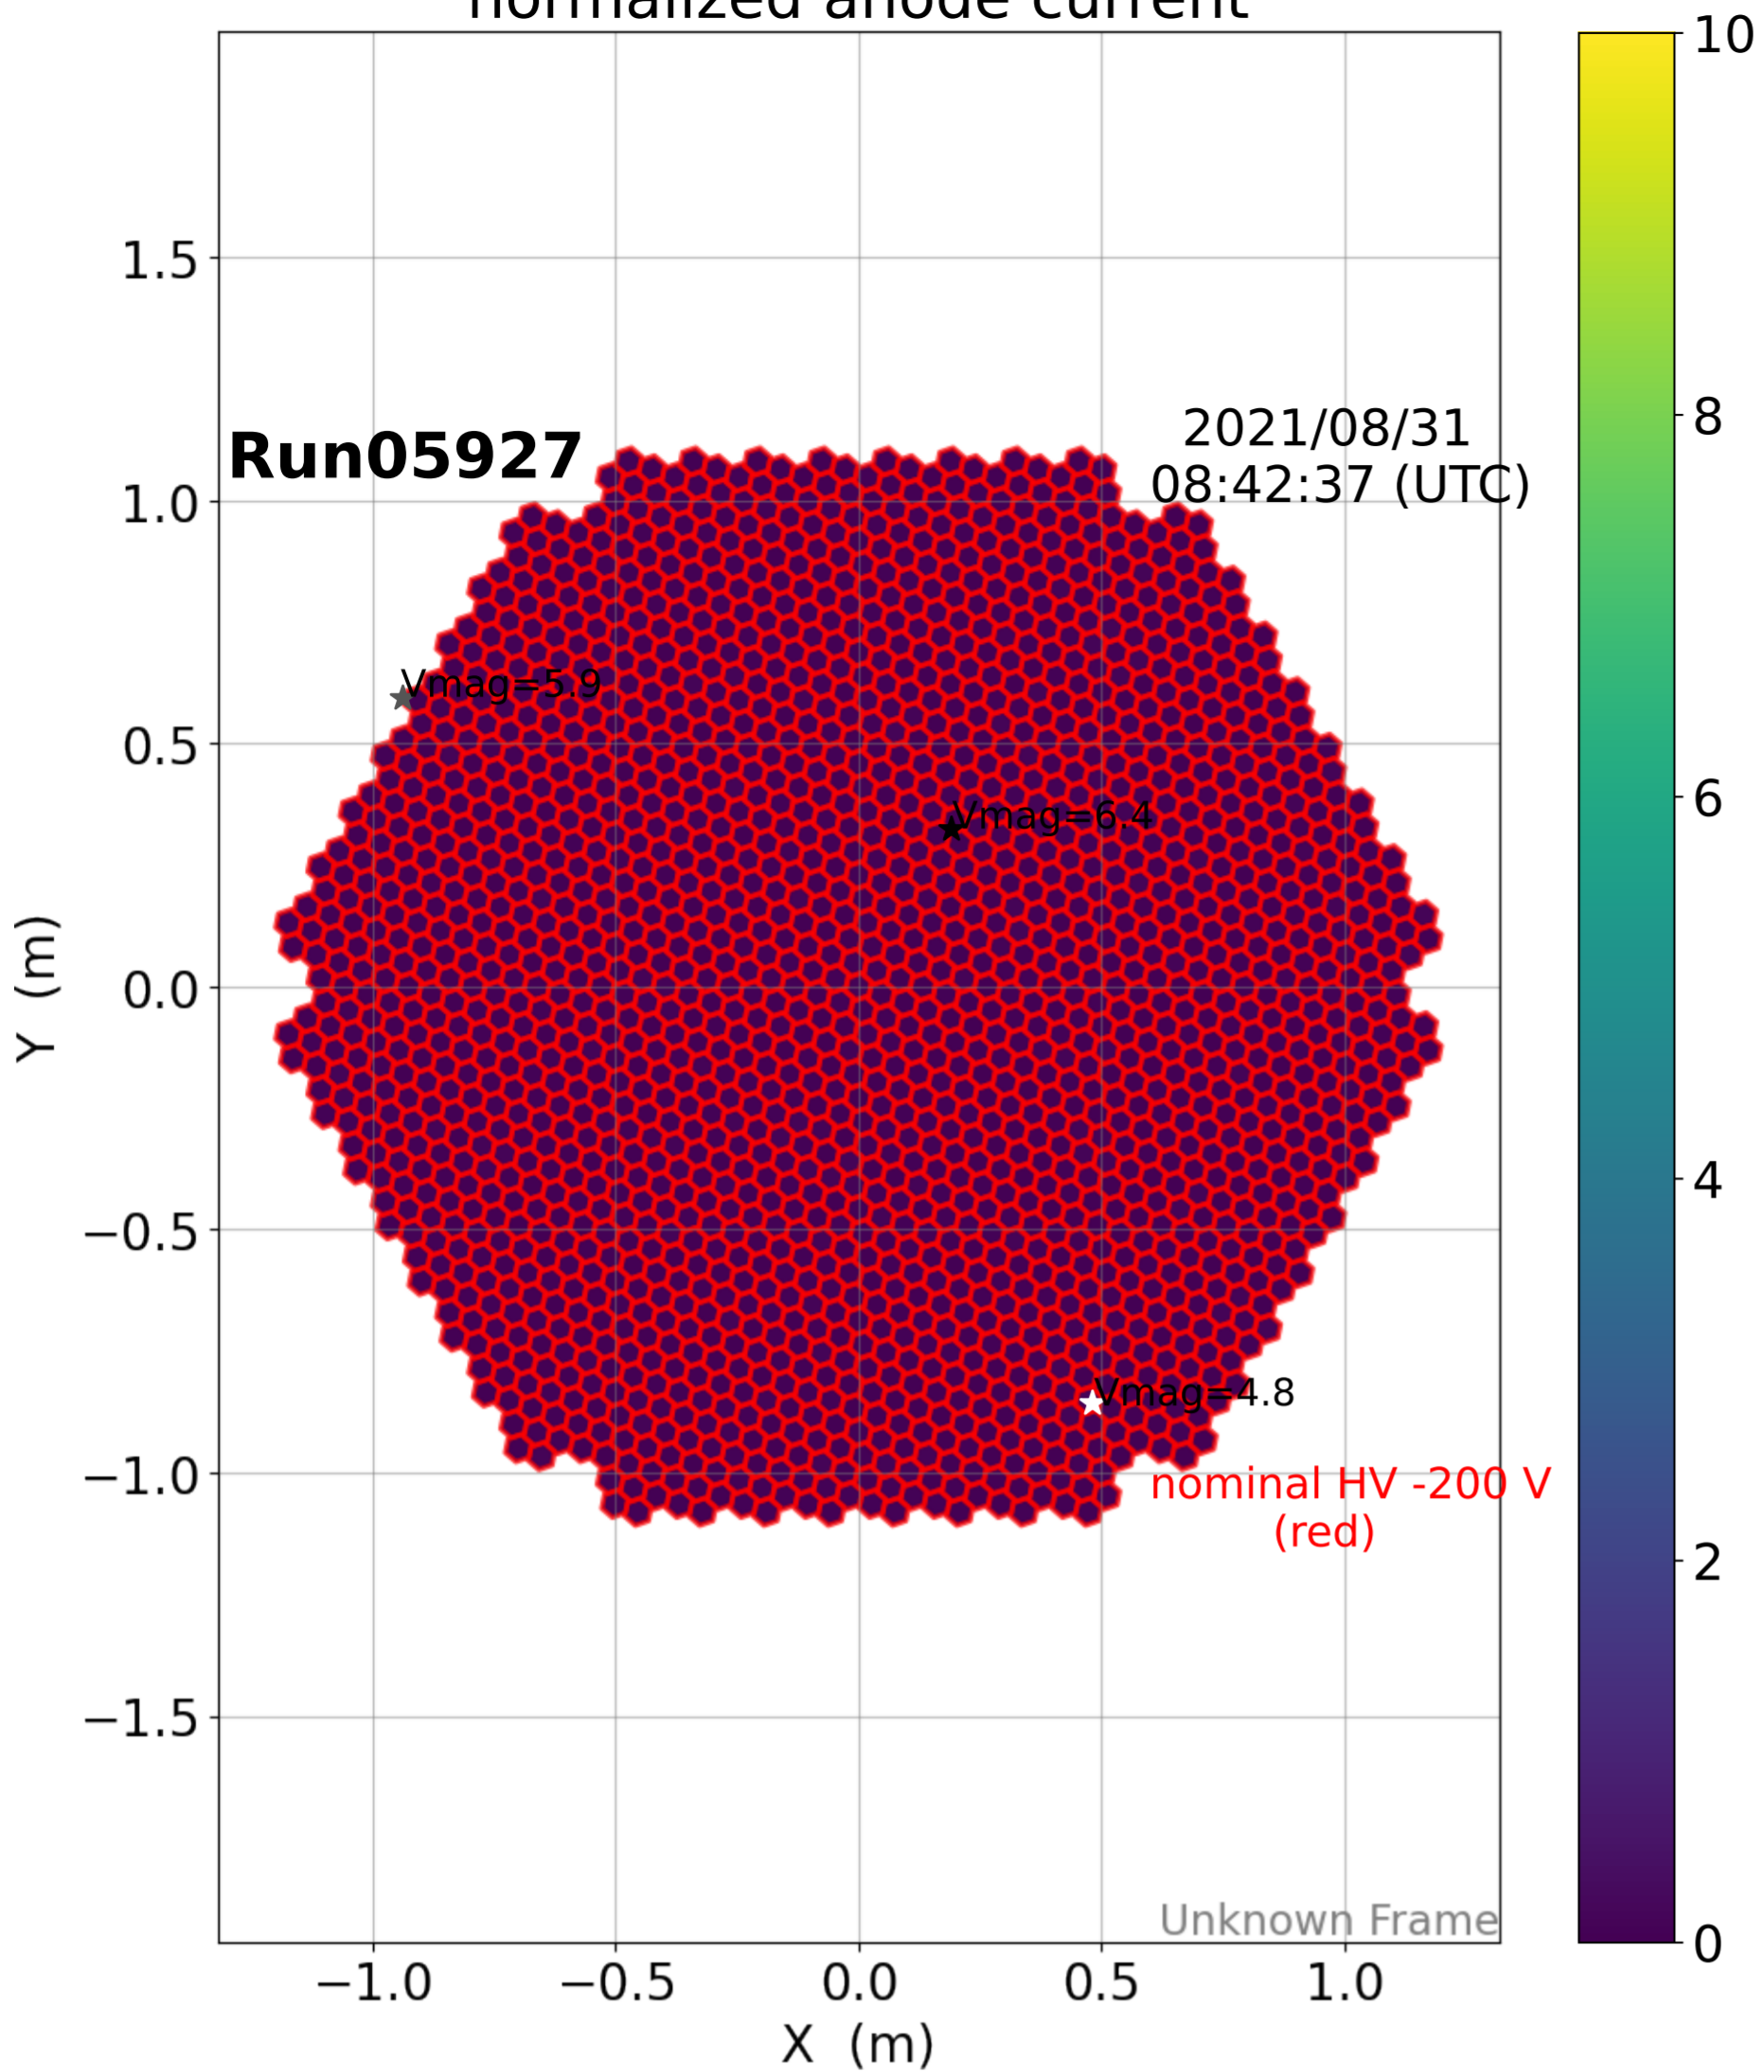

L1 local rate [Hz]

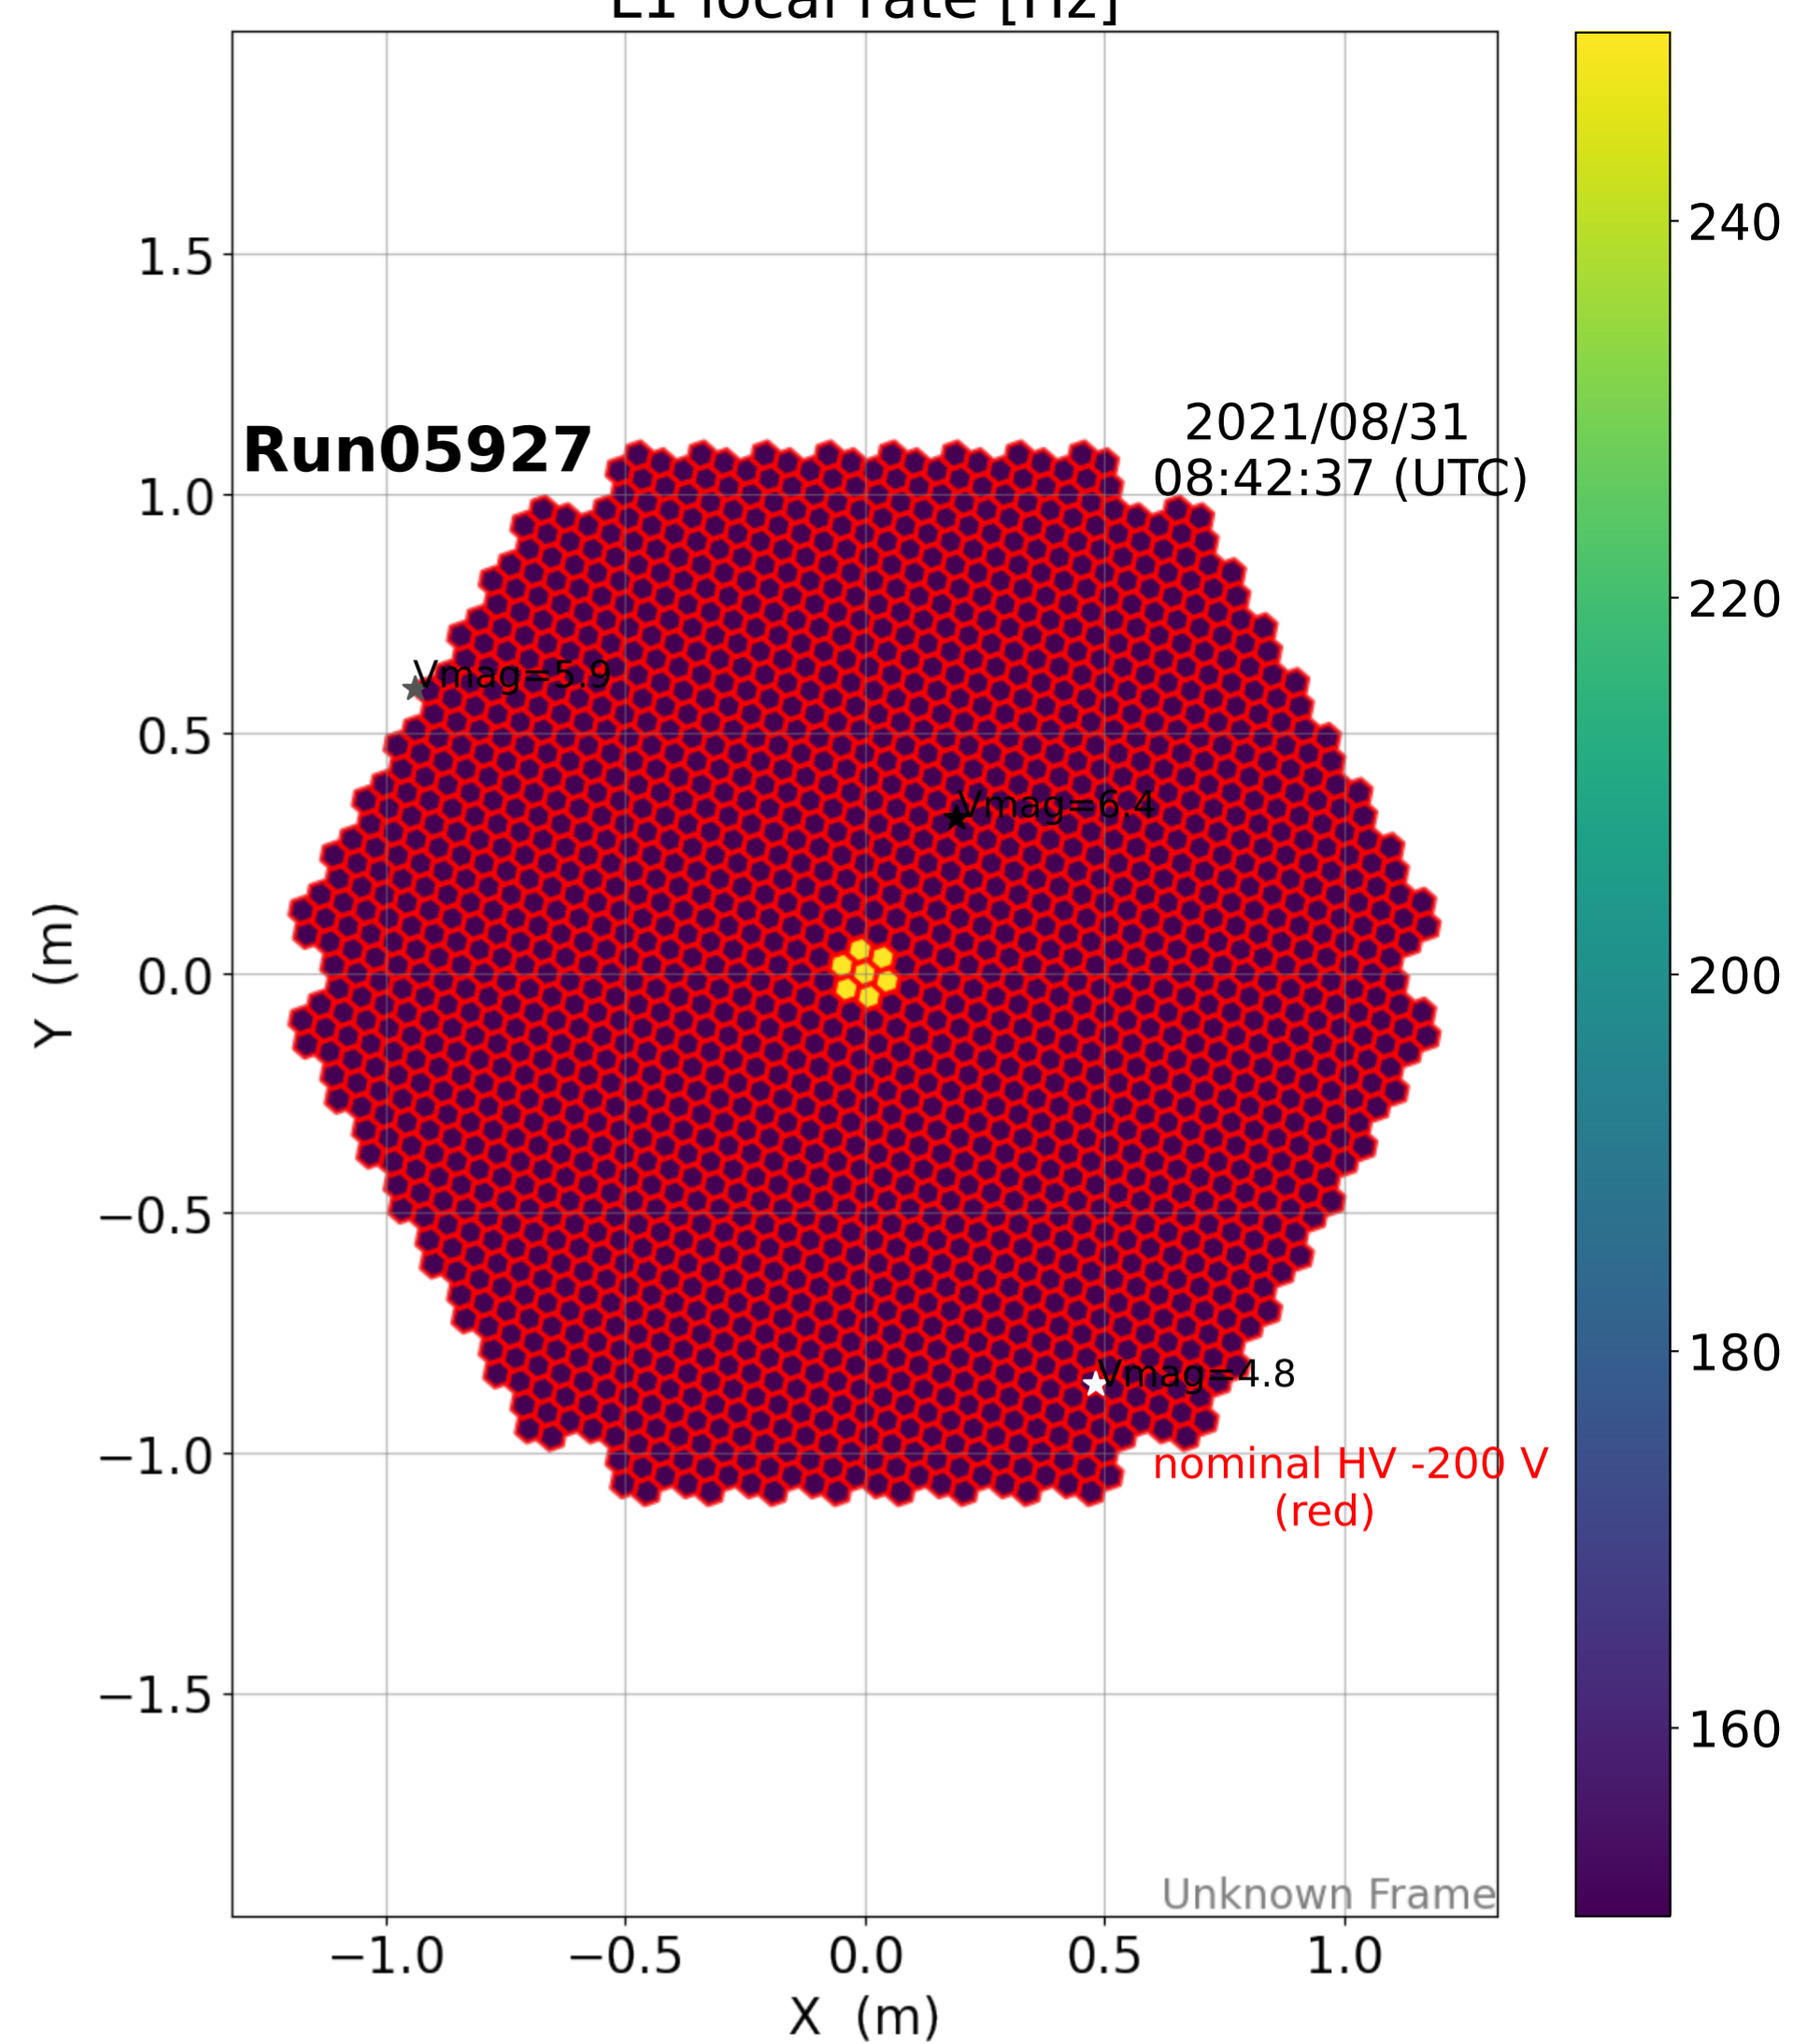

normalized anode current

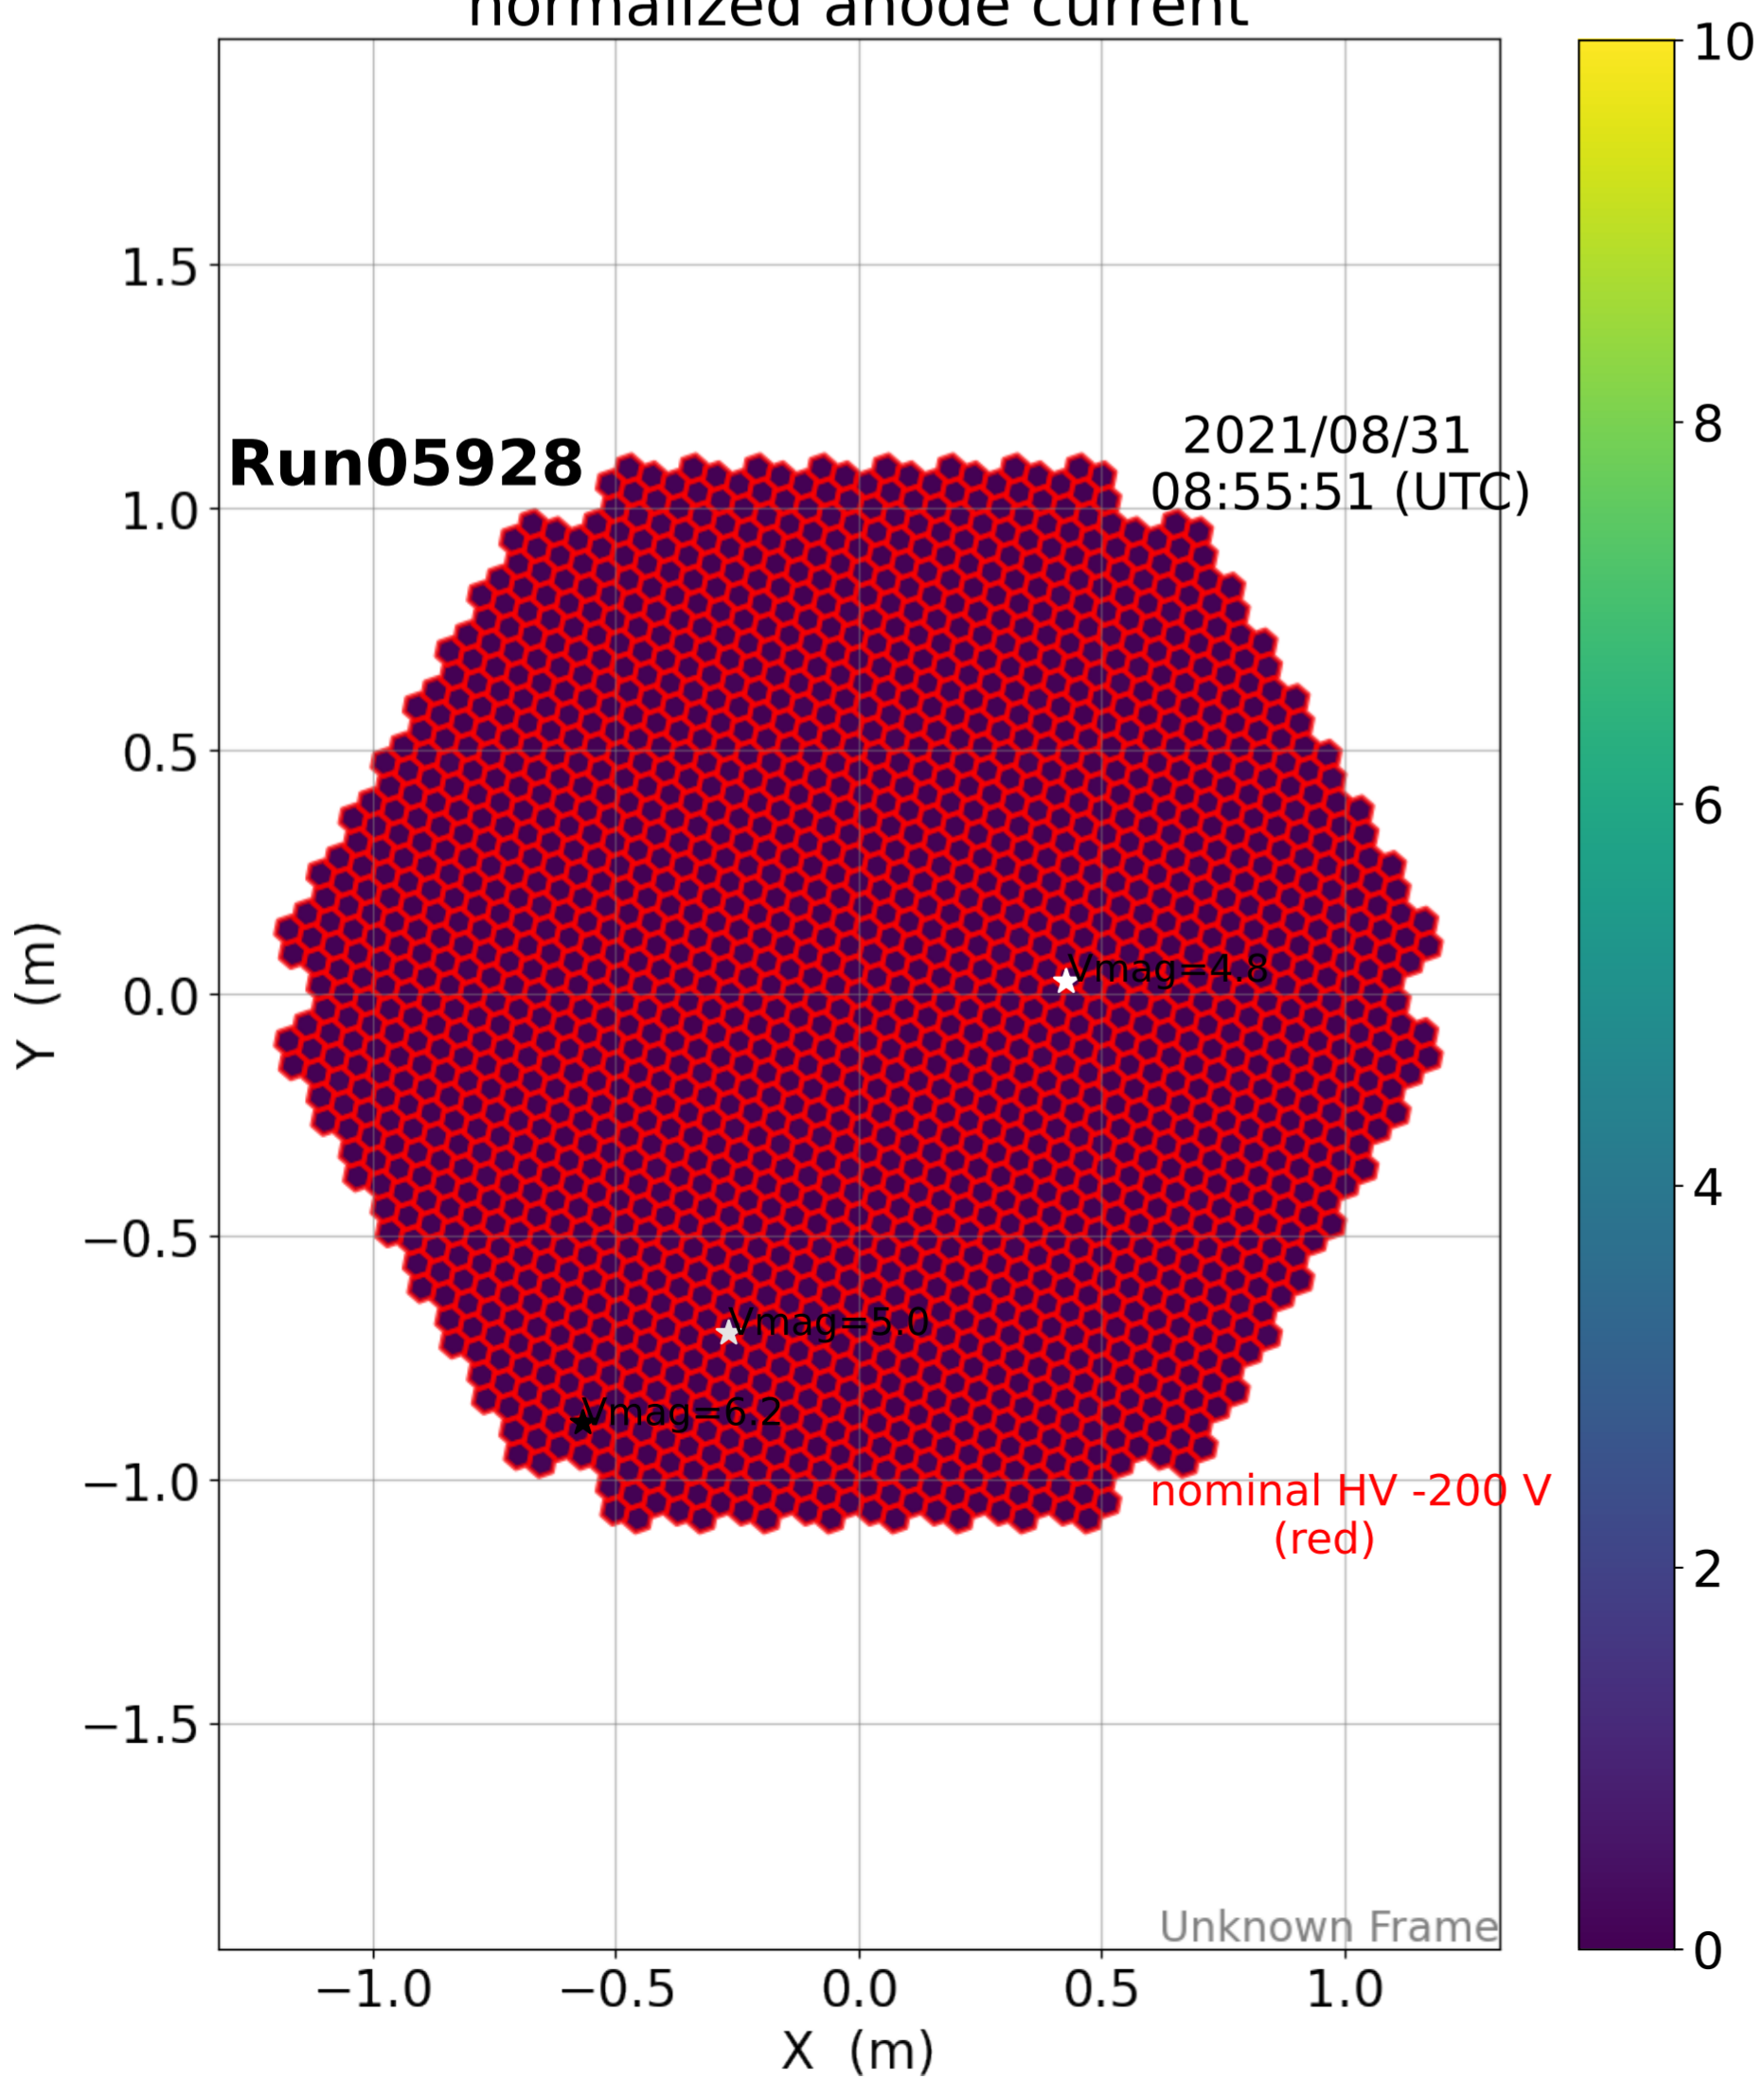

L1 local rate [Hz]

